

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083119\
 Data File : PS006489.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2019 17:48
 Operator : SM\AJ
 Sample : K4619-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP1-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 01:04:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.485	5.216	270.0E6	135.8E6	312.845	276.129
Target Compounds							
1) T	Dalapon	2.118	0.000	8197966	0	7.524	N.D. #
2) T	3,5-DICHL...	0.000	4.545	0	19148238	N.D.	31.613
3) T	4-Nitroph...	5.293	0.000	5330982	0	14.200	N.D. #
5) T	DICAMBA	5.650	0.000	13073574	0	4.071	N.D. #
7) T	MCPA	5.963	5.594	24994071	39353658	7.917	19.256 #
9) T	2,4-D	6.549	0.000	184.2E6	0	226.071	N.D. #
11) T	2,4,5-TP ...	7.240	0.000	54942401	0	12.044	N.D. #
12) T	2,4,5-T	0.000	7.228	0	23618478	N.D.	9.500
13) T	2,4-DB	8.094	0.000	73641623	0	118.246	N.D. #
16) T	DCPA	9.418	0.000	64674417	0	11.159	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083119\
Data File : PS006489.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2019 17:48
Operator : SM\AJ
Sample : K4619-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP1-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 01:04:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

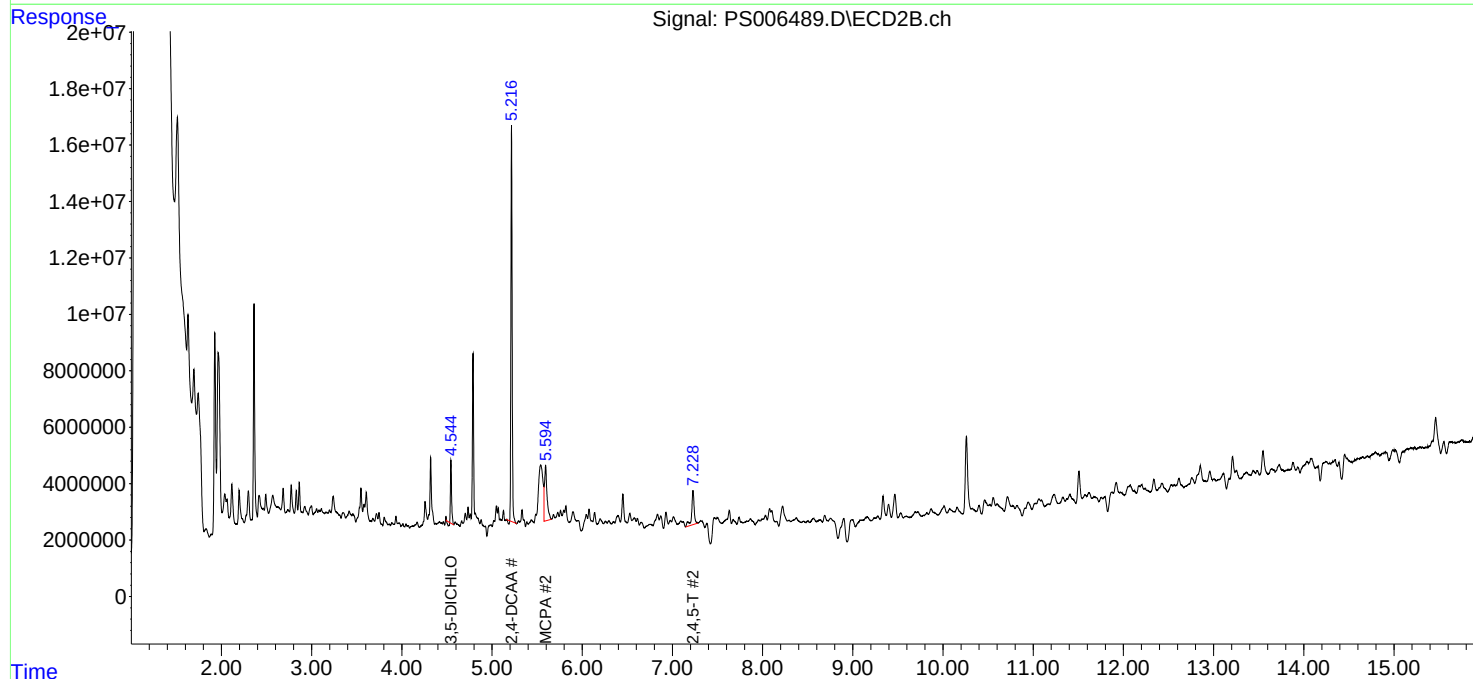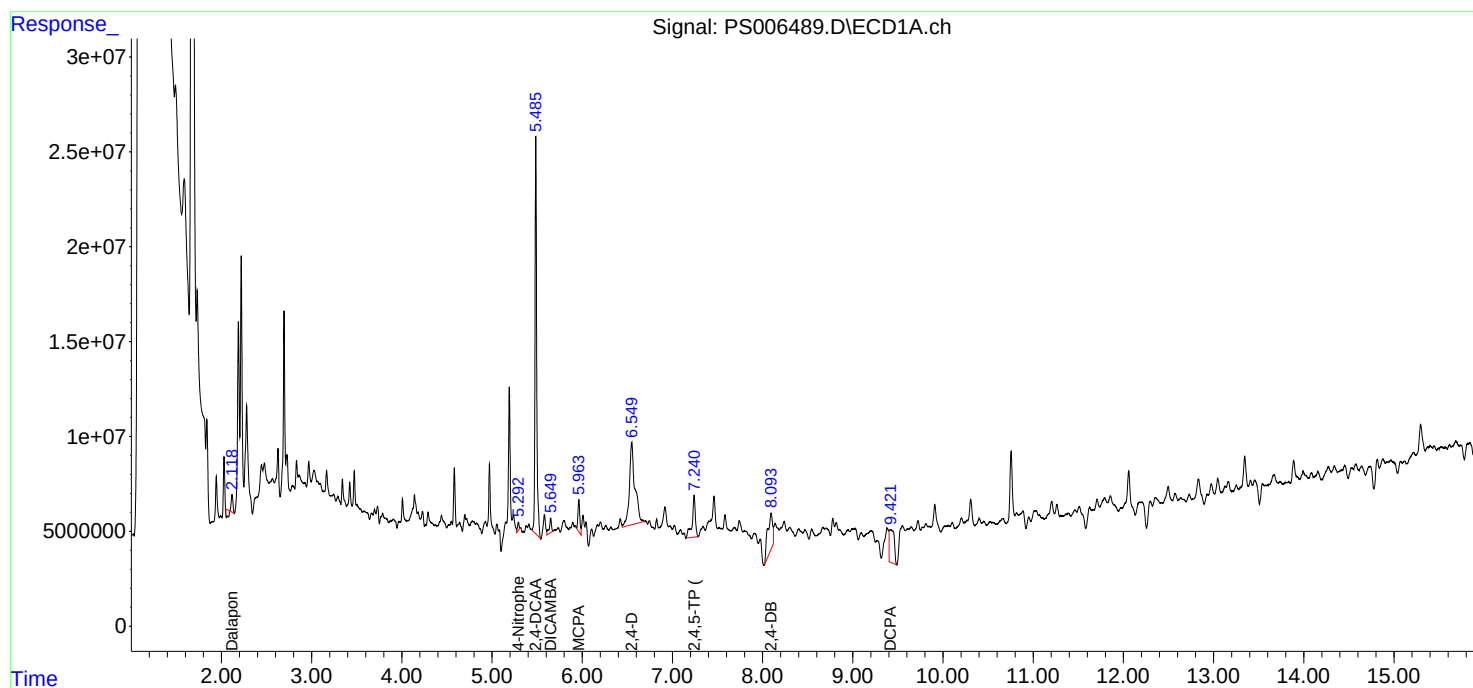


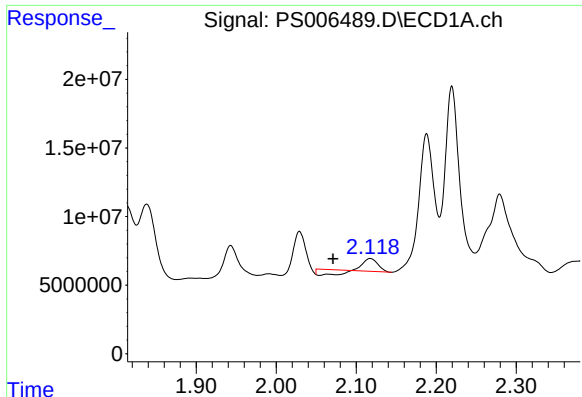

#1 Dalapon


R.T.: 2.118 min
Delta R.T.: 0.047 min
Response: 8197966
Conc: 7.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP1-COMP

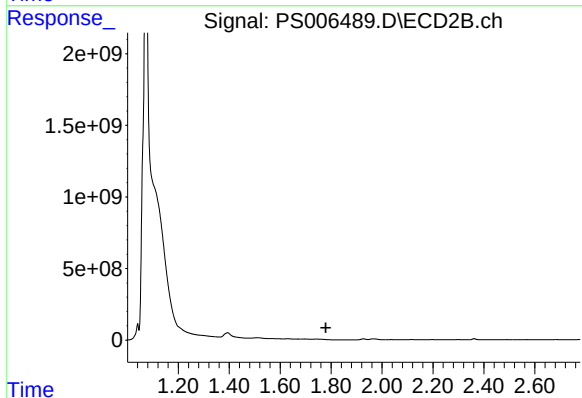


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.779 min
Response: 0
Conc: N.D.

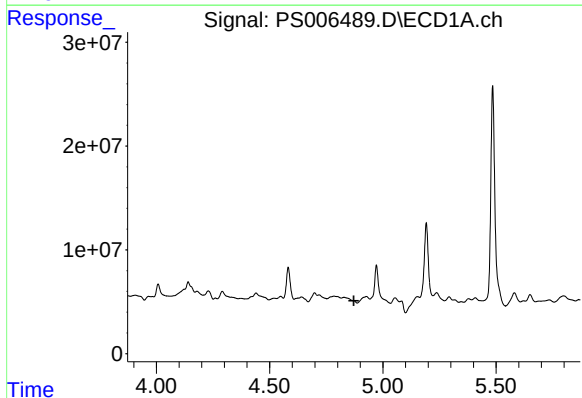


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.872 min
Response: 0
Conc: N.D.

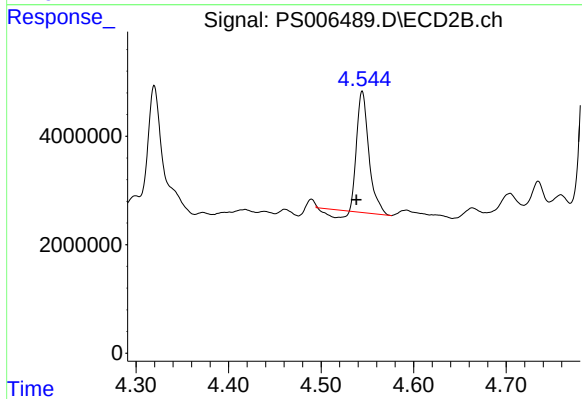

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.545 min
Delta R.T.: 0.007 min
Response: 19148238
Conc: 31.61 ng/ml

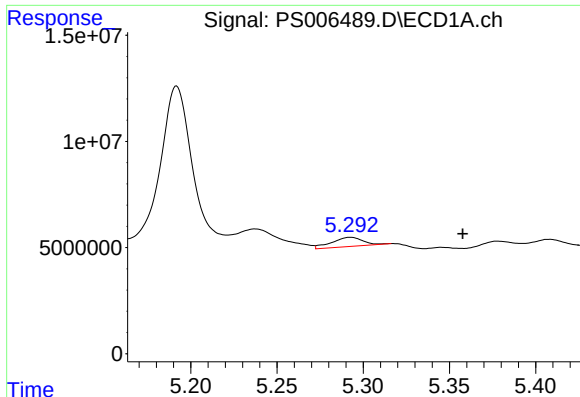

#3 4-Nitrophenol


R.T.: 5.293 min
Delta R.T.: -0.065 min
Response: 5330982
Conc: 14.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP1-COMP

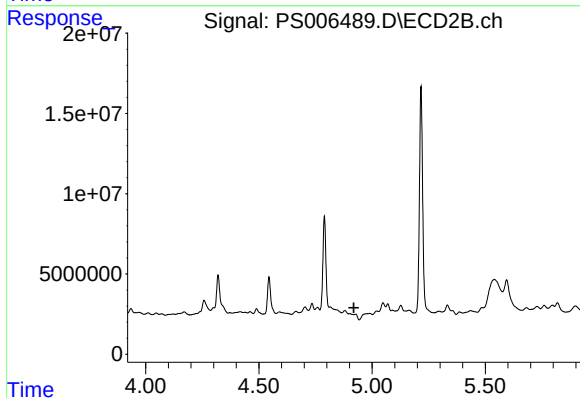


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 4.920 min
Response: 0
Conc: N.D.

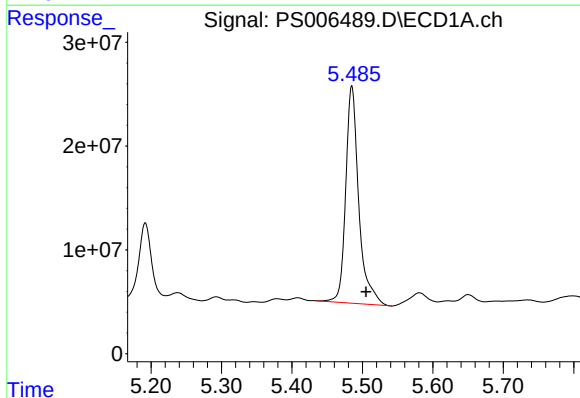


#4 2,4-DCAA

R.T.: 5.485 min
Delta R.T.: -0.020 min
Response: 270048398
Conc: 312.85 ng/ml

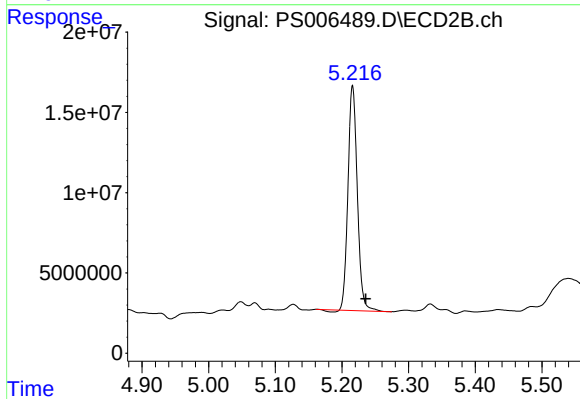

#4 2,4-DCAA


R.T.: 5.216 min
Delta R.T.: -0.020 min
Response: 135814783
Conc: 276.13 ng/ml

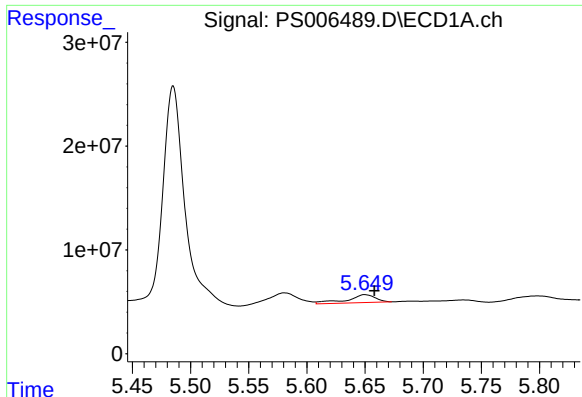

#5 DICAMBA


R.T.: 5.650 min
Delta R.T.: -0.008 min
Response: 13073574
Conc: 4.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP1-COMP

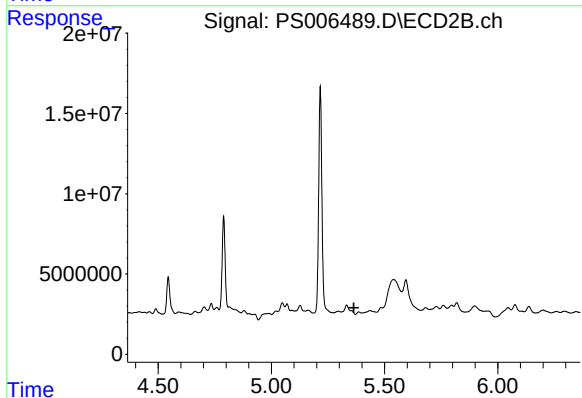


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.364 min
Response: 0
Conc: N.D.

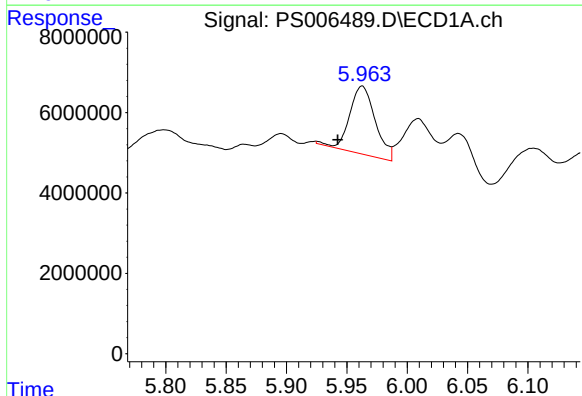


#7 MCPA

R.T.: 5.963 min
Delta R.T.: 0.020 min
Response: 24994071
Conc: 7.92 ug/ml

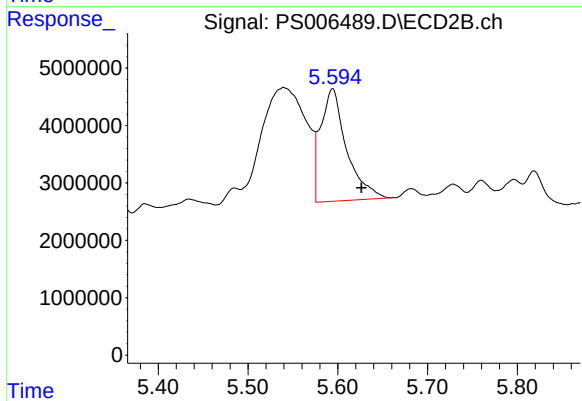

#7 MCPA


R.T.: 5.594 min
Delta R.T.: -0.032 min
Response: 39353658
Conc: 19.26 ug/ml

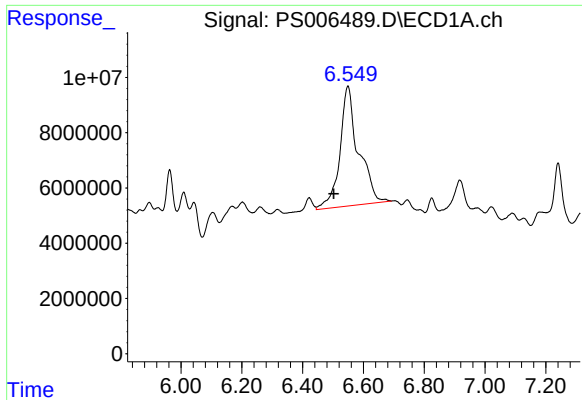

#9 2,4-D


R.T.: 6.549 min
Delta R.T.: 0.046 min
Response: 184199343
Conc: 226.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP1-COMP

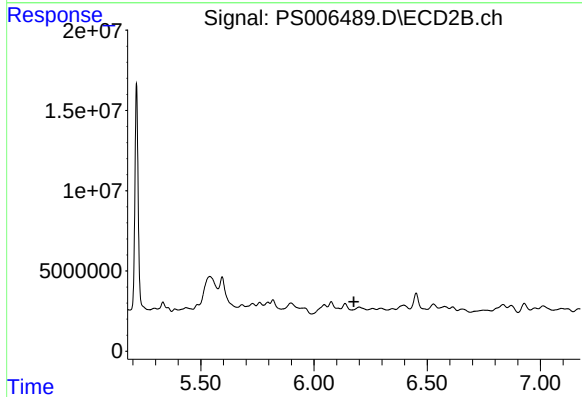


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

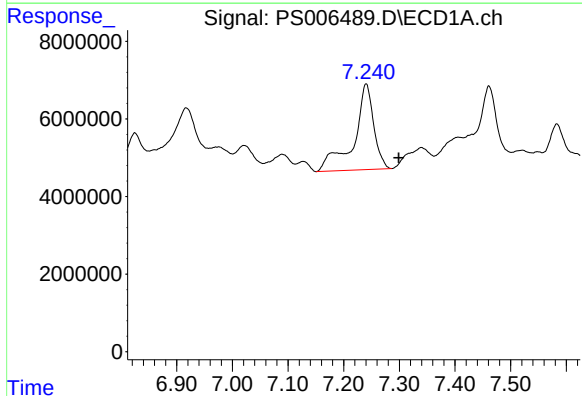


#11 2,4,5-TP (SILVEX)

R.T.: 7.240 min
Delta R.T.: -0.059 min
Response: 54942401
Conc: 12.04 ng/ml

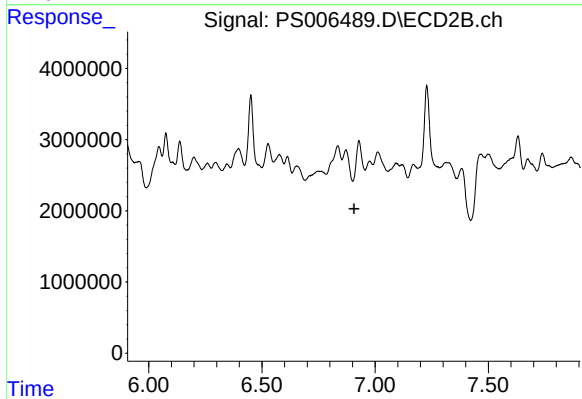

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 6.907 min
Response: 0
Conc: N.D.

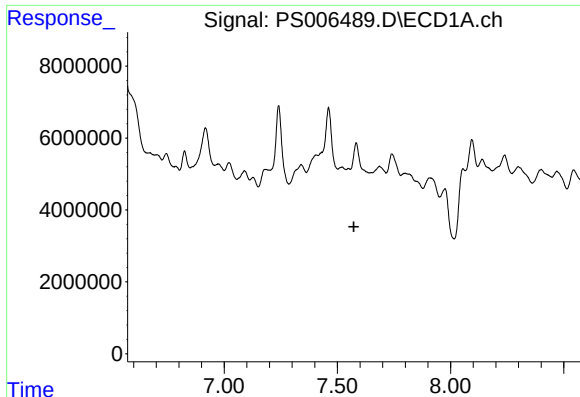

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP1-COMP

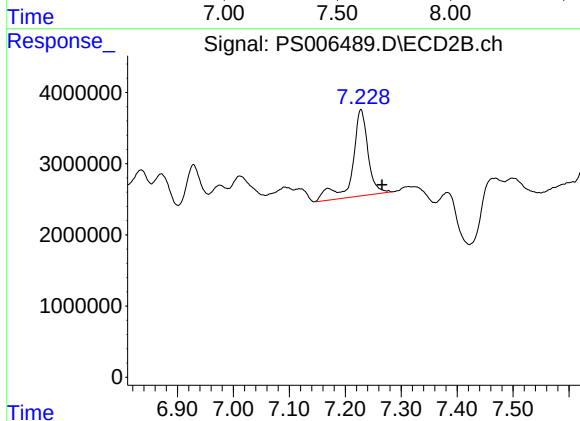


#12 2,4,5-T

R.T.: 7.228 min
Delta R.T.: -0.038 min
Response: 23618478
Conc: 9.50 ng/ml

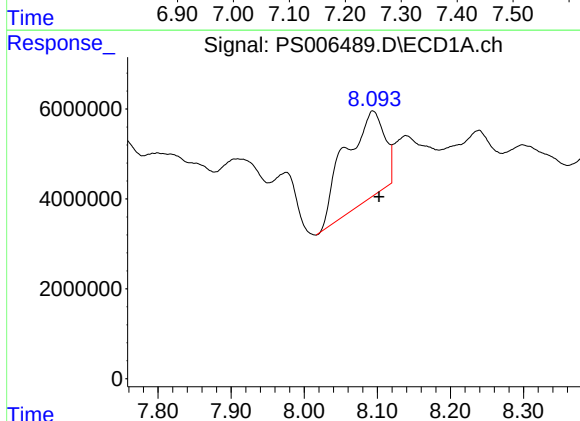


#13 2,4-DB

R.T.: 8.094 min
Delta R.T.: -0.008 min
Response: 73641623
Conc: 118.25 ng/ml

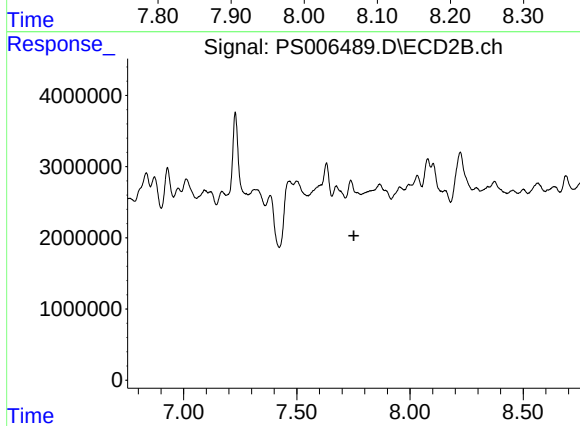

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 7.752 min
Response: 0
Conc: N.D.

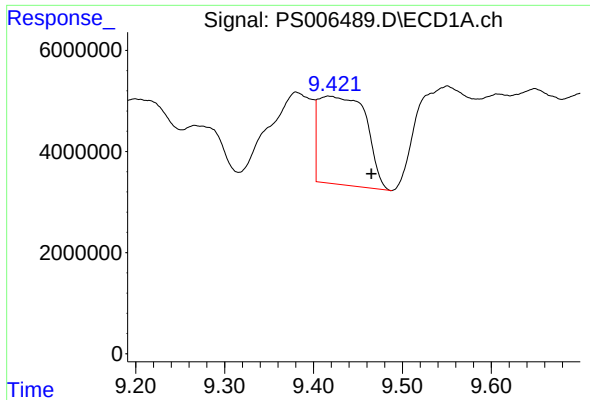

#16 DCPA

R.T.: 9.418 min
Delta R.T.: -0.047 min
Response: 64674417
Conc: 11.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP1-COMP

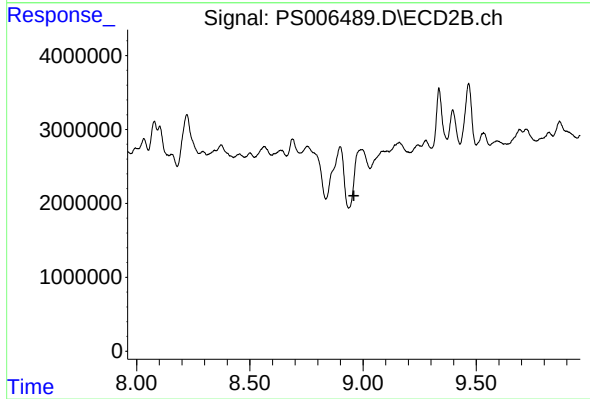

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 8.959 min
Response: 0
Conc: N.D.