

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083119\
 Data File : PS006503.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2019 22:57
 Operator : SM\AJ
 Sample : K4619-12
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP4-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 01:10:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.481	5.211	286.6E6	122.8E6	332.043	249.733
Target Compounds							
1) T	Dalapon	2.115	1.739	8855634	167.4E6	8.127	266.833 #
5) T	DICAMBA	5.646	5.328	22537883	18262644	7.018	9.901 #
7) T	MCPA	5.959	5.588	10260032	36211268	3.250	17.718 #
9) T	2,4-D	6.546	0.000	170.2E6	0	208.860	N.D. #
13) T	2,4-DB	8.089	0.000	60445947	0	97.057	N.D. #
15) T	Picloram	0.000	8.987	0	14984540	N.D.	3.322
16) T	DCPA	0.000	8.987	0	14984540	N.D.	4.297



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083119\
Data File : PS006503.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2019 22:57
Operator : SM\AJ
Sample : K4619-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP4-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 01:10:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

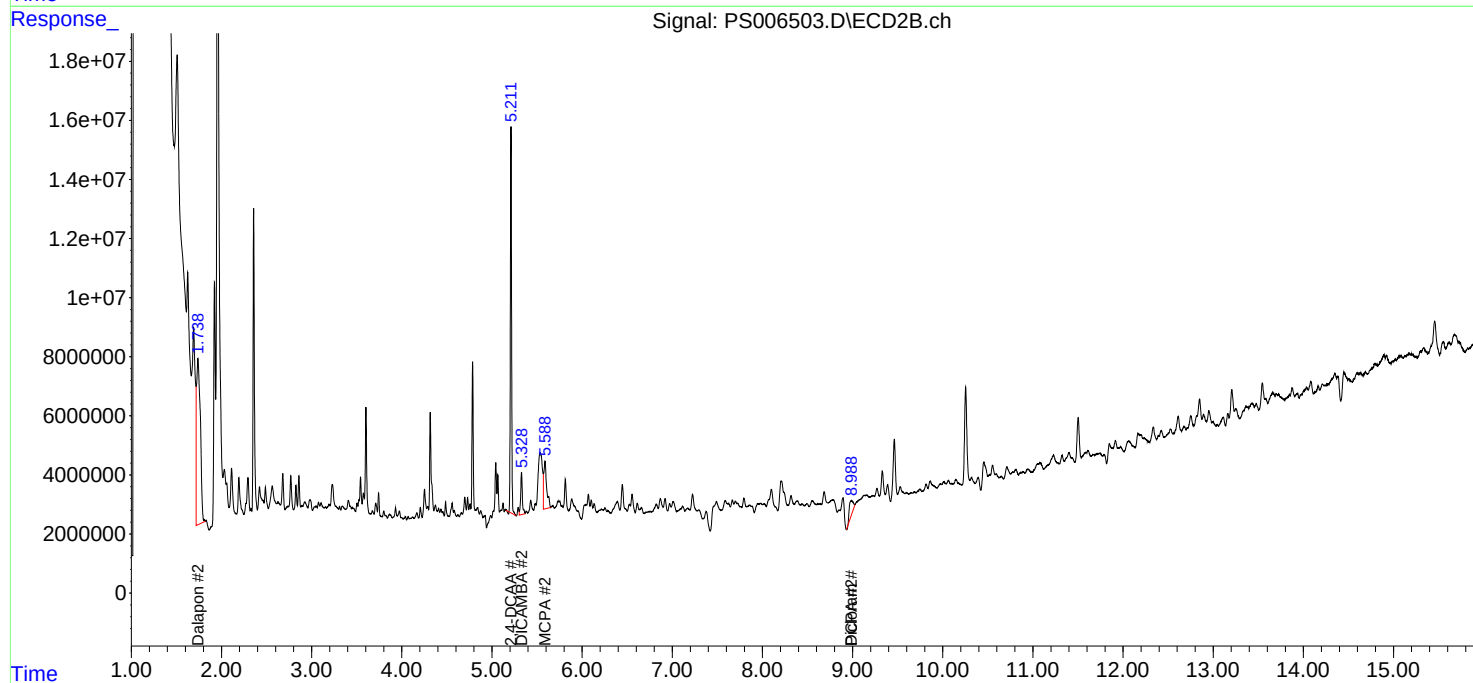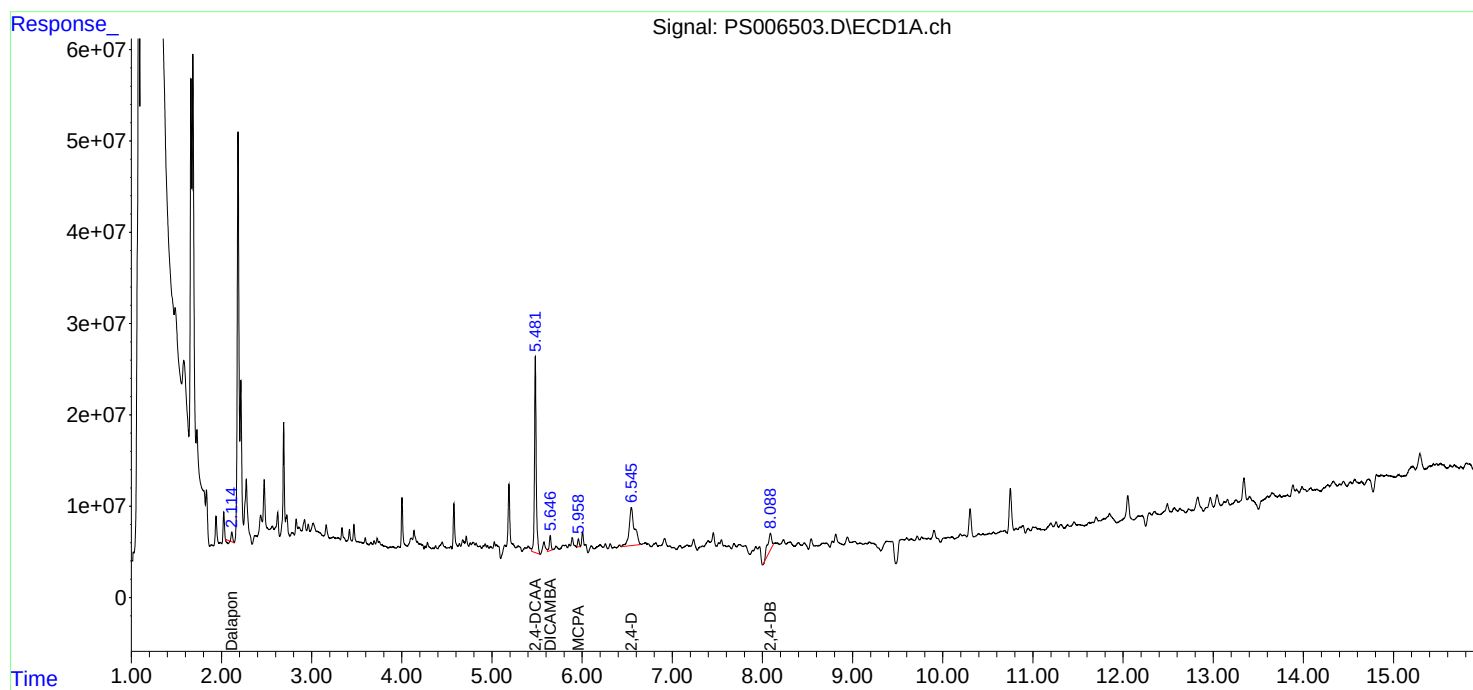


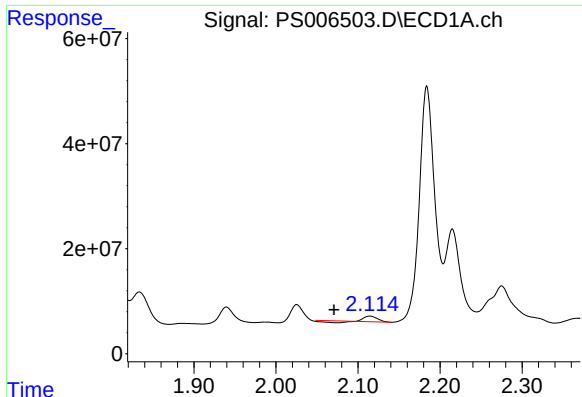

#1 Dalapon


R.T.: 2.115 min
Delta R.T.: 0.044 min
Response: 8855634
Conc: 8.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP4-COMP

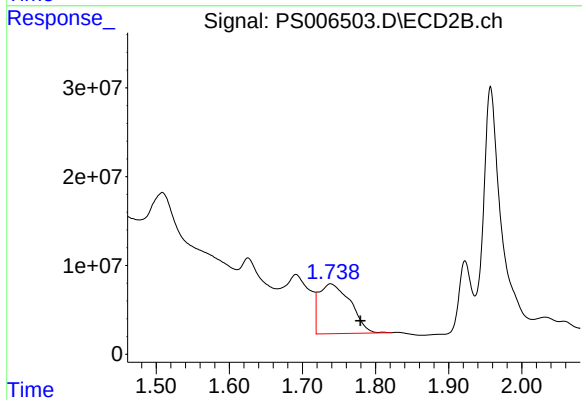


#1 Dalapon

R.T.: 1.739 min
Delta R.T.: -0.040 min
Response: 167435926
Conc: 266.83 ng/ml

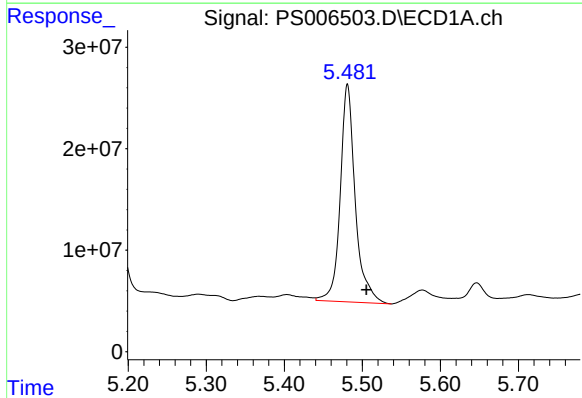


#4 2,4-DCAA

R.T.: 5.481 min
Delta R.T.: -0.024 min
Response: 286620100
Conc: 332.04 ng/ml

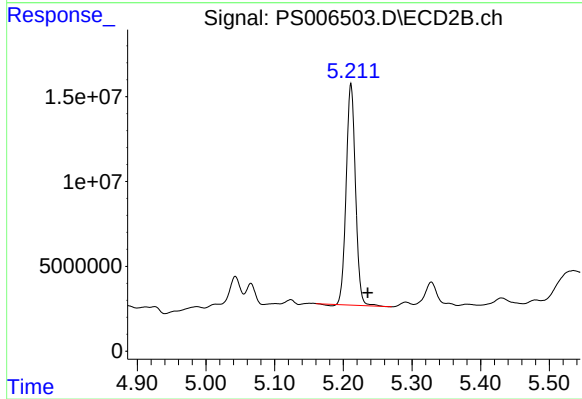

#4 2,4-DCAA


R.T.: 5.211 min
Delta R.T.: -0.024 min
Response: 122831856
Conc: 249.73 ng/ml

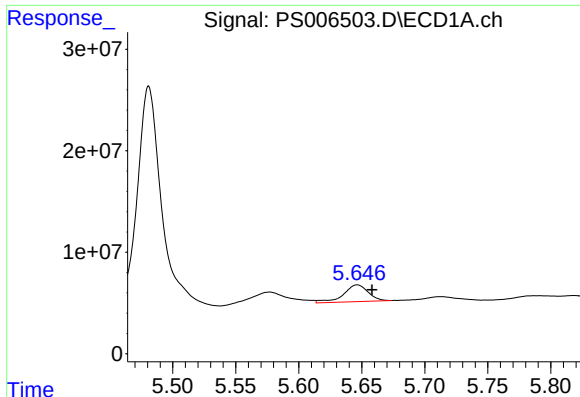

#5 DICAMBA


R.T.: 5.646 min
Delta R.T.: -0.012 min
Response: 22537883
Conc: 7.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP4-COMP

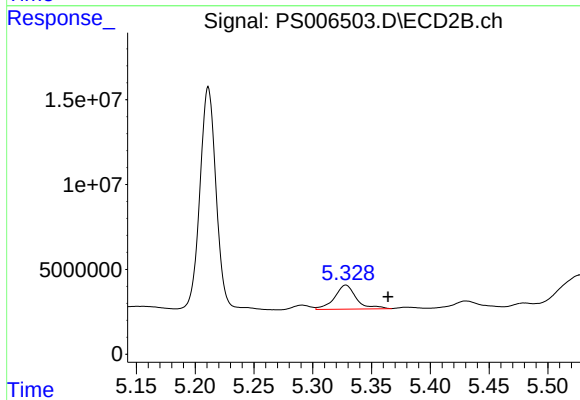


#5 DICAMBA

R.T.: 5.328 min
Delta R.T.: -0.036 min
Response: 18262644
Conc: 9.90 ng/ml

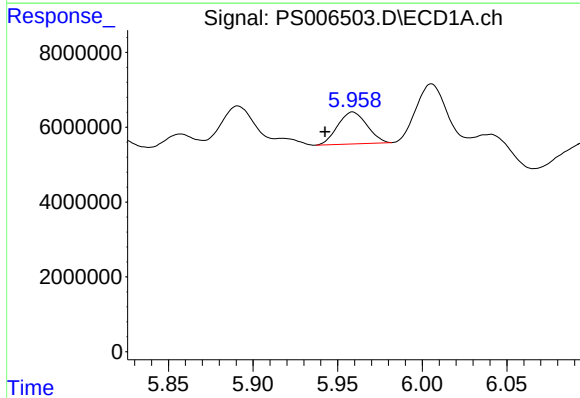


#7 MCPA

R.T.: 5.959 min
Delta R.T.: 0.016 min
Response: 10260032
Conc: 3.25 ug/ml

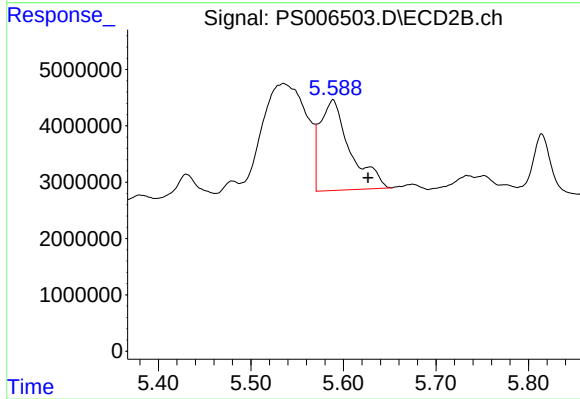

#7 MCPA


R.T.: 5.588 min
Delta R.T.: -0.038 min
Response: 36211268
Conc: 17.72 ug/ml

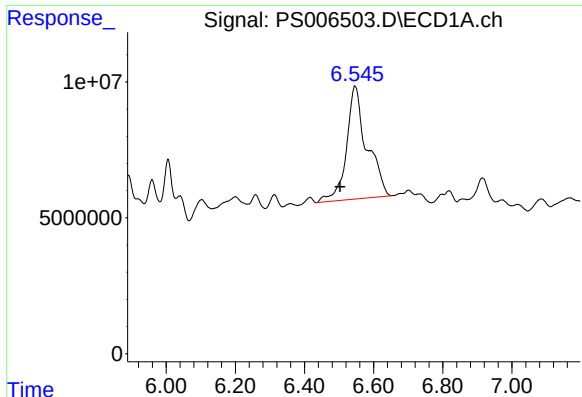

#9 2,4-D


R.T.: 6.546 min
Delta R.T.: 0.043 min
Response: 170175653
Conc: 208.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP4-COMP

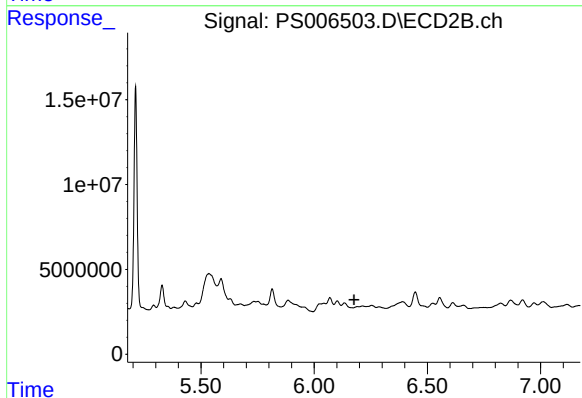


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

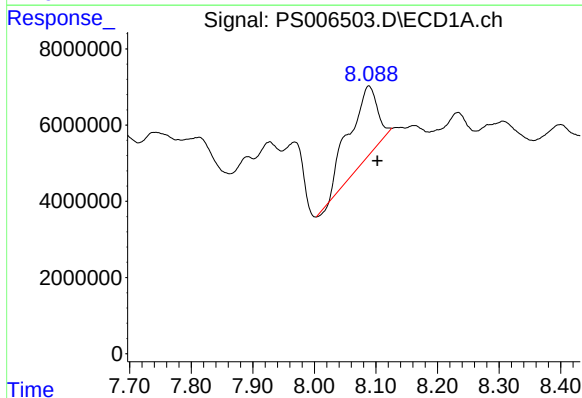


#13 2,4-DB

R.T.: 8.089 min
Delta R.T.: -0.014 min
Response: 60445947
Conc: 97.06 ng/ml

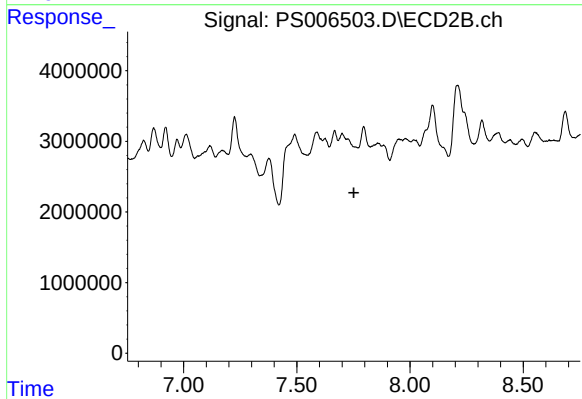

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.752 min
Response: 0
Conc: N.D.

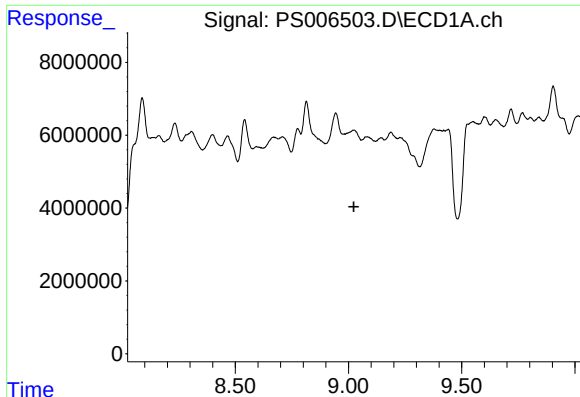

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 9.024 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP4-COMP

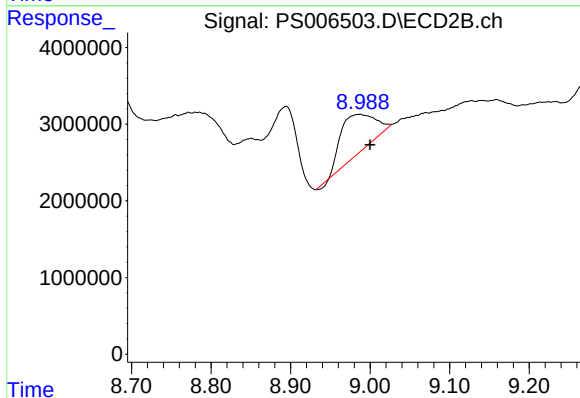


#15 Picloram

R.T.: 8.987 min
Delta R.T.: -0.014 min
Response: 14984540
Conc: 3.32 ng/ml

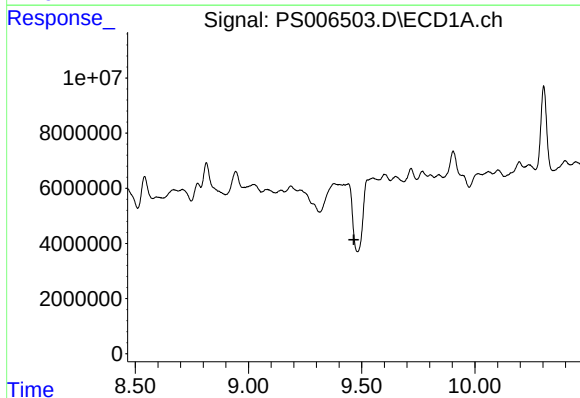

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.465 min
Response: 0
Conc: N.D.

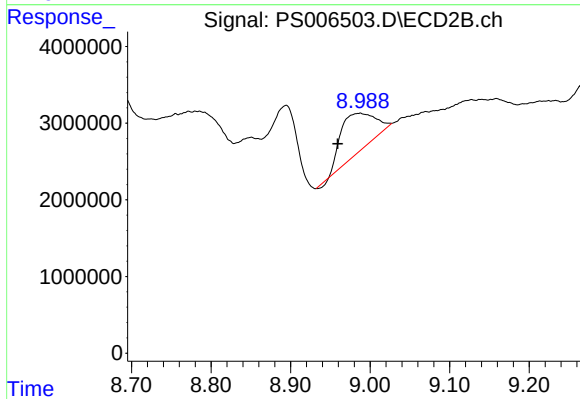

#16 DCPA

R.T.: 8.987 min
Delta R.T.: 0.027 min
Response: 14984540
Conc: 4.30 ng/ml