

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083119\
 Data File : PS006508.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2019 00:47
 Operator : SM\AJ
 Sample : K4619-27
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP9-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:13:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.477	5.207	259.0E6	126.3E6	300.071	256.703
Target Compounds							
1) T	Dalapon	2.110	1.734	-10604137	165.0E6	N.D.	262.937
2) T	3,5-DICHL...	0.000	4.536	0	30867053	N.D.	50.960
7) T	MCPA	5.954	5.585	13699557	34419421	4.339	16.842 #
9) T	2,4-D	6.543	0.000	193.0E6	0	236.875	N.D. #
13) T	2,4-DB	8.083	0.000	35947998	0	57.721	N.D. #
15) T	Picloram	0.000	8.988	0	14556783	N.D.	3.227
16) T	DCPA	9.405	8.988	149.3E6	14556783	25.763	4.174 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083119\
Data File : PS006508.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2019 00:47
Operator : SM\AJ
Sample : K4619-27
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP9-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:13:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

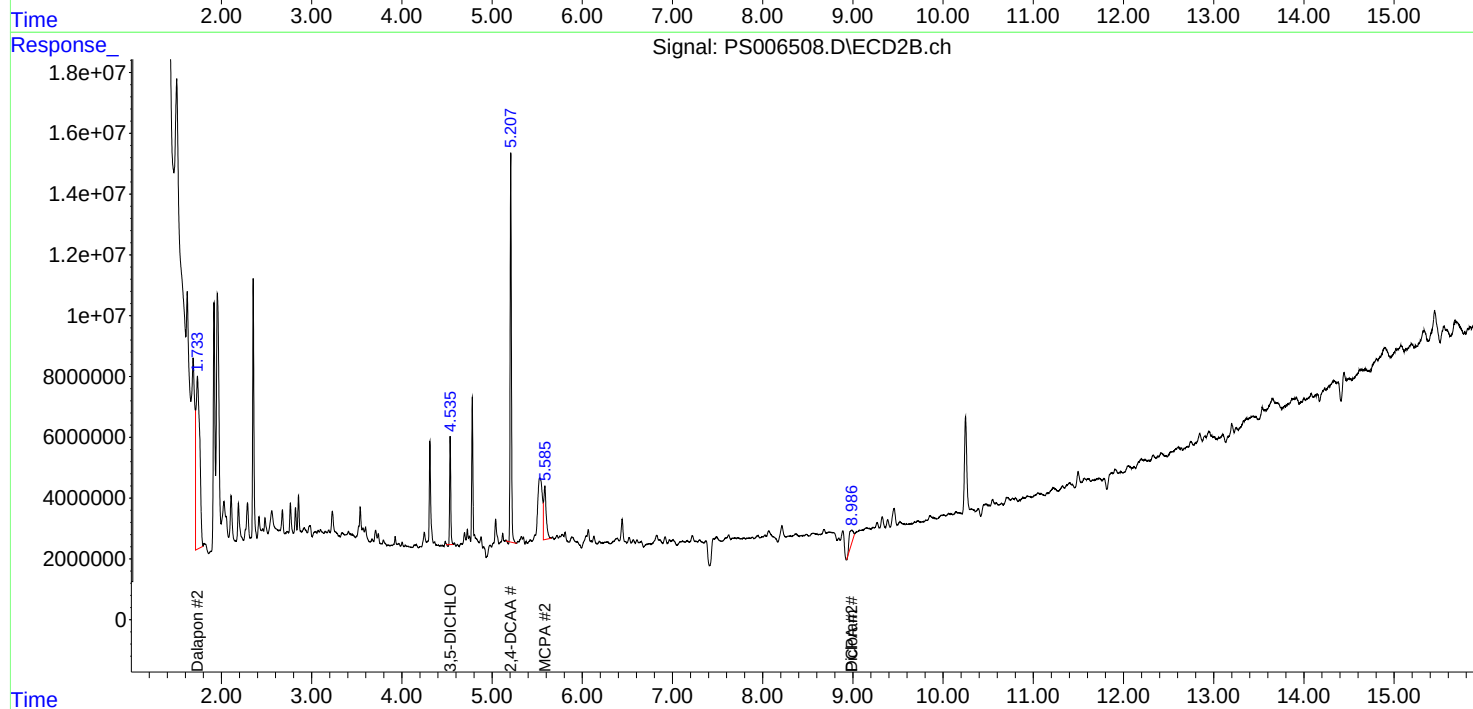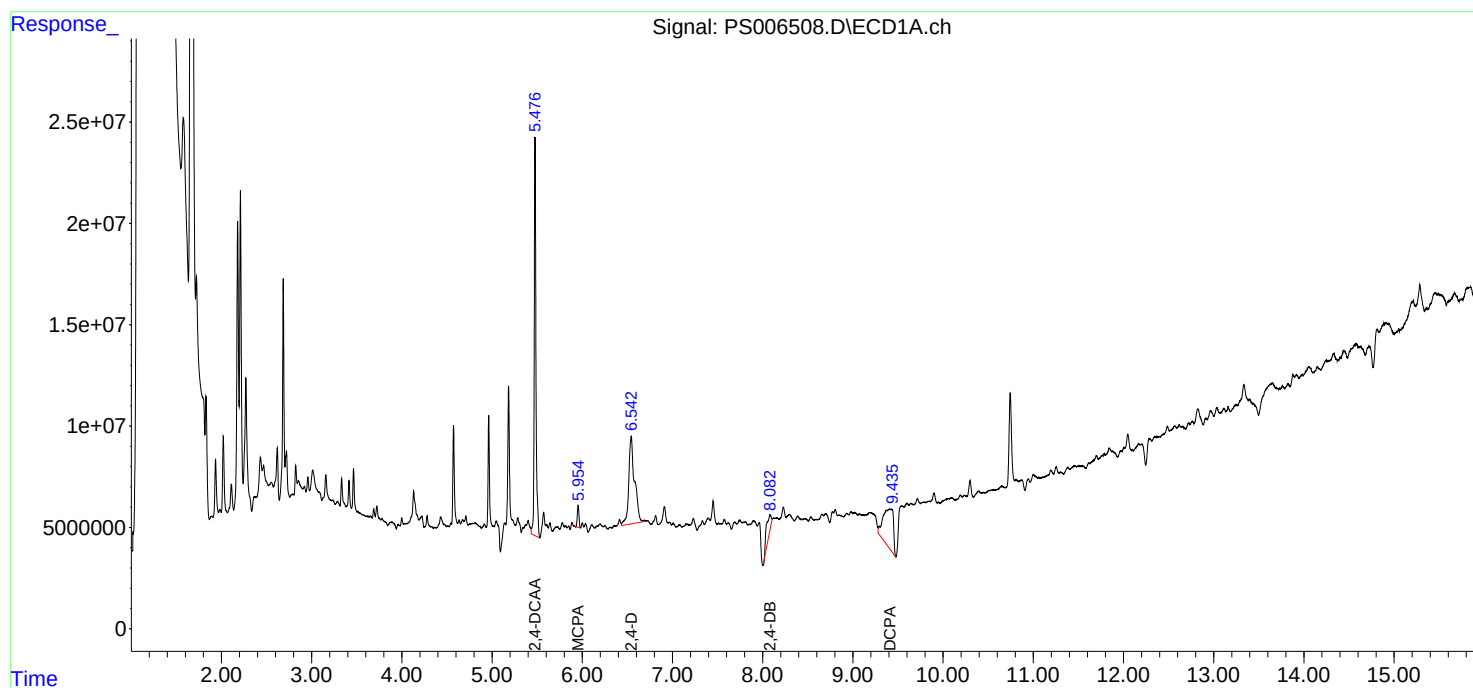


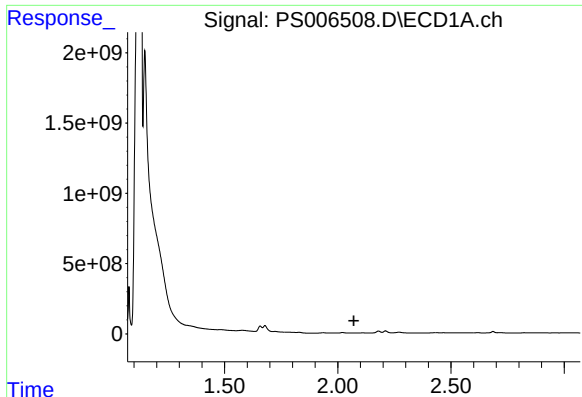

#1 Dalapon


R.T.: 2.110 min
Delta R.T.: 0.039 min
Response: -10604137
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP9-COMP

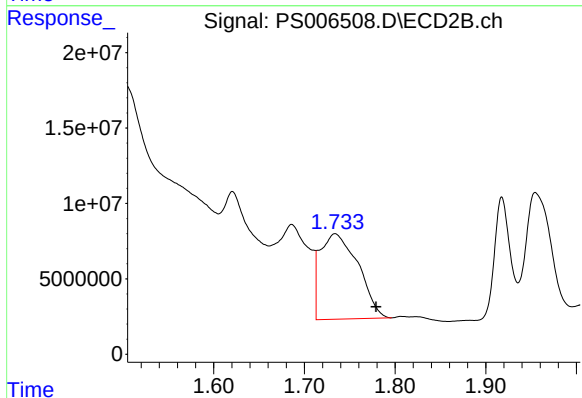


#1 Dalapon

R.T.: 1.734 min
Delta R.T.: -0.045 min
Response: 164991045
Conc: 262.94 ng/ml

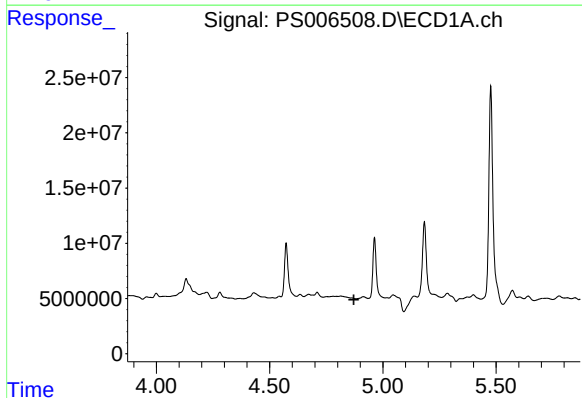


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.872 min
Response: 0
Conc: N.D.

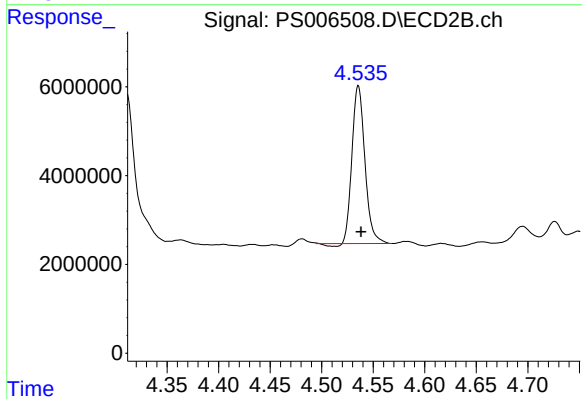

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.536 min
Delta R.T.: -0.002 min
Response: 30867053
Conc: 50.96 ng/ml

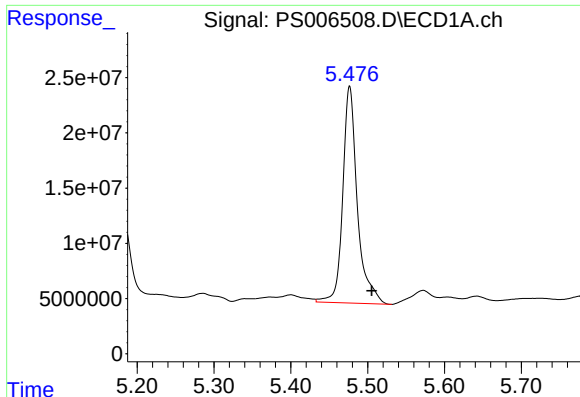

#4 2,4-DCAA


R.T.: 5.477 min
Delta R.T.: -0.029 min
Response: 259021798
Conc: 300.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP9-COMP

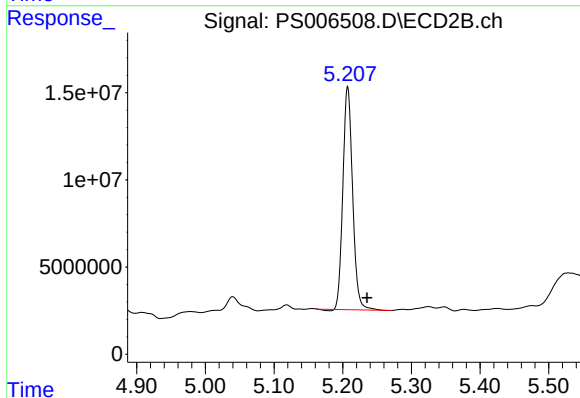


#4 2,4-DCAA

R.T.: 5.207 min
Delta R.T.: -0.028 min
Response: 126259639
Conc: 256.70 ng/ml

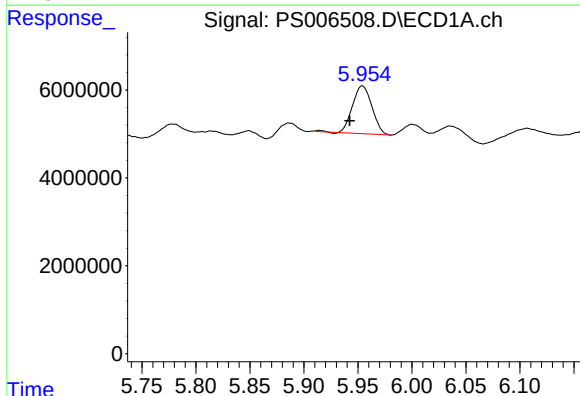


#7 MCPA

R.T.: 5.954 min
Delta R.T.: 0.012 min
Response: 13699557
Conc: 4.34 ug/ml

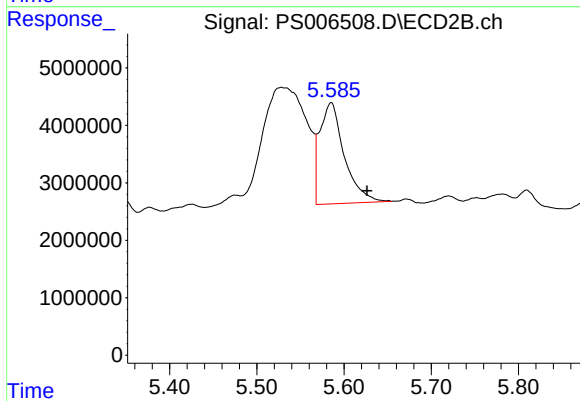

#7 MCPA


R.T.: 5.585 min
Delta R.T.: -0.042 min
Response: 34419421
Conc: 16.84 ug/ml

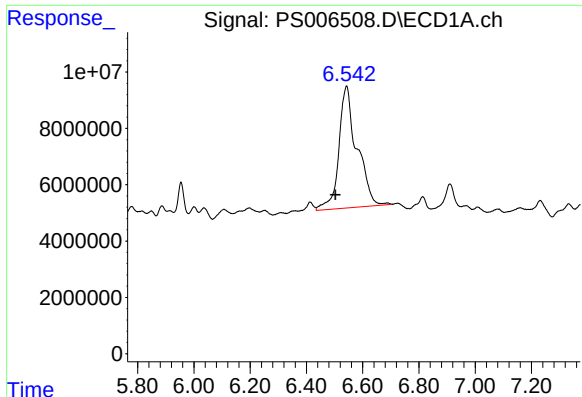

#9 2,4-D


R.T.: 6.543 min
Delta R.T.: 0.040 min
Response: 193001833
Conc: 236.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP9-COMP

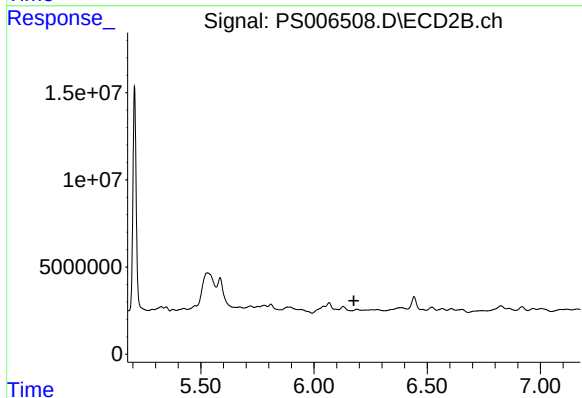


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

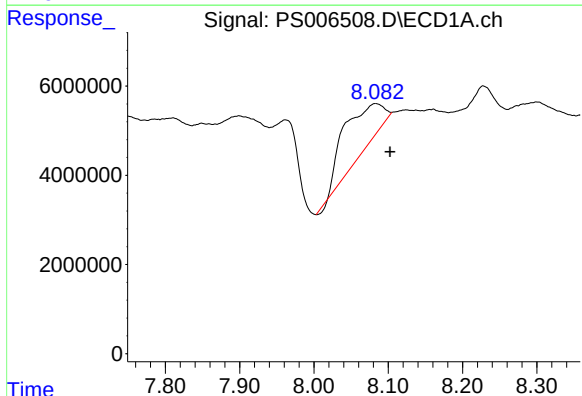


#13 2,4-DB

R.T.: 8.083 min
Delta R.T.: -0.019 min
Response: 35947998
Conc: 57.72 ng/ml

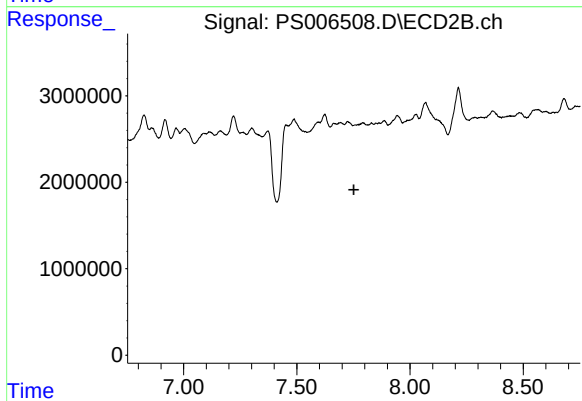

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.752 min
Response: 0
Conc: N.D.

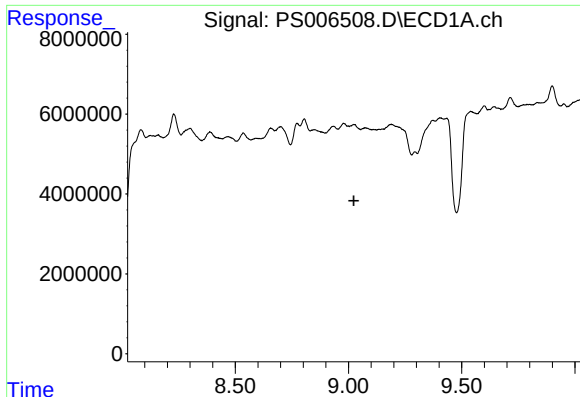

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 9.024 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP9-COMP

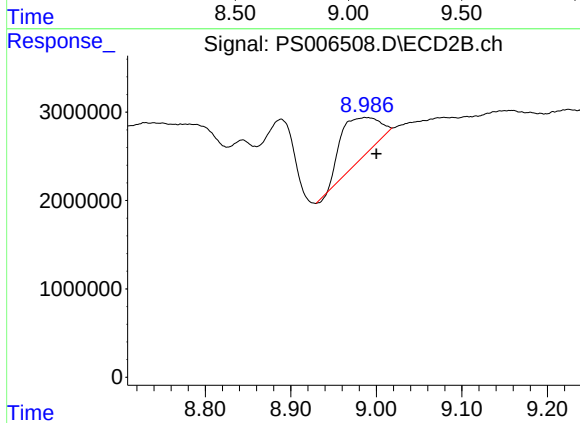


#15 Picloram

R.T.: 8.988 min
Delta R.T.: -0.012 min
Response: 14556783
Conc: 3.23 ng/ml

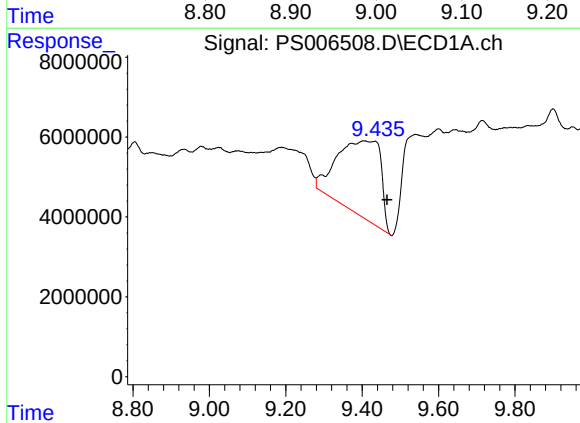

#16 DCPA

R.T.: 9.405 min
Delta R.T.: -0.060 min
Response: 149313700
Conc: 25.76 ng/ml

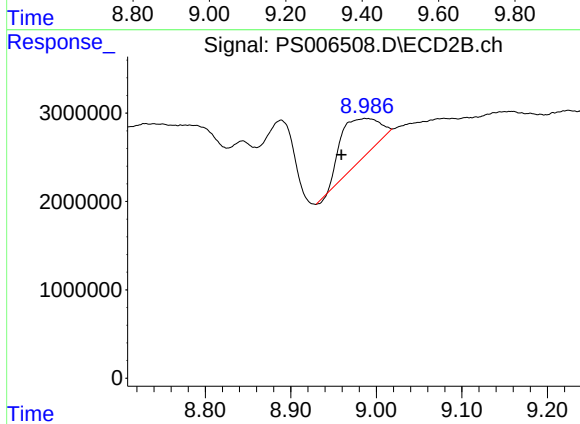

#16 DCPA

R.T.: 8.988 min
Delta R.T.: 0.029 min
Response: 14556783
Conc: 4.17 ng/ml