

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083119\
 Data File : PS006509.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2019 01:10
 Operator : SM\AJ
 Sample : K4619-30
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP10-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:13:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.480	5.211	192.6E6	91531312	223.080	186.095
Target Compounds							
1) T	Dalapon	2.114	0.000	5855712	0	5.374	N.D. #
5) T	DICAMBA	5.643	0.000	14184020	0	4.416	N.D. #
7) T	MCPA	5.958	5.588	21255996	35111922	6.733	17.180 #
9) T	2,4-D	6.544	0.000	137.6E6	0	168.847	N.D. #
10) T	Pentachlo...	0.000	6.568	0	13264994	N.D.	1.962
11) T	2,4,5-TP ...	7.231	0.000	25621041	0	5.616	N.D. #
13) T	2,4-DB	8.112	0.000	184.9E6	0	296.969	N.D. #
16) T	DCPA	9.444	0.000	45289555	0	7.815	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083119\
Data File : PS006509.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2019 01:10
Operator : SM\AJ
Sample : K4619-30
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP10-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:13:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

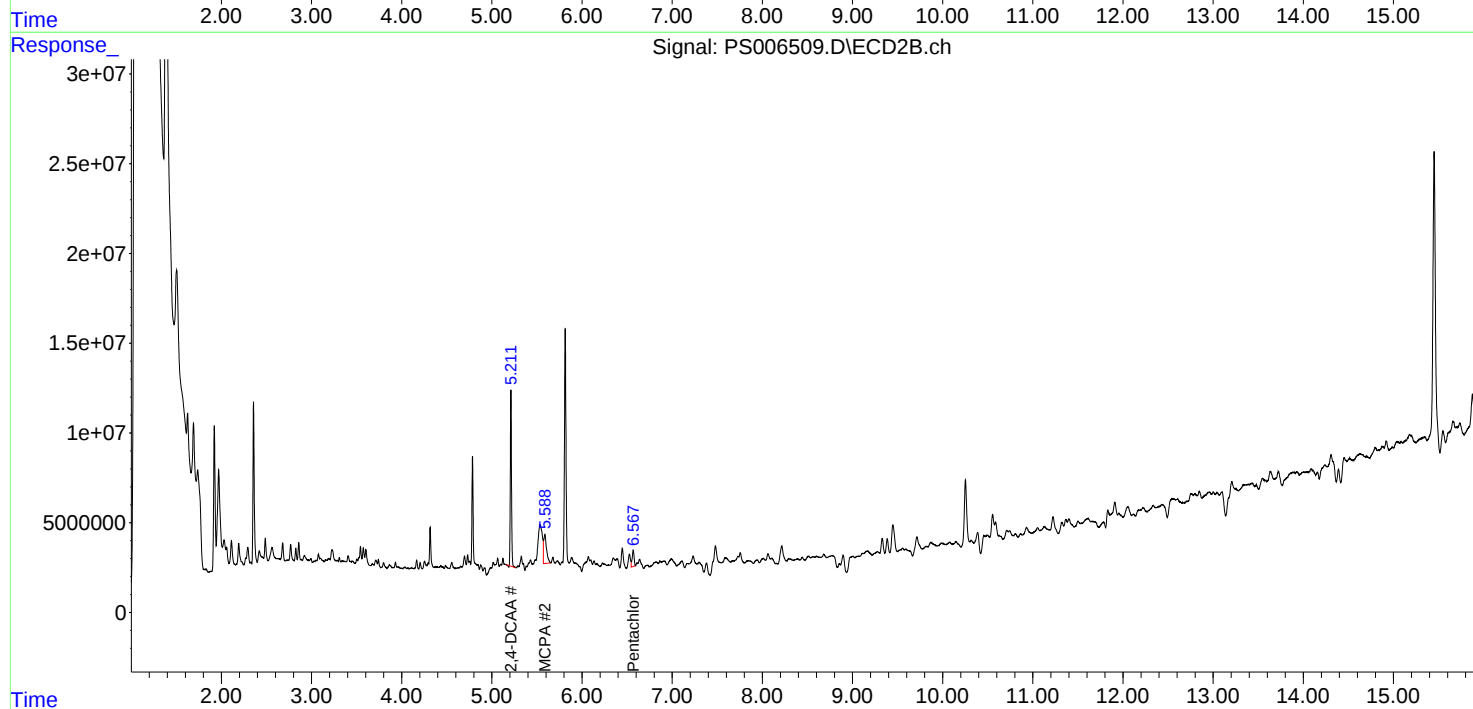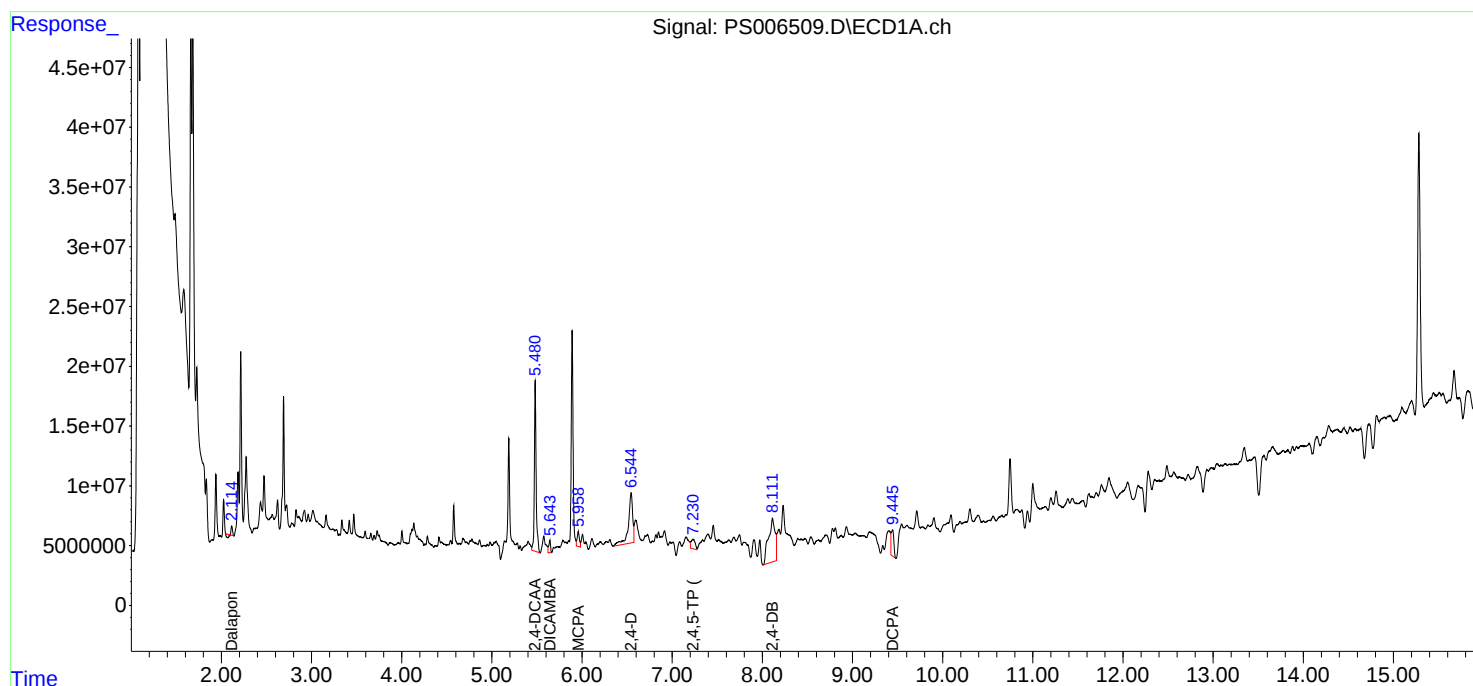


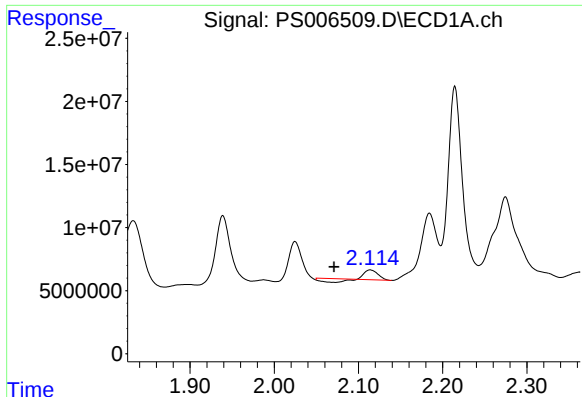

#1 Dalapon


R.T.: 2.114 min
Delta R.T.: 0.043 min
Response: 5855712
Conc: 5.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP10-COMP

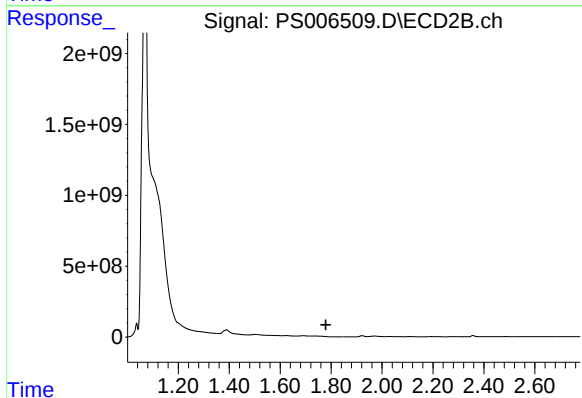


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.779 min
Response: 0
Conc: N.D.

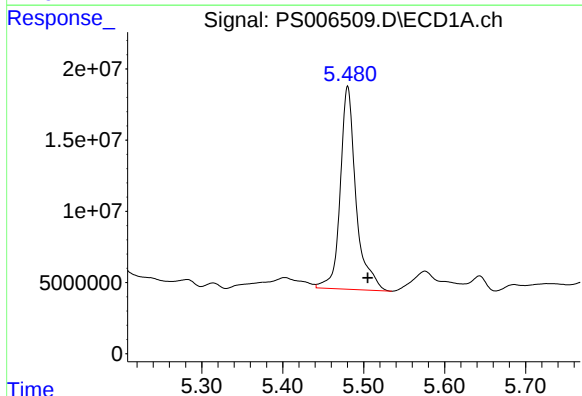


#4 2,4-DCAA

R.T.: 5.480 min
Delta R.T.: -0.025 min
Response: 192562501
Conc: 223.08 ng/ml

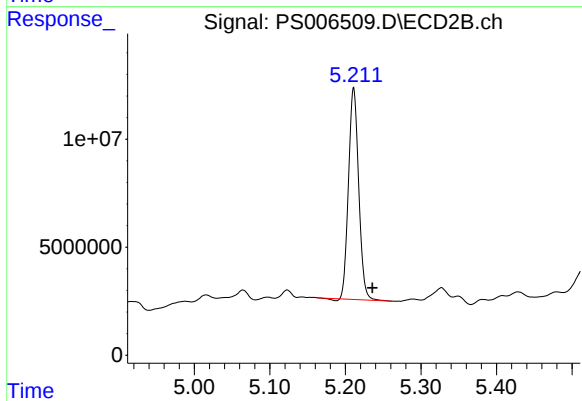

#4 2,4-DCAA


R.T.: 5.211 min
Delta R.T.: -0.025 min
Response: 91531312
Conc: 186.10 ng/ml

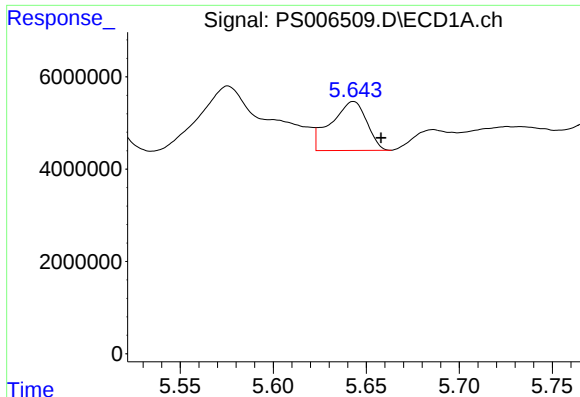

#5 DICAMBA


R.T.: 5.643 min
Delta R.T.: -0.015 min
Response: 14184020
Conc: 4.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP10-COMP

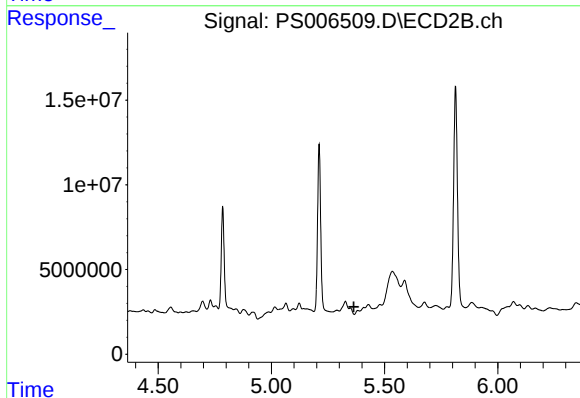


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.364 min
Response: 0
Conc: N.D.

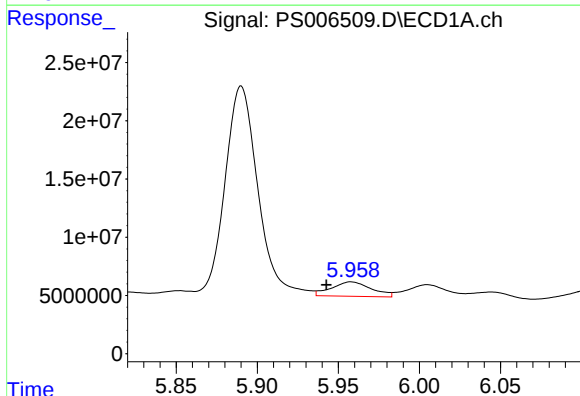


#7 MCPA

R.T.: 5.958 min
Delta R.T.: 0.015 min
Response: 21255996
Conc: 6.73 ug/ml

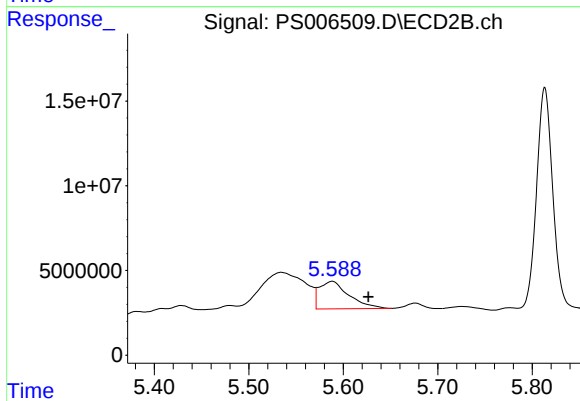

#7 MCPA


R.T.: 5.588 min
Delta R.T.: -0.038 min
Response: 35111922
Conc: 17.18 ug/ml

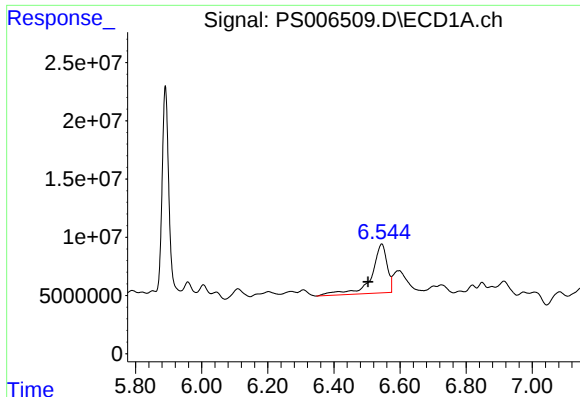

#9 2,4-D


R.T.: 6.544 min
Delta R.T.: 0.042 min
Response: 137573882
Conc: 168.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP10-COMP

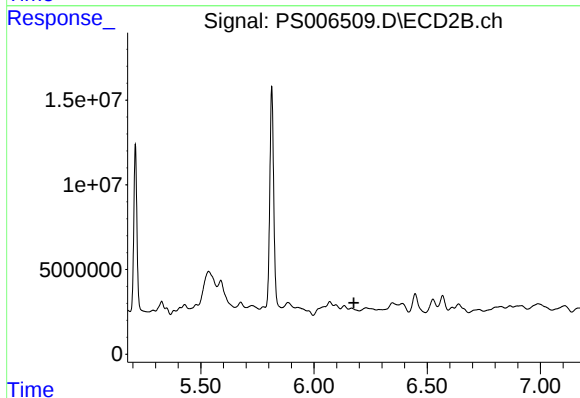


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

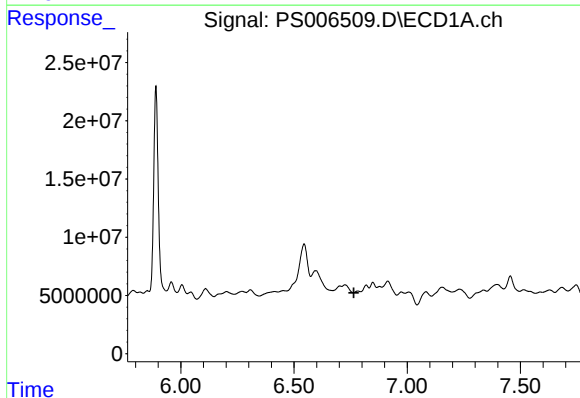


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.764 min
Response: 0
Conc: N.D.

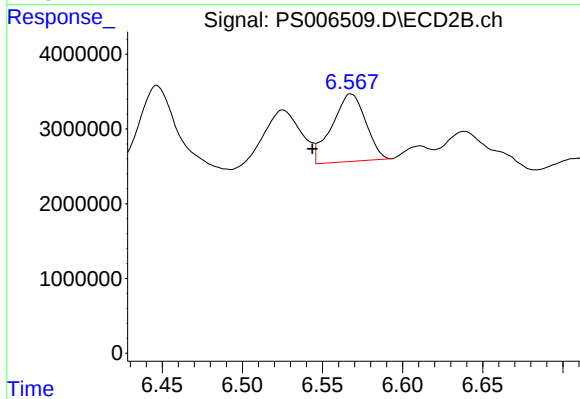

#10 Pentachlorophenol


R.T.: 6.568 min
Delta R.T.: 0.024 min
Response: 13264994
Conc: 1.96 ng/ml

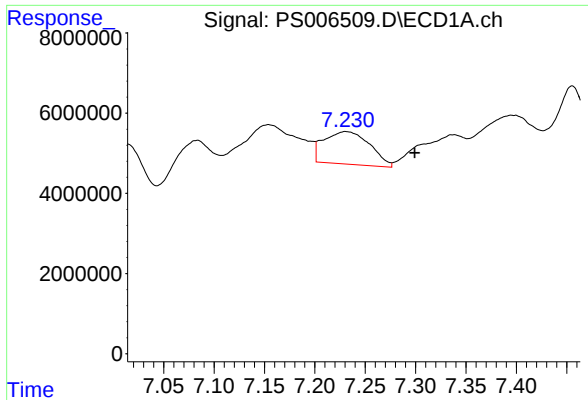

#11 2,4,5-TP (SILVEX)


R.T.: 7.231 min
Delta R.T.: -0.068 min
Response: 25621041
Conc: 5.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP10-COMP

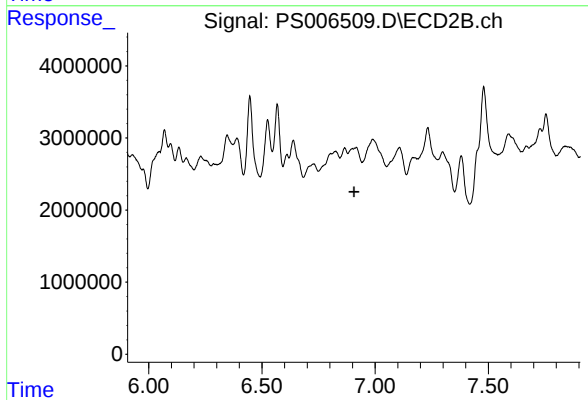


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 6.907 min
Response: 0
Conc: N.D.

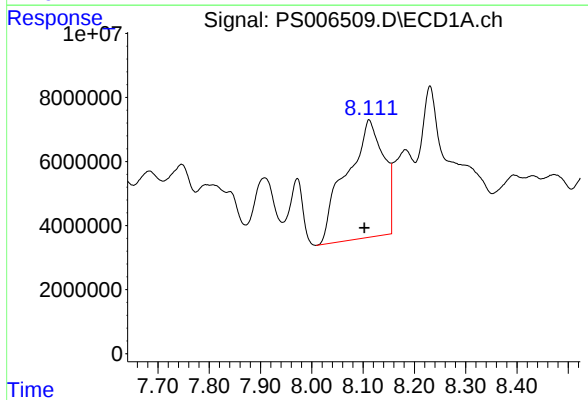


#13 2,4-DB

R.T.: 8.112 min
Delta R.T.: 0.010 min
Response: 184947878
Conc: 296.97 ng/ml

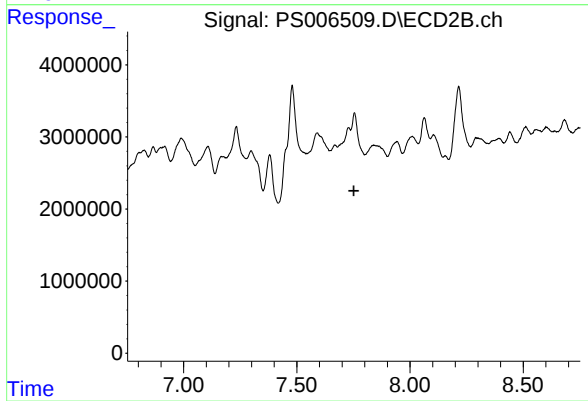

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.752 min
Response: 0
Conc: N.D.

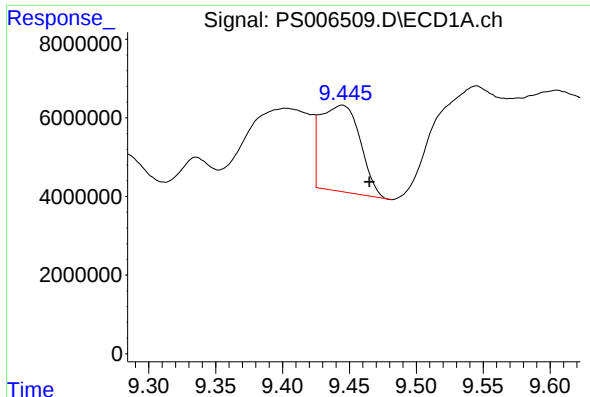

#16 DCPA

R.T.: 9.444 min
Delta R.T.: -0.021 min
Response: 45289555
Conc: 7.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP10-COMP

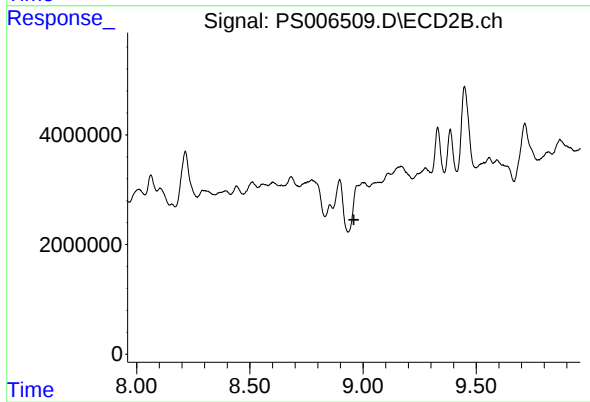

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 8.959 min
Response: 0
Conc: N.D.