

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083119\
 Data File : PS006510.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2019 01:32
 Operator : SM\AJ
 Sample : K4619-33
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP11-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:14:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.500	5.230	212.7E6	104.7E6	246.465	212.826
Target Compounds							
1) T	Dalapon	2.044	1.757	41336003	166.6E6	37.936	265.429 #
3) T	4-Nitroph...	5.305	0.000	4222992	0	11.249	N.D. #
5) T	DICAMBA	5.665	0.000	11337886	0	3.530	N.D. #
7) T	MCPA	0.000	5.606	0	33139638	N.D.	16.215
9) T	2,4-D	6.568	0.000	203.2E6	0	249.447	N.D. #
11) T	2,4,5-TP ...	7.253	0.000	23679013	0	5.191	N.D. #
13) T	2,4-DB	8.145	0.000	88808735	0	142.599	N.D. #
15) T	Picloram	0.000	9.011	0	22730452	N.D.	5.039
16) T	DCPA	9.465	9.011	47192217	22730452	8.143	6.518



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083119\
Data File : PS006510.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2019 01:32
Operator : SM\AJ
Sample : K4619-33
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP11-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:14:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

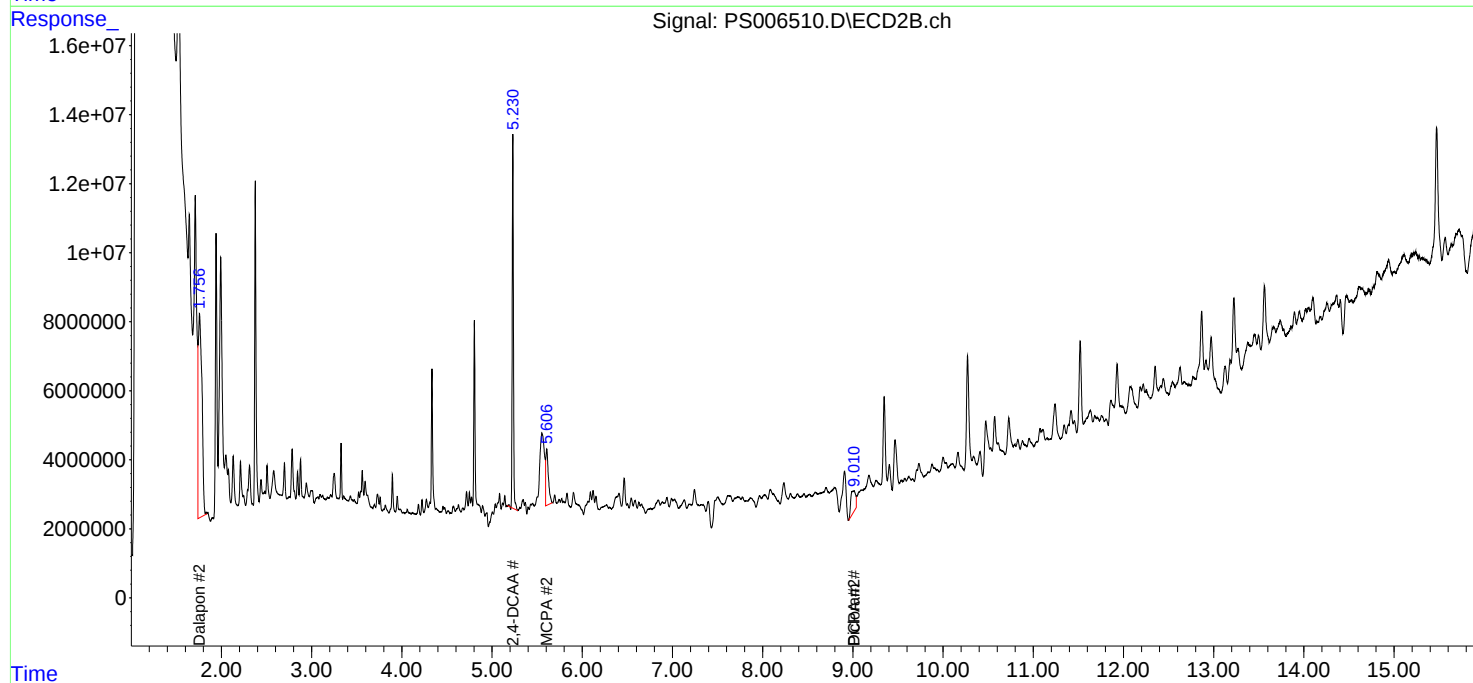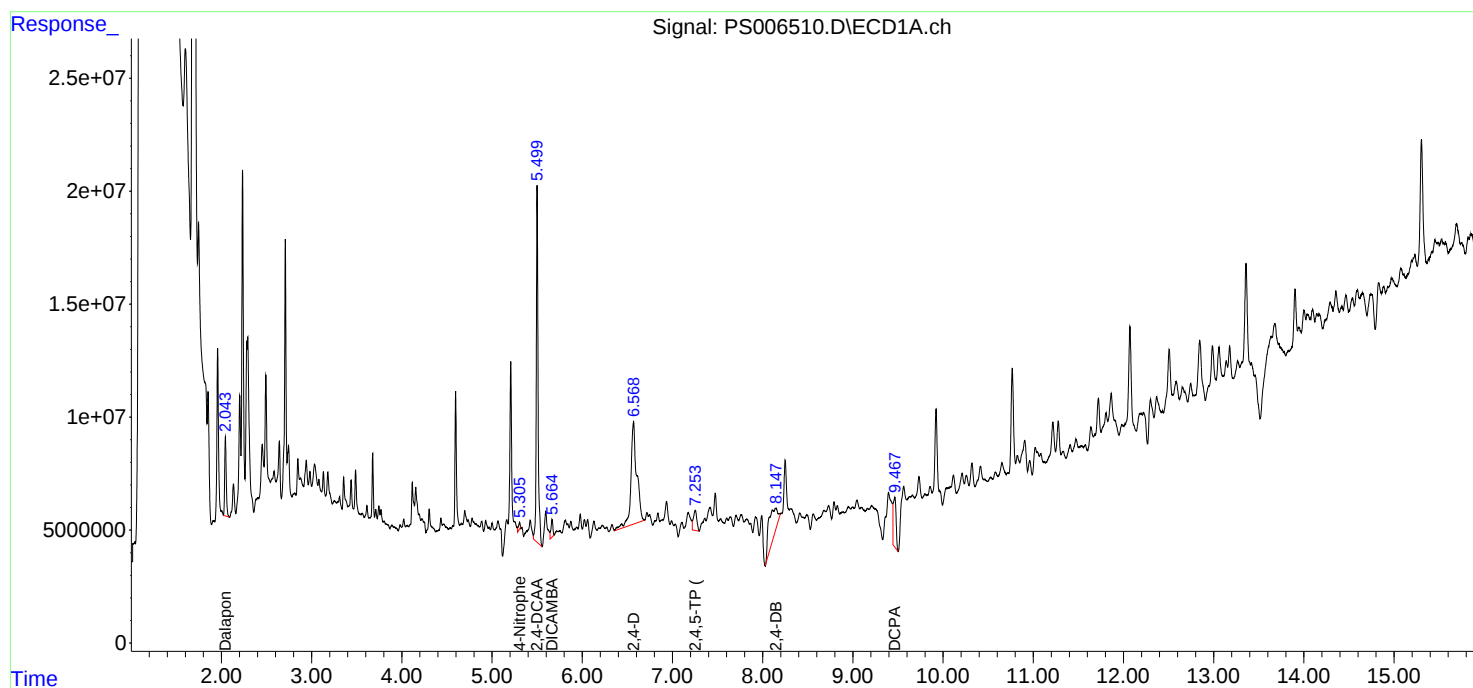


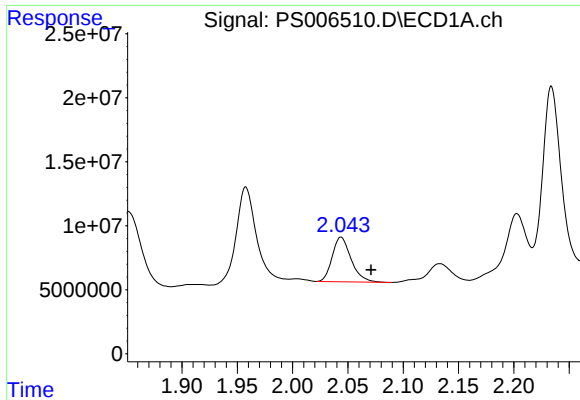

#1 Dalapon


R.T.: 2.044 min
Delta R.T.: -0.027 min
Response: 41336003
Conc: 37.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP11-COMP

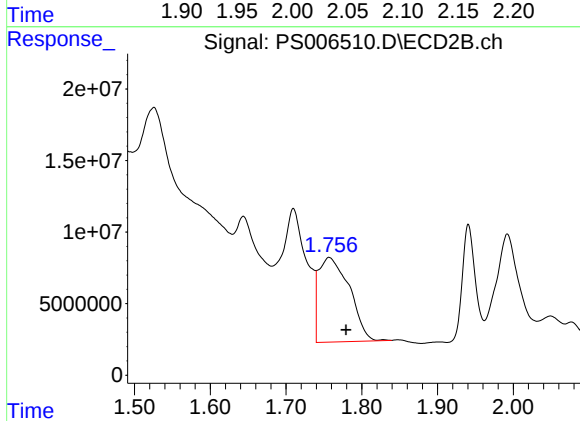


#1 Dalapon

R.T.: 1.757 min
Delta R.T.: -0.022 min
Response: 166554714
Conc: 265.43 ng/ml

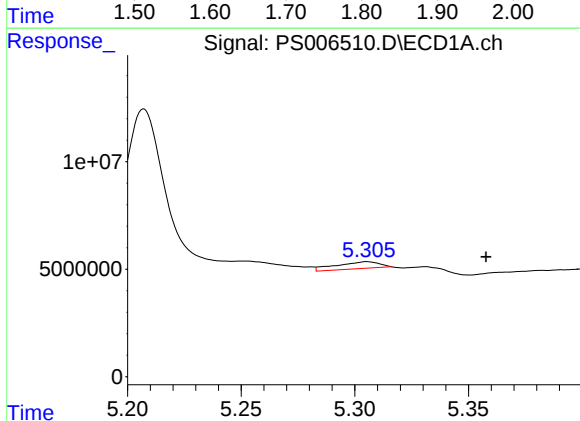


#3 4-Nitrophenol

R.T.: 5.305 min
Delta R.T.: -0.053 min
Response: 4222992
Conc: 11.25 ng/ml

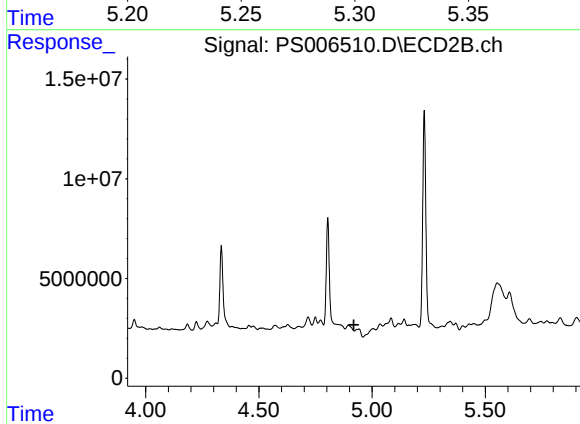

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.920 min
Response: 0
Conc: N.D.

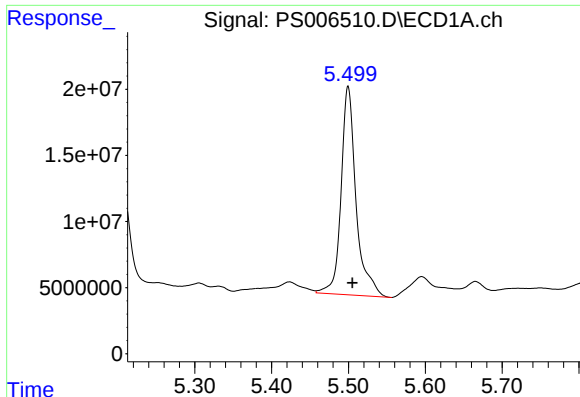

#4 2,4-DCAA


R.T.: 5.500 min
Delta R.T.: -0.006 min
Response: 212748839
Conc: 246.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP11-COMP

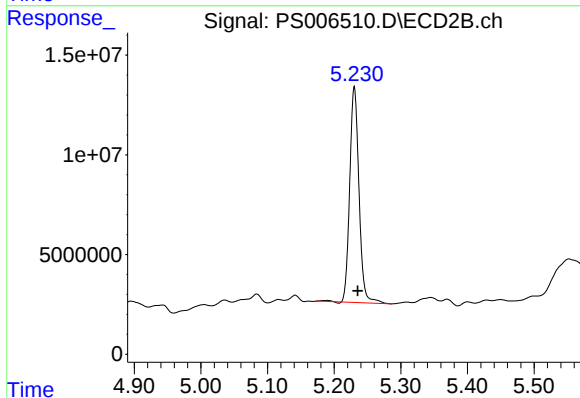


#4 2,4-DCAA

R.T.: 5.230 min
Delta R.T.: -0.005 min
Response: 104679089
Conc: 212.83 ng/ml

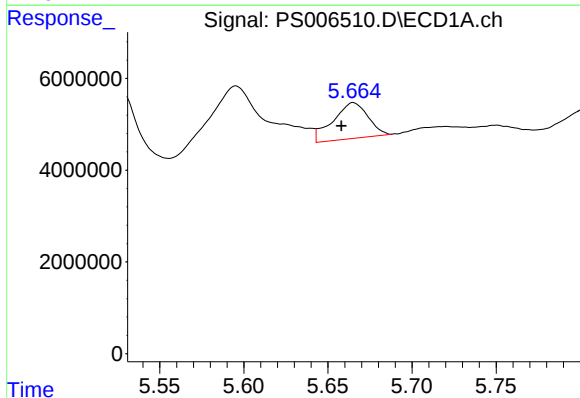


#5 DICAMBA

R.T.: 5.665 min
Delta R.T.: 0.007 min
Response: 11337886
Conc: 3.53 ng/ml

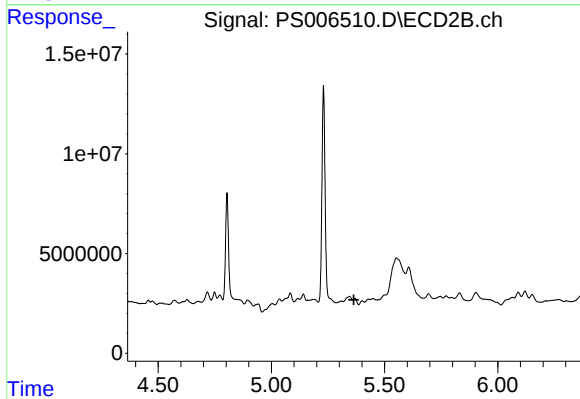

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.364 min
Response: 0
Conc: N.D.

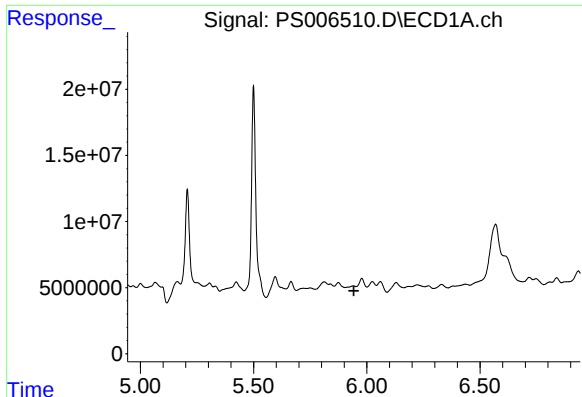

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.943 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP11-COMP

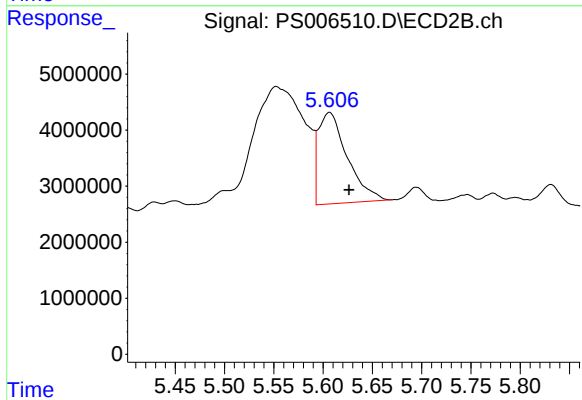


#7 MCPA

R.T.: 5.606 min
Delta R.T.: -0.020 min
Response: 33139638
Conc: 16.22 ug/ml

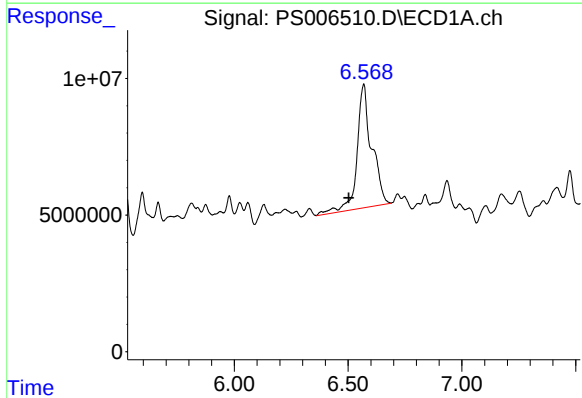


#9 2,4-D

R.T.: 6.568 min
Delta R.T.: 0.066 min
Response: 203245891
Conc: 249.45 ng/ml

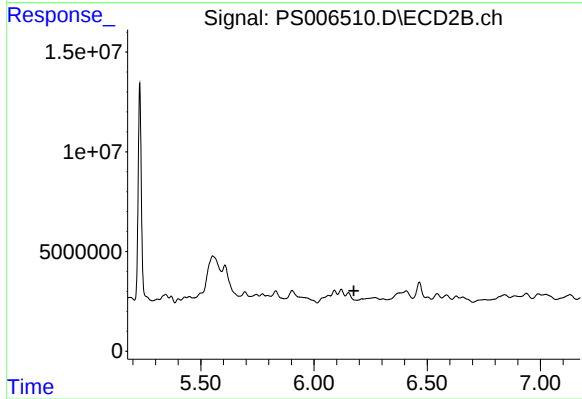

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

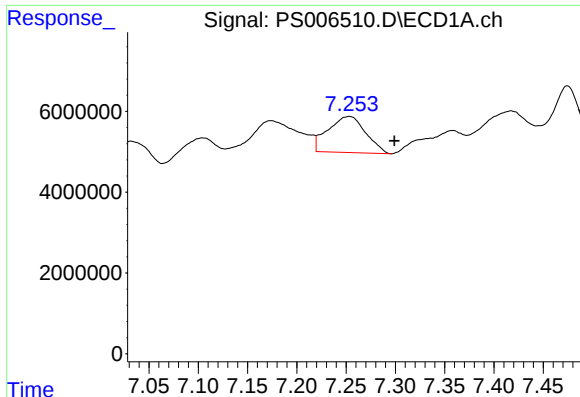

#11 2,4,5-TP (SILVEX)


R.T.: 7.253 min
Delta R.T.: -0.046 min
Response: 23679013
Conc: 5.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP11-COMP

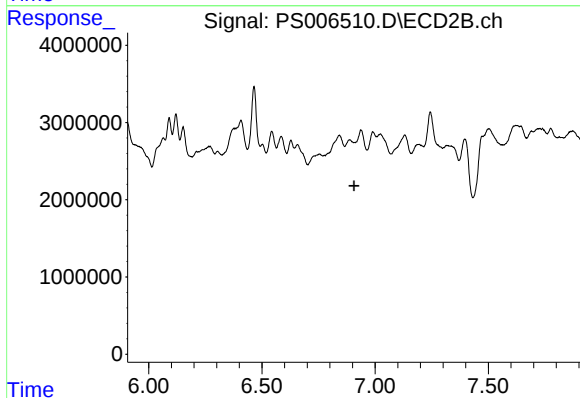


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 6.907 min
Response: 0
Conc: N.D.

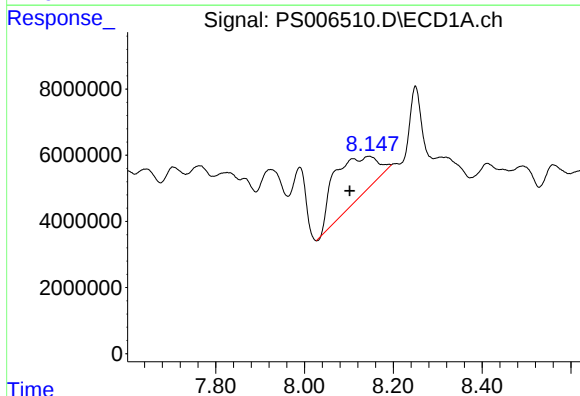


#13 2,4-DB

R.T.: 8.145 min
Delta R.T.: 0.043 min
Response: 88808735
Conc: 142.60 ng/ml

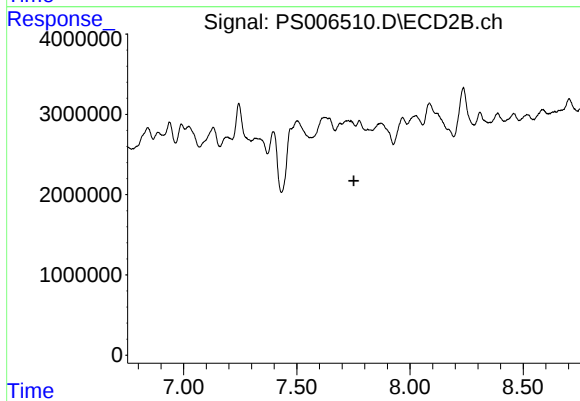

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.752 min
Response: 0
Conc: N.D.

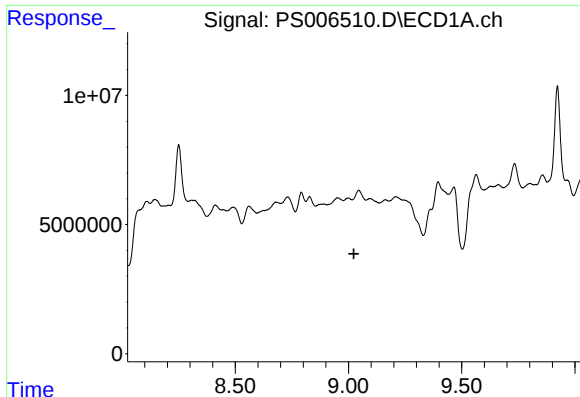

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 9.024 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP11-COMP

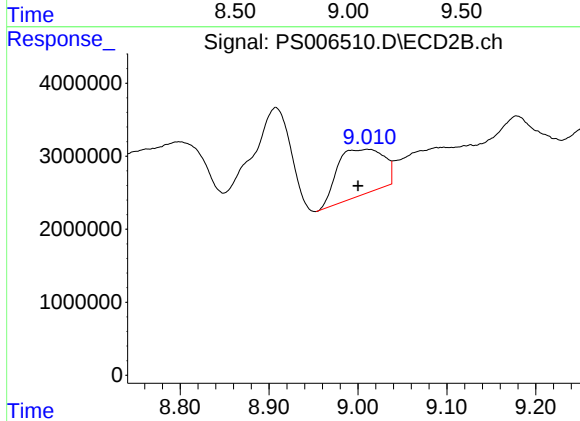


#15 Picloram

R.T.: 9.011 min
Delta R.T.: 0.011 min
Response: 22730452
Conc: 5.04 ng/ml

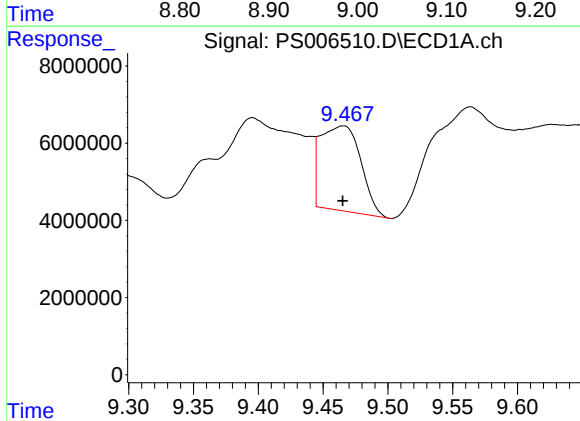

#16 DCPA

R.T.: 9.465 min
Delta R.T.: 0.000 min
Response: 47192217
Conc: 8.14 ng/ml

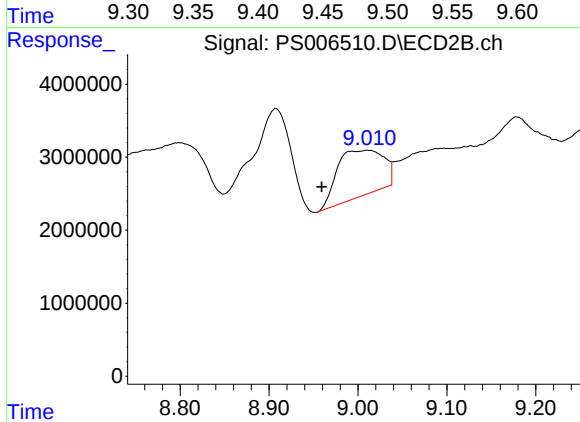

#16 DCPA

R.T.: 9.011 min
Delta R.T.: 0.052 min
Response: 22730452
Conc: 6.52 ng/ml