

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083122\
 Data File : PS020393.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2022 08:42
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:15:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.191	6.732	406819	1257657	<MDL	1.543 #
Target Compounds							
1) T	Dalapon	2.975	0.000	489959	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.450f	0.000	9367510	0	2.408	N.D. #
3) T	4-Nitroph...	7.049	6.402	16288451	692036	11.727	1.409 #
5) T	DICAMBA	7.381	6.985f	730540	4239976	<MDL	1.190 #
6) T	MCPD	7.541	6.985	1315505	4239976	<MDL	1.554 #
7) T	MCPA	7.679	0.000	14723349	0	1.143	N.D. #
8) T	DICHLORPROP	8.011f	0.000	5795961	0	2.025	N.D. #
10) T	Pentachlo...	8.605	0.000	3946786	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.162	0.000	583348	0	<MDL	N.D. #
12) T	2,4,5-T	9.400	9.040f	61617498	6115058	3.395	1.201 #
15) T	Picloram	10.956	10.843	77839098	36686415	2.462	4.863 #
16) T	DCPA	11.401	0.000	8691342	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083122\
Data File : PS020393.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2022 08:42
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:15:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

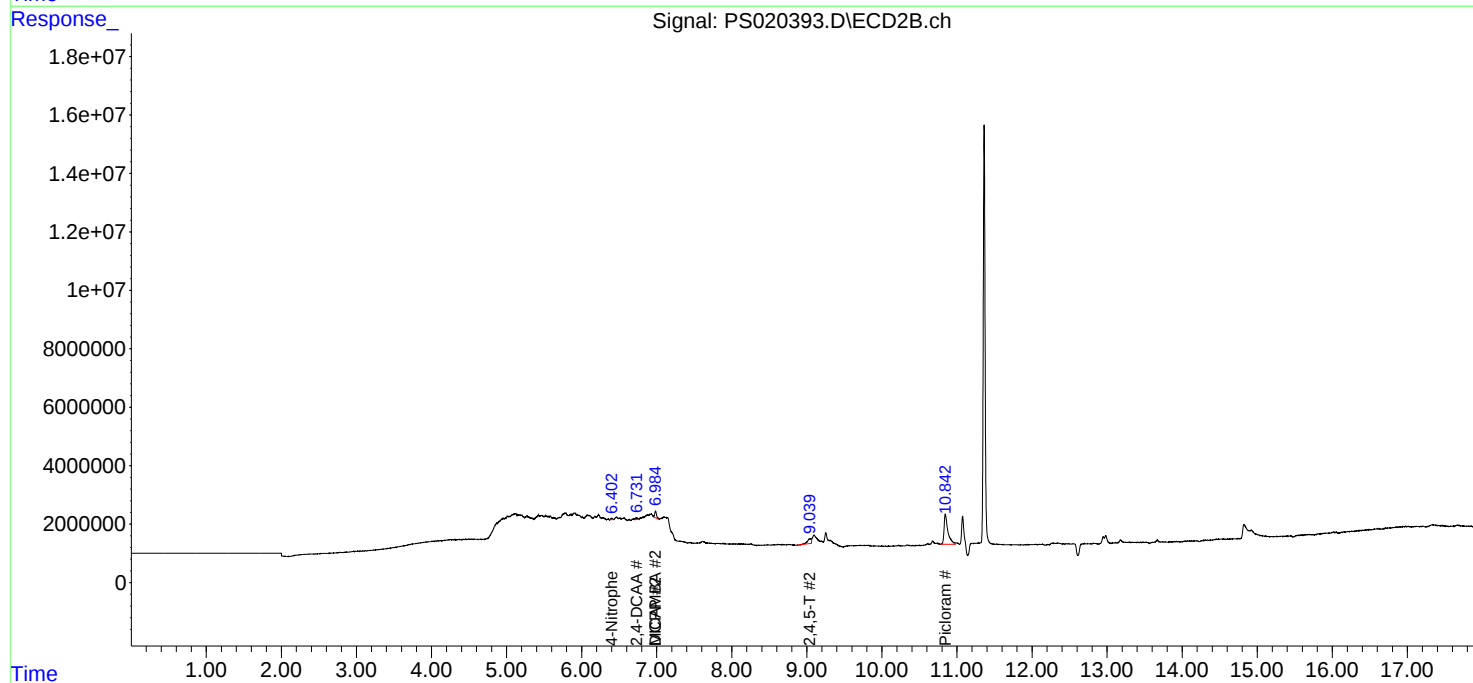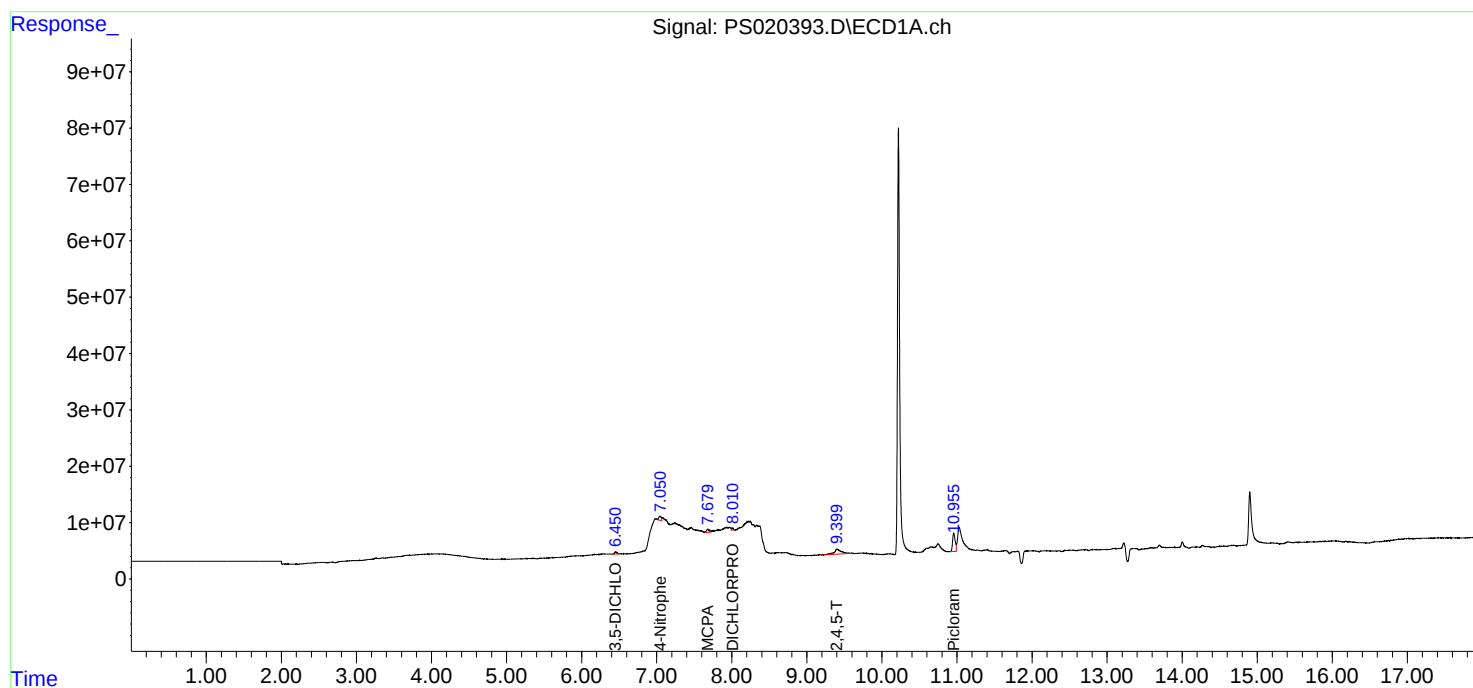


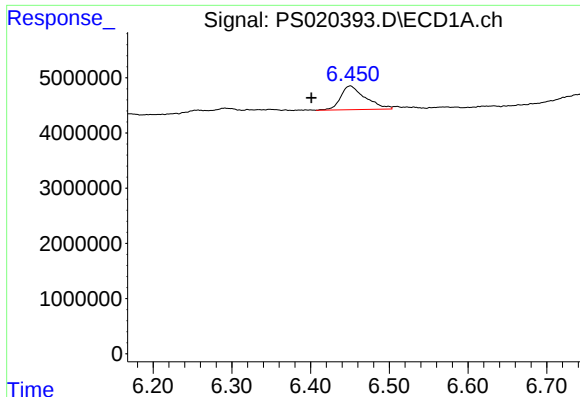

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.450 min
Delta R.T.: 0.049 min
Response: 9367510
Conc: 2.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

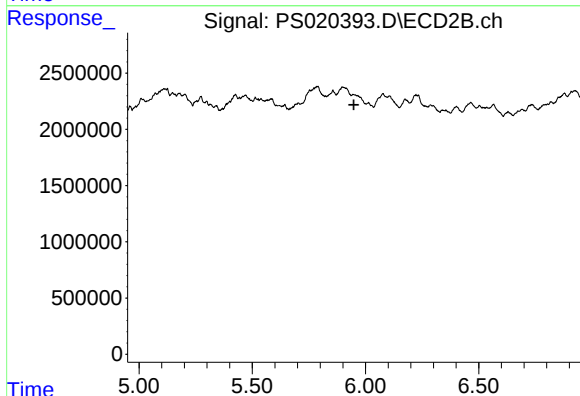


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

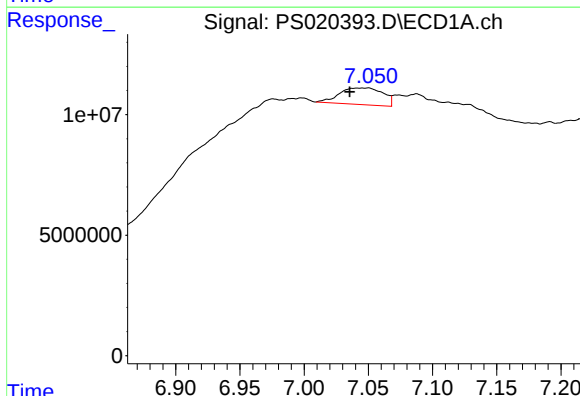


#3 4-Nitrophenol

R.T.: 7.049 min
Delta R.T.: 0.014 min
Response: 16288451
Conc: 11.73 ng/ml

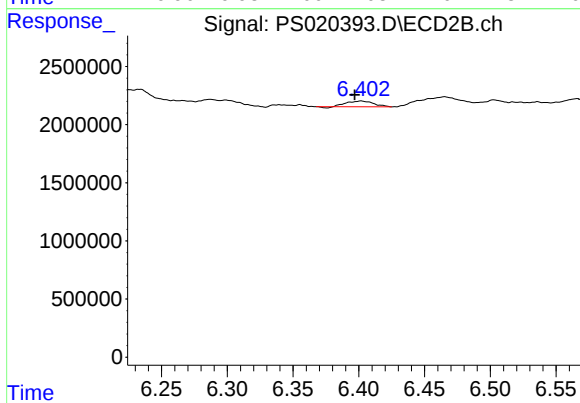

#3 4-Nitrophenol


R.T.: 6.402 min
Delta R.T.: 0.005 min
Response: 692036
Conc: 1.41 ng/ml

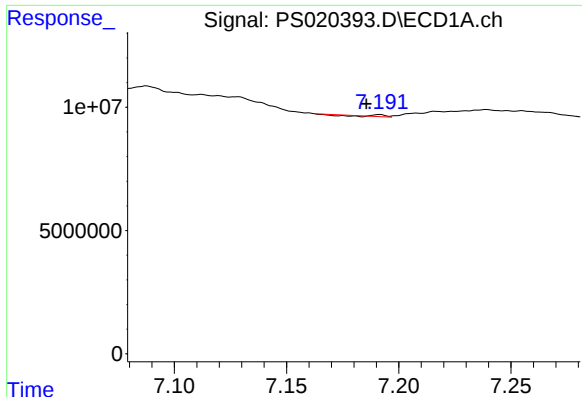

#4 2,4-DCAA


R.T.: 7.191 min
Delta R.T.: 0.006 min
Response: 406819
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

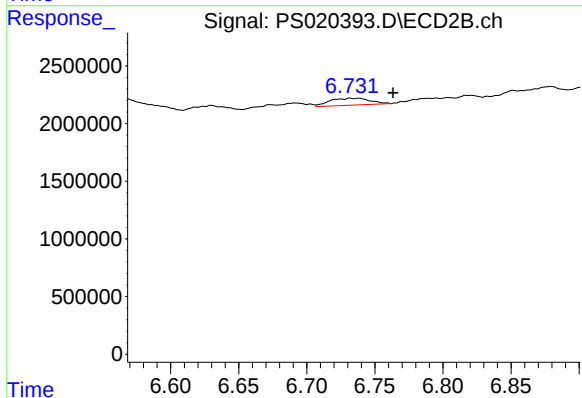


#4 2,4-DCAA

R.T.: 6.732 min
Delta R.T.: -0.031 min
Response: 1257657
Conc: 1.54 ng/ml

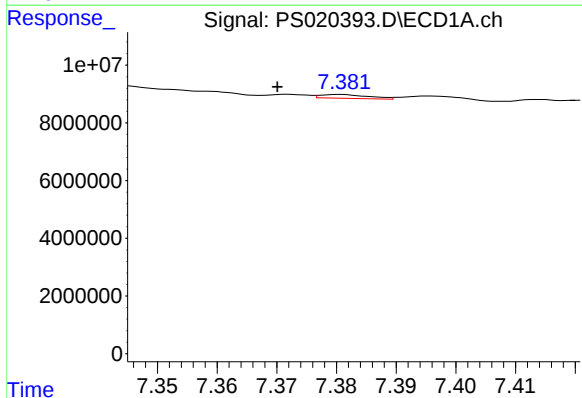


#5 DICAMBA

R.T.: 7.381 min
Delta R.T.: 0.010 min
Response: 730540
Conc: N.D.

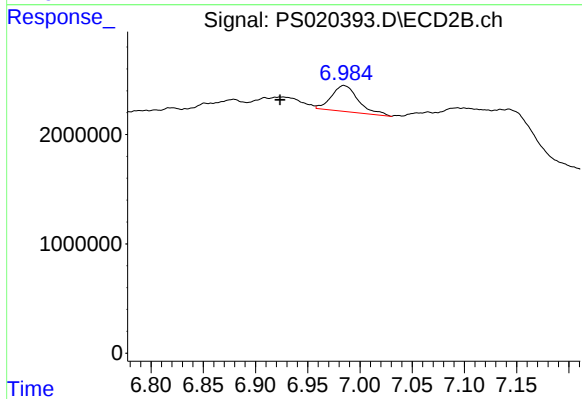

#5 DICAMBA


R.T.: 6.985 min
Delta R.T.: 0.061 min
Response: 4239976
Conc: 1.19 ng/ml

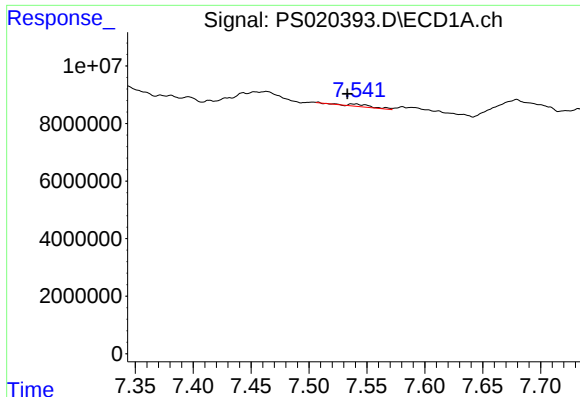

#6 MCPP


R.T.: 7.541 min
Delta R.T.: 0.007 min
Response: 1315505
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

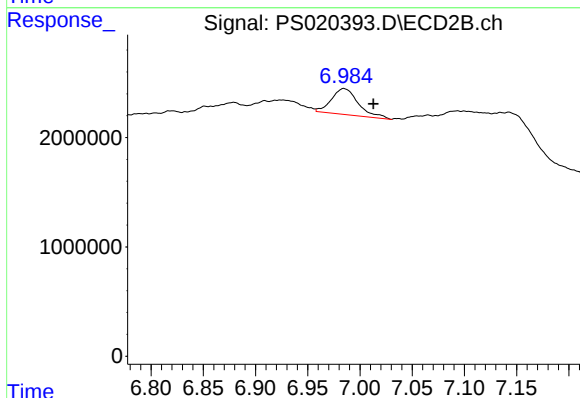


#6 MCPP

R.T.: 6.985 min
Delta R.T.: -0.028 min
Response: 4239976
Conc: 1.55 ug/ml

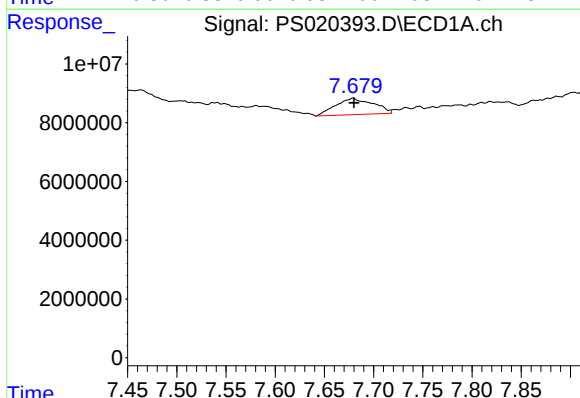


#7 MCPA

R.T.: 7.679 min
Delta R.T.: -0.001 min
Response: 14723349
Conc: 1.14 ug/ml

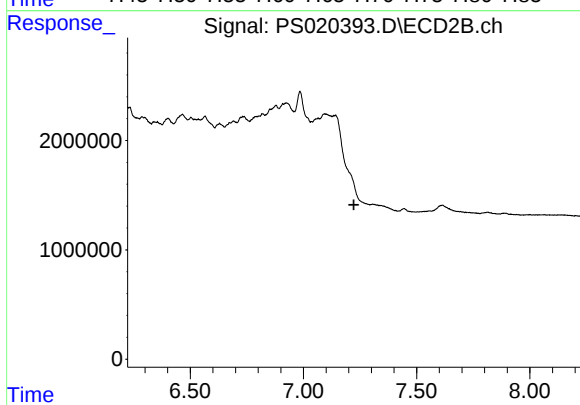

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.223 min
Response: 0
Conc: N.D.

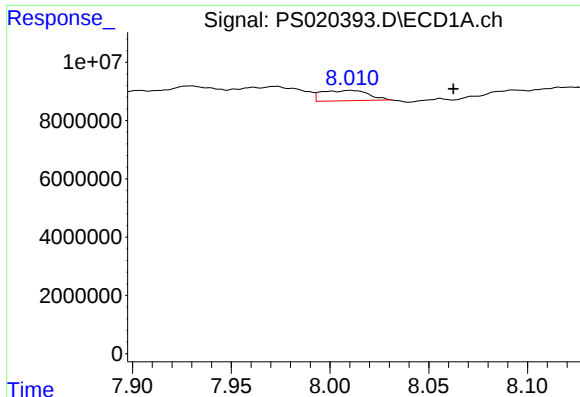

#8 DICHLORPROP


R.T.: 8.011 min
Delta R.T.: -0.052 min
Response: 5795961
Conc: 2.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

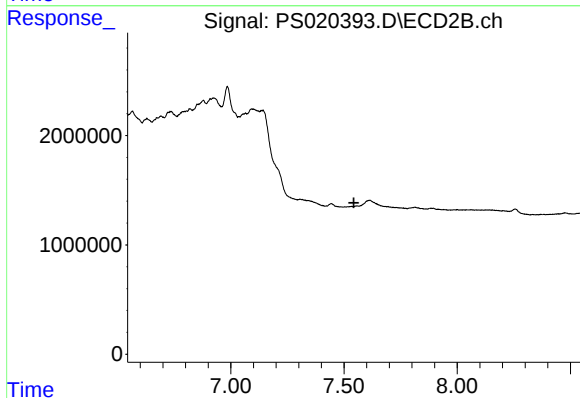


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.544 min
Response: 0
Conc: N.D.

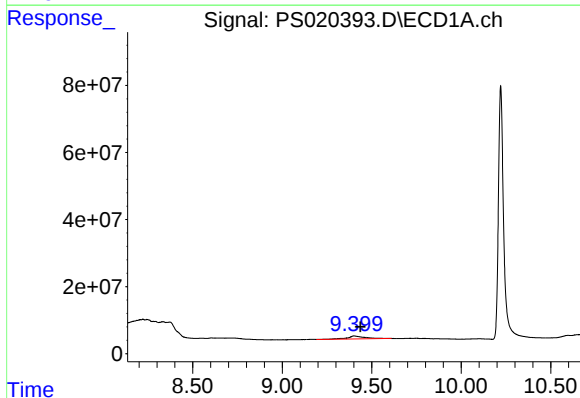


#12 2,4,5-T

R.T.: 9.400 min
Delta R.T.: -0.036 min
Response: 61617498
Conc: 3.39 ng/ml

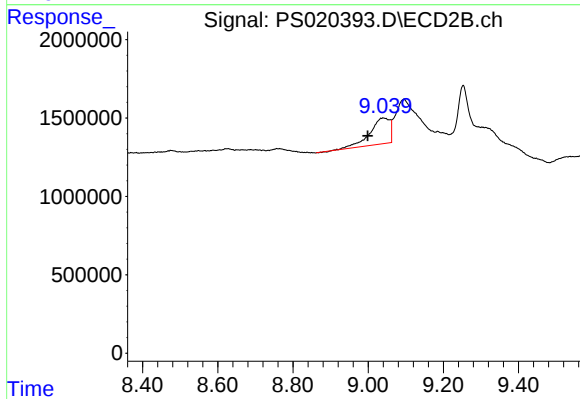

#12 2,4,5-T


R.T.: 9.040 min
Delta R.T.: 0.041 min
Response: 6115058
Conc: 1.20 ng/ml

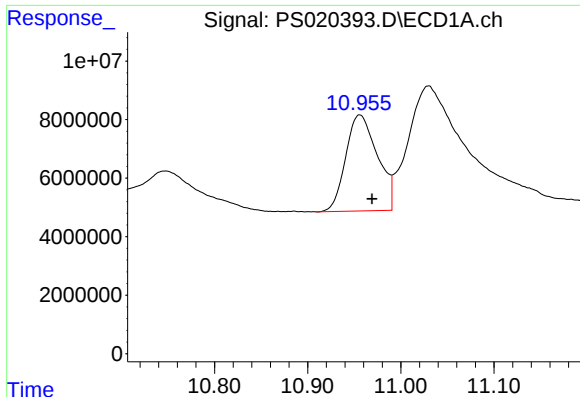

#15 Picloram

R.T.: 10.956 min
Delta R.T.: -0.013 min
Response: 77839098
Conc: 2.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

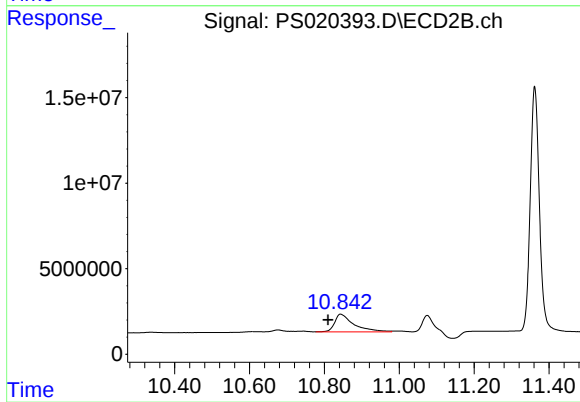

#15 Picloram

R.T.: 10.843 min
Delta R.T.: 0.032 min
Response: 36686415
Conc: 4.86 ng/ml