

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083122\
 Data File : PS020394.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2022 09:06
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:16:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.187	6.763	1452.9E6	419.3E6	492.714	514.468
Target Compounds							
2) T	3,5-DICHL...	6.461f	0.000	45468709	0	11.689	N.D. #
5) T	DICAMBA	0.000	6.992f	0	11206593	N.D.	3.144
6) T	MCP	0.000	6.992	0	11206593	N.D.	4.108
7) T	MCPA	7.663	0.000	488819	0	<MDL	N.D. #
9) T	2,4-D	8.366f	0.000	3981910	0	1.322	N.D. #
11) T	2,4,5-TP ...	9.184	0.000	1991836	0	<MDL	N.D. #
12) T	2,4,5-T	9.484f	0.000	15694890	0	<MDL	N.D. #
13) T	2,4-DB	9.954	0.000	660609	0	<MDL	N.D. #
14) T	DINOSEB	11.095	0.000	100.2E6	0	6.298	N.D. #
15) T	Picloram	10.969	0.000	117.9E6	0	3.729	N.D. #
16) T	DCPA	11.407	10.694f	683827	3347996	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083122\
Data File : PS020394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2022 09:06
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:16:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

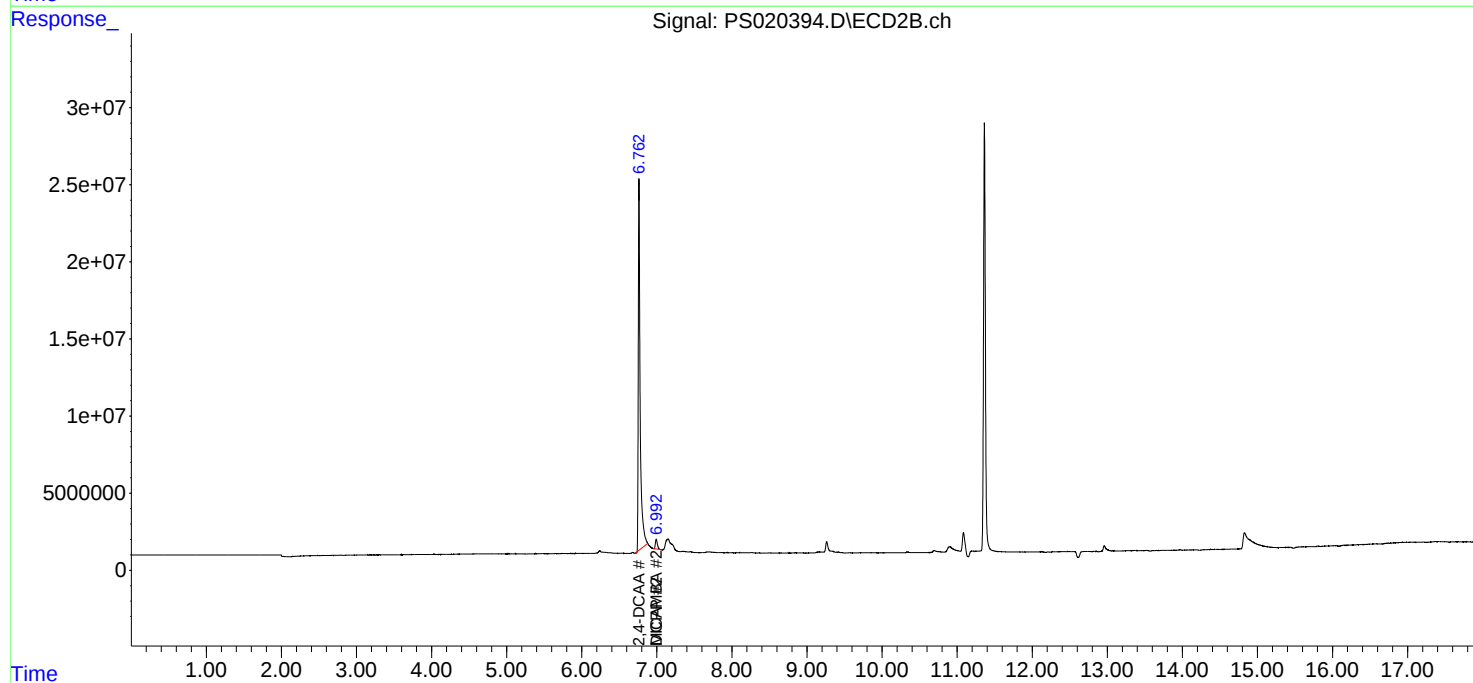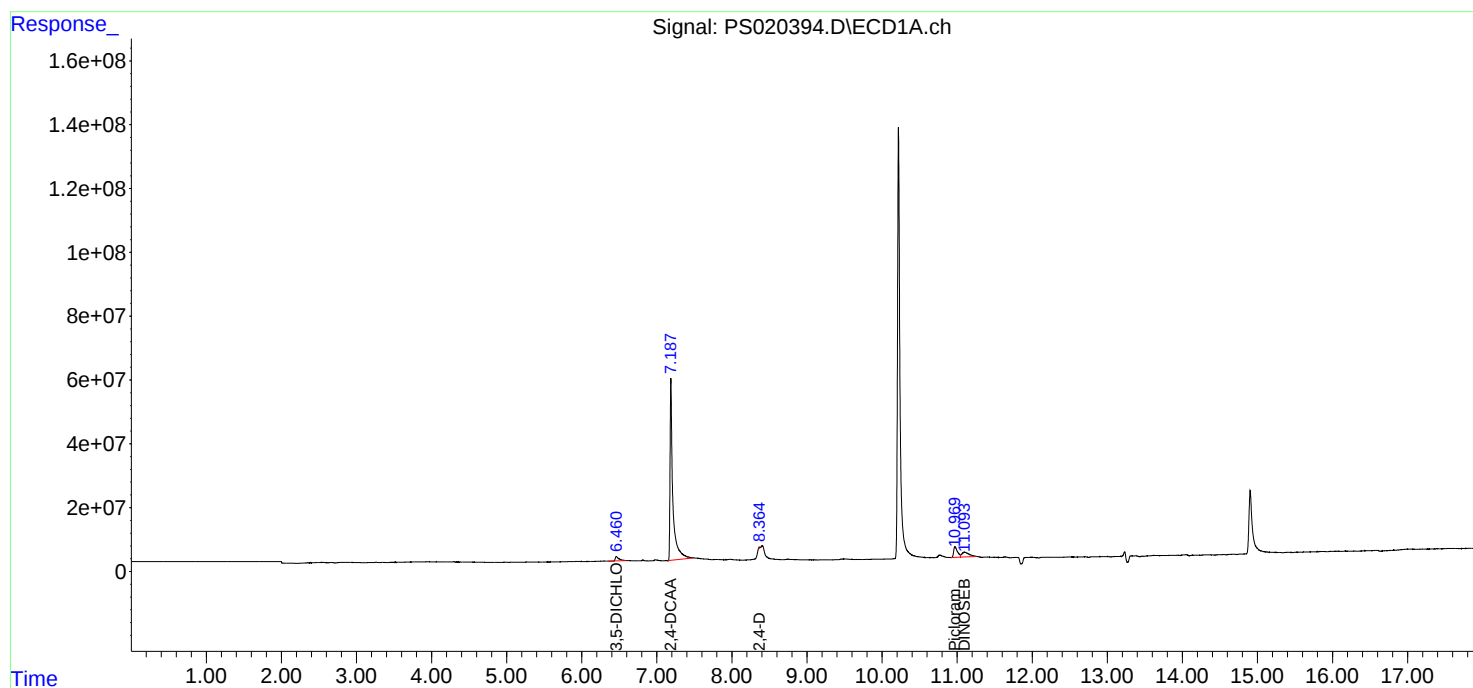


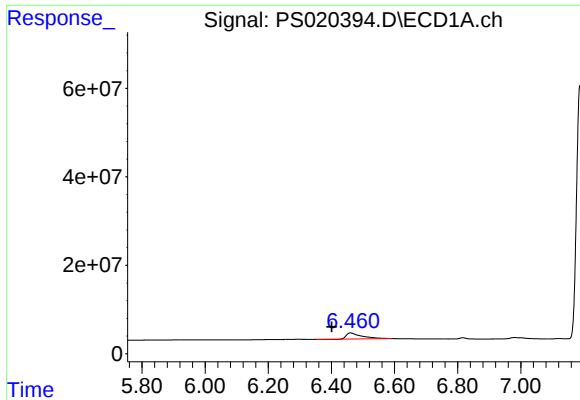

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.461 min
Delta R.T.: 0.060 min
Response: 45468709
Conc: 11.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

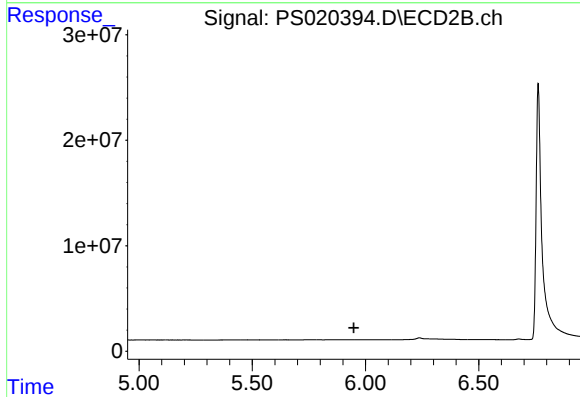


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

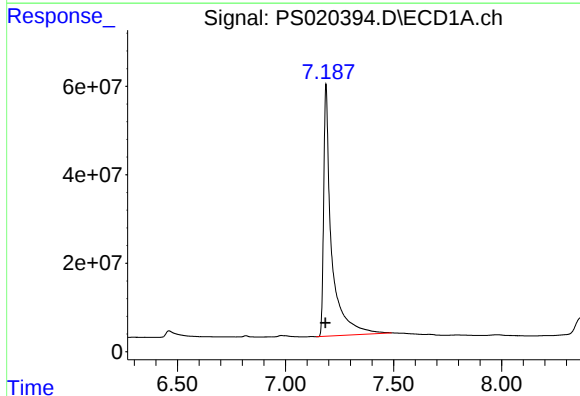


#4 2,4-DCAA

R.T.: 7.187 min
Delta R.T.: 0.002 min
Response: 1452878324
Conc: 492.71 ng/ml

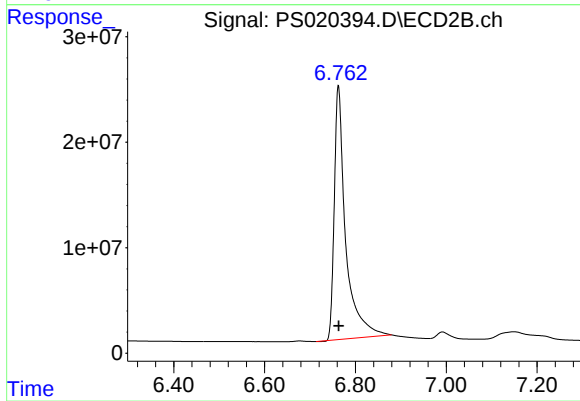

#4 2,4-DCAA


R.T.: 6.763 min
Delta R.T.: 0.000 min
Response: 419269009
Conc: 514.47 ng/ml

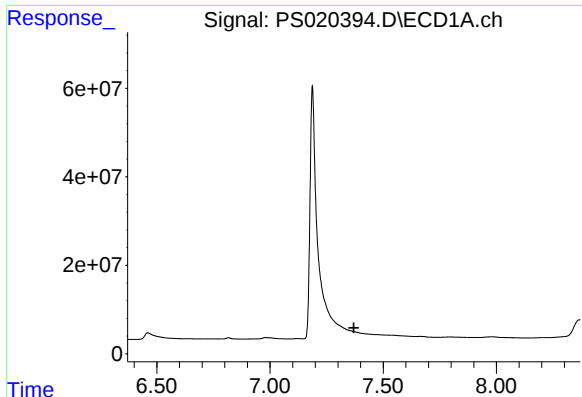

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.370 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

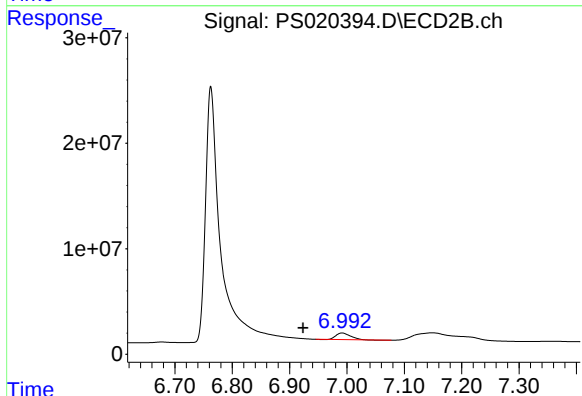


#5 DICAMBA

R.T.: 6.992 min
Delta R.T.: 0.068 min
Response: 11206593
Conc: 3.14 ng/ml

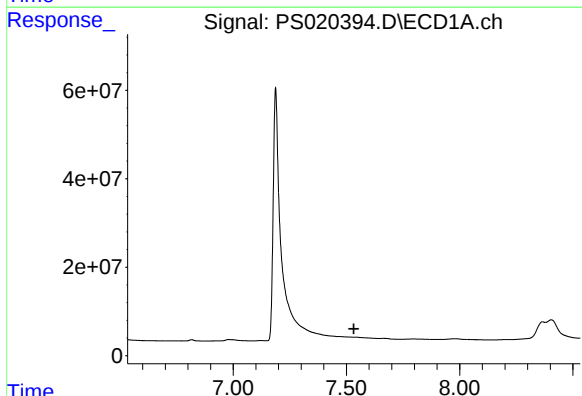


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.533 min
Response: 0
Conc: N.D.

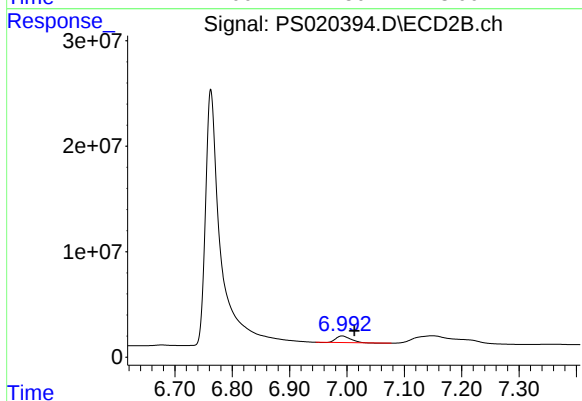

#6 MCP


R.T.: 6.992 min
Delta R.T.: -0.021 min
Response: 11206593
Conc: 4.11 ug/ml

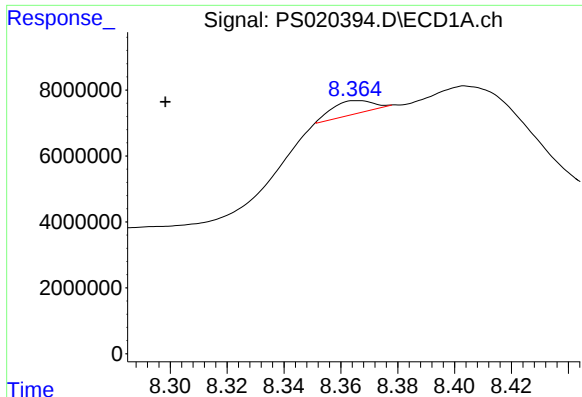

#9 2,4-D


R.T.: 8.366 min
Delta R.T.: 0.068 min
Response: 3981910
Conc: 1.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

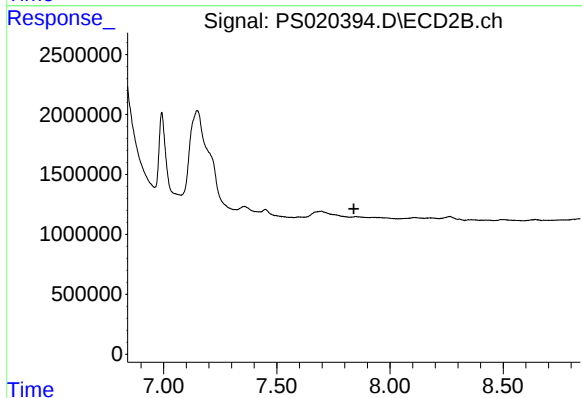


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.840 min
Response: 0
Conc: N.D.

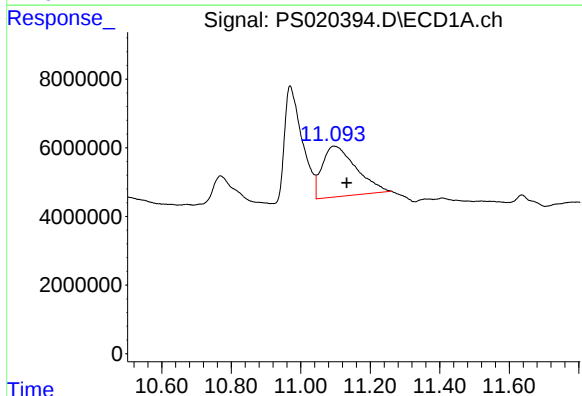


#14 DINOSEB

R.T.: 11.095 min
Delta R.T.: -0.037 min
Response: 100201581
Conc: 6.30 ng/ml

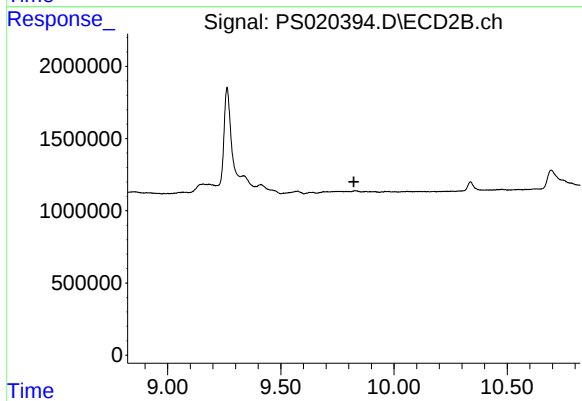

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.823 min
Response: 0
Conc: N.D.

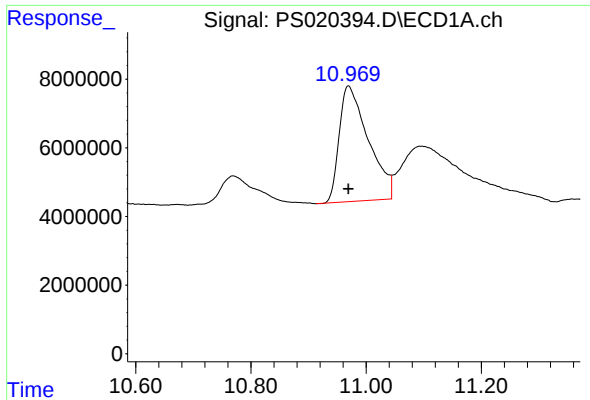

#15 Picloram

R.T.: 10.969 min
Delta R.T.: 0.000 min
Response: 117896877
Conc: 3.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

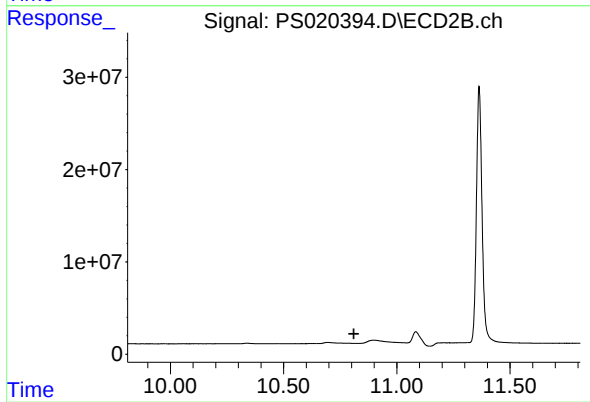

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.810 min
Response: 0
Conc: N.D.