

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083122\
 Data File : PS020398.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2022 10:46
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:17:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.185	6.762	1448.5E6	428.8E6	491.224	526.215
Target Compounds							
2) T	3,5-DICHL...	6.454f	0.000	68904786	0	17.714	N.D. #
5) T	DICAMBA	0.000	6.988f	0	17623899	N.D.	4.945
6) T	MCP	7.519	6.988	-192320	17623899	N.D.	6.461
7) T	MCPA	7.658	7.187	1592063	18415473	<MDL	4.375 #
11) T	2,4,5-TP ...	9.169	0.000	1695013	0	<MDL	N.D. #
12) T	2,4,5-T	9.442	0.000	14088145	0	<MDL	N.D. #
13) T	2,4-DB	9.923f	0.000	2690334	0	<MDL	N.D. #
15) T	Picloram	10.953	10.873f	194.9E6	10971326	6.165	1.454 #
16) T	DCPA	11.406	0.000	2230656	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083122\
Data File : PS020398.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2022 10:46
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:17:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

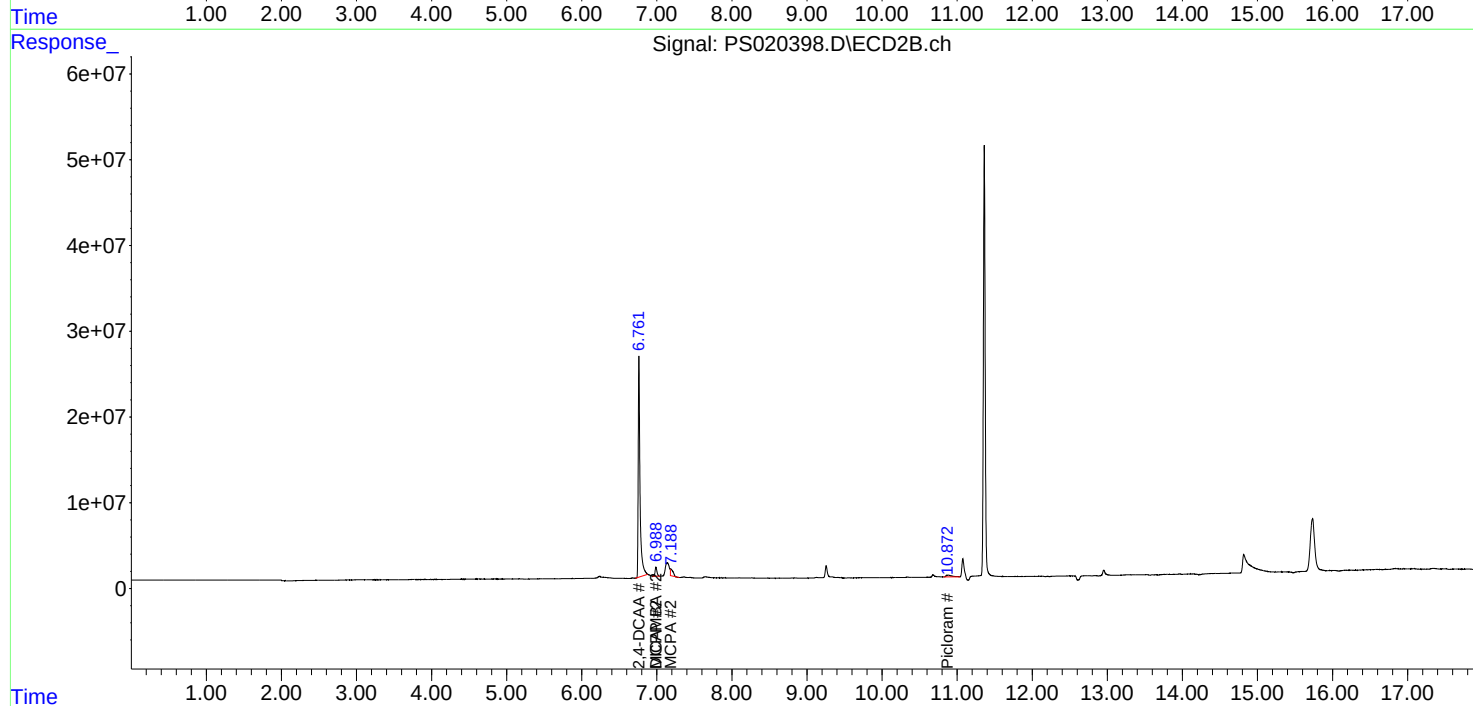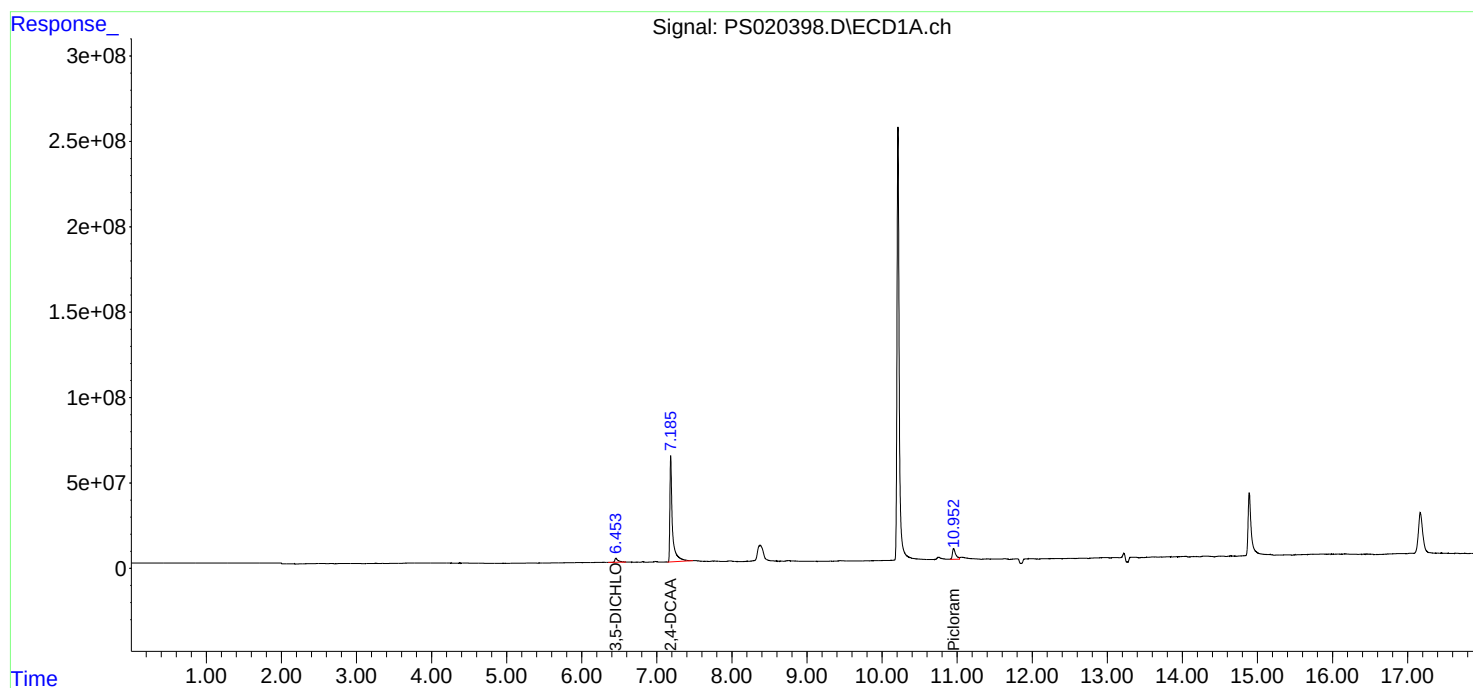


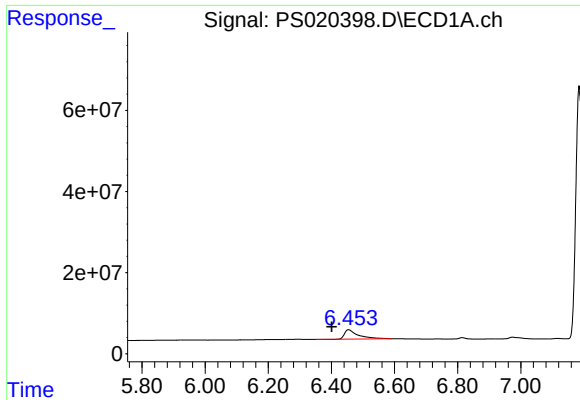

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.454 min
Delta R.T.: 0.053 min
Response: 68904786
Conc: 17.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

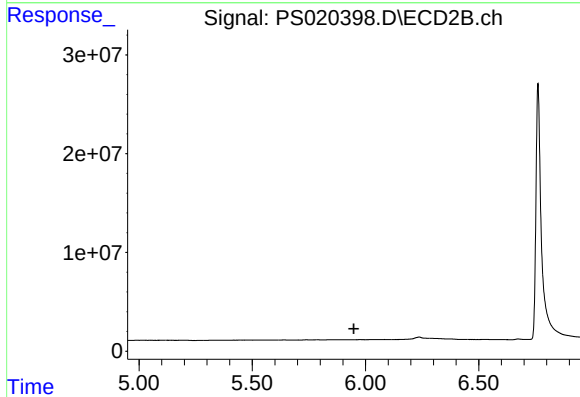


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

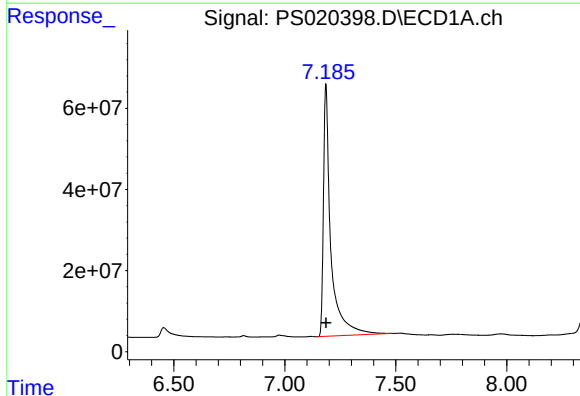


#4 2,4-DCAA

R.T.: 7.185 min
Delta R.T.: 0.000 min
Response: 1448483520
Conc: 491.22 ng/ml

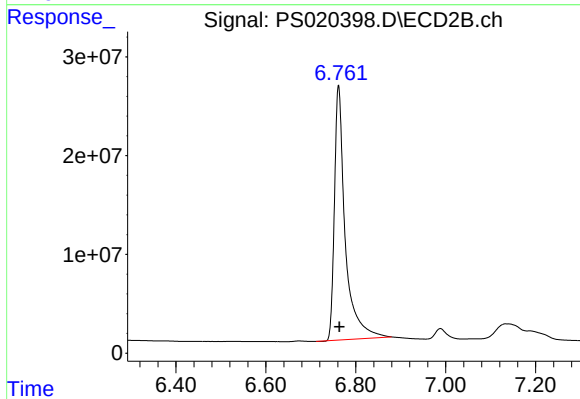

#4 2,4-DCAA


R.T.: 6.762 min
Delta R.T.: -0.002 min
Response: 428841650
Conc: 526.21 ng/ml

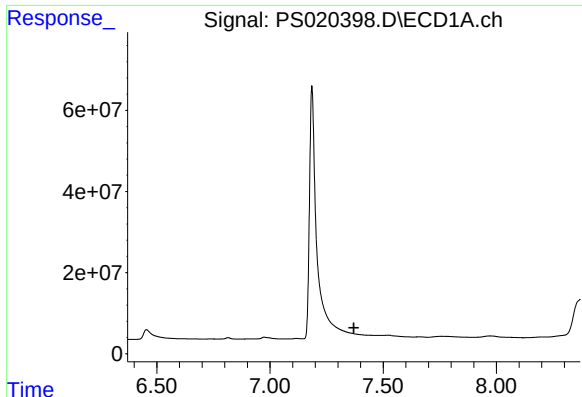

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.370 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

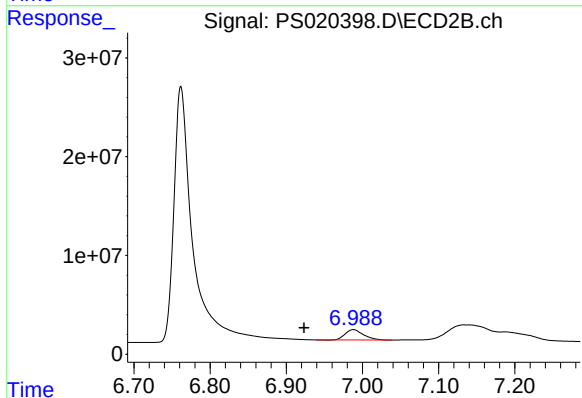


#5 DICAMBA

R.T.: 6.988 min
Delta R.T.: 0.065 min
Response: 17623899
Conc: 4.94 ng/ml

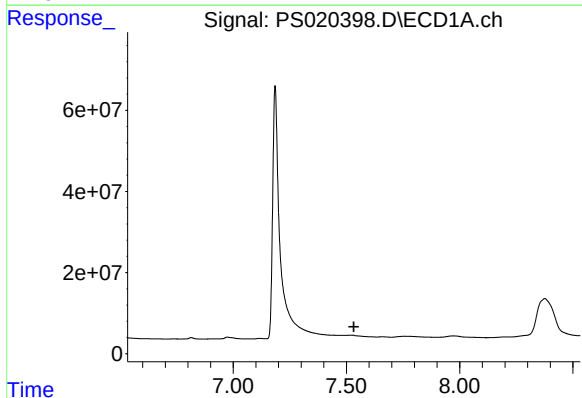


#6 MCP

R.T.: 7.519 min
Delta R.T.: -0.014 min
Response: -192320
Conc: N.D.

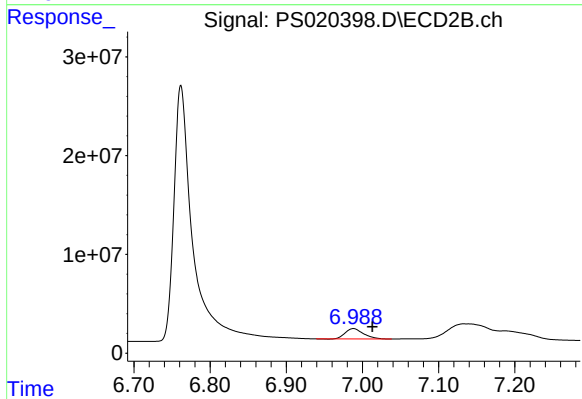

#6 MCP


R.T.: 6.988 min
Delta R.T.: -0.025 min
Response: 17623899
Conc: 6.46 ug/ml

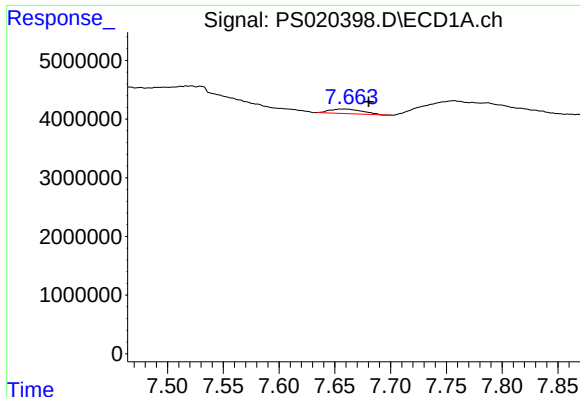

#7 MCPA


R.T.: 7.658 min
Delta R.T.: -0.022 min
Response: 1592063
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

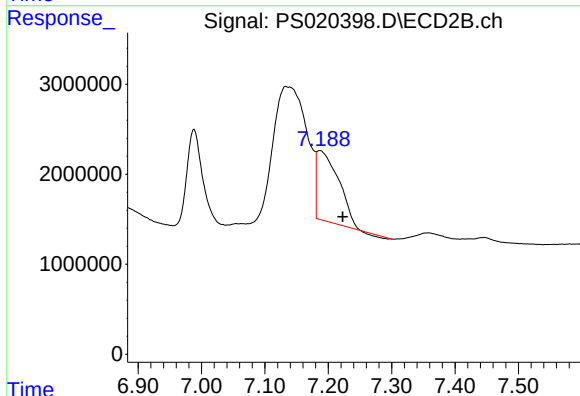


#7 MCPA

R.T.: 7.187 min
Delta R.T.: -0.036 min
Response: 18415473
Conc: 4.37 ug/ml

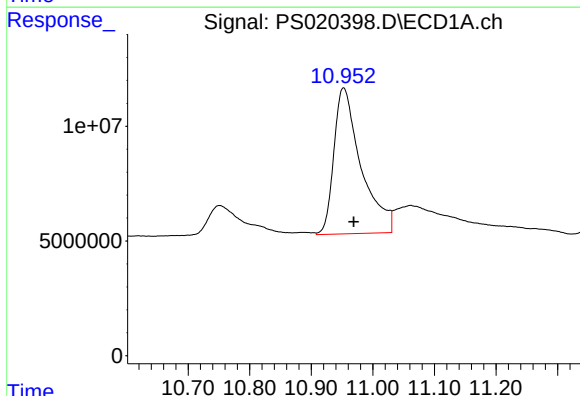

#15 Picloram

R.T.: 10.953 min
Delta R.T.: -0.017 min
Response: 194932907
Conc: 6.17 ng/ml

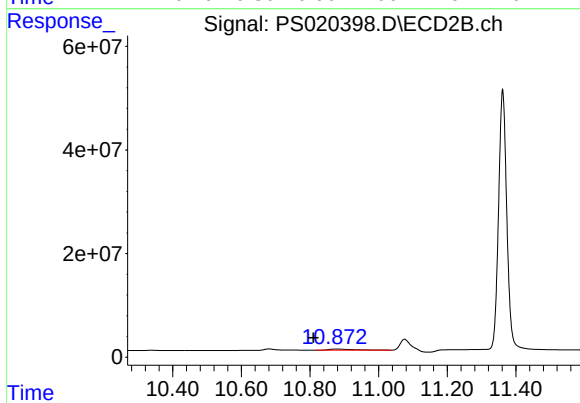

#15 Picloram

R.T.: 10.873 min
Delta R.T.: 0.063 min
Response: 10971326
Conc: 1.45 ng/ml