

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083122\
 Data File : PS020414.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2022 01:06
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:23:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.183	6.761	1496.7E6	452.4E6	507.559	555.115
Target Compounds							
2) T	3,5-DICHL...	6.440	0.000	638.6E6	0	164.181	N.D. #
3) T	4-Nitroph...	0.000	6.371	0	1456370	N.D.	2.965
5) T	DICAMBA	0.000	6.981f	0	186.3E6	N.D.	52.257
6) T	MCP	0.000	6.981	0	186.3E6	N.D.	68.277
7) T	MCPA	7.653	0.000	792944	0	<MDL	N.D. #
9) T	2,4-D	8.368f	0.000	380.1E6	0	126.209	N.D. #
11) T	2,4,5-TP ...	9.165	0.000	1941775	0	<MDL	N.D. #
12) T	2,4,5-T	9.430	0.000	14897823	0	<MDL	N.D. #
14) T	DINOSEB	11.185f	0.000	9994171	0	<MDL	N.D. #
15) T	Picloram	10.938	10.860f	599.0E6	10577901	18.944	1.402 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083122\
Data File : PS020414.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2022 01:06
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:23:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

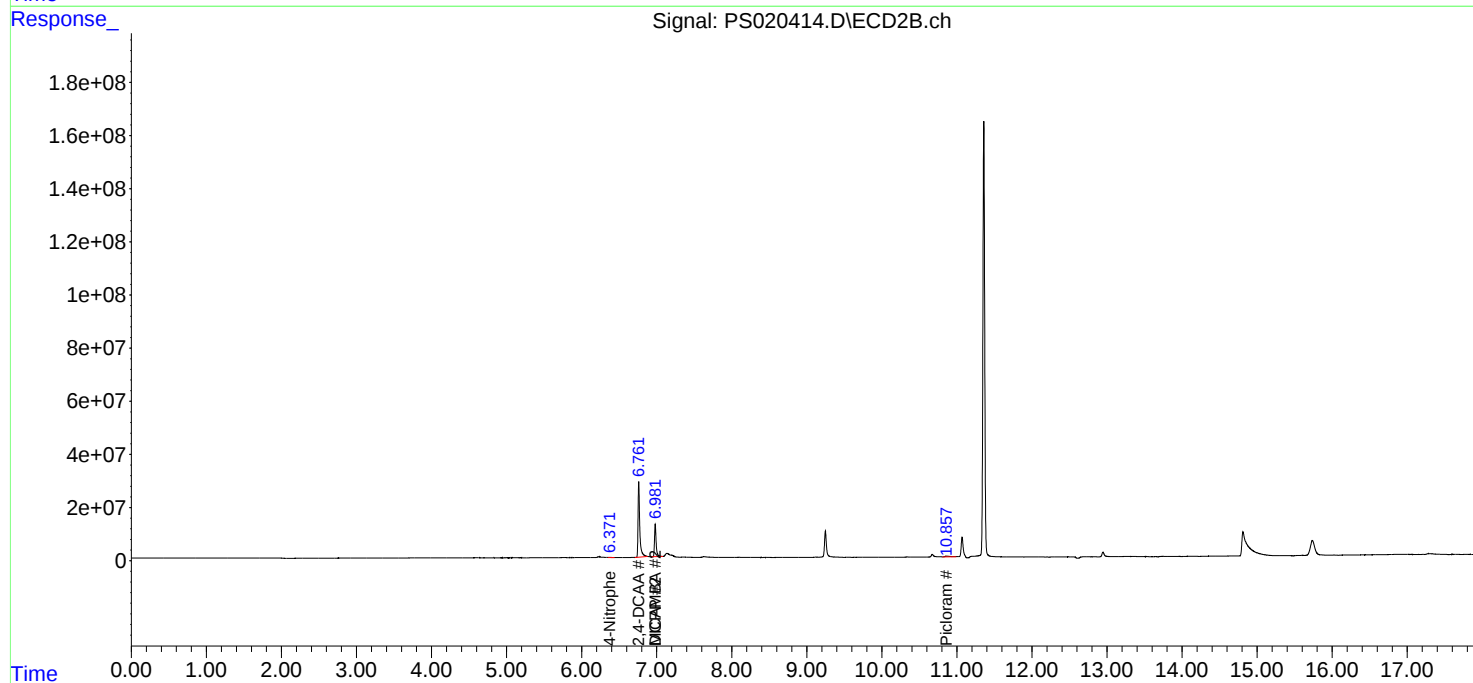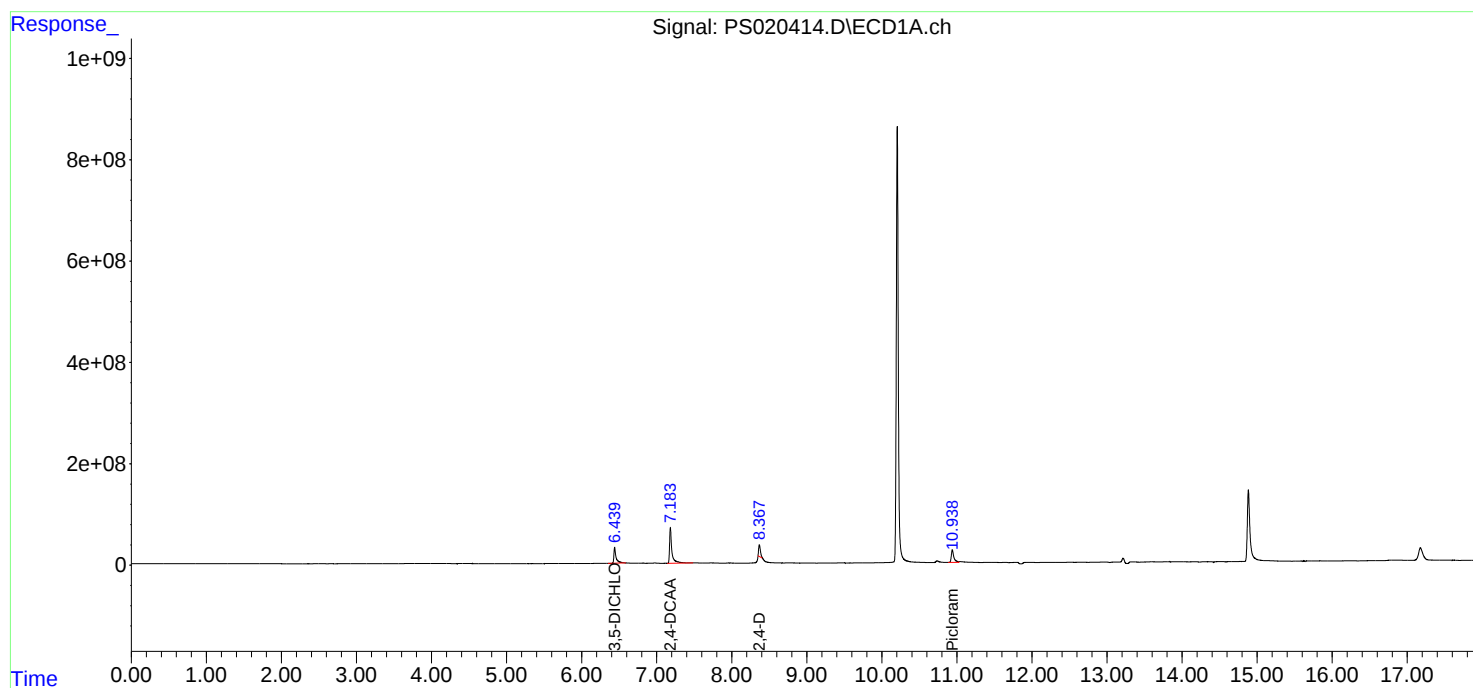


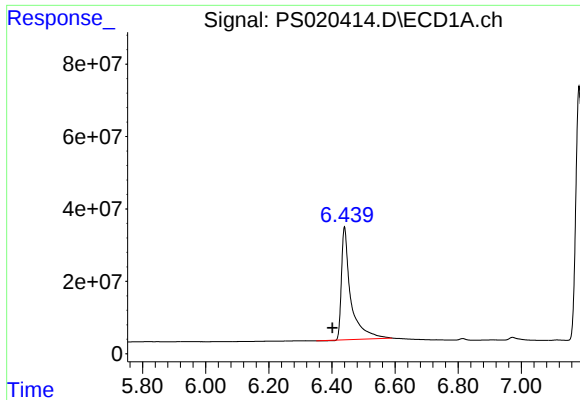

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.440 min
Delta R.T.: 0.039 min
Response: 638647203
Conc: 164.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

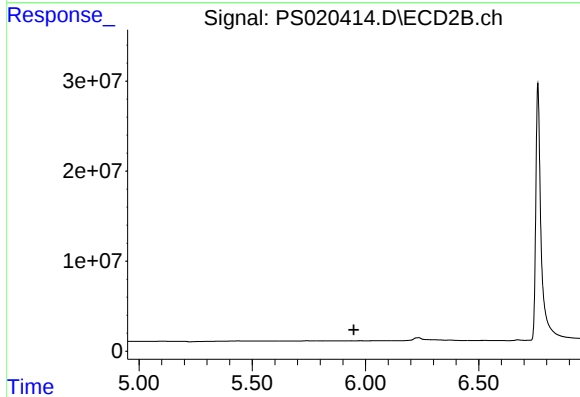


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

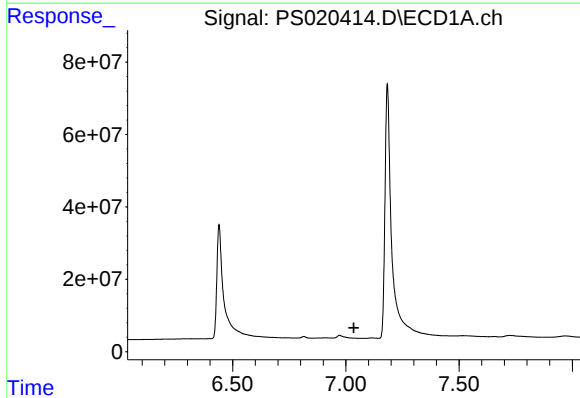


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.035 min
Response: 0
Conc: N.D.

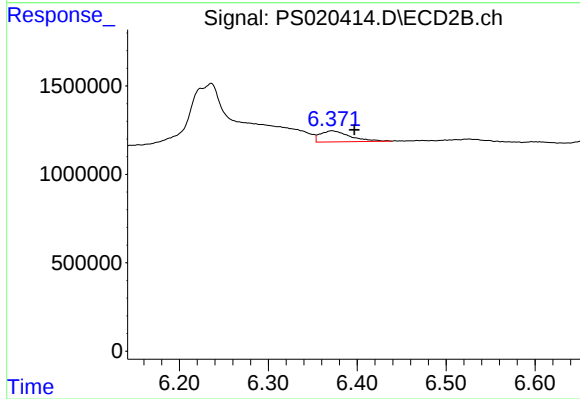

#3 4-Nitrophenol


R.T.: 6.371 min
Delta R.T.: -0.025 min
Response: 1456370
Conc: 2.97 ng/ml

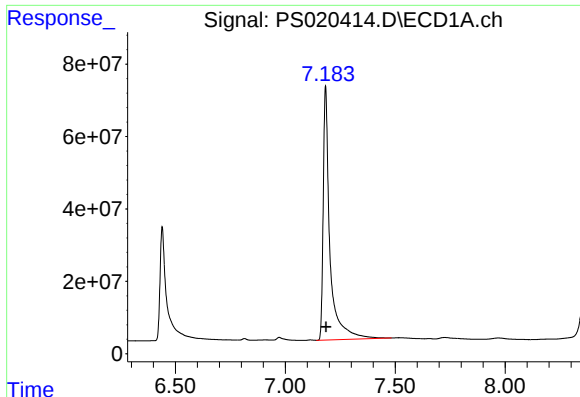

#4 2,4-DCAA


R.T.: 7.183 min
Delta R.T.: -0.002 min
Response: 1496651745
Conc: 507.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

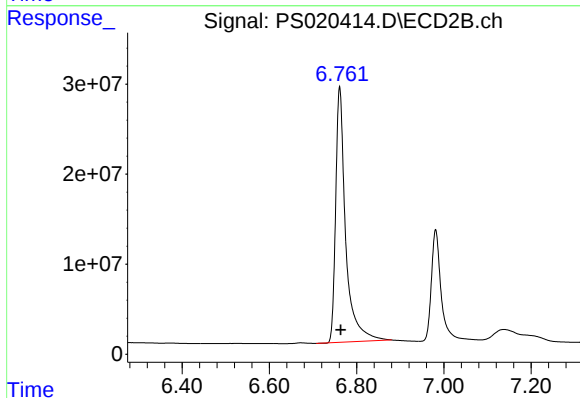


#4 2,4-DCAA

R.T.: 6.761 min
Delta R.T.: -0.002 min
Response: 452394423
Conc: 555.12 ng/ml

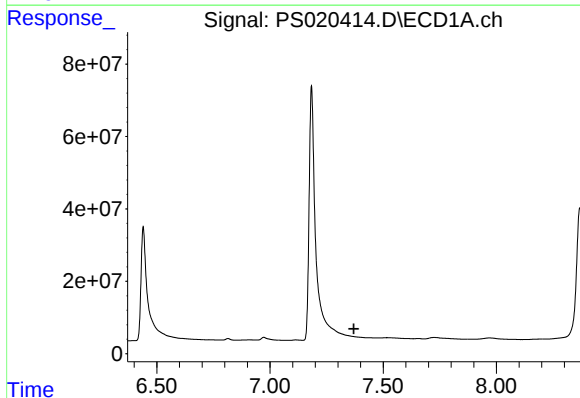


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.370 min
Response: 0
Conc: N.D.

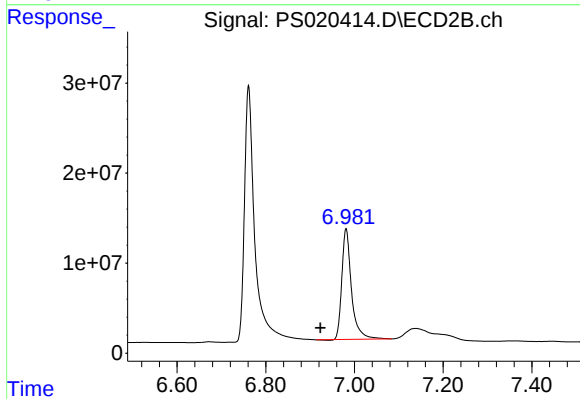

#5 DICAMBA


R.T.: 6.981 min
Delta R.T.: 0.058 min
Response: 186250315
Conc: 52.26 ng/ml

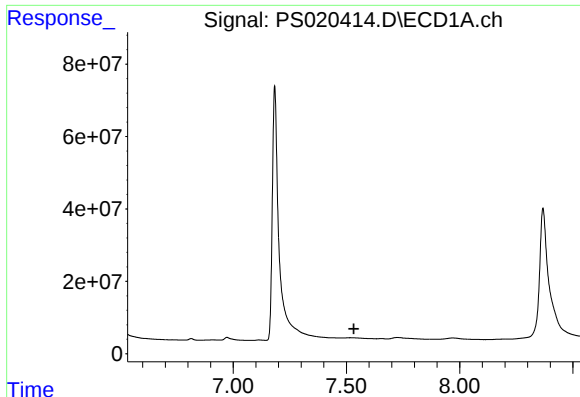

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.533 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

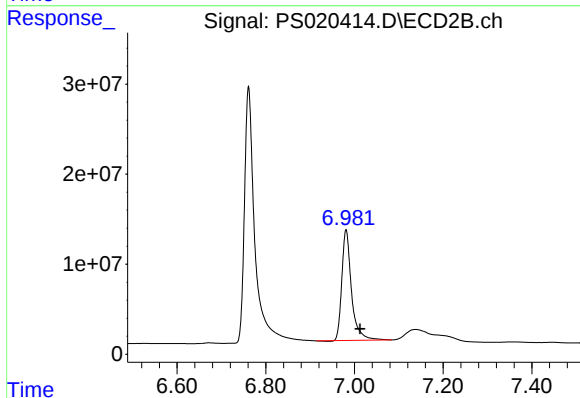


#6 MCP

R.T.: 6.981 min
Delta R.T.: -0.032 min
Response: 186250315
Conc: 68.28 ug/ml

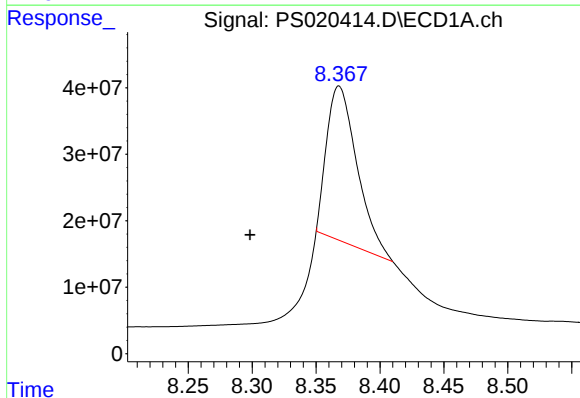


#9 2,4-D

R.T.: 8.368 min
Delta R.T.: 0.070 min
Response: 380100676
Conc: 126.21 ng/ml

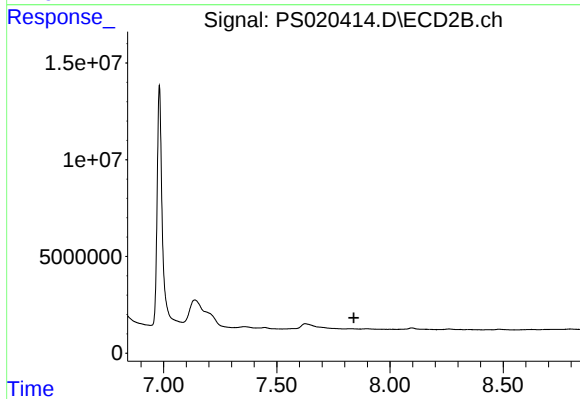

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.840 min
Response: 0
Conc: N.D.

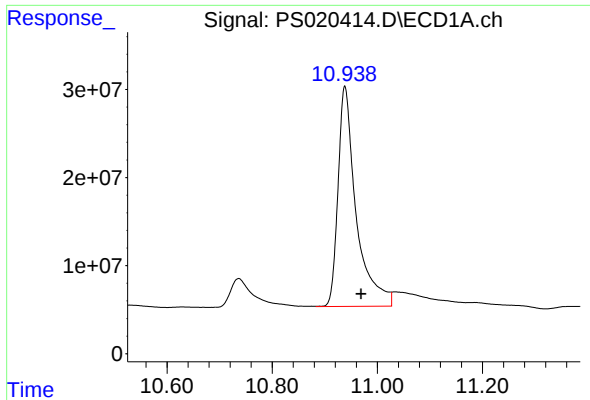

#15 Picloram

R.T.: 10.938 min
Delta R.T.: -0.031 min
Response: 598984032
Conc: 18.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

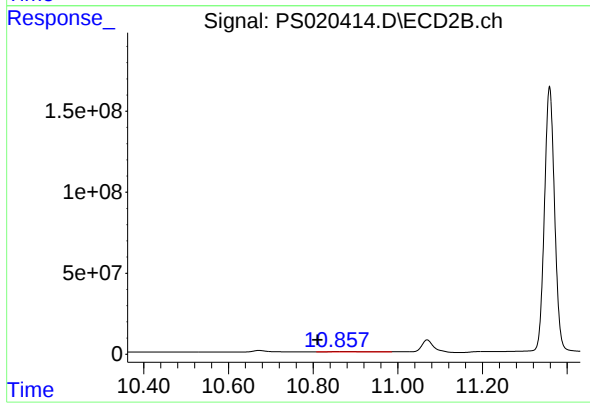

#15 Picloram

R.T.: 10.860 min
Delta R.T.: 0.049 min
Response: 10577901
Conc: 1.40 ng/ml