

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083123\
 Data File : PS024238.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2023 12:34
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 00:38:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 28 16:48:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.365	6.789	1085.9E6	359.7E6	545.057	535.572
Target Compounds							
1) T	Dalapon	2.516	2.573	4913508	3536770	2.261	3.354 #
2) T	3,5-DICHL...	5.703	5.933f	55376	261253	<MDL	<MDL #
3) T	4-Nitroph...	6.204	0.000	11118278	0	8.949	N.D. #
5) T	DICAMBA	6.496	6.996f	713907	3916822	<MDL	1.360 #
6) T	MCP	6.685	6.996f	2425872	3916822	<MDL	2.045 #
7) T	MCPA	6.726f	0.000	191881	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.580	0	2065726	N.D.	2.843
9) T	2,4-D	7.256	7.795f	81512674	894552	30.645	1.004 #
10) T	Pentachlo...	7.528	0.000	3629766	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.043	8.631	1456643	1009960	<MDL	<MDL #
12) T	2,4,5-T	8.307	9.051f	333458	1136642	<MDL	<MDL #
14) T	DINOSEB	9.882	9.911f	1823119	444182	<MDL	<MDL #
15) T	Picloram	9.667	10.796	67944662	14983879	4.160	2.523 #
16) T	DCPA	10.096	10.796	3404012	14983879	<MDL	2.921 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083123\
Data File : PS024238.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2023 12:34
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 00:38:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
Quant Title : 8080.M
QLast Update : Mon Aug 28 16:48:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

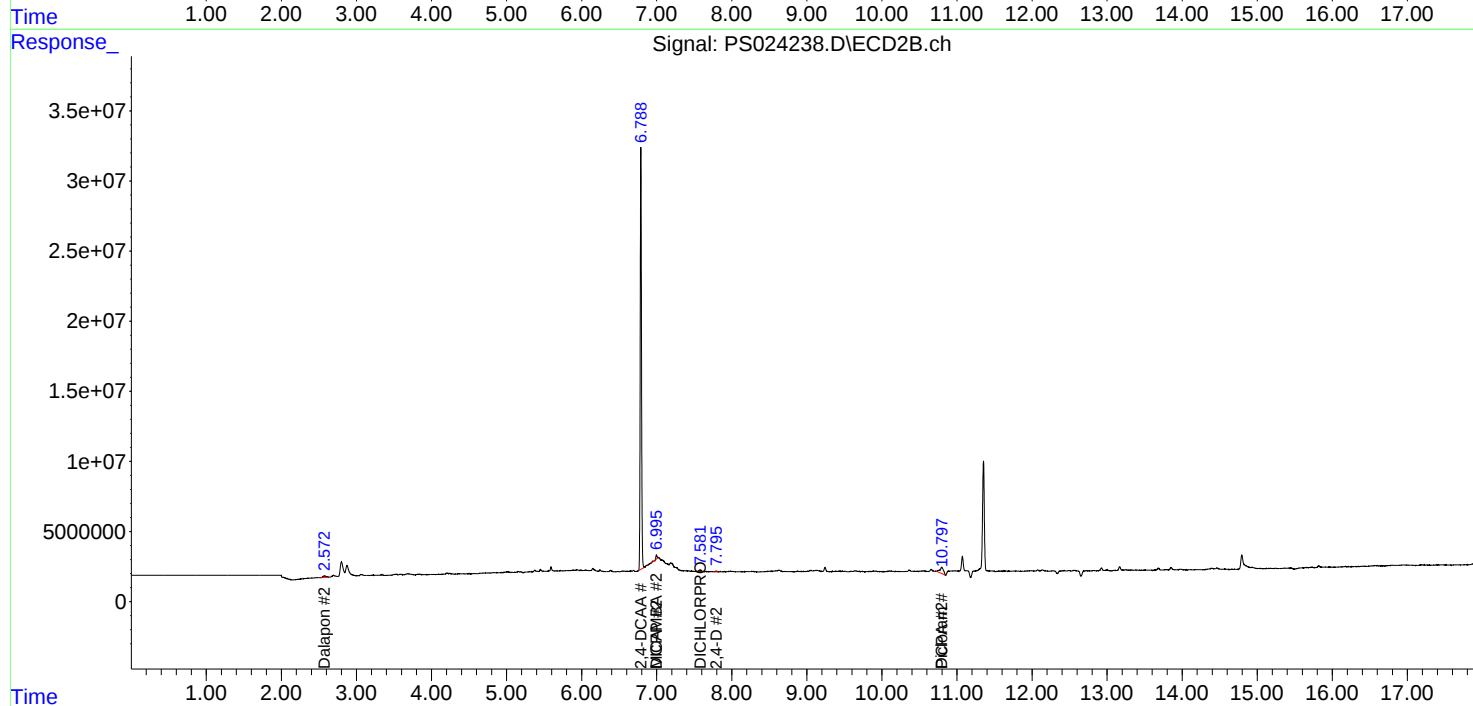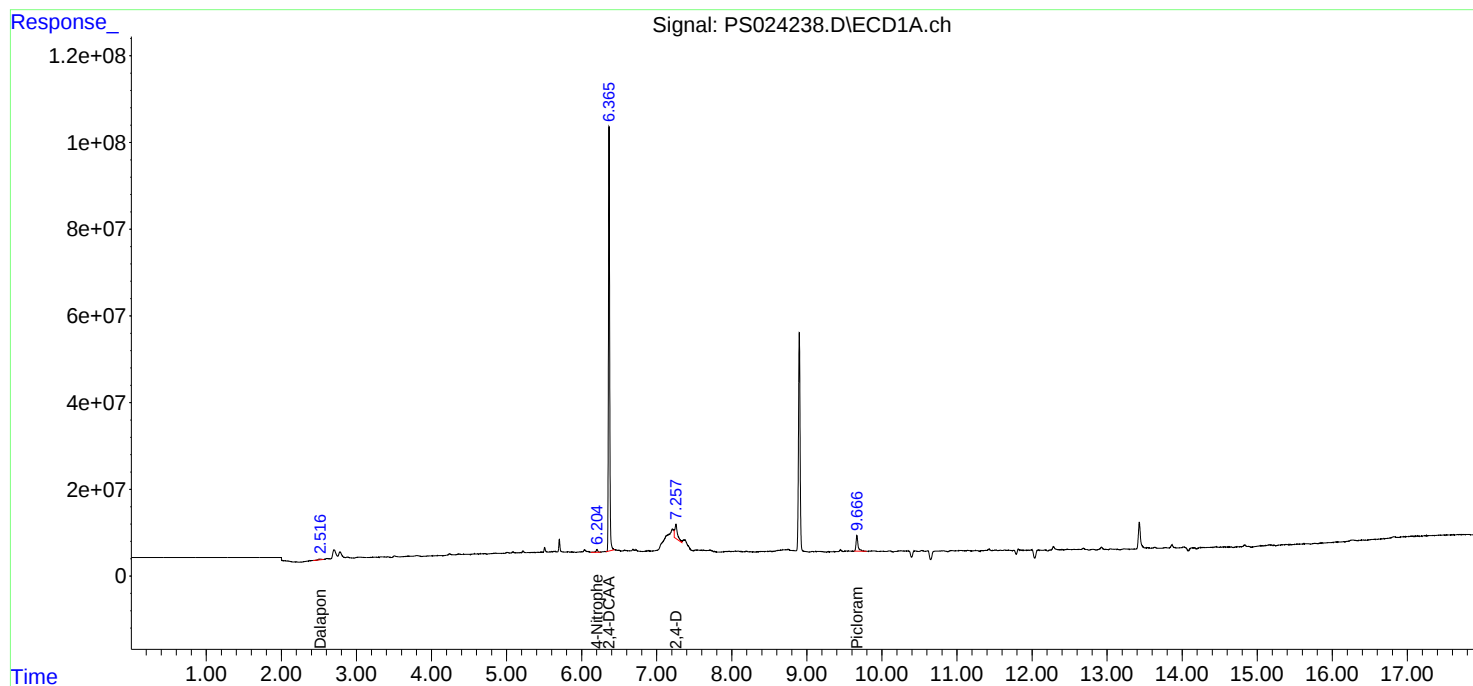


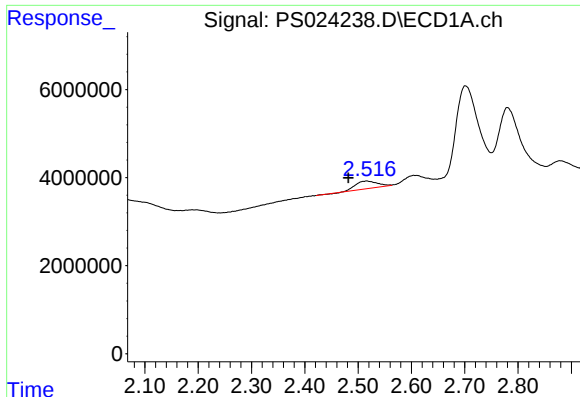

#1 Dalapon


R.T.: 2.516 min
Delta R.T.: 0.034 min
Response: 4913508
Conc: 2.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

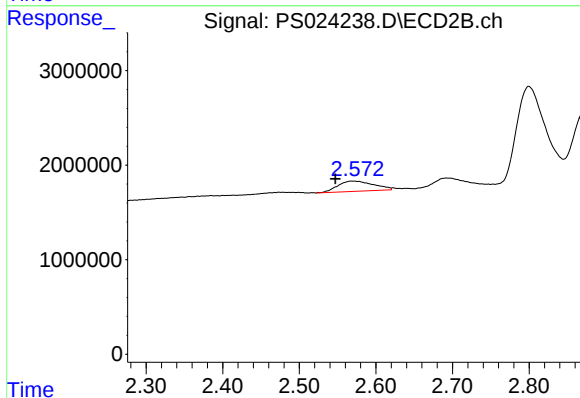


#1 Dalapon

R.T.: 2.573 min
Delta R.T.: 0.026 min
Response: 3536770
Conc: 3.35 ng/ml

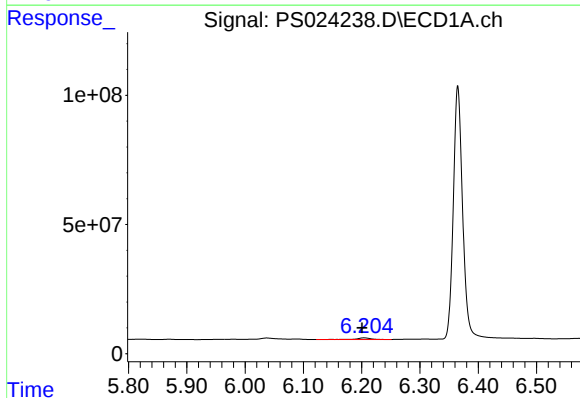


#3 4-Nitrophenol

R.T.: 6.204 min
Delta R.T.: 0.003 min
Response: 11118278
Conc: 8.95 ng/ml

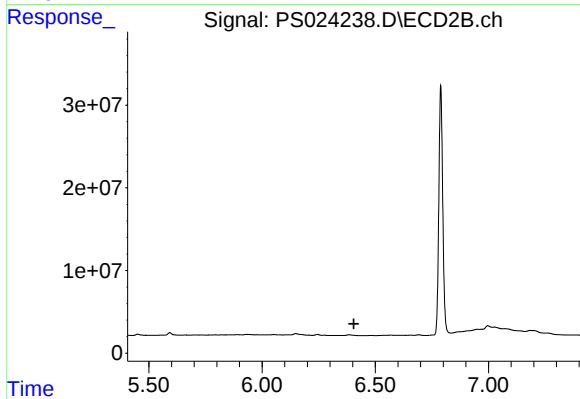

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.405 min
Response: 0
Conc: N.D.

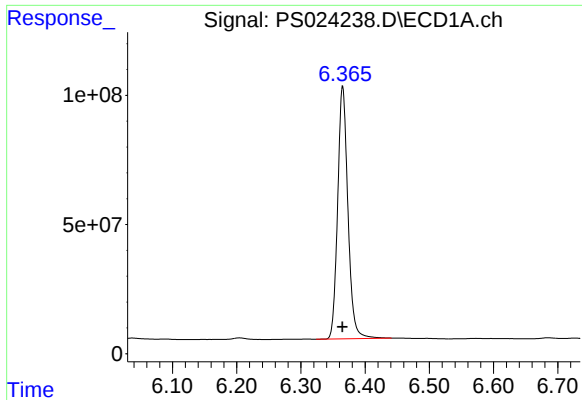

#4 2,4-DCAA


R.T.: 6.365 min
Delta R.T.: 0.000 min
Response: 1085928598
Conc: 545.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

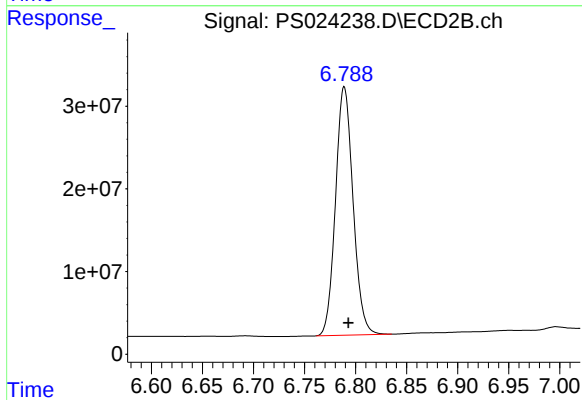


#4 2,4-DCAA

R.T.: 6.789 min
Delta R.T.: -0.004 min
Response: 359685810
Conc: 535.57 ng/ml

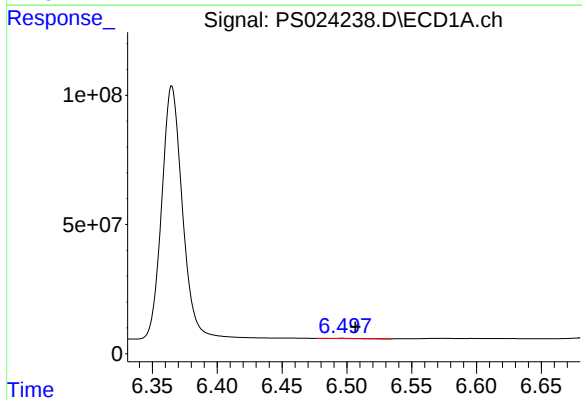


#5 DICAMBA

R.T.: 6.496 min
Delta R.T.: -0.011 min
Response: 713907
Conc: N.D.

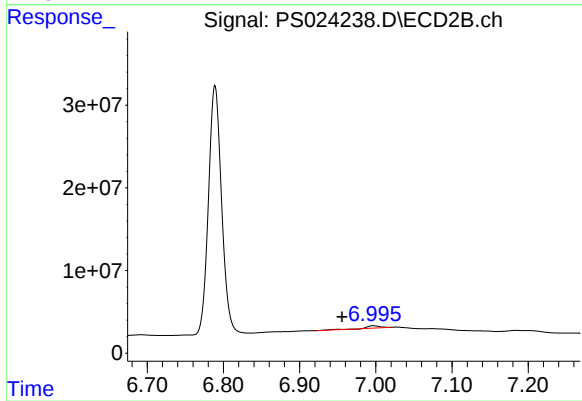

#5 DICAMBA


R.T.: 6.996 min
Delta R.T.: 0.040 min
Response: 3916822
Conc: 1.36 ng/ml

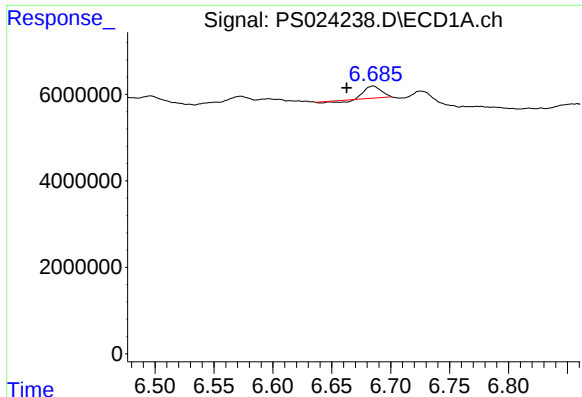

#6 MCP


R.T.: 6.685 min
Delta R.T.: 0.022 min
Response: 2425872
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

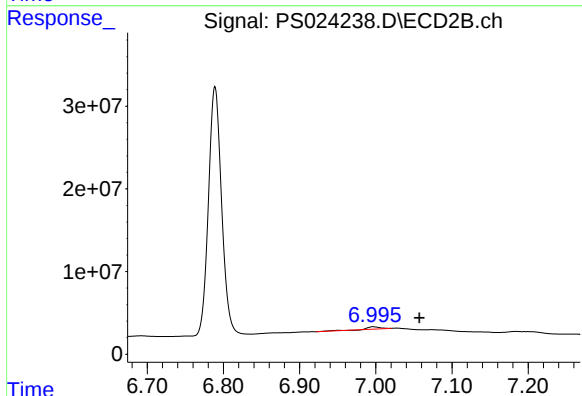


#6 MCP

R.T.: 6.996 min
Delta R.T.: -0.061 min
Response: 3916822
Conc: 2.04 ug/ml

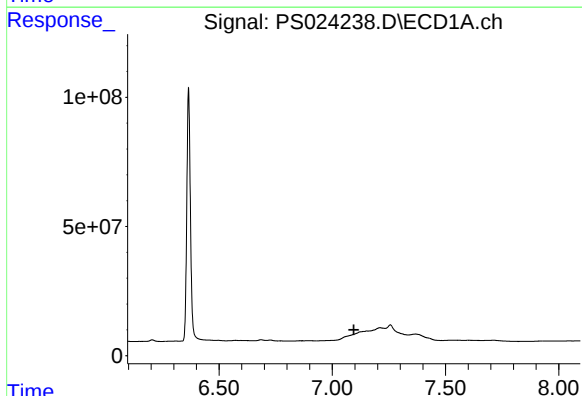


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.095 min
Response: 0
Conc: N.D.

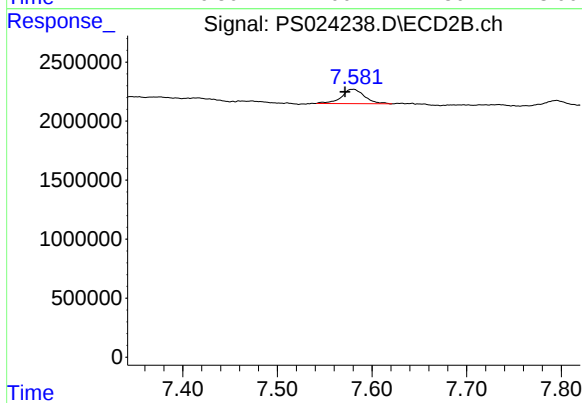

#8 DICHLORPROP


R.T.: 7.580 min
Delta R.T.: 0.008 min
Response: 2065726
Conc: 2.84 ng/ml

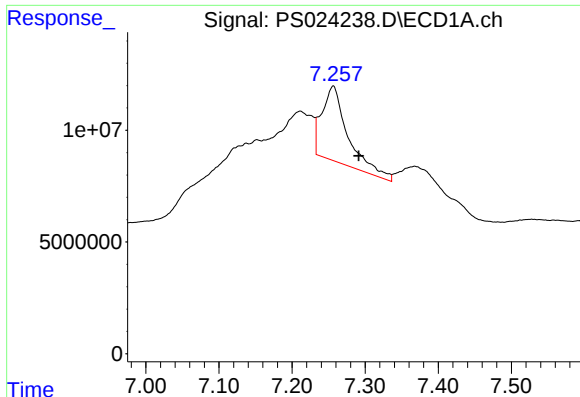

#9 2,4-D


R.T.: 7.256 min
Delta R.T.: -0.035 min
Response: 81512674
Conc: 30.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

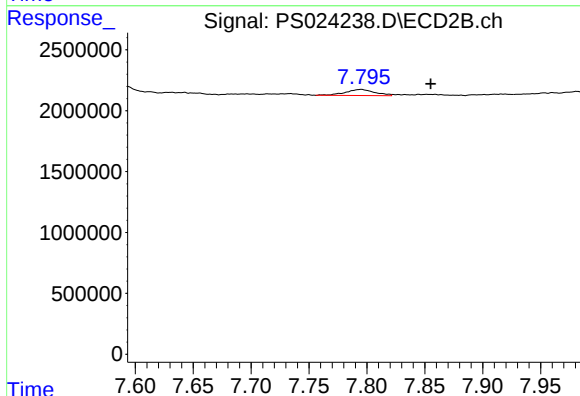


#9 2,4-D

R.T.: 7.795 min
Delta R.T.: -0.060 min
Response: 894552
Conc: 1.00 ng/ml

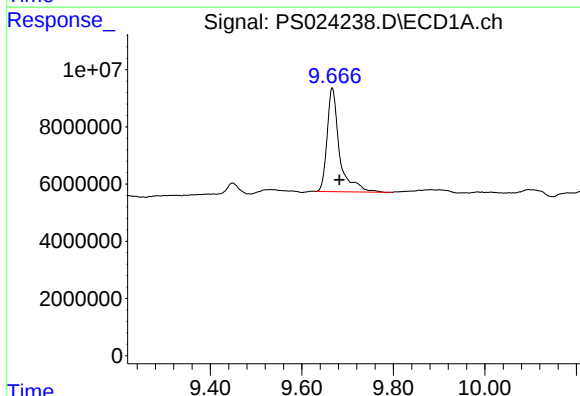


#15 Picloram

R.T.: 9.667 min
Delta R.T.: -0.015 min
Response: 67944662
Conc: 4.16 ng/ml

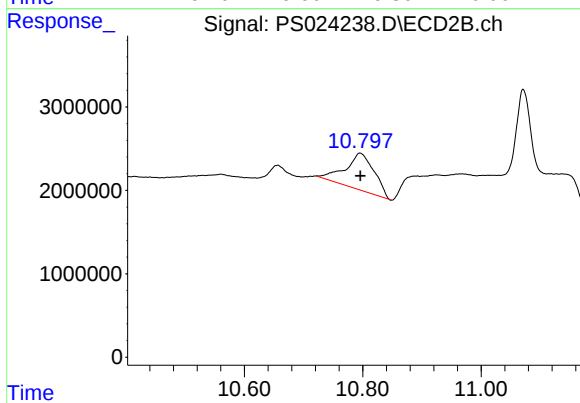

#15 Picloram


R.T.: 10.796 min
Delta R.T.: 0.000 min
Response: 14983879
Conc: 2.52 ng/ml

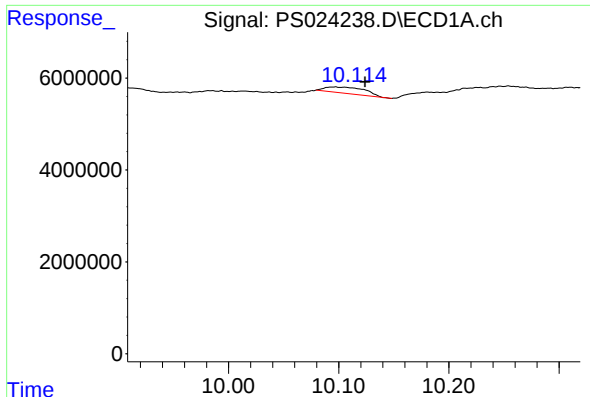

#16 DCPA

R.T.: 10.096 min
Delta R.T.: -0.027 min
Response: 3404012
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

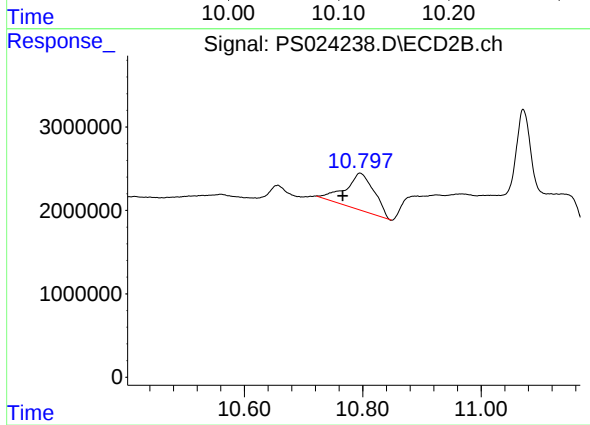

#16 DCPA

R.T.: 10.796 min
Delta R.T.: 0.029 min
Response: 14983879
Conc: 2.92 ng/ml