

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090120\
 Data File : PS011997.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2020 11:19
 Operator : DD\AJ
 Sample : L3712-18RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 12:07:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.221	6.912	875.5E6	510.8E6	802.634	955.084
Target Compounds							
2) T	3,5-DICHL...	6.476	6.094	2239481	81291026	1.545	98.820 #
3) T	4-Nitroph...	7.058	0.000	488597	0	<MDL	N.D. #
5) T	DICAMBA	7.398	7.073	6903780	20235158	1.686	9.366 #
6) T	MCP	7.574	7.214	7290709	17522595	2.282	9.914 #
7) T	MCPA	7.701	0.000	111.7E6	0	24.551	N.D. #
8) T	DICHLORPROP	0.000	7.737	0	27584676	N.D.	48.854
9) T	2,4-D	8.400	0.000	218.9E6	0	193.899	N.D. #
11) T	2,4,5-TP ...	0.000	8.748	0	16341319	N.D.	5.589
12) T	2,4,5-T	9.416	0.000	42547916	0	7.180	N.D. #
15) T	Picloram	10.981	0.000	38200854	0	4.888	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090120\
Data File : PS011997.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2020 11:19
Operator : DD\AJ
Sample : L3712-18RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 12:07:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

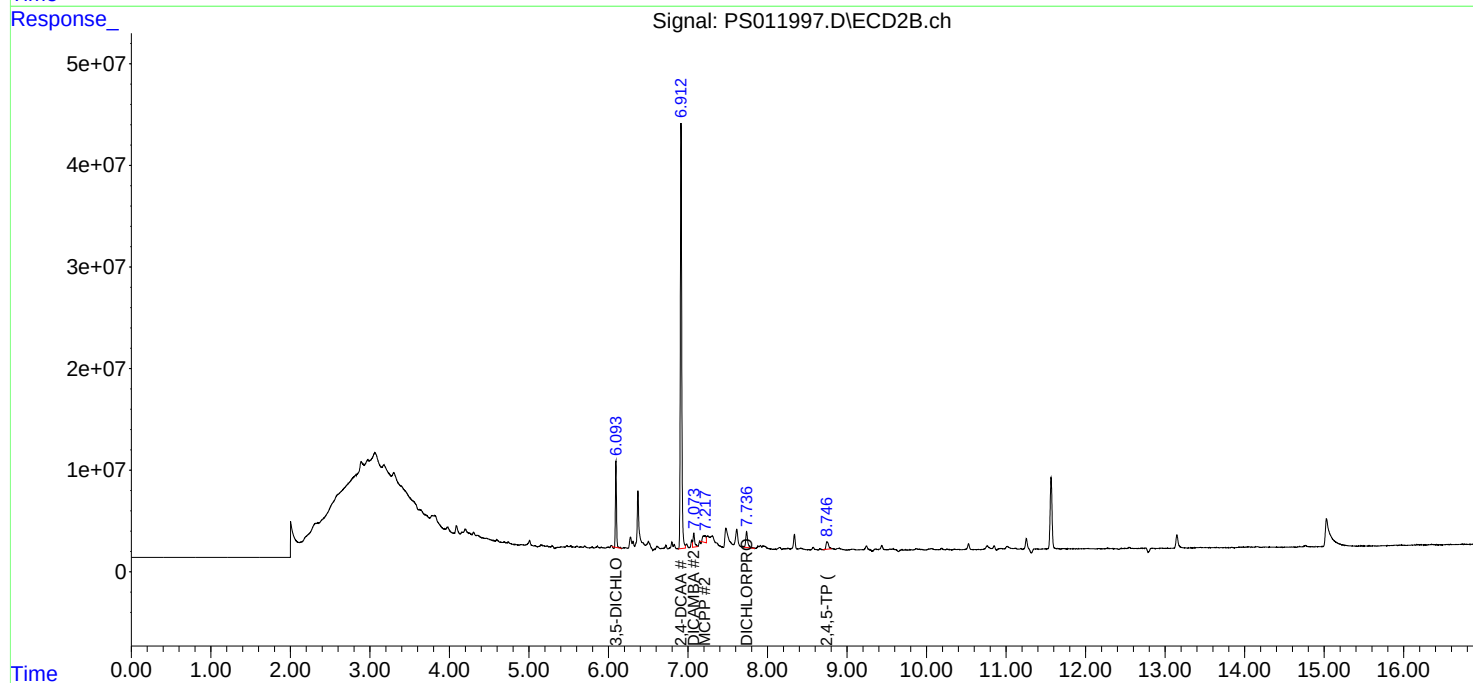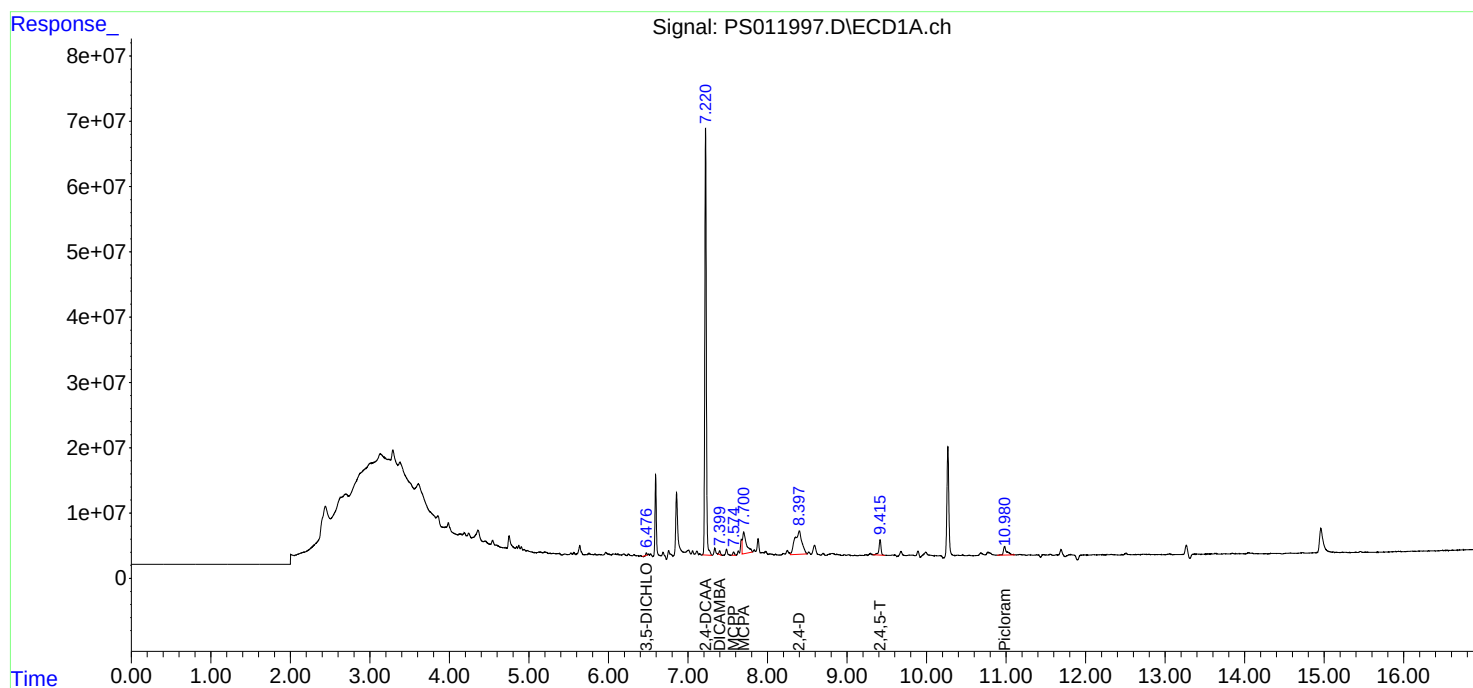


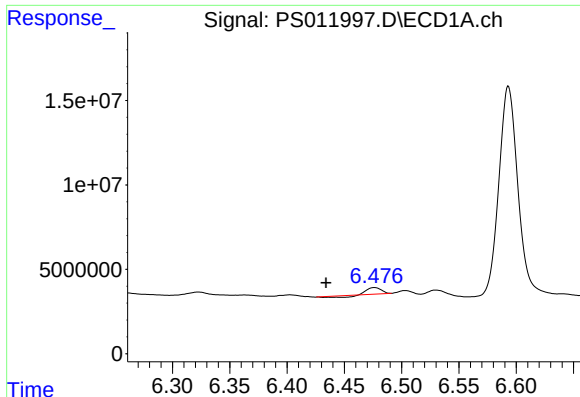

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.476 min
Delta R.T.: 0.042 min
Response: 2239481
Conc: 1.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

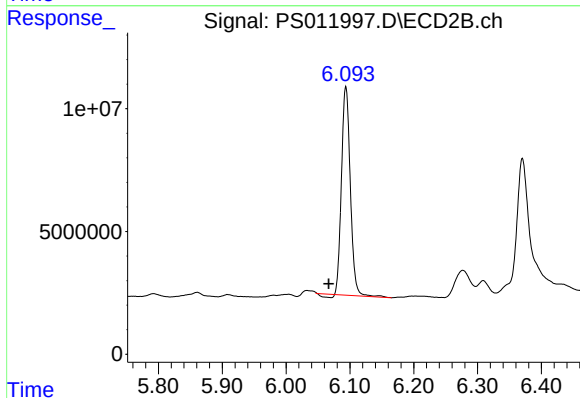


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.094 min
Delta R.T.: 0.027 min
Response: 81291026
Conc: 98.82 ng/ml

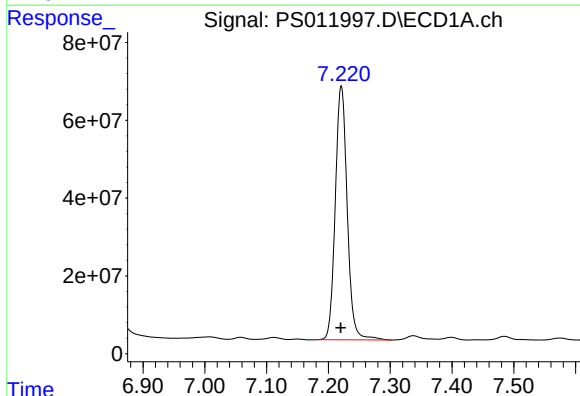


#4 2,4-DCAA

R.T.: 7.221 min
Delta R.T.: 0.000 min
Response: 875487523
Conc: 802.63 ng/ml

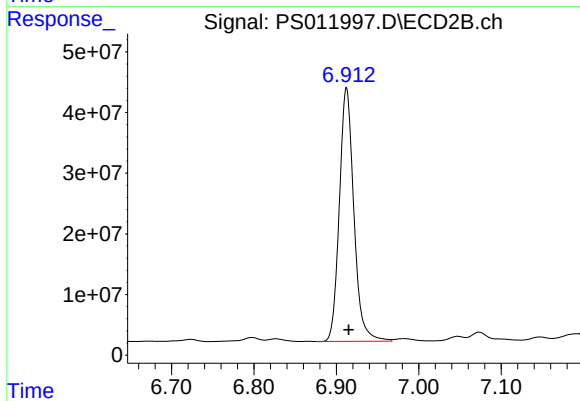

#4 2,4-DCAA


R.T.: 6.912 min
Delta R.T.: -0.003 min
Response: 510766440
Conc: 955.08 ng/ml

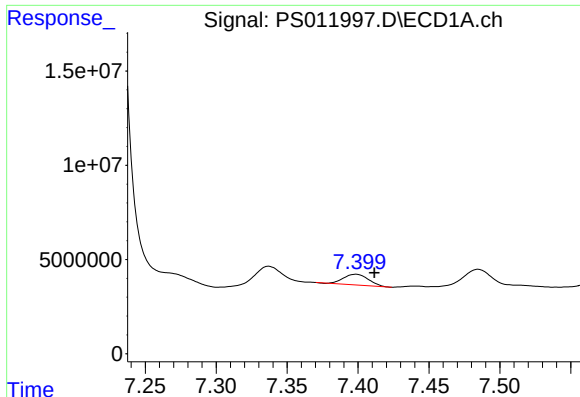

#5 DICAMBA


R.T.: 7.398 min
Delta R.T.: -0.013 min
Response: 6903780
Conc: 1.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

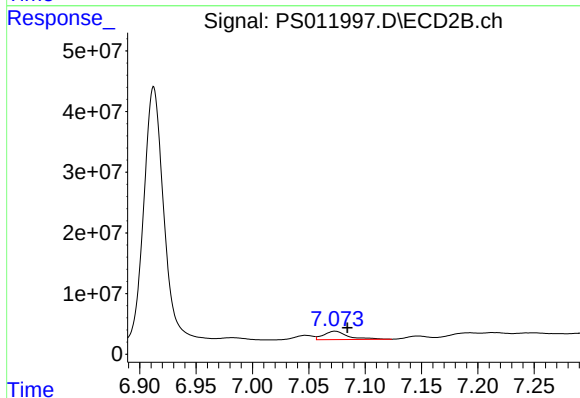


#5 DICAMBA

R.T.: 7.073 min
Delta R.T.: -0.011 min
Response: 20235158
Conc: 9.37 ng/ml

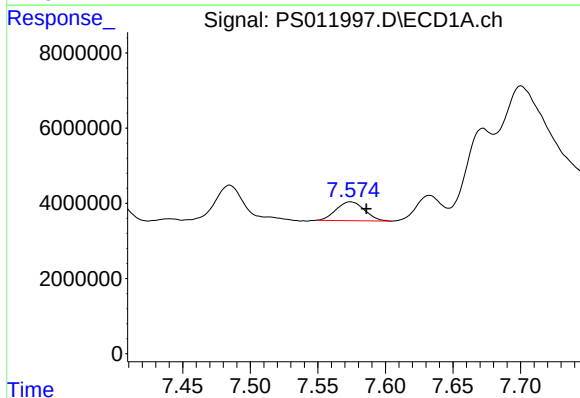


#6 MCP

R.T.: 7.574 min
Delta R.T.: -0.012 min
Response: 7290709
Conc: 2.28 ug/ml

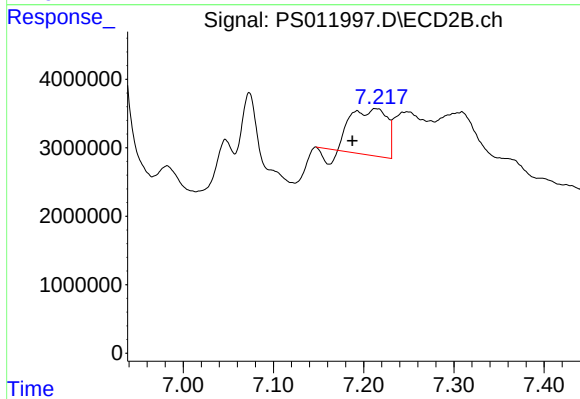

#6 MCP


R.T.: 7.214 min
Delta R.T.: 0.026 min
Response: 17522595
Conc: 9.91 ug/ml

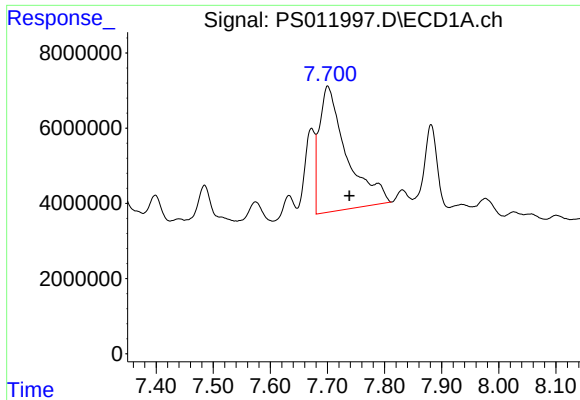

#7 MCPA


R.T.: 7.701 min
Delta R.T.: -0.037 min
Response: 111668294
Conc: 24.55 ug/ml

Instrument :
ECD_S
ClientSampleId :

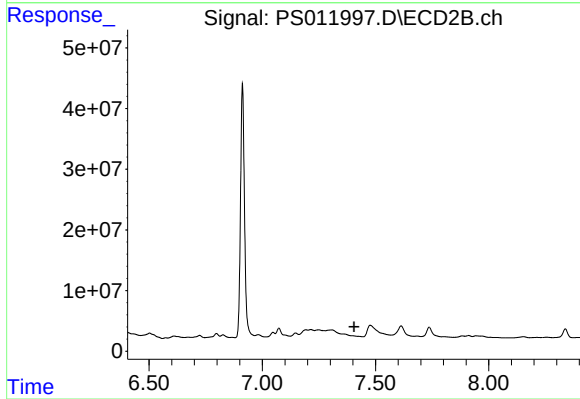


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.405 min
Response: 0
Conc: N.D.

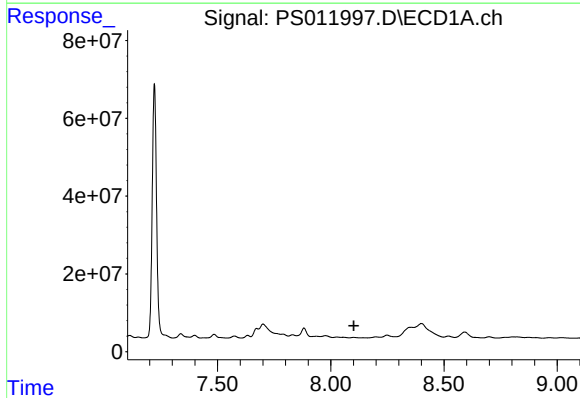


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

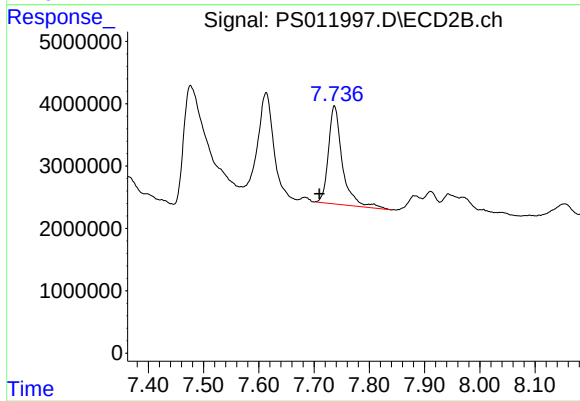

#8 DICHLORPROP


R.T.: 7.737 min
Delta R.T.: 0.027 min
Response: 27584676
Conc: 48.85 ng/ml

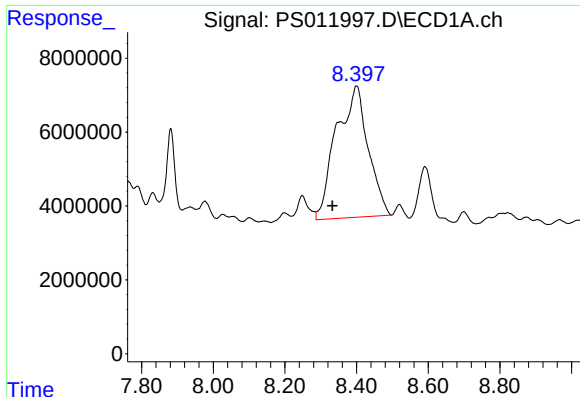

#9 2,4-D


R.T.: 8.400 min
Delta R.T.: 0.068 min
Response: 218930301
Conc: 193.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

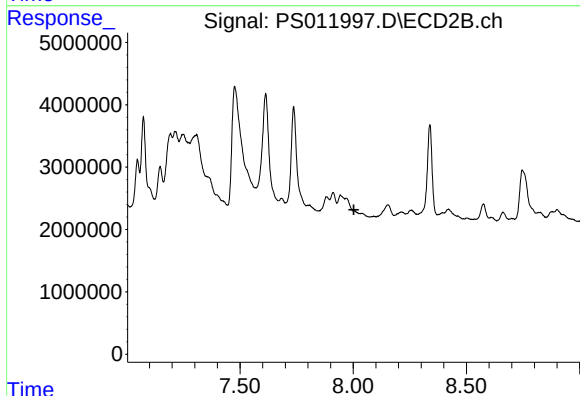


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

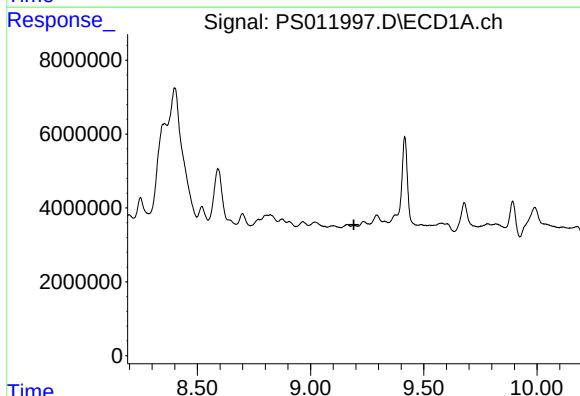


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

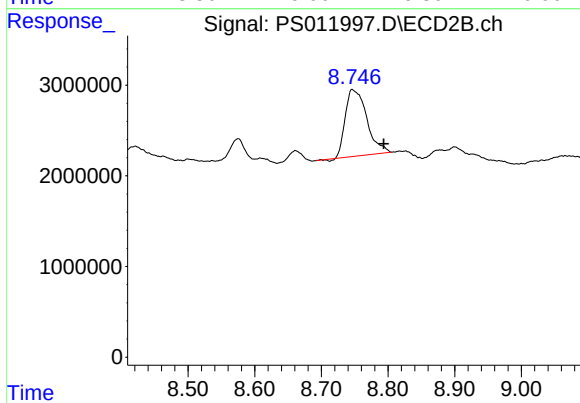

#11 2,4,5-TP (SILVEX)


R.T.: 8.748 min
Delta R.T.: -0.046 min
Response: 16341319
Conc: 5.59 ng/ml

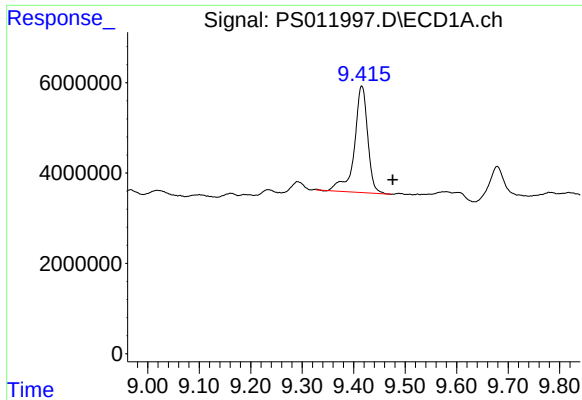

#12 2,4,5-T


R.T.: 9.416 min
Delta R.T.: -0.060 min
Response: 42547916
Conc: 7.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

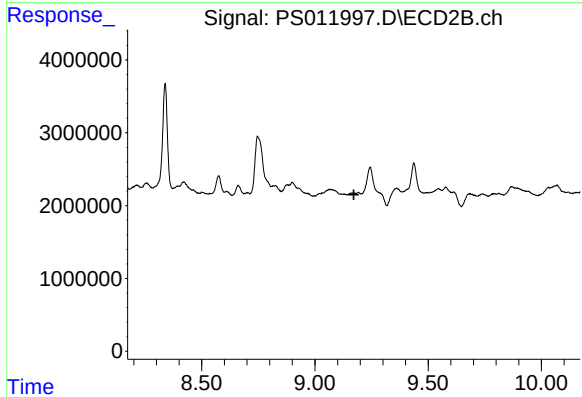


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

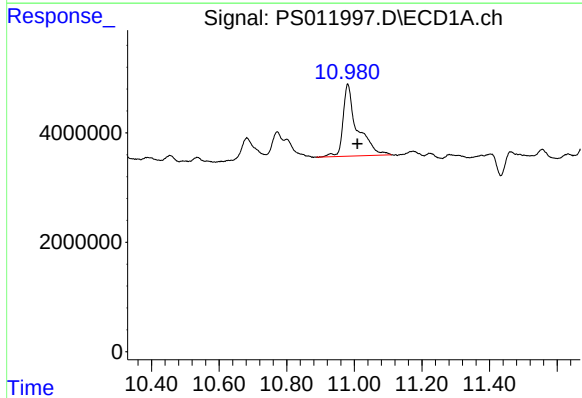

#15 Picloram

R.T.: 10.981 min
Delta R.T.: -0.029 min
Response: 38200854
Conc: 4.89 ng/ml

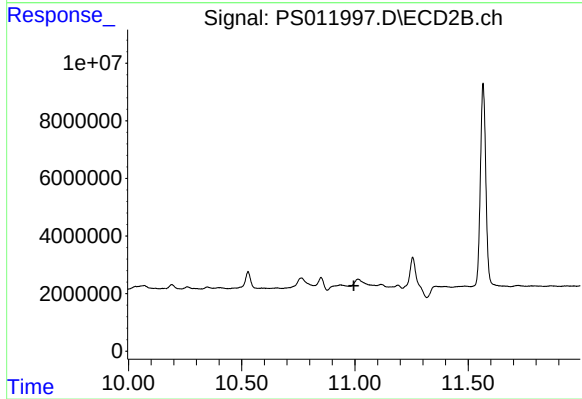

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.