

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090120\
 Data File : PS011998.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2020 11:42
 Operator : DD\AJ
 Sample : PB131290BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 12:07:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.914	650.5E6	386.9E6	596.349	723.385
Target Compounds							
1) T	Dalapon	2.998	2.583	32965408	54517918	26.464	72.128 #
2) T	3,5-DICHL...	0.000	6.096	0	96479027	N.D.	117.283
3) T	4-Nitroph...	7.056	0.000	1678338	0	2.849	N.D. #
5) T	DICAMBA	7.397	7.049	11149884	15101647	2.722	6.990 #
6) T	MCPD	7.572	0.000	10096325	0	3.160	N.D. #
7) T	MCPA	7.670	0.000	75218468	0	16.537	N.D. #
8) T	DICHLORPROP	0.000	7.742	0	51366184	N.D.	90.972
9) T	2,4-D	8.290	7.976	12482466	-1789691	11.055	N.D. #
10) T	Pentachlo...	8.696	0.000	27431758	0	1.907	N.D. #
12) T	2,4,5-T	9.414	0.000	34432782	0	5.811	N.D. #
15) T	Picloram	0.000	10.939	0	12117829	N.D.	2.674
16) T	DCPA	0.000	10.939	0	12117829	N.D.	3.296



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090120\
Data File : PS011998.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2020 11:42
Operator : DD\AJ
Sample : PB131290BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 12:07:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

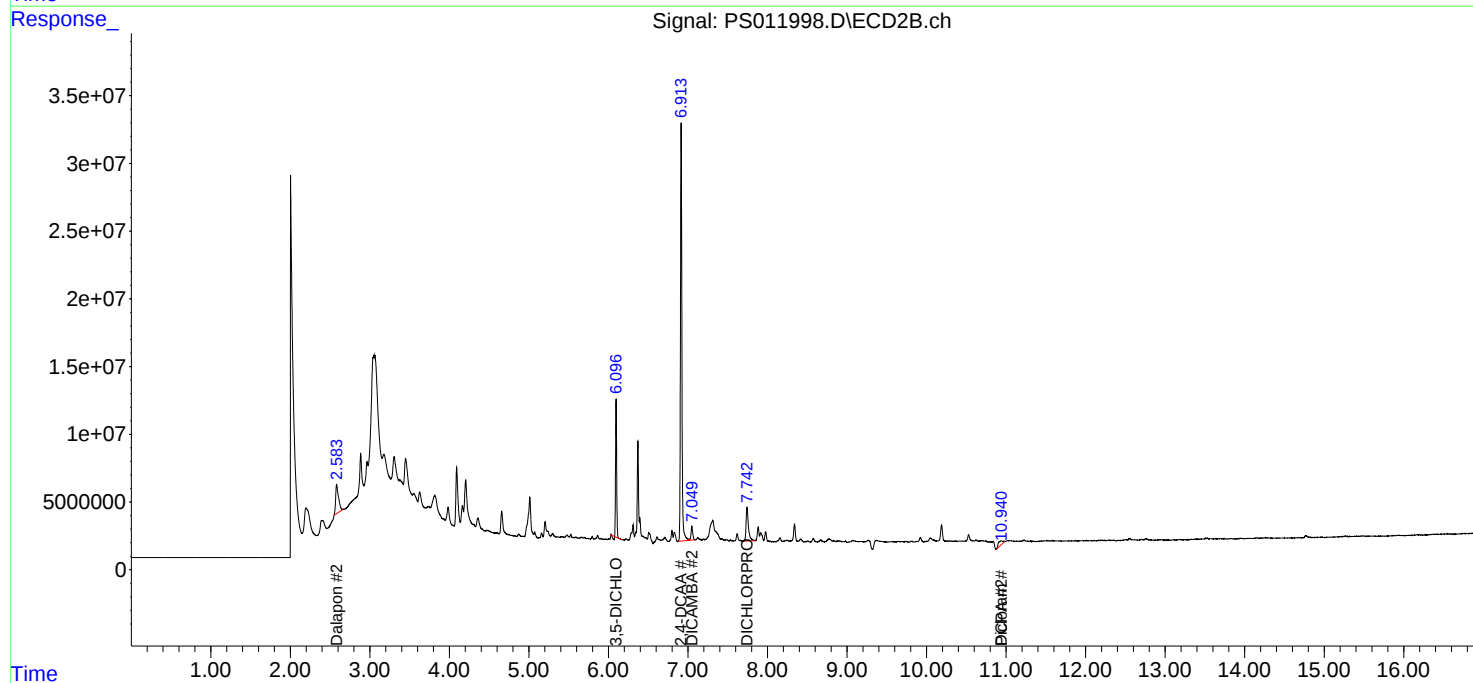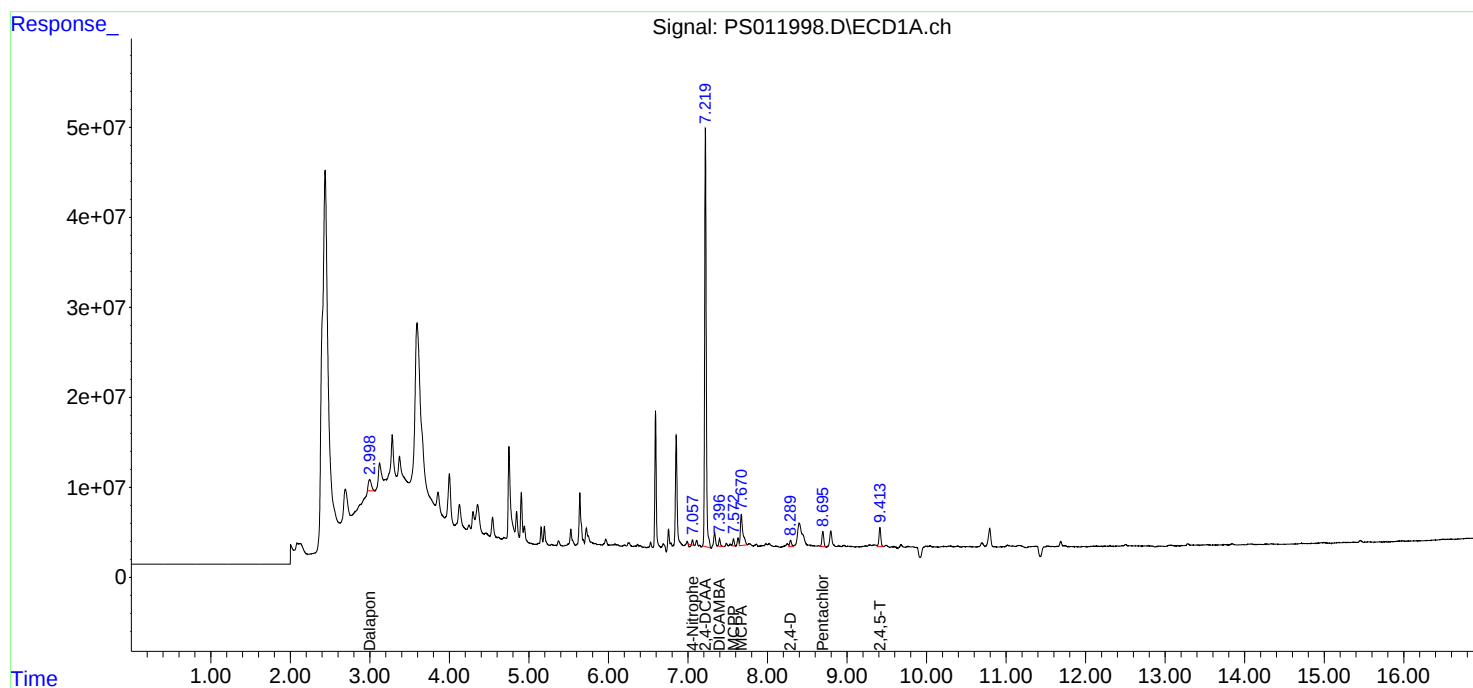


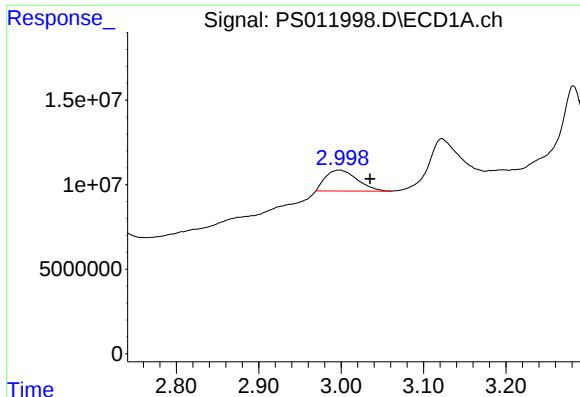

#1 Dalapon


R.T.: 2.998 min
Delta R.T.: -0.037 min
Response: 32965408
Conc: 26.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

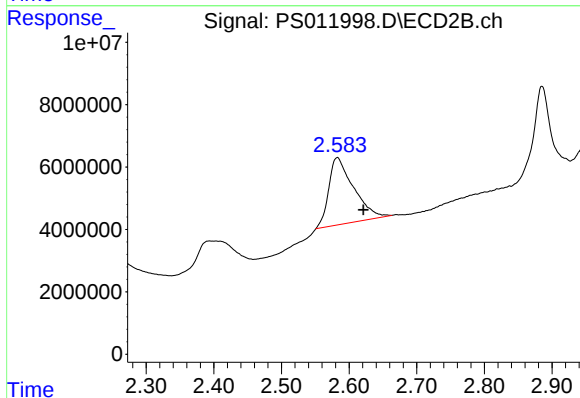


#1 Dalapon

R.T.: 2.583 min
Delta R.T.: -0.039 min
Response: 54517918
Conc: 72.13 ng/ml

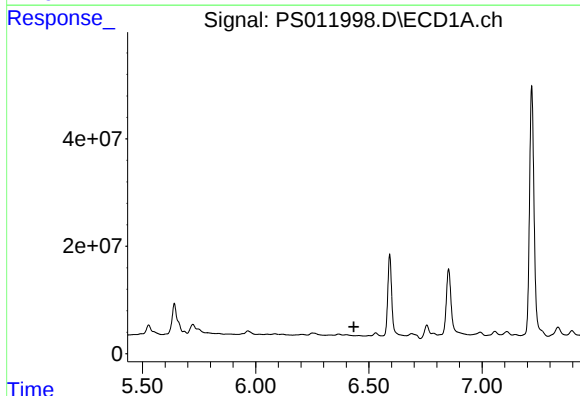


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

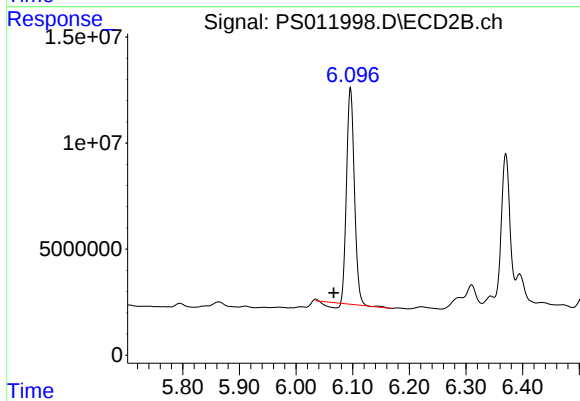

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.096 min
Delta R.T.: 0.030 min
Response: 96479027
Conc: 117.28 ng/ml

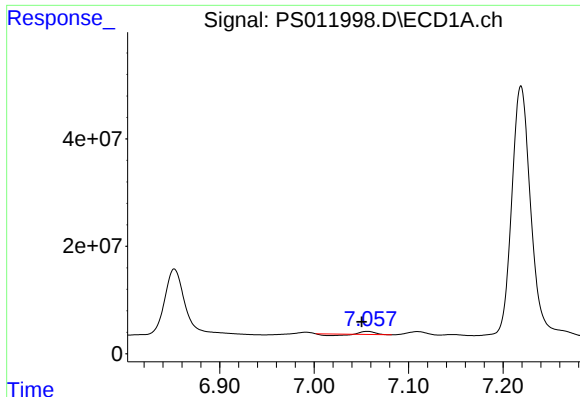

#3 4-Nitrophenol


R.T.: 7.056 min
Delta R.T.: 0.006 min
Response: 1678338
Conc: 2.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

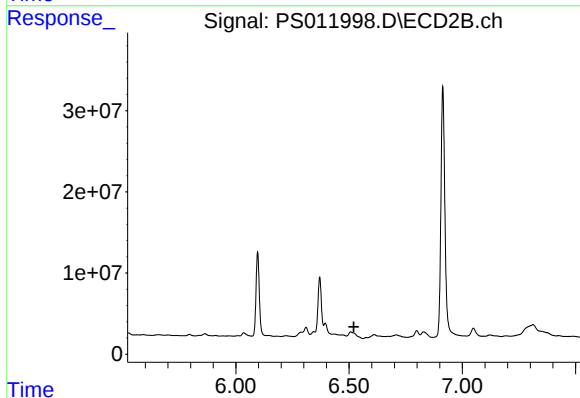


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.521 min
Response: 0
Conc: N.D.

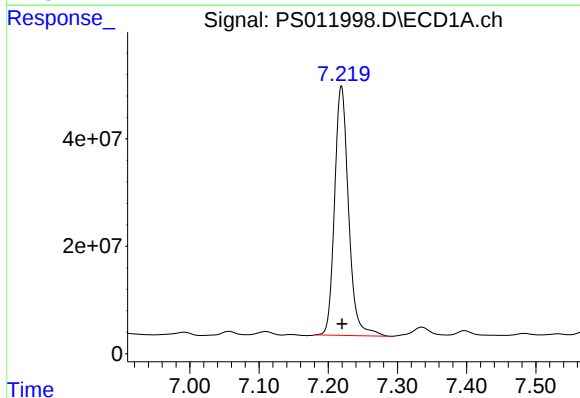


#4 2,4-DCAA

R.T.: 7.219 min
Delta R.T.: -0.001 min
Response: 650478723
Conc: 596.35 ng/ml

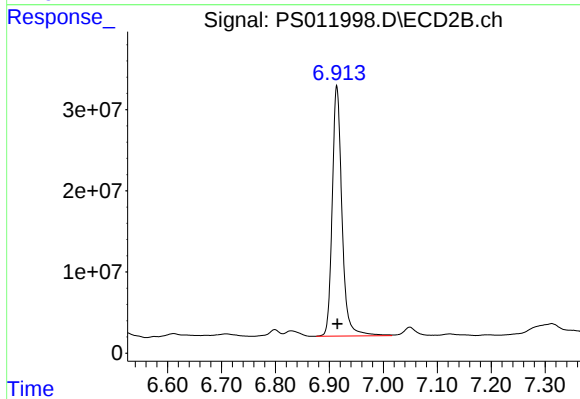

#4 2,4-DCAA


R.T.: 6.914 min
Delta R.T.: -0.001 min
Response: 386856807
Conc: 723.39 ng/ml

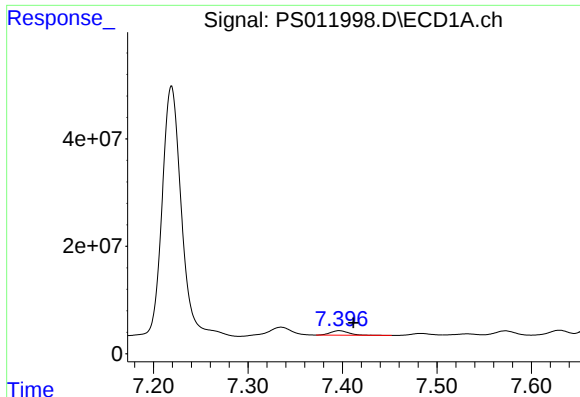

#5 DICAMBA


R.T.: 7.397 min
Delta R.T.: -0.015 min
Response: 11149884
Conc: 2.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

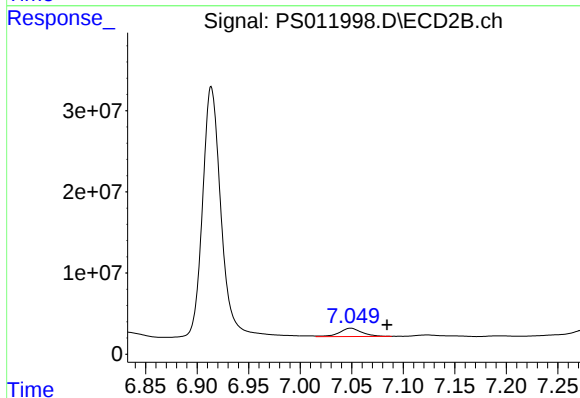


#5 DICAMBA

R.T.: 7.049 min
Delta R.T.: -0.035 min
Response: 15101647
Conc: 6.99 ng/ml

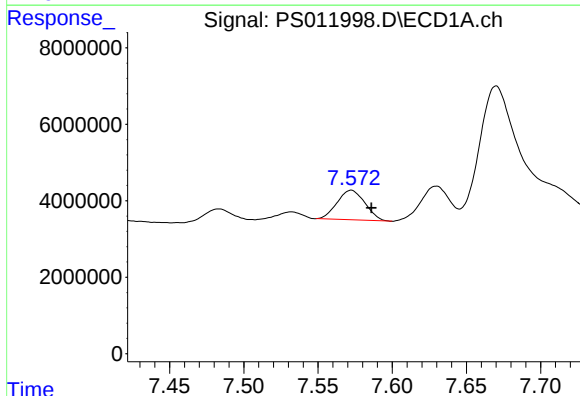


#6 MCP

R.T.: 7.572 min
Delta R.T.: -0.014 min
Response: 10096325
Conc: 3.16 ug/ml

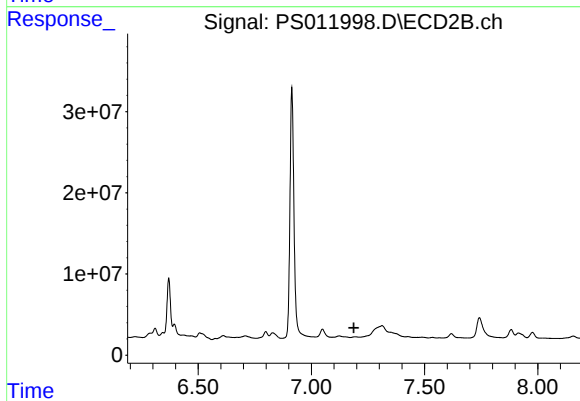

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

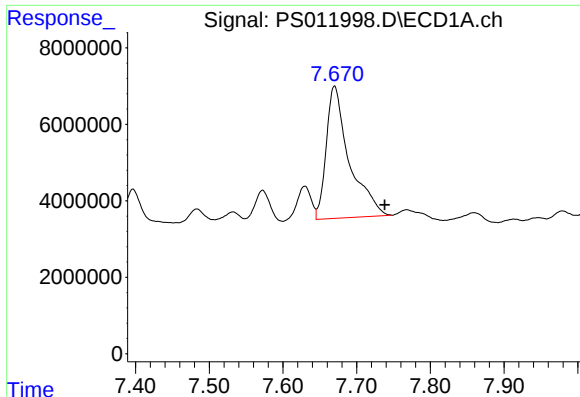

#7 MCPA


R.T.: 7.670 min
Delta R.T.: -0.068 min
Response: 75218468
Conc: 16.54 ug/ml

Instrument :
ECD_S
ClientSampleId :

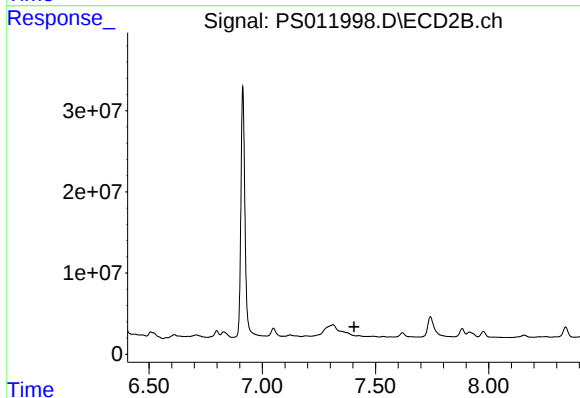


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.405 min
Response: 0
Conc: N.D.

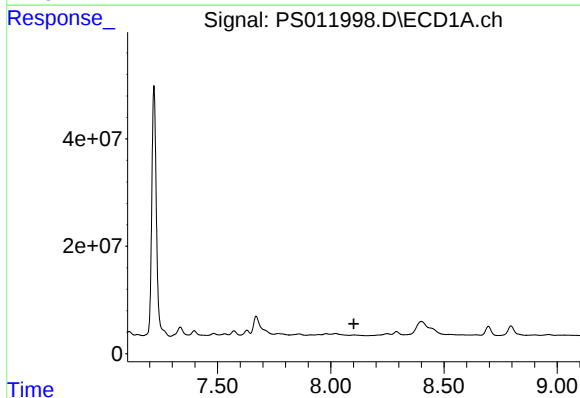


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

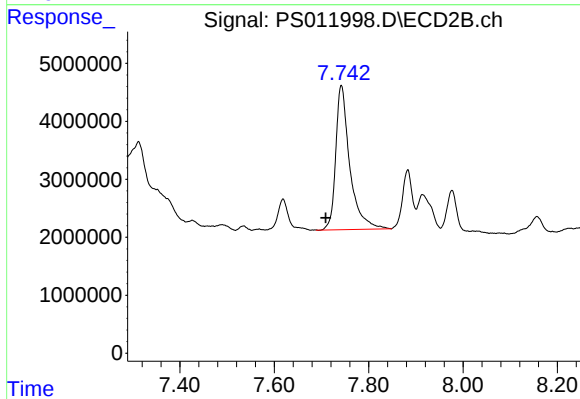

#8 DICHLORPROP


R.T.: 7.742 min
Delta R.T.: 0.033 min
Response: 51366184
Conc: 90.97 ng/ml

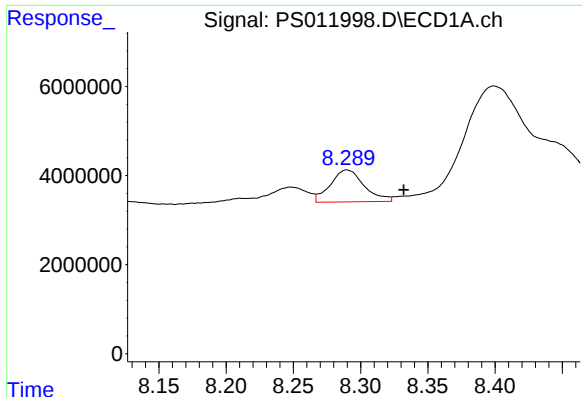

#9 2,4-D


R.T.: 8.290 min
Delta R.T.: -0.042 min
Response: 12482466
Conc: 11.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

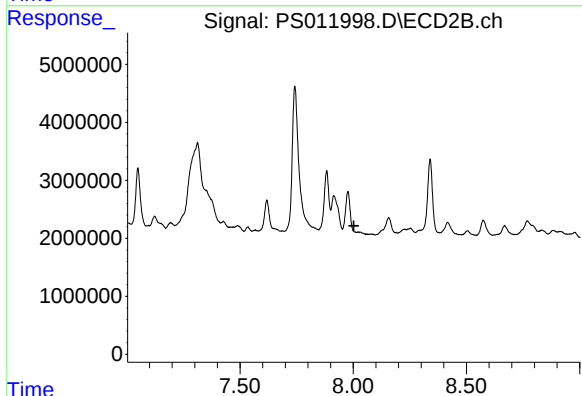


#9 2,4-D

R.T.: 7.976 min
Delta R.T.: -0.027 min
Response: -1789691
Conc: N.D.

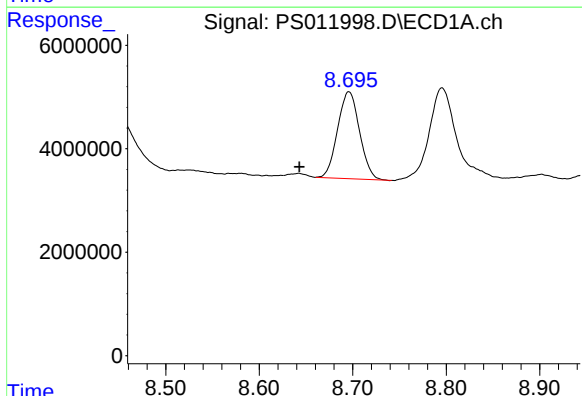


#10 Pentachlorophenol

R.T.: 8.696 min
Delta R.T.: 0.053 min
Response: 27431758
Conc: 1.91 ng/ml

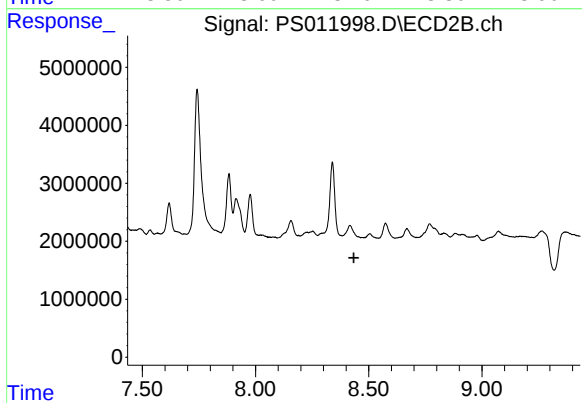

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.434 min
Response: 0
Conc: N.D.

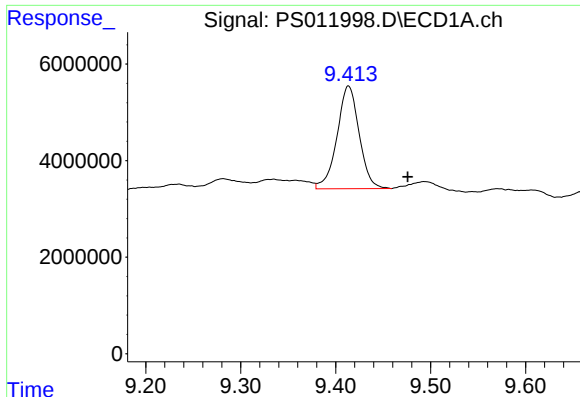

#12 2,4,5-T


R.T.: 9.414 min
Delta R.T.: -0.062 min
Response: 34432782
Conc: 5.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

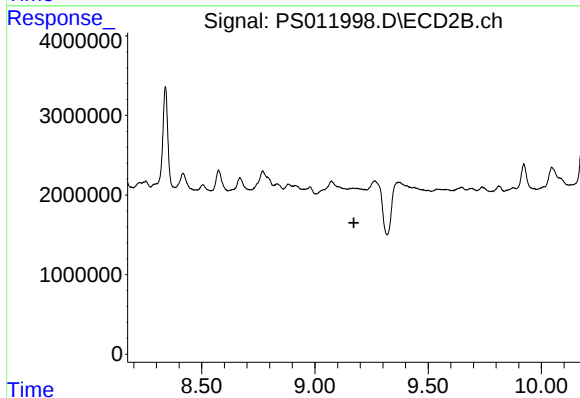


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

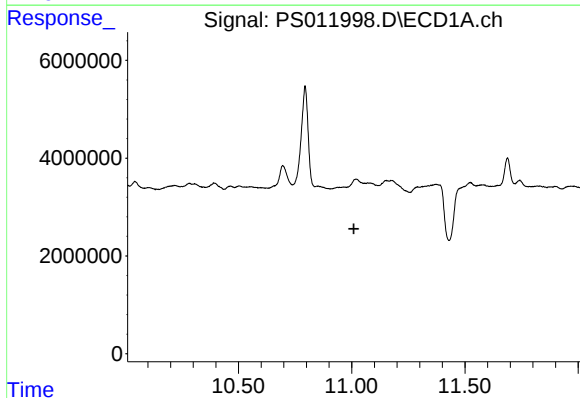


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.009 min
Response: 0
Conc: N.D.

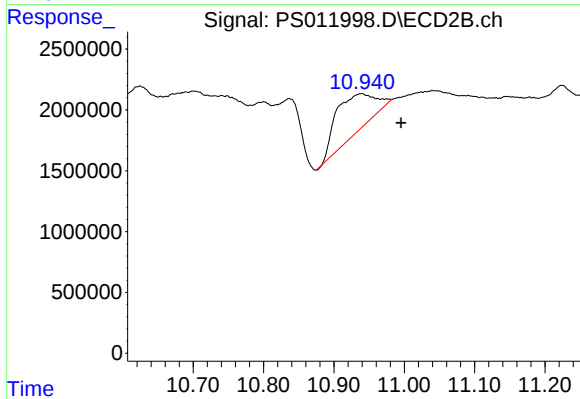

#15 Picloram


R.T.: 10.939 min
Delta R.T.: -0.056 min
Response: 12117829
Conc: 2.67 ng/ml

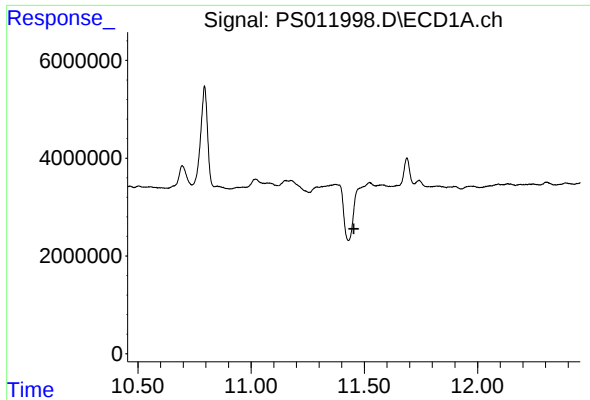

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.454 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

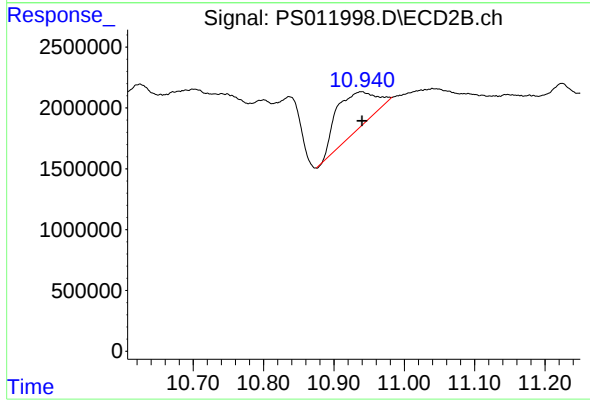

#16 DCPA

R.T.: 10.939 min
Delta R.T.: -0.001 min
Response: 12117829
Conc: 3.30 ng/ml