

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090120\
 Data File : PS012004.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2020 14:00
 Operator : DD\AJ
 Sample : L3712-18RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 14:17:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.218	6.914	902.7E6	531.4E6	827.605	993.593
Target Compounds							
2) T	3,5-DICHL...	6.474	6.095	1771357	83677327	1.222	101.721 #
3) T	4-Nitroph...	7.055	0.000	792524	0	1.345	N.D. #
5) T	DICAMBA	7.396	7.074	7368365	21973138	1.799	10.170 #
7) T	MCPA	7.685	7.467	270.6E6	100.6E6	59.488	36.717 #
8) T	DICHLORPROP	0.000	7.734	0	57639434	N.D.	102.082
9) T	2,4-D	8.400	0.000	147.4E6	0	130.550	N.D. #
11) T	2,4,5-TP ...	0.000	8.750	0	23619773	N.D.	8.079
12) T	2,4,5-T	9.412	0.000	45009002	0	7.595	N.D. #
15) T	Picloram	10.974	0.000	39812928	0	5.094	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090120\
Data File : PS012004.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2020 14:00
Operator : DD\AJ
Sample : L3712-18RE
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 14:17:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

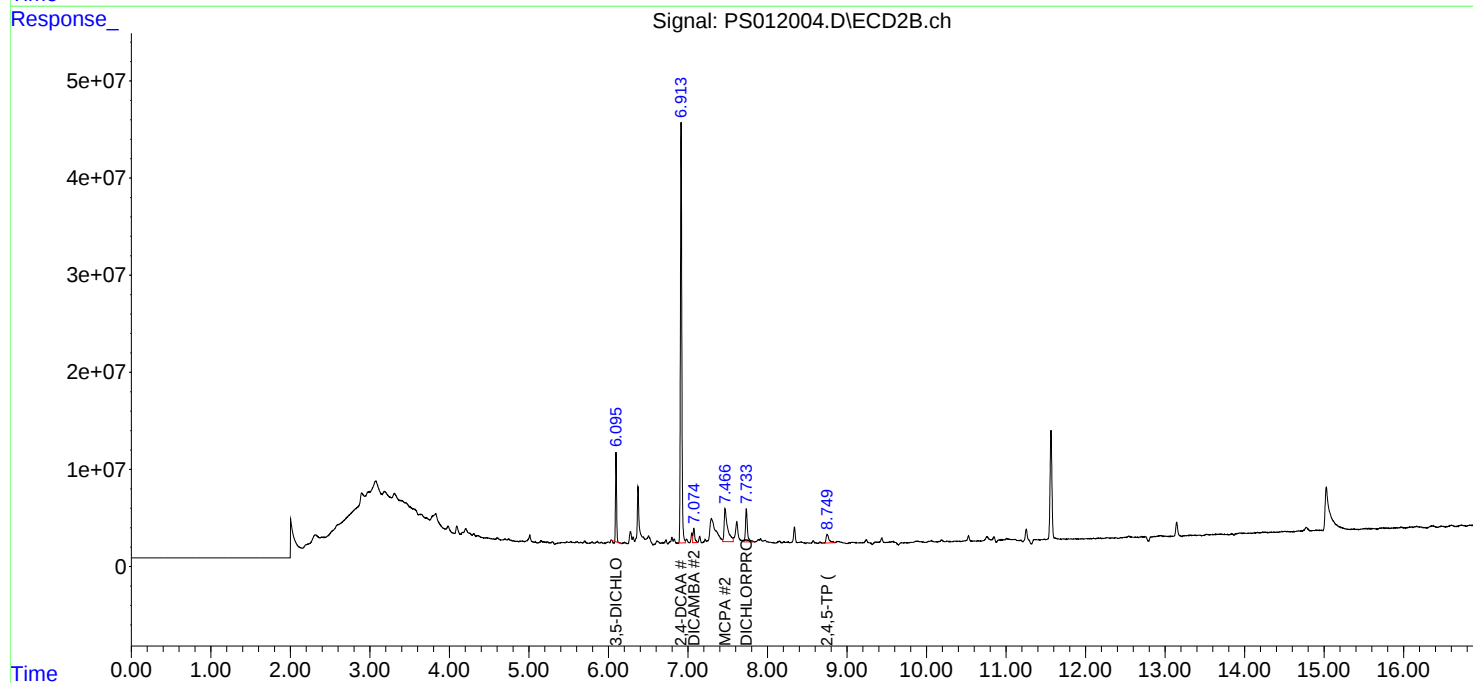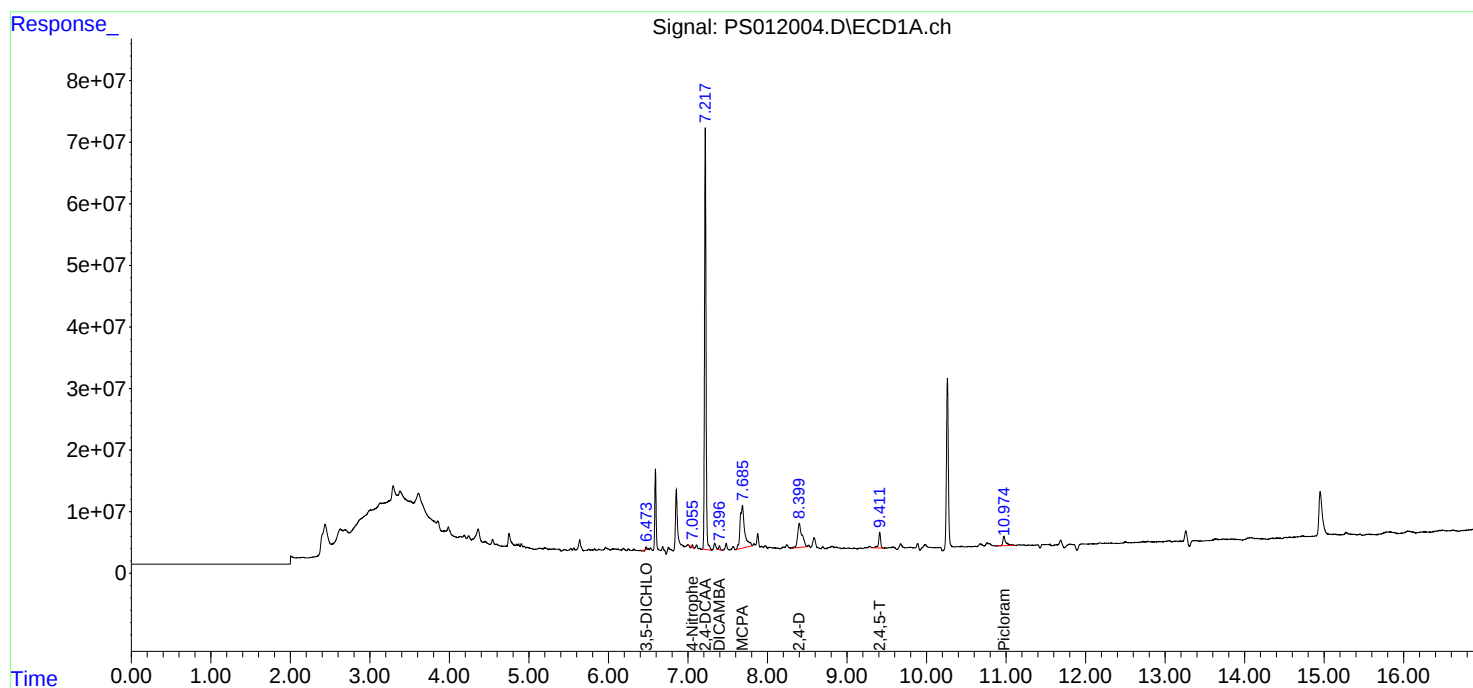


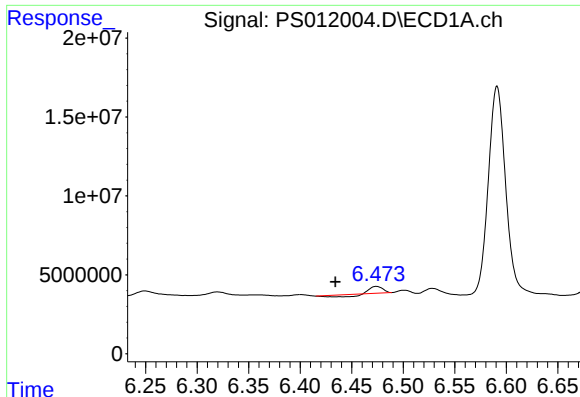

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.474 min
Delta R.T.: 0.040 min
Response: 1771357
Conc: 1.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

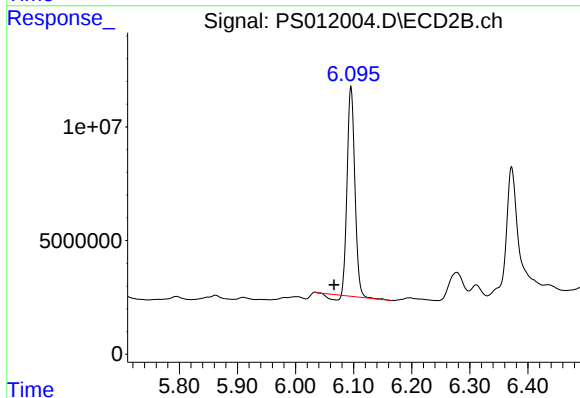


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.029 min
Response: 83677327
Conc: 101.72 ng/ml

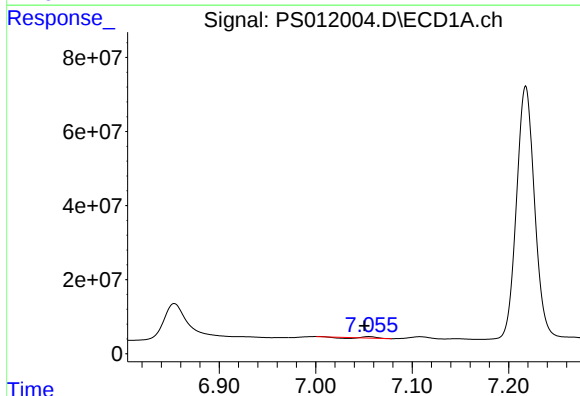


#3 4-Nitrophenol

R.T.: 7.055 min
Delta R.T.: 0.005 min
Response: 792524
Conc: 1.35 ng/ml

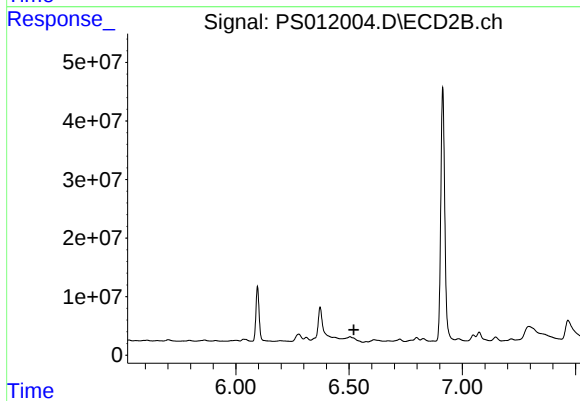

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

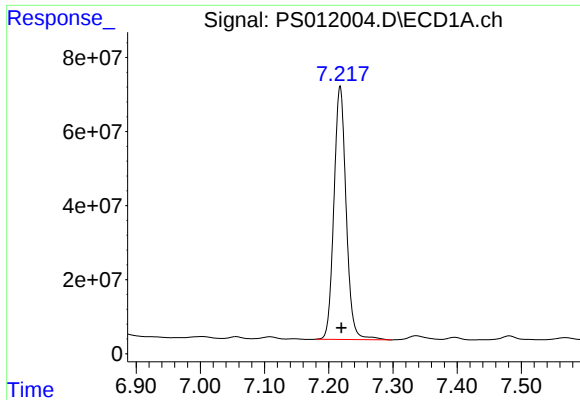

#4 2,4-DCAA


R.T.: 7.218 min
Delta R.T.: -0.002 min
Response: 902725367
Conc: 827.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

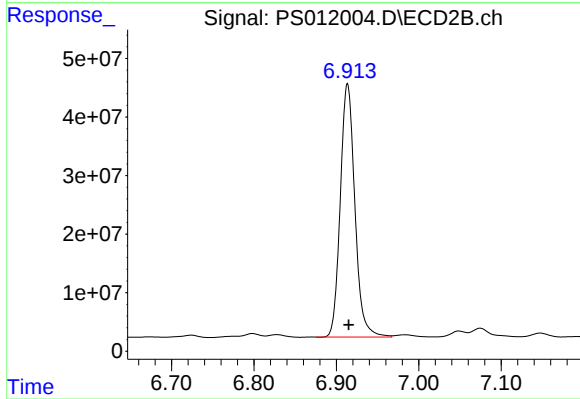


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: -0.002 min
Response: 531360336
Conc: 993.59 ng/ml

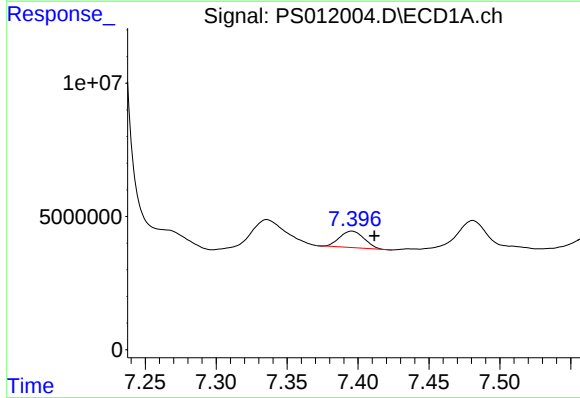


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.016 min
Response: 7368365
Conc: 1.80 ng/ml

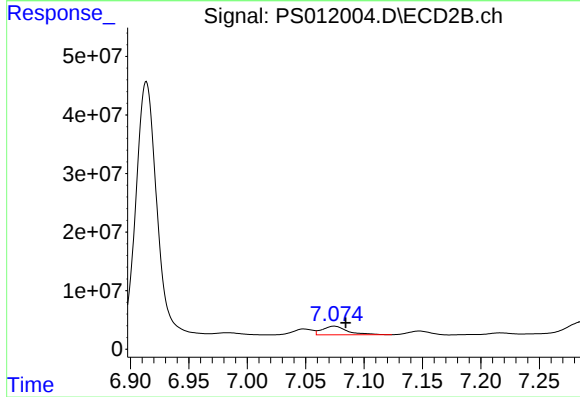

#5 DICAMBA


R.T.: 7.074 min
Delta R.T.: -0.010 min
Response: 21973138
Conc: 10.17 ng/ml

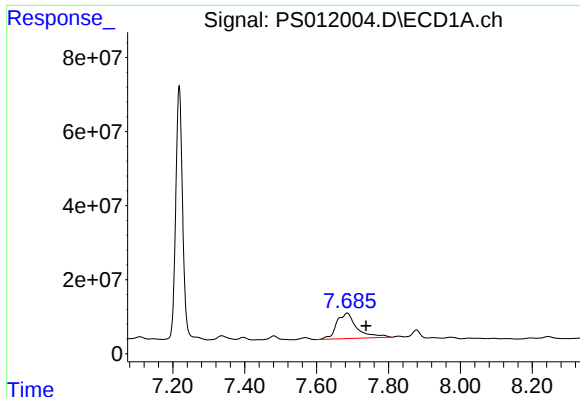

#7 MCPA


R.T.: 7.685 min
Delta R.T.: -0.053 min
Response: 270579222
Conc: 59.49 ug/ml

Instrument :
ECD_S
ClientSampleId :

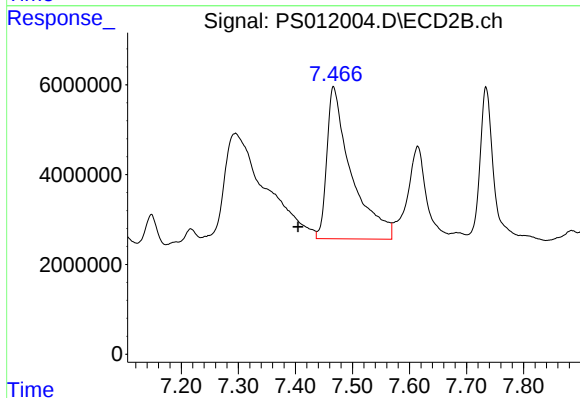


#7 MCPA

R.T.: 7.467 min
Delta R.T.: 0.062 min
Response: 100609020
Conc: 36.72 ug/ml

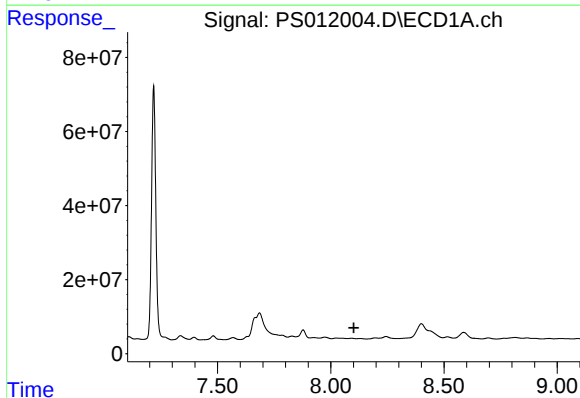


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

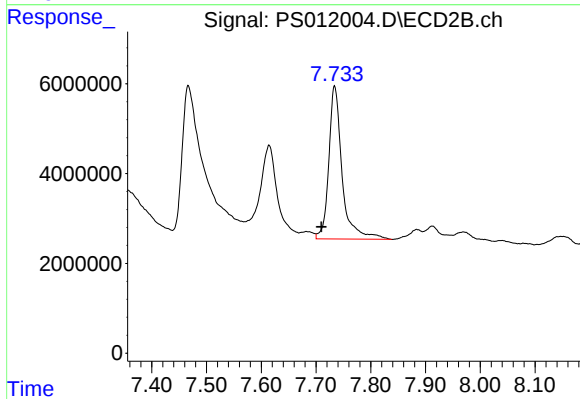

#8 DICHLORPROP


R.T.: 7.734 min
Delta R.T.: 0.025 min
Response: 57639434
Conc: 102.08 ng/ml

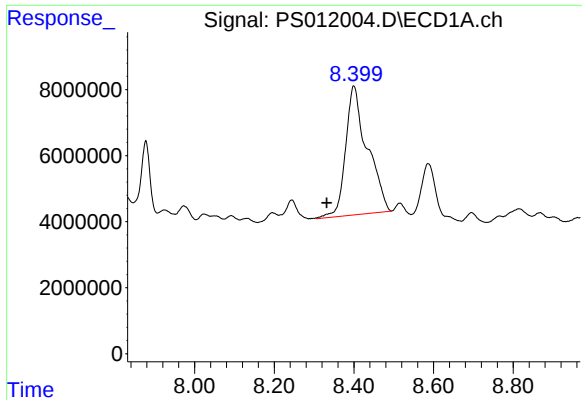

#9 2,4-D


R.T.: 8.400 min
Delta R.T.: 0.068 min
Response: 147402916
Conc: 130.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

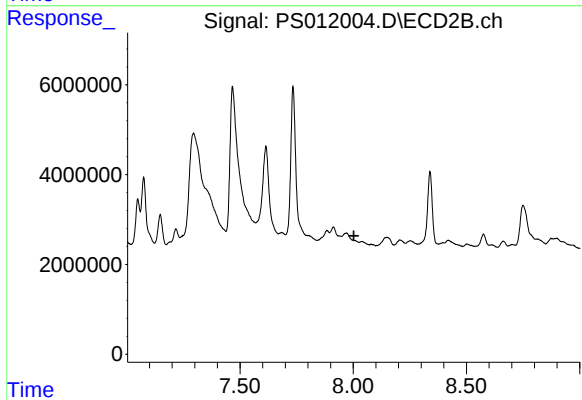


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

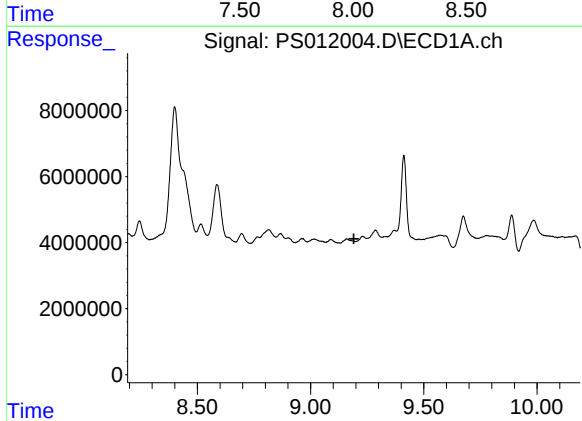


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

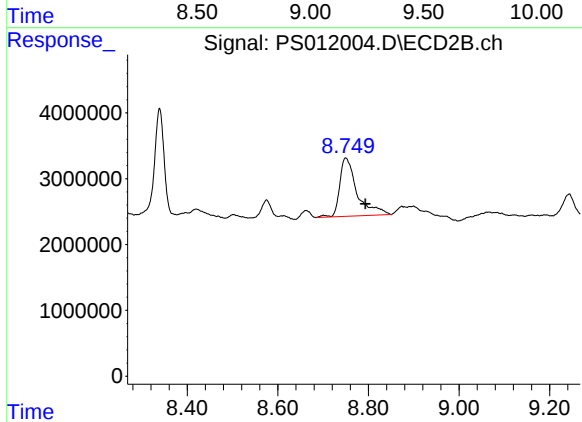

#11 2,4,5-TP (SILVEX)


R.T.: 8.750 min
Delta R.T.: -0.043 min
Response: 23619773
Conc: 8.08 ng/ml

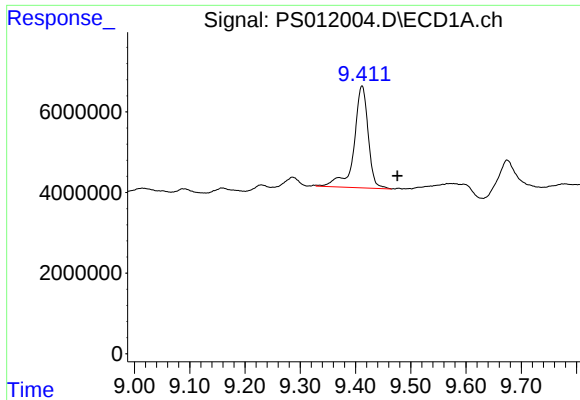

#12 2,4,5-T


R.T.: 9.412 min
Delta R.T.: -0.064 min
Response: 45009002
Conc: 7.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

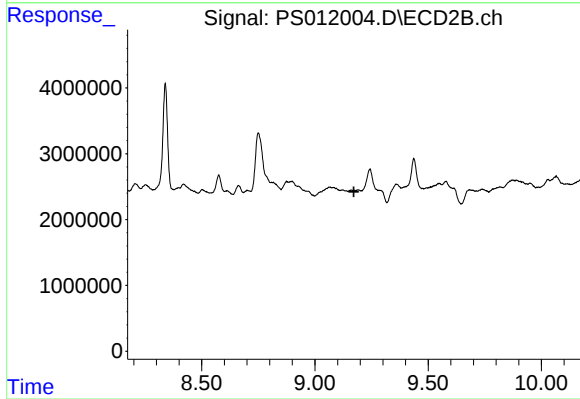


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

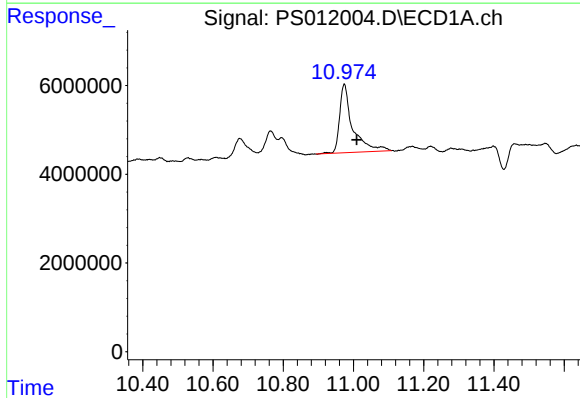

#15 Picloram

R.T.: 10.974 min
Delta R.T.: -0.036 min
Response: 39812928
Conc: 5.09 ng/ml

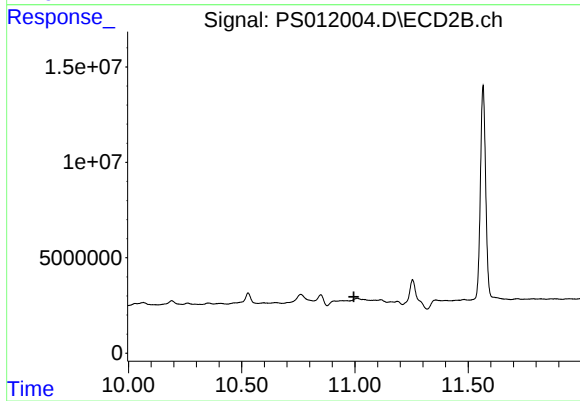

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.