

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\ps090122\
 Data File : PS020416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2022 10:42
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 01:03:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.207	6.801	2069901	1273900	<MDL	1.563 #
Target Compounds							
1) T	Dalapon	3.040	0.000	1667241	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.446f	0.000	31925373	0	8.207	N.D. #
3) T	4-Nitroph...	7.058	0.000	192940	0	<MDL	N.D. #
5) T	DICAMBA	7.375	6.867f	4851224	515803	<MDL	<MDL #
6) T	MCP	7.597f	6.981	-2569309	10067657	N.D.	3.691
7) T	MCPA	7.684	0.000	11036495	0	<MDL	N.D. #
8) T	DICHLORPROP	8.077	7.600f	-2888774	1944841	N.D.	2.080
9) T	2,4-D	8.310	0.000	1060202	0	<MDL	N.D. #
10) T	Pentachlo...	8.602	0.000	5862068	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.158	0.000	1234379	0	<MDL	N.D. #
12) T	2,4,5-T	9.392f	9.015	56738241	4448168	3.126	<MDL #
13) T	2,4-DB	9.952	0.000	1892932	0	<MDL	N.D. #
15) T	Picloram	10.947	10.835	146.0E6	69608328	4.619	9.226 #
16) T	DCPA	11.402	10.743	3251502	1899855	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\ps090122\
Data File : PS020416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2022 10:42
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 01:03:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

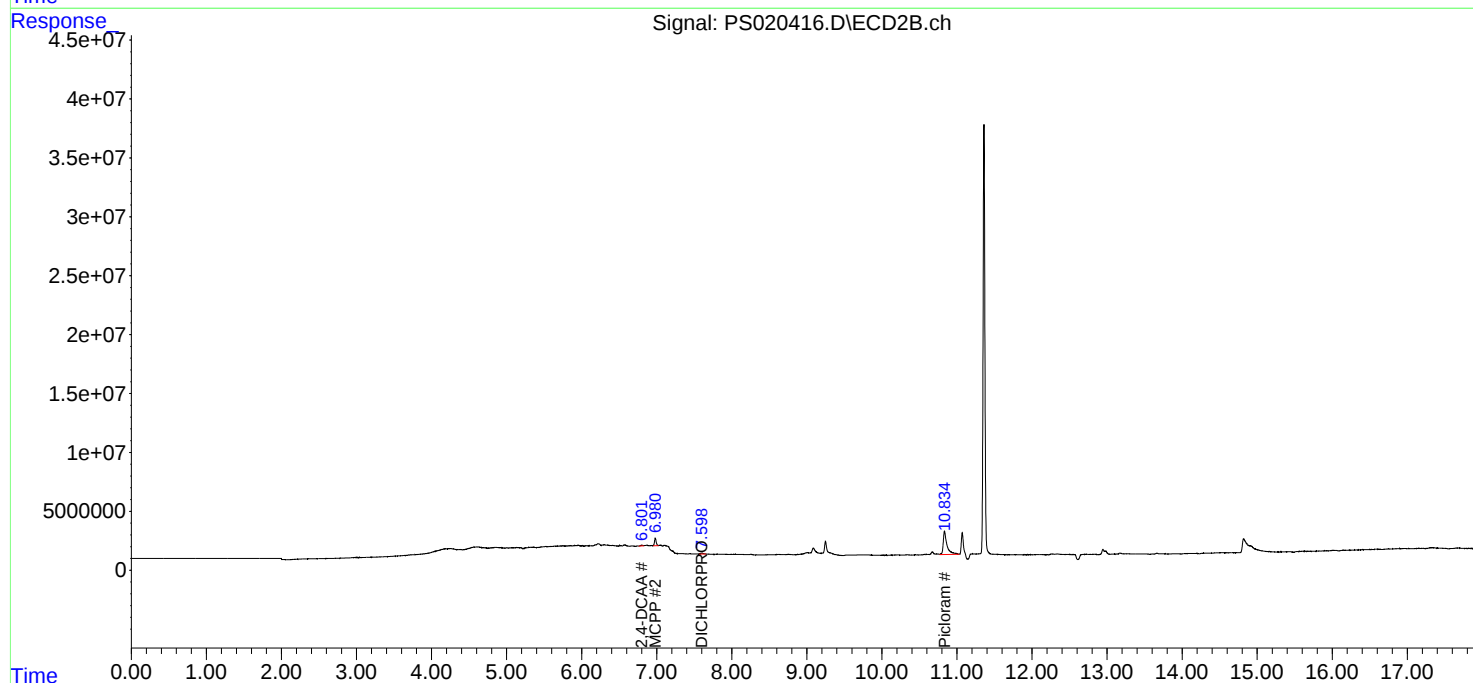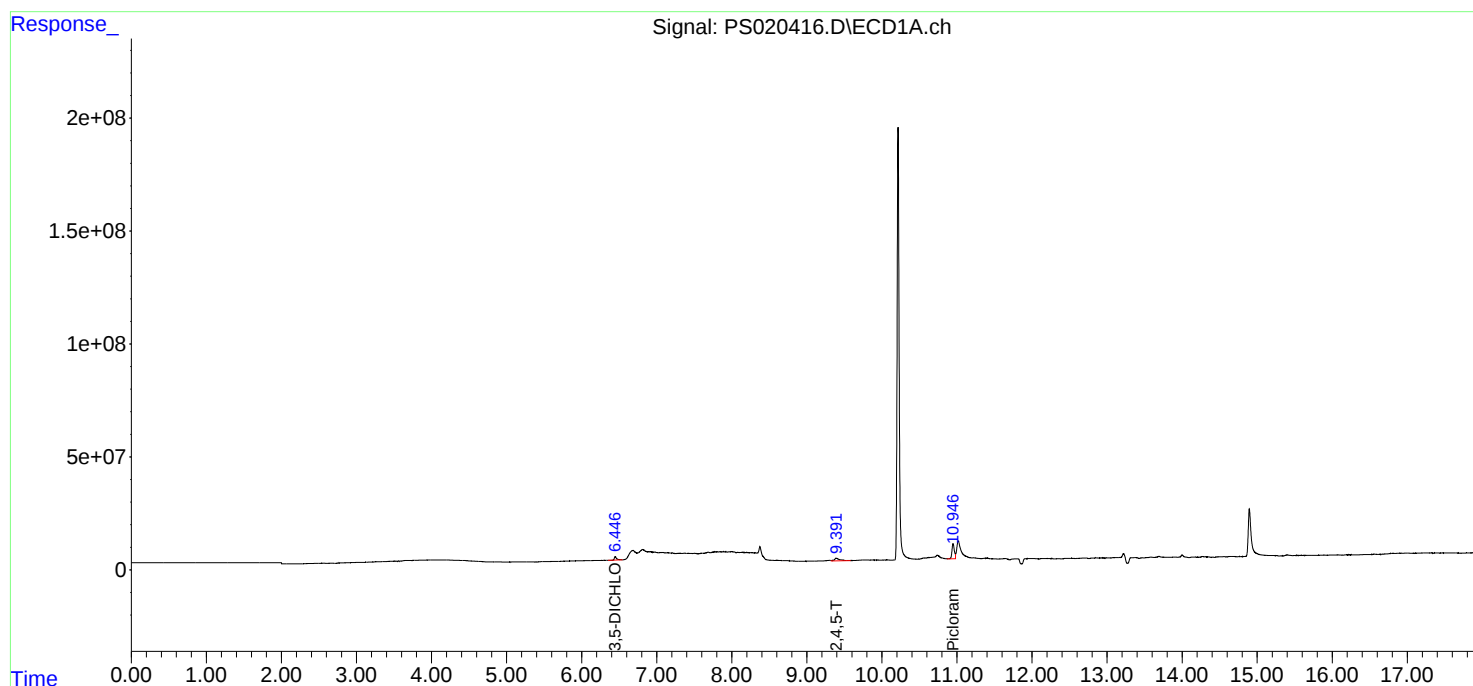


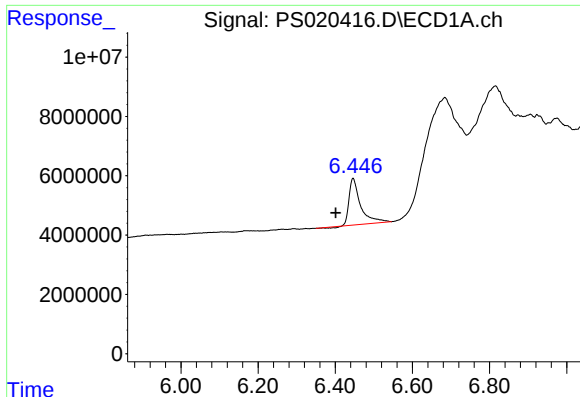

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.446 min
Delta R.T.: 0.045 min
Response: 31925373
Conc: 8.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

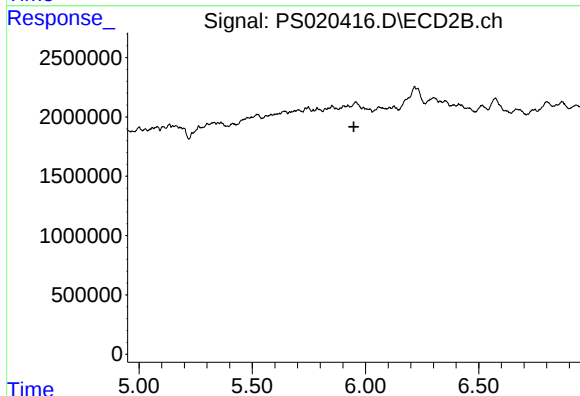


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

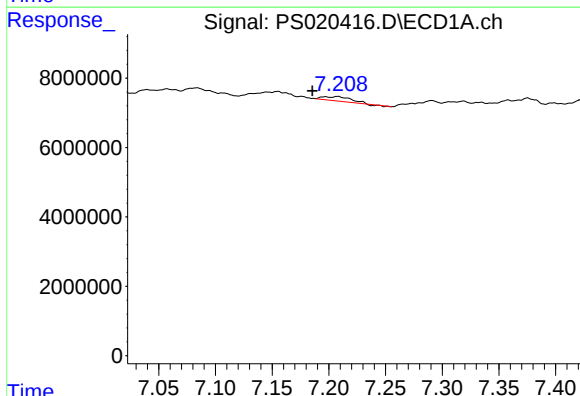


#4 2,4-DCAA

R.T.: 7.207 min
Delta R.T.: 0.022 min
Response: 2069901
Conc: N.D.

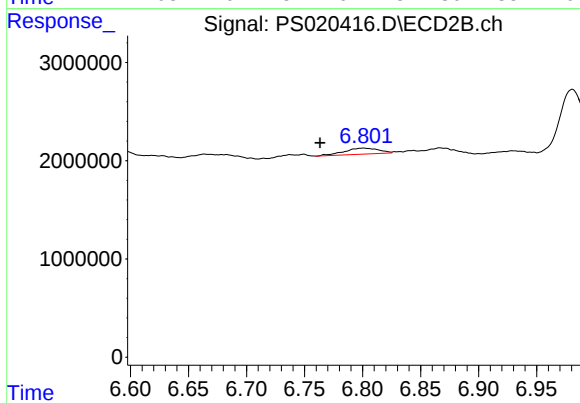

#4 2,4-DCAA


R.T.: 6.801 min
Delta R.T.: 0.037 min
Response: 1273900
Conc: 1.56 ng/ml

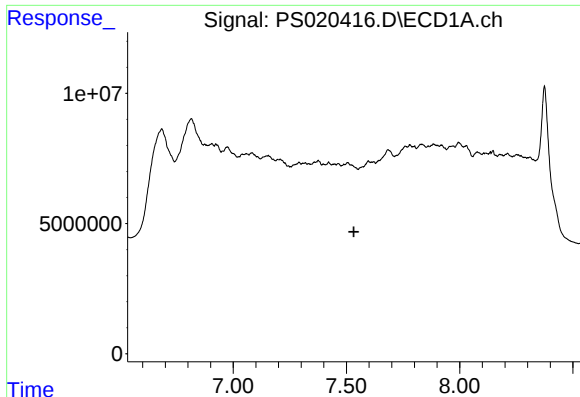

#6 MCP


R.T.: 7.597 min
Delta R.T.: 0.063 min
Response: -2569309
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

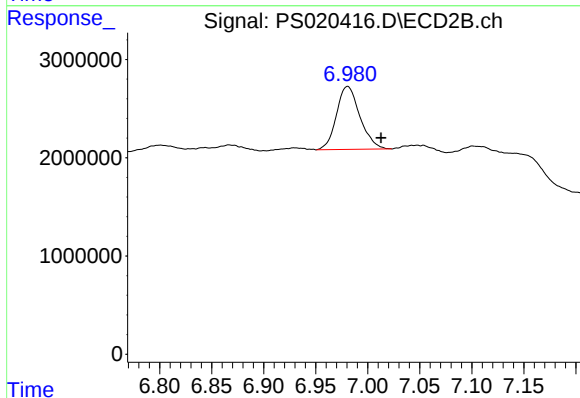


#6 MCP

R.T.: 6.981 min
Delta R.T.: -0.032 min
Response: 10067657
Conc: 3.69 ug/ml

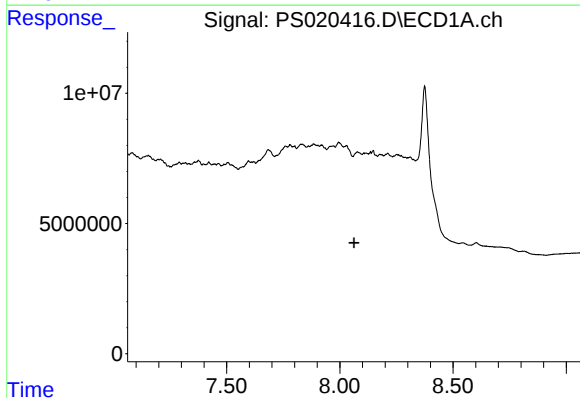


#8 DICHLORPROP

R.T.: 8.077 min
Delta R.T.: 0.015 min
Response: -2888774
Conc: N.D.

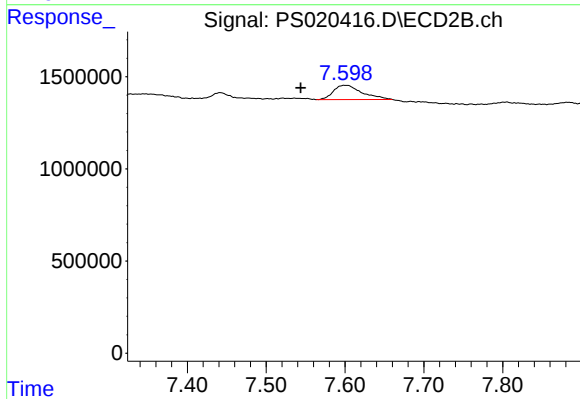

#8 DICHLORPROP


R.T.: 7.600 min
Delta R.T.: 0.056 min
Response: 1944841
Conc: 2.08 ng/ml

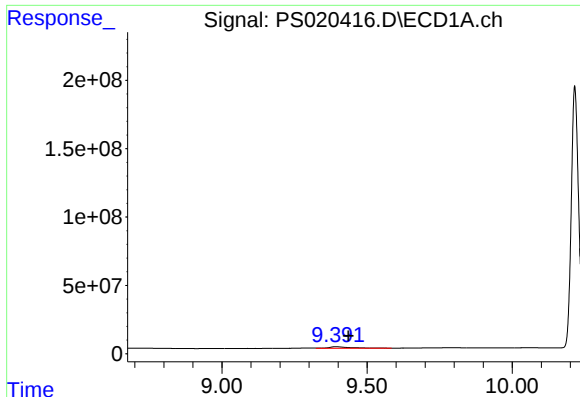

#12 2,4,5-T


R.T.: 9.392 min
Delta R.T.: -0.044 min
Response: 56738241
Conc: 3.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

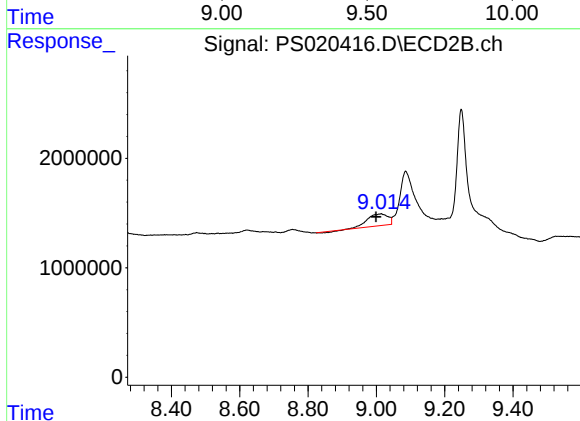


#12 2,4,5-T

R.T.: 9.015 min
Delta R.T.: 0.016 min
Response: 4448168
Conc: N.D.

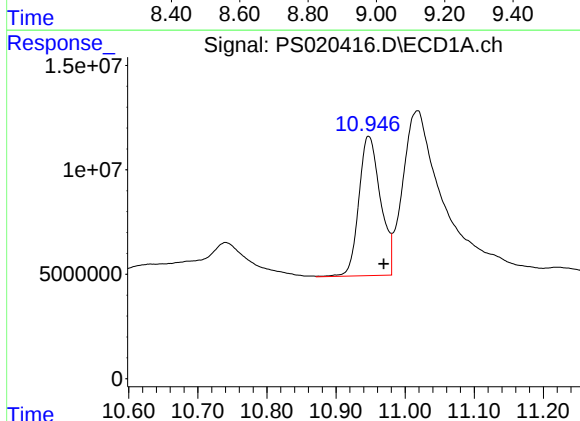

#15 Picloram

R.T.: 10.947 min
Delta R.T.: -0.022 min
Response: 146042464
Conc: 4.62 ng/ml

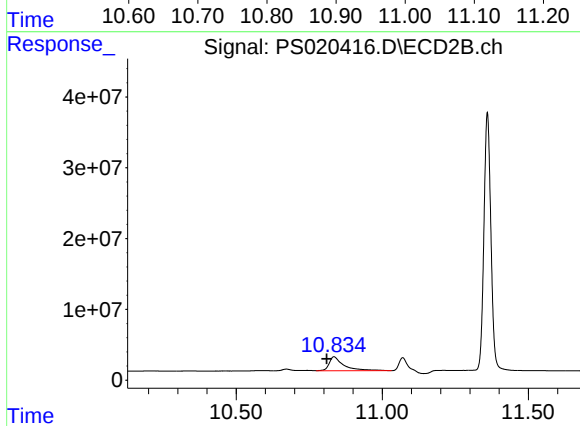

#15 Picloram

R.T.: 10.835 min
Delta R.T.: 0.024 min
Response: 69608328
Conc: 9.23 ng/ml