

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\ps090122\
 Data File : PS020417.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2022 11:06
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 01:04:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.184	6.760	1476.2E6	460.0E6	500.633	564.454
Target Compounds							
2) T	3,5-DICHL...	6.437	0.000	1915.3E6	0	492.381	N.D. #
3) T	4-Nitroph...	0.000	6.373	0	478665	N.D.	<MDL
5) T	DICAMBA	7.437f	6.978f	4575354	605.2E6	<MDL	169.796 #
6) T	MCP	0.000	6.978	0	605.2E6	N.D.	221.848
11) T	2,4,5-TP ...	9.165	0.000	2138042	0	<MDL	N.D. #
12) T	2,4,5-T	9.431	0.000	21713481	0	1.196	N.D. #
13) T	2,4-DB	0.000	9.551f	0	3167758	N.D.	4.658
14) T	DINOSEB	0.000	9.828	0	1530155	N.D.	<MDL
15) T	Picloram	10.933	10.771	1419.4E6	3980207	44.893	<MDL #
16) T	DCPA	11.409	10.771	3935397	3980207	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\ps090122\
Data File : PS020417.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2022 11:06
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 01:04:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

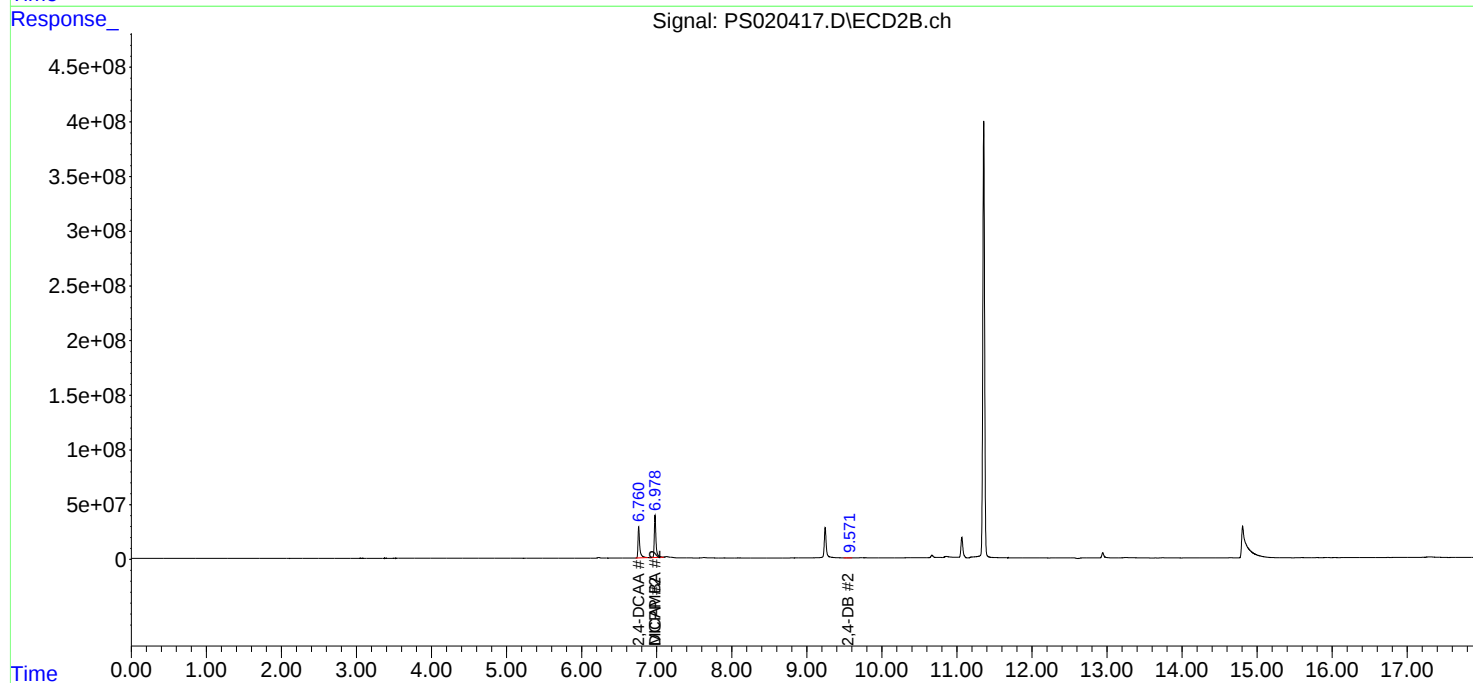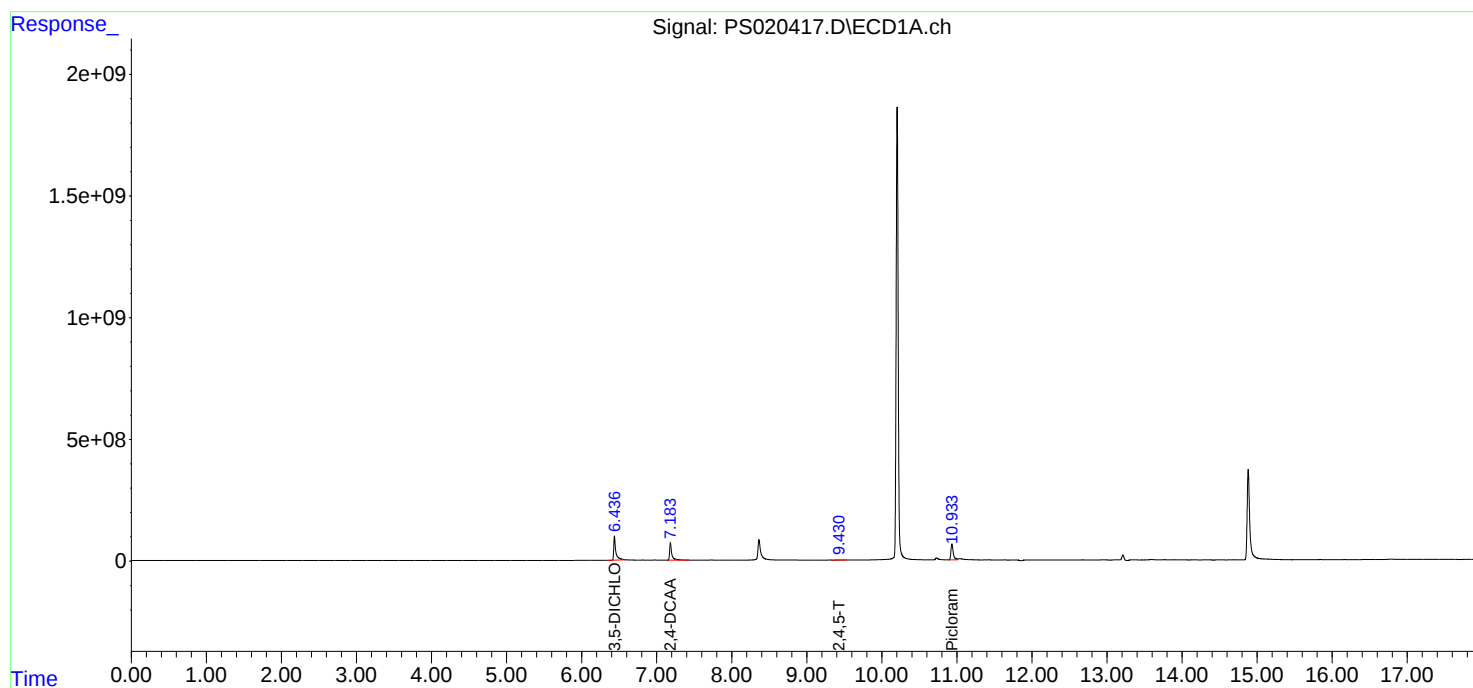


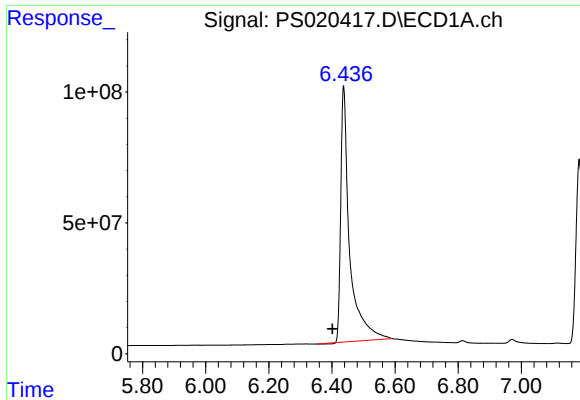

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.437 min
Delta R.T.: 0.036 min
Response: 1915315238
Conc: 492.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

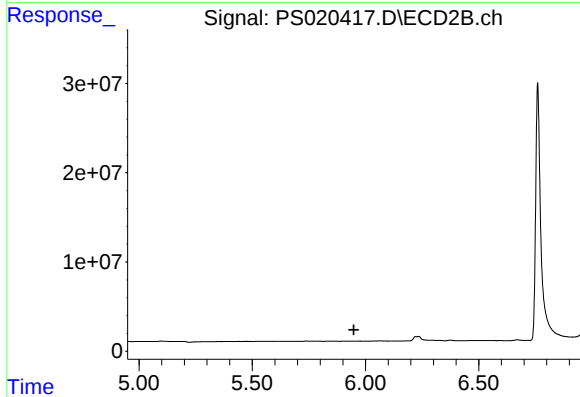


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

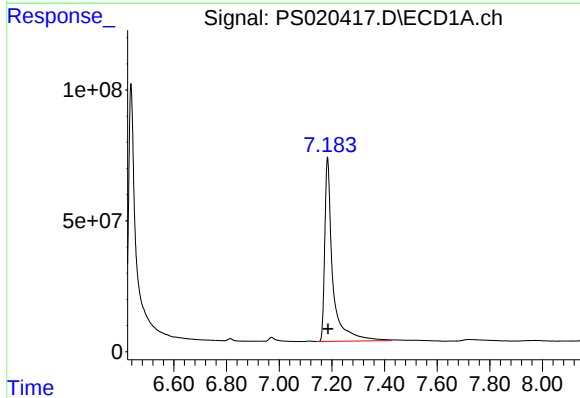


#4 2,4-DCAA

R.T.: 7.184 min
Delta R.T.: -0.002 min
Response: 1476229419
Conc: 500.63 ng/ml

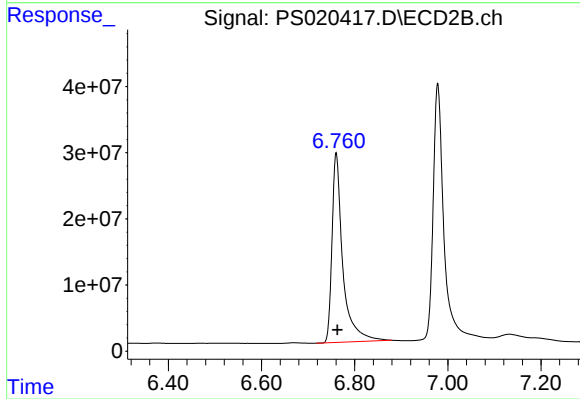

#4 2,4-DCAA


R.T.: 6.760 min
Delta R.T.: -0.003 min
Response: 460004740
Conc: 564.45 ng/ml

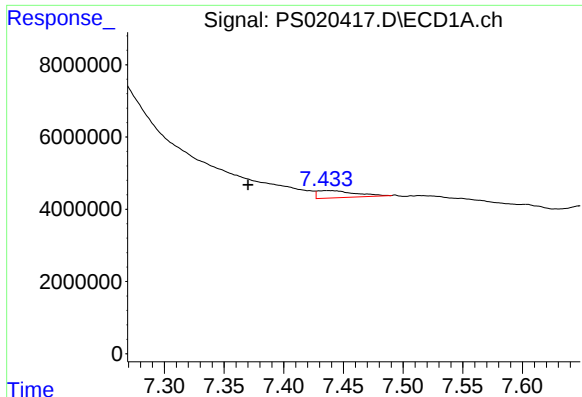

#5 DICAMBA


R.T.: 7.437 min
Delta R.T.: 0.067 min
Response: 4575354
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

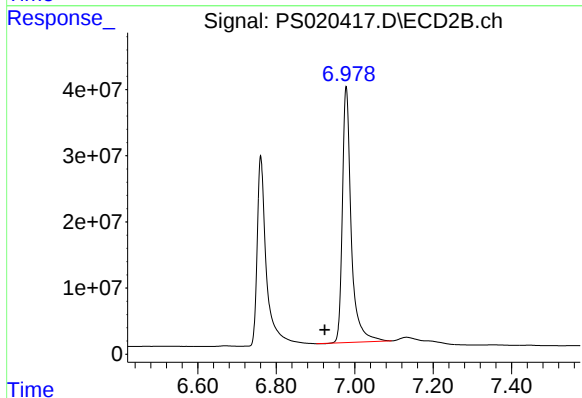


#5 DICAMBA

R.T.: 6.978 min
Delta R.T.: 0.055 min
Response: 605173987
Conc: 169.80 ng/ml

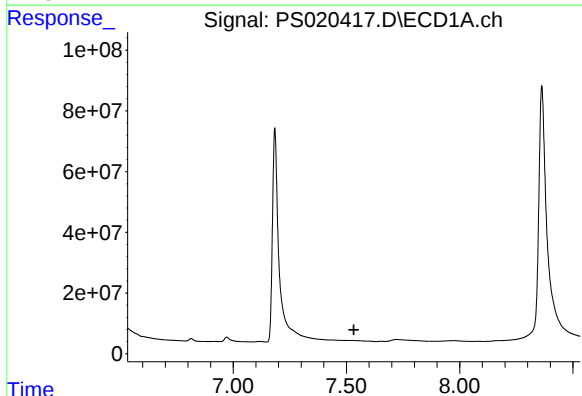


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.533 min
Response: 0
Conc: N.D.

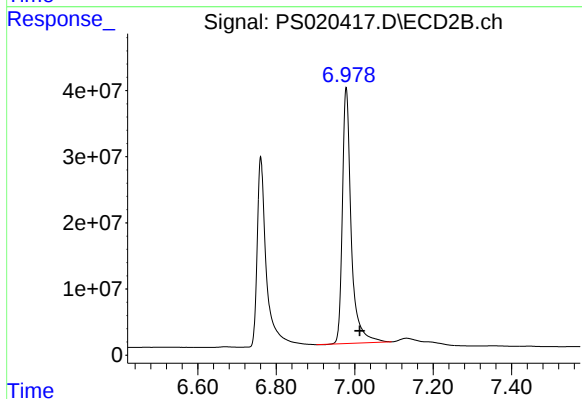

#6 MCP


R.T.: 6.978 min
Delta R.T.: -0.035 min
Response: 605173987
Conc: 221.85 ug/ml

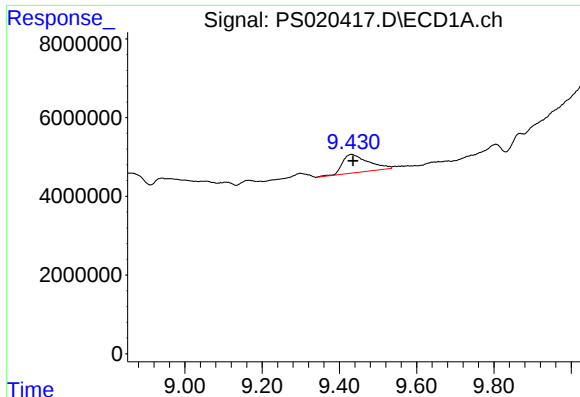

#12 2,4,5-T


R.T.: 9.431 min
Delta R.T.: -0.005 min
Response: 21713481
Conc: 1.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

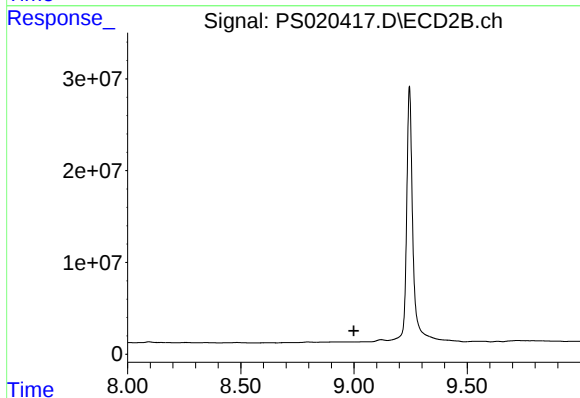


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.999 min
Response: 0
Conc: N.D.

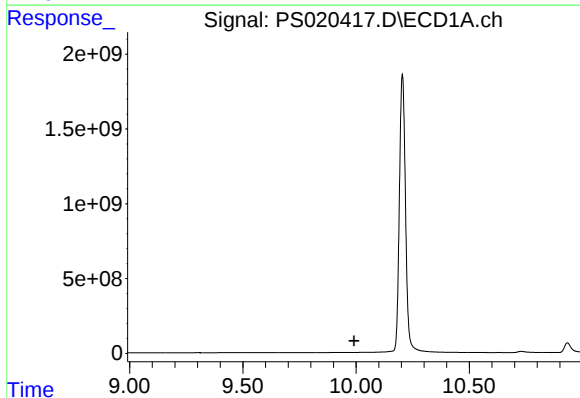


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.991 min
Response: 0
Conc: N.D.

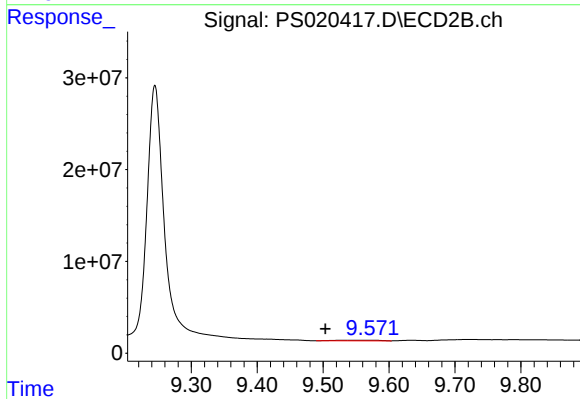

#13 2,4-DB


R.T.: 9.551 min
Delta R.T.: 0.048 min
Response: 3167758
Conc: 4.66 ng/ml

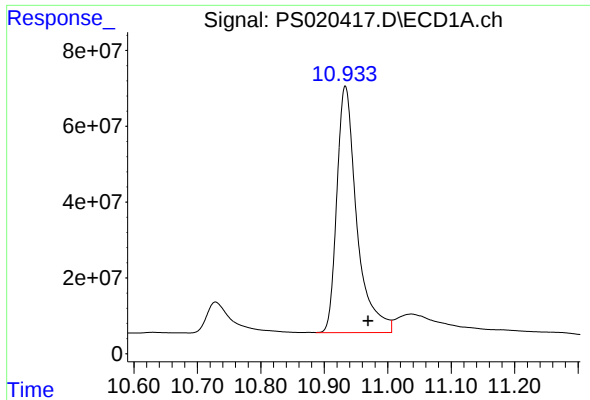

#15 Picloram

R.T.: 10.933 min
Delta R.T.: -0.036 min
Response: 1419437283
Conc: 44.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

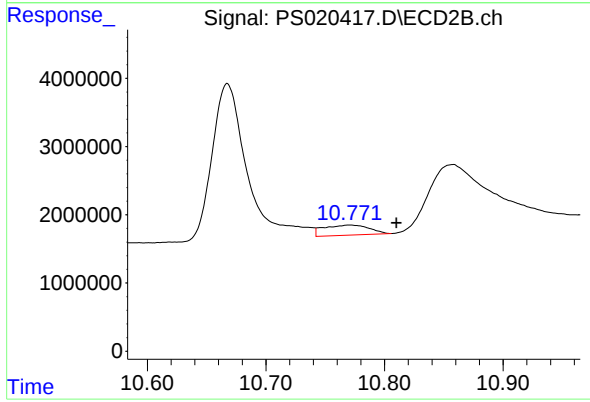

#15 Picloram

R.T.: 10.771 min
Delta R.T.: -0.039 min
Response: 3980207
Conc: N.D.