

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\ps090122\
 Data File : PS020424.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2022 18:32
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 01:06:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.182	6.760	1493.5E6	469.1E6	506.488	575.620
Target Compounds							
2) T	3,5-DICHL...	6.436	0.000	2004.4E6	0	515.286	N.D. #
3) T	4-Nitroph...	6.969f	6.370	2711369	541757	1.952	1.103 #
5) T	DICAMBA	0.000	6.978f	0	644.3E6	N.D.	180.771
6) T	MCP	0.000	6.978	0	644.3E6	N.D.	236.188
7) T	MCPA	7.691	0.000	61718714	0	4.792	N.D. #
8) T	DICHLORPROP	8.081	7.606f	47569	15274448	<MDL	16.334 #
11) T	2,4,5-TP ...	9.161	0.000	2804271	0	<MDL	N.D. #
12) T	2,4,5-T	9.424	9.034	7795633	456977	<MDL	<MDL #
13) T	2,4-DB	0.000	9.535	0	4721754	N.D.	6.942
14) T	DINOSEB	11.177f	9.829	14138830	1546994	<MDL	<MDL #
15) T	Picloram	10.930	10.770f	1558.0E6	6025127	49.276	<MDL #
16) T	DCPA	11.425	10.770	5405530	6025127	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\ps090122\
Data File : PS020424.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2022 18:32
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 01:06:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

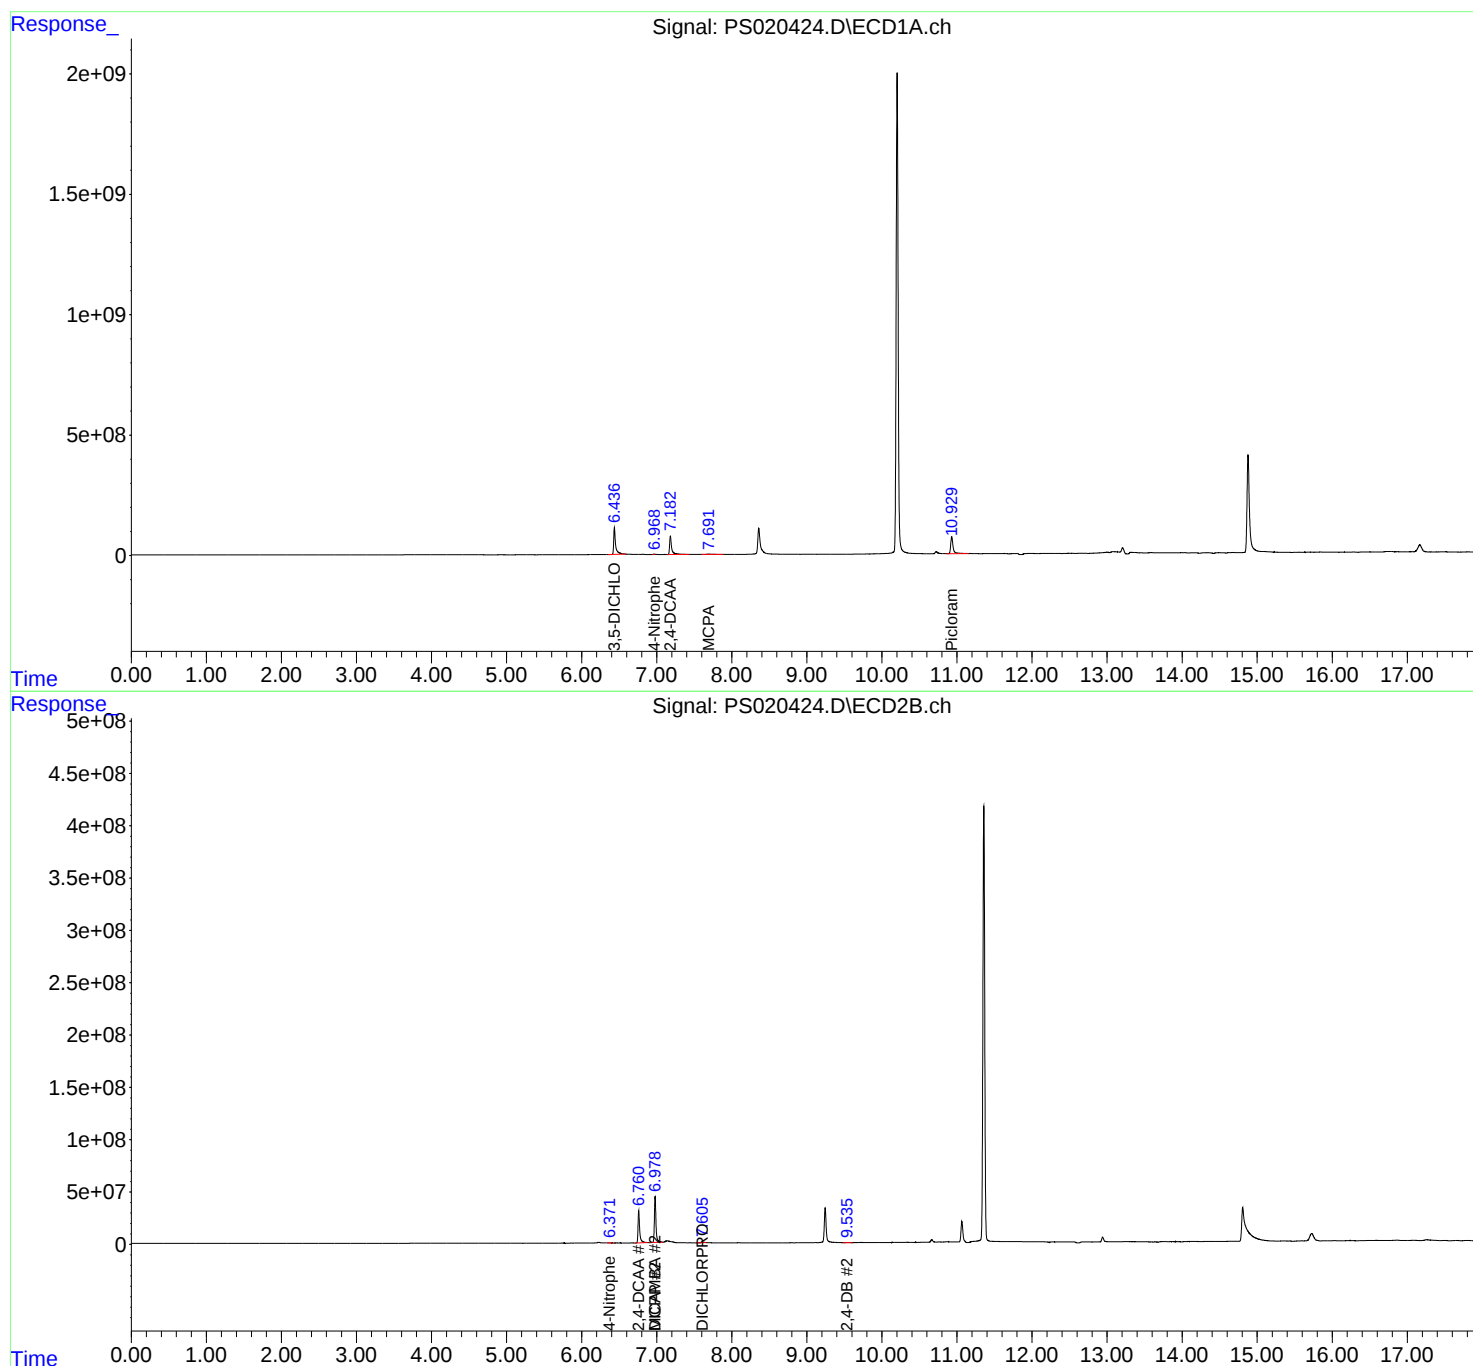


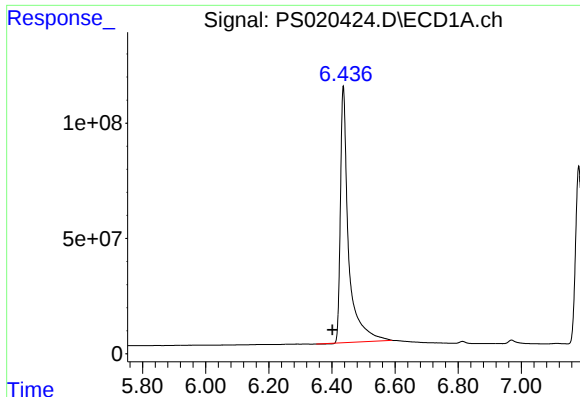

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.436 min
Delta R.T.: 0.035 min
Response: 2004412752
Conc: 515.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

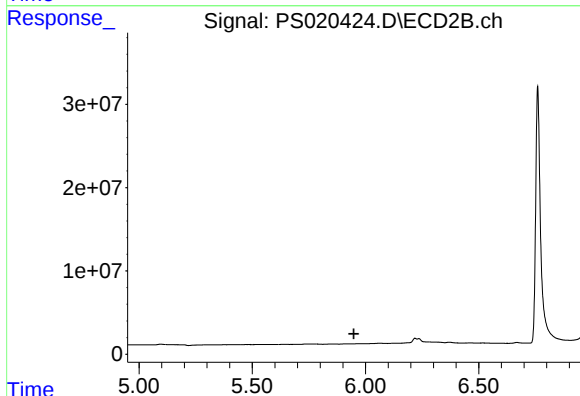


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

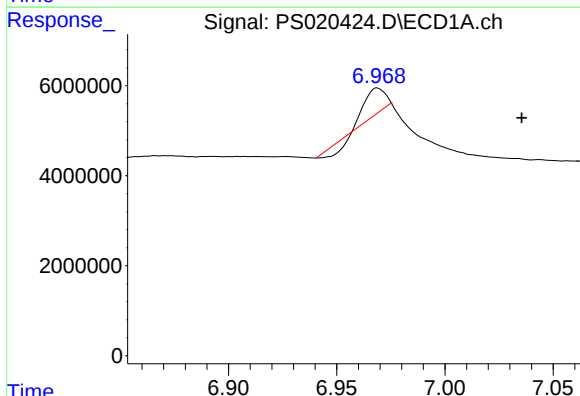


#3 4-Nitrophenol

R.T.: 6.969 min
Delta R.T.: -0.066 min
Response: 2711369
Conc: 1.95 ng/ml

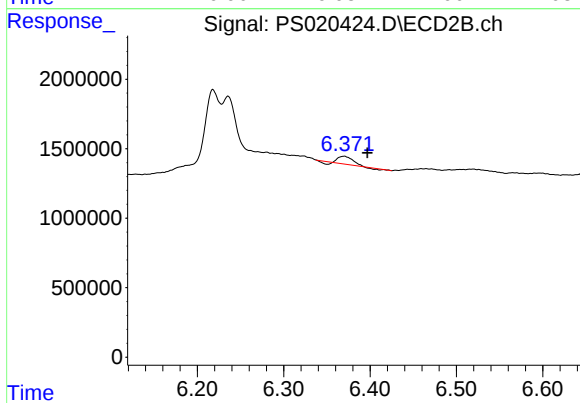

#3 4-Nitrophenol


R.T.: 6.370 min
Delta R.T.: -0.027 min
Response: 541757
Conc: 1.10 ng/ml

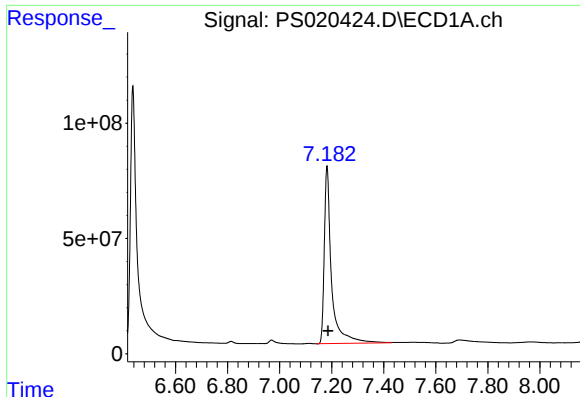

#4 2,4-DCAA


R.T.: 7.182 min
Delta R.T.: -0.003 min
Response: 1493494640
Conc: 506.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

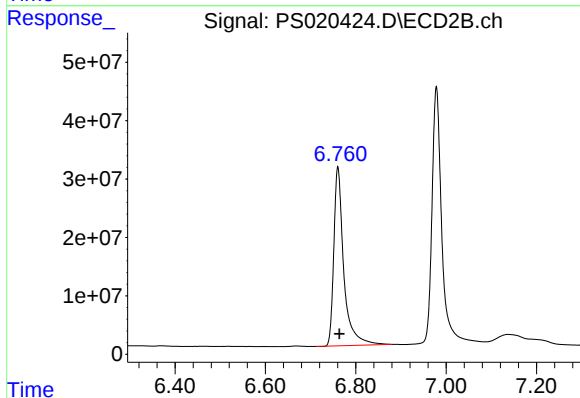


#4 2,4-DCAA

R.T.: 6.760 min
Delta R.T.: -0.003 min
Response: 469105017
Conc: 575.62 ng/ml

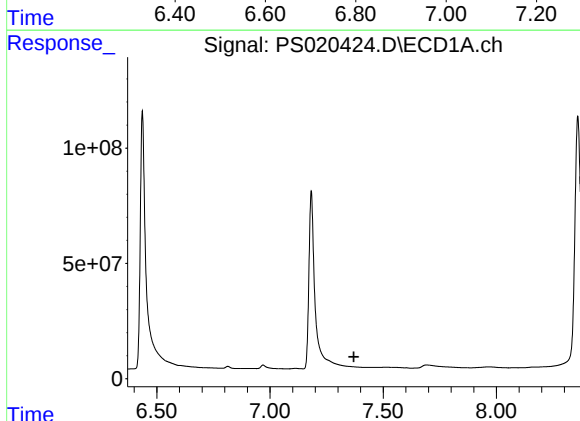


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.370 min
Response: 0
Conc: N.D.

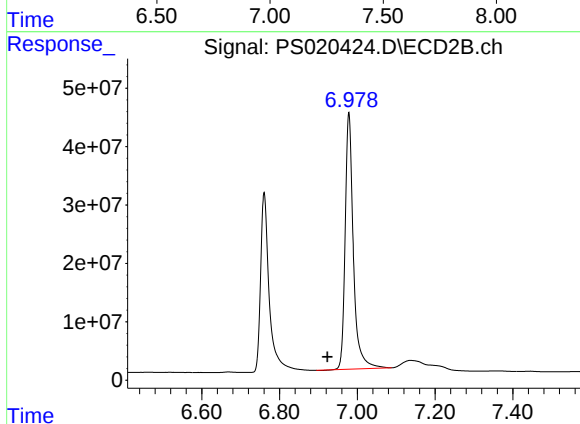

#5 DICAMBA


R.T.: 6.978 min
Delta R.T.: 0.055 min
Response: 644290993
Conc: 180.77 ng/ml

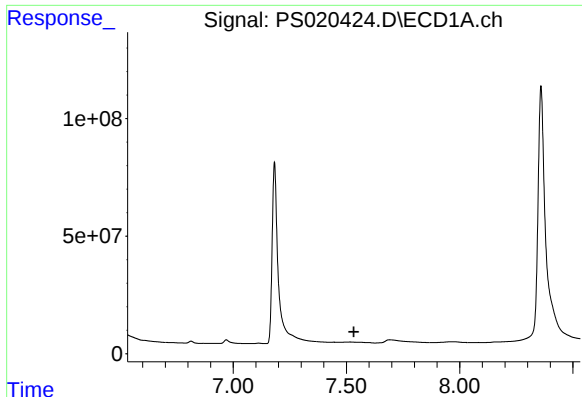

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.533 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

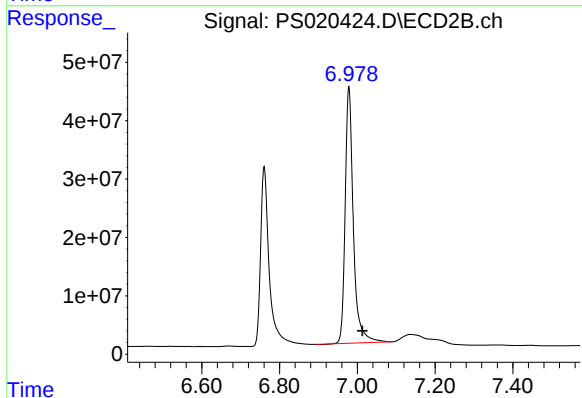


#6 MCPP

R.T.: 6.978 min
Delta R.T.: -0.035 min
Response: 644290993
Conc: 236.19 ug/ml

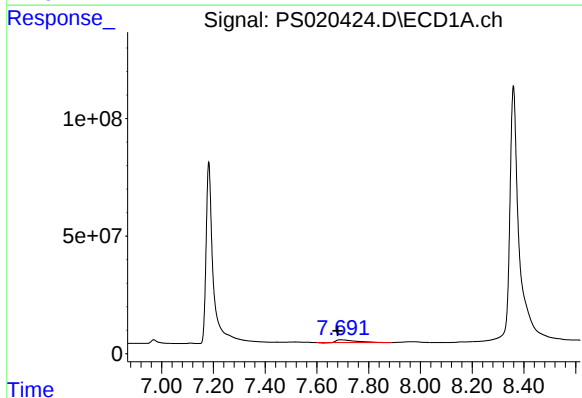


#7 MCPA

R.T.: 7.691 min
Delta R.T.: 0.011 min
Response: 61718714
Conc: 4.79 ug/ml

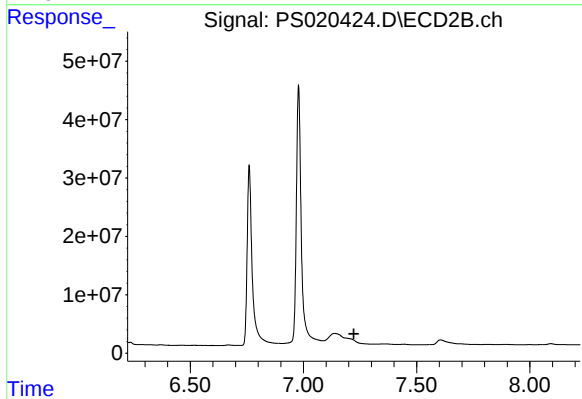

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.223 min
Response: 0
Conc: N.D.

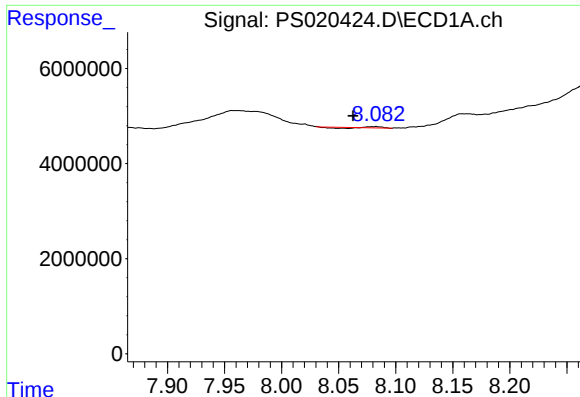

#8 DICHLORPROP


R.T.: 8.081 min
Delta R.T.: 0.019 min
Response: 47569
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

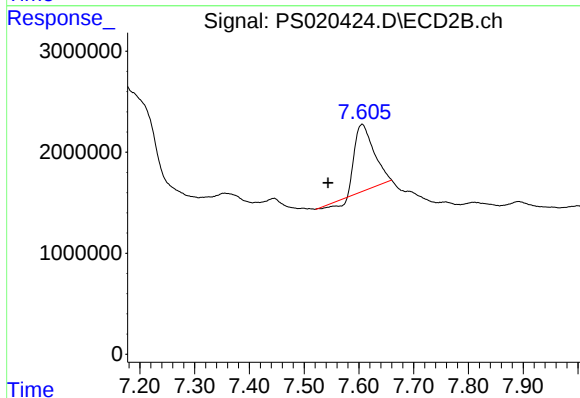


#8 DICHLORPROP

R.T.: 7.606 min
Delta R.T.: 0.062 min
Response: 15274448
Conc: 16.33 ng/ml

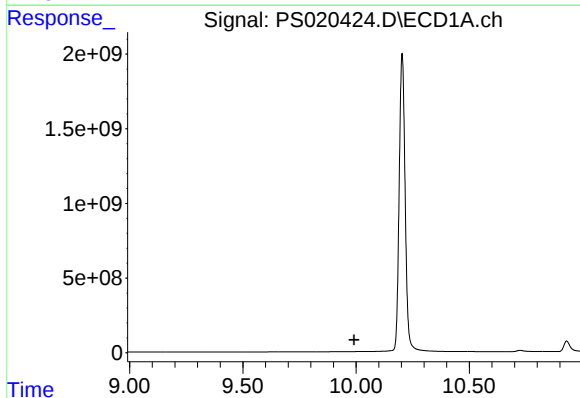


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.991 min
Response: 0
Conc: N.D.

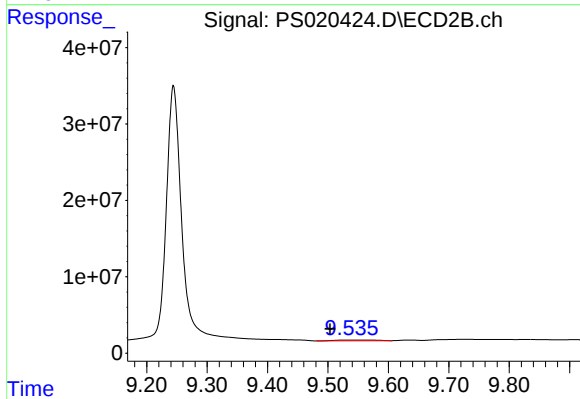

#13 2,4-DB


R.T.: 9.535 min
Delta R.T.: 0.031 min
Response: 4721754
Conc: 6.94 ng/ml

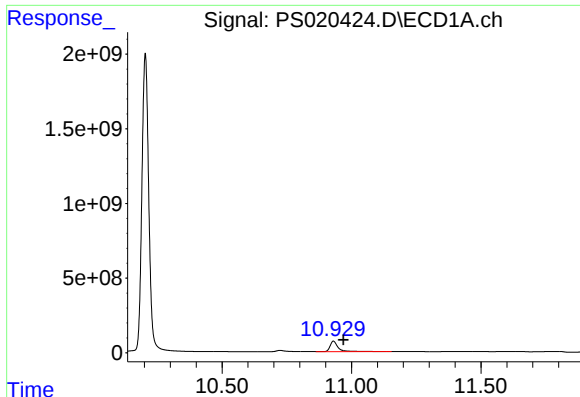

#15 Picloram

R.T.: 10.930 min
Delta R.T.: -0.039 min
Response: 1558049881
Conc: 49.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

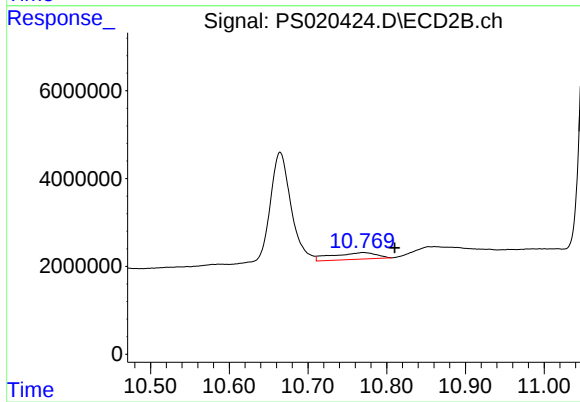

#15 Picloram

R.T.: 10.770 min
Delta R.T.: -0.040 min
Response: 6025127
Conc: N.D.