

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
 Data File : PS012034.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2020 12:23
 Operator : DD\AJ
 Sample : L3506-15
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 15:29:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.220	6.915	216.5E6	134.8E6	198.463	251.983 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.095	0	65184295	N.D.	79.240
3) T	4-Nitroph...	7.057	0.000	4391098	0	7.455	N.D. #
5) T	DICAMBA	0.000	7.048	0	7379179	N.D.	3.415
6) T	MCP	7.629	0.000	5935536	0	1.858	N.D. #
7) T	MCPA	7.696	7.474	102.6E6	46528167	22.565	16.980
8) T	DICHLORPROP	0.000	7.737	0	16792941	N.D.	29.741
9) T	2,4-D	8.400	7.942	111.6E6	9907326	98.850	13.486 #
12) T	2,4,5-T	9.414	0.000	31138048	0	5.255	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
Data File : PS012034.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2020 12:23
Operator : DD\AJ
Sample : L3506-15
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 15:29:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

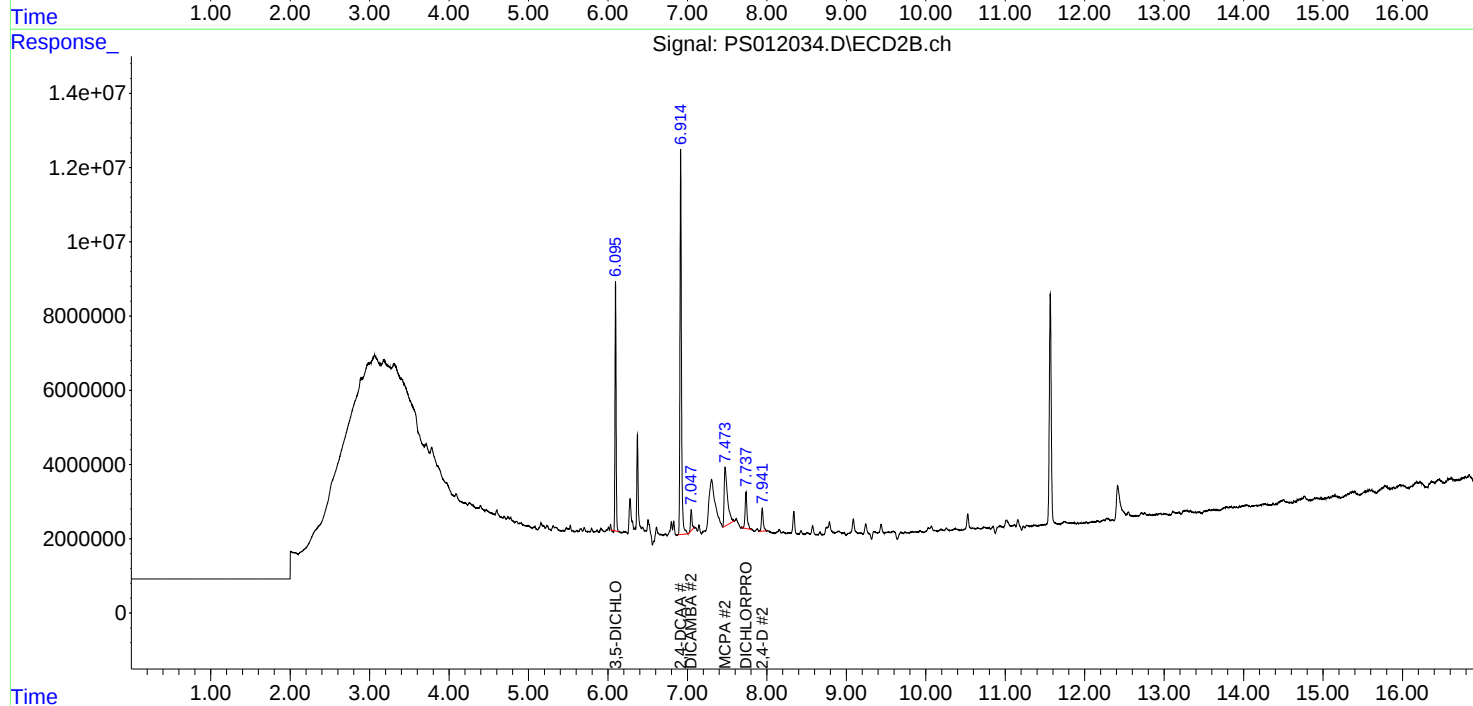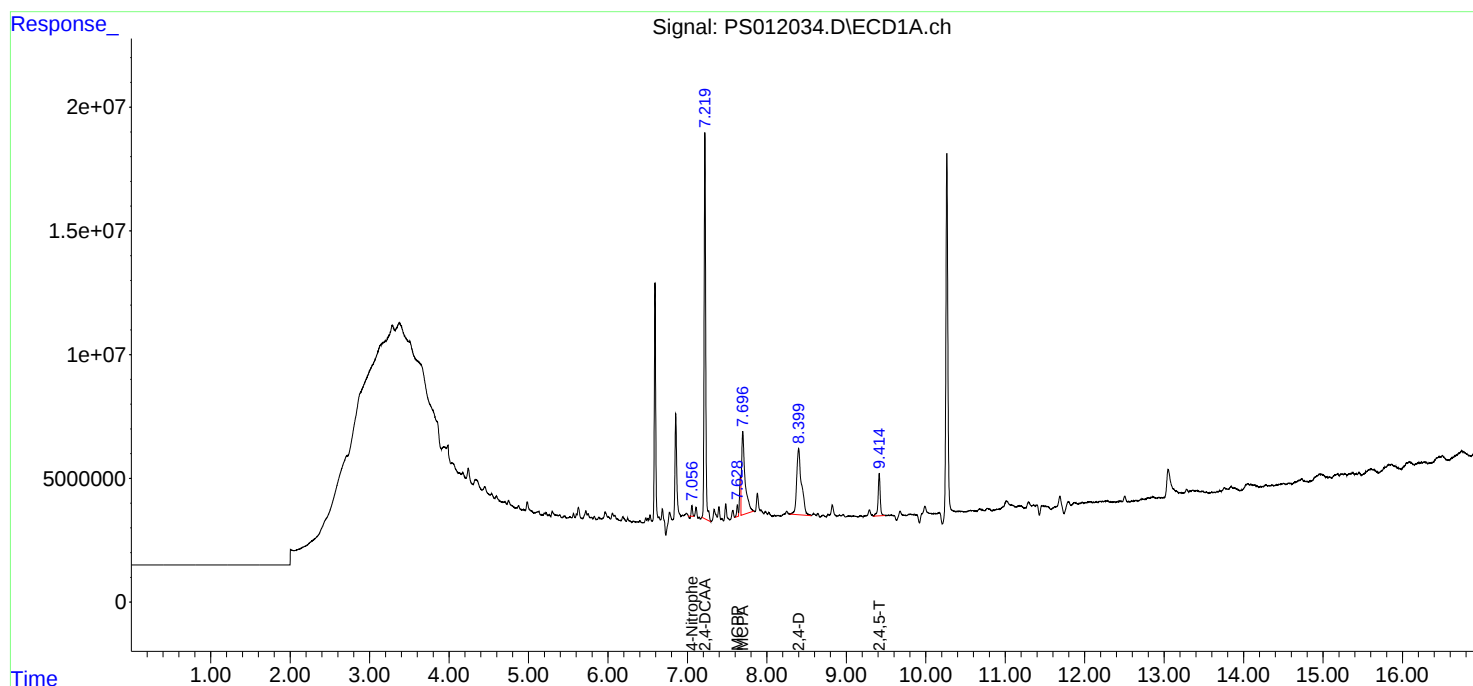


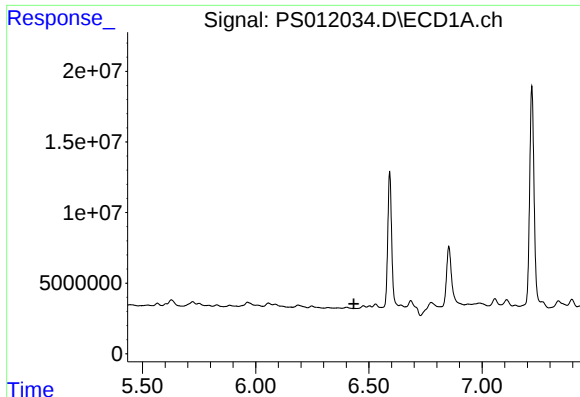

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

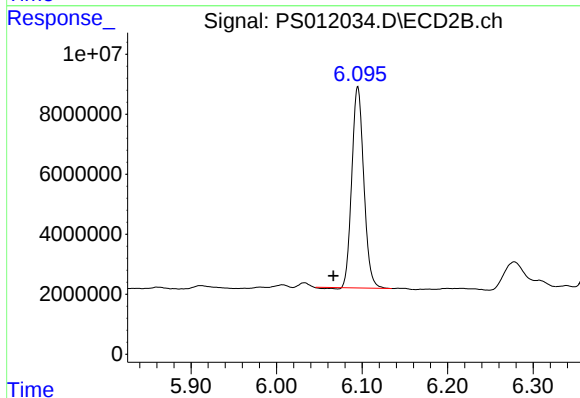


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.028 min
Response: 65184295
Conc: 79.24 ng/ml

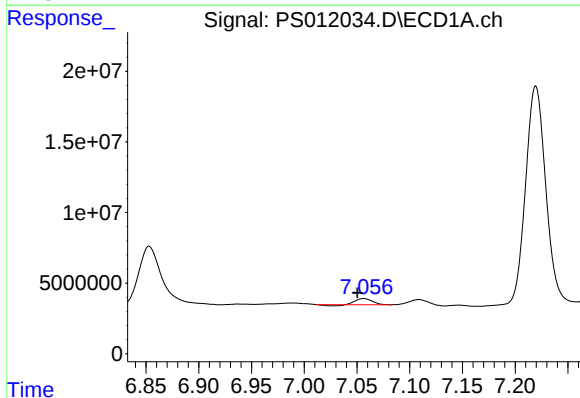


#3 4-Nitrophenol

R.T.: 7.057 min
Delta R.T.: 0.006 min
Response: 4391098
Conc: 7.45 ng/ml

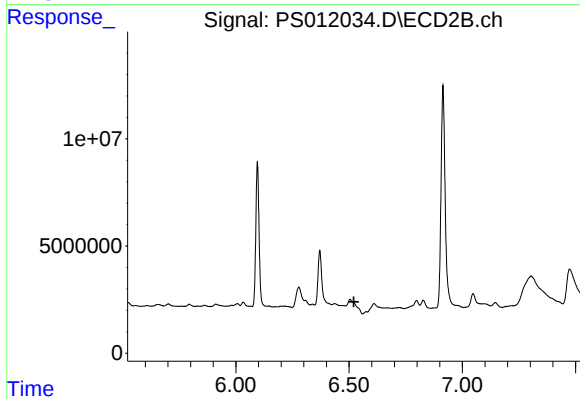

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

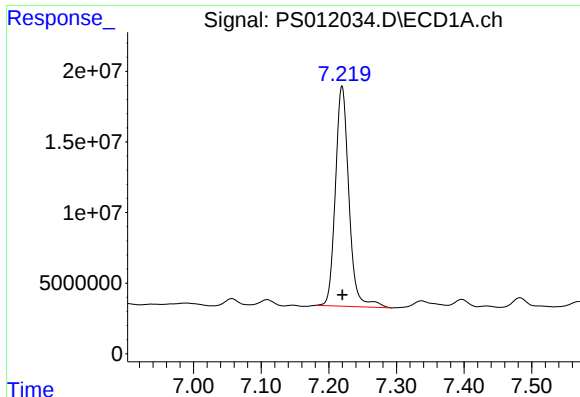

#4 2,4-DCAA


R.T.: 7.220 min
Delta R.T.: 0.000 min
Response: 216477232
Conc: 198.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

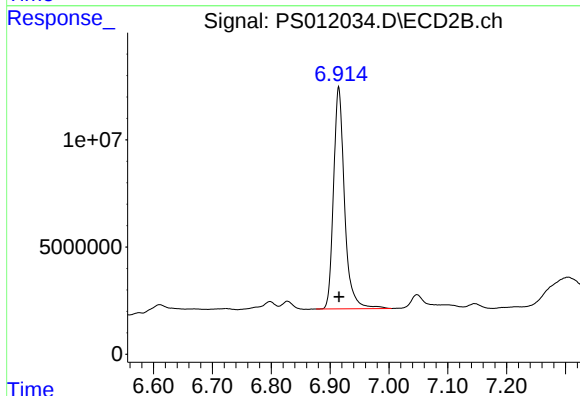


#4 2,4-DCAA

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 134757038
Conc: 251.98 ng/ml

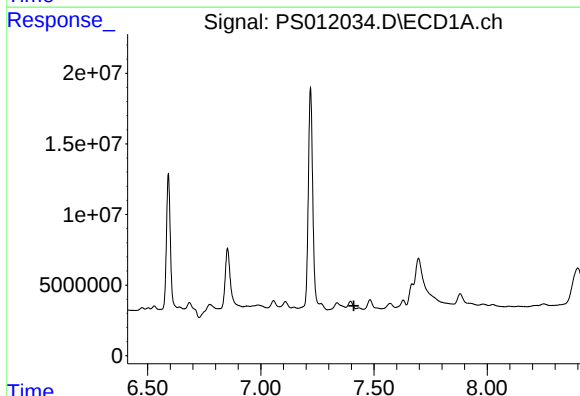


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.412 min
Response: 0
Conc: N.D.

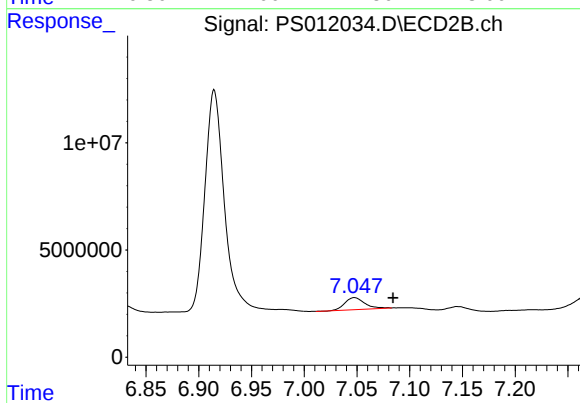

#5 DICAMBA


R.T.: 7.048 min
Delta R.T.: -0.037 min
Response: 7379179
Conc: 3.42 ng/ml

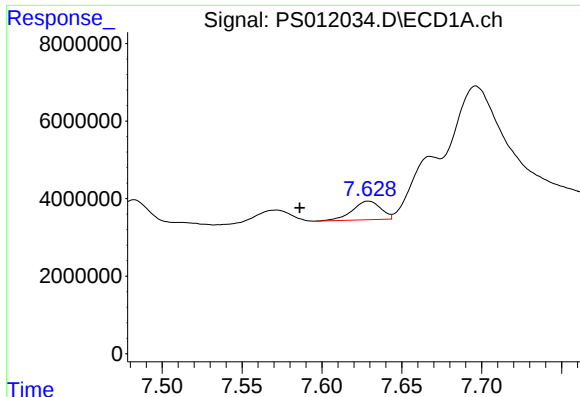

#6 MCPP


R.T.: 7.629 min
Delta R.T.: 0.043 min
Response: 5935536
Conc: 1.86 ug/ml

Instrument :
ECD_S
ClientSampleId :

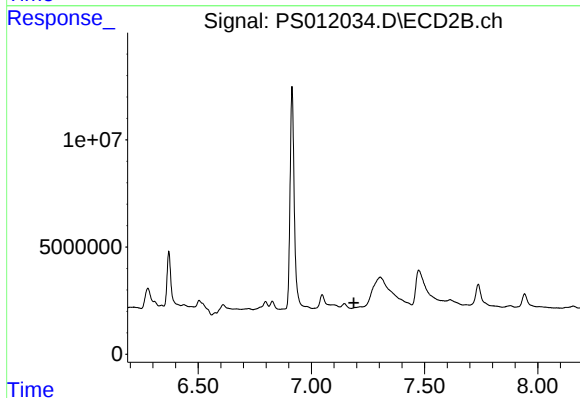


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

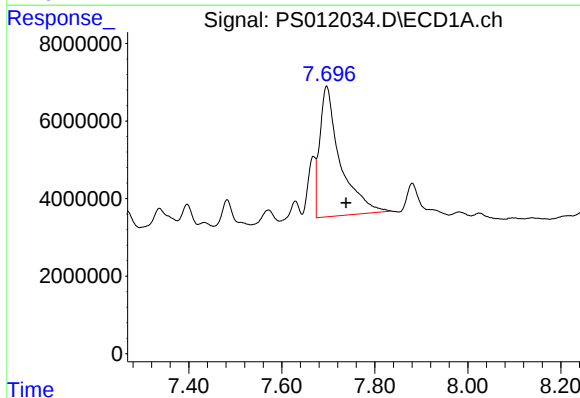


#7 MCPA

R.T.: 7.696 min
Delta R.T.: -0.042 min
Response: 102635486
Conc: 22.56 ug/ml

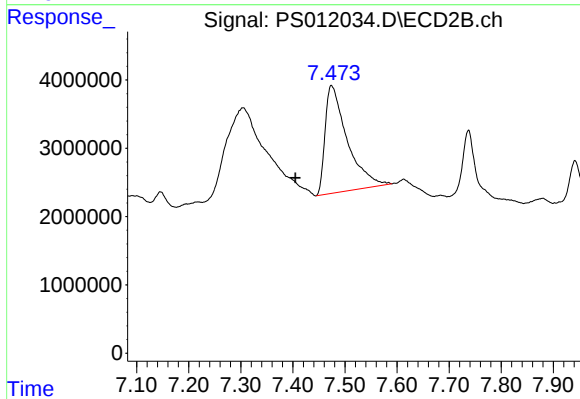

#7 MCPA


R.T.: 7.474 min
Delta R.T.: 0.069 min
Response: 46528167
Conc: 16.98 ug/ml

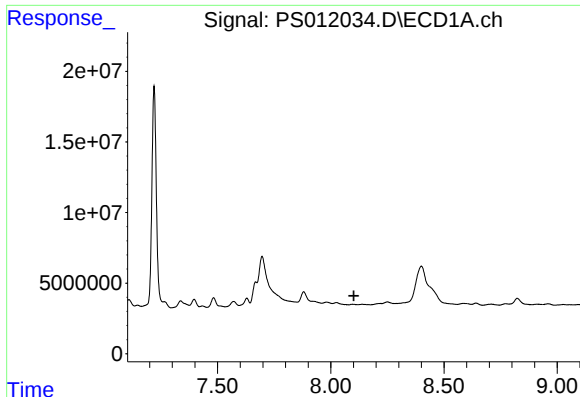

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

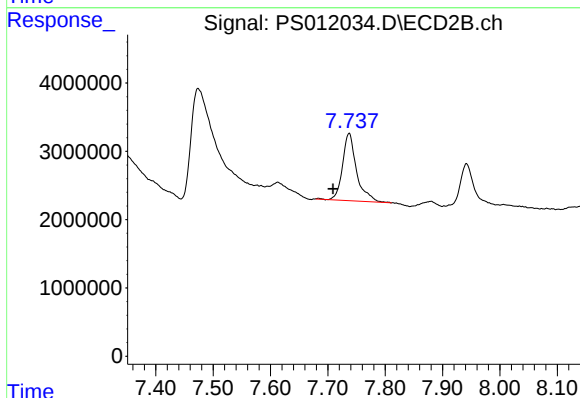


#8 DICHLORPROP

R.T.: 7.737 min
Delta R.T.: 0.028 min
Response: 16792941
Conc: 29.74 ng/ml

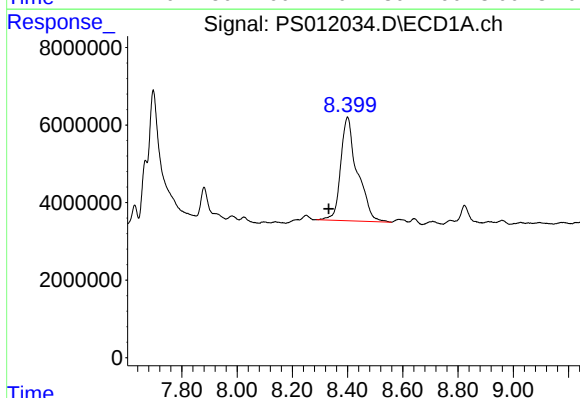


#9 2,4-D

R.T.: 8.400 min
Delta R.T.: 0.068 min
Response: 111611295
Conc: 98.85 ng/ml

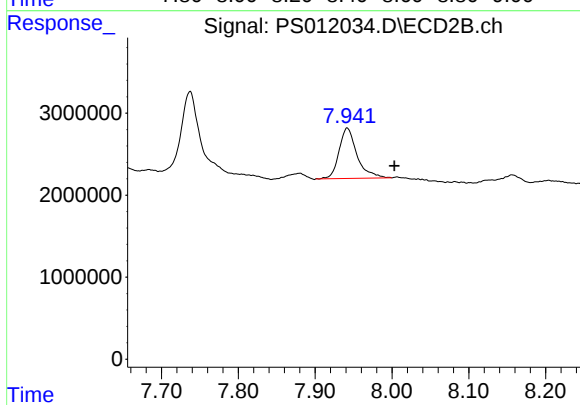

#9 2,4-D


R.T.: 7.942 min
Delta R.T.: -0.062 min
Response: 9907326
Conc: 13.49 ng/ml

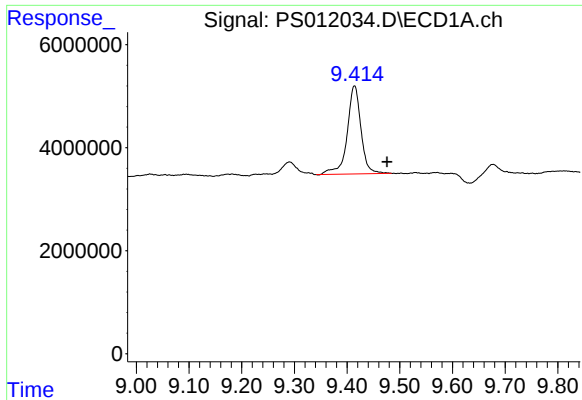

#12 2,4,5-T

R.T.: 9.414 min
Delta R.T.: -0.062 min
Response: 31138048
Conc: 5.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

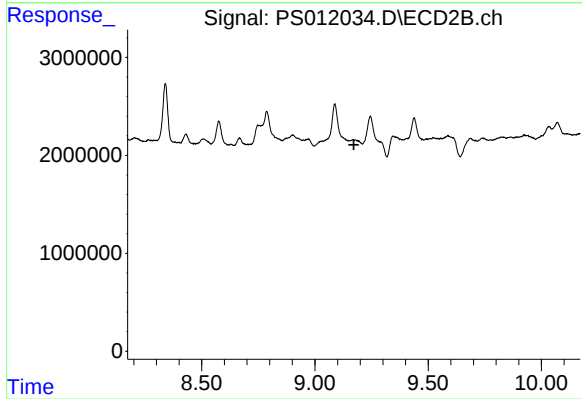

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.