

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
 Data File : PS012035.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2020 12:46
 Operator : DD\AJ
 Sample : L3849-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 15:30:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	265.8E6	164.4E6	243.652	307.335 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.095	0	87305578	N.D.	106.131
3) T	4-Nitroph...	7.056	0.000	4890324	0	8.302	N.D. #
5) T	DICAMBA	7.396	7.047	7803082	11357714	1.905	5.257 #
6) T	MCP	7.629	0.000	7731747	0	2.420	N.D. #
7) T	MCPA	7.693	7.468	155.5E6	89249193	34.192	32.571
8) T	DICHLORPROP	0.000	7.738	0	13209922	N.D.	23.395
9) T	2,4-D	8.398	0.000	96875499	0	85.799	N.D. #
12) T	2,4,5-T	9.412	0.000	24646513	0	4.159	N.D. #
14) T	DINOSEB	11.207	0.000	13174756	0	2.807	N.D. #
16) T	DCPA	11.456	0.000	5789186	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
Data File : PS012035.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2020 12:46
Operator : DD\AJ
Sample : L3849-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 15:30:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

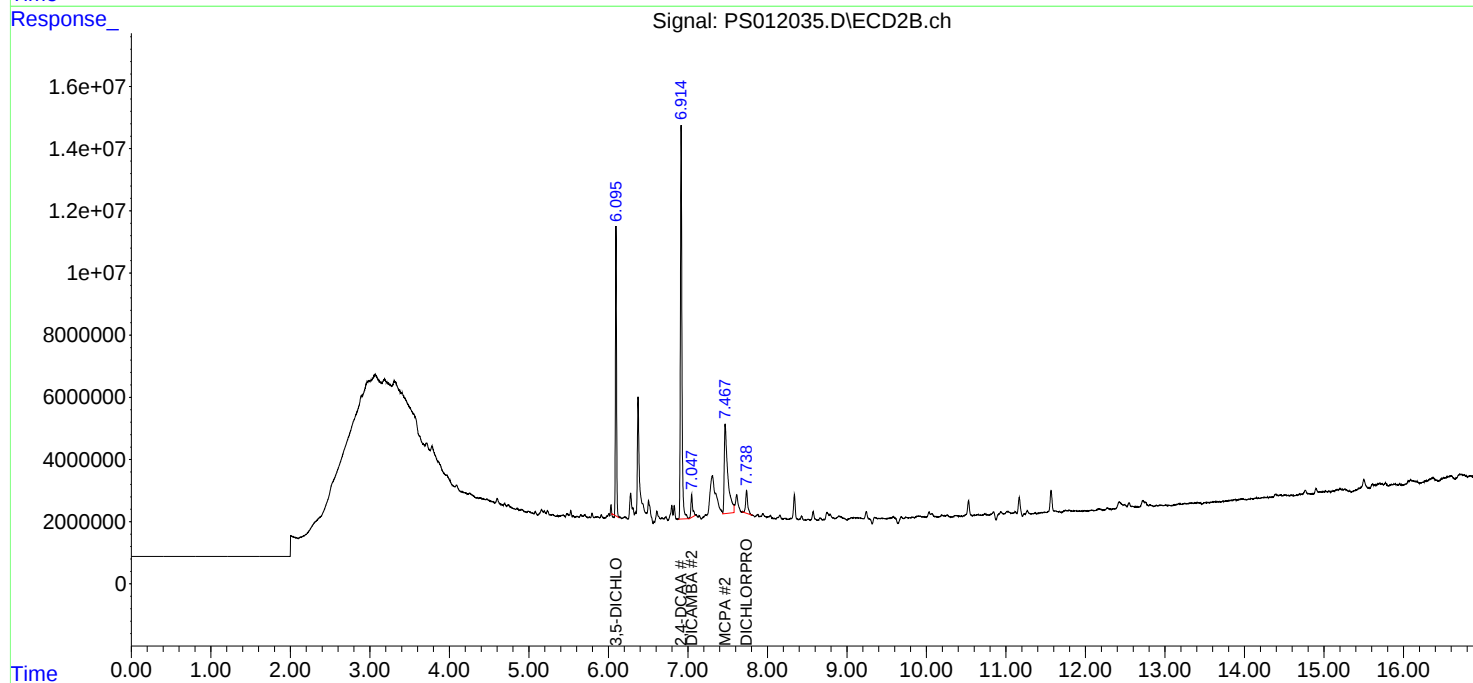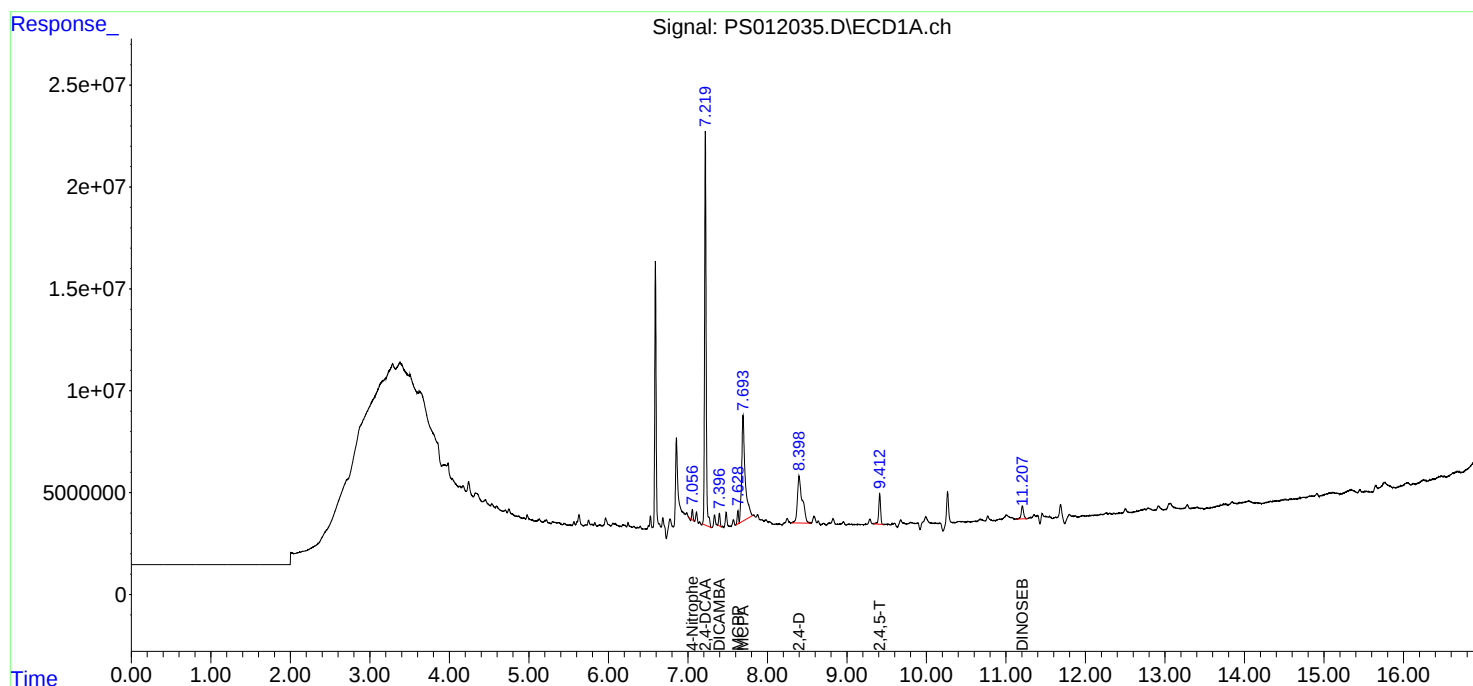


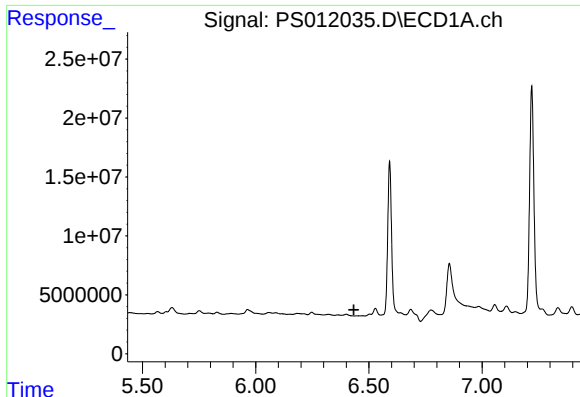

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

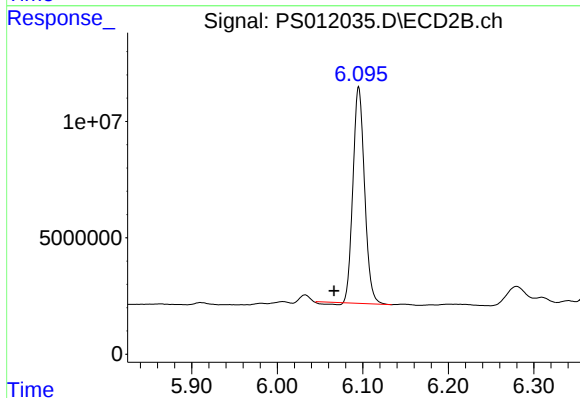


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.029 min
Response: 87305578
Conc: 106.13 ng/ml

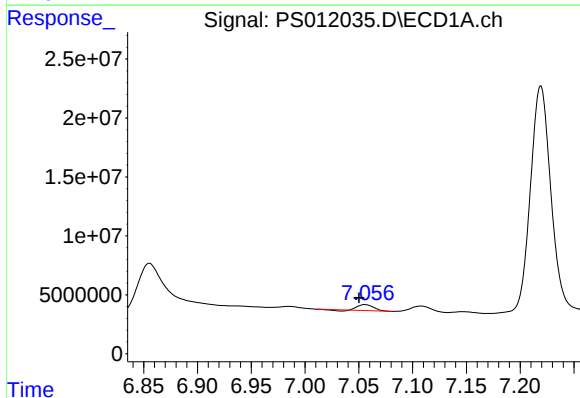


#3 4-Nitrophenol

R.T.: 7.056 min
Delta R.T.: 0.005 min
Response: 4890324
Conc: 8.30 ng/ml

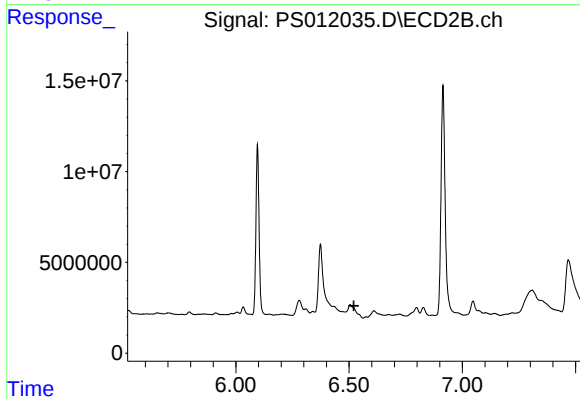

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

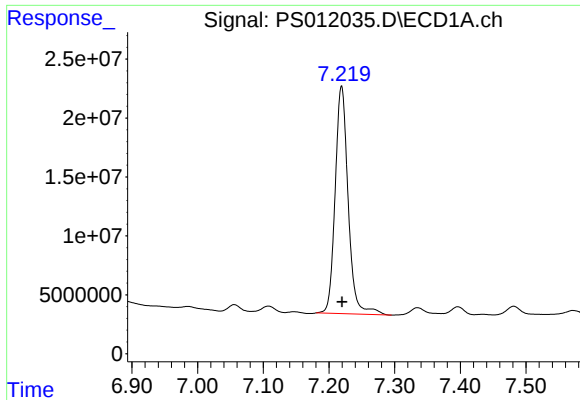

#4 2,4-DCAA


R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 265768351
Conc: 243.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

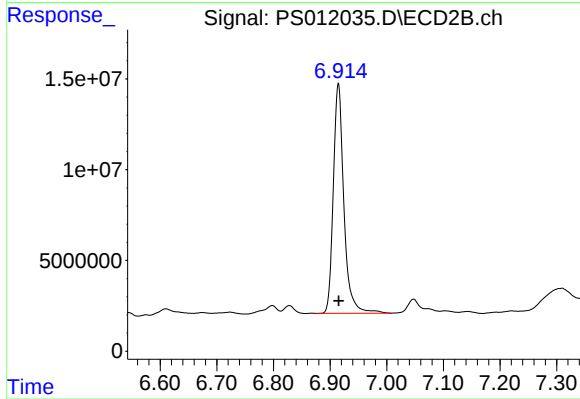


#4 2,4-DCAA

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 164358440
Conc: 307.33 ng/ml

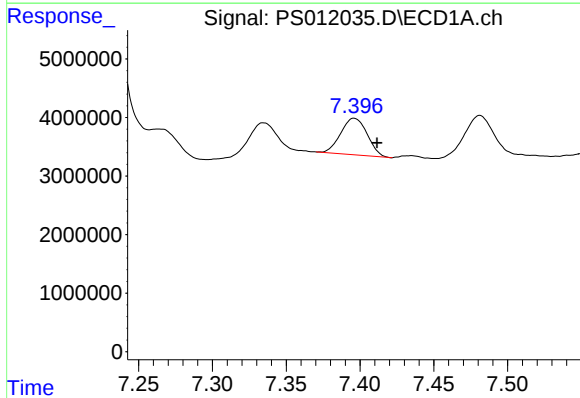


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.016 min
Response: 7803082
Conc: 1.91 ng/ml

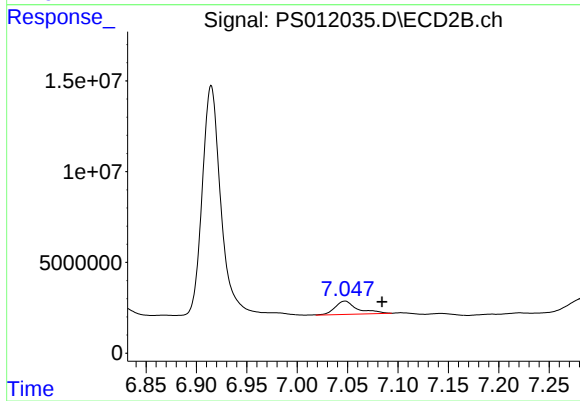

#5 DICAMBA


R.T.: 7.047 min
Delta R.T.: -0.037 min
Response: 11357714
Conc: 5.26 ng/ml

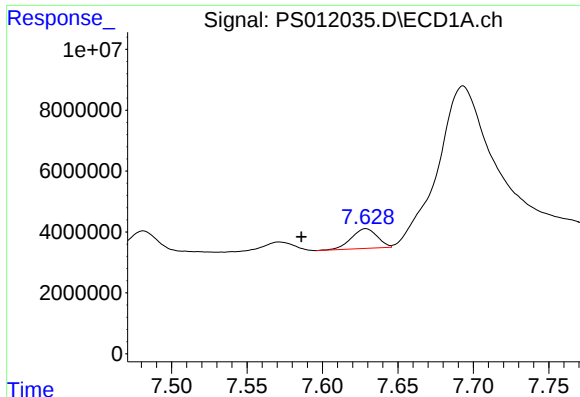

#6 MCPP


R.T.: 7.629 min
Delta R.T.: 0.043 min
Response: 7731747
Conc: 2.42 ug/ml

Instrument :
ECD_S
ClientSampleId :

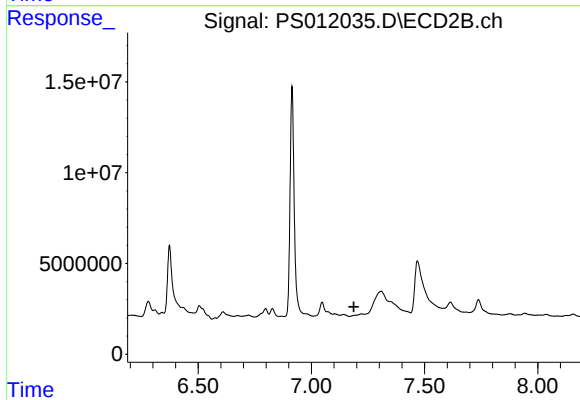


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

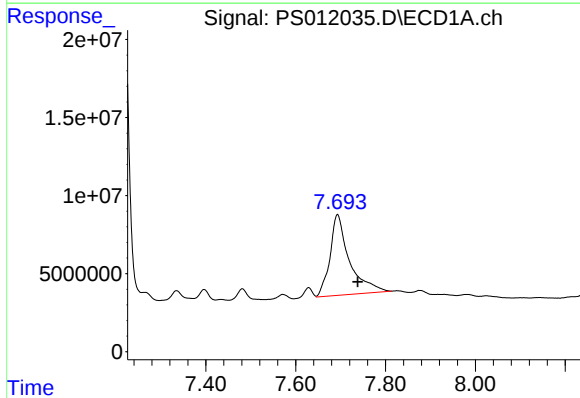


#7 MCPA

R.T.: 7.693 min
Delta R.T.: -0.045 min
Response: 155522844
Conc: 34.19 ug/ml

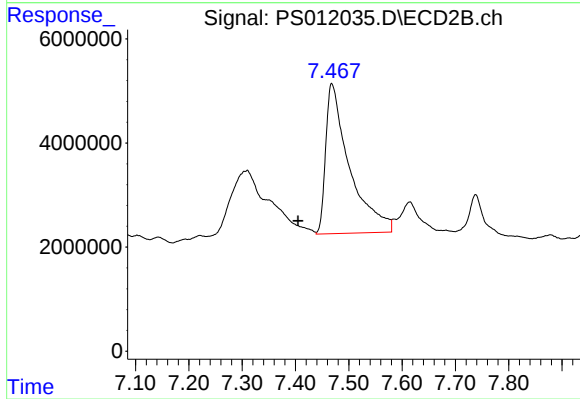

#7 MCPA


R.T.: 7.468 min
Delta R.T.: 0.063 min
Response: 89249193
Conc: 32.57 ug/ml

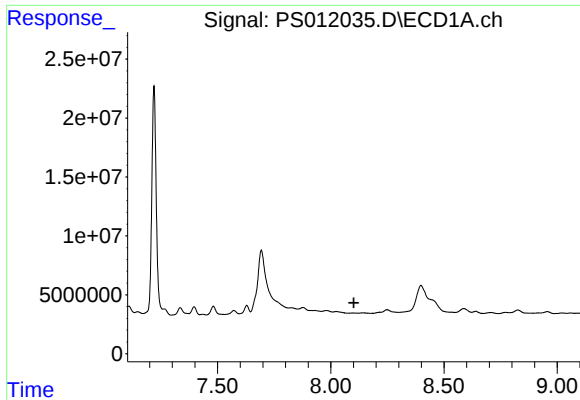

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

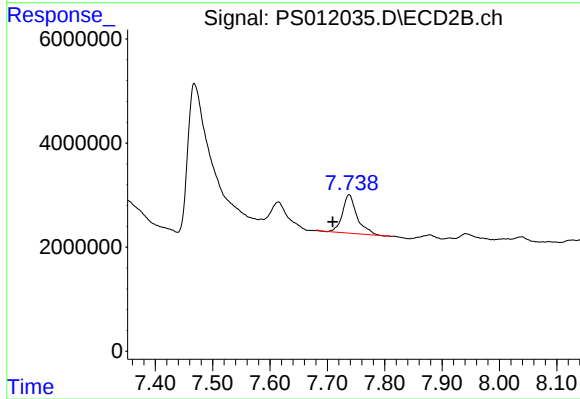


#8 DICHLORPROP

R.T.: 7.738 min
Delta R.T.: 0.029 min
Response: 13209922
Conc: 23.40 ng/ml

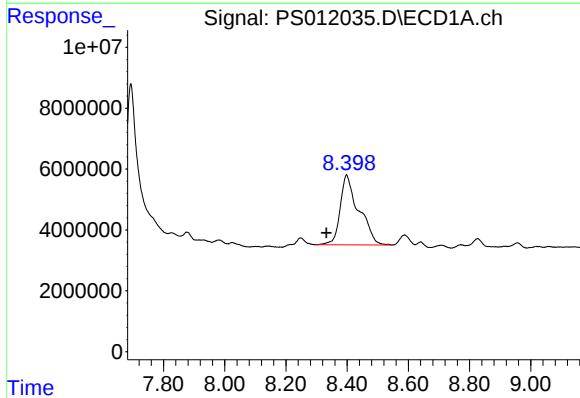


#9 2,4-D

R.T.: 8.398 min
Delta R.T.: 0.066 min
Response: 96875499
Conc: 85.80 ng/ml

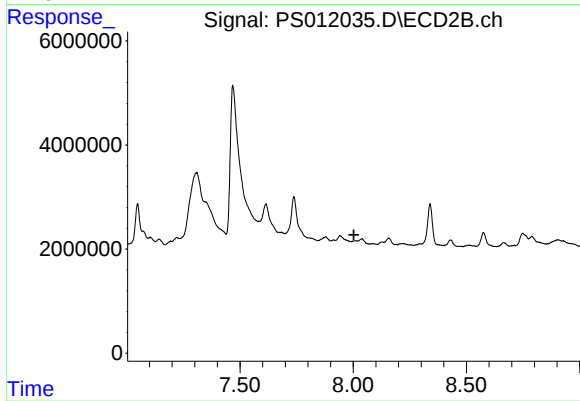

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

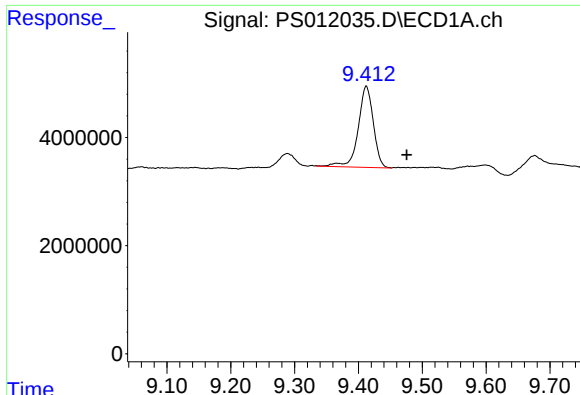

#12 2,4,5-T


R.T.: 9.412 min
Delta R.T.: -0.064 min
Response: 24646513
Conc: 4.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

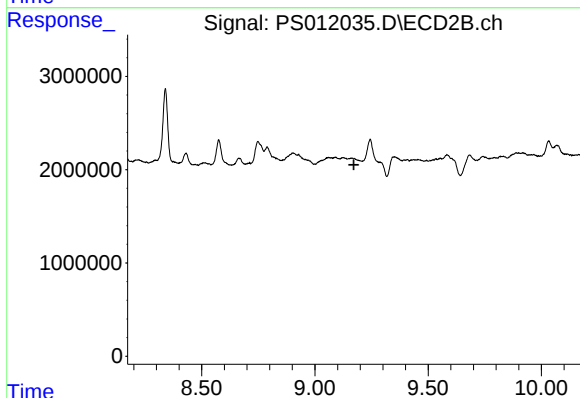


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

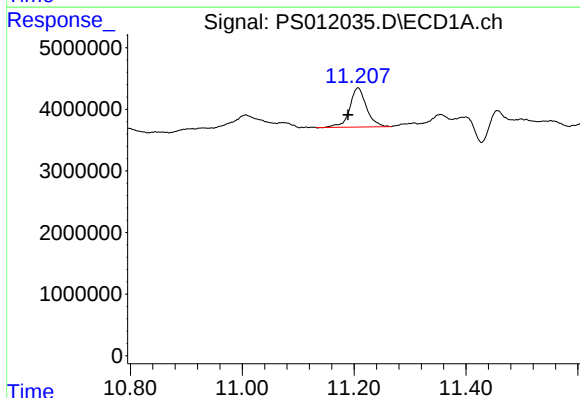

#14 DINOSEB

R.T.: 11.207 min
Delta R.T.: 0.018 min
Response: 13174756
Conc: 2.81 ng/ml

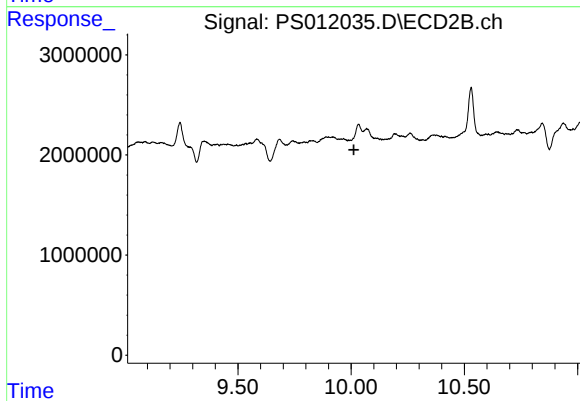

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.012 min
Response: 0
Conc: N.D.