

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
 Data File : PS012038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2020 13:54
 Operator : DD\AJ
 Sample : L3850-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 15:31:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	290.6E6	179.9E6	266.384	336.451 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	88033294	N.D.	107.016
3) T	4-Nitroph...	7.056	0.000	4693814	0	7.969	N.D. #
5) T	DICAMBA	7.396	7.048	8108773	9608069	1.980	4.447 #
6) T	MCP	7.629	0.000	8723480	0	2.730	N.D. #
7) T	MCPA	7.692	7.466	189.7E6	95592592	41.697	34.886
8) T	DICHLORPROP	0.000	7.738	0	9587488	N.D.	16.980
9) T	2,4-D	8.399	8.048	105.4E6	8320334	93.354	11.325 #
12) T	2,4,5-T	9.412	0.000	34382848	0	5.802	N.D. #
14) T	DINOSEB	0.000	10.031	0	7562351	N.D.	3.557
15) T	Picloram	11.001	0.000	33104879	0	4.236	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
Data File : PS012038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2020 13:54
Operator : DD\AJ
Sample : L3850-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 15:31:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

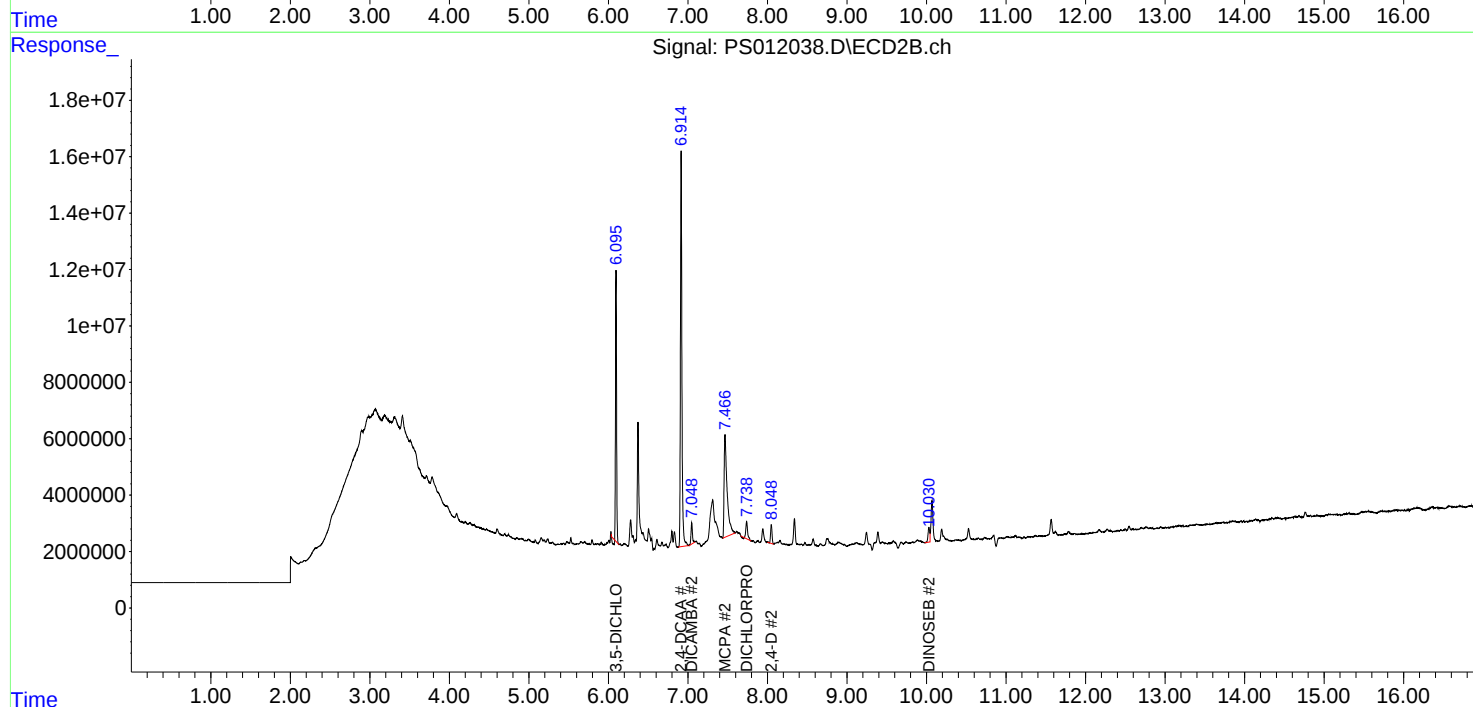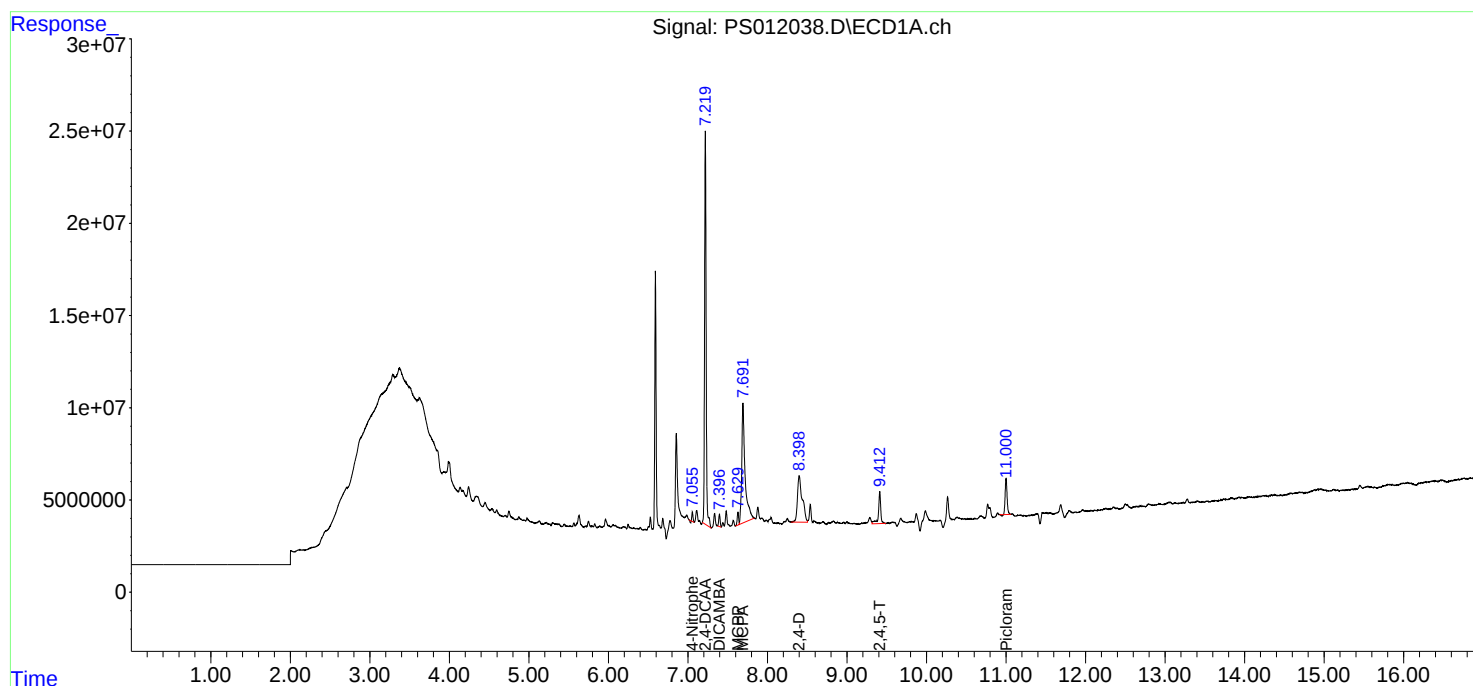


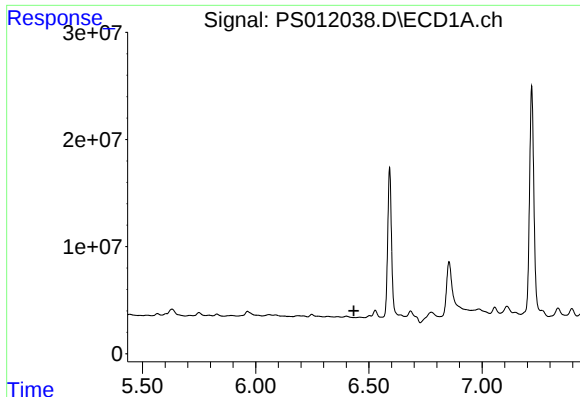

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

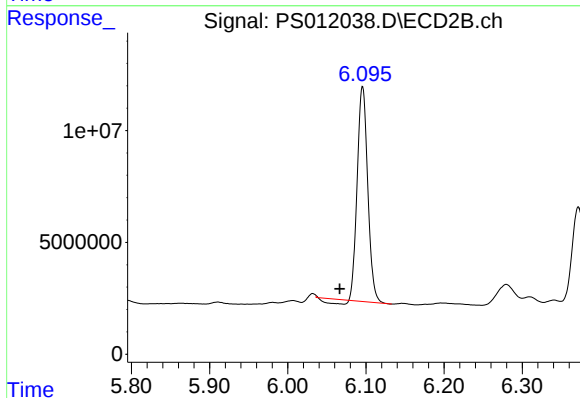


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 88033294
Conc: 107.02 ng/ml

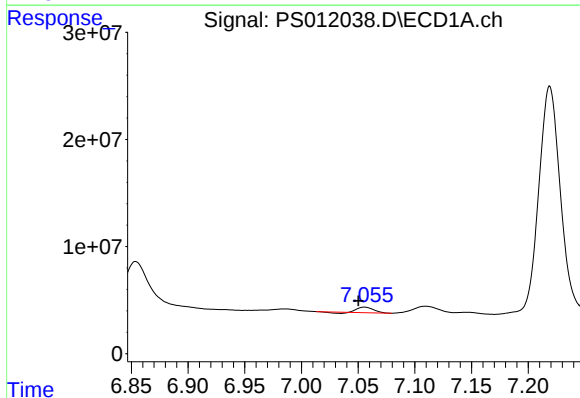


#3 4-Nitrophenol

R.T.: 7.056 min
Delta R.T.: 0.005 min
Response: 4693814
Conc: 7.97 ng/ml

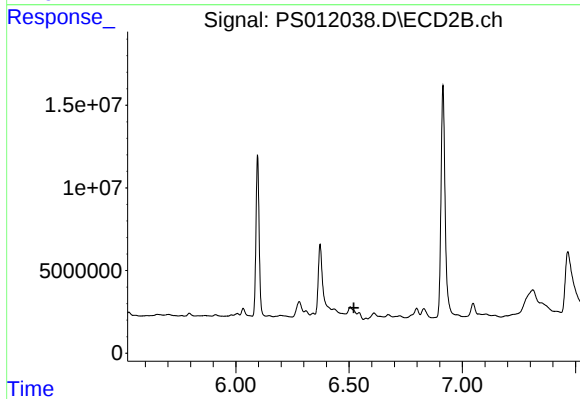

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

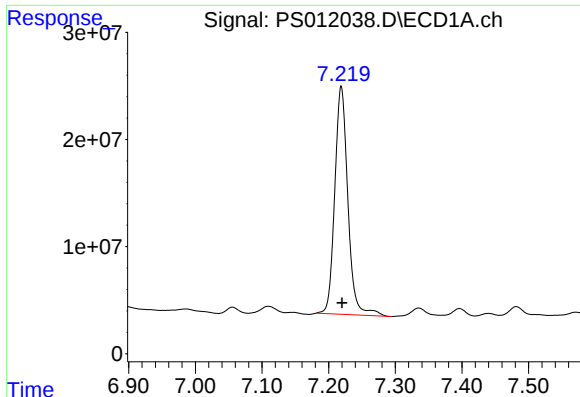

#4 2,4-DCAA


R.T.: 7.219 min
Delta R.T.: -0.001 min
Response: 290563152
Conc: 266.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

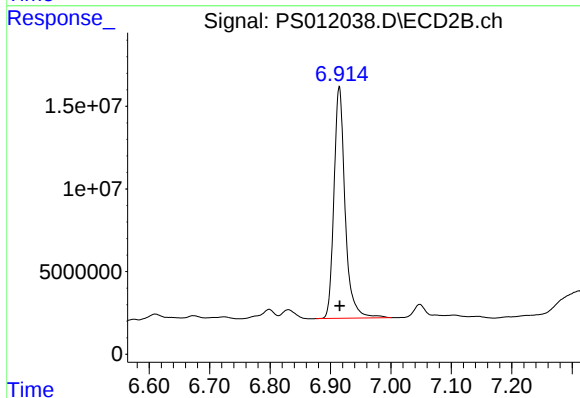


#4 2,4-DCAA

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 179929261
Conc: 336.45 ng/ml

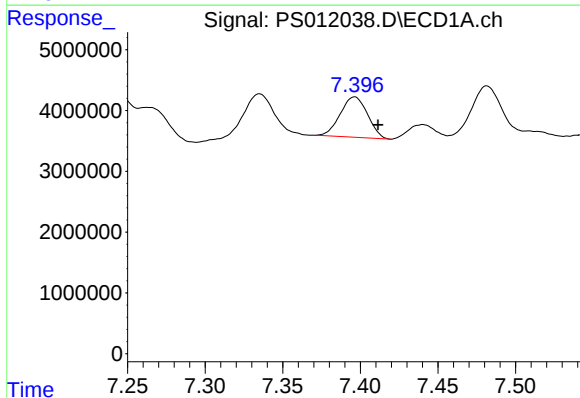


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.015 min
Response: 8108773
Conc: 1.98 ng/ml

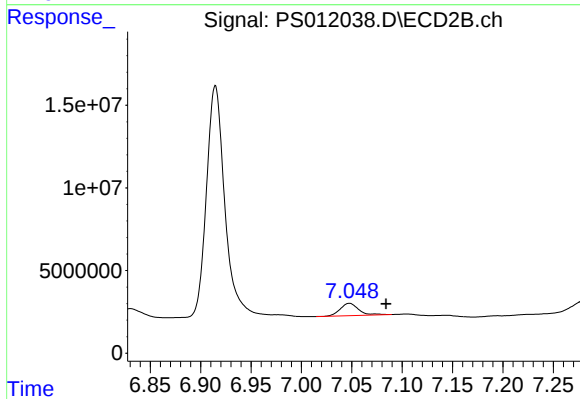

#5 DICAMBA


R.T.: 7.048 min
Delta R.T.: -0.037 min
Response: 9608069
Conc: 4.45 ng/ml

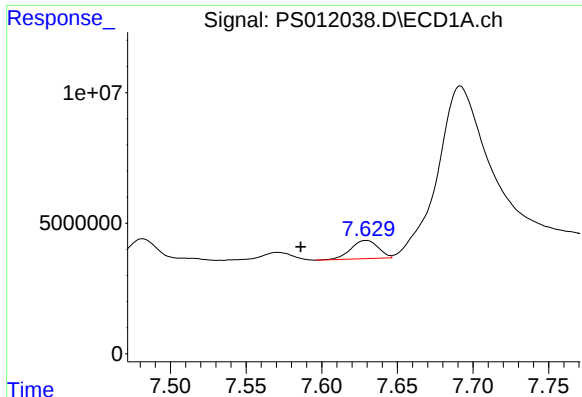

#6 MCPP


R.T.: 7.629 min
Delta R.T.: 0.043 min
Response: 8723480
Conc: 2.73 ug/ml

Instrument :
ECD_S
ClientSampleId :

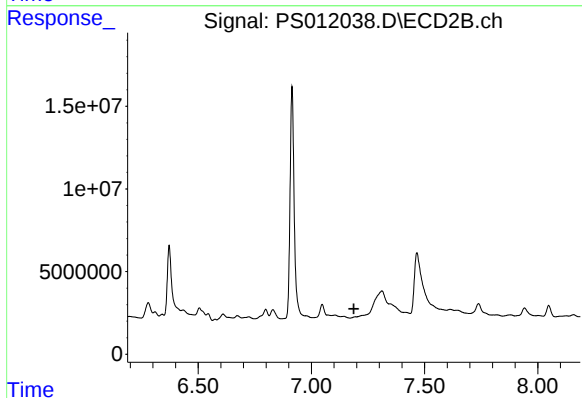


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

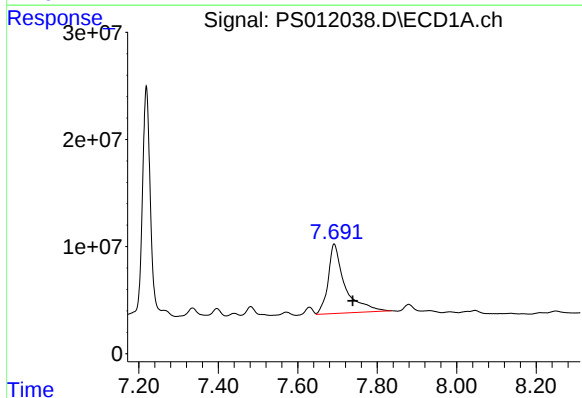


#7 MCPA

R.T.: 7.692 min
Delta R.T.: -0.046 min
Response: 189656057
Conc: 41.70 ug/ml

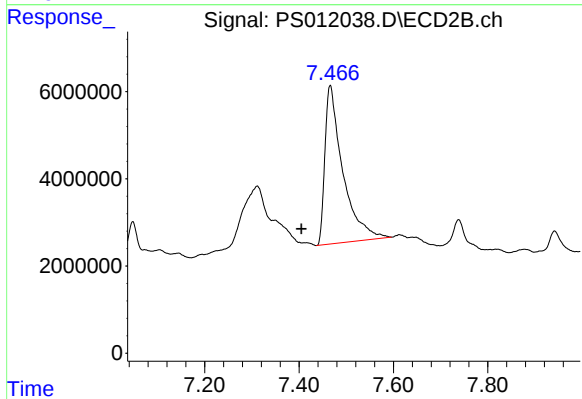

#7 MCPA


R.T.: 7.466 min
Delta R.T.: 0.061 min
Response: 95592592
Conc: 34.89 ug/ml

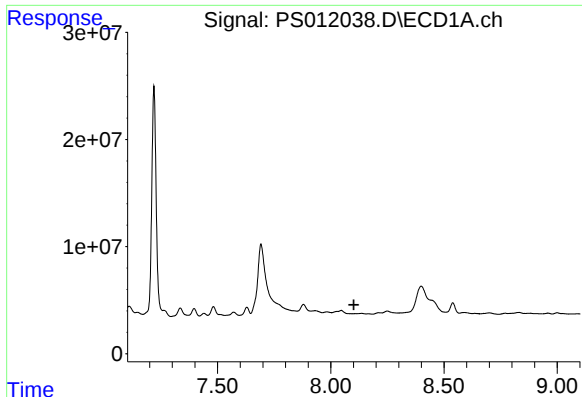

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

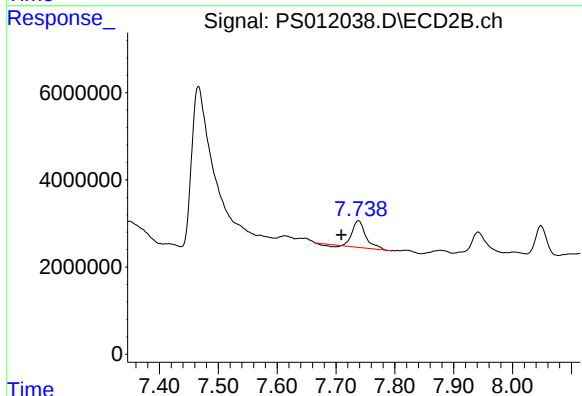


#8 DICHLORPROP

R.T.: 7.738 min
Delta R.T.: 0.029 min
Response: 9587488
Conc: 16.98 ng/ml

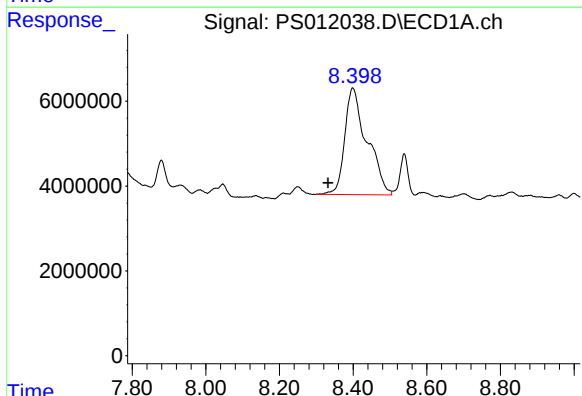


#9 2,4-D

R.T.: 8.399 min
Delta R.T.: 0.067 min
Response: 105405113
Conc: 93.35 ng/ml

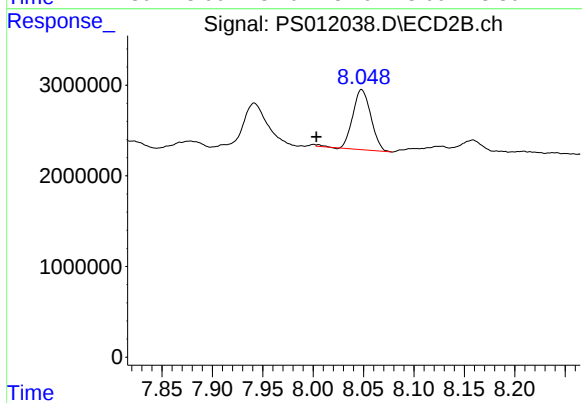

#9 2,4-D


R.T.: 8.048 min
Delta R.T.: 0.045 min
Response: 8320334
Conc: 11.33 ng/ml

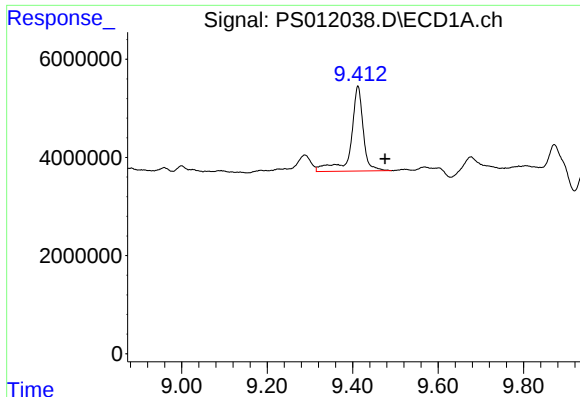

#12 2,4,5-T


R.T.: 9.412 min
Delta R.T.: -0.063 min
Response: 34382848
Conc: 5.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

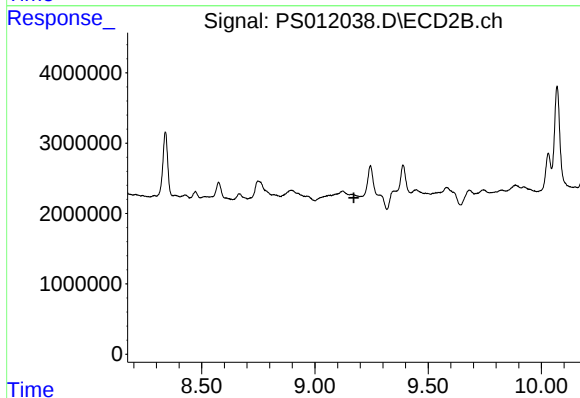


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

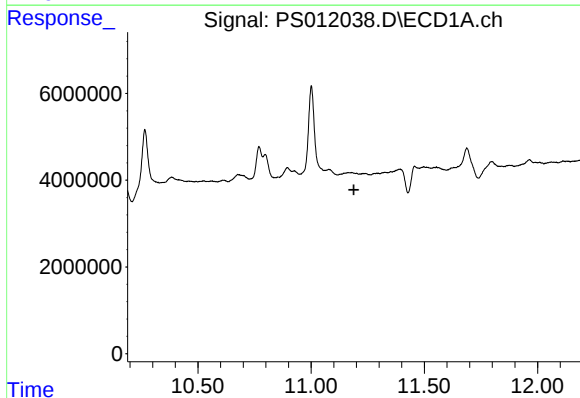


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.189 min
Response: 0
Conc: N.D.

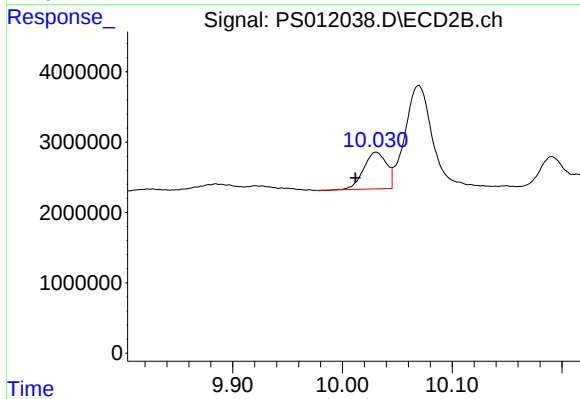

#14 DINOSEB


R.T.: 10.031 min
Delta R.T.: 0.019 min
Response: 7562351
Conc: 3.56 ng/ml

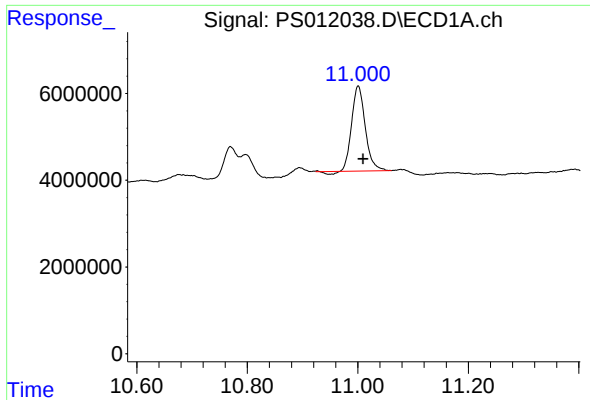

#15 Picloram

R.T.: 11.001 min
Delta R.T.: -0.009 min
Response: 33104879
Conc: 4.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

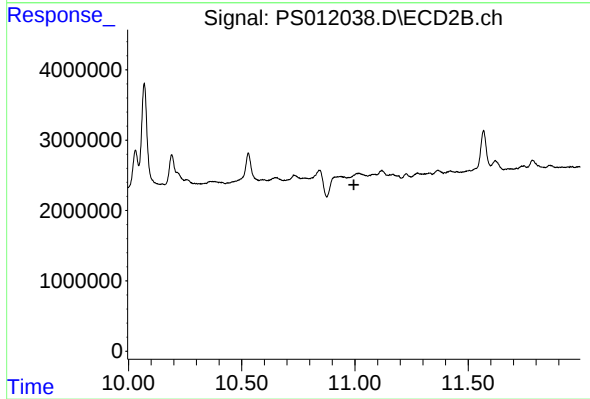

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.