

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
 Data File : PS012039.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2020 14:17
 Operator : DD\AJ
 Sample : L3850-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 15:31:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.218	6.911	306.9E6	236.4E6	281.377	442.083 #
Target Compounds							
2) T	3,5-DICHL...	6.501	6.048	7110726	4557102	4.905	5.540
3) T	4-Nitroph...	7.055	6.488	4205821	11525914	7.140	31.612 #
5) T	DICAMBA	7.397	7.051	10778872	103.6E6	2.632	47.974 #
6) T	MCP	7.571	7.184	10965040	-3837583	3.432	N.D. #
7) T	MCPA	7.788	7.368	405.3E6	29579565	89.099	10.795 #
8) T	DICHLORPROP	0.000	7.734	0	29024258	N.D.	51.403
11) T	2,4,5-TP ...	9.227	8.746	66850150	39700273	11.497	13.579
12) T	2,4,5-T	9.474	0.000	85198090	0	14.377	N.D. #
13) T	2,4-DB	9.965	9.698	7405969	14792476	9.321	35.370 #
15) T	Picloram	11.017	0.000	23914726	0	3.060	N.D. #
16) T	DCPA	11.448	0.000	8812834	0	1.159	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
Data File : PS012039.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2020 14:17
Operator : DD\AJ
Sample : L3850-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 15:31:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

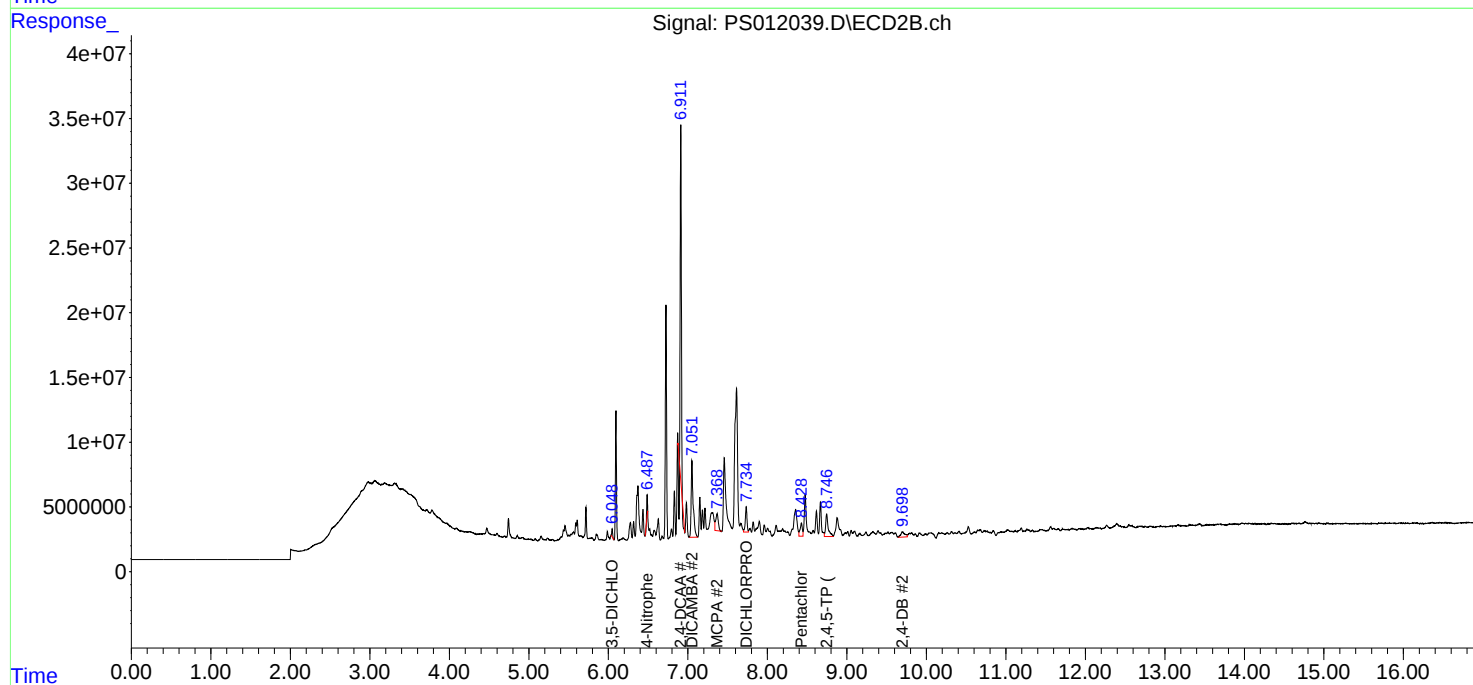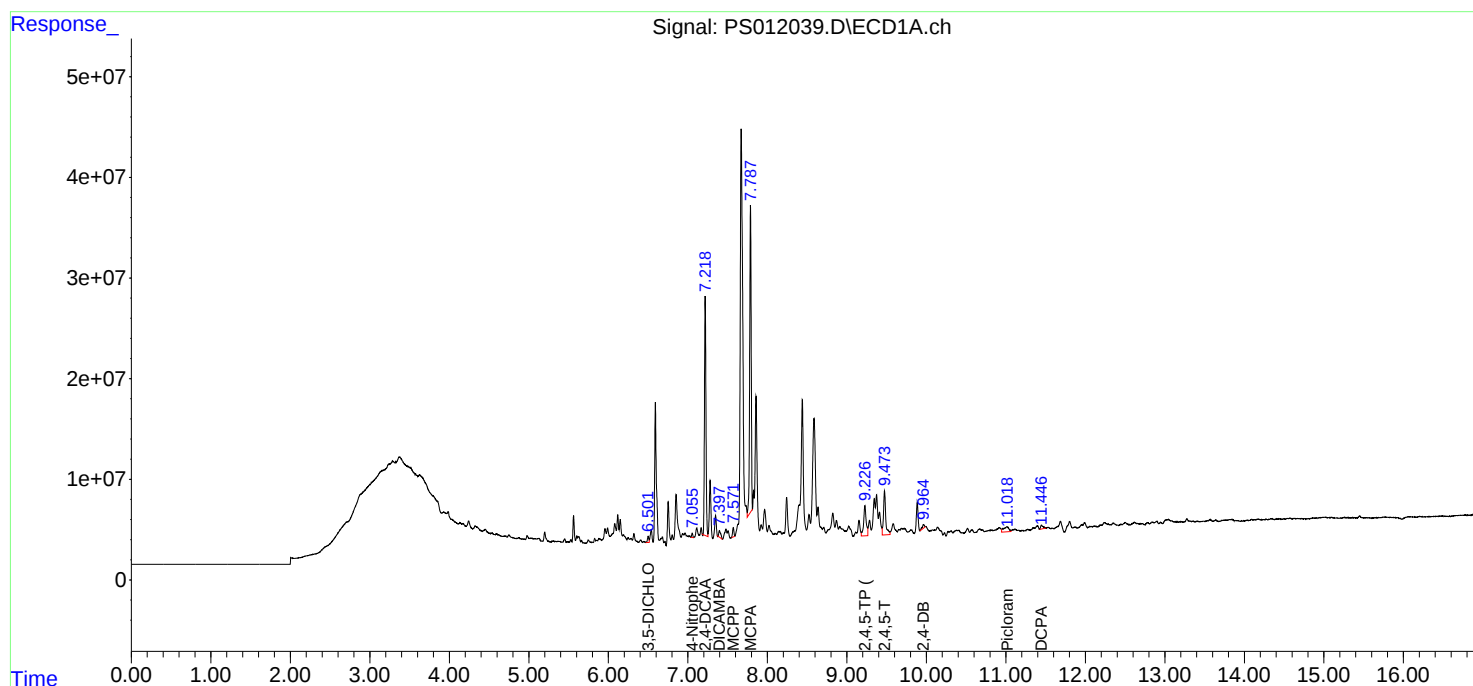


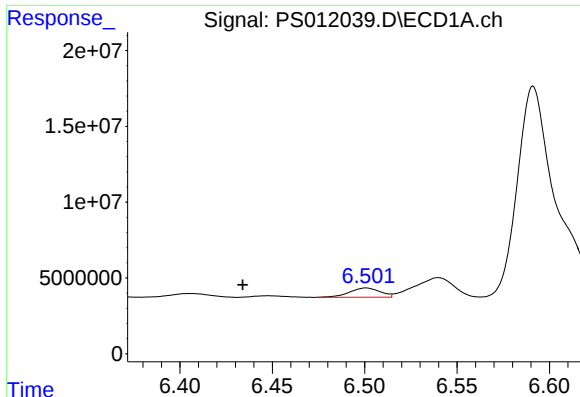

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.501 min
Delta R.T.: 0.067 min
Response: 7110726
Conc: 4.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

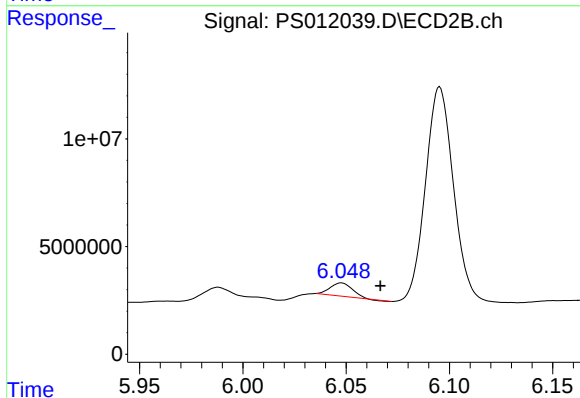


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.048 min
Delta R.T.: -0.019 min
Response: 4557102
Conc: 5.54 ng/ml

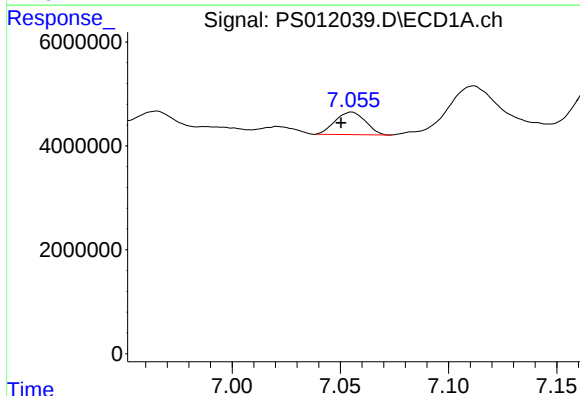


#3 4-Nitrophenol

R.T.: 7.055 min
Delta R.T.: 0.005 min
Response: 4205821
Conc: 7.14 ng/ml

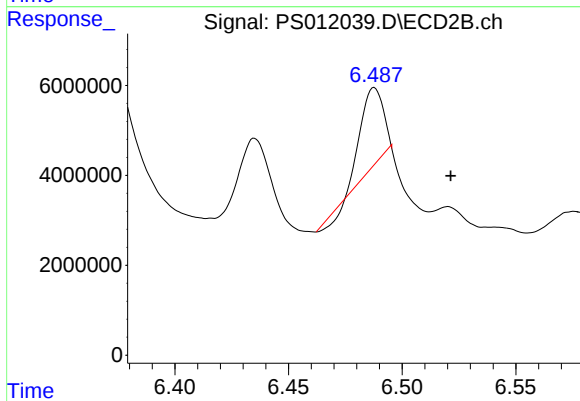

#3 4-Nitrophenol


R.T.: 6.488 min
Delta R.T.: -0.033 min
Response: 11525914
Conc: 31.61 ng/ml

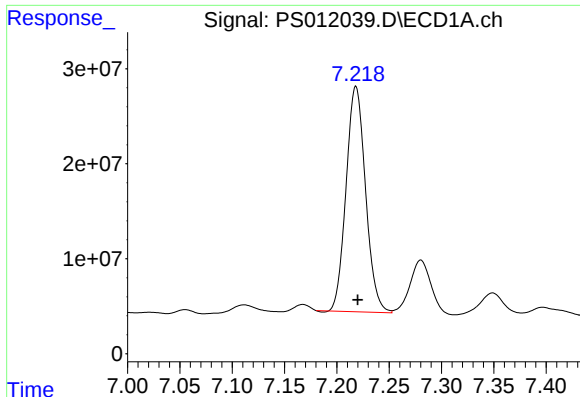

#4 2,4-DCAA


R.T.: 7.218 min
Delta R.T.: -0.002 min
Response: 306917135
Conc: 281.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

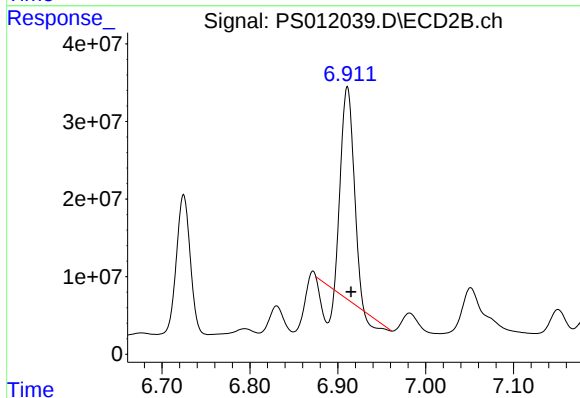


#4 2,4-DCAA

R.T.: 6.911 min
Delta R.T.: -0.004 min
Response: 236420273
Conc: 442.08 ng/ml

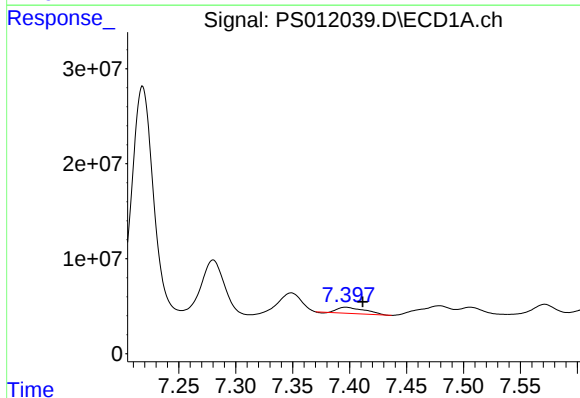


#5 DICAMBA

R.T.: 7.397 min
Delta R.T.: -0.015 min
Response: 10778872
Conc: 2.63 ng/ml

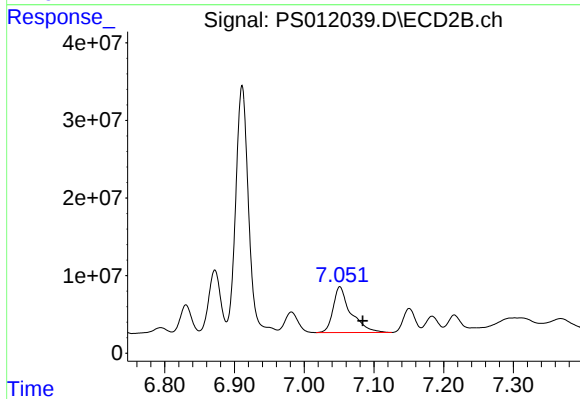

#5 DICAMBA


R.T.: 7.051 min
Delta R.T.: -0.033 min
Response: 103647968
Conc: 47.97 ng/ml

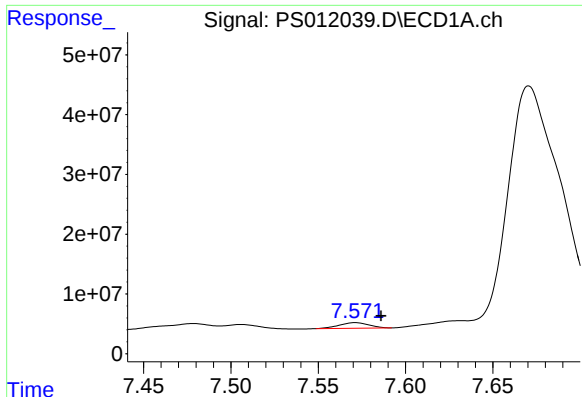

#6 MCPP


R.T.: 7.571 min
Delta R.T.: -0.015 min
Response: 10965040
Conc: 3.43 ug/ml

Instrument :
ECD_S
ClientSampleId :

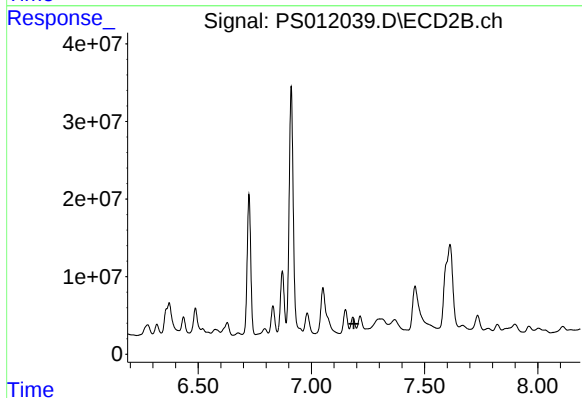


#6 MCPP

R.T.: 7.184 min
Delta R.T.: -0.004 min
Response: -3837583
Conc: N.D.

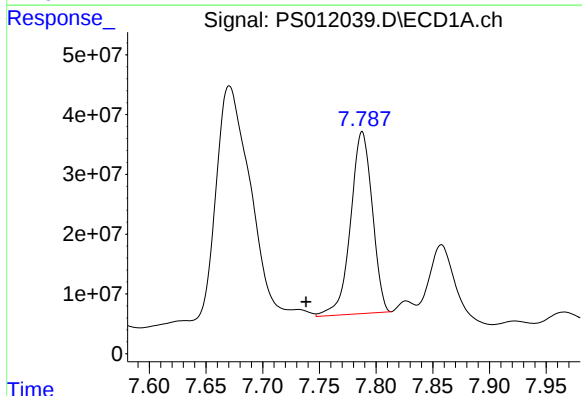


#7 MCPA

R.T.: 7.788 min
Delta R.T.: 0.050 min
Response: 405263405
Conc: 89.10 ug/ml

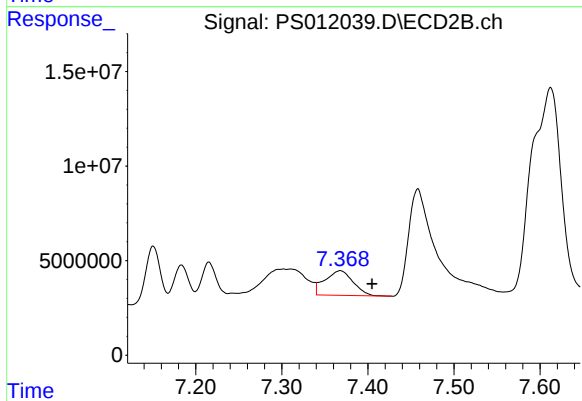

#7 MCPA


R.T.: 7.368 min
Delta R.T.: -0.037 min
Response: 29579565
Conc: 10.79 ug/ml

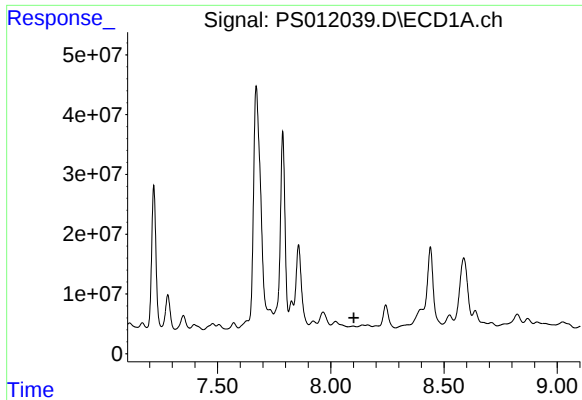

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

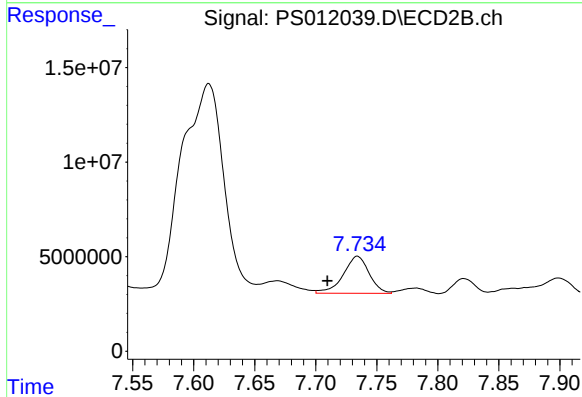


#8 DICHLORPROP

R.T.: 7.734 min
Delta R.T.: 0.025 min
Response: 29024258
Conc: 51.40 ng/ml

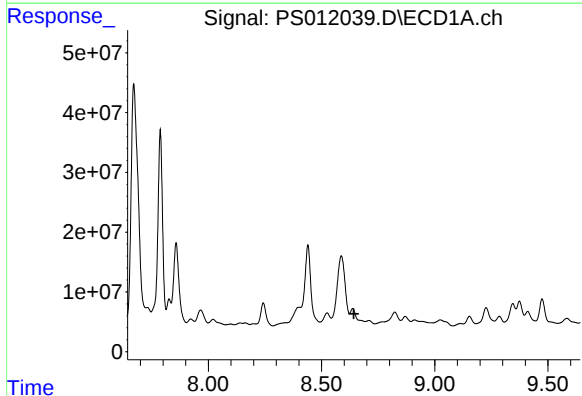


#10 Pentachlorophenol

R.T.: 8.637 min
Delta R.T.: -0.005 min
Response: -135613962
Conc: N.D.

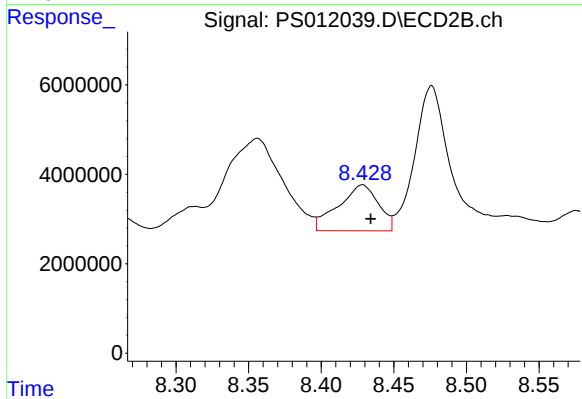

#10 Pentachlorophenol


R.T.: 8.428 min
Delta R.T.: -0.006 min
Response: 19723310
Conc: 2.90 ng/ml

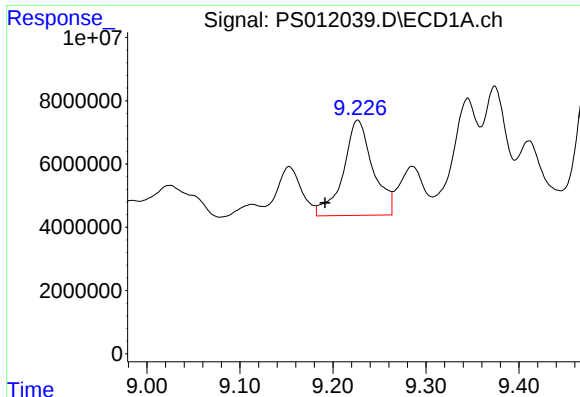

#11 2,4,5-TP (SILVEX)


R.T.: 9.227 min
Delta R.T.: 0.035 min
Response: 66850150
Conc: 11.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

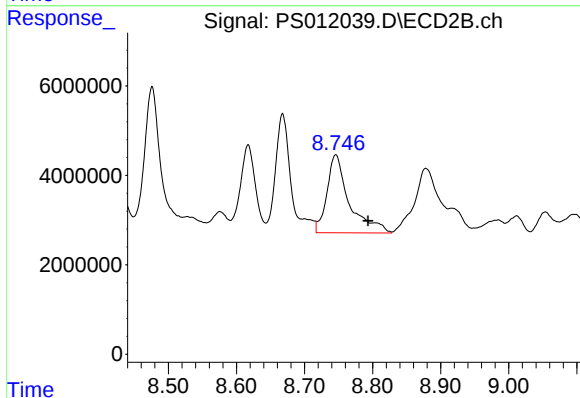


#11 2,4,5-TP (SILVEX)

R.T.: 8.746 min
Delta R.T.: -0.048 min
Response: 39700273
Conc: 13.58 ng/ml

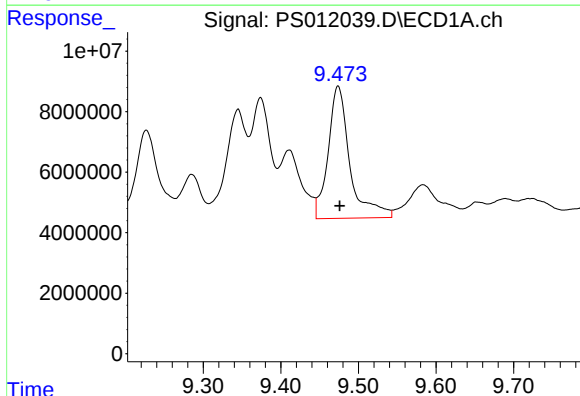


#12 2,4,5-T

R.T.: 9.474 min
Delta R.T.: -0.002 min
Response: 85198090
Conc: 14.38 ng/ml

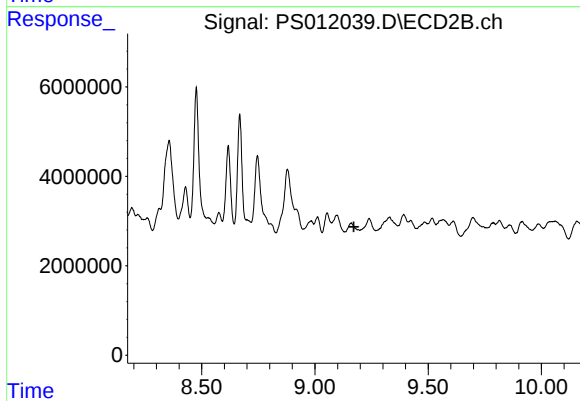

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.

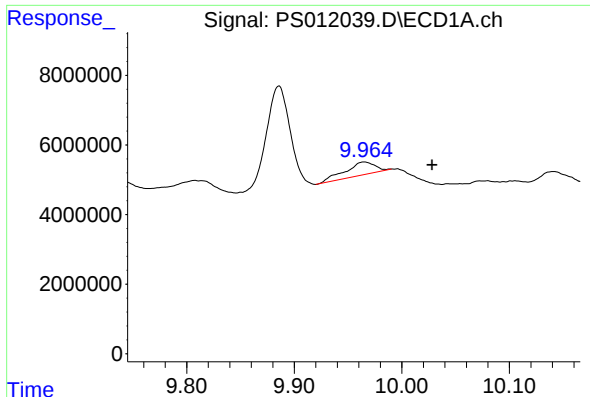

#13 2,4-DB


R.T.: 9.965 min
Delta R.T.: -0.063 min
Response: 7405969
Conc: 9.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

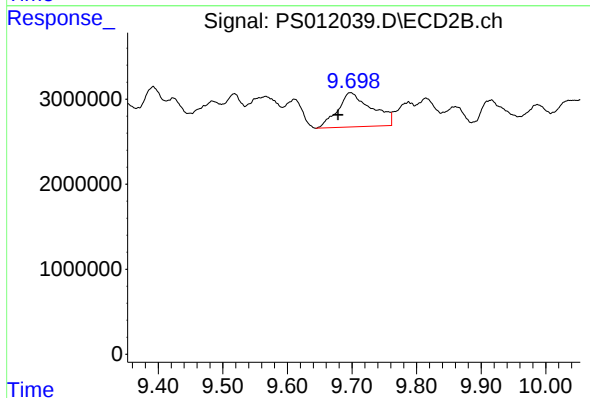


#13 2,4-DB

R.T.: 9.698 min
Delta R.T.: 0.019 min
Response: 14792476
Conc: 35.37 ng/ml

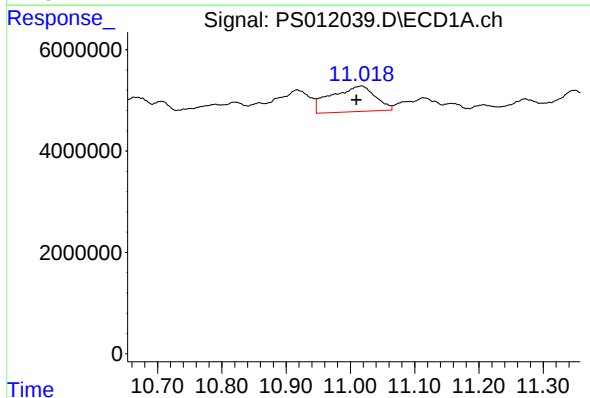


#15 Picloram

R.T.: 11.017 min
Delta R.T.: 0.007 min
Response: 23914726
Conc: 3.06 ng/ml

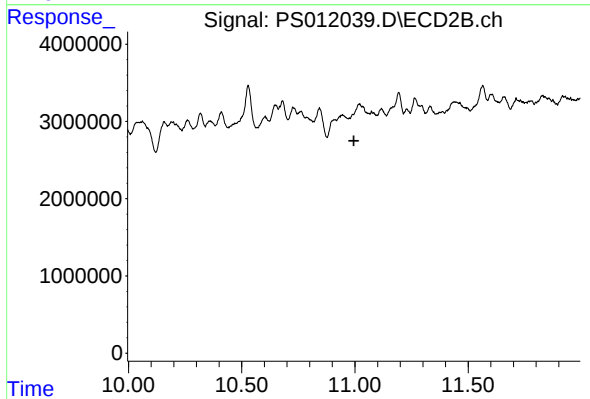

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 10.995 min
Response: 0
Conc: N.D.

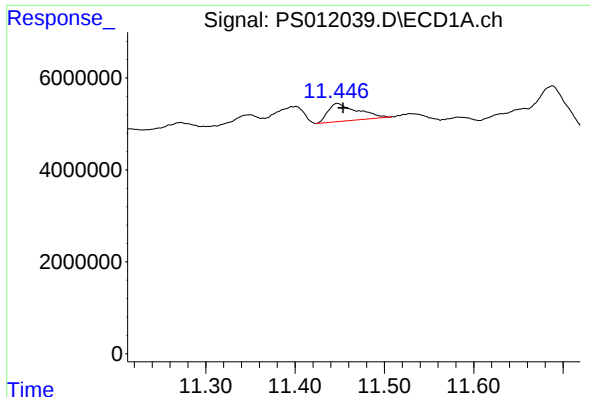

#16 DCPA

R.T.: 11.448 min
Delta R.T.: -0.006 min
Response: 8812834
Conc: 1.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

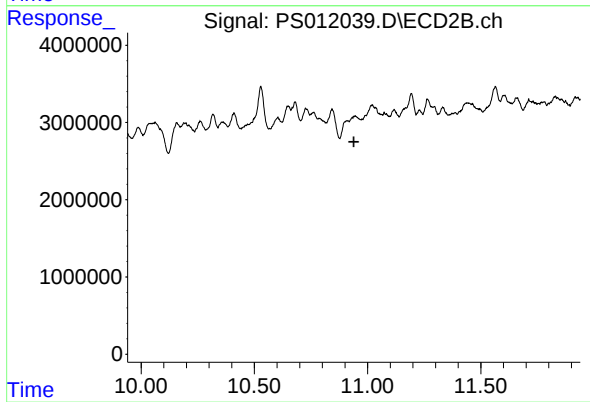

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.940 min
Response: 0
Conc: N.D.