

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
 Data File : PS012040.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2020 14:40
 Operator : DD\AJ
 Sample : L3851-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 15:31:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.218	6.915	265.7E6	159.8E6	243.591	298.790
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	70610567	N.D.	85.836
3) T	4-Nitroph...	7.056	0.000	3985308	0	6.766	N.D. #
5) T	DICAMBA	7.396	7.048	7041429	5461660	1.719	2.528 #
6) T	MCP	7.628	0.000	8352252	0	2.614	N.D. #
7) T	MCPA	7.686	7.460	251.6E6	154.0E6	55.311	56.184
8) T	DICHLORPROP	0.000	7.735	0	11517933	N.D.	20.399
9) T	2,4-D	8.399	0.000	112.0E6	0	99.161	N.D. #
12) T	2,4,5-T	9.413	0.000	29774870	0	5.025	N.D. #
15) T	Picloram	10.998	0.000	10226112	0	1.308	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
Data File : PS012040.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2020 14:40
Operator : DD\AJ
Sample : L3851-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 15:31:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

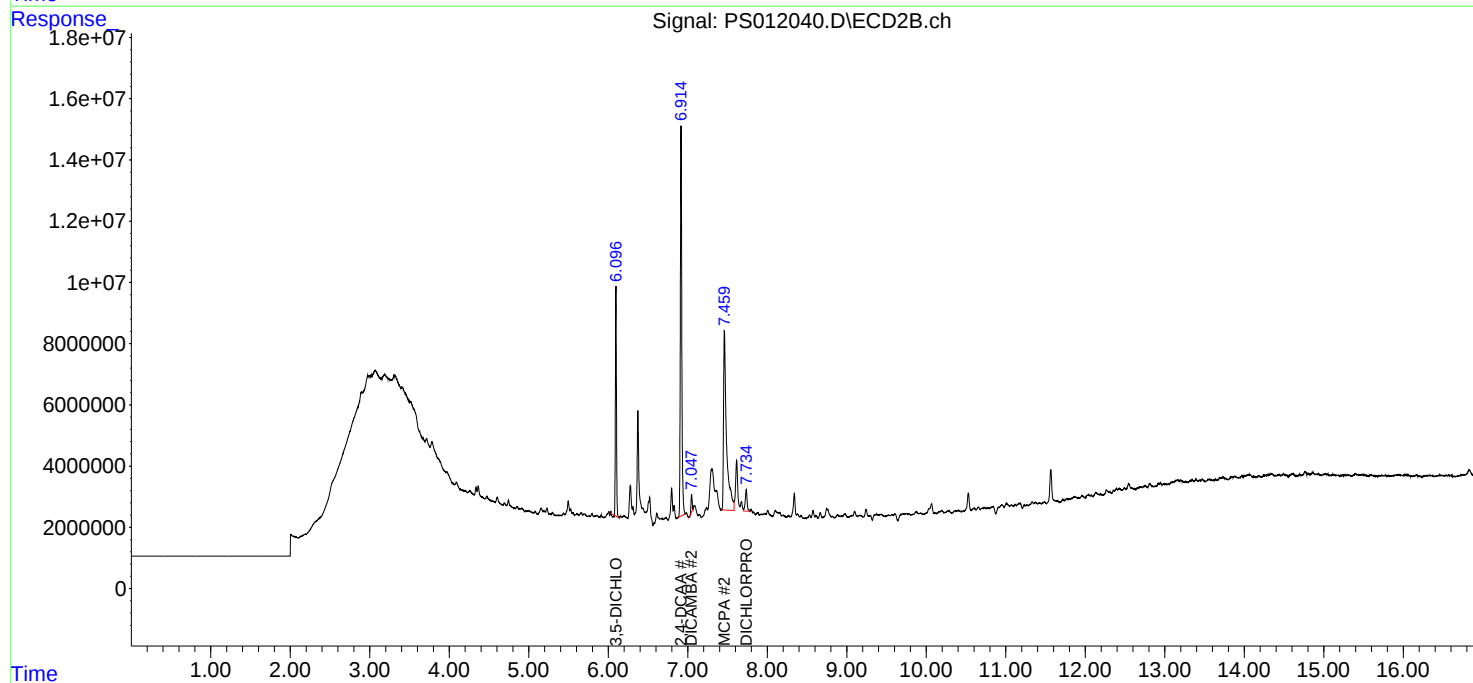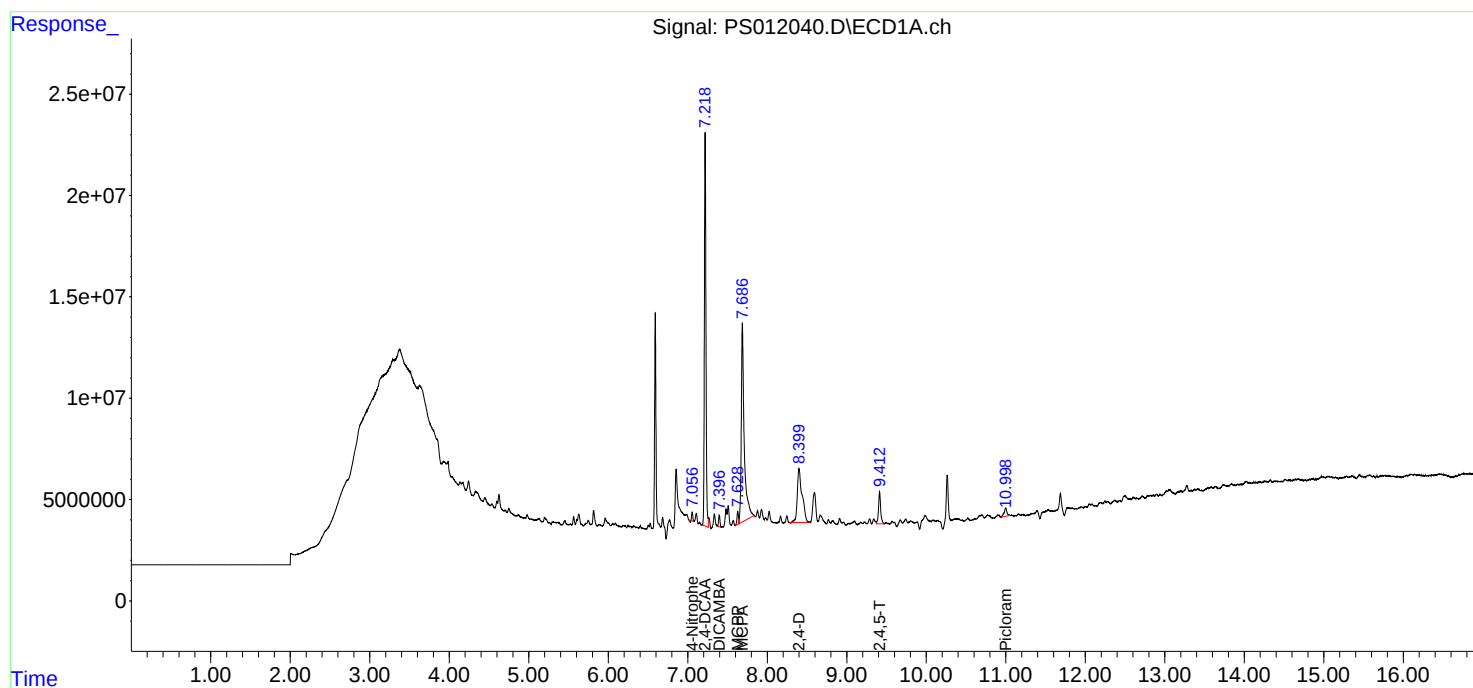


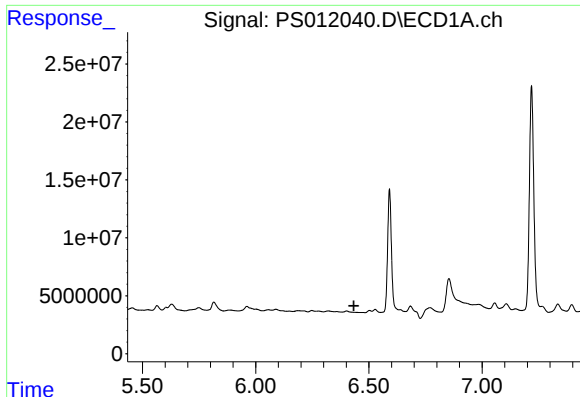

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

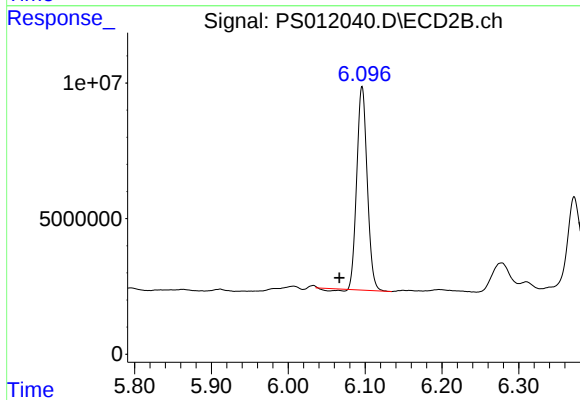


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 70610567
Conc: 85.84 ng/ml

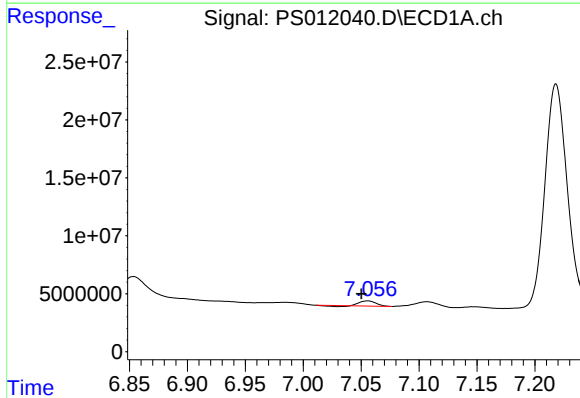


#3 4-Nitrophenol

R.T.: 7.056 min
Delta R.T.: 0.005 min
Response: 3985308
Conc: 6.77 ng/ml

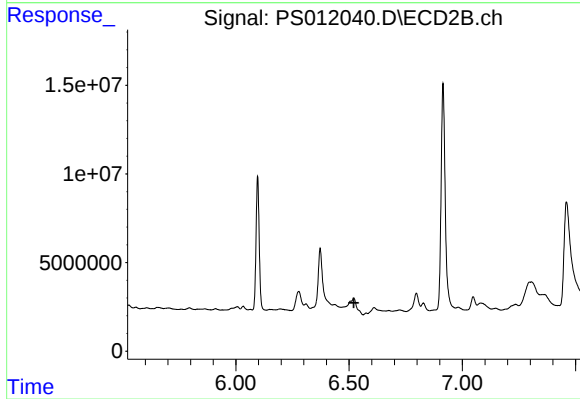

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

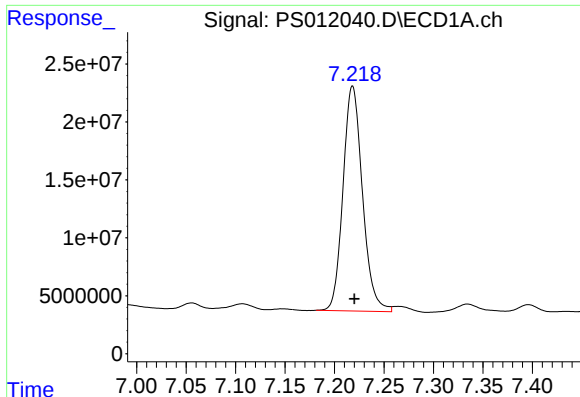

#4 2,4-DCAA


R.T.: 7.218 min
Delta R.T.: -0.002 min
Response: 265701274
Conc: 243.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

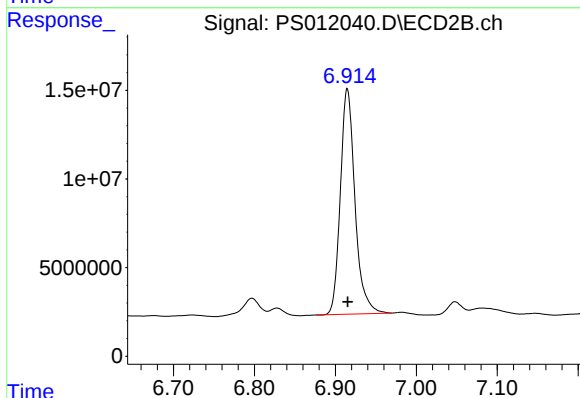


#4 2,4-DCAA

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 159788690
Conc: 298.79 ng/ml

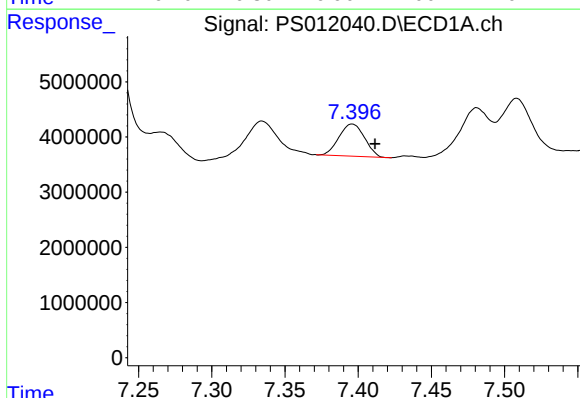


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.016 min
Response: 7041429
Conc: 1.72 ng/ml

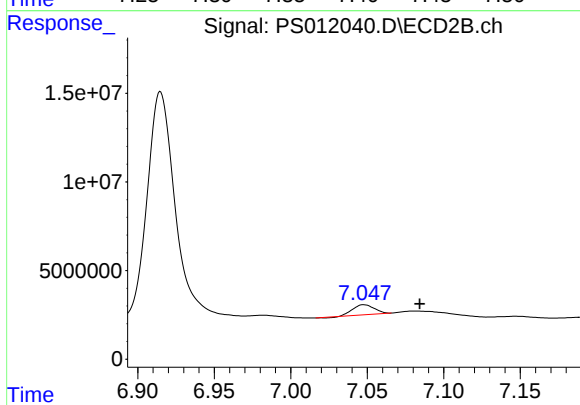

#5 DICAMBA


R.T.: 7.048 min
Delta R.T.: -0.036 min
Response: 5461660
Conc: 2.53 ng/ml

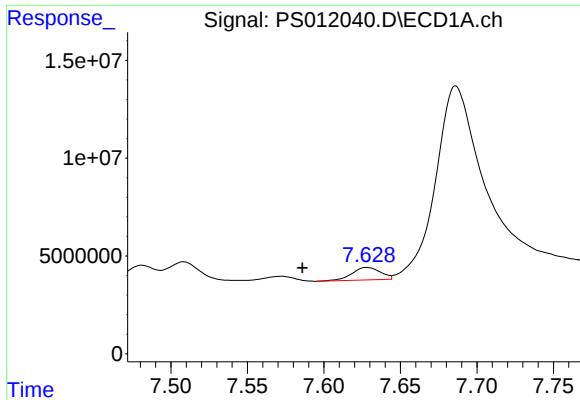

#6 MCPP


R.T.: 7.628 min
Delta R.T.: 0.042 min
Response: 8352252
Conc: 2.61 ug/ml

Instrument :
ECD_S
ClientSampleId :

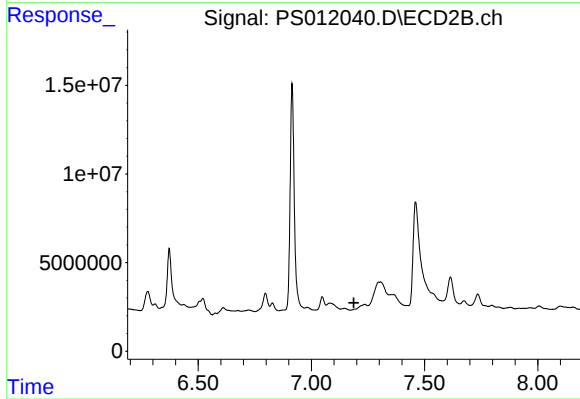


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

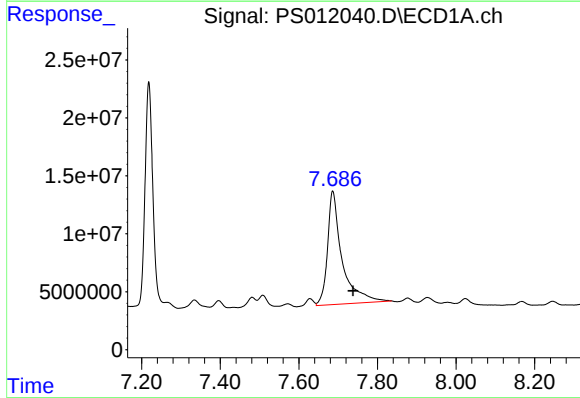


#7 MCPA

R.T.: 7.686 min
Delta R.T.: -0.052 min
Response: 251582721
Conc: 55.31 ug/ml

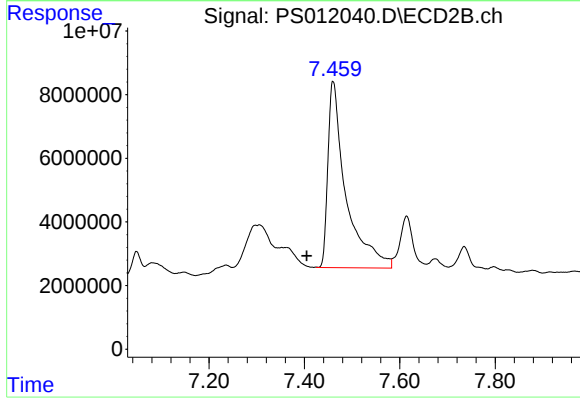

#7 MCPA


R.T.: 7.460 min
Delta R.T.: 0.056 min
Response: 153951071
Conc: 56.18 ug/ml

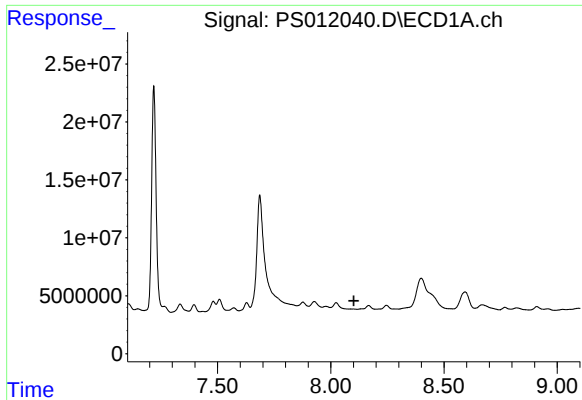

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

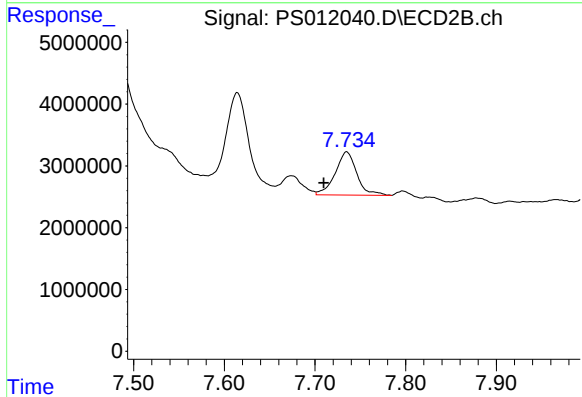


#8 DICHLORPROP

R.T.: 7.735 min
Delta R.T.: 0.025 min
Response: 11517933
Conc: 20.40 ng/ml

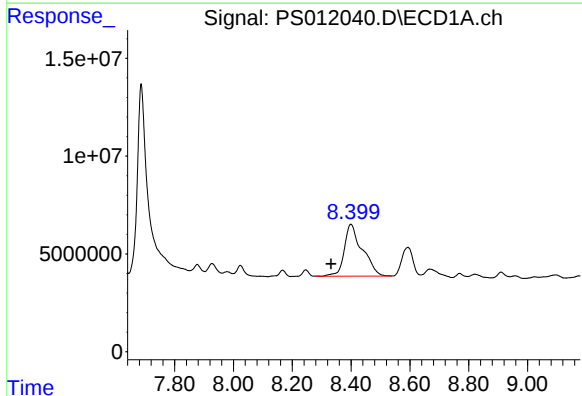


#9 2,4-D

R.T.: 8.399 min
Delta R.T.: 0.067 min
Response: 111961510
Conc: 99.16 ng/ml

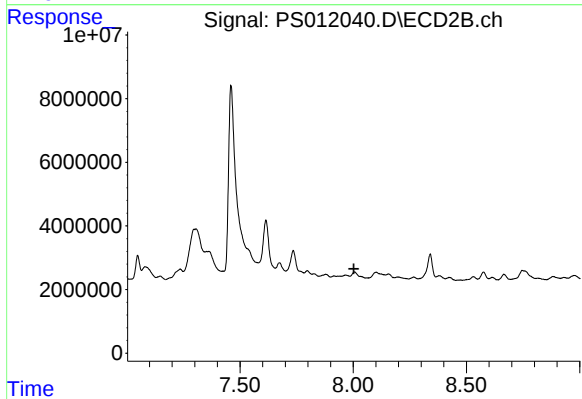

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

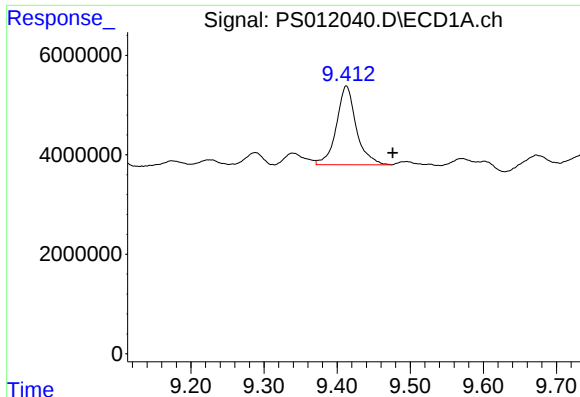

#12 2,4,5-T


R.T.: 9.413 min
Delta R.T.: -0.063 min
Response: 29774870
Conc: 5.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

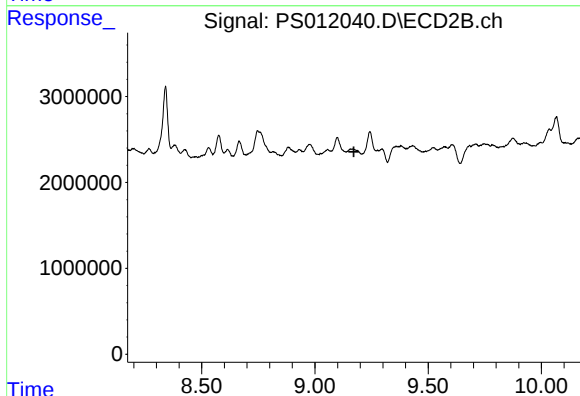


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

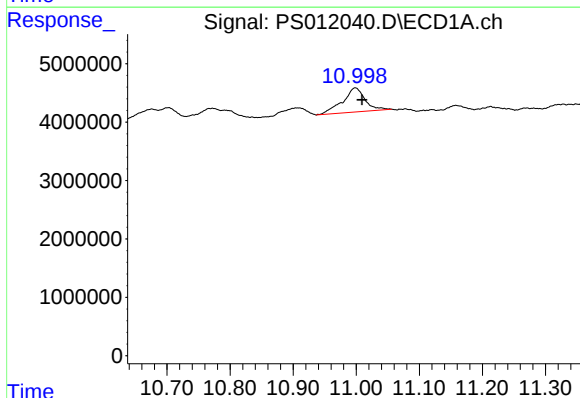

#15 Picloram

R.T.: 10.998 min
Delta R.T.: -0.011 min
Response: 10226112
Conc: 1.31 ng/ml

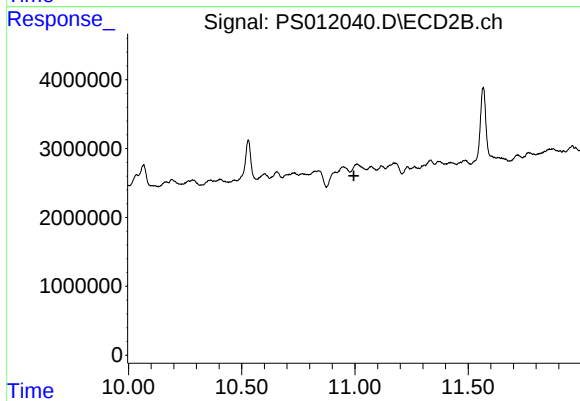

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.