

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
 Data File : PS012041.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2020 15:03
 Operator : DD\AJ
 Sample : L3851-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 15:32:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	249.1E6	157.2E6	228.341	294.033 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	71809131	N.D.	87.293
3) T	4-Nitroph...	7.055	0.000	4831681	0	8.203	N.D. #
5) T	DICAMBA	7.396	7.048	8347736	10042701	2.038	4.648 #
6) T	MCP	7.628	0.000	8417668	0	2.635	N.D. #
7) T	MCPA	7.690	7.464	227.8E6	155.9E6	50.075	56.909
8) T	DICHLORPROP	0.000	7.739	0	16605089	N.D.	29.408
9) T	2,4-D	8.399	0.000	116.1E6	0	102.816	N.D. #
12) T	2,4,5-T	9.412	0.000	21738456	0	3.668	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
Data File : PS012041.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2020 15:03
Operator : DD\AJ
Sample : L3851-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 15:32:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

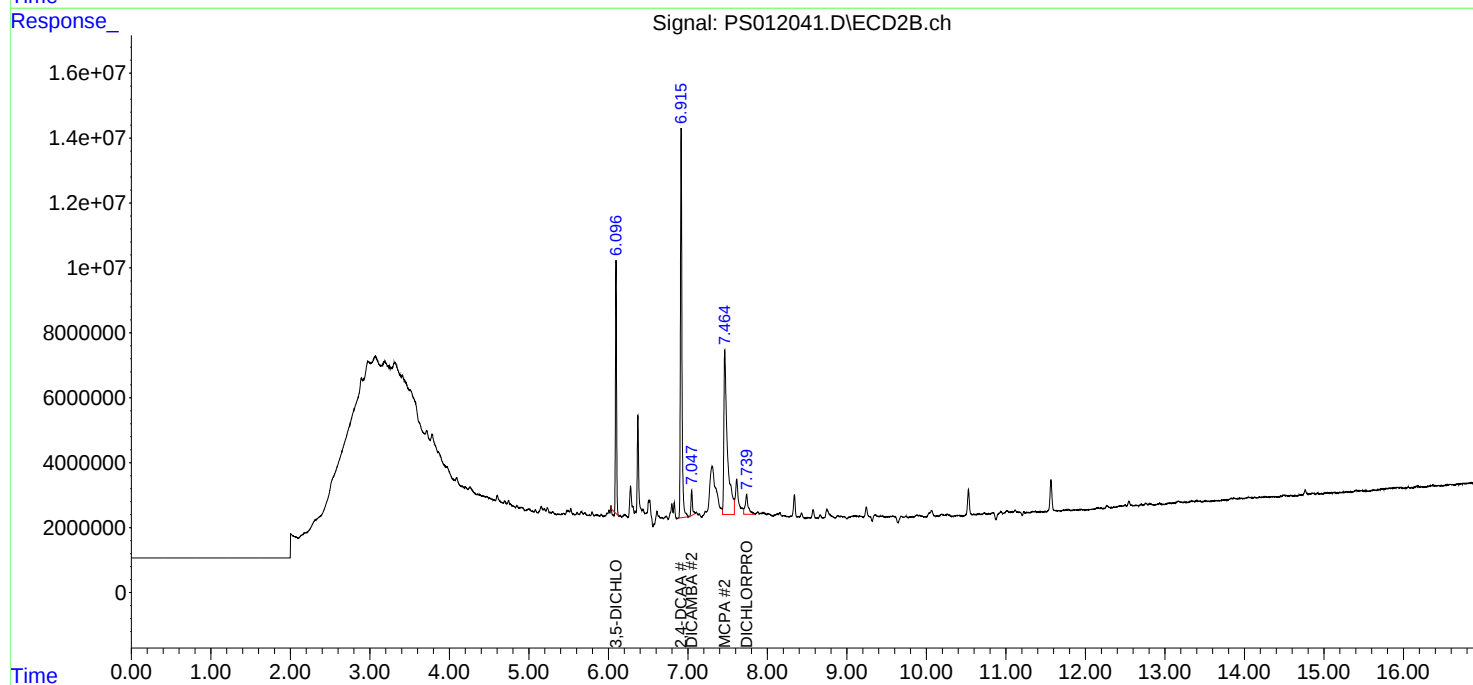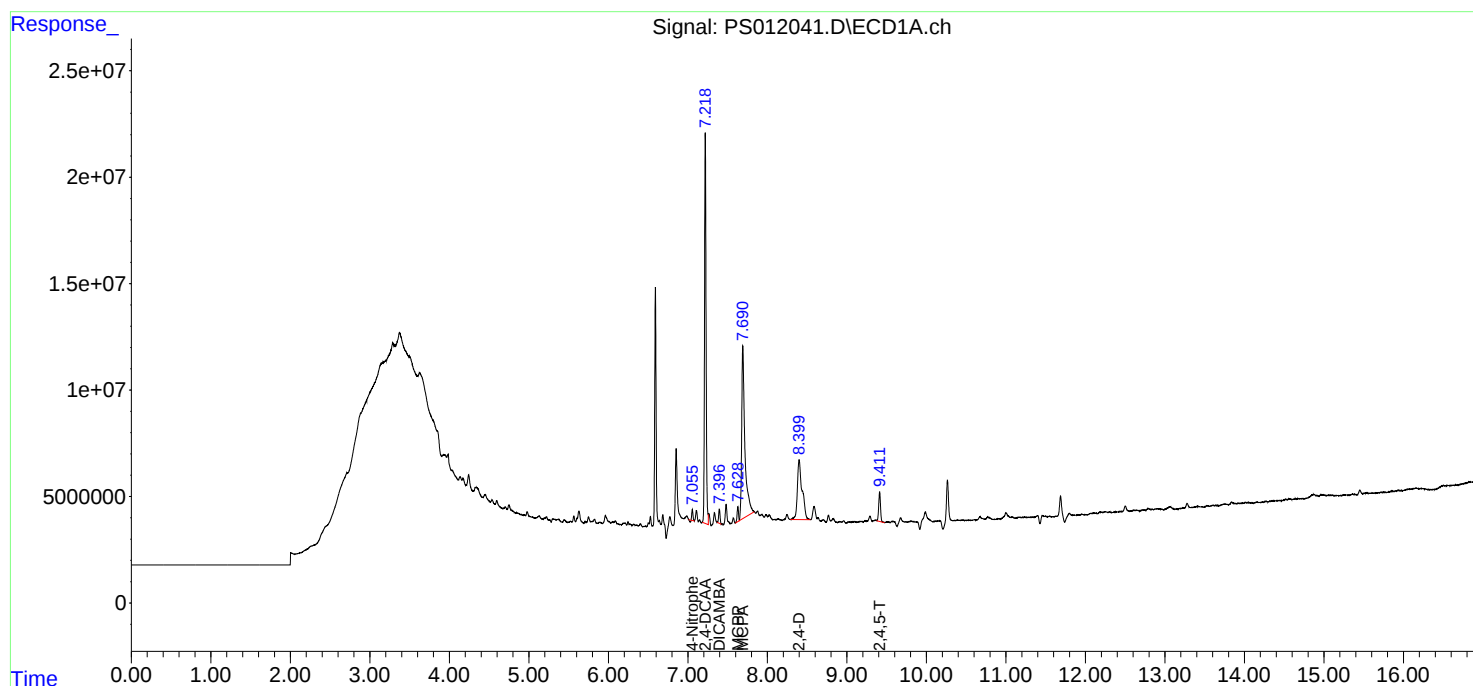


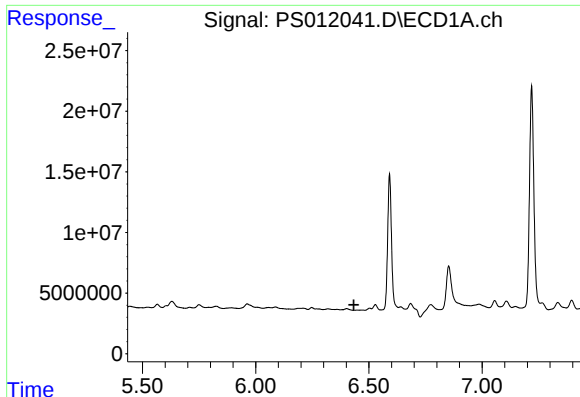

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

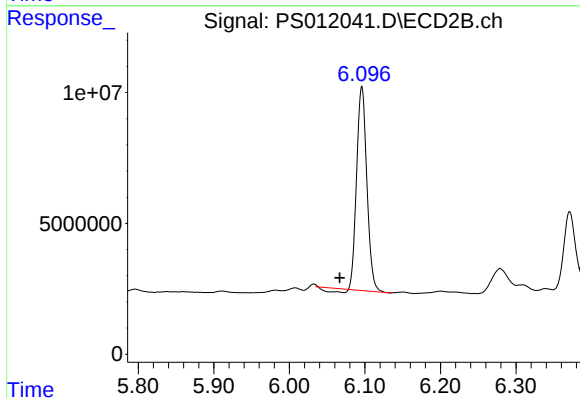


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 71809131
Conc: 87.29 ng/ml

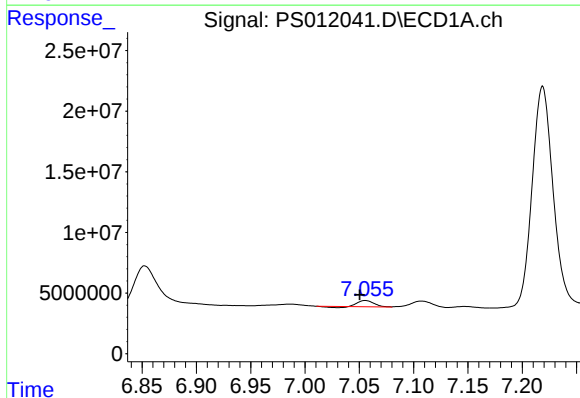


#3 4-Nitrophenol

R.T.: 7.055 min
Delta R.T.: 0.005 min
Response: 4831681
Conc: 8.20 ng/ml

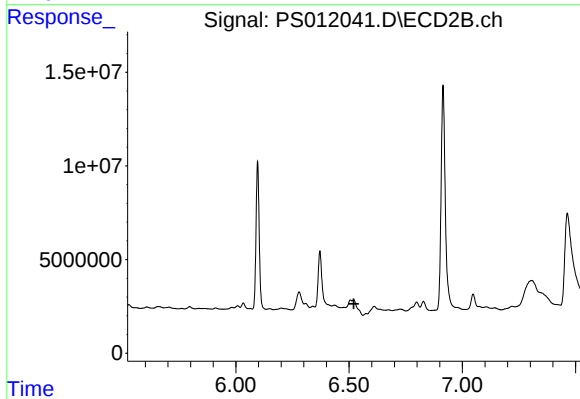

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

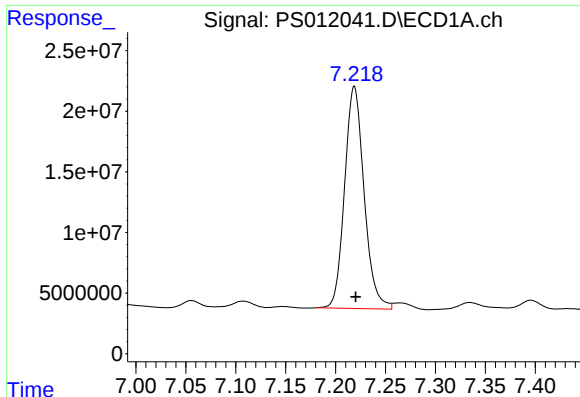

#4 2,4-DCAA


R.T.: 7.219 min
Delta R.T.: -0.001 min
Response: 249066739
Conc: 228.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

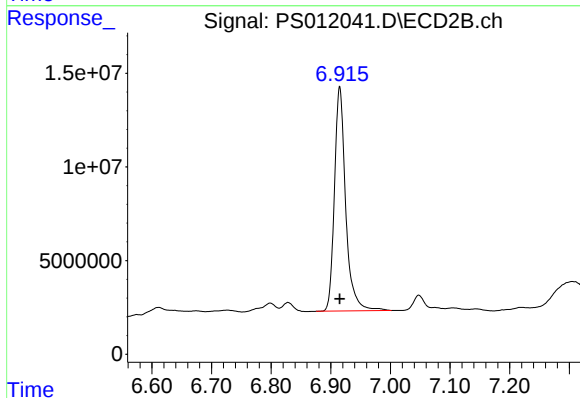


#4 2,4-DCAA

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 157245160
Conc: 294.03 ng/ml

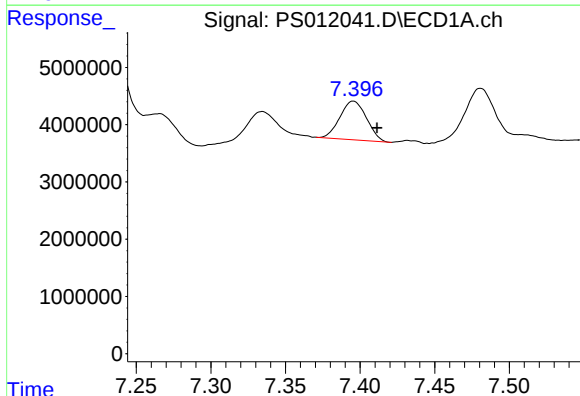


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.016 min
Response: 8347736
Conc: 2.04 ng/ml

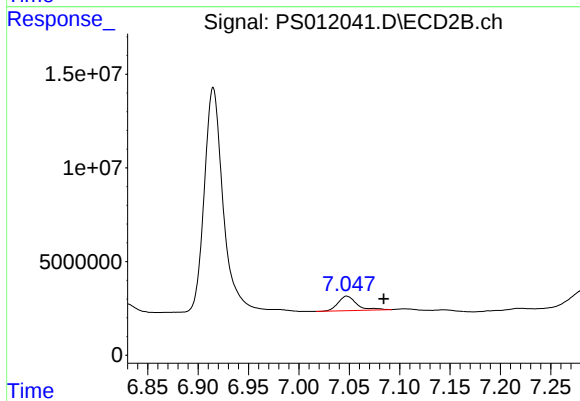

#5 DICAMBA


R.T.: 7.048 min
Delta R.T.: -0.036 min
Response: 10042701
Conc: 4.65 ng/ml

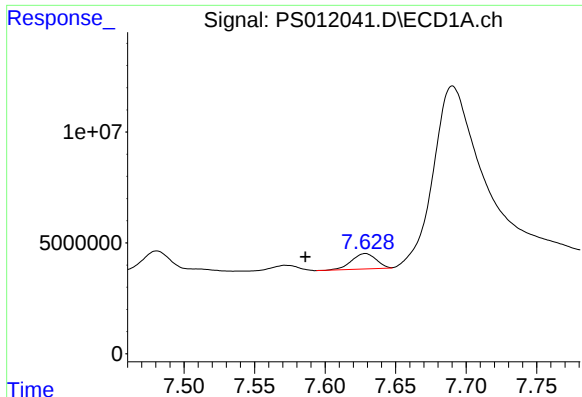

#6 MCPP


R.T.: 7.628 min
Delta R.T.: 0.042 min
Response: 8417668
Conc: 2.63 ug/ml

Instrument :
ECD_S
ClientSampleId :

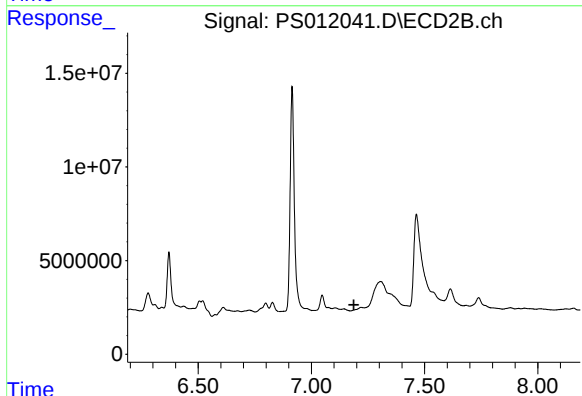


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

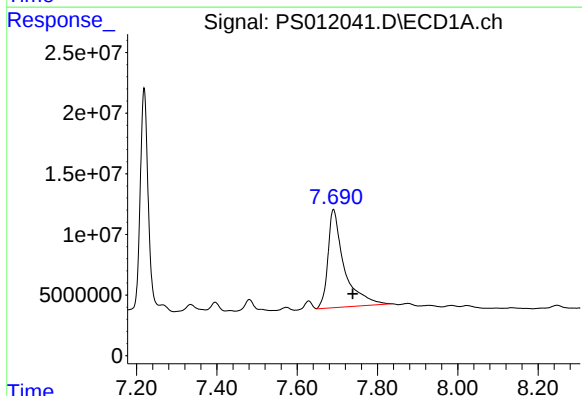


#7 MCPA

R.T.: 7.690 min
Delta R.T.: -0.048 min
Response: 227767598
Conc: 50.08 ug/ml

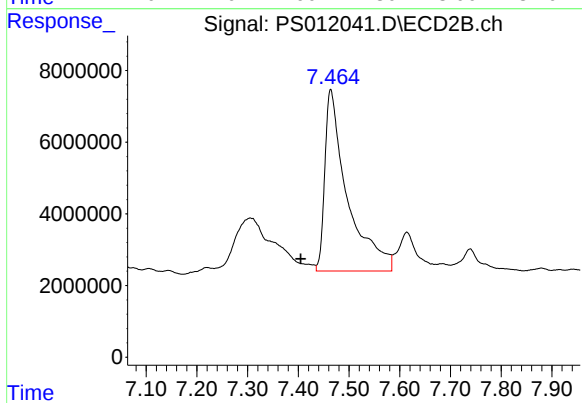

#7 MCPA


R.T.: 7.464 min
Delta R.T.: 0.059 min
Response: 155939859
Conc: 56.91 ug/ml

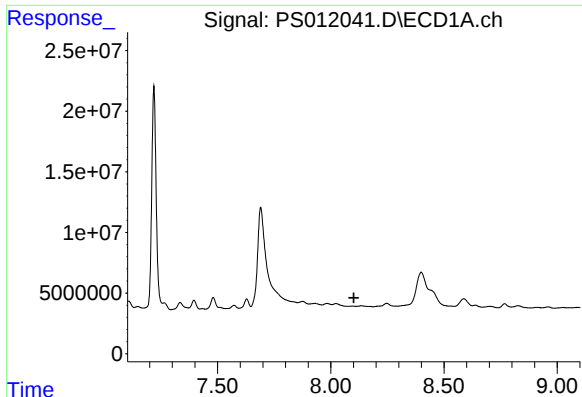

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

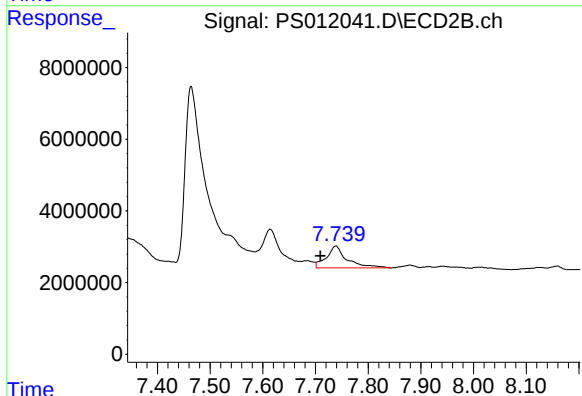


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.029 min
Response: 16605089
Conc: 29.41 ng/ml

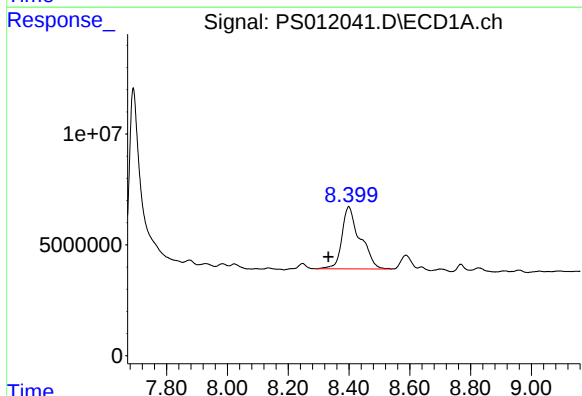


#9 2,4-D

R.T.: 8.399 min
Delta R.T.: 0.067 min
Response: 116089110
Conc: 102.82 ng/ml

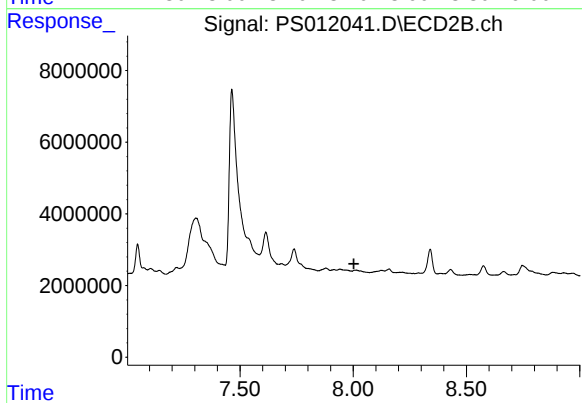

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

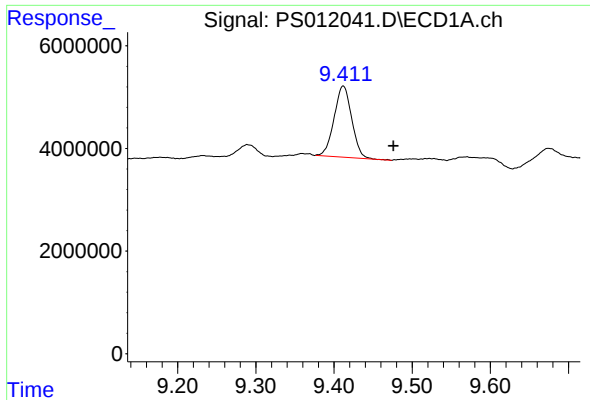

#12 2,4,5-T

R.T.: 9.412 min
Delta R.T.: -0.064 min
Response: 21738456
Conc: 3.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

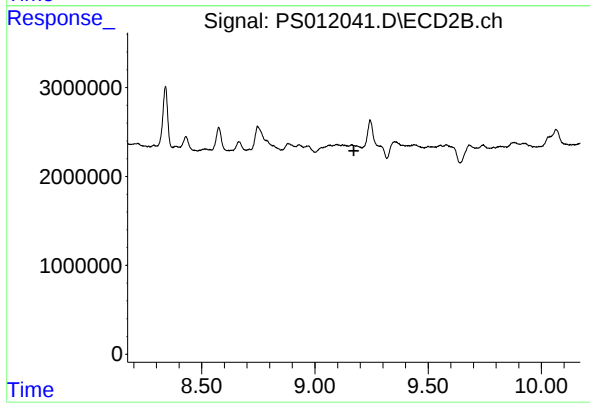

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.