

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
 Data File : PS012046.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2020 16:58
 Operator : DD\AJ
 Sample : L3851-15
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 05:03:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	221.0E6	139.1E6	202.599	260.185 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	72562019	N.D.	88.208
3) T	4-Nitroph...	7.054	0.000	6878868	0	11.678	N.D. #
5) T	DICAMBA	7.396	7.048	8472711	8637432	2.069	3.998 #
6) T	MCP	7.628	0.000	7562281	0	2.367	N.D. #
7) T	MCPA	7.696	7.470	187.1E6	117.3E6	41.138	42.803
9) T	2,4-D	8.399	0.000	141.0E6	0	124.915	N.D. #
12) T	2,4,5-T	9.412	0.000	23707030	0	4.001	N.D. #
14) T	DINOSEB	11.224	0.000	7717501	0	1.644	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
Data File : PS012046.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2020 16:58
Operator : DD\AJ
Sample : L3851-15
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 05:03:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

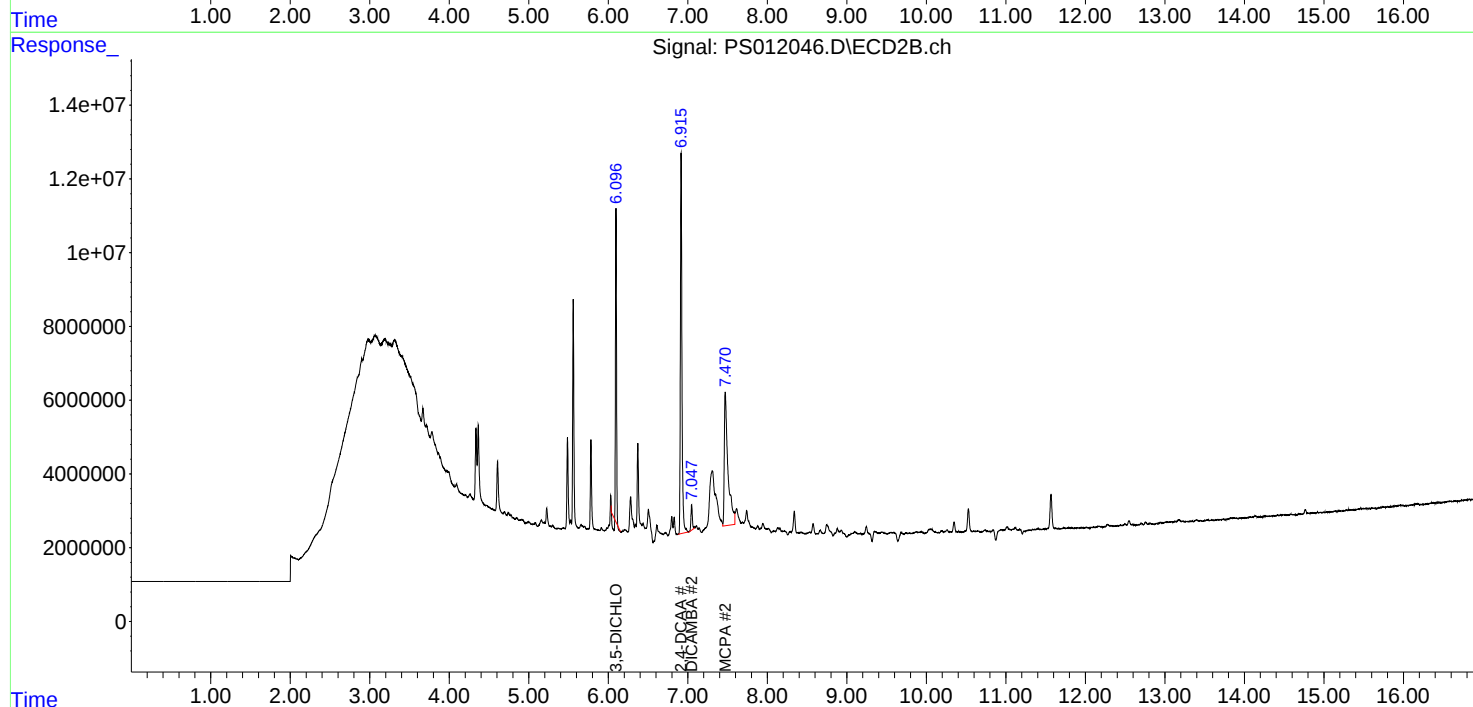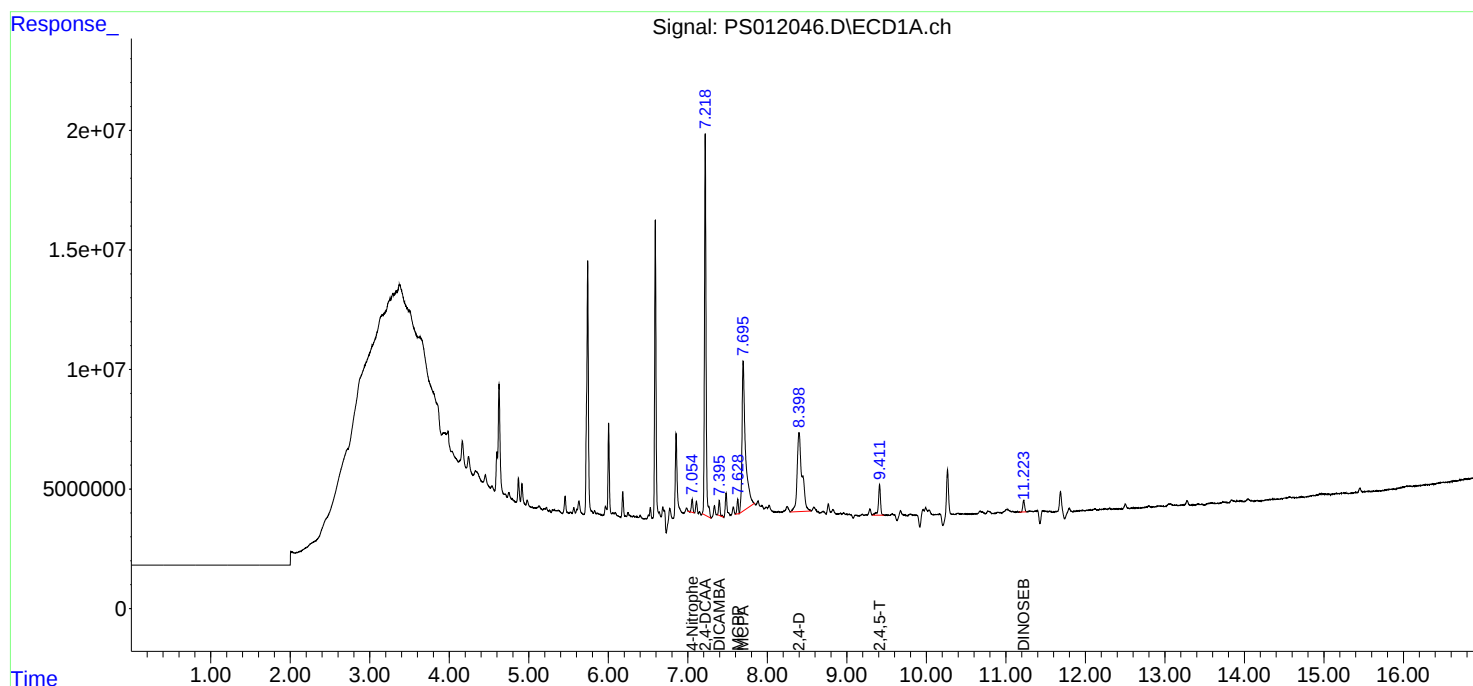


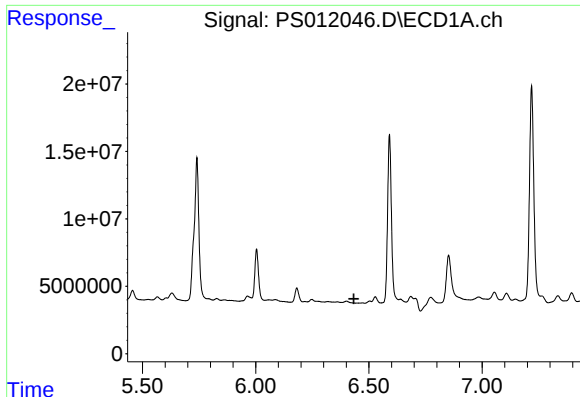

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

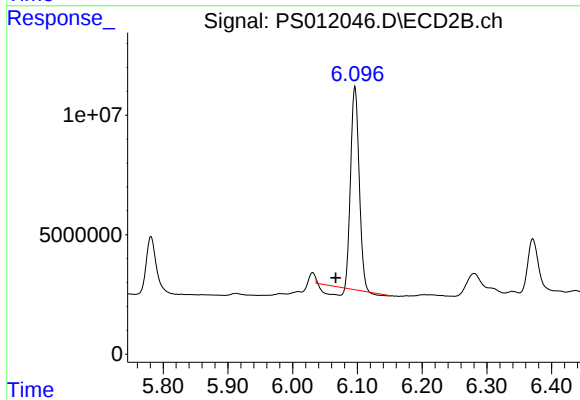


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.030 min
Response: 72562019
Conc: 88.21 ng/ml

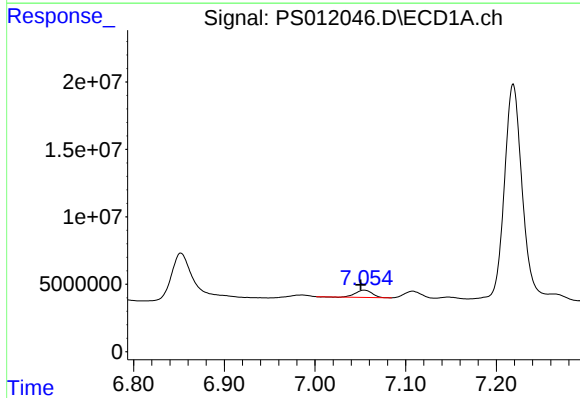


#3 4-Nitrophenol

R.T.: 7.054 min
Delta R.T.: 0.004 min
Response: 6878868
Conc: 11.68 ng/ml

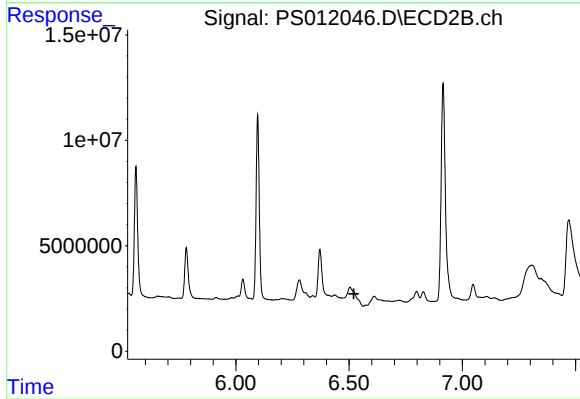

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

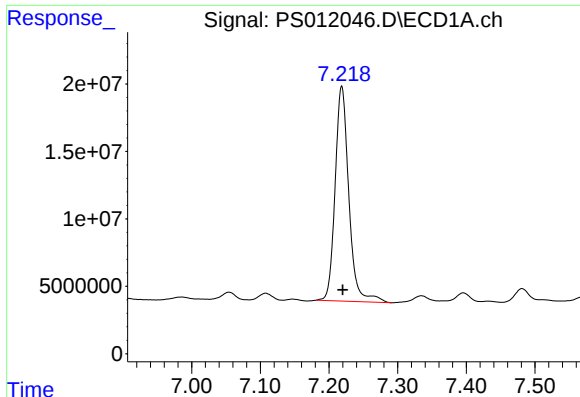

#4 2,4-DCAA


R.T.: 7.219 min
Delta R.T.: -0.001 min
Response: 220989000
Conc: 202.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

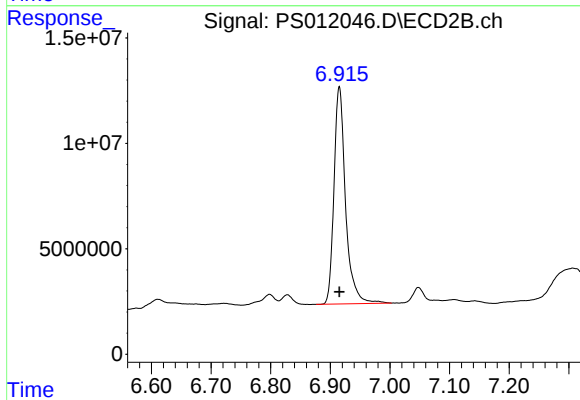


#4 2,4-DCAA

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 139143670
Conc: 260.19 ng/ml

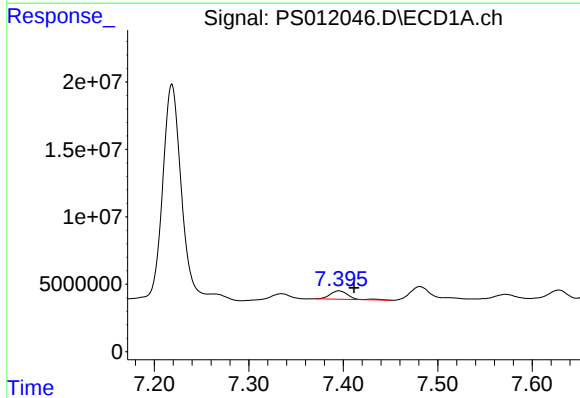


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.016 min
Response: 8472711
Conc: 2.07 ng/ml

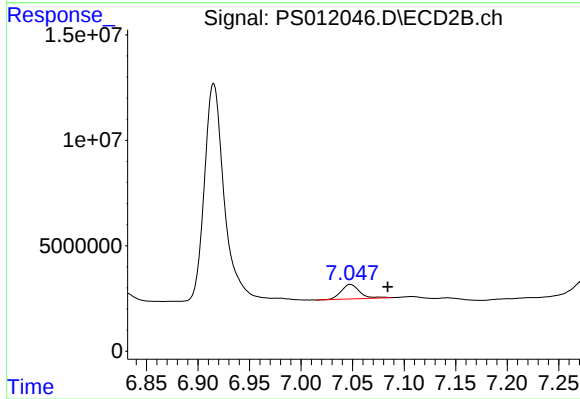

#5 DICAMBA


R.T.: 7.048 min
Delta R.T.: -0.036 min
Response: 8637432
Conc: 4.00 ng/ml

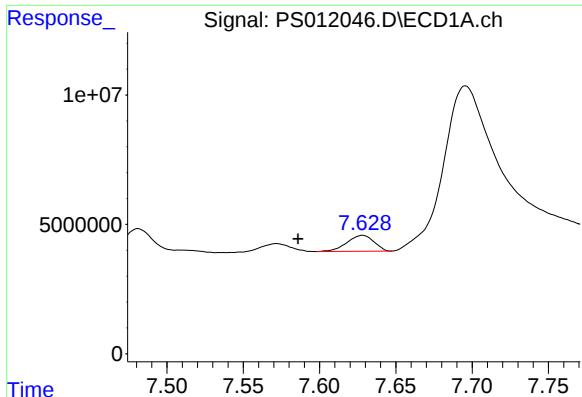

#6 MCPP


R.T.: 7.628 min
Delta R.T.: 0.042 min
Response: 7562281
Conc: 2.37 ug/ml

Instrument :
ECD_S
ClientSampleId :

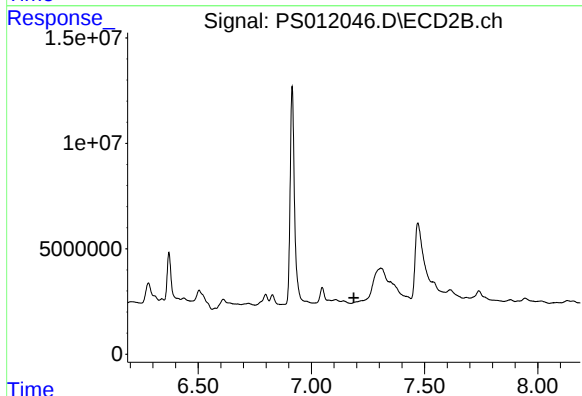


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

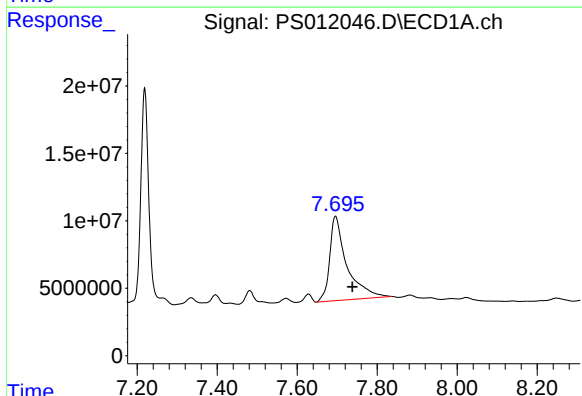


#7 MCPA

R.T.: 7.696 min
Delta R.T.: -0.042 min
Response: 187113693
Conc: 41.14 ug/ml

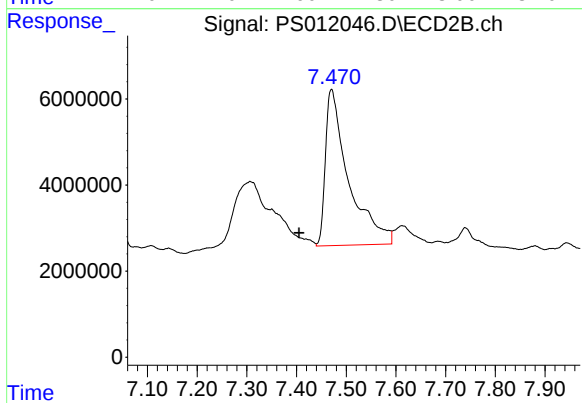

#7 MCPA


R.T.: 7.470 min
Delta R.T.: 0.066 min
Response: 117286194
Conc: 42.80 ug/ml

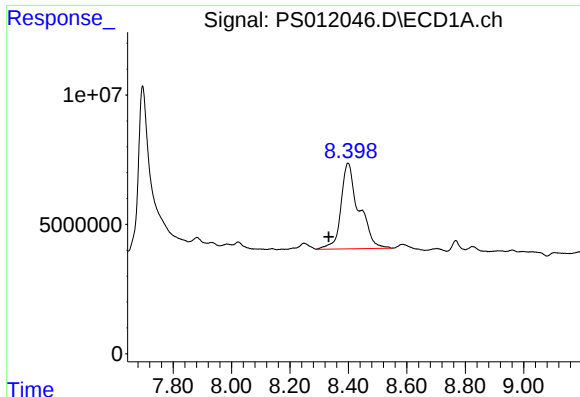

#9 2,4-D


R.T.: 8.399 min
Delta R.T.: 0.067 min
Response: 141040834
Conc: 124.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

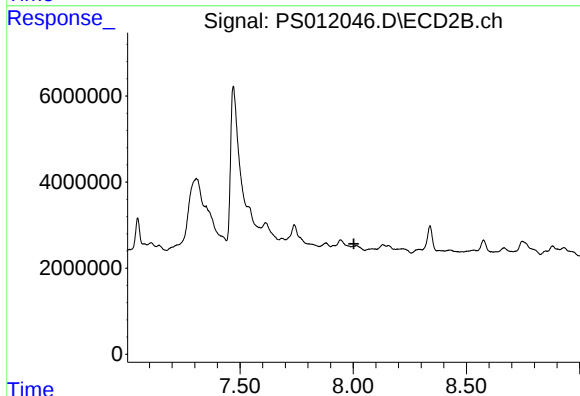


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

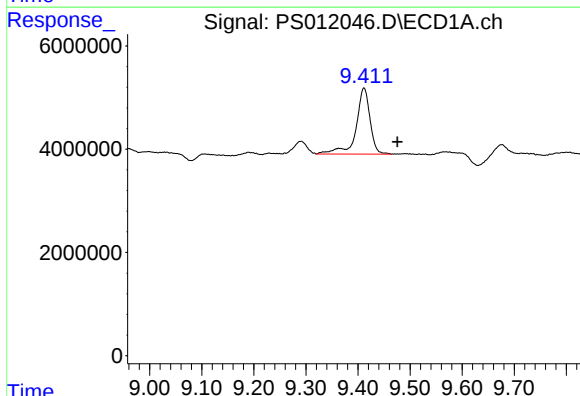


#12 2,4,5-T

R.T.: 9.412 min
Delta R.T.: -0.064 min
Response: 23707030
Conc: 4.00 ng/ml

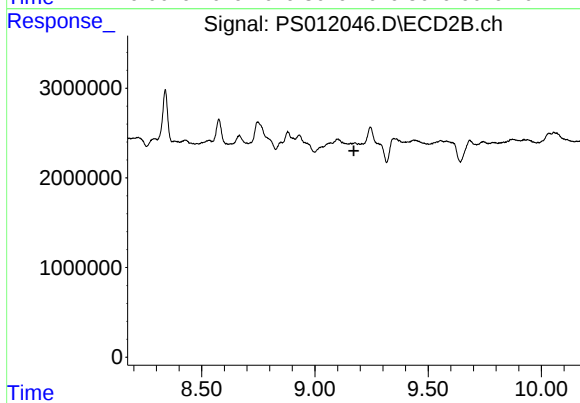

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

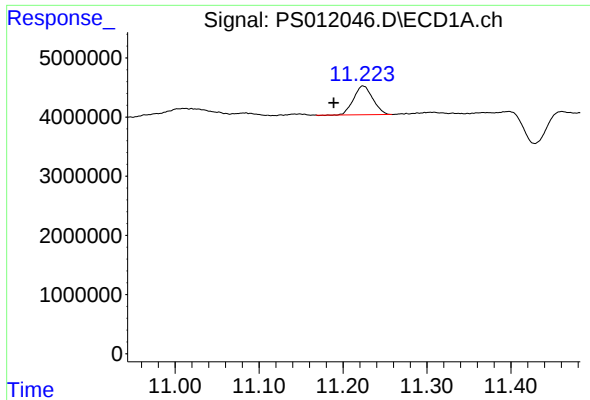

#14 DINOSEB

R.T.: 11.224 min
Delta R.T.: 0.035 min
Response: 7717501
Conc: 1.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

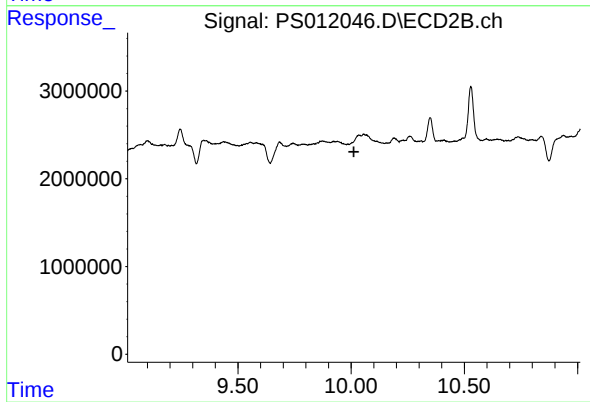

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.012 min
Response: 0
Conc: N.D.