

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
 Data File : PS012048.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2020 17:44
 Operator : DD\AJ
 Sample : L3852-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 05:04:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	215.9E6	134.9E6	197.900	252.164 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.095	0	71625553	N.D.	87.070
5) T	DICAMBA	7.396	7.075	6696223	23669747	1.635	10.956 #
6) T	MCP	7.628	0.000	7540662	0	2.360	N.D. #
7) T	MCPA	7.687	7.462	279.0E6	179.6E6	61.329	65.526
9) T	2,4-D	8.397	0.000	140.4E6	0	124.304	N.D. #
12) T	2,4,5-T	9.412	0.000	25267304	0	4.264	N.D. #
16) T	DCPA	11.515	0.000	26034755	0	3.424	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
Data File : PS012048.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2020 17:44
Operator : DD\AJ
Sample : L3852-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 05:04:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

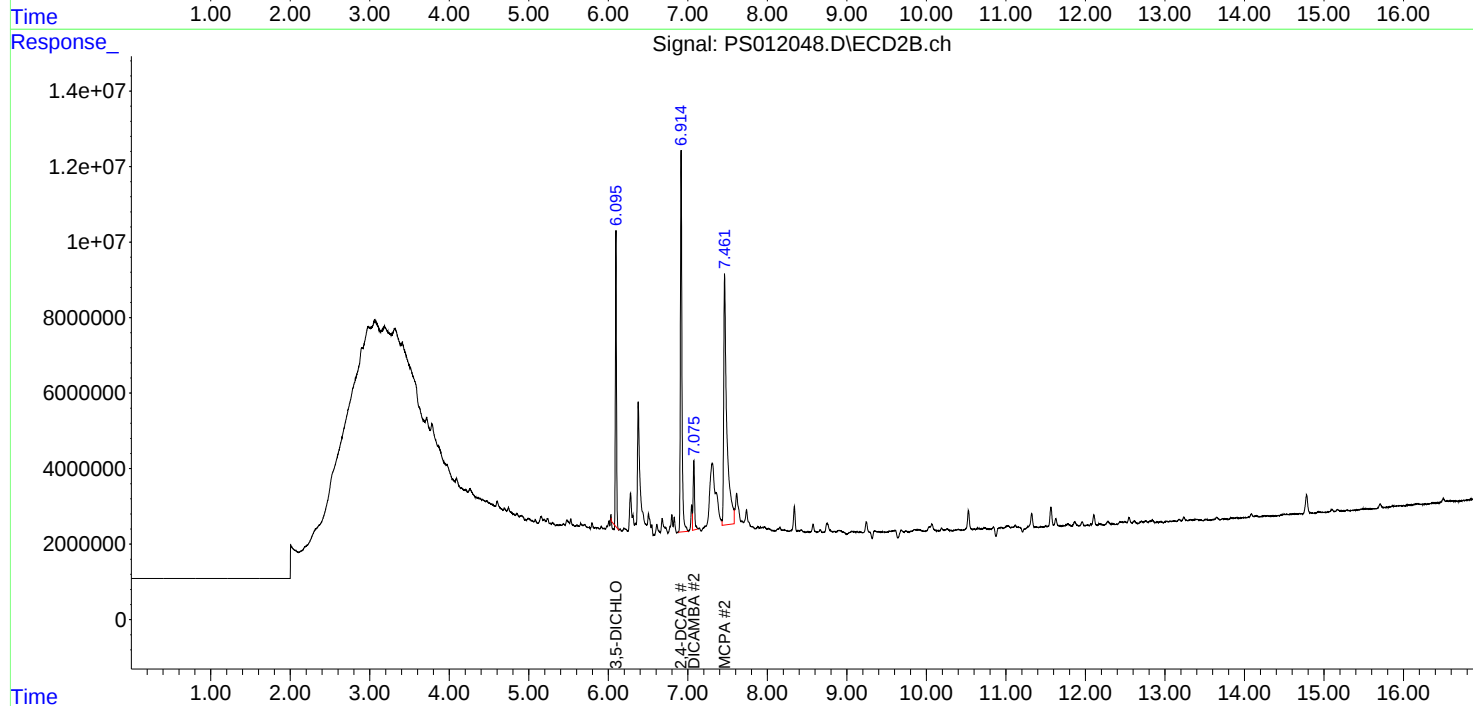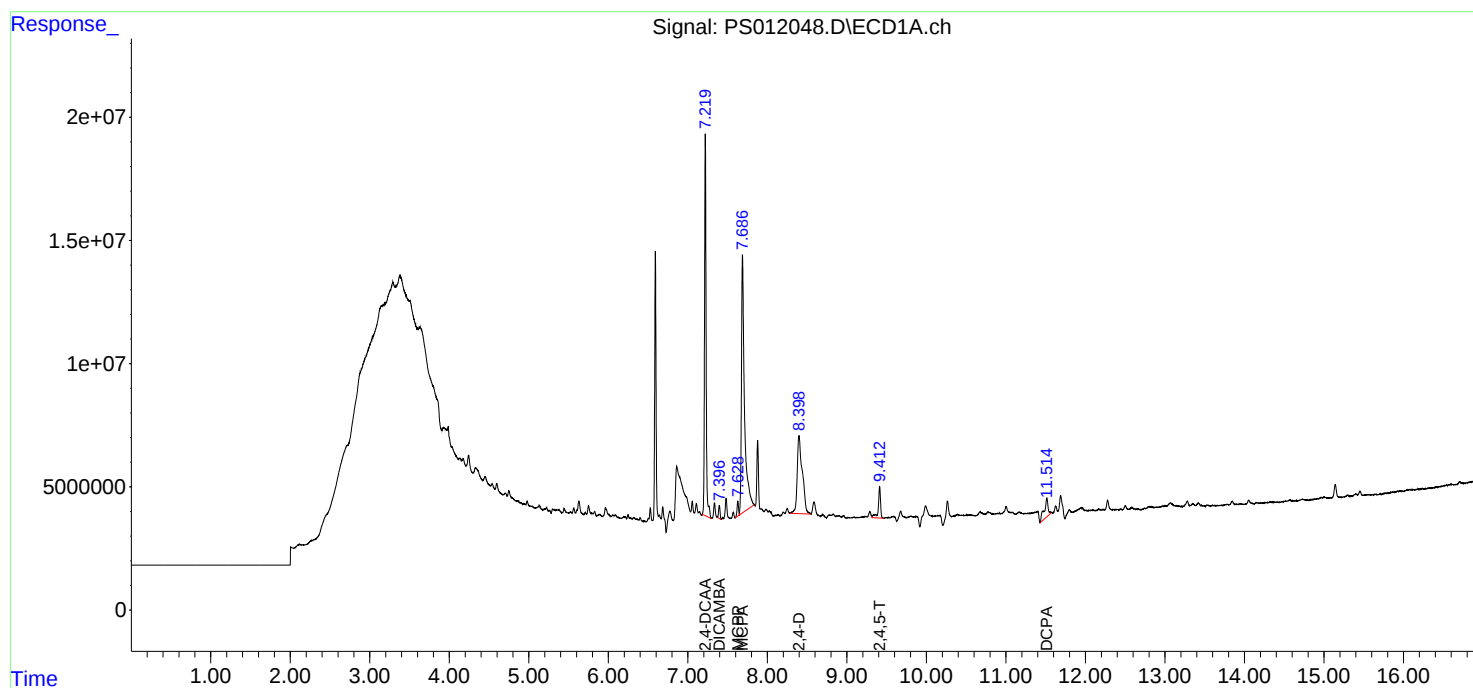


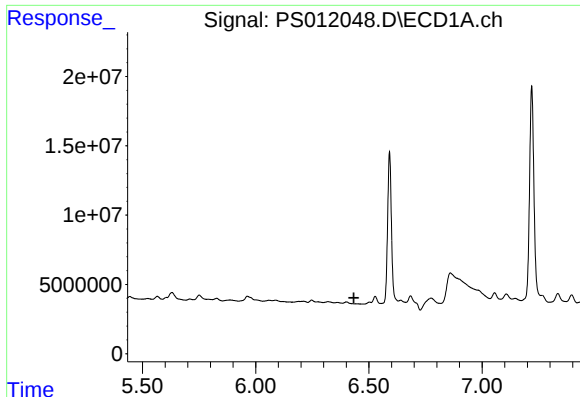

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

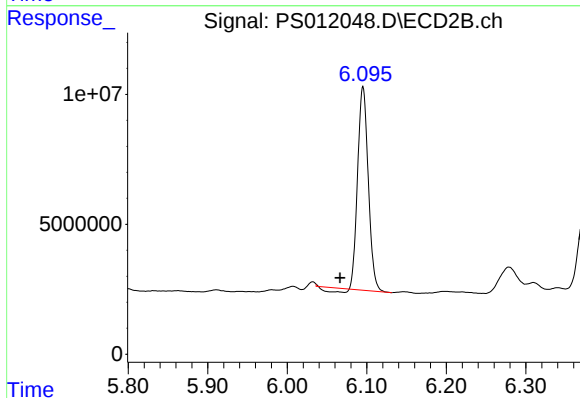


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.029 min
Response: 7162553
Conc: 87.07 ng/ml

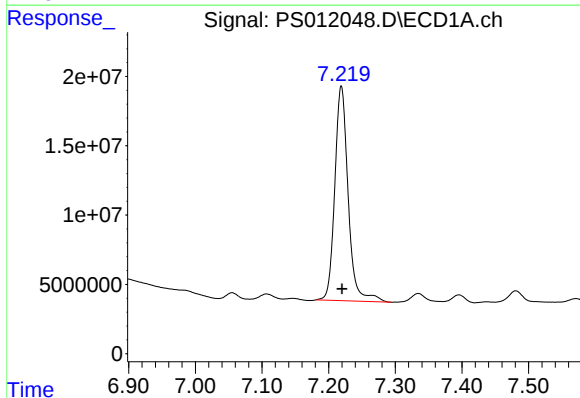


#4 2,4-DCAA

R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 215863457
Conc: 197.90 ng/ml

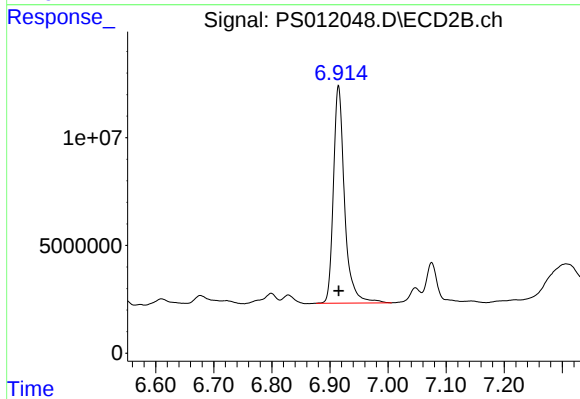

#4 2,4-DCAA


R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 134854022
Conc: 252.16 ng/ml

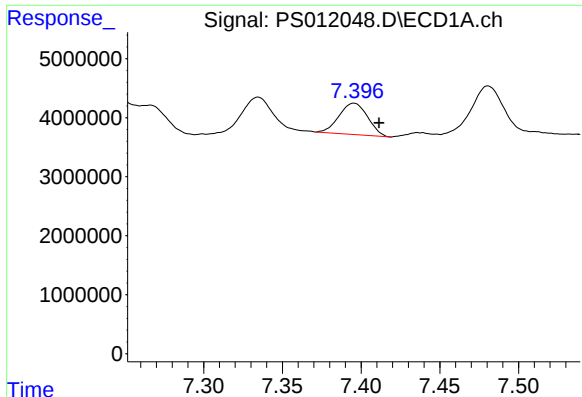

#5 DICAMBA


R.T.: 7.396 min
Delta R.T.: -0.016 min
Response: 6696223
Conc: 1.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

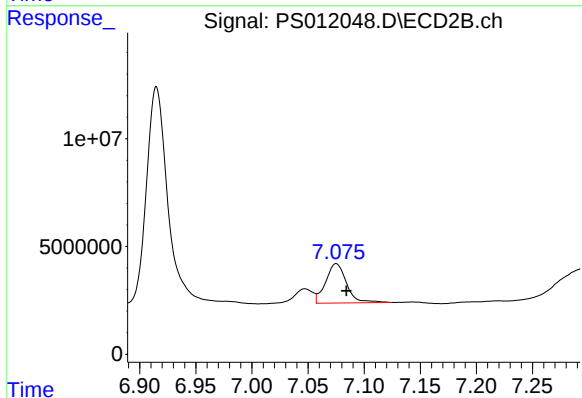


#5 DICAMBA

R.T.: 7.075 min
Delta R.T.: -0.009 min
Response: 23669747
Conc: 10.96 ng/ml

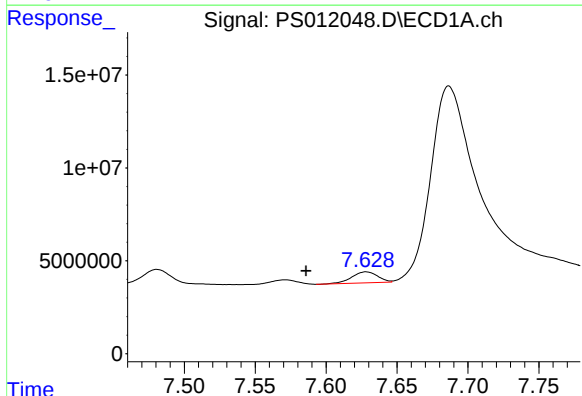


#6 MCP

R.T.: 7.628 min
Delta R.T.: 0.042 min
Response: 7540662
Conc: 2.36 ug/ml

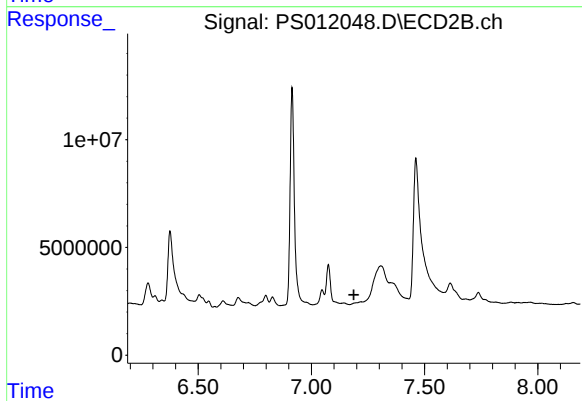

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

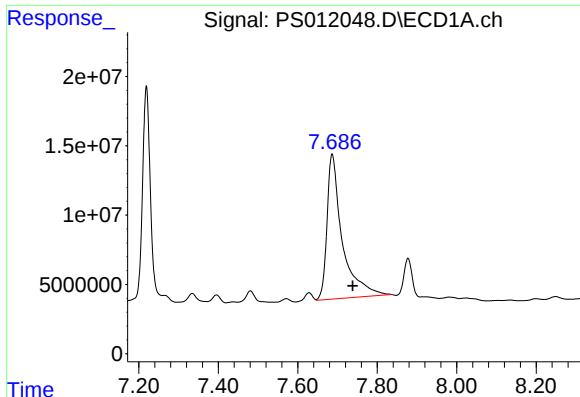

#7 MCPA


R.T.: 7.687 min
Delta R.T.: -0.052 min
Response: 278954542
Conc: 61.33 ug/ml

Instrument :
ECD_S
ClientSampleId :

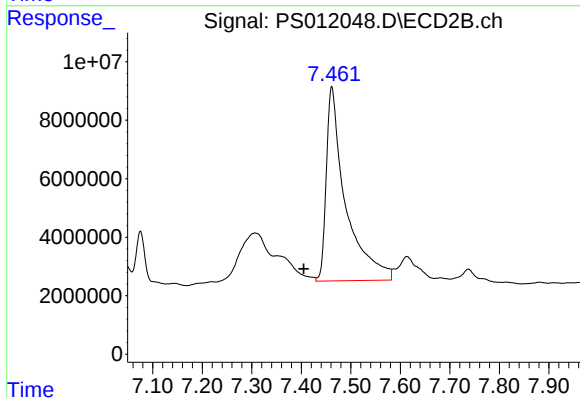


#7 MCPA

R.T.: 7.462 min
Delta R.T.: 0.057 min
Response: 179550729
Conc: 65.53 ug/ml

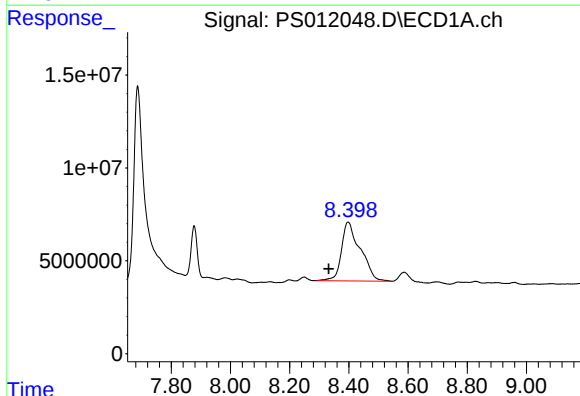


#9 2,4-D

R.T.: 8.397 min
Delta R.T.: 0.065 min
Response: 140350808
Conc: 124.30 ng/ml

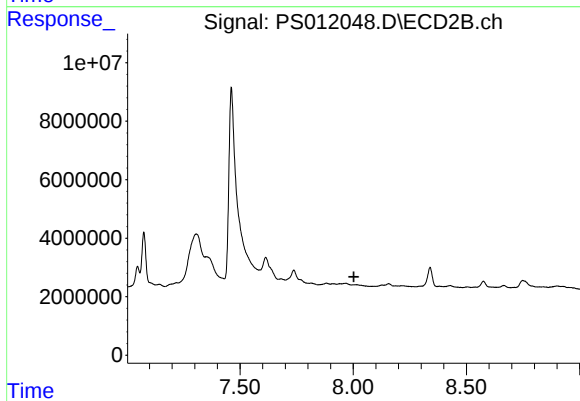

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

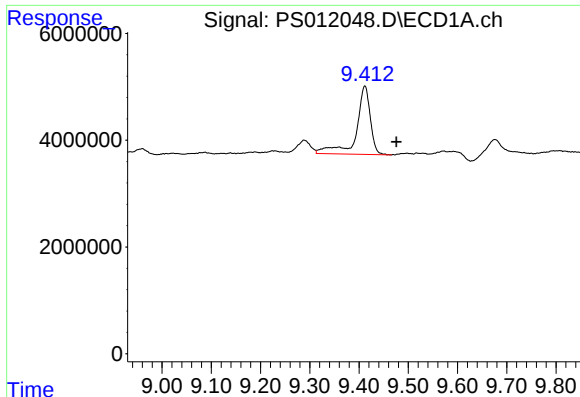

#12 2,4,5-T


R.T.: 9.412 min
Delta R.T.: -0.064 min
Response: 25267304
Conc: 4.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

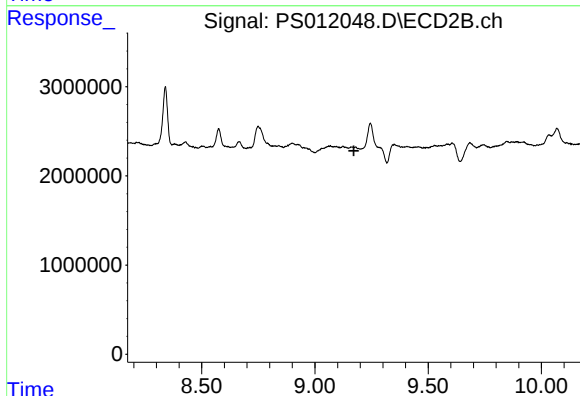


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

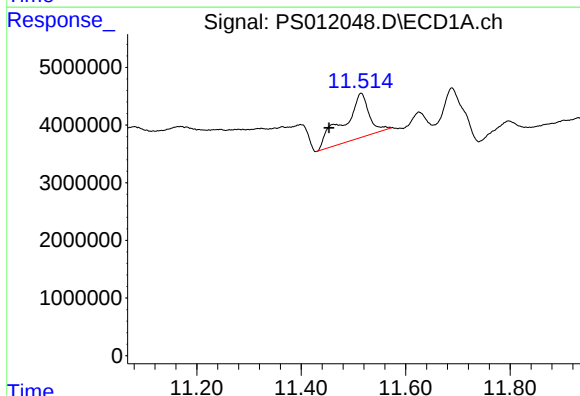

#16 DCPA

R.T.: 11.515 min
Delta R.T.: 0.061 min
Response: 26034755
Conc: 3.42 ng/ml

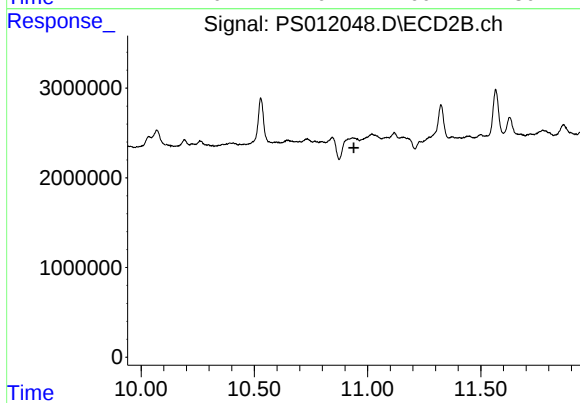

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.940 min
Response: 0
Conc: N.D.