

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
 Data File : PS012050.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2020 18:30
 Operator : DD\AJ
 Sample : L3852-09
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 05:05:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.913	290.2E6	172.7E6	266.033	322.877
Target Compounds							
2) T	3,5-DICHL...	0.000	6.094	0	77843107	N.D.	94.628
3) T	4-Nitroph...	7.056	6.554	-342268	11263698	N.D.	30.892
5) T	DICAMBA	7.442	7.074	7198620	8569411	1.757	3.966 #
6) T	MCP	7.629	0.000	11615817	0	3.636	N.D. #
7) T	MCPA	7.679	7.454	583.6E6	363.4E6	128.312	132.630
8) T	DICHLORPROP	8.049	7.733	7548344	12547552	7.513	22.222 #
9) T	2,4-D	8.399	0.000	116.8E6	0	103.483	N.D. #
12) T	2,4,5-T	9.411	9.238	23197913	10527615	3.915	3.557
14) T	DINOSEB	0.000	10.030	0	8981233	N.D.	4.225
15) T	Picloram	10.996	0.000	19433560	0	2.487	N.D. #
16) T	DCPA	11.444	0.000	10567476	0	1.390	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
Data File : PS012050.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2020 18:30
Operator : DD\AJ
Sample : L3852-09
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 05:05:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

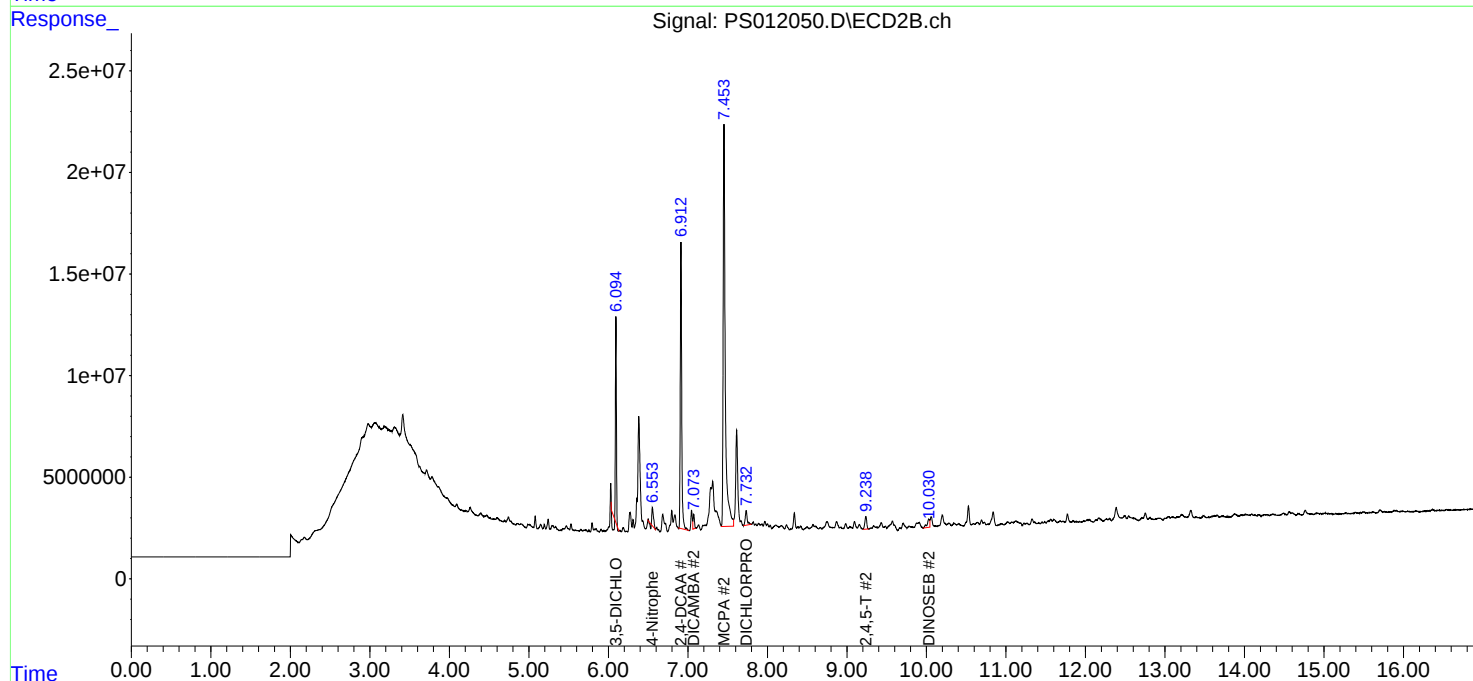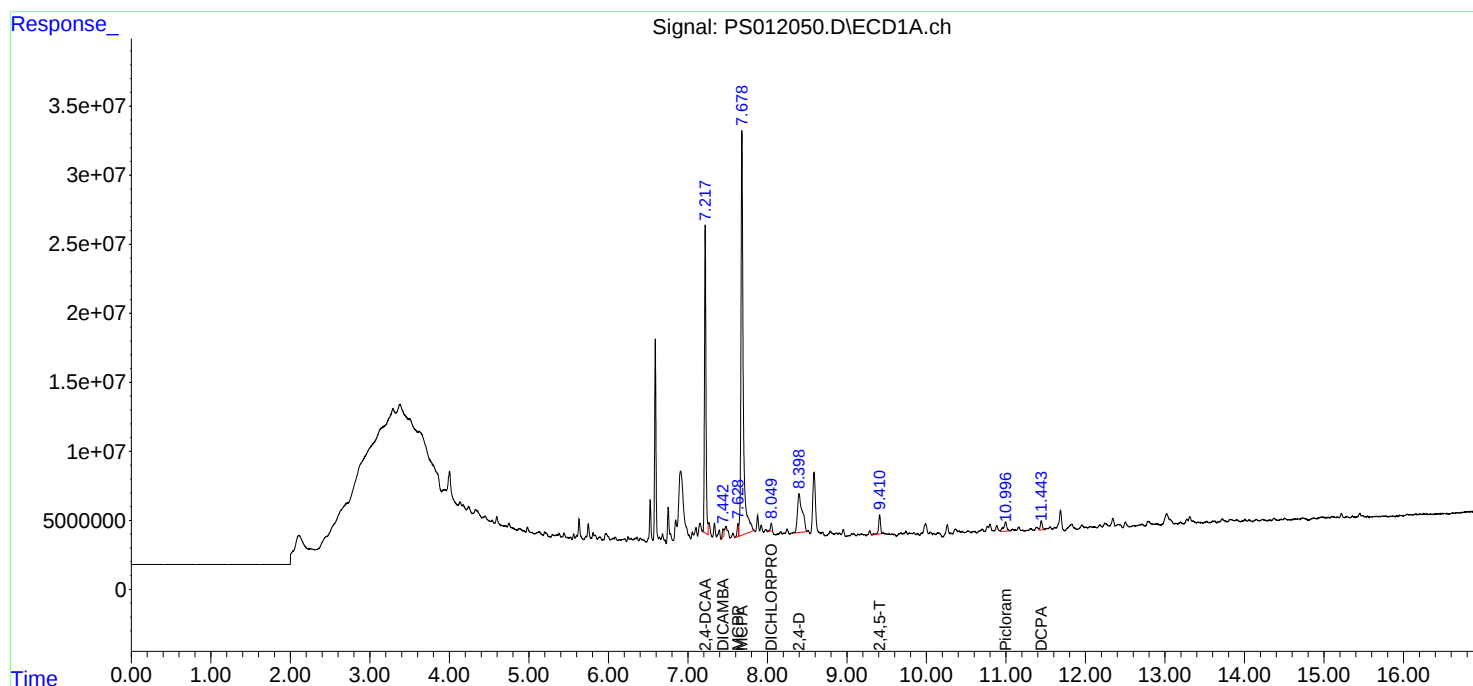


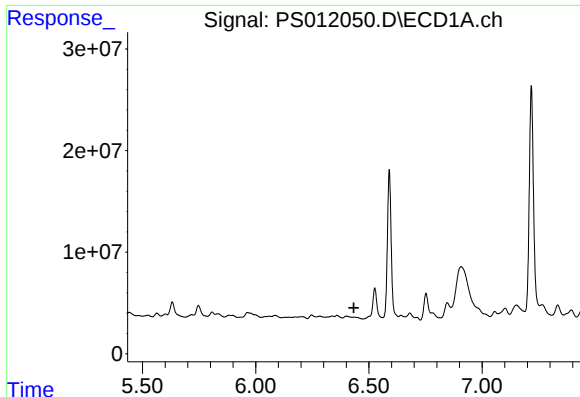

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

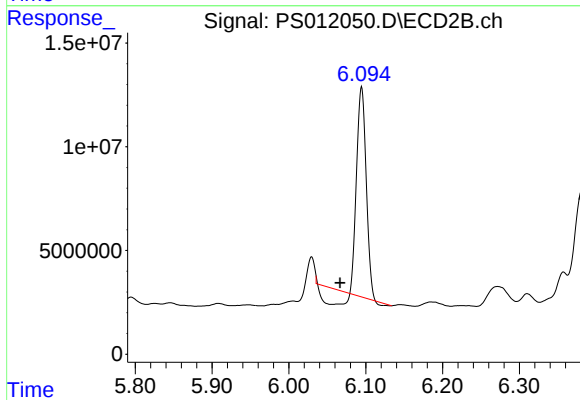


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.094 min
Delta R.T.: 0.028 min
Response: 77843107
Conc: 94.63 ng/ml

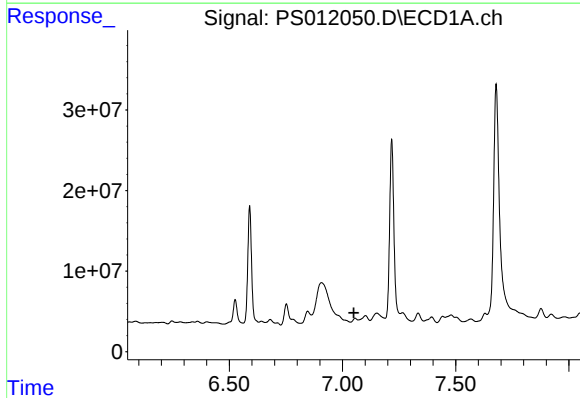


#3 4-Nitrophenol

R.T.: 7.056 min
Delta R.T.: 0.005 min
Response: -342268
Conc: N.D.

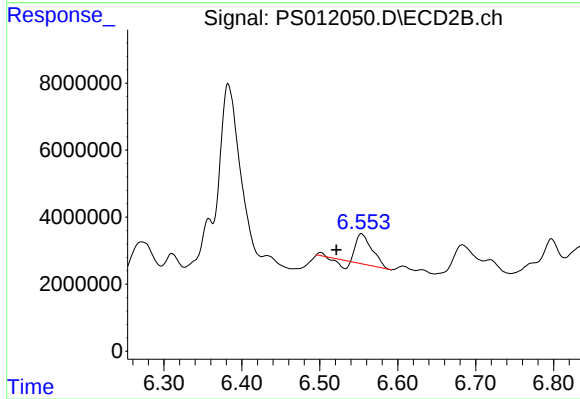

#3 4-Nitrophenol


R.T.: 6.554 min
Delta R.T.: 0.032 min
Response: 11263698
Conc: 30.89 ng/ml

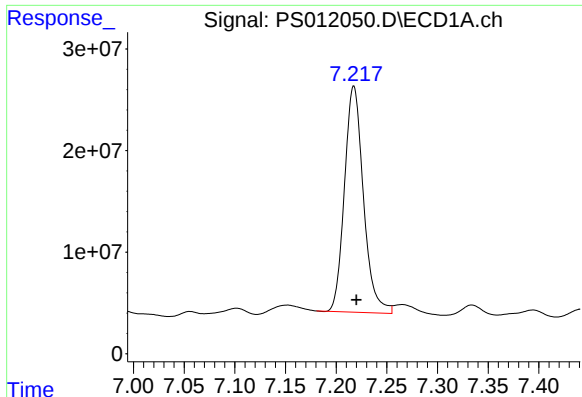

#4 2,4-DCAA


R.T.: 7.217 min
Delta R.T.: -0.003 min
Response: 290180335
Conc: 266.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

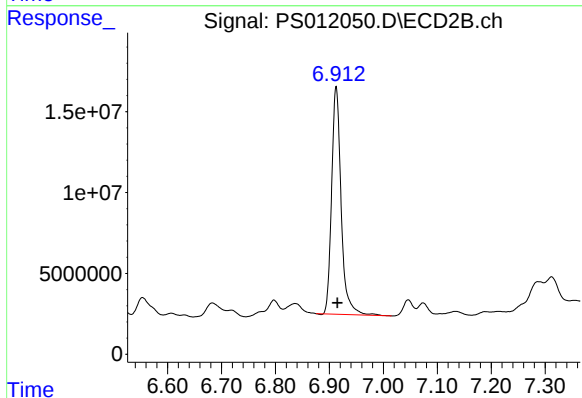


#4 2,4-DCAA

R.T.: 6.913 min
Delta R.T.: -0.002 min
Response: 172670262
Conc: 322.88 ng/ml

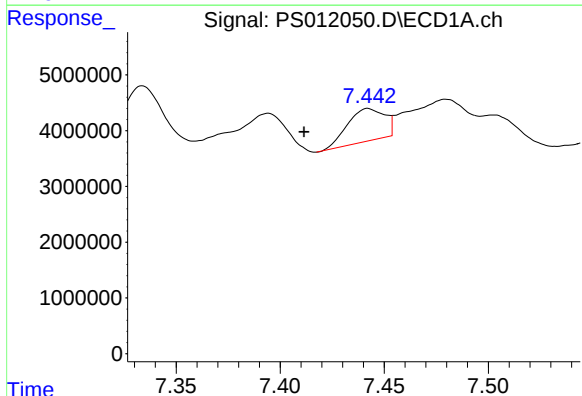


#5 DICAMBA

R.T.: 7.442 min
Delta R.T.: 0.031 min
Response: 7198620
Conc: 1.76 ng/ml

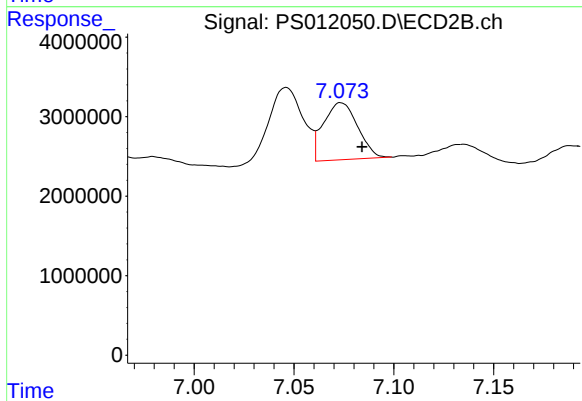

#5 DICAMBA


R.T.: 7.074 min
Delta R.T.: -0.011 min
Response: 8569411
Conc: 3.97 ng/ml

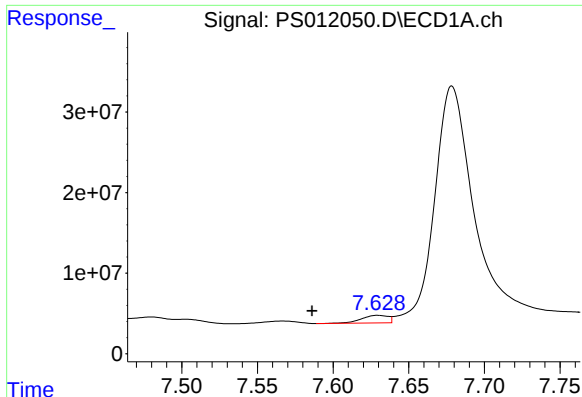

#6 MCPP


R.T.: 7.629 min
Delta R.T.: 0.043 min
Response: 11615817
Conc: 3.64 ug/ml

Instrument :
ECD_S
ClientSampleId :

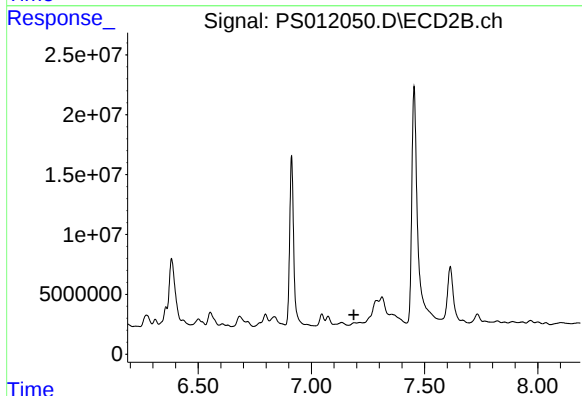


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

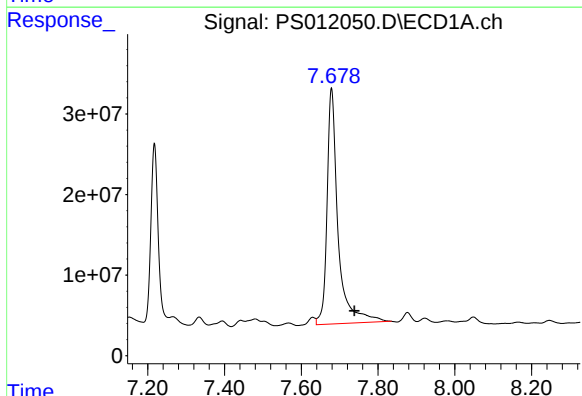


#7 MCPA

R.T.: 7.679 min
Delta R.T.: -0.060 min
Response: 583624334
Conc: 128.31 ug/ml

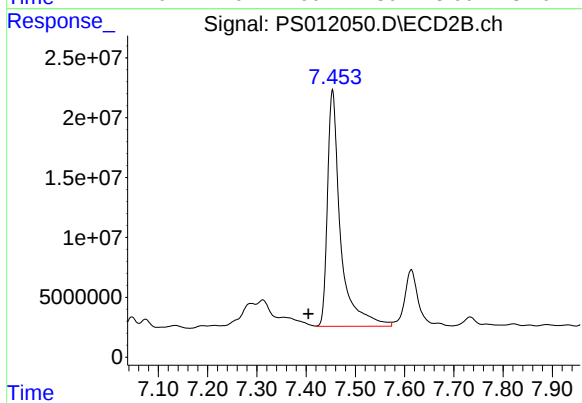

#7 MCPA


R.T.: 7.454 min
Delta R.T.: 0.049 min
Response: 363424846
Conc: 132.63 ug/ml

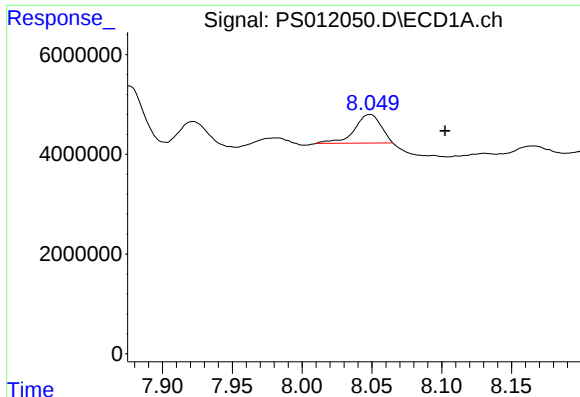

#8 DICHLORPROP


R.T.: 8.049 min
Delta R.T.: -0.054 min
Response: 7548344
Conc: 7.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

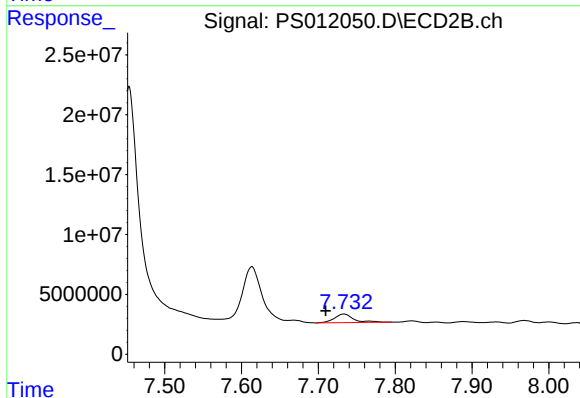


#8 DICHLORPROP

R.T.: 7.733 min
Delta R.T.: 0.024 min
Response: 12547552
Conc: 22.22 ng/ml

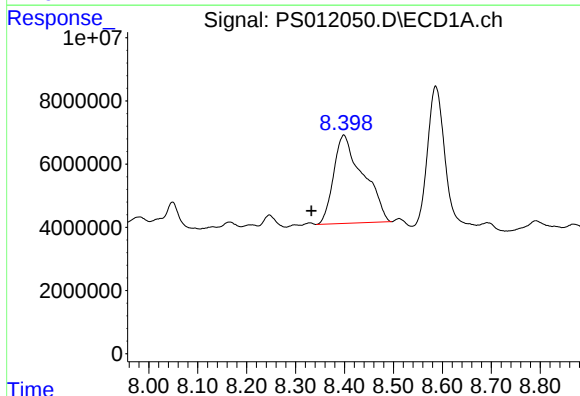


#9 2,4-D

R.T.: 8.399 min
Delta R.T.: 0.067 min
Response: 116841415
Conc: 103.48 ng/ml

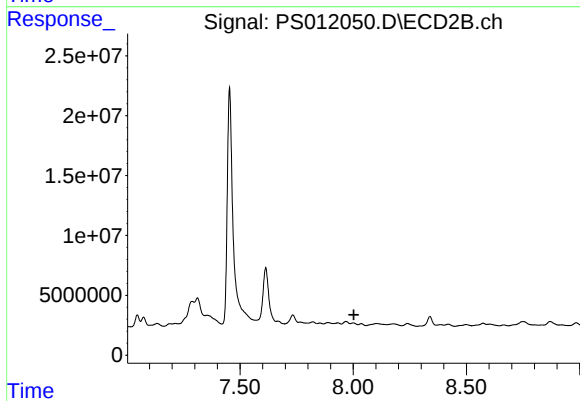

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

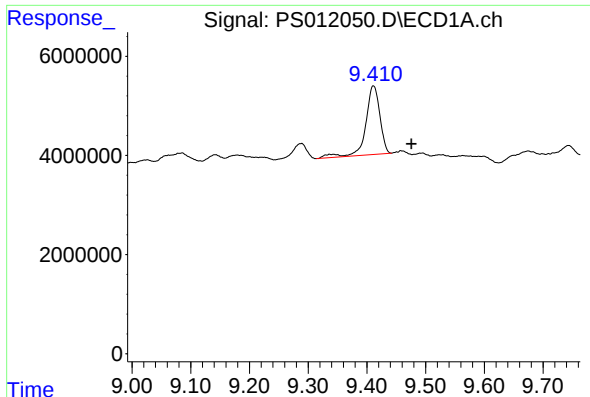

#12 2,4,5-T


R.T.: 9.411 min
Delta R.T.: -0.065 min
Response: 23197913
Conc: 3.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

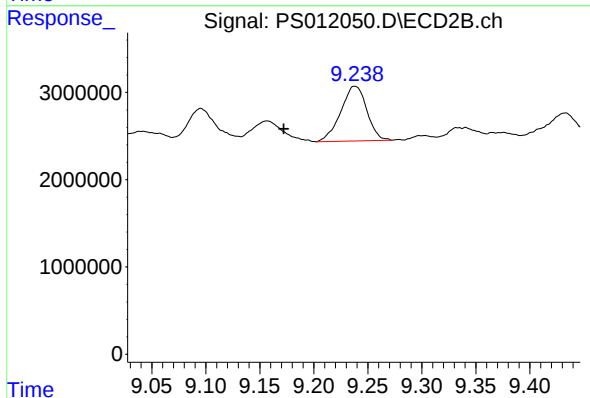


#12 2,4,5-T

R.T.: 9.238 min
Delta R.T.: 0.066 min
Response: 10527615
Conc: 3.56 ng/ml

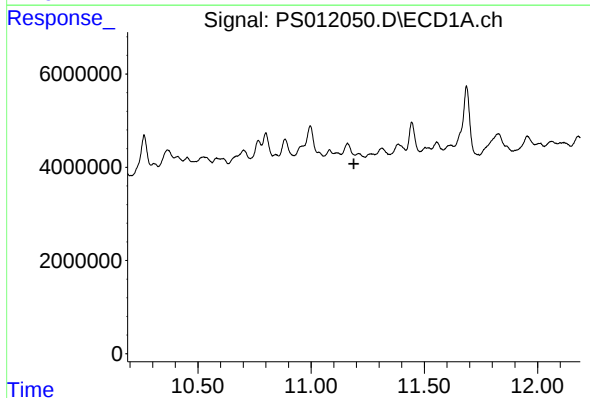


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.189 min
Response: 0
Conc: N.D.

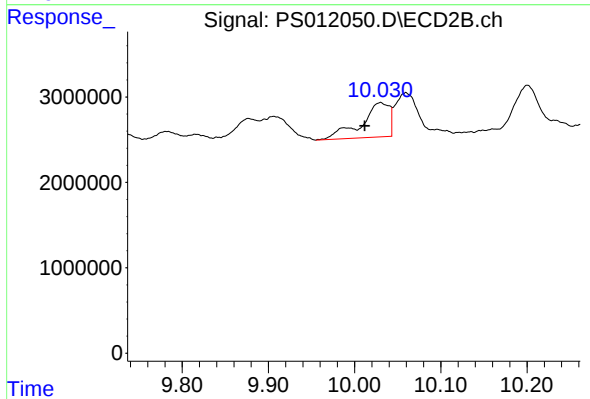

#14 DINOSEB


R.T.: 10.030 min
Delta R.T.: 0.018 min
Response: 8981233
Conc: 4.22 ng/ml

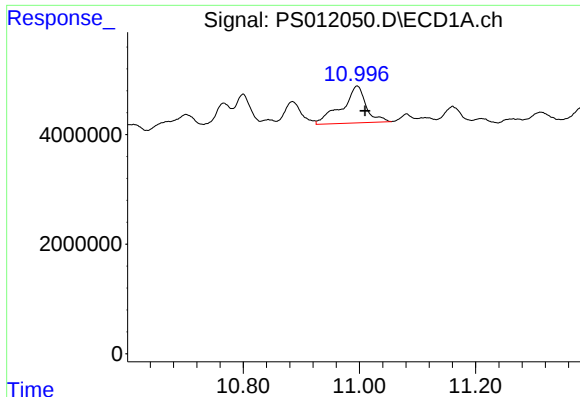

#15 Picloram


R.T.: 10.996 min
Delta R.T.: -0.013 min
Response: 19433560
Conc: 2.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

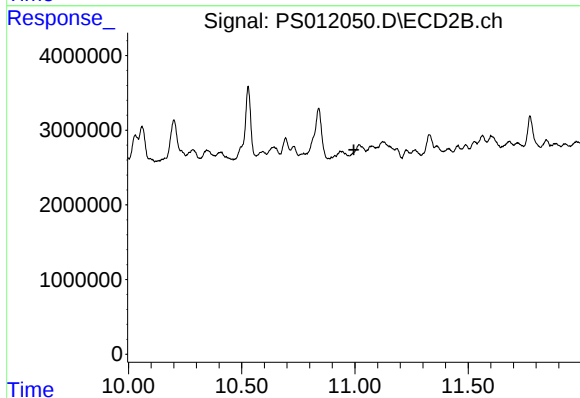


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.

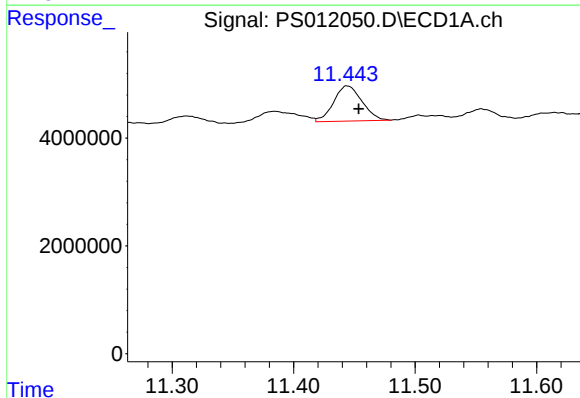

#16 DCPA

R.T.: 11.444 min
Delta R.T.: -0.009 min
Response: 10567476
Conc: 1.39 ng/ml

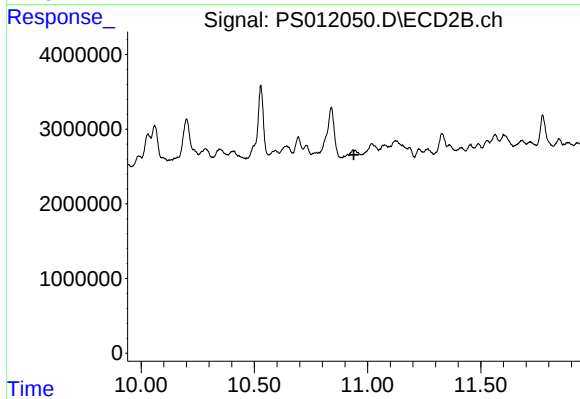

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.940 min
Response: 0
Conc: N.D.