

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
 Data File : PS012051.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2020 18:53
 Operator : DD\AJ
 Sample : L3853-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 05:05:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.218	6.914	271.5E6	174.1E6	248.911	325.498 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.095	0	98593350	N.D.	119.853
3) T	4-Nitroph...	7.054	0.000	5032846	0	8.544	N.D. #
5) T	DICAMBA	7.395	7.075	10019891	11602043	2.446	5.370 #
6) T	MCP	7.629	7.216	13848898	5936801	4.334	3.359
7) T	MCPA	7.685	7.460	225.7E6	152.3E6	49.610	55.569
8) T	DICHLORPROP	0.000	7.734	0	11311632	N.D.	20.033
9) T	2,4-D	8.397	0.000	135.5E6	0	120.043	N.D. #
11) T	2,4,5-TP ...	0.000	8.755	0	14142559	N.D.	4.837
12) T	2,4,5-T	9.412	0.000	53335482	0	9.001	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
Data File : PS012051.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2020 18:53
Operator : DD\AJ
Sample : L3853-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 05:05:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

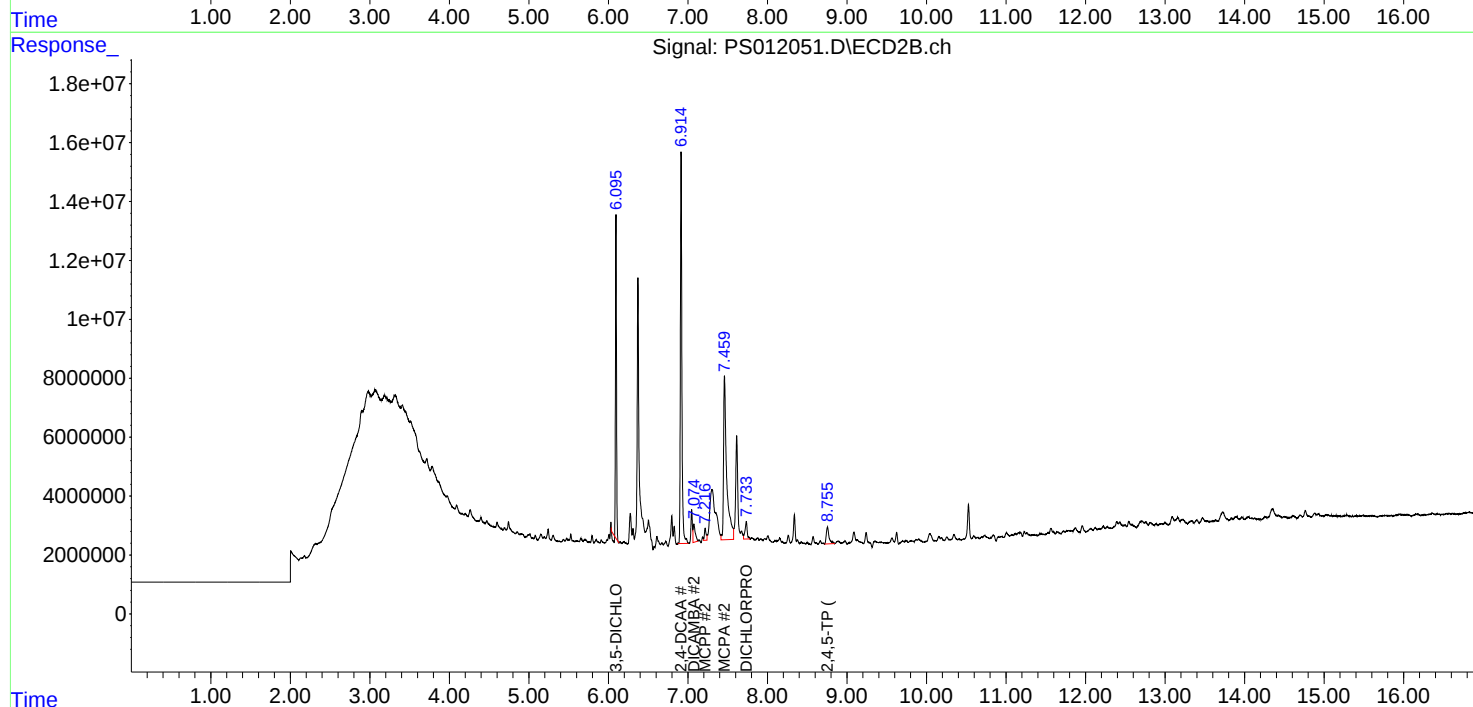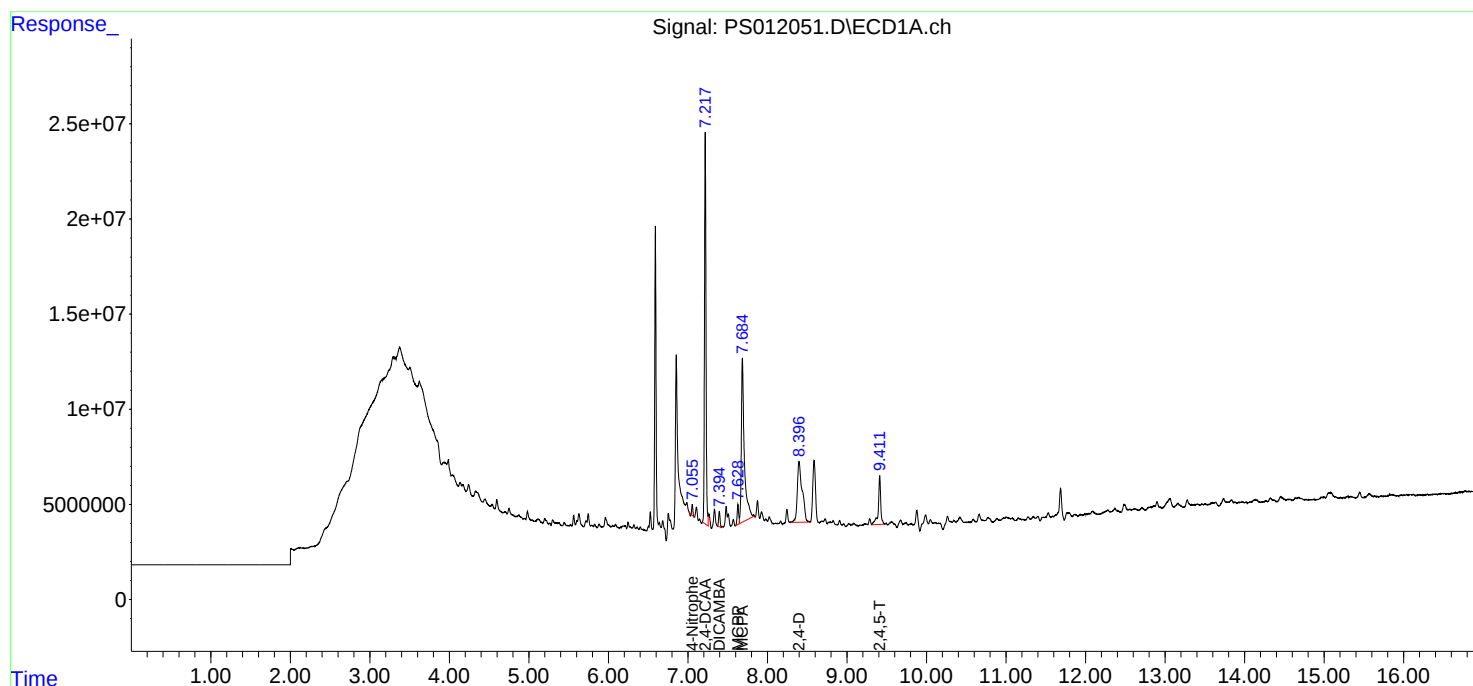


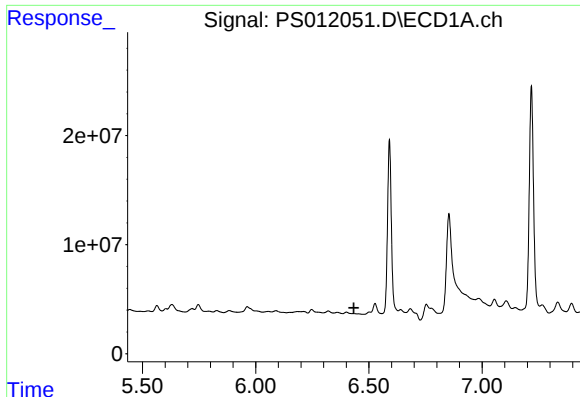

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

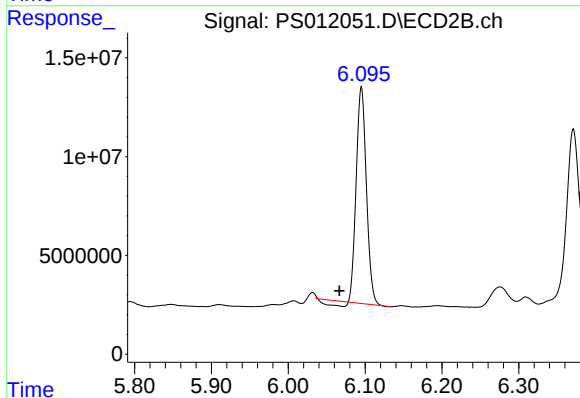


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.029 min
Response: 98593350
Conc: 119.85 ng/ml

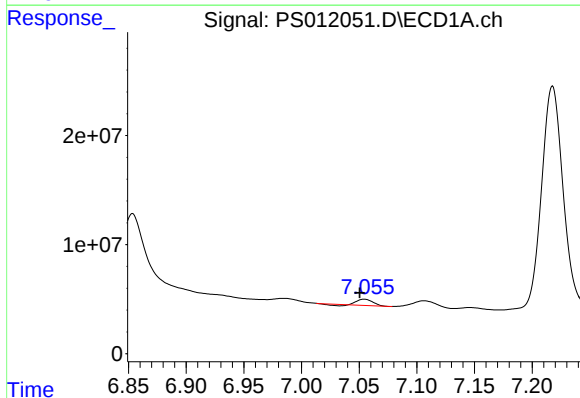


#3 4-Nitrophenol

R.T.: 7.054 min
Delta R.T.: 0.004 min
Response: 5032846
Conc: 8.54 ng/ml

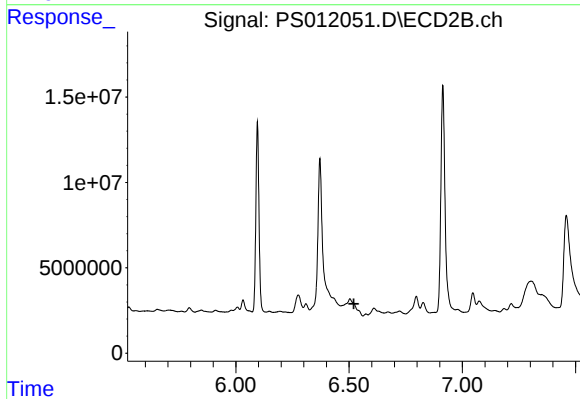

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

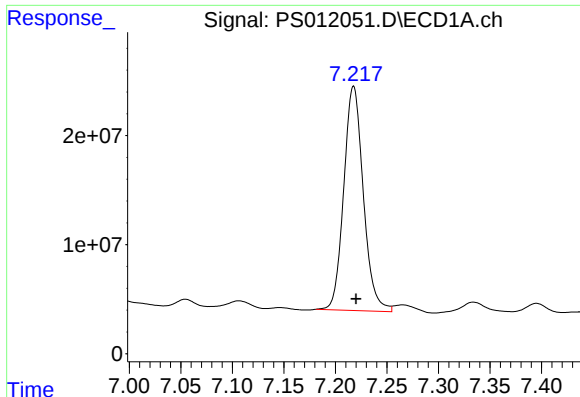

#4 2,4-DCAA


R.T.: 7.218 min
Delta R.T.: -0.002 min
Response: 271504332
Conc: 248.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

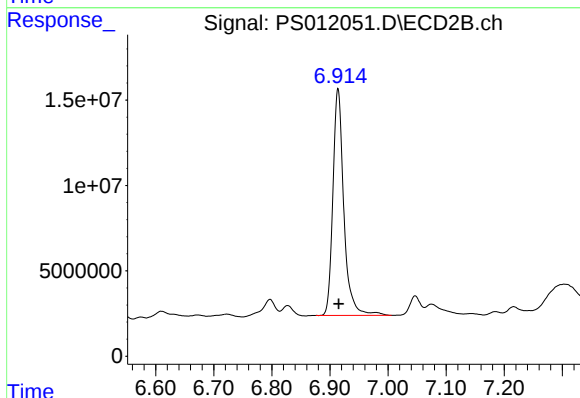


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: -0.001 min
Response: 174071794
Conc: 325.50 ng/ml

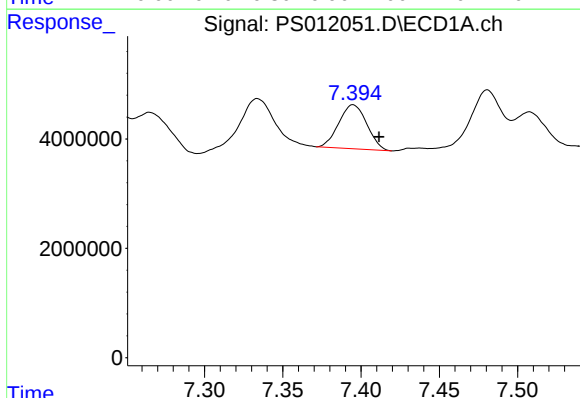


#5 DICAMBA

R.T.: 7.395 min
Delta R.T.: -0.016 min
Response: 10019891
Conc: 2.45 ng/ml

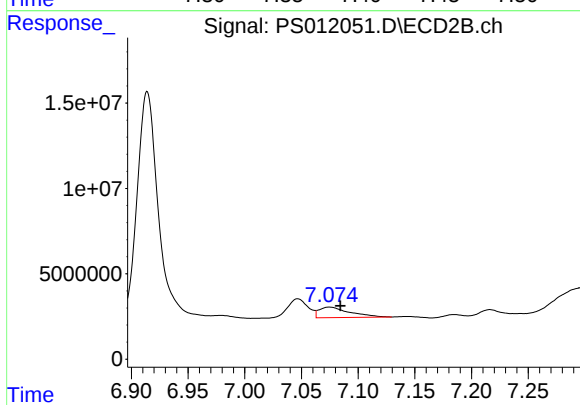

#5 DICAMBA


R.T.: 7.075 min
Delta R.T.: -0.009 min
Response: 11602043
Conc: 5.37 ng/ml

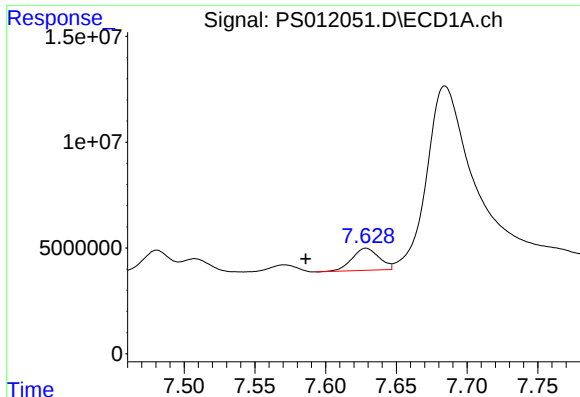

#6 MCP


R.T.: 7.629 min
Delta R.T.: 0.043 min
Response: 13848898
Conc: 4.33 ug/ml

Instrument :
ECD_S
ClientSampleId :

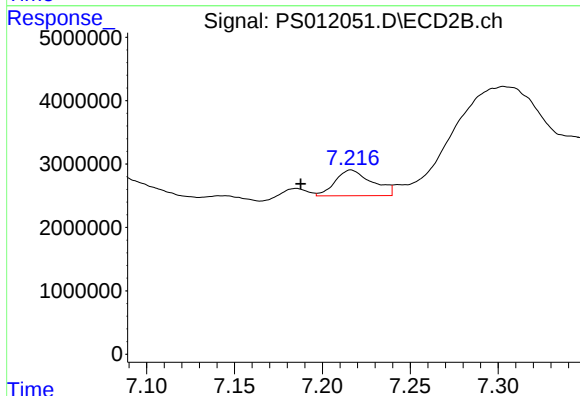


#6 MCP

R.T.: 7.216 min
Delta R.T.: 0.029 min
Response: 5936801
Conc: 3.36 ug/ml

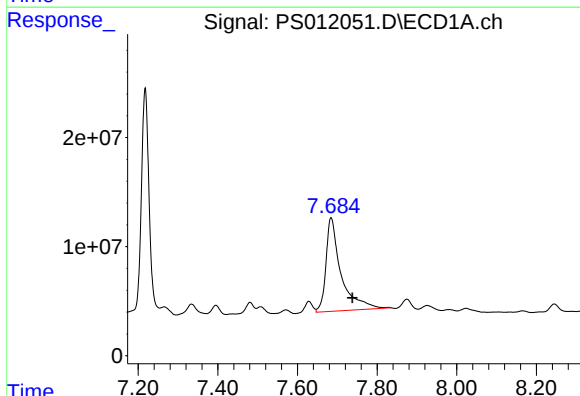


#7 MCPA

R.T.: 7.685 min
Delta R.T.: -0.054 min
Response: 225651633
Conc: 49.61 ug/ml

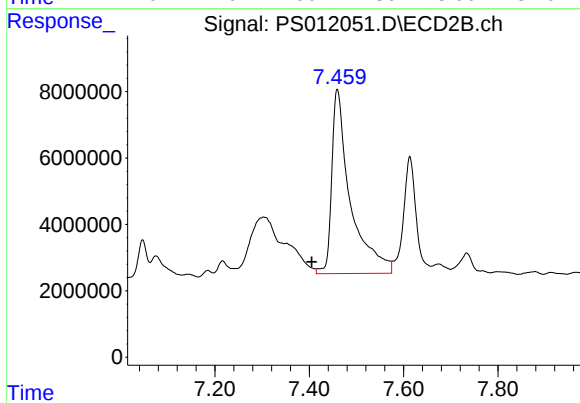

#7 MCPA


R.T.: 7.460 min
Delta R.T.: 0.055 min
Response: 152267849
Conc: 55.57 ug/ml

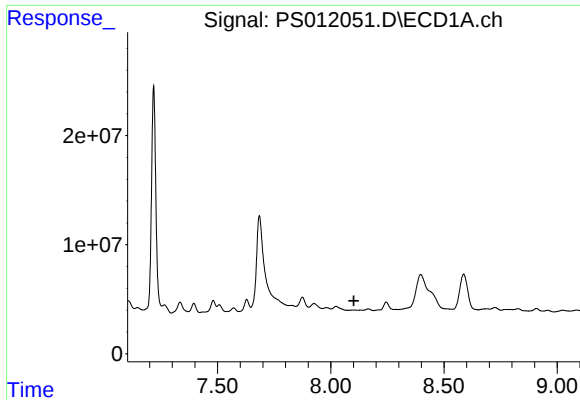

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

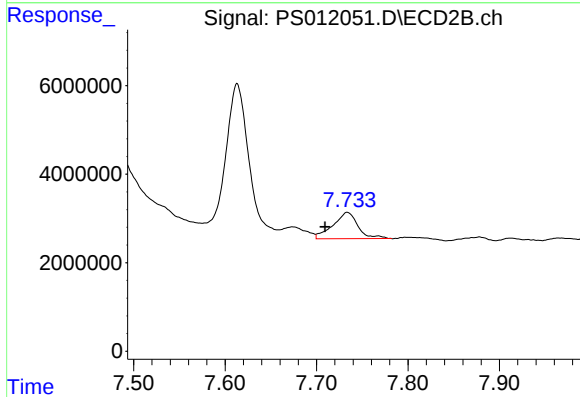


#8 DICHLORPROP

R.T.: 7.734 min
Delta R.T.: 0.024 min
Response: 11311632
Conc: 20.03 ng/ml

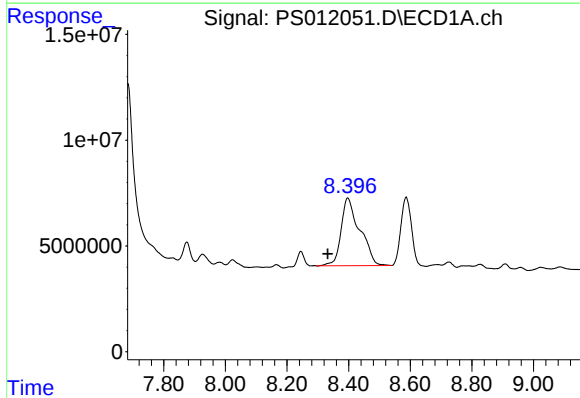


#9 2,4-D

R.T.: 8.397 min
Delta R.T.: 0.065 min
Response: 135539864
Conc: 120.04 ng/ml

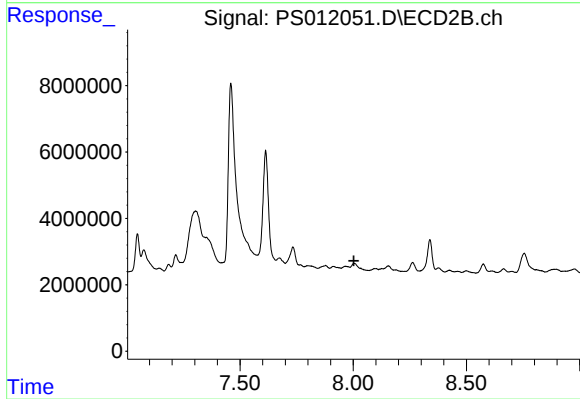

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

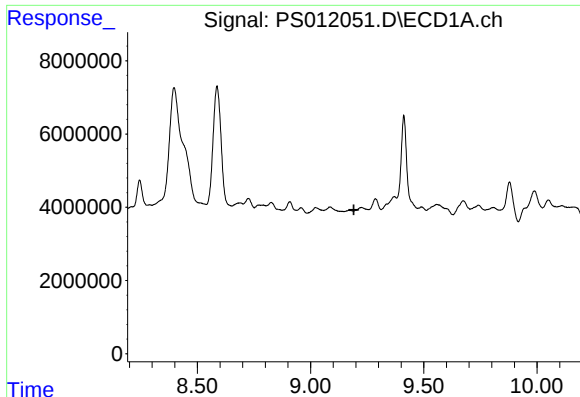

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

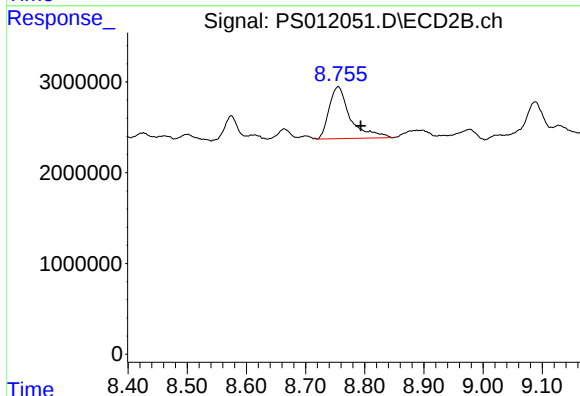


#11 2,4,5-TP (SILVEX)

R.T.: 8.755 min
Delta R.T.: -0.039 min
Response: 14142559
Conc: 4.84 ng/ml

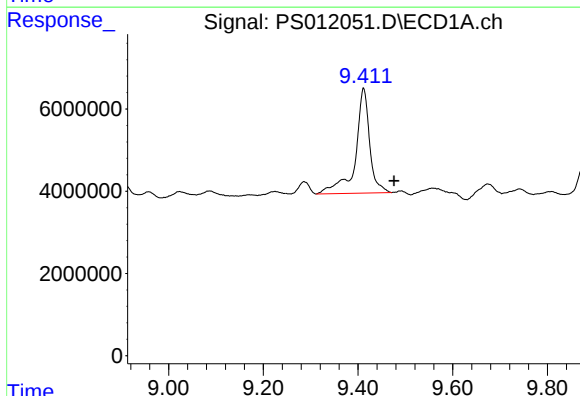

#12 2,4,5-T

R.T.: 9.412 min
Delta R.T.: -0.064 min
Response: 53335482
Conc: 9.00 ng/ml

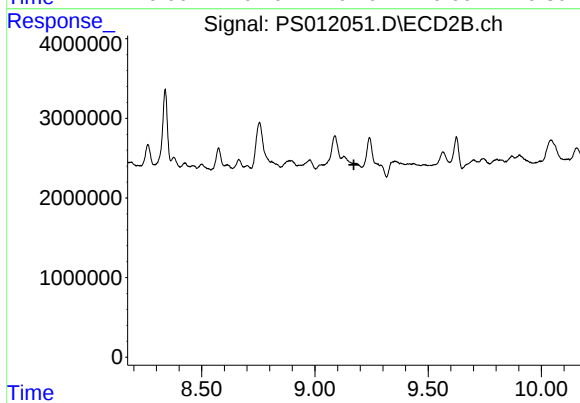

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.