

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
 Data File : PS012053.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2020 19:39
 Operator : DD\AJ
 Sample : PB131375BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 05:06:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	496.1E6	293.5E6	454.827	548.891
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	90955290	N.D.	110.568
3) T	4-Nitroph...	7.056	0.000	2262830	0	3.842	N.D. #
5) T	DICAMBA	7.396	7.049	11683065	10831533	2.852	5.013 #
6) T	MCP	7.630	0.000	12585454	0	3.939	N.D. #
7) T	MCPA	7.764	7.375	27160095	34195442	5.971	12.479 #
9) T	2,4-D	8.399	0.000	142.6E6	0	126.255	N.D. #
12) T	2,4,5-T	9.413	0.000	19460042	0	3.284	N.D. #
16) T	DCPA	11.522	0.000	32302019	0	4.248	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
Data File : PS012053.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2020 19:39
Operator : DD\AJ
Sample : PB131375BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 05:06:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

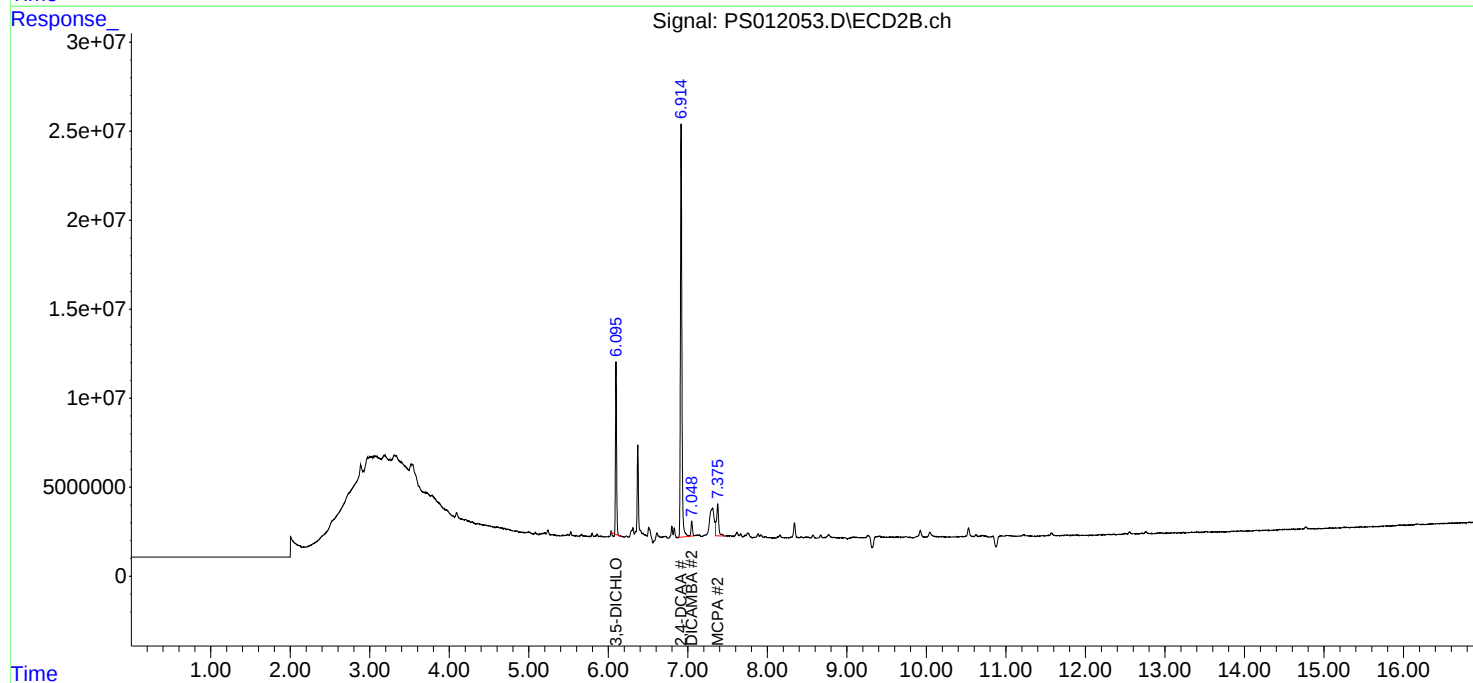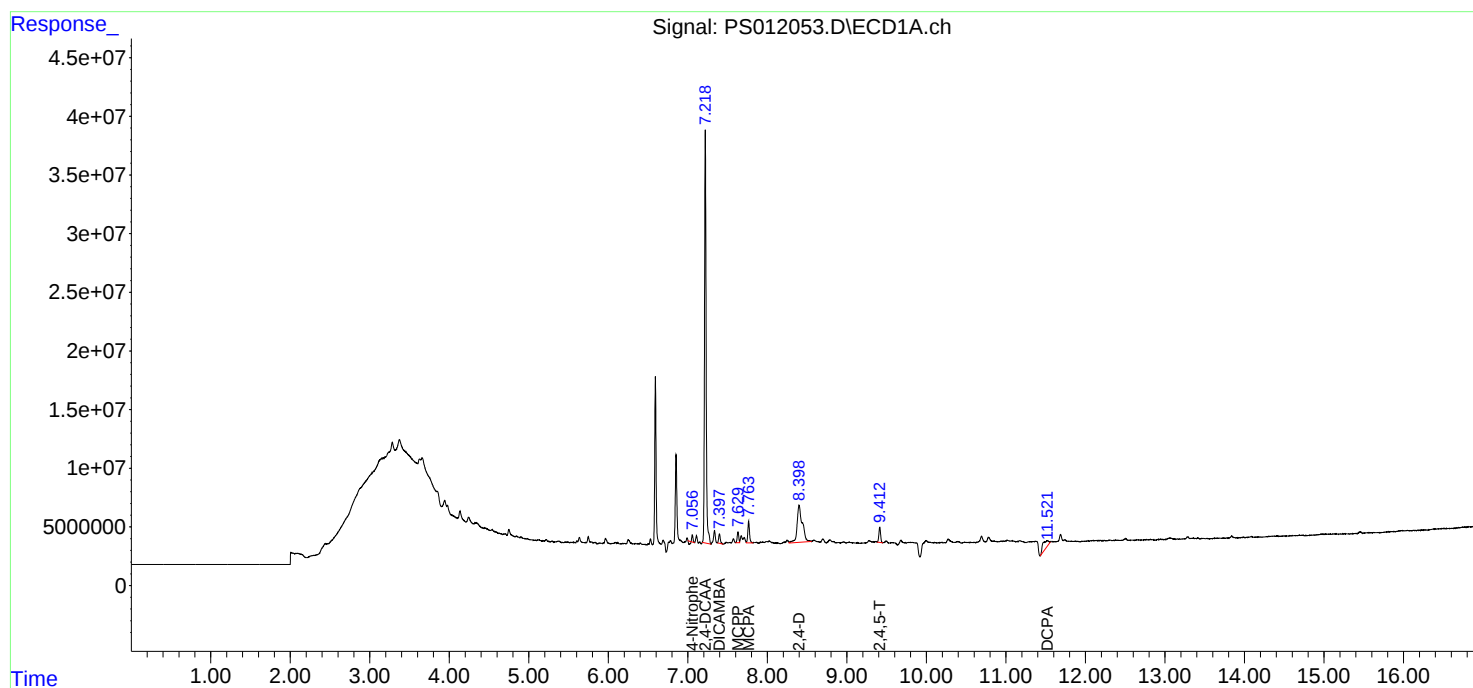


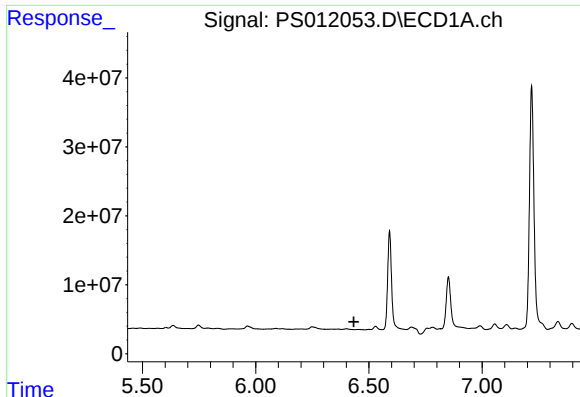

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

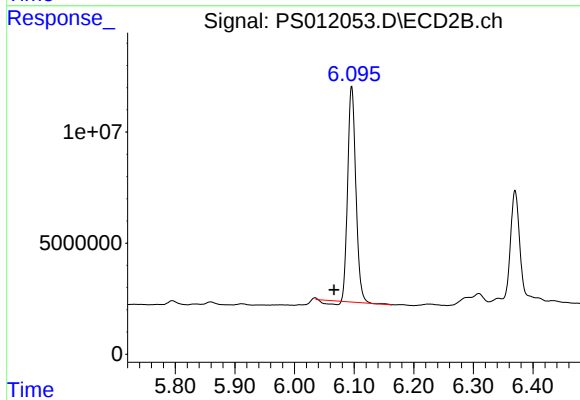


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 90955290
Conc: 110.57 ng/ml

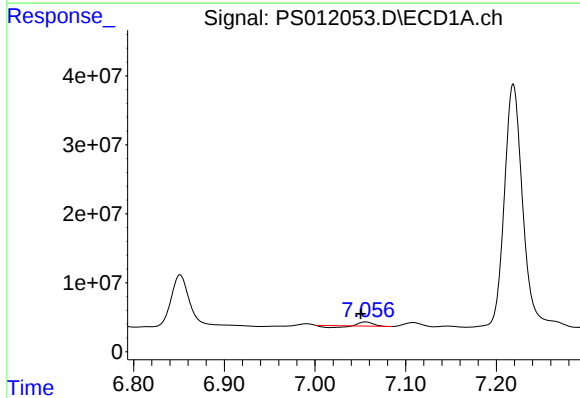


#3 4-Nitrophenol

R.T.: 7.056 min
Delta R.T.: 0.005 min
Response: 2262830
Conc: 3.84 ng/ml

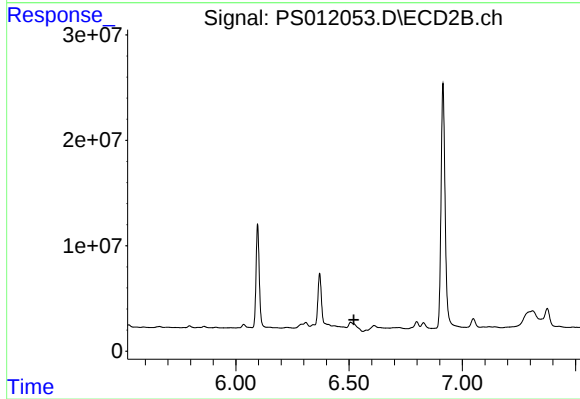

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

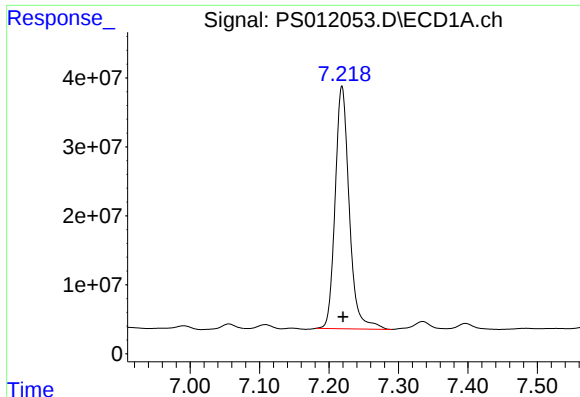

#4 2,4-DCAA


R.T.: 7.219 min
Delta R.T.: -0.001 min
Response: 496111148
Conc: 454.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

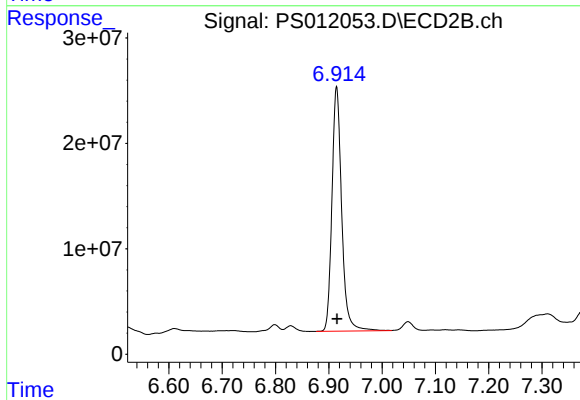


#4 2,4-DCAA

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 293539526
Conc: 548.89 ng/ml

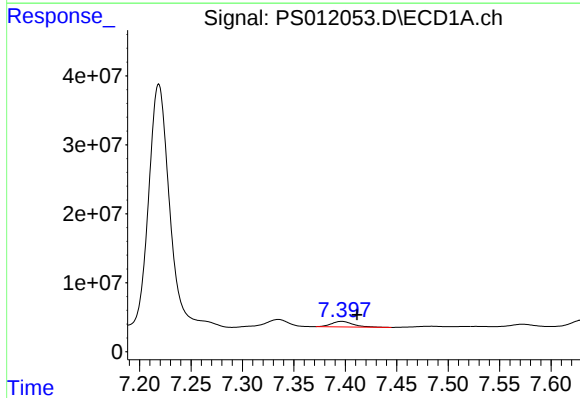


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.015 min
Response: 11683065
Conc: 2.85 ng/ml

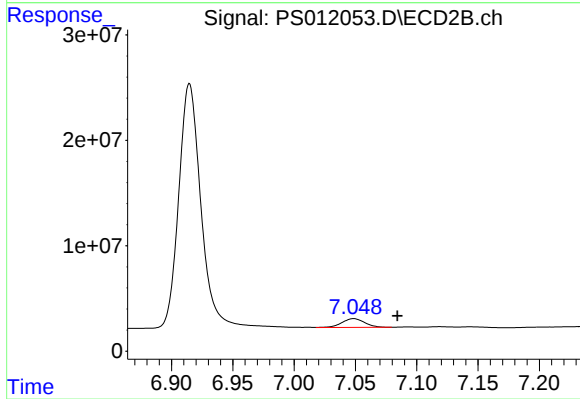

#5 DICAMBA


R.T.: 7.049 min
Delta R.T.: -0.036 min
Response: 10831533
Conc: 5.01 ng/ml

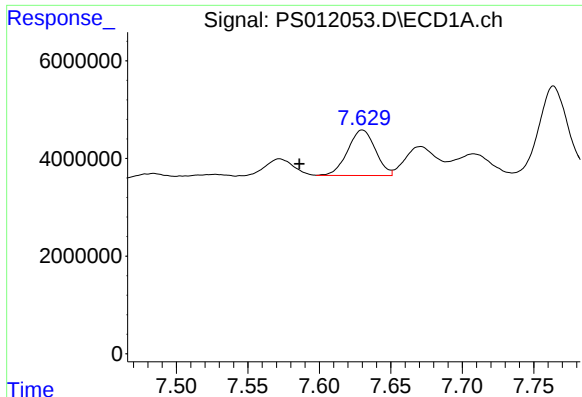

#6 MCP


R.T.: 7.630 min
Delta R.T.: 0.044 min
Response: 12585454
Conc: 3.94 ug/ml

Instrument :
ECD_S
ClientSampleId :

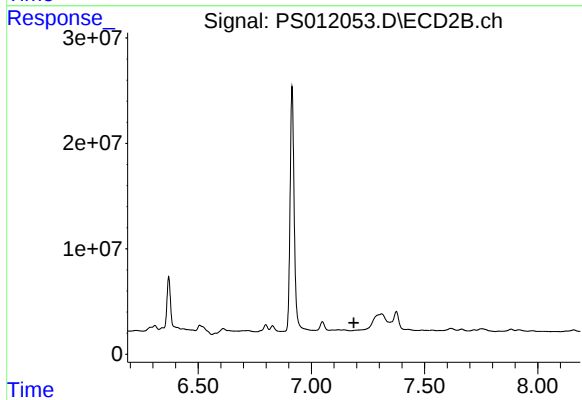


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

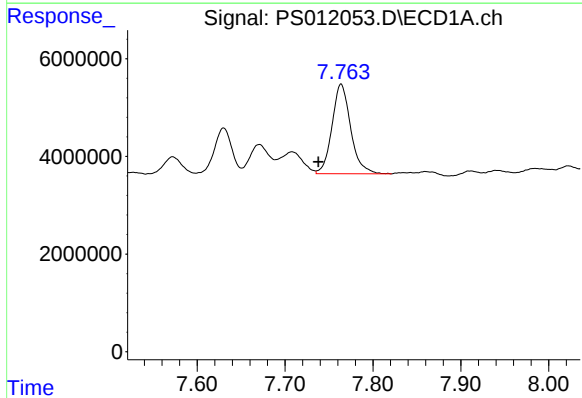


#7 MCP

R.T.: 7.764 min
Delta R.T.: 0.026 min
Response: 27160095
Conc: 5.97 ug/ml

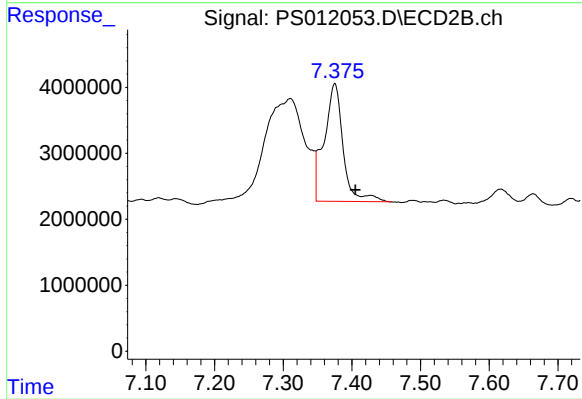

#7 MCP


R.T.: 7.375 min
Delta R.T.: -0.030 min
Response: 34195442
Conc: 12.48 ug/ml

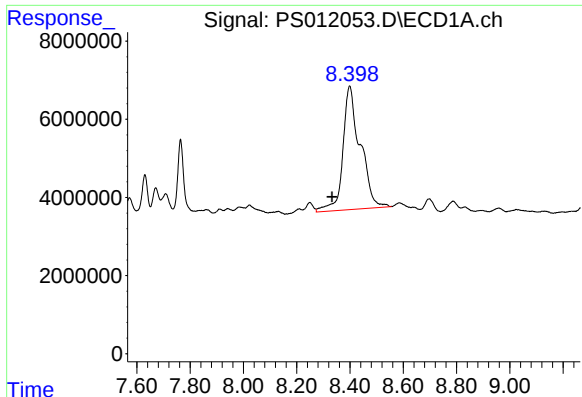

#9 2,4-D


R.T.: 8.399 min
Delta R.T.: 0.067 min
Response: 142553098
Conc: 126.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

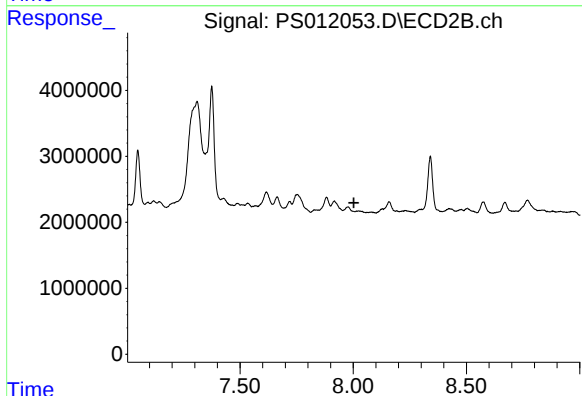


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

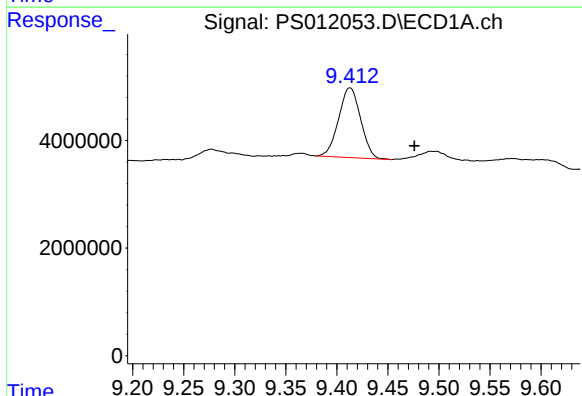


#12 2,4,5-T

R.T.: 9.413 min
Delta R.T.: -0.063 min
Response: 19460042
Conc: 3.28 ng/ml

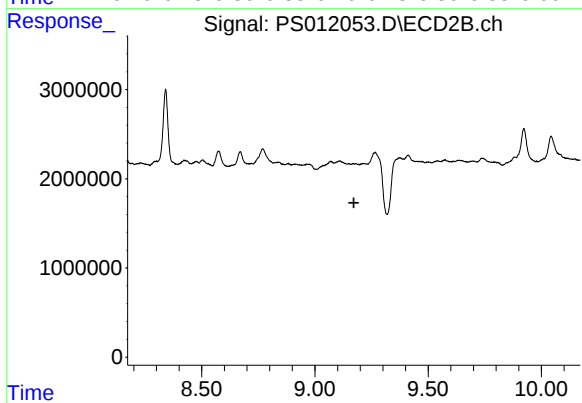

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

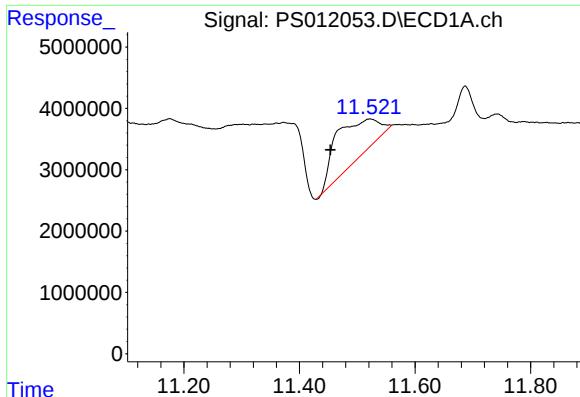

#16 DCPA

R.T.: 11.522 min
Delta R.T.: 0.068 min
Response: 32302019
Conc: 4.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

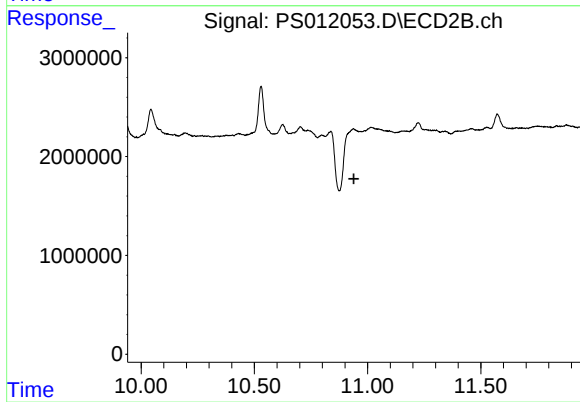

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.940 min
Response: 0
Conc: N.D.