

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
 Data File : PS012057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2020 21:11
 Operator : DD\AJ
 Sample : PB131375TB
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 05:08:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	246.6E6	154.5E6	226.098	288.918 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	90922891	N.D.	110.528
3) T	4-Nitroph...	7.055	0.000	3571746	0	6.064	N.D. #
5) T	DICAMBA	7.396	7.048	8687905	9976578	2.121	4.618 #
6) T	MCP	7.571	0.000	8182544	0	2.561	N.D. #
7) T	MCPA	7.696	7.401	163.5E6	5767857	35.944	2.105 #
9) T	2,4-D	8.399	7.942	132.1E6	55164973	117.014	75.089 #
12) T	2,4,5-T	9.410	9.242	33833798	22586880	5.710	7.630 #
15) T	Picloram	11.031	11.015	45912913	32556370	5.875	7.183



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
Data File : PS012057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2020 21:11
Operator : DD\AJ
Sample : PB131375TB
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 05:08:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

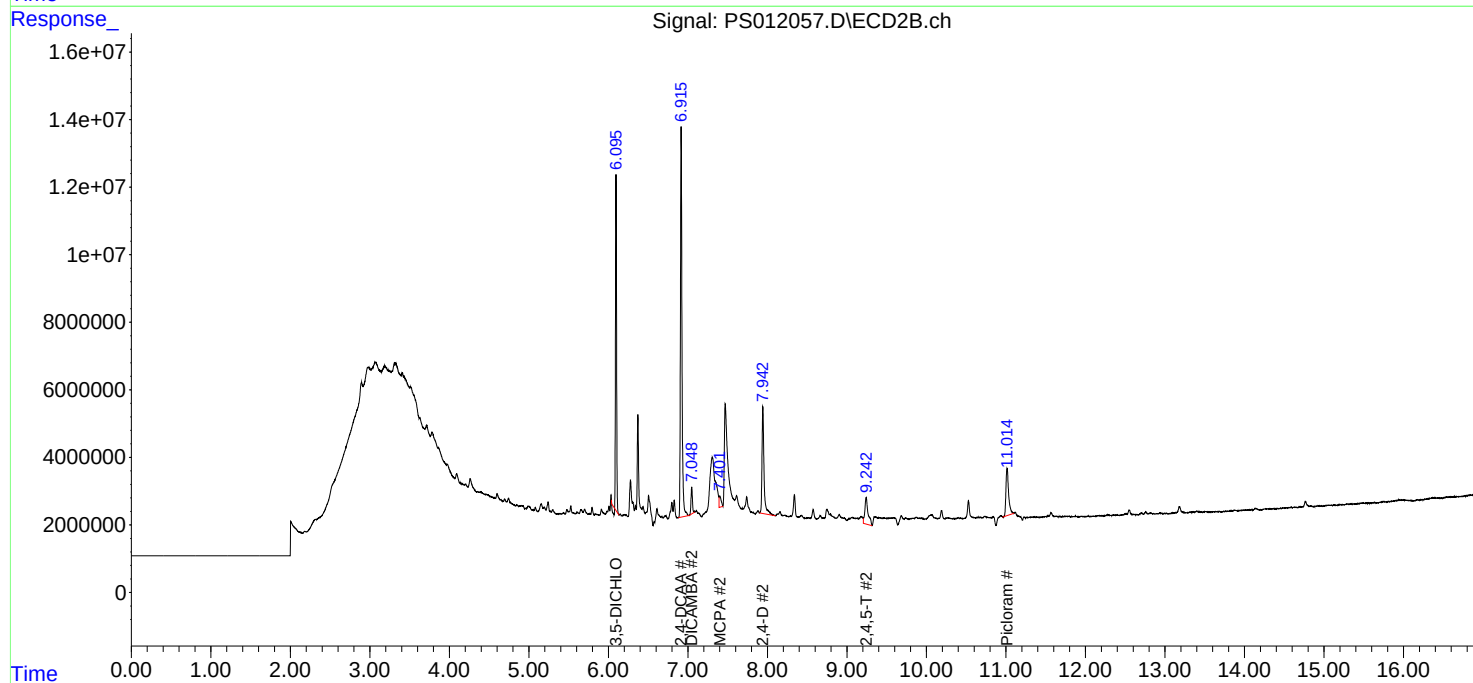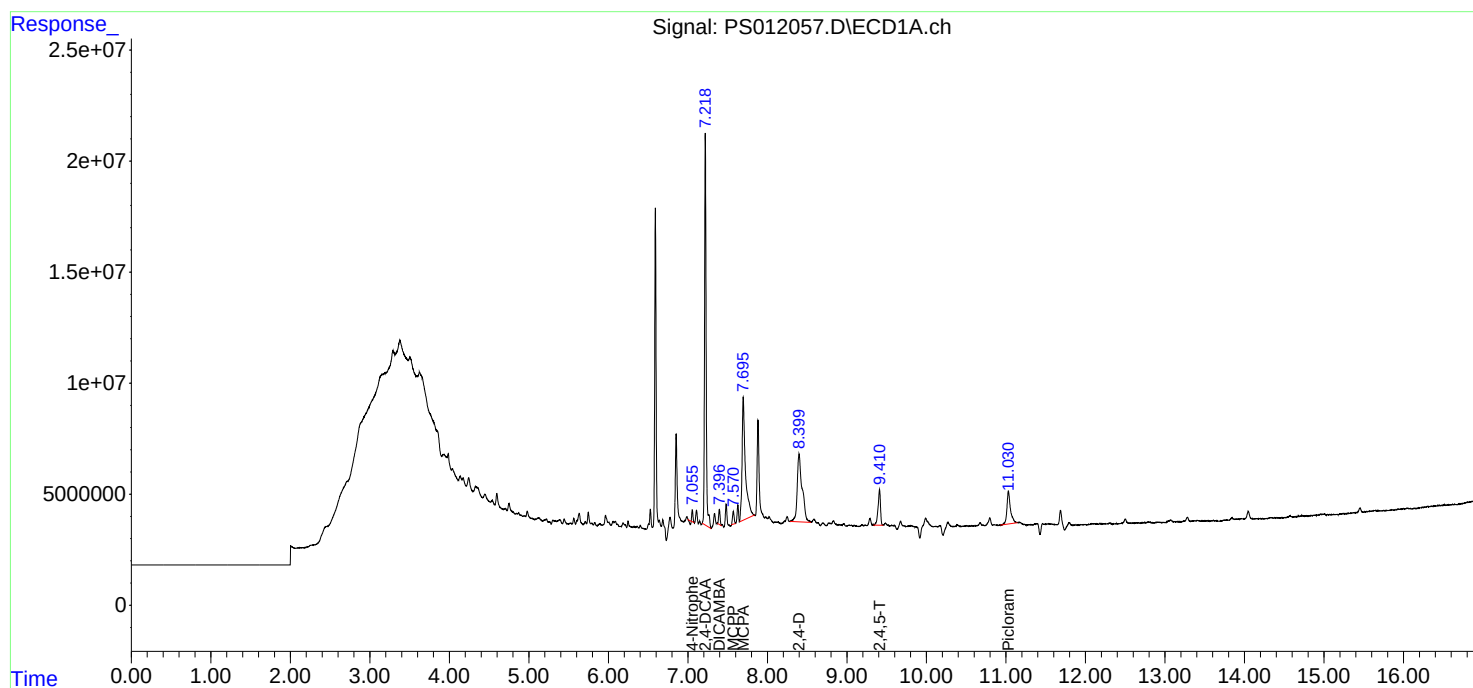


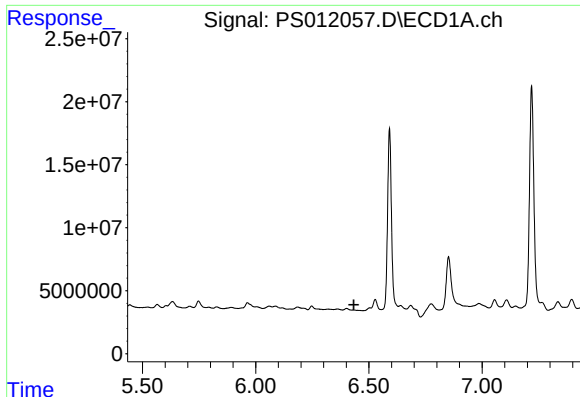

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

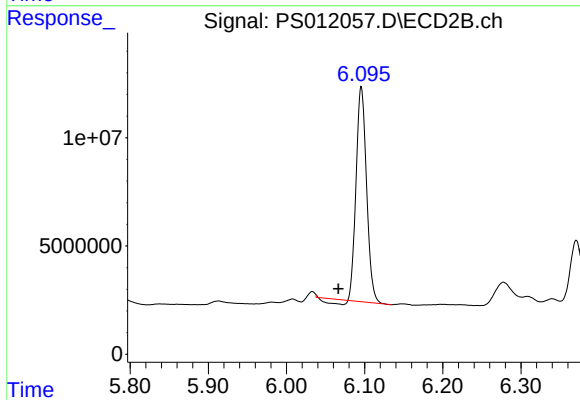


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 90922891
Conc: 110.53 ng/ml

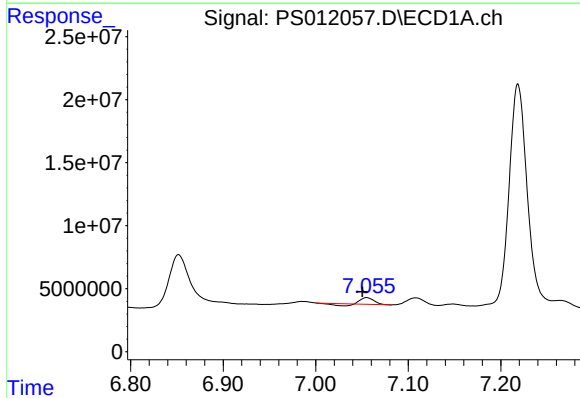


#3 4-Nitrophenol

R.T.: 7.055 min
Delta R.T.: 0.005 min
Response: 3571746
Conc: 6.06 ng/ml

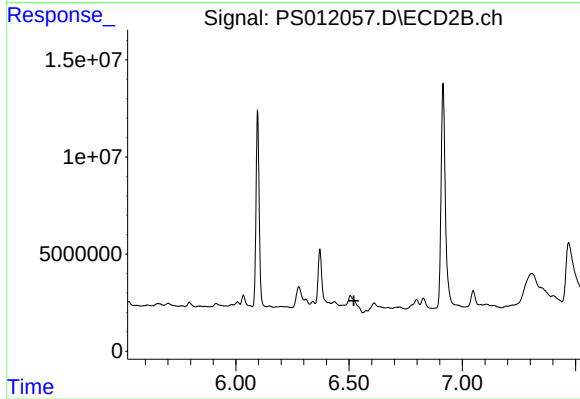

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

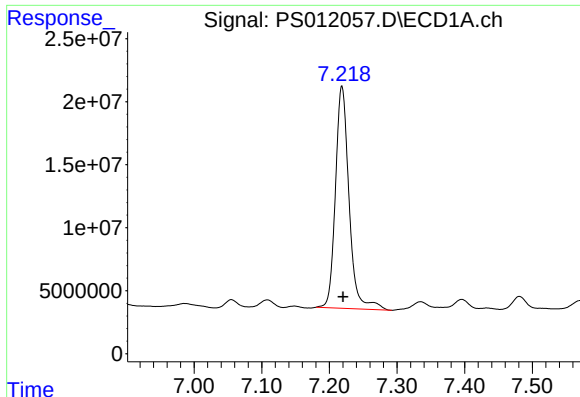

#4 2,4-DCAA


R.T.: 7.219 min
Delta R.T.: -0.001 min
Response: 246620778
Conc: 226.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

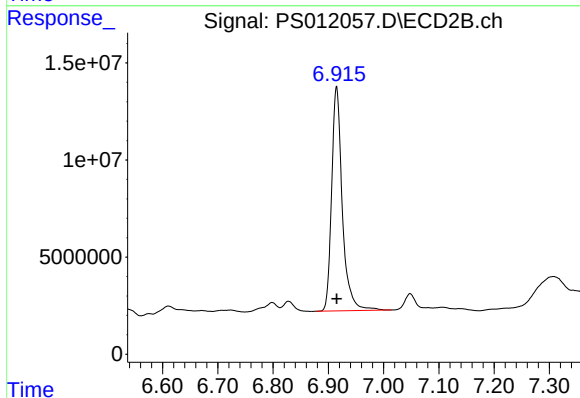


#4 2,4-DCAA

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 154509645
Conc: 288.92 ng/ml

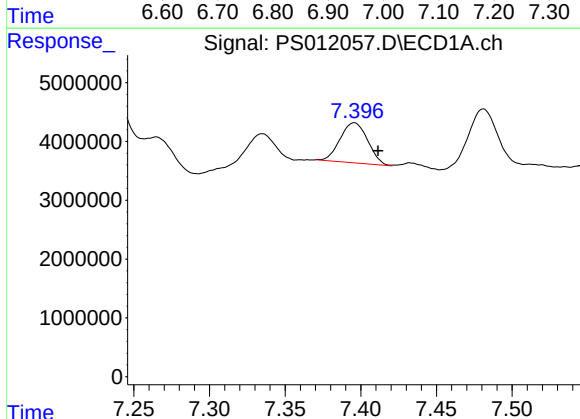


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.016 min
Response: 8687905
Conc: 2.12 ng/ml

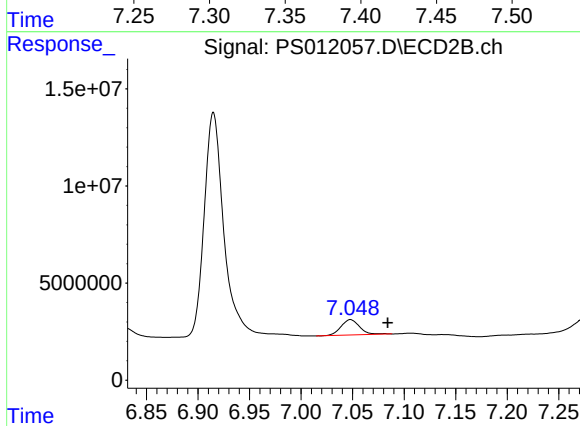

#5 DICAMBA


R.T.: 7.048 min
Delta R.T.: -0.036 min
Response: 9976578
Conc: 4.62 ng/ml

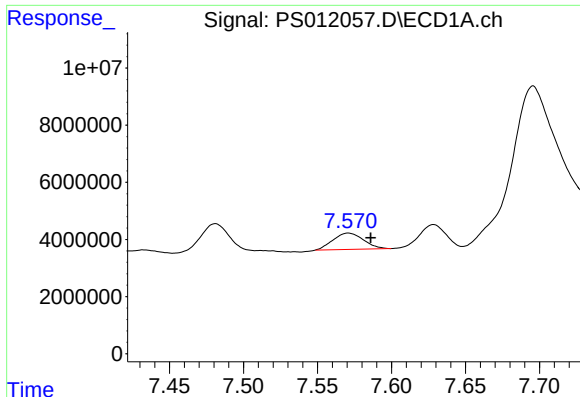

#6 MCP


R.T.: 7.571 min
Delta R.T.: -0.015 min
Response: 8182544
Conc: 2.56 ug/ml

Instrument :
ECD_S
ClientSampleId :

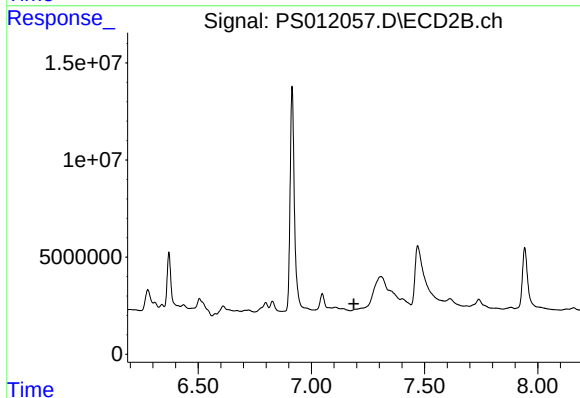


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

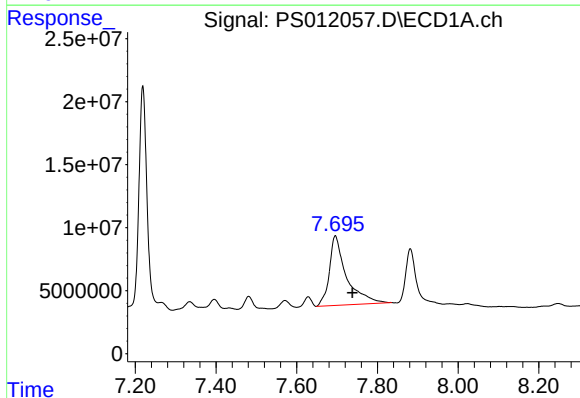


#7 MCP

R.T.: 7.696 min
Delta R.T.: -0.042 min
Response: 163489726
Conc: 35.94 ug/ml

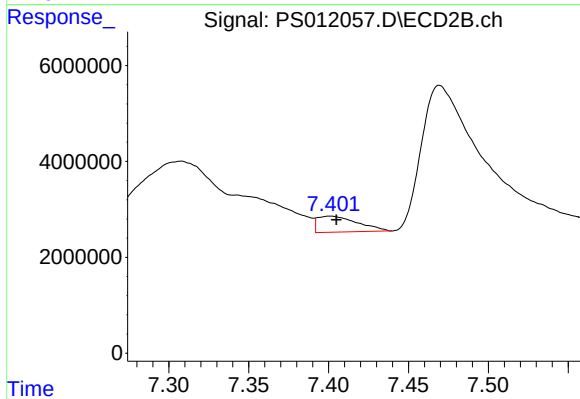

#7 MCP


R.T.: 7.401 min
Delta R.T.: -0.004 min
Response: 5767857
Conc: 2.10 ug/ml

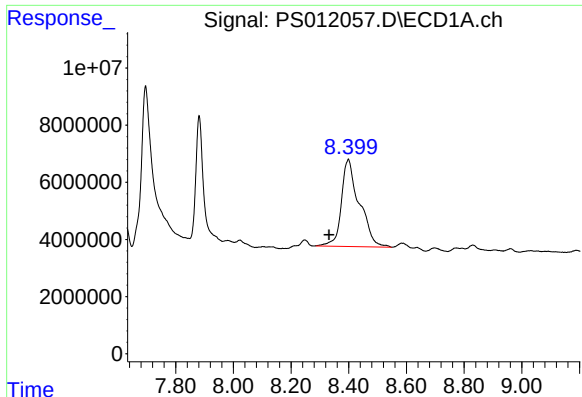

#9 2,4-D


R.T.: 8.399 min
Delta R.T.: 0.066 min
Response: 132119905
Conc: 117.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

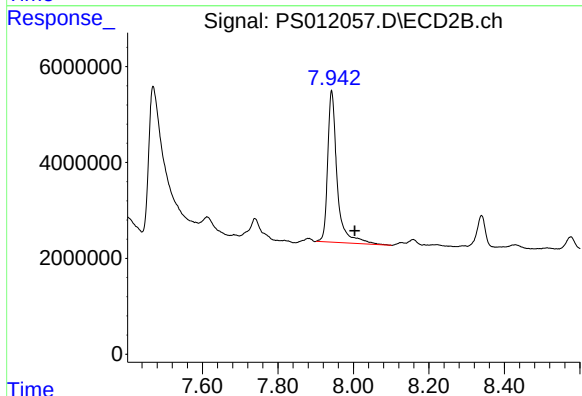


#9 2,4-D

R.T.: 7.942 min
Delta R.T.: -0.061 min
Response: 55164973
Conc: 75.09 ng/ml

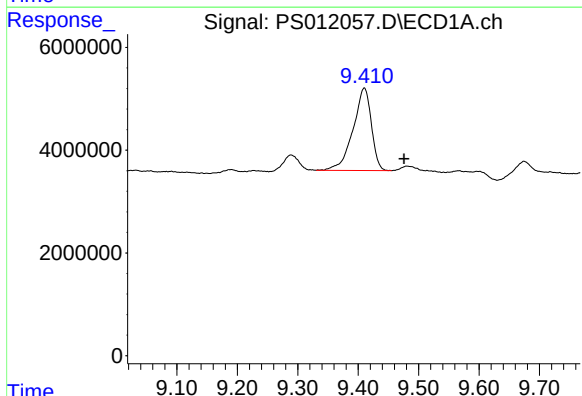


#12 2,4,5-T

R.T.: 9.410 min
Delta R.T.: -0.066 min
Response: 33833798
Conc: 5.71 ng/ml

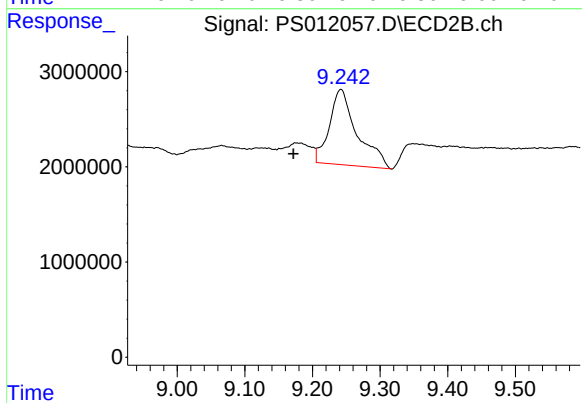

#12 2,4,5-T


R.T.: 9.242 min
Delta R.T.: 0.070 min
Response: 22586880
Conc: 7.63 ng/ml

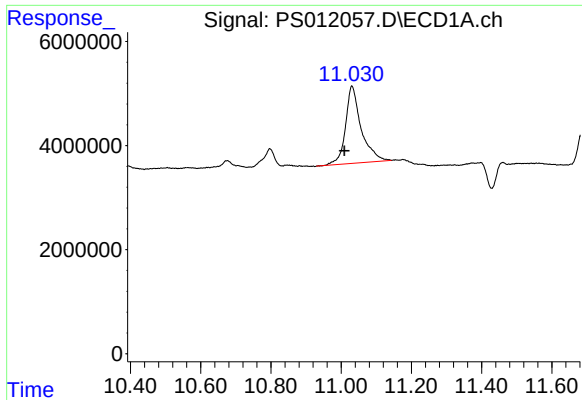

#15 Picloram

R.T.: 11.031 min
Delta R.T.: 0.021 min
Response: 45912913
Conc: 5.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

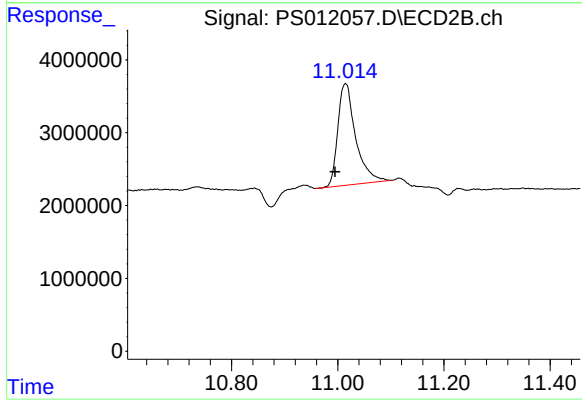

#15 Picloram

R.T.: 11.015 min
Delta R.T.: 0.019 min
Response: 32556370
Conc: 7.18 ng/ml