

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
 Data File : PS012062.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2020 23:06
 Operator : DD\AJ
 Sample : L3837-05
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 05:10:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	224.7E6	138.7E6	205.982	259.370 #
Target Compounds							
1) T	Dalapon	2.996	2.585	35874098	59292721	28.799	78.445 #
2) T	3,5-DICHL...	0.000	6.096	0	74886257	N.D.	91.034
3) T	4-Nitroph...	7.108	0.000	6539209	0	11.101	N.D. #
5) T	DICAMBA	7.395	7.048	7426301	9430959	1.813	4.365 #
6) T	MCPD	7.571	0.000	7399064	0	2.316	N.D. #
7) T	MCPA	7.696	7.470	208.6E6	132.2E6	45.869	48.249
9) T	2,4-D	8.397	0.000	118.4E6	0	104.871	N.D. #
10) T	Pentachlo...	8.694	0.000	17298528	0	1.203	N.D. #
11) T	2,4,5-TP ...	0.000	8.792	0	41357988	N.D.	14.146
12) T	2,4,5-T	9.412	0.000	42052760	0	7.097	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
Data File : PS012062.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2020 23:06
Operator : DD\AJ
Sample : L3837-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 05:10:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

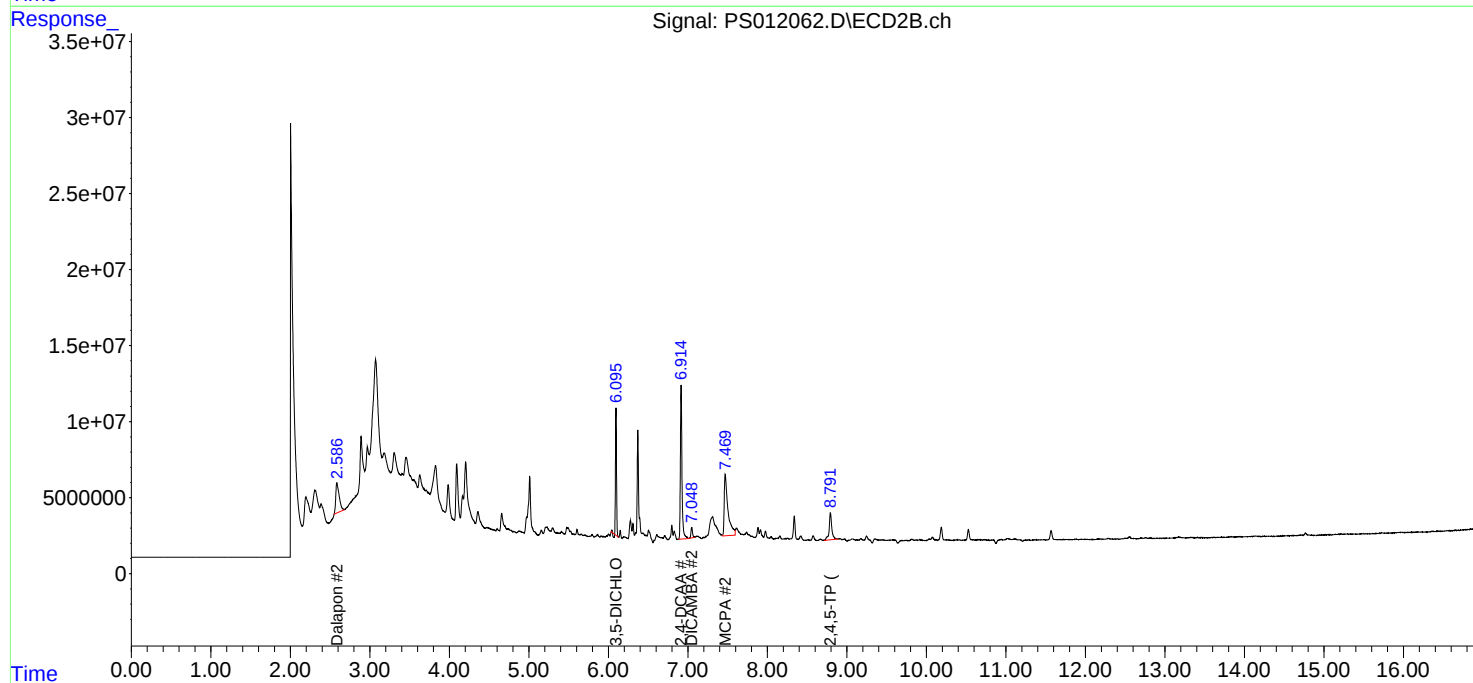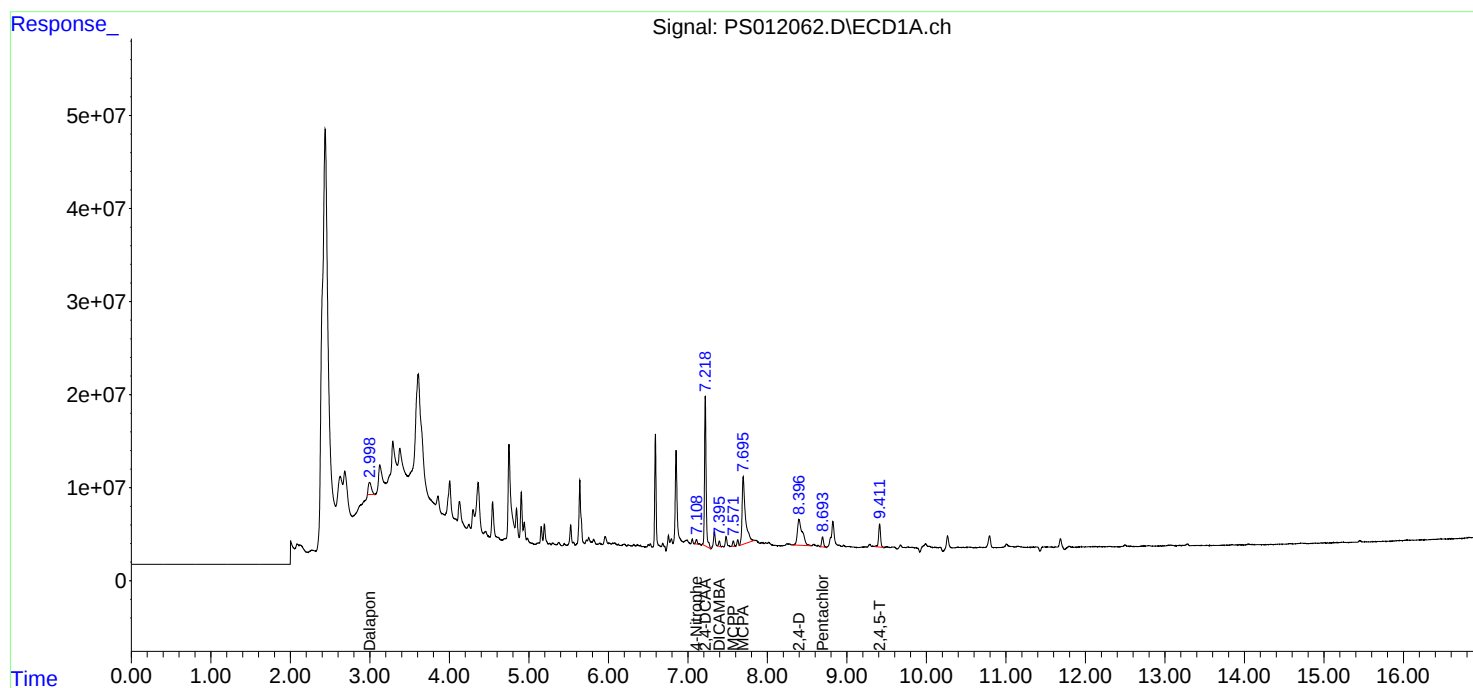


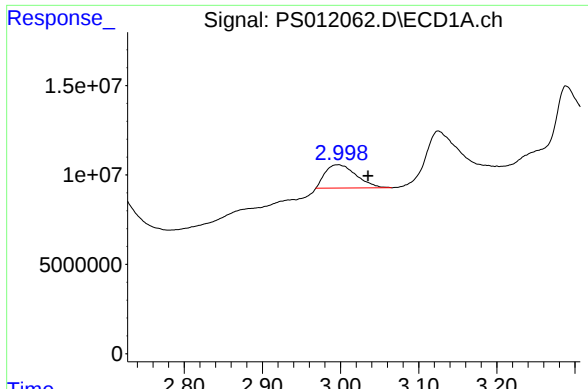

#1 Dalapon


R.T.: 2.996 min
Delta R.T.: -0.039 min
Response: 35874098
Conc: 28.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

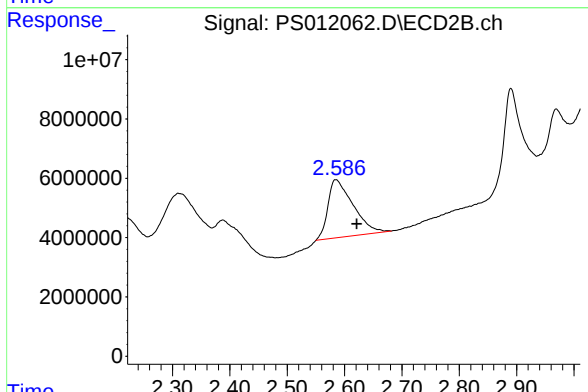


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: -0.036 min
Response: 59292721
Conc: 78.45 ng/ml

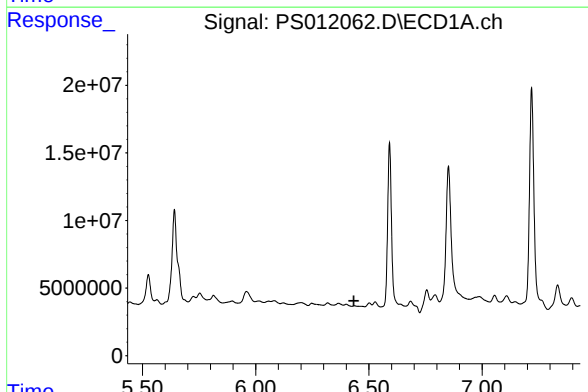


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

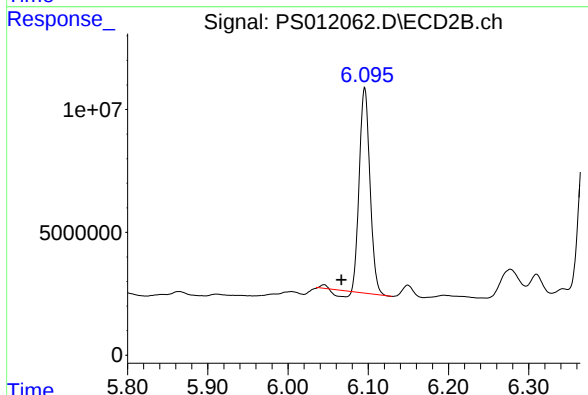

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 74886257
Conc: 91.03 ng/ml

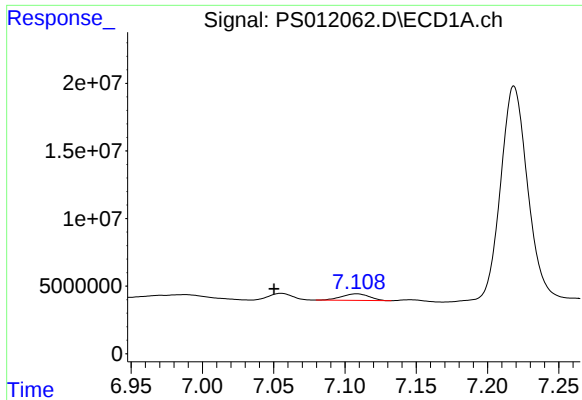

#3 4-Nitrophenol


R.T.: 7.108 min
Delta R.T.: 0.058 min
Response: 6539209
Conc: 11.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

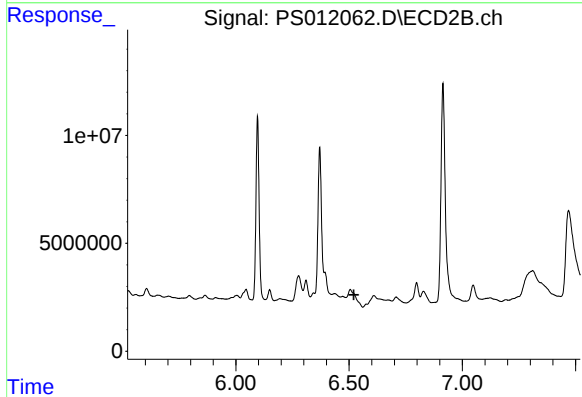


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.521 min
Response: 0
Conc: N.D.

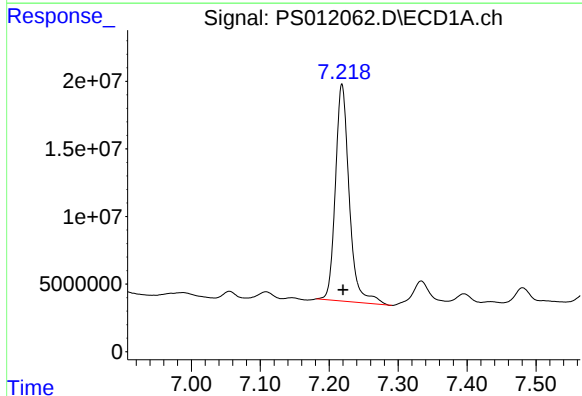


#4 2,4-DCAA

R.T.: 7.219 min
Delta R.T.: -0.001 min
Response: 224678206
Conc: 205.98 ng/ml

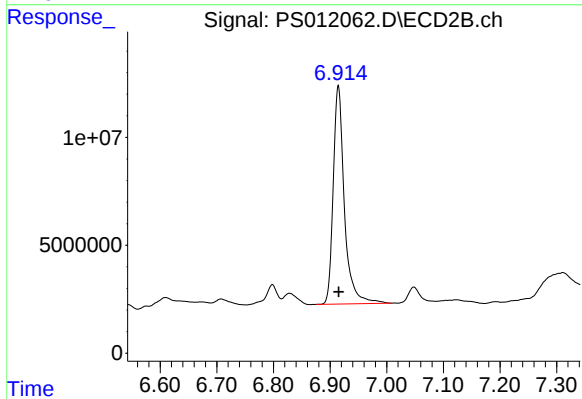

#4 2,4-DCAA


R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 138707748
Conc: 259.37 ng/ml

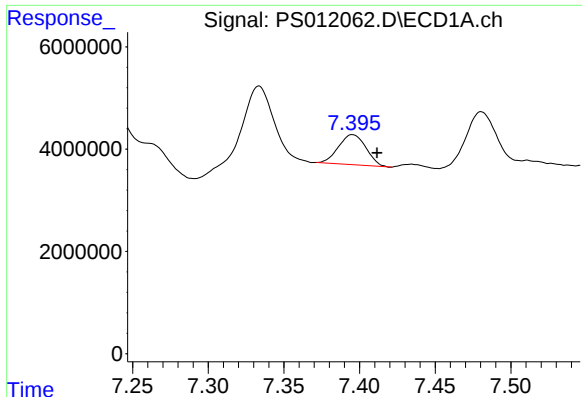

#5 DICAMBA


R.T.: 7.395 min
Delta R.T.: -0.016 min
Response: 7426301
Conc: 1.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

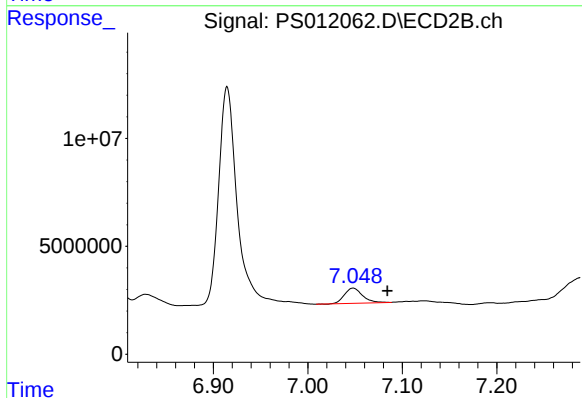


#5 DICAMBA

R.T.: 7.048 min
Delta R.T.: -0.036 min
Response: 9430959
Conc: 4.37 ng/ml

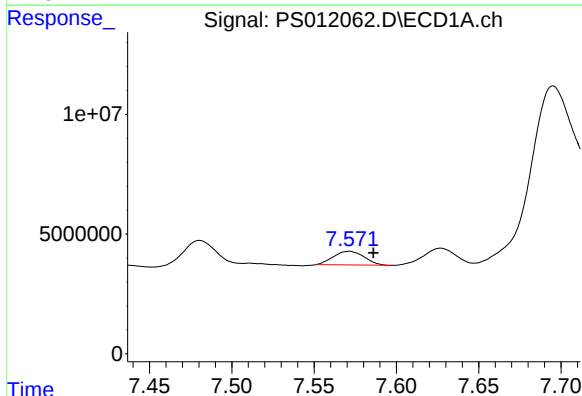


#6 MCP

R.T.: 7.571 min
Delta R.T.: -0.015 min
Response: 7399064
Conc: 2.32 ug/ml

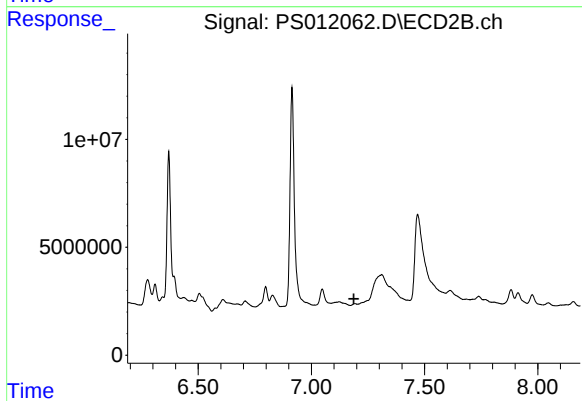

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

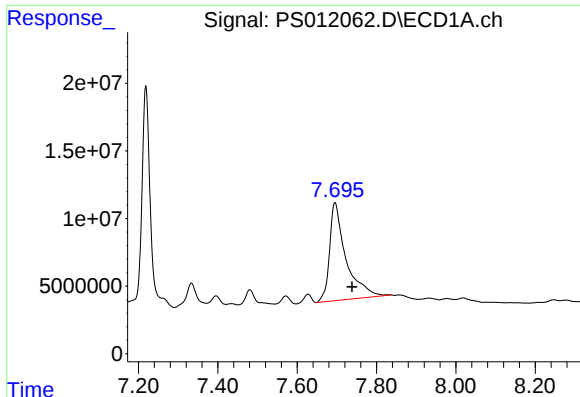

#7 MCPA


R.T.: 7.696 min
Delta R.T.: -0.043 min
Response: 208632520
Conc: 45.87 ug/ml

Instrument :
ECD_S
ClientSampleId :

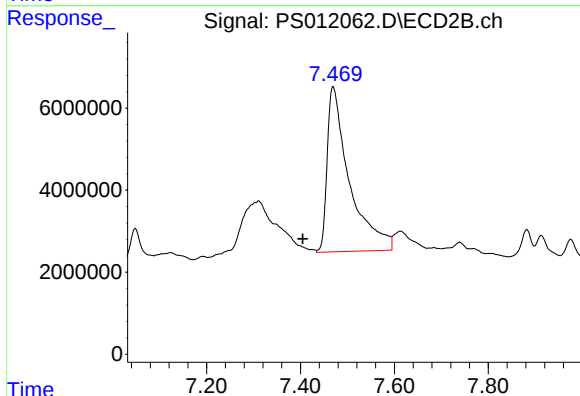


#7 MCPA

R.T.: 7.470 min
Delta R.T.: 0.065 min
Response: 132208674
Conc: 48.25 ug/ml

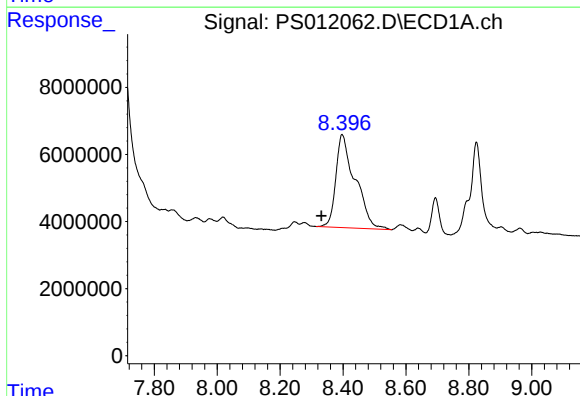


#9 2,4-D

R.T.: 8.397 min
Delta R.T.: 0.065 min
Response: 118409586
Conc: 104.87 ng/ml

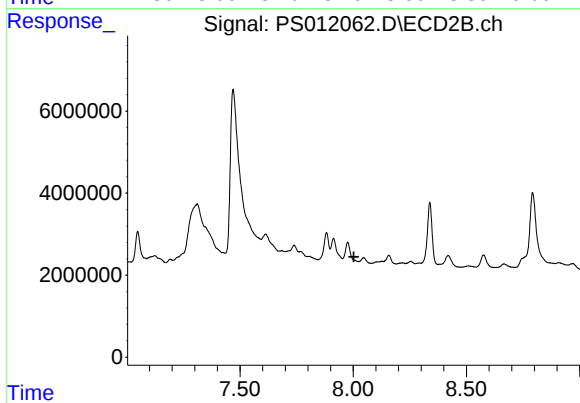

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

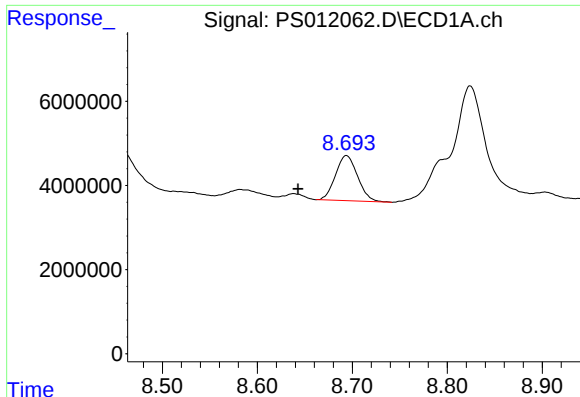

#10 Pentachlorophenol


R.T.: 8.694 min
Delta R.T.: 0.051 min
Response: 17298528
Conc: 1.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

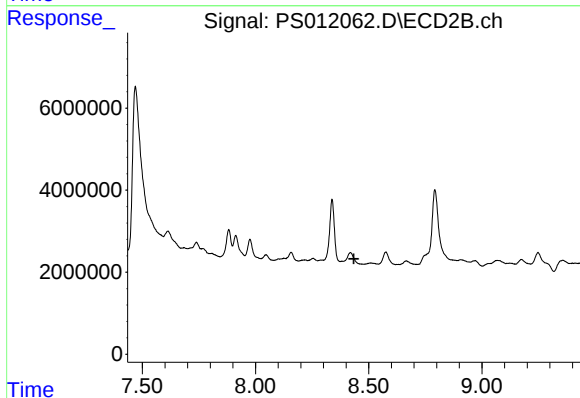


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.434 min
Response: 0
Conc: N.D.

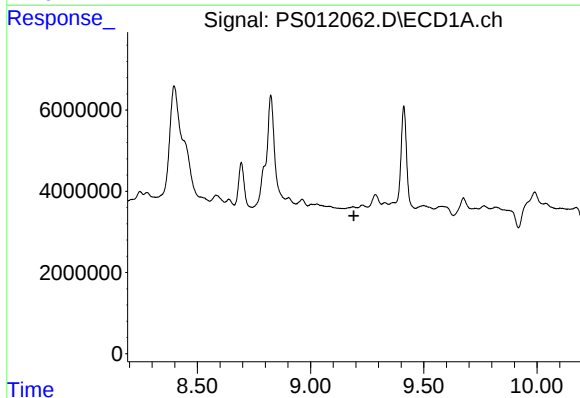


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

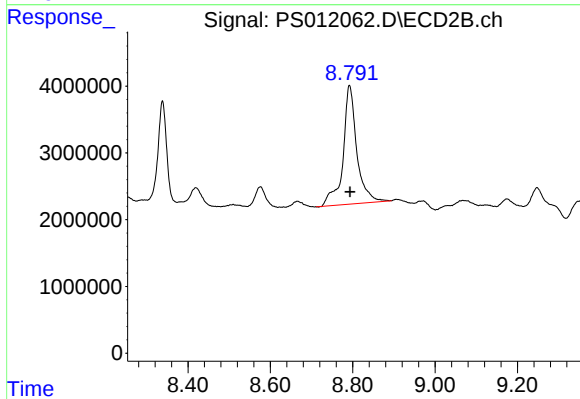

#11 2,4,5-TP (SILVEX)


R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 41357988
Conc: 14.15 ng/ml

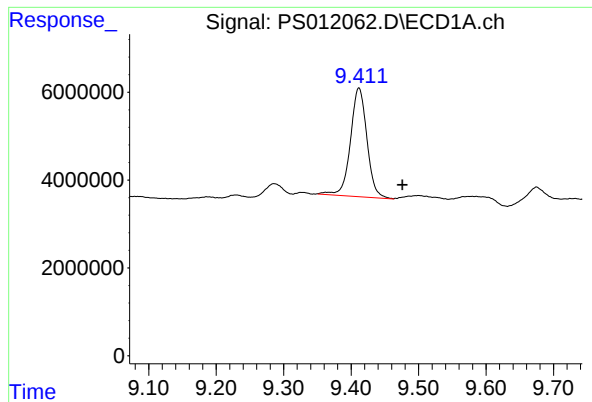

#12 2,4,5-T

R.T.: 9.412 min
Delta R.T.: -0.064 min
Response: 42052760
Conc: 7.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

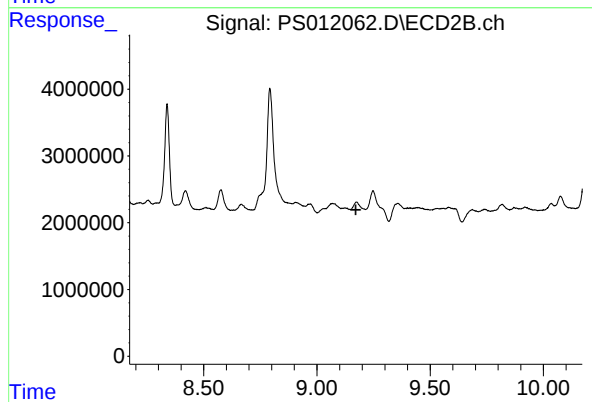

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.