

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
 Data File : PS012063.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2020 23:29
 Operator : DD\AJ
 Sample : L3866-05
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 05:10:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.218	6.914	231.8E6	142.7E6	212.488	266.884 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	79413059	N.D.	96.537
3) T	4-Nitroph...	7.055	0.000	3935438	0	6.681	N.D. #
5) T	DICAMBA	7.396	7.048	8170697	9138790	1.995	4.230 #
6) T	MCP	7.629	0.000	9536410	0	2.985	N.D. #
7) T	MCPA	7.695	7.469	236.1E6	148.9E6	51.910	54.331
9) T	2,4-D	8.400	0.000	115.7E6	0	102.436	N.D. #
11) T	2,4,5-TP ...	0.000	8.794	0	15087326	N.D.	5.160
12) T	2,4,5-T	9.412	0.000	25251073	0	4.261	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090220\
Data File : PS012063.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2020 23:29
Operator : DD\AJ
Sample : L3866-05
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 05:10:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

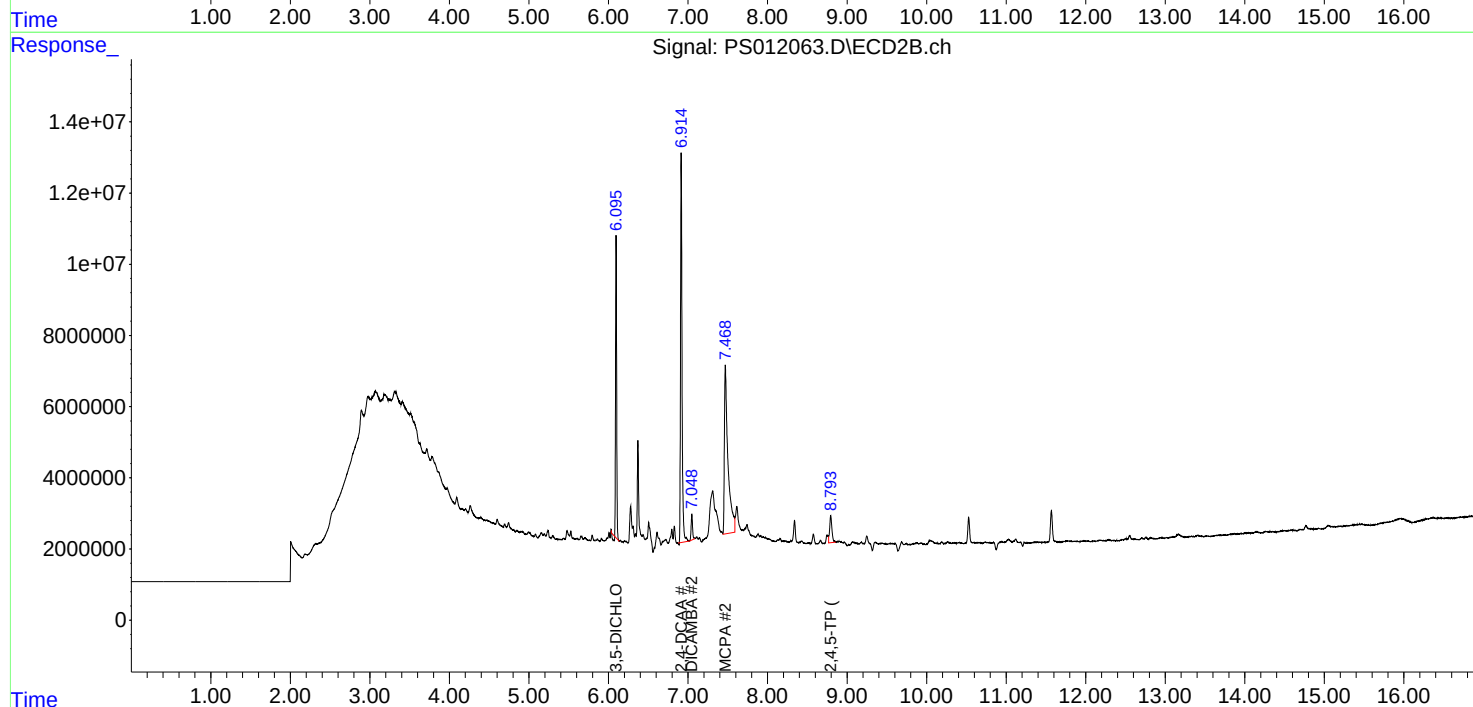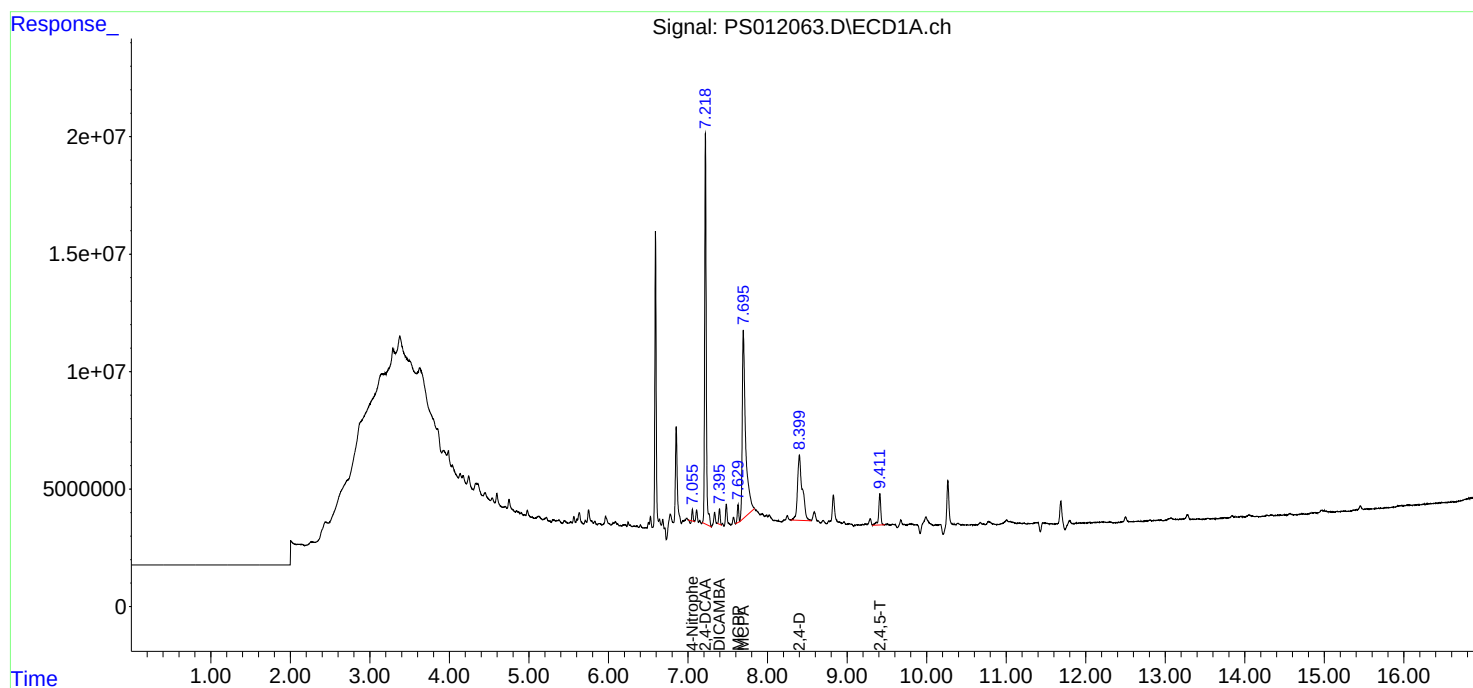


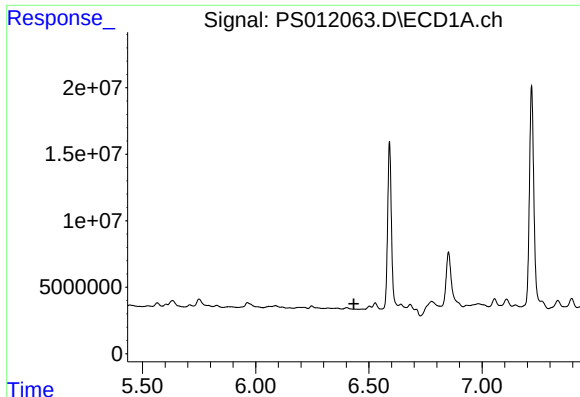

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

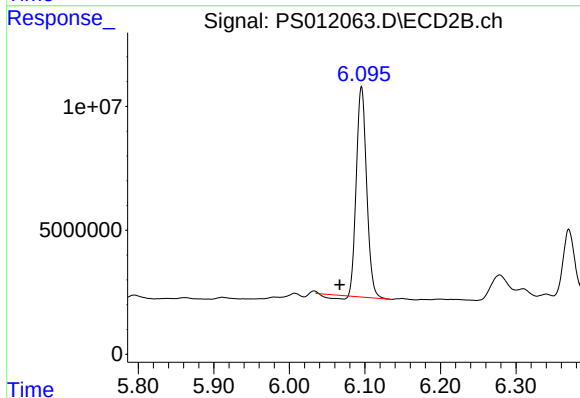


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 79413059
Conc: 96.54 ng/ml

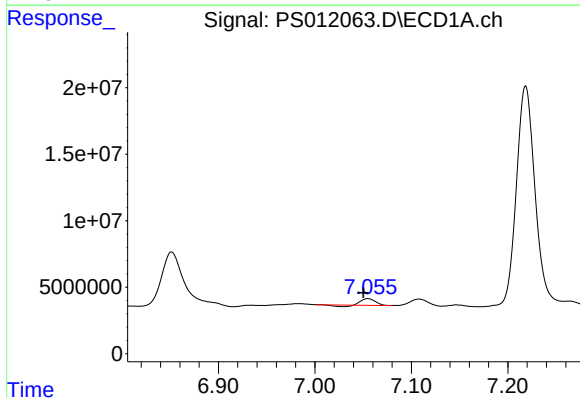


#3 4-Nitrophenol

R.T.: 7.055 min
Delta R.T.: 0.005 min
Response: 3935438
Conc: 6.68 ng/ml

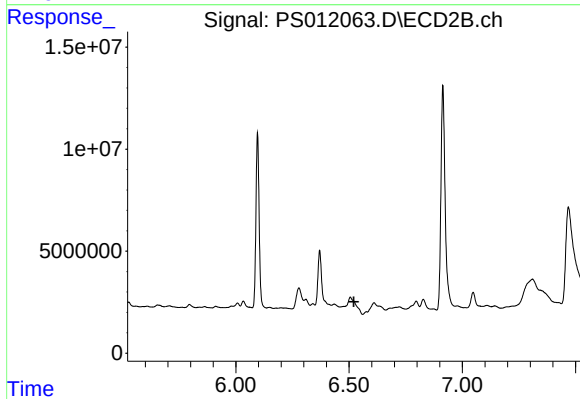

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

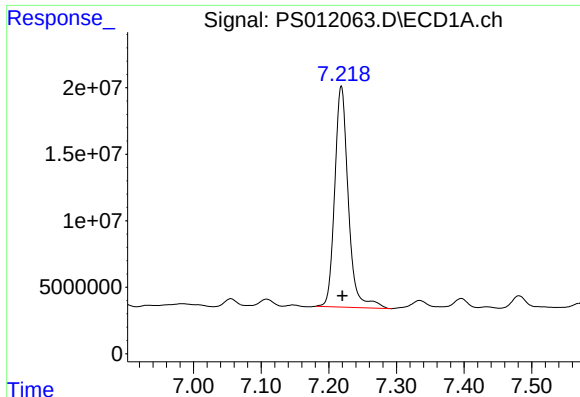

#4 2,4-DCAA


R.T.: 7.218 min
Delta R.T.: -0.002 min
Response: 231775374
Conc: 212.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

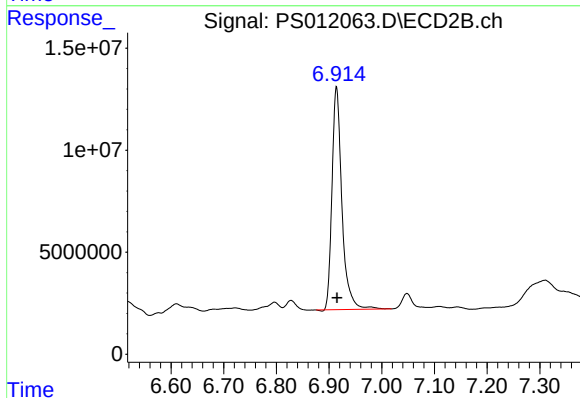


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 142726064
Conc: 266.88 ng/ml

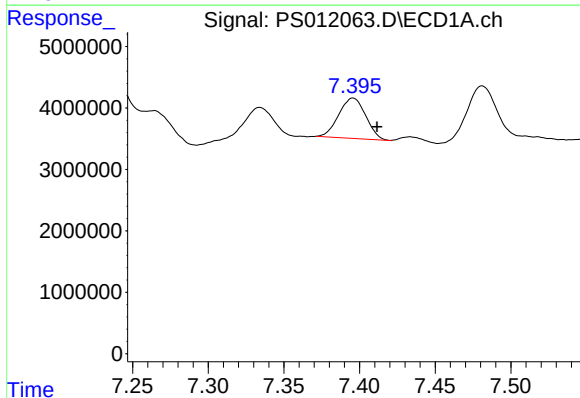


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.016 min
Response: 8170697
Conc: 1.99 ng/ml

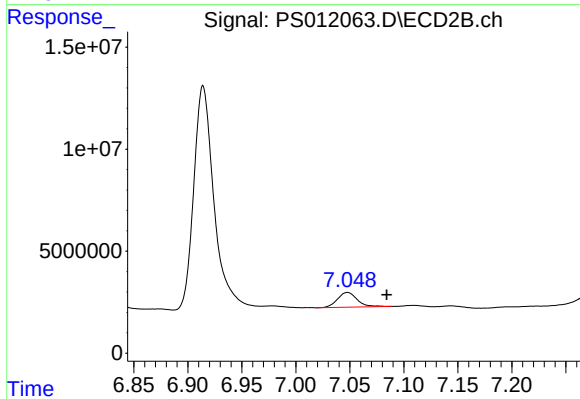

#5 DICAMBA


R.T.: 7.048 min
Delta R.T.: -0.036 min
Response: 9138790
Conc: 4.23 ng/ml

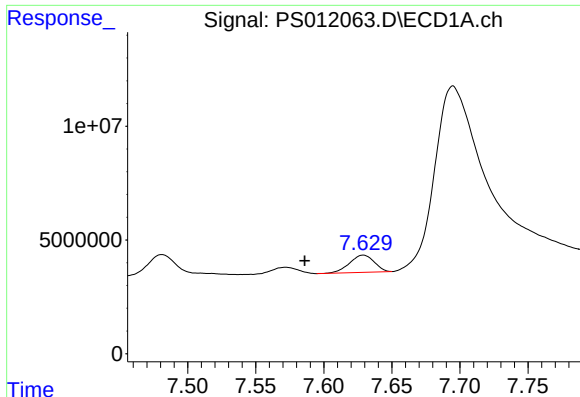

#6 MCPP


R.T.: 7.629 min
Delta R.T.: 0.043 min
Response: 9536410
Conc: 2.98 ug/ml

Instrument :
ECD_S
ClientSampleId :

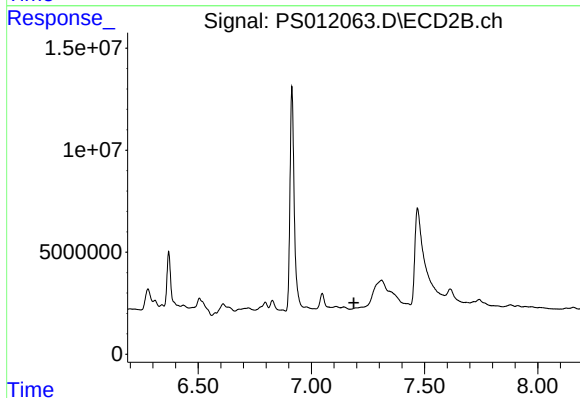


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

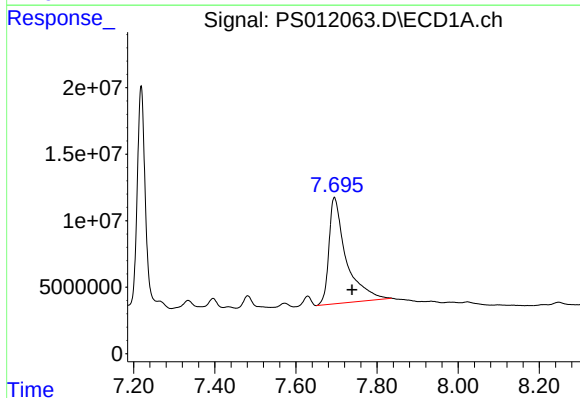


#7 MCPA

R.T.: 7.695 min
Delta R.T.: -0.043 min
Response: 236113604
Conc: 51.91 ug/ml

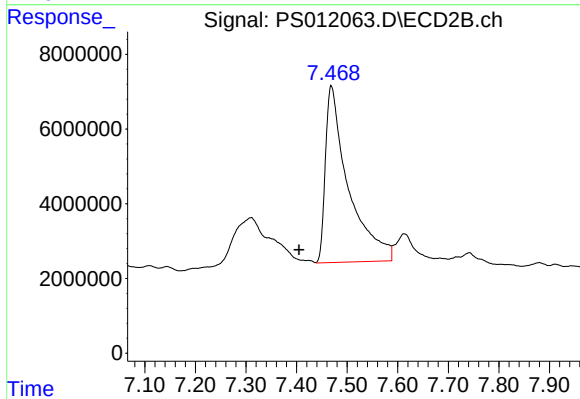

#7 MCPA


R.T.: 7.469 min
Delta R.T.: 0.064 min
Response: 148874455
Conc: 54.33 ug/ml

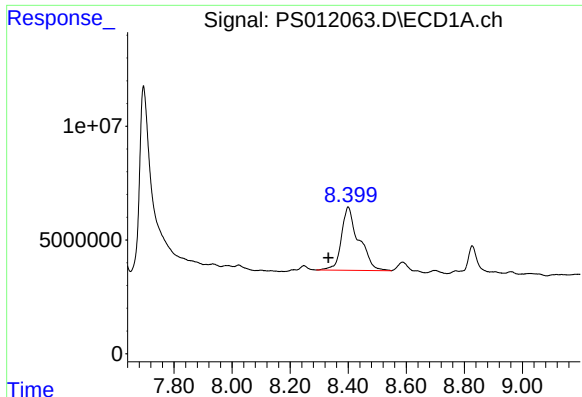

#9 2,4-D


R.T.: 8.400 min
Delta R.T.: 0.068 min
Response: 115659948
Conc: 102.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

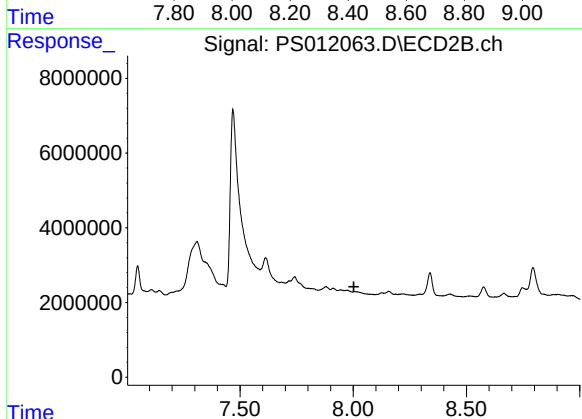


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

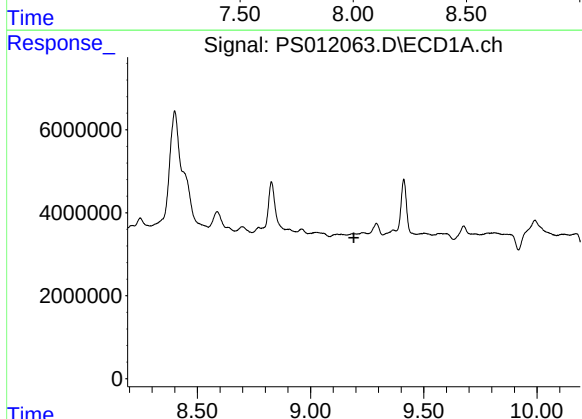


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

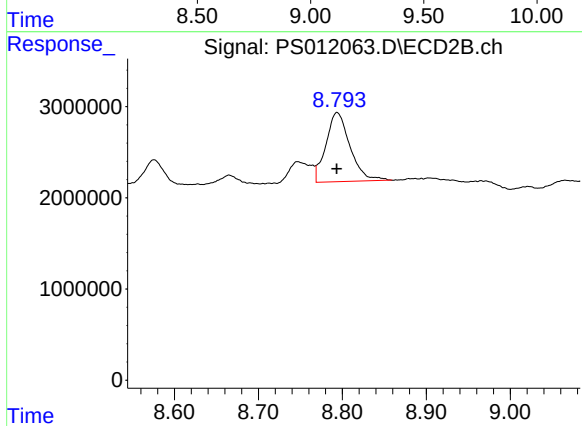

#11 2,4,5-TP (SILVEX)


R.T.: 8.794 min
Delta R.T.: 0.000 min
Response: 15087326
Conc: 5.16 ng/ml

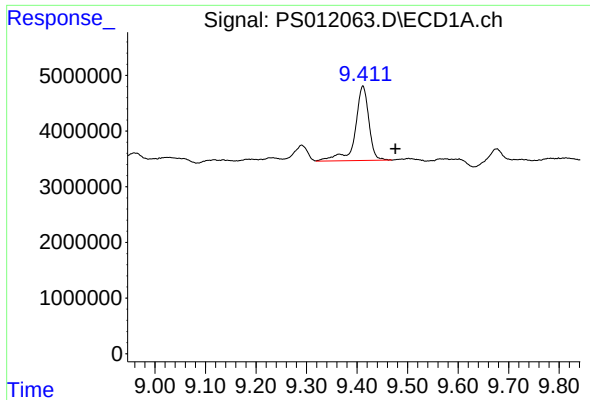

#12 2,4,5-T

R.T.: 9.412 min
Delta R.T.: -0.064 min
Response: 25251073
Conc: 4.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

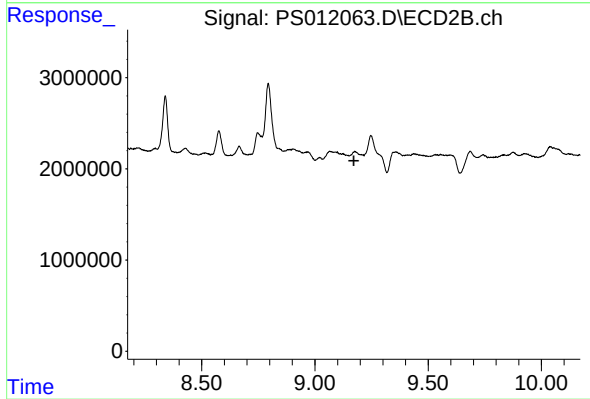

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.