

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090222\
 Data File : PS020427.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2022 10:27
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 01:11:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 03 01:09:33 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.188	6.763	1356.1E6	382.4E6	384.749	355.841
Target Compounds							
1) T	Dalapon	3.048f	0.000	1550416	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.390	0.000	111010	0	<MDL	N.D. #
3) T	4-Nitroph...	7.004f	0.000	3006001	0	1.937	N.D. #
9) T	2,4-D	8.358f	0.000	103.6E6	0	22.078	N.D. #
10) T	Pentachlo...	8.542f	0.000	9767688	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.103f	0.000	2901617	0	<MDL	N.D. #
12) T	2,4,5-T	9.490f	0.000	10538451	0	<MDL	N.D. #
14) T	DINOSEB	11.133	0.000	116.0E6	0	5.038	N.D. #
15) T	Picloram	10.941	0.000	8144195	0	<MDL	N.D. #
16) T	DCPA	11.402	0.000	7448744	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090222\
Data File : PS020427.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2022 10:27
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 01:11:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
Quant Title : 8080.M
QLast Update : Sat Sep 03 01:09:33 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

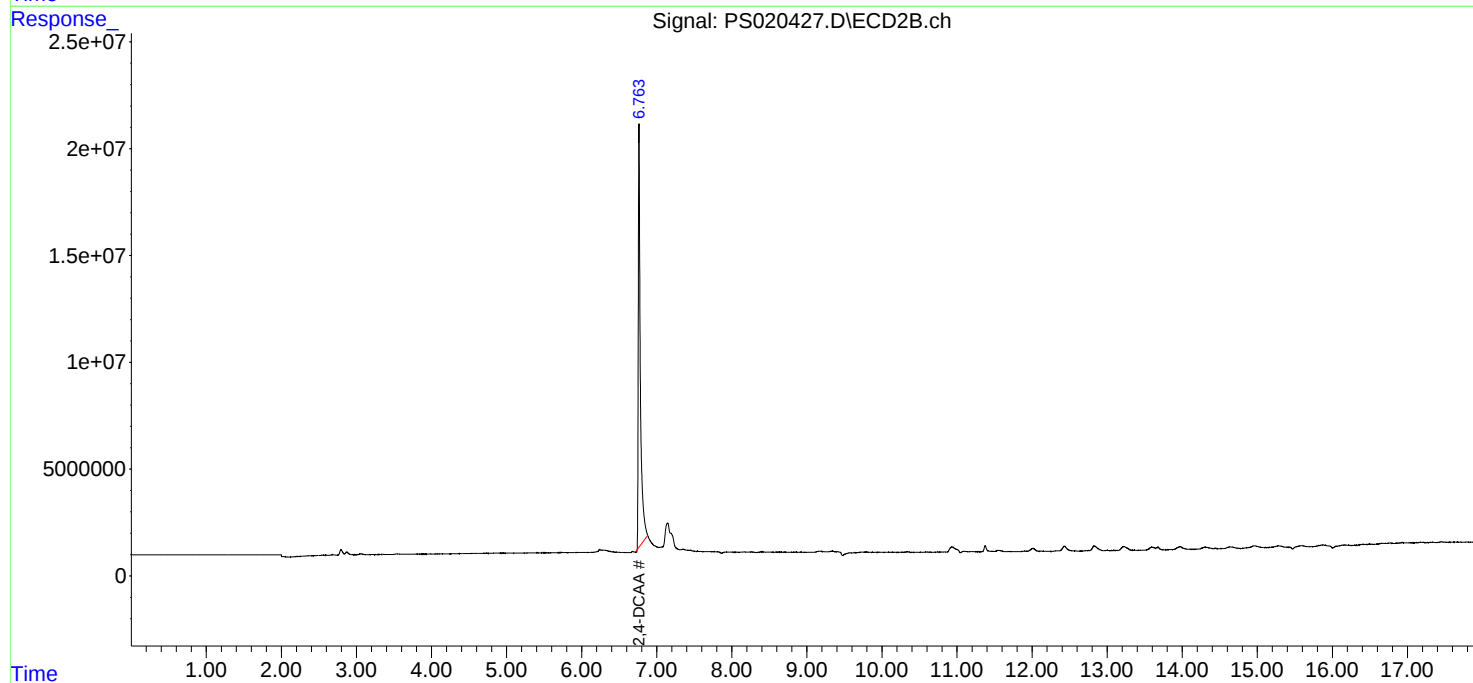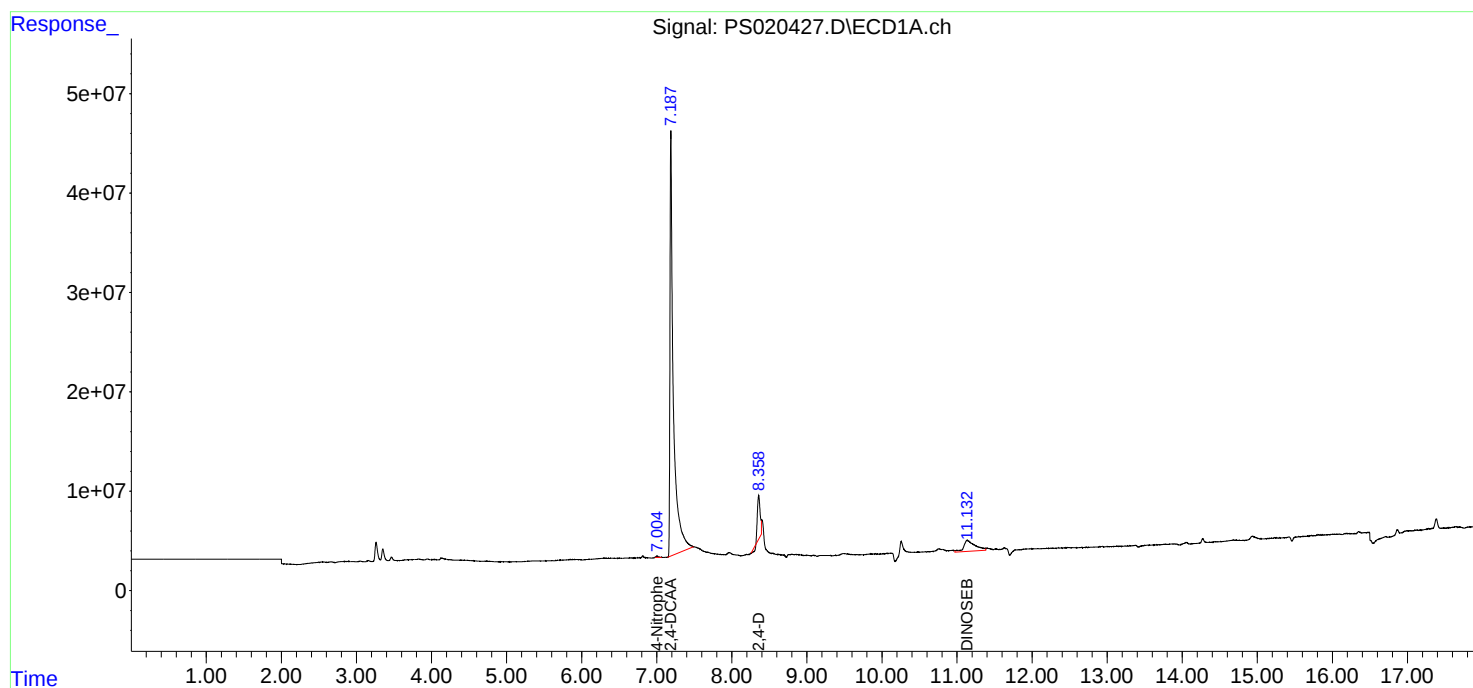


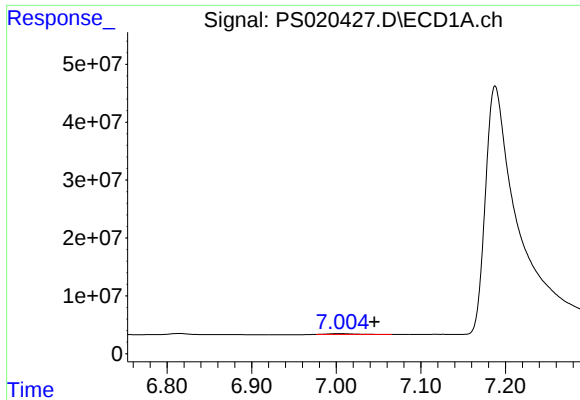

#3 4-Nitrophenol


R.T.: 7.004 min
Delta R.T.: -0.041 min
Response: 3006001
Conc: 1.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

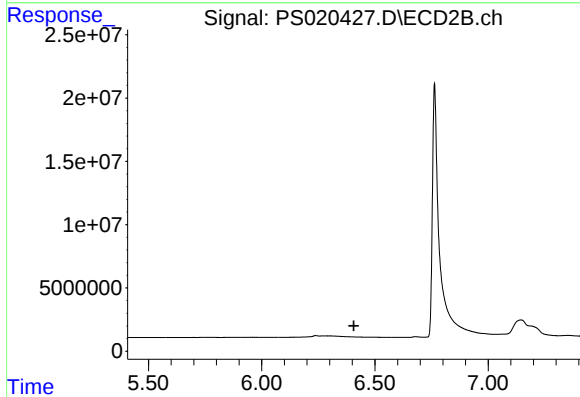


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.407 min
Response: 0
Conc: N.D.

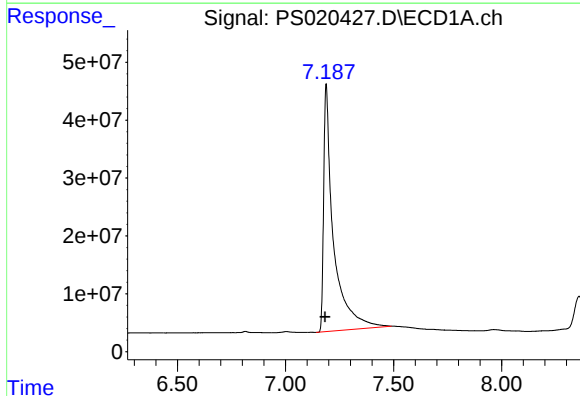


#4 2,4-DCAA

R.T.: 7.188 min
Delta R.T.: 0.005 min
Response: 1356111092
Conc: 384.75 ng/ml

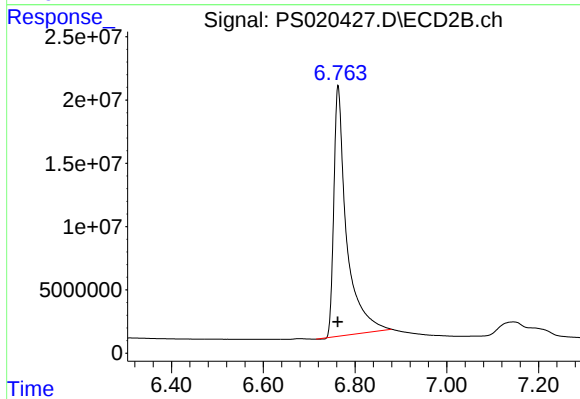

#4 2,4-DCAA


R.T.: 6.763 min
Delta R.T.: 0.000 min
Response: 382358193
Conc: 355.84 ng/ml

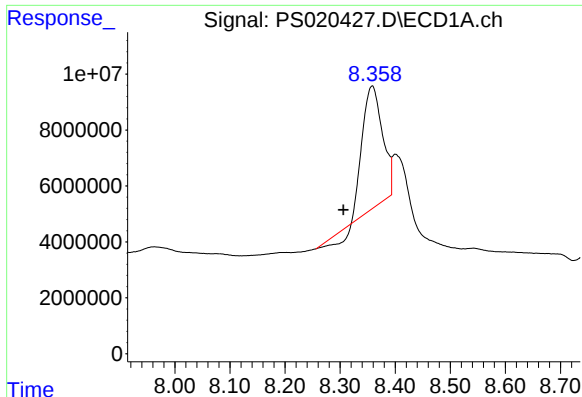

#9 2,4-D


R.T.: 8.358 min
Delta R.T.: 0.052 min
Response: 103579090
Conc: 22.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

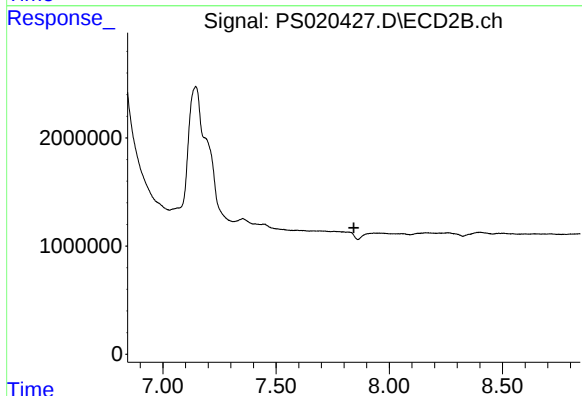


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.844 min
Response: 0
Conc: N.D.

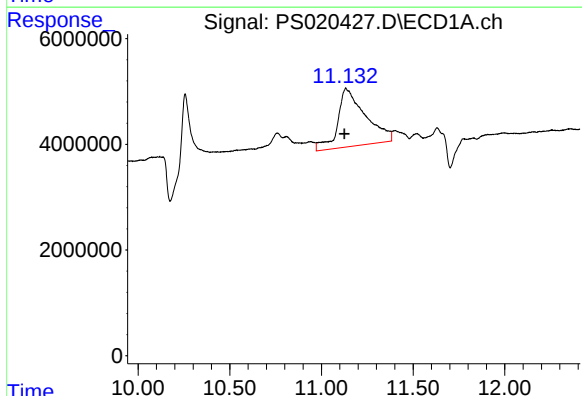

#14 DINOSEB

R.T.: 11.133 min
Delta R.T.: 0.007 min
Response: 116032804
Conc: 5.04 ng/ml

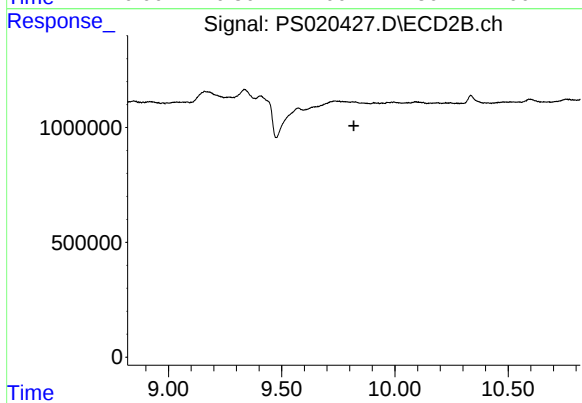

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.819 min
Response: 0
Conc: N.D.