

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090222\
 Data File : PS020430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2022 11:40
 Operator : AJ\MA
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 00:56:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 03 00:56:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.177	6.757	2563.1E6	782.7E6	750.000	750.000
Target Compounds							
1) T	Dalapon	2.997	2.511	3389.1E6	959.3E6	682.500	682.500
2) T	3,5-DICHL...	6.394	5.944	3220.2E6	1154.8E6	697.500	697.500
3) T	4-Nitroph...	7.013	6.382	1080.1E6	430.7E6	682.500	682.500
5) T	DICAMBA	7.364	6.919	9696.3E6	3334.0E6	705.000	705.000
6) T	MCPD	7.533	7.016	764.0E6	257.5E6	70.500	70.500
7) T	MCPA	7.682	7.228	1062.0E6	368.7E6	69.750	69.750
8) T	DICHLORPROP	8.056	7.539	2500.2E6	859.6E6	705.000	705.000
9) T	2,4-D	8.290	7.832	3251.5E6	1049.7E6	705.000	705.000
10) T	Pentachlo...	8.589	8.252	33676.7E6	11763.1E6	712.500	712.500
11) T	2,4,5-TP ...	9.140	8.614	14609.2E6	5069.2E6	712.500	712.500
12) T	2,4,5-T	9.427	8.992	15951.7E6	4802.3E6	712.500	712.500
13) T	2,4-DB	9.980	9.496	3104.5E6	632.4E6	712.500	712.500
14) T	DINOSEB	11.125	9.818	15510.1E6	3643.6E6	705.000	705.000
15) T	Picloram	10.957	10.800	29369.4E6	7259.4E6	712.500	712.500
16) T	DCPA	11.394	10.744	22176.1E6	6243.9E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090222\
Data File : PS020430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2022 11:40
Operator : AJ\MA
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 00:56:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
Quant Title : 8080.M
QLast Update : Sat Sep 03 00:56:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

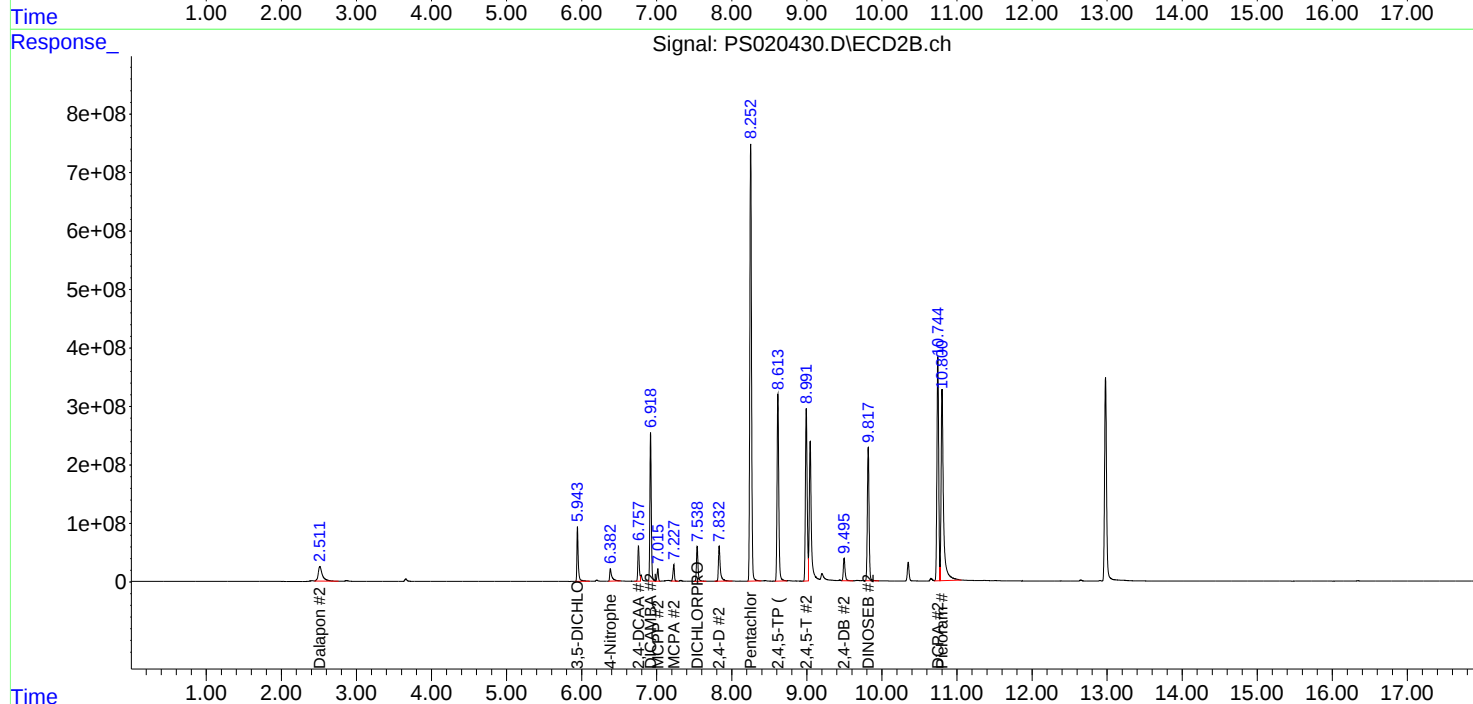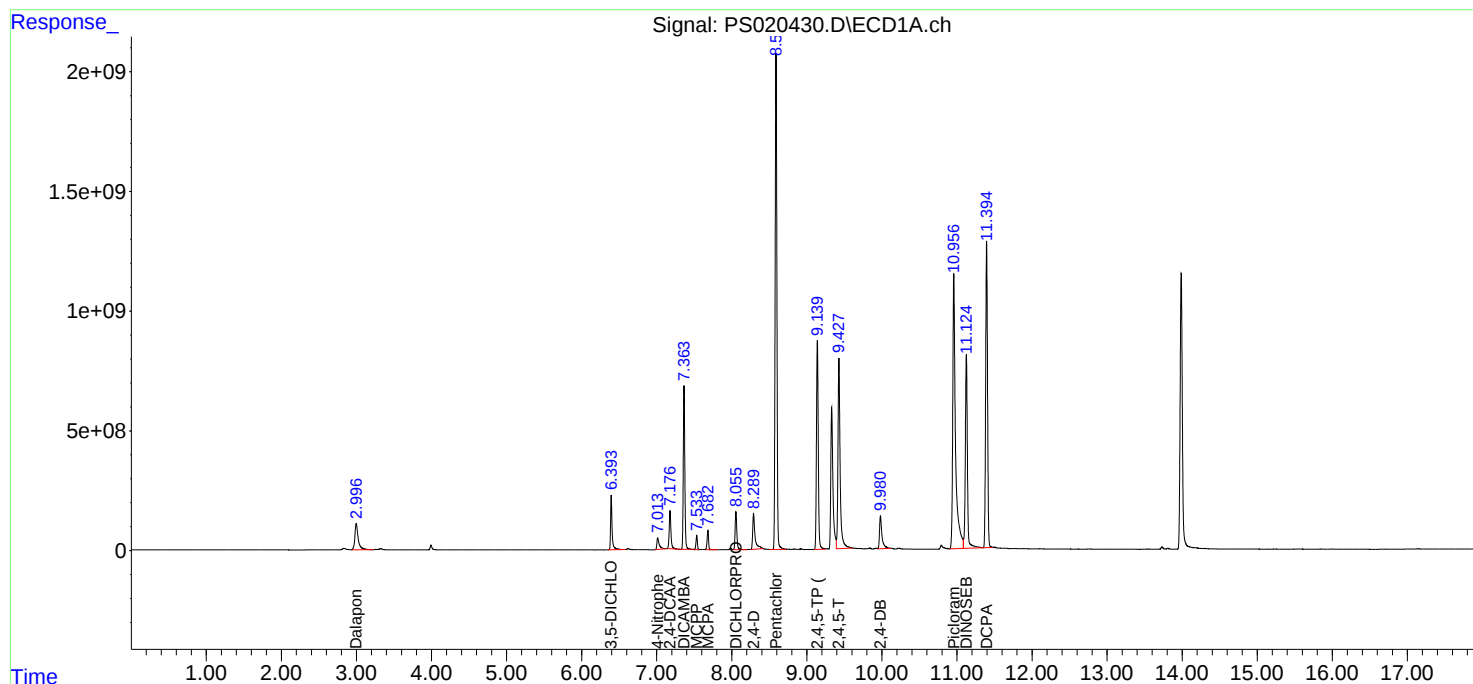


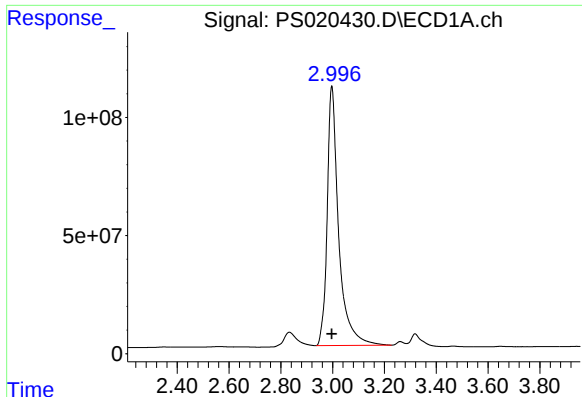

#1 Dalapon


R.T.: 2.997 min
Delta R.T.: 0.000 min
Response: 3389135471
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

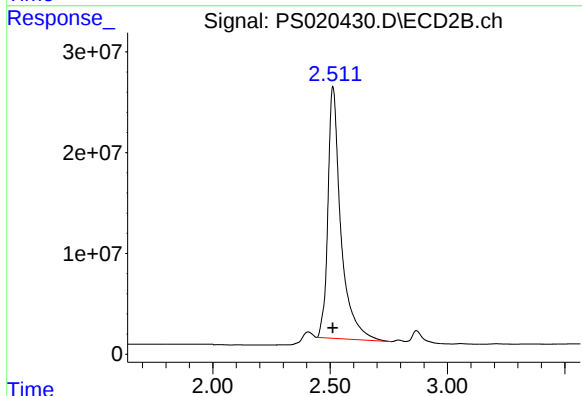


#1 Dalapon

R.T.: 2.511 min
Delta R.T.: 0.000 min
Response: 959256096
Conc: 682.50 ng/ml

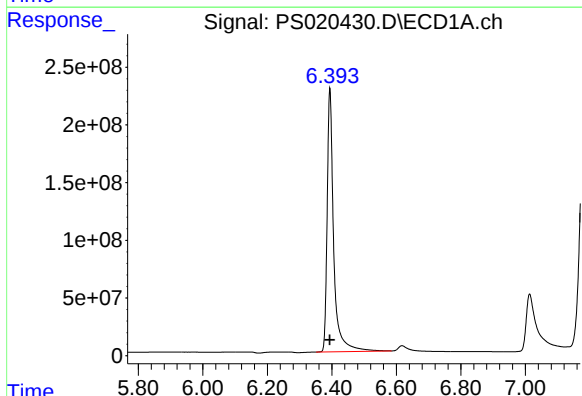


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.394 min
Delta R.T.: 0.000 min
Response: 3220208141
Conc: 697.50 ng/ml

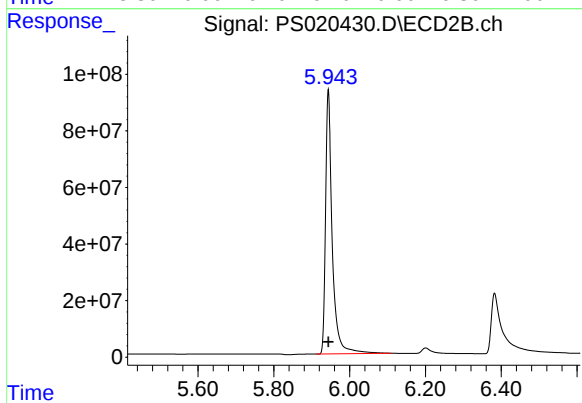

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 1154783606
Conc: 697.50 ng/ml

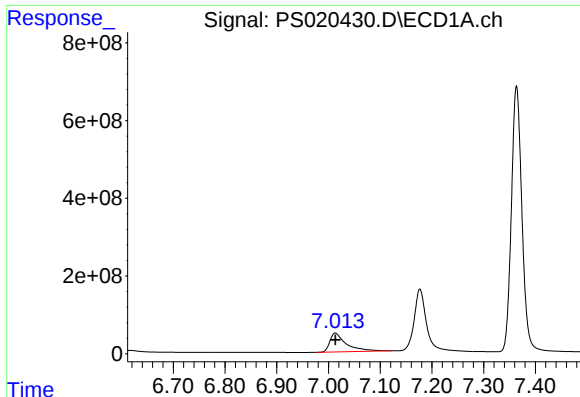

#3 4-Nitrophenol


R.T.: 7.013 min
Delta R.T.: 0.000 min
Response: 1080138866
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

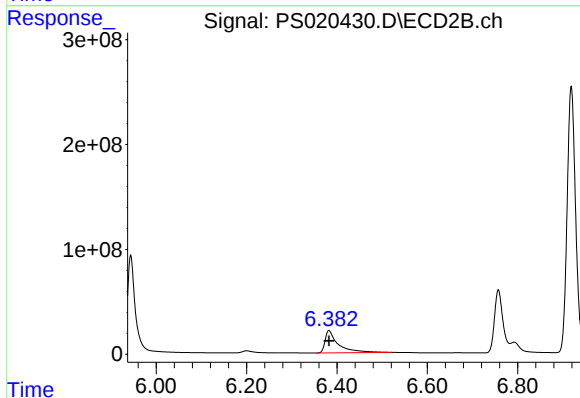


#3 4-Nitrophenol

R.T.: 6.382 min
Delta R.T.: 0.000 min
Response: 430684279
Conc: 682.50 ng/ml

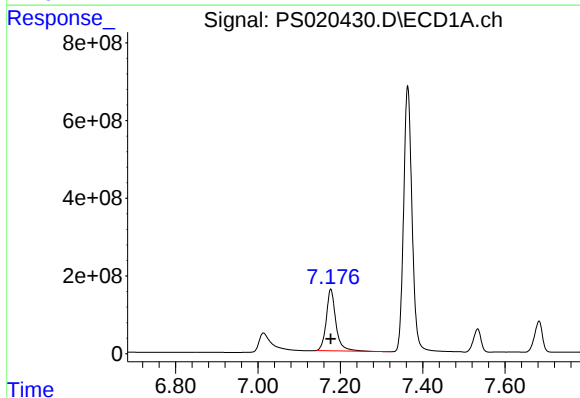


#4 2,4-DCAA

R.T.: 7.177 min
Delta R.T.: 0.000 min
Response: 2563129285
Conc: 750.00 ng/ml

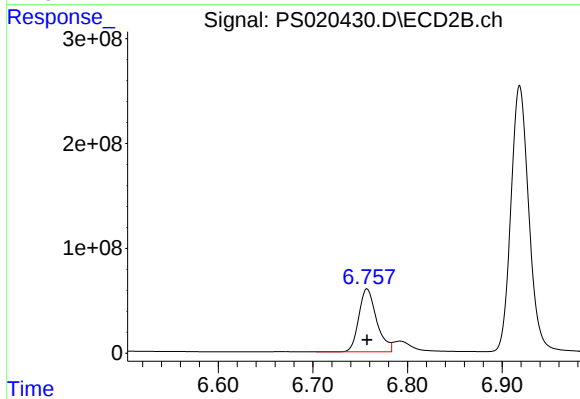

#4 2,4-DCAA


R.T.: 6.757 min
Delta R.T.: 0.000 min
Response: 782744193
Conc: 750.00 ng/ml

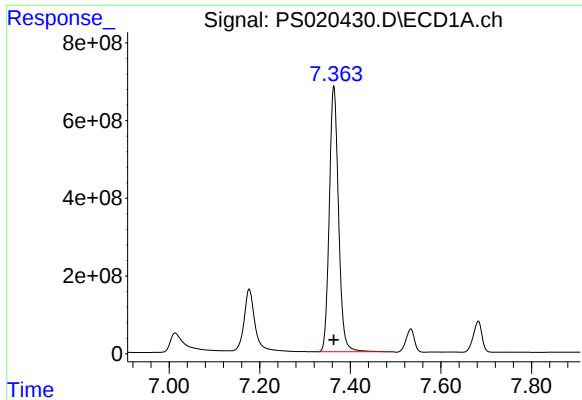

#5 DICAMBA


R.T.: 7.364 min
Delta R.T.: 0.000 min
Response: 9696310964
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

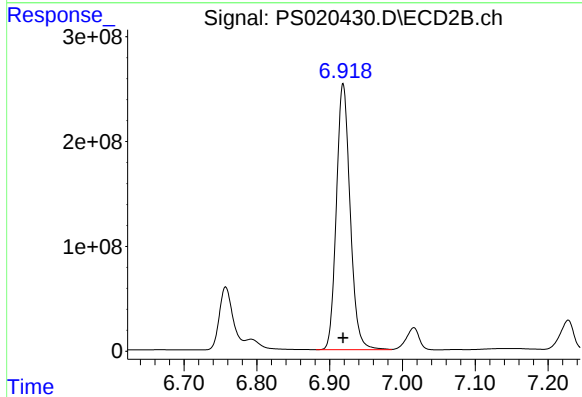


#5 DICAMBA

R.T.: 6.919 min
Delta R.T.: 0.000 min
Response: 3333994985
Conc: 705.00 ng/ml

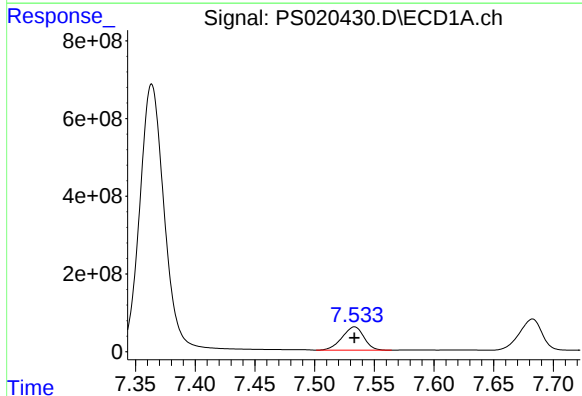


#6 MCP

R.T.: 7.533 min
Delta R.T.: 0.000 min
Response: 764016783
Conc: 70.50 ug/ml

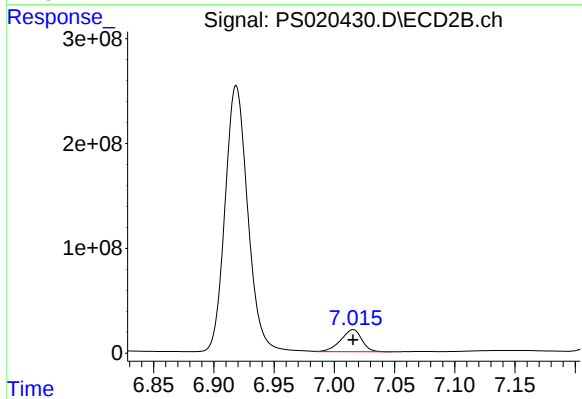

#6 MCP


R.T.: 7.016 min
Delta R.T.: 0.000 min
Response: 257483057
Conc: 70.50 ug/ml

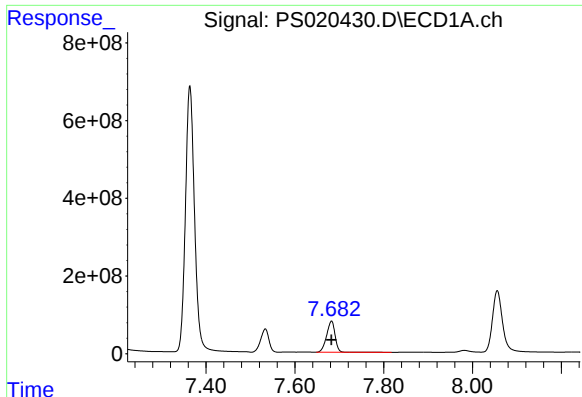

#7 MCPA


R.T.: 7.682 min
Delta R.T.: 0.000 min
Response: 1062005590
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

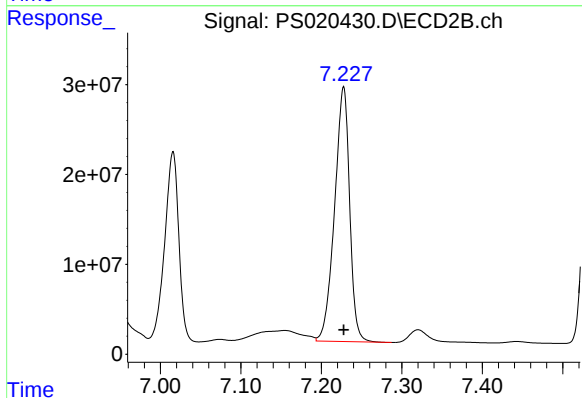


#7 MCPA

R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 368741028
Conc: 69.75 ug/ml

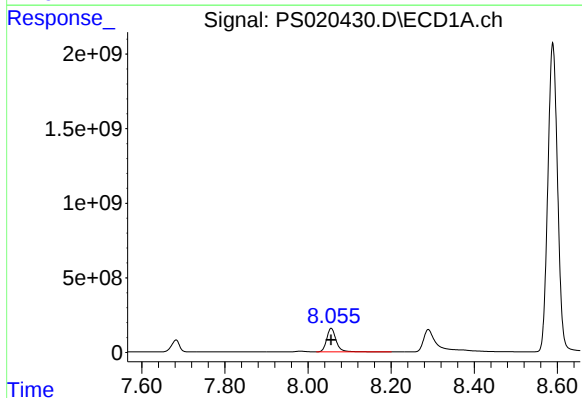


#8 DICHLORPROP

R.T.: 8.056 min
Delta R.T.: 0.000 min
Response: 2500181333
Conc: 705.00 ng/ml

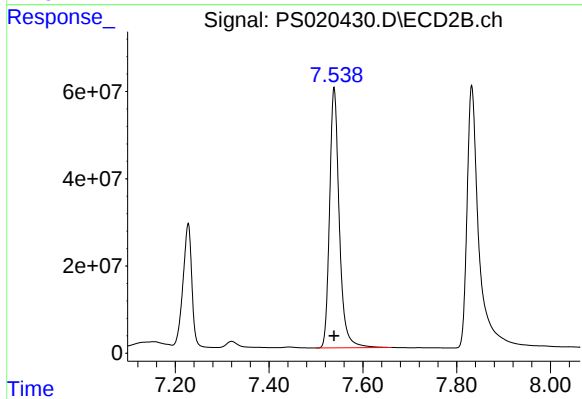

#8 DICHLORPROP


R.T.: 7.539 min
Delta R.T.: 0.000 min
Response: 859568754
Conc: 705.00 ng/ml

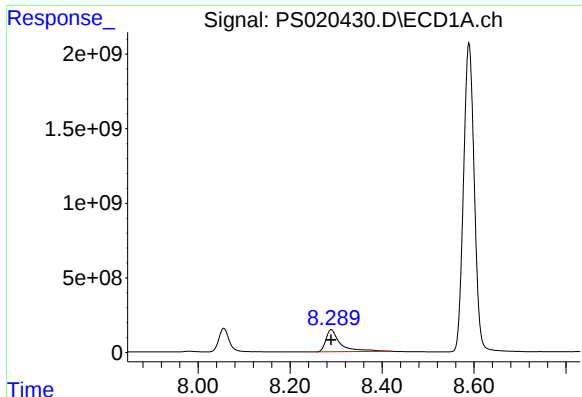

#9 2,4-D


R.T.: 8.290 min
Delta R.T.: 0.000 min
Response: 3251489884
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

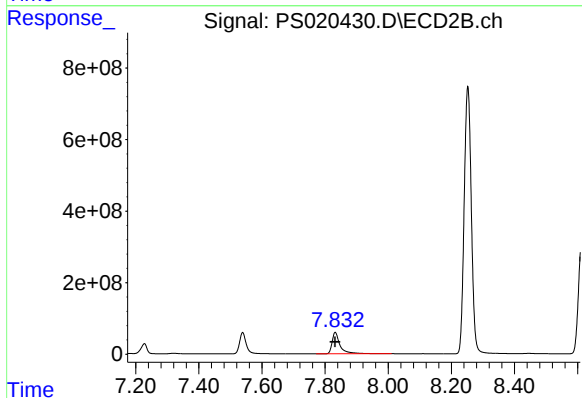


#9 2,4-D

R.T.: 7.832 min
Delta R.T.: 0.000 min
Response: 1049667015
Conc: 705.00 ng/ml

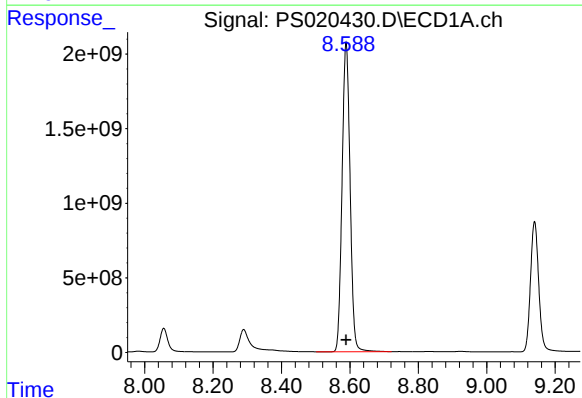


#10 Pentachlorophenol

R.T.: 8.589 min
Delta R.T.: 0.000 min
Response: 33676704144
Conc: 712.50 ng/ml

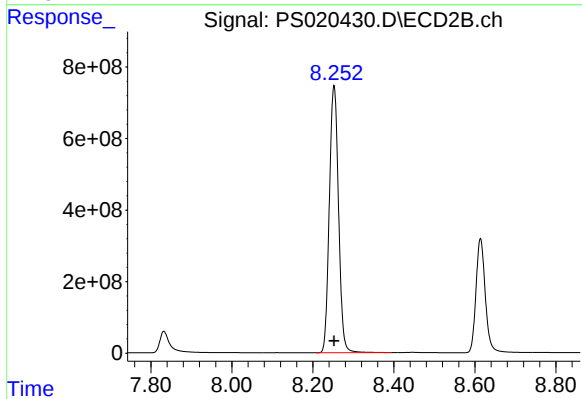

#10 Pentachlorophenol


R.T.: 8.252 min
Delta R.T.: 0.000 min
Response: 11763077726
Conc: 712.50 ng/ml

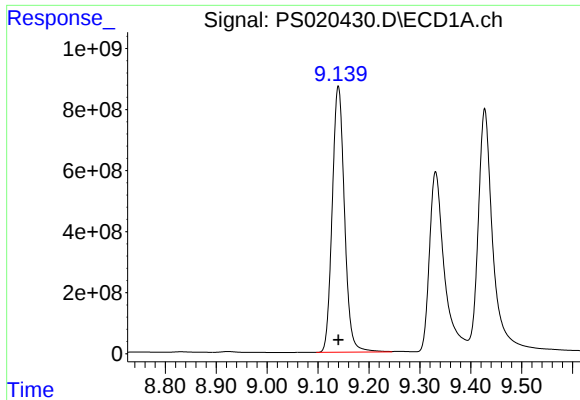

#11 2,4,5-TP (SILVEX)


R.T.: 9.140 min
Delta R.T.: 0.000 min
Response: 14609216389
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

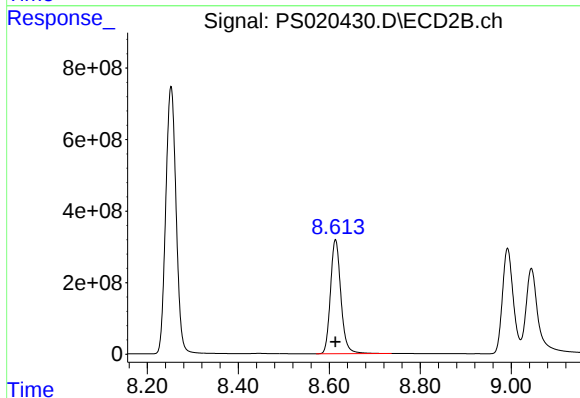


#11 2,4,5-TP (SILVEX)

R.T.: 8.614 min
Delta R.T.: 0.000 min
Response: 5069243768
Conc: 712.50 ng/ml

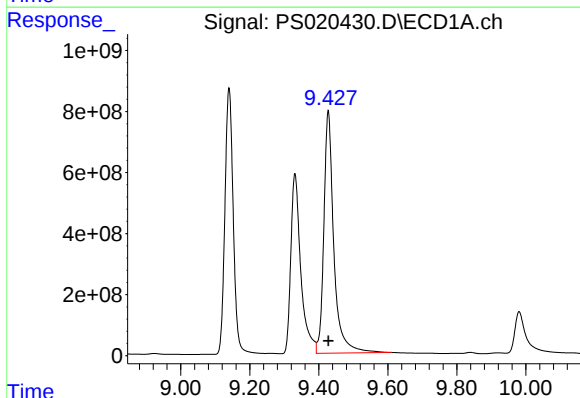


#12 2,4,5-T

R.T.: 9.427 min
Delta R.T.: 0.000 min
Response: 15951681865
Conc: 712.50 ng/ml

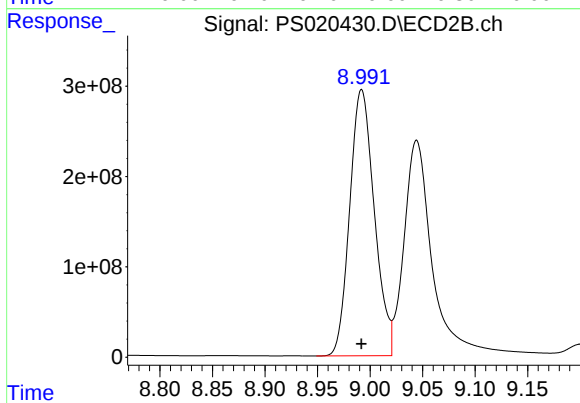

#12 2,4,5-T


R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 4802296996
Conc: 712.50 ng/ml

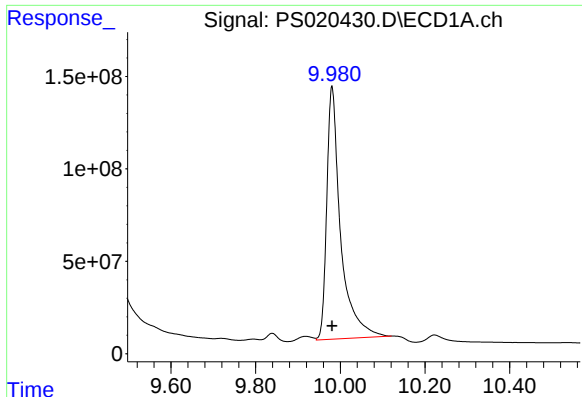

#13 2,4-DB


R.T.: 9.980 min
Delta R.T.: 0.000 min
Response: 3104526825
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

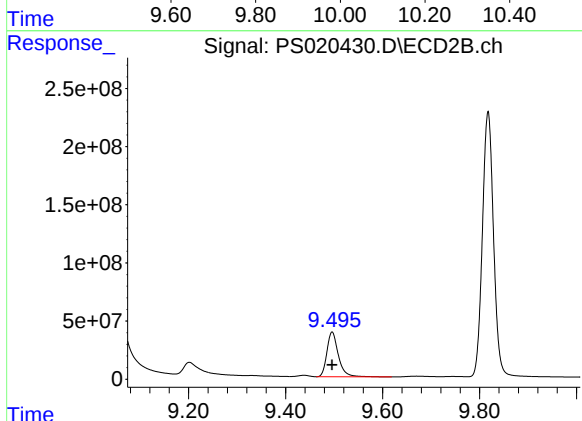


#13 2,4-DB

R.T.: 9.496 min
Delta R.T.: 0.000 min
Response: 632415540
Conc: 712.50 ng/ml

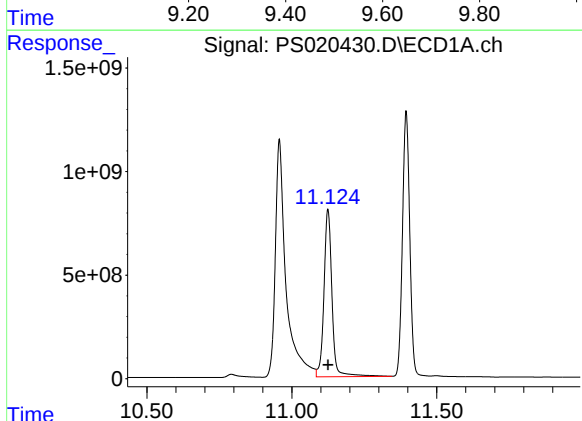


#14 DINOSEB

R.T.: 11.125 min
Delta R.T.: 0.000 min
Response: 15510061192
Conc: 705.00 ng/ml

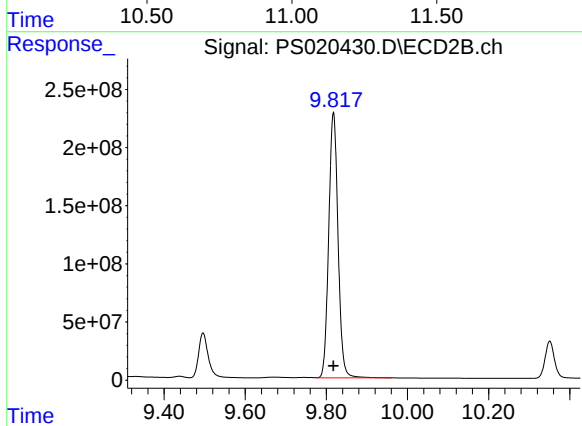

#14 DINOSEB


R.T.: 9.818 min
Delta R.T.: 0.000 min
Response: 3643586427
Conc: 705.00 ng/ml

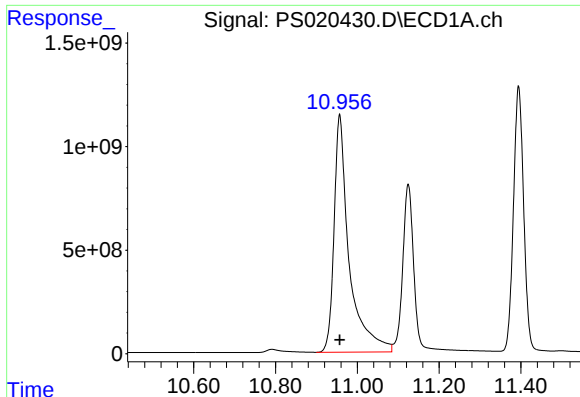

#15 Picloram


R.T.: 10.957 min
Delta R.T.: 0.000 min
Response: 29369443678
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

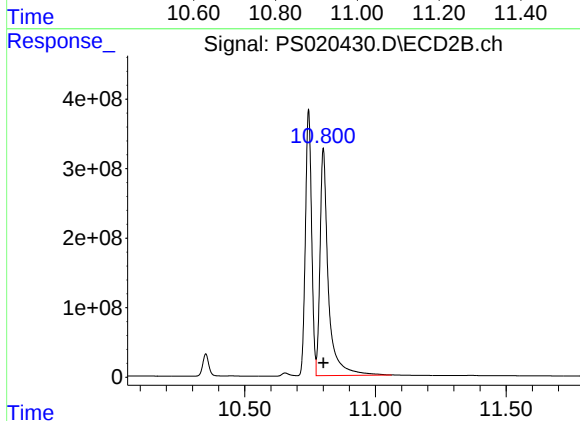


#15 Picloram

R.T.: 10.800 min
Delta R.T.: 0.000 min
Response: 7259441669
Conc: 712.50 ng/ml

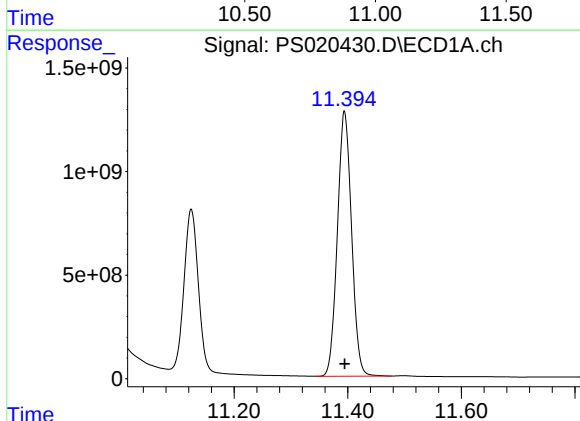

#16 DCPA

R.T.: 11.394 min
Delta R.T.: 0.000 min
Response: 22176075633
Conc: 720.00 ng/ml

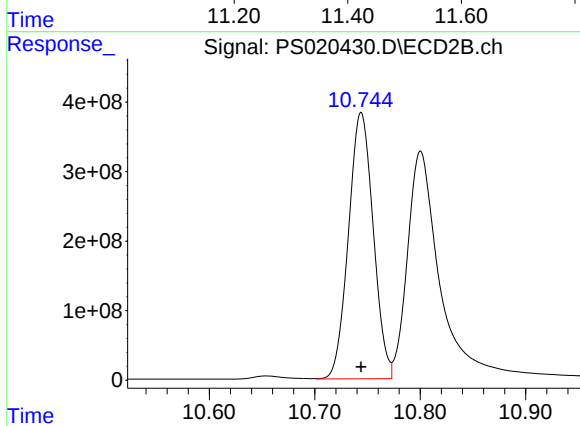

#16 DCPA

R.T.: 10.744 min
Delta R.T.: 0.000 min
Response: 6243934610
Conc: 720.00 ng/ml