

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090222\
 Data File : PS020432.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2022 12:28
 Operator : AJ\MA
 Sample : HSTDICC1500
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC1500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 00:59:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 03 00:56:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.174	6.755	4973.3E6	1611.5E6	1477.282	1521.704
Target Compounds							
1) T	Dalapon	2.996	2.511	6605.5E6	1927.0E6	1365.000	1368.015
2) T	3,5-DICHL...	6.392	5.942	6092.5E6	2273.6E6	1356.277	1384.065
3) T	4-Nitroph...	7.004	6.376	2486.5E6	904.9E6	1460.842	1398.645
5) T	DICAMBA	7.363	6.918	17965.0E6	6393.8E6	1356.117	1380.404
6) T	MCPD	7.540	7.024	1607.7E6	539.6E6	144.581	144.295
7) T	MCPA	7.690	7.238	2184.4E6	758.4E6	141.456	141.454
8) T	DICHLORPROP	8.054	7.537	4833.9E6	1720.3E6	1386.127	1410.461
9) T	2,4-D	8.284	7.829	5809.1E6	2126.7E6	1330.538	1419.140
10) T	Pentachlo...	8.592	8.252	46393.5E6	19945.9E6	1162.418	1307.640
11) T	2,4,5-TP ...	9.138	8.612	26438.3E6	9424.9E6	1353.820	1373.019
12) T	2,4,5-T	9.424	8.989	28216.2E6	9148.6E6	1337.603	1390.348
13) T	2,4-DB	9.975	9.493	6430.1E6	1331.5E6	1449.927	1461.588
14) T	DINOSEB	11.124	9.817	27376.4E6	7013.1E6	1322.021	1382.977
15) T	Picloram	10.950	10.796	53396.5E6	13999.9E6	1357.110	1399.069
16) T	DCPA	11.394	10.744	39467.3E6	11411.4E6	1356.079	1375.139



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090222\
Data File : PS020432.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2022 12:28
Operator : AJ\MA
Sample : HSTDICC1500
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 00:59:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
Quant Title : 8080.M
QLast Update : Sat Sep 03 00:56:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

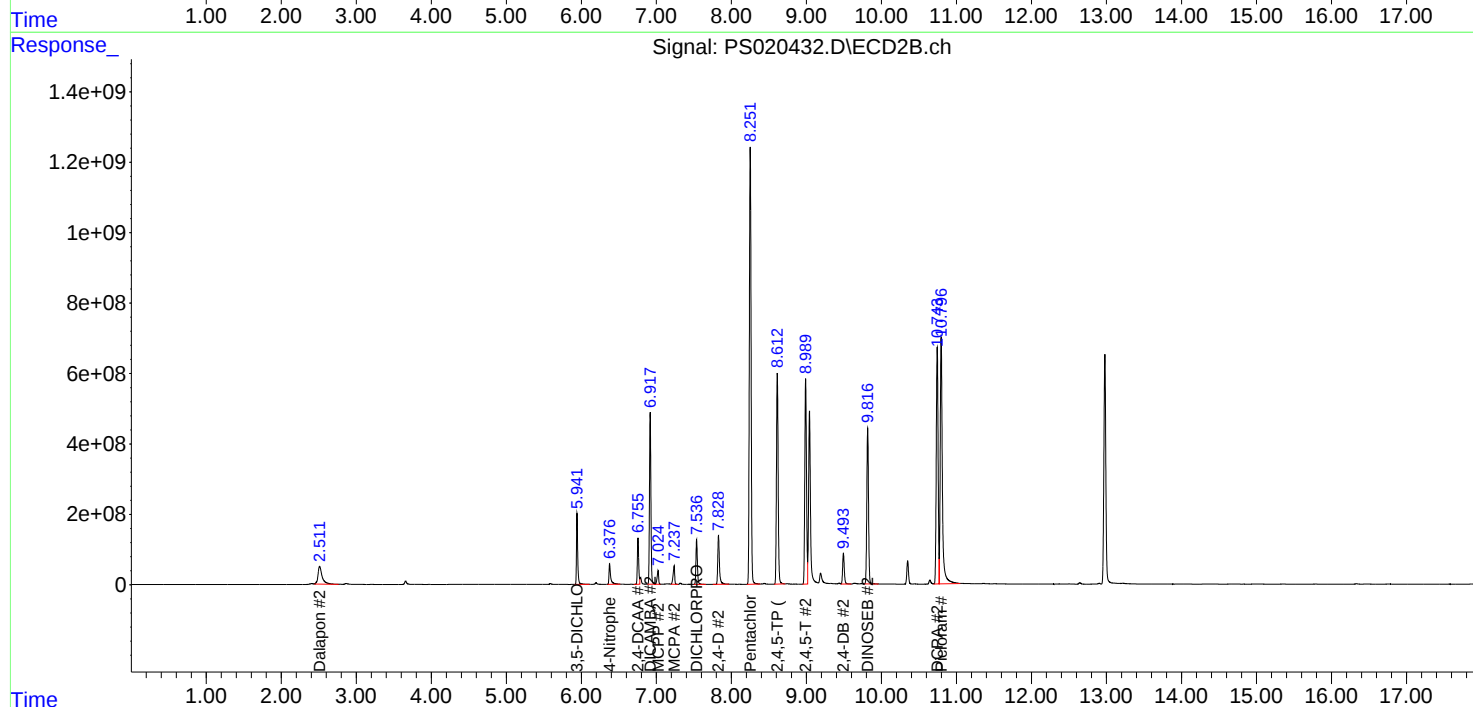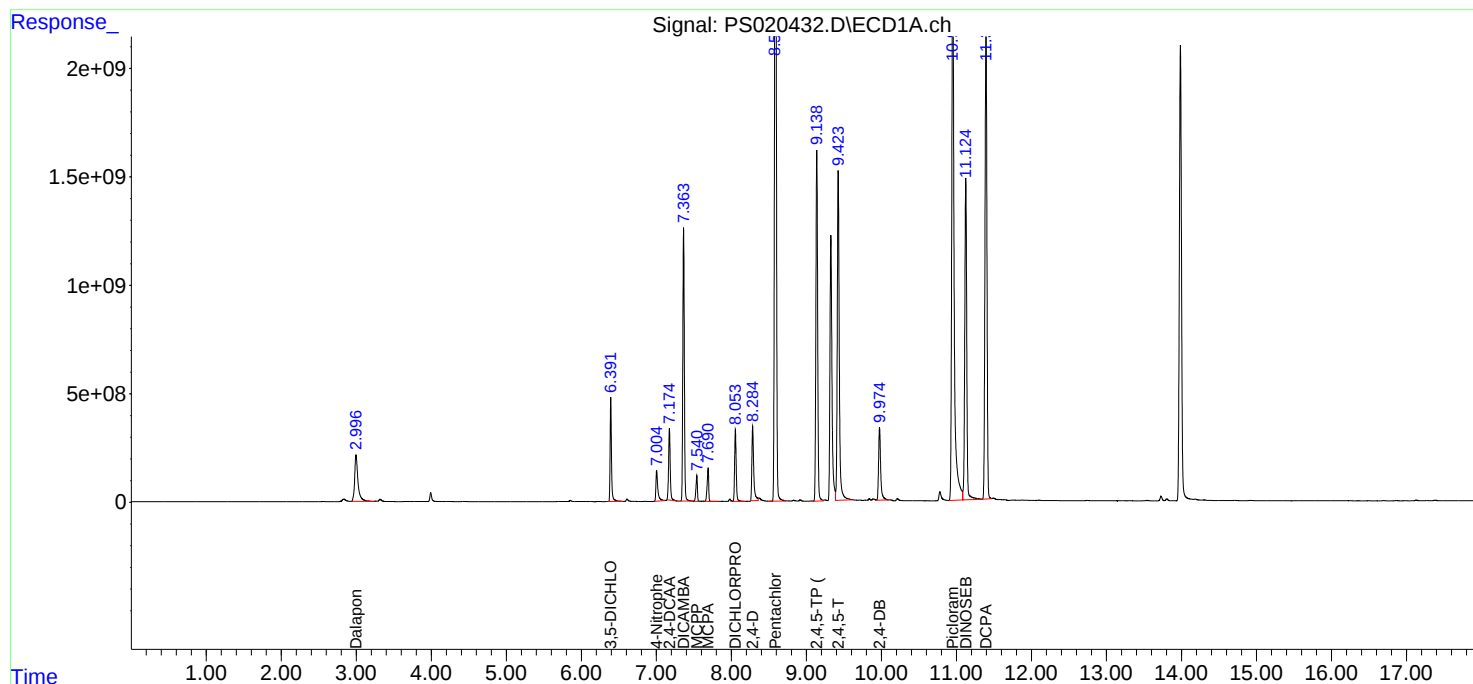


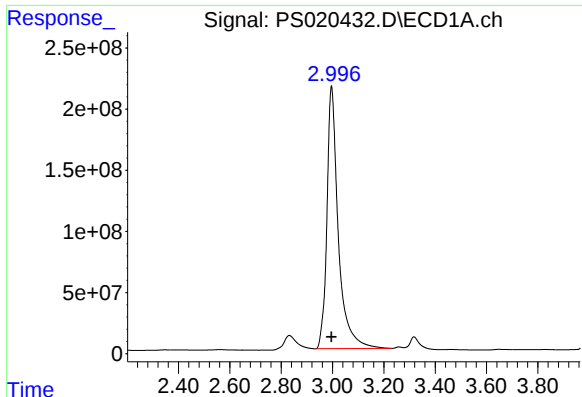

#1 Dalapon


R.T.: 2.996 min
Delta R.T.: 0.000 min
Response: 6605497665
Conc: 1365.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

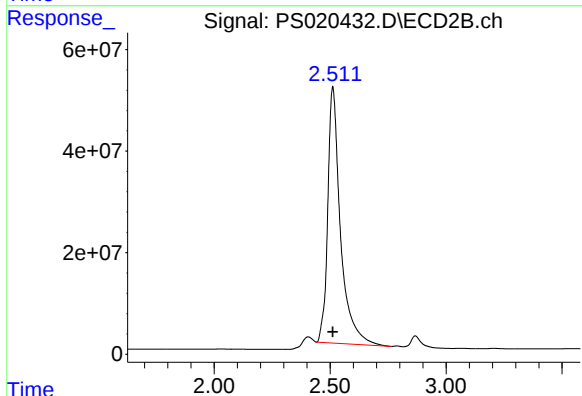


#1 Dalapon

R.T.: 2.511 min
Delta R.T.: 0.000 min
Response: 1927004790
Conc: 1368.01 ng/ml

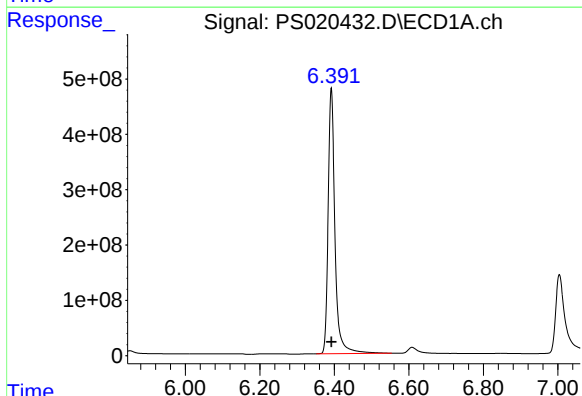


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.392 min
Delta R.T.: 0.000 min
Response: 6092525665
Conc: 1356.28 ng/ml

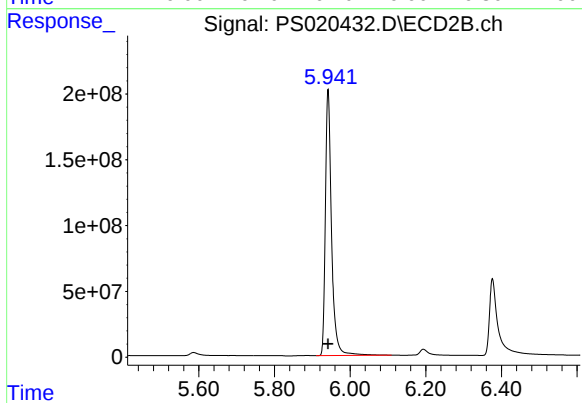

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.942 min
Delta R.T.: 0.000 min
Response: 2273642208
Conc: 1384.07 ng/ml

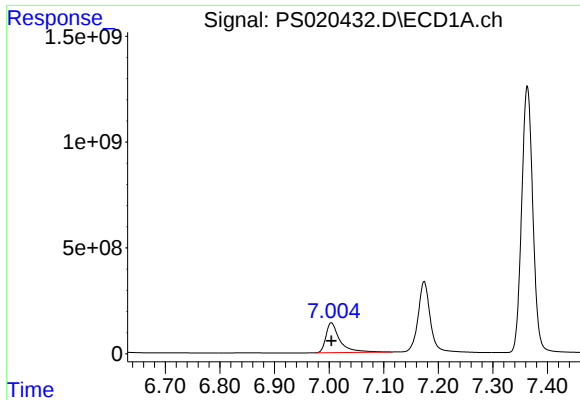

#3 4-Nitrophenol


R.T.: 7.004 min
Delta R.T.: 0.000 min
Response: 2486548246
Conc: 1460.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

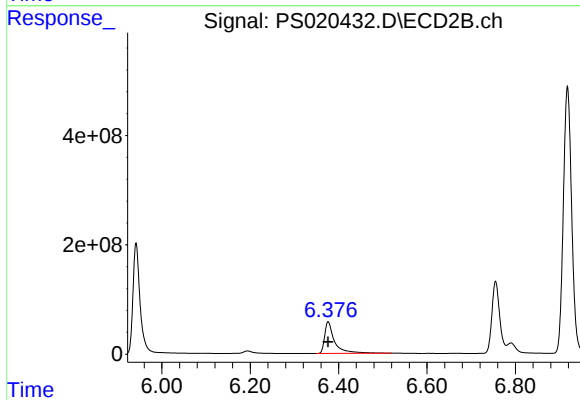


#3 4-Nitrophenol

R.T.: 6.376 min
Delta R.T.: 0.000 min
Response: 904904201
Conc: 1398.64 ng/ml

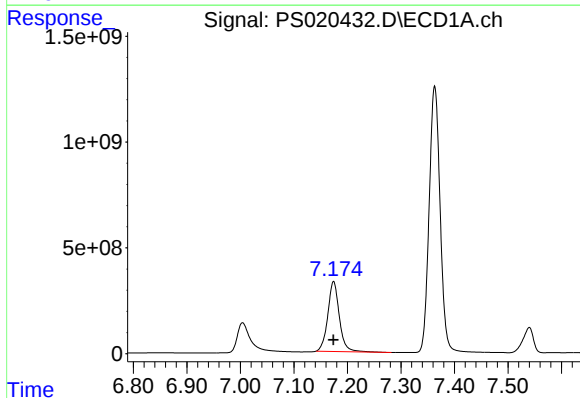


#4 2,4-DCAA

R.T.: 7.174 min
Delta R.T.: 0.000 min
Response: 4973295333
Conc: 1477.28 ng/ml

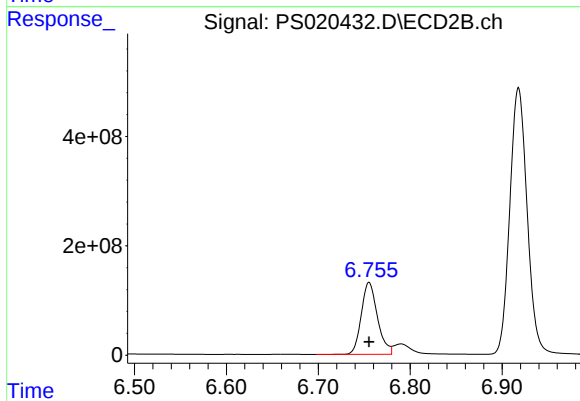

#4 2,4-DCAA


R.T.: 6.755 min
Delta R.T.: 0.000 min
Response: 1611456610
Conc: 1521.70 ng/ml

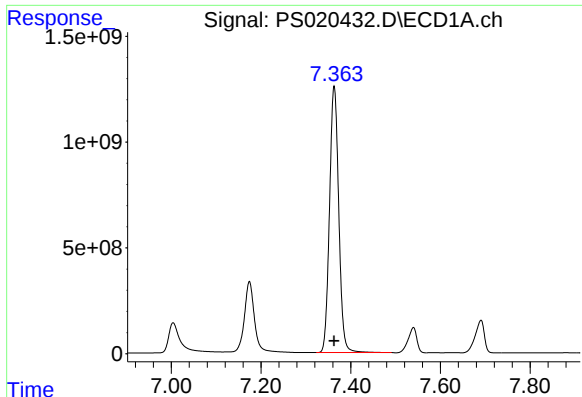

#5 DICAMBA


R.T.: 7.363 min
Delta R.T.: 0.000 min
Response: 17964991952
Conc: 1356.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

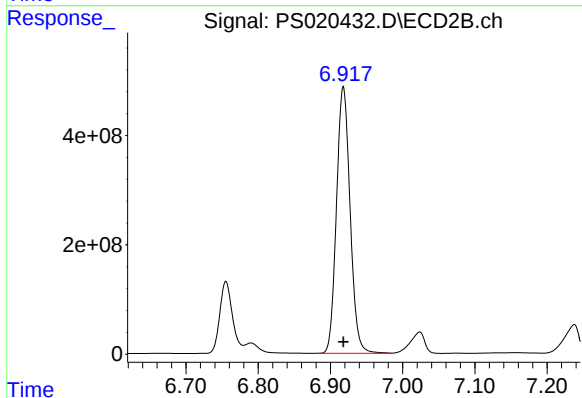


#5 DICAMBA

R.T.: 6.918 min
Delta R.T.: 0.000 min
Response: 6393824471
Conc: 1380.40 ng/ml

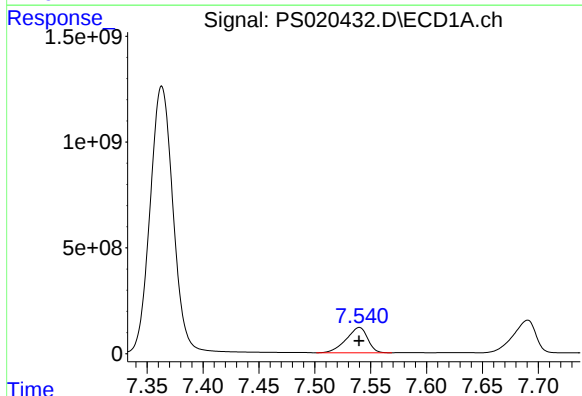


#6 MCP

R.T.: 7.540 min
Delta R.T.: 0.000 min
Response: 1607672659
Conc: 144.58 ug/ml

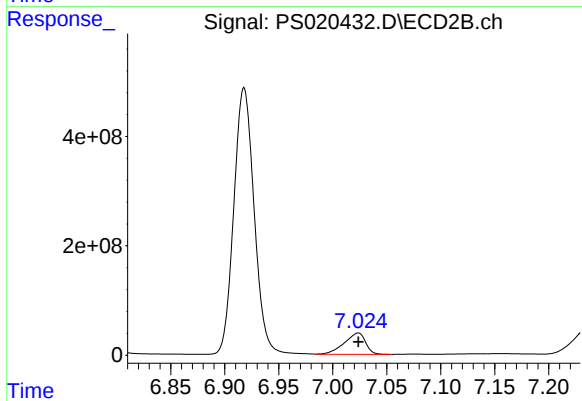

#6 MCP


R.T.: 7.024 min
Delta R.T.: 0.000 min
Response: 539607764
Conc: 144.29 ug/ml

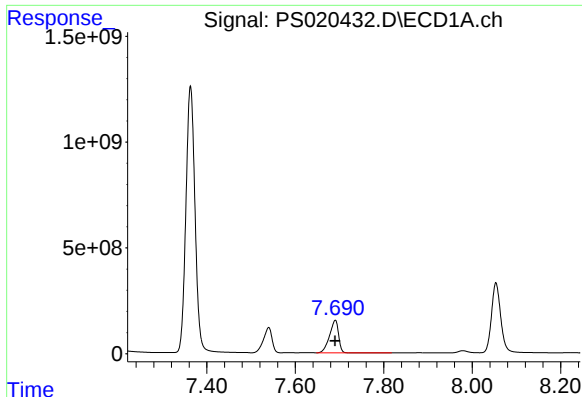

#7 MCPA


R.T.: 7.690 min
Delta R.T.: 0.000 min
Response: 2184407846
Conc: 141.46 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

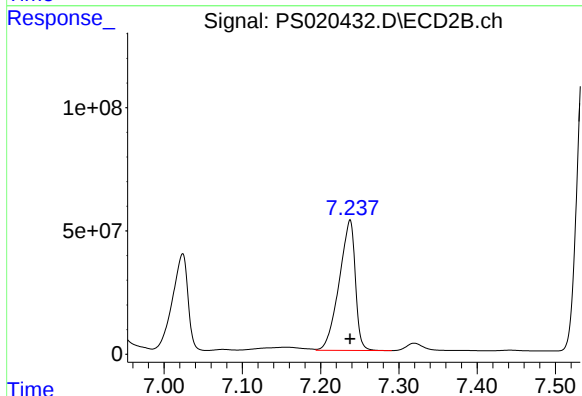


#7 MCPA

R.T.: 7.238 min
Delta R.T.: 0.000 min
Response: 758433324
Conc: 141.45 ug/ml

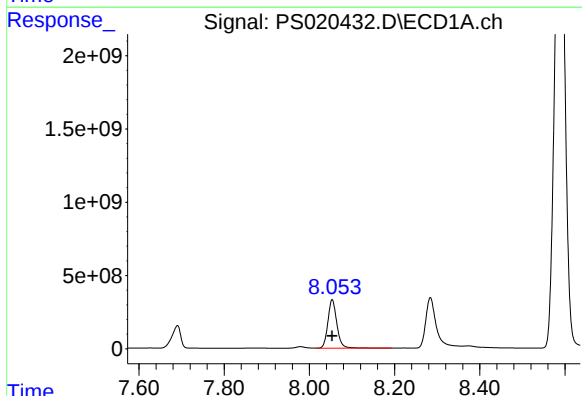


#8 DICHLORPROP

R.T.: 8.054 min
Delta R.T.: 0.000 min
Response: 4833855939
Conc: 1386.13 ng/ml

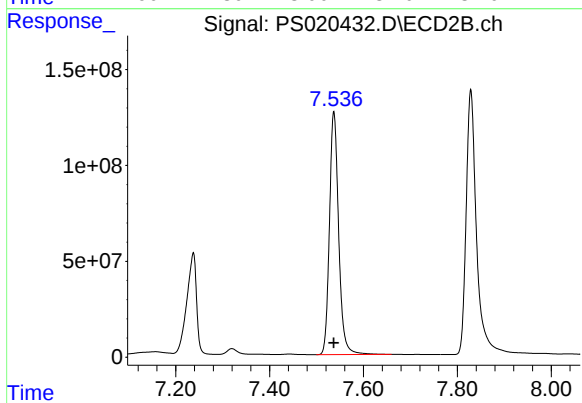

#8 DICHLORPROP


R.T.: 7.537 min
Delta R.T.: 0.000 min
Response: 1720262761
Conc: 1410.46 ng/ml

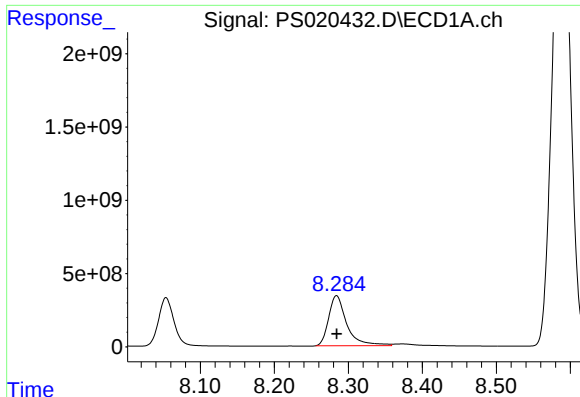

#9 2,4-D


R.T.: 8.284 min
Delta R.T.: 0.000 min
Response: 5809122192
Conc: 1330.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

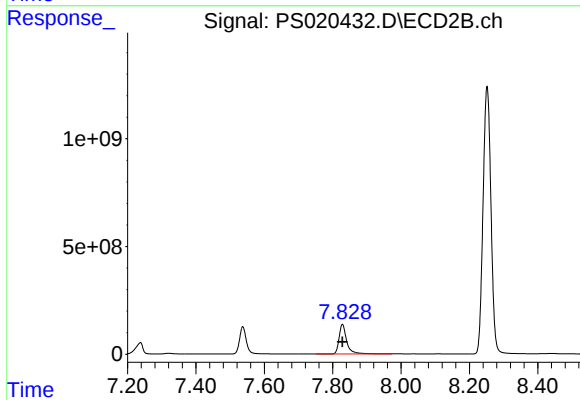


#9 2,4-D

R.T.: 7.829 min
Delta R.T.: 0.000 min
Response: 2126729404
Conc: 1419.14 ng/ml

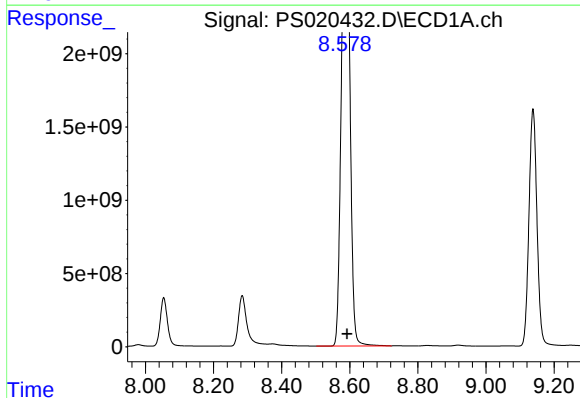


#10 Pentachlorophenol

R.T.: 8.592 min
Delta R.T.: 0.000 min
Response: 46393489964
Conc: 1162.42 ng/ml

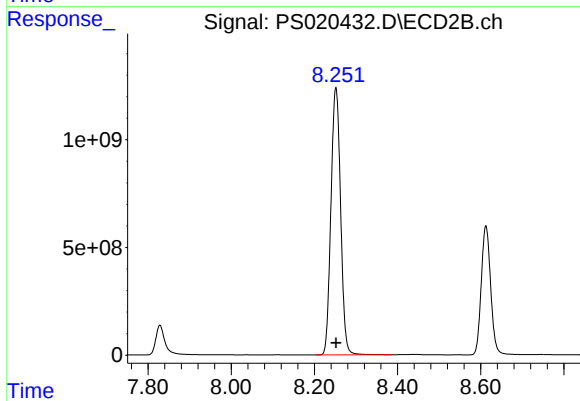

#10 Pentachlorophenol


R.T.: 8.252 min
Delta R.T.: 0.000 min
Response: 19945882353
Conc: 1307.64 ng/ml

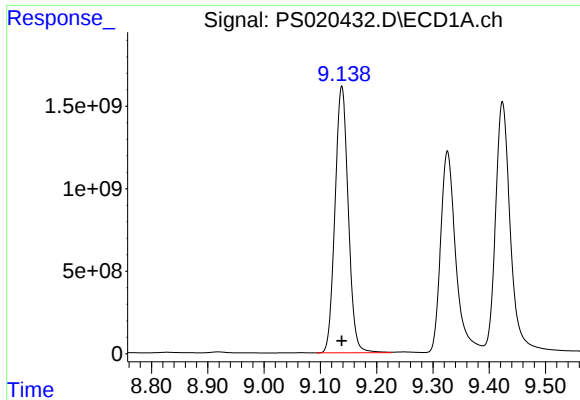

#11 2,4,5-TP (SILVEX)


R.T.: 9.138 min
Delta R.T.: 0.000 min
Response: 26438335001
Conc: 1353.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

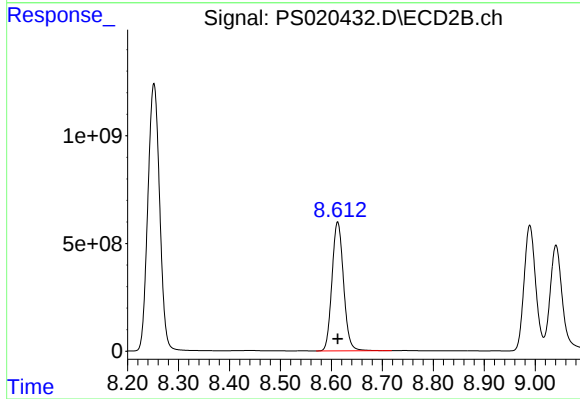


#11 2,4,5-TP (SILVEX)

R.T.: 8.612 min
Delta R.T.: 0.000 min
Response: 9424852122
Conc: 1373.02 ng/ml

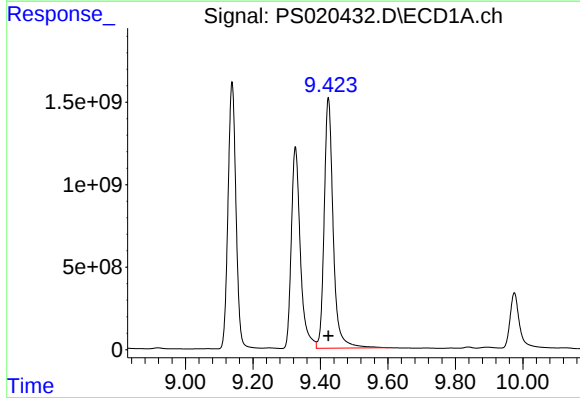


#12 2,4,5-T

R.T.: 9.424 min
Delta R.T.: 0.000 min
Response: 28216157433
Conc: 1337.60 ng/ml

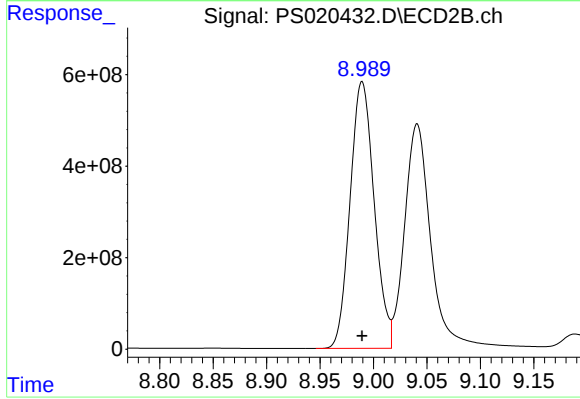

#12 2,4,5-T


R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 9148568961
Conc: 1390.35 ng/ml

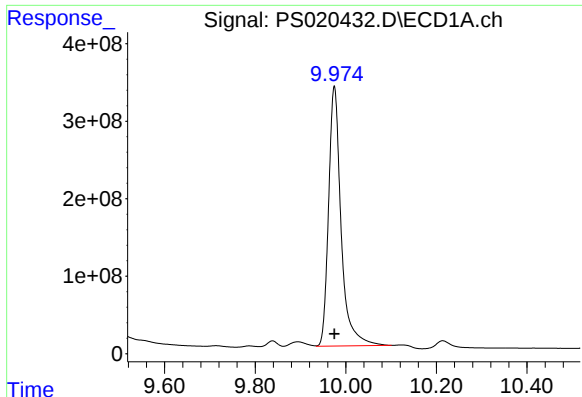

#13 2,4-DB


R.T.: 9.975 min
Delta R.T.: 0.000 min
Response: 6430143618
Conc: 1449.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

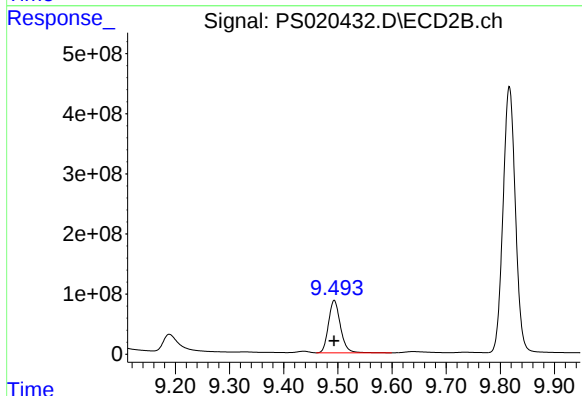


#13 2,4-DB

R.T.: 9.493 min
Delta R.T.: 0.000 min
Response: 1331493066
Conc: 1461.59 ng/ml

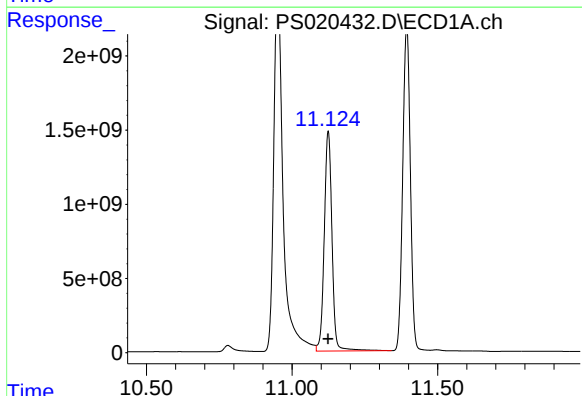


#14 DINOSEB

R.T.: 11.124 min
Delta R.T.: 0.000 min
Response: 27376401399
Conc: 1322.02 ng/ml

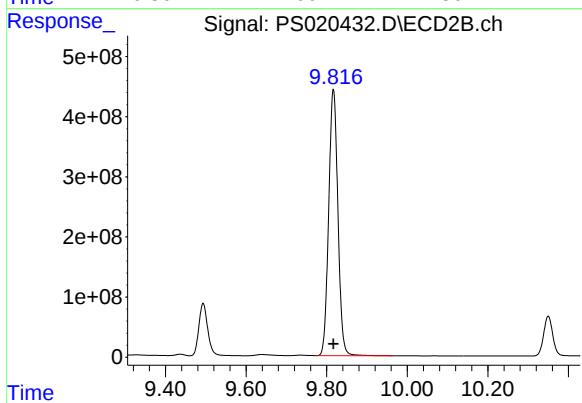

#14 DINOSEB


R.T.: 9.817 min
Delta R.T.: 0.000 min
Response: 7013102583
Conc: 1382.98 ng/ml

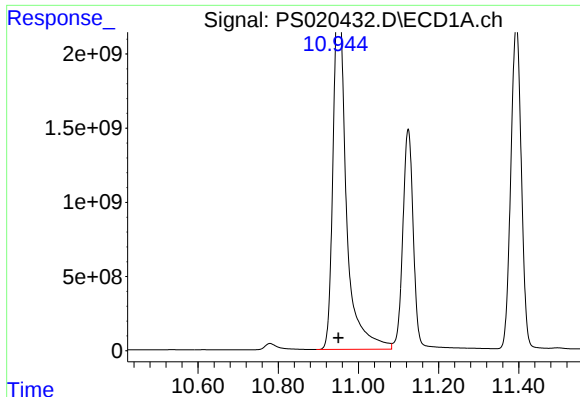

#15 Picloram


R.T.: 10.950 min
Delta R.T.: 0.000 min
Response: 53396527319
Conc: 1357.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

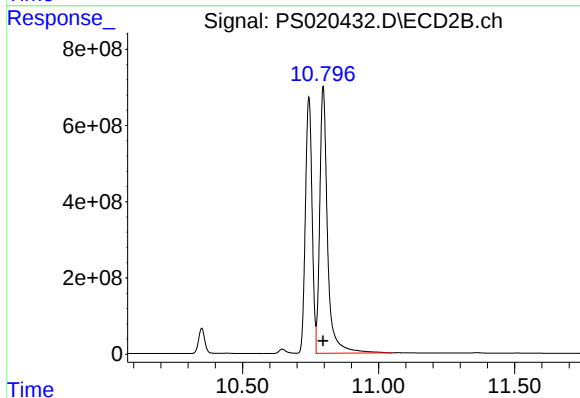


#15 Picloram

R.T.: 10.796 min
Delta R.T.: 0.000 min
Response: 13999929070
Conc: 1399.07 ng/ml

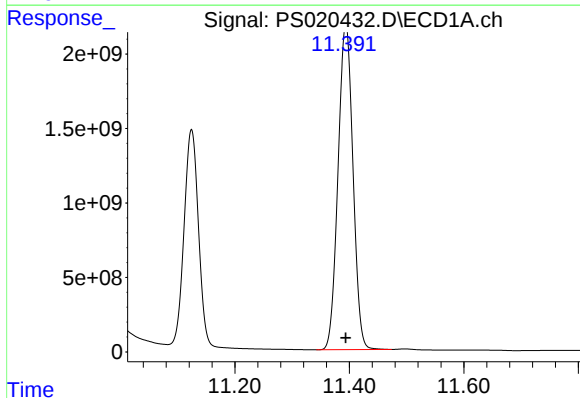

#16 DCPA

R.T.: 11.394 min
Delta R.T.: 0.000 min
Response: 39467261867
Conc: 1356.08 ng/ml

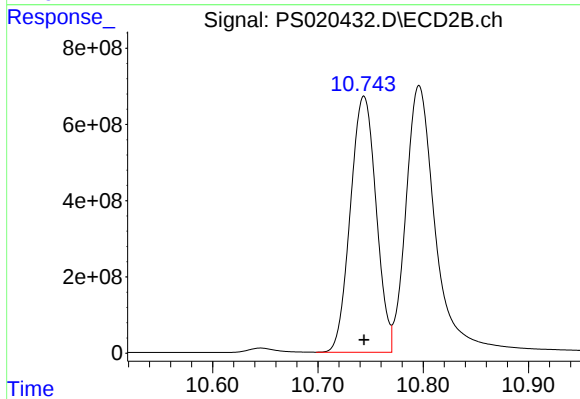

#16 DCPA

R.T.: 10.744 min
Delta R.T.: 0.000 min
Response: 11411395042
Conc: 1375.14 ng/ml