

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090320\
 Data File : PS012079.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2020 12:10
 Operator : DD\AJ
 Sample : L3852-06RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 13:20:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.916	211.3E6	132.9E6	193.707	248.451 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	75574188	N.D.	91.870
3) T	4-Nitroph...	7.056	0.000	3402835	0	5.777	N.D. #
5) T	DICAMBA	7.396	7.048	7260261	8714694	1.773	4.034 #
6) T	MCP	7.628	0.000	7119607	0	2.228	N.D. #
7) T	MCPA	7.695	7.472	205.1E6	103.6E6	45.092	37.793
8) T	DICHLORPROP	0.000	7.739	0	28984695	N.D.	51.333
9) T	2,4-D	8.399	0.000	24234923	0	21.464	N.D. #
12) T	2,4,5-T	9.411	0.000	22873222	0	3.860	N.D. #
13) T	2,4-DB	9.981	0.000	9139931	0	11.503	N.D. #
16) T	DCPA	11.468	0.000	10160712	0	1.336	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090320\
Data File : PS012079.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2020 12:10
Operator : DD\AJ
Sample : L3852-06RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 13:20:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

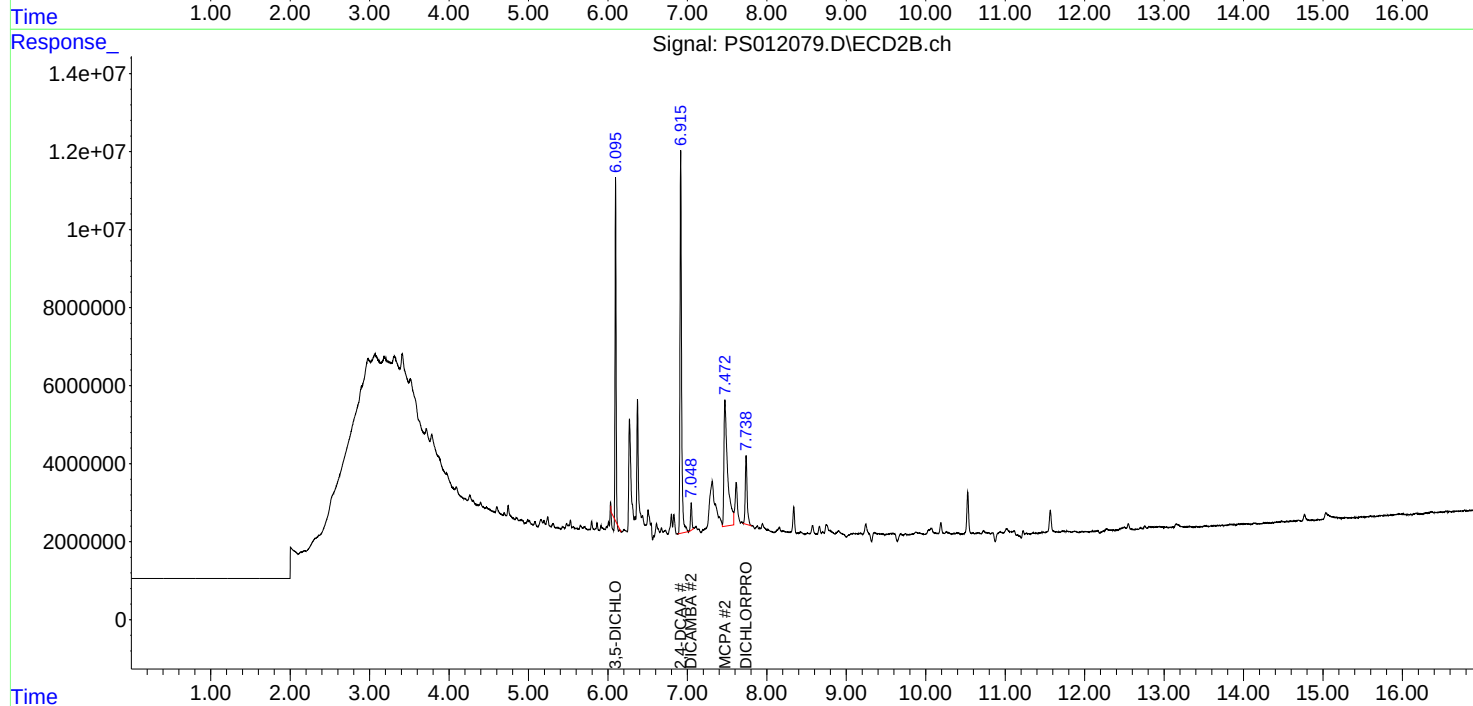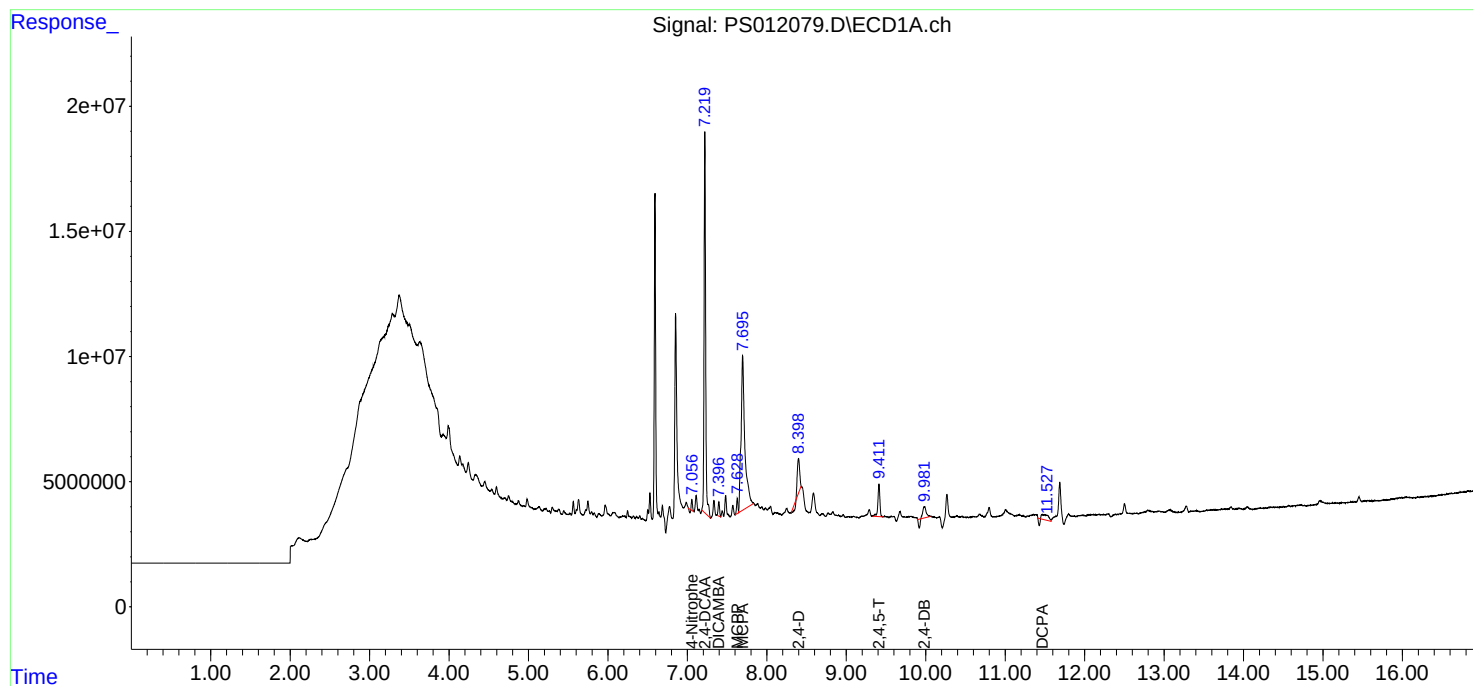


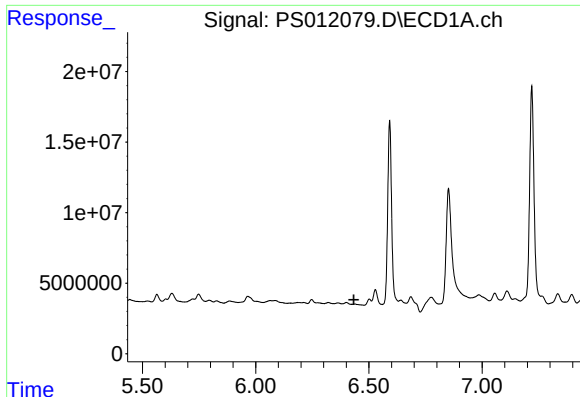

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

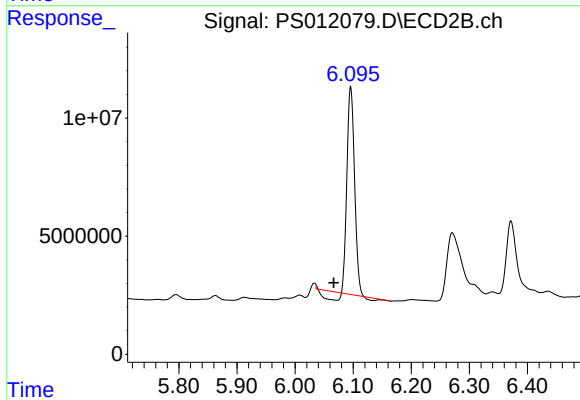


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 75574188
Conc: 91.87 ng/ml

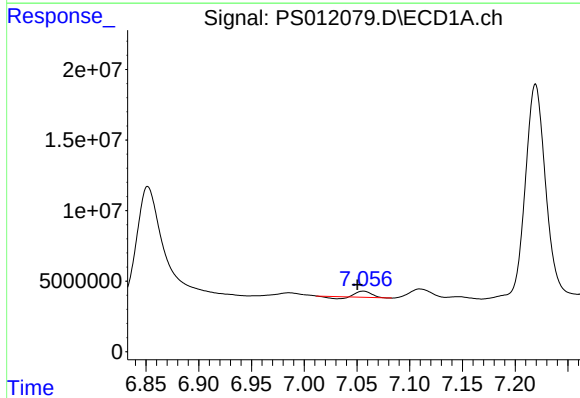


#3 4-Nitrophenol

R.T.: 7.056 min
Delta R.T.: 0.006 min
Response: 3402835
Conc: 5.78 ng/ml

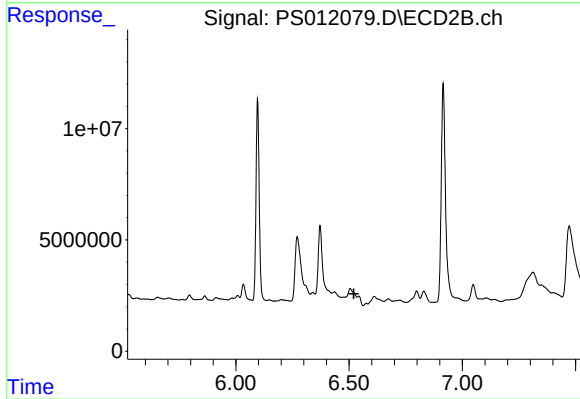

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

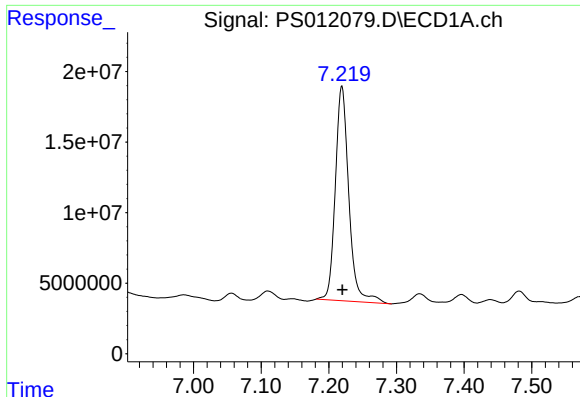

#4 2,4-DCAA


R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 211289229
Conc: 193.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

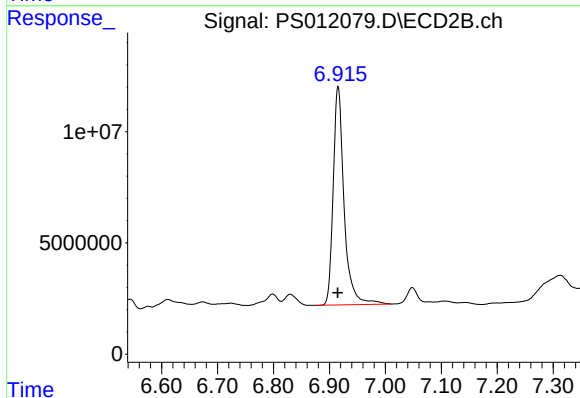


#4 2,4-DCAA

R.T.: 6.916 min
Delta R.T.: 0.000 min
Response: 132868061
Conc: 248.45 ng/ml

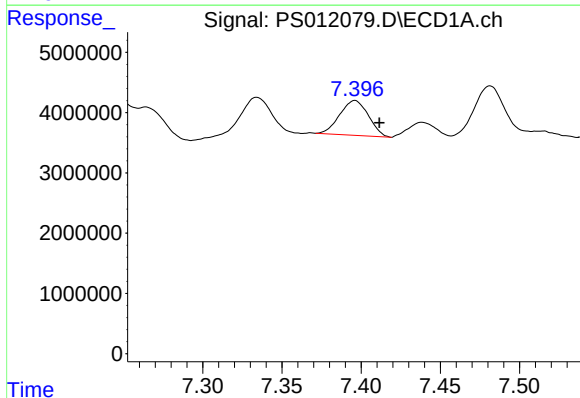


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.015 min
Response: 7260261
Conc: 1.77 ng/ml

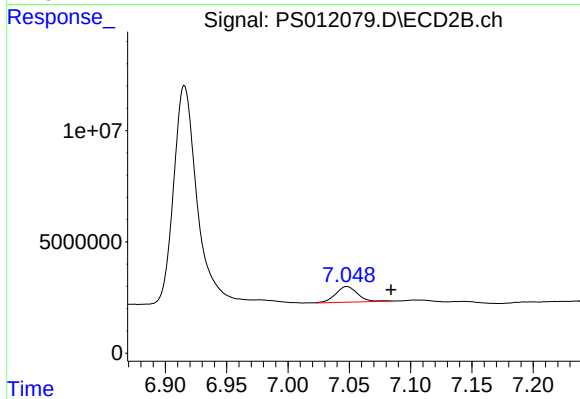

#5 DICAMBA


R.T.: 7.048 min
Delta R.T.: -0.036 min
Response: 8714694
Conc: 4.03 ng/ml

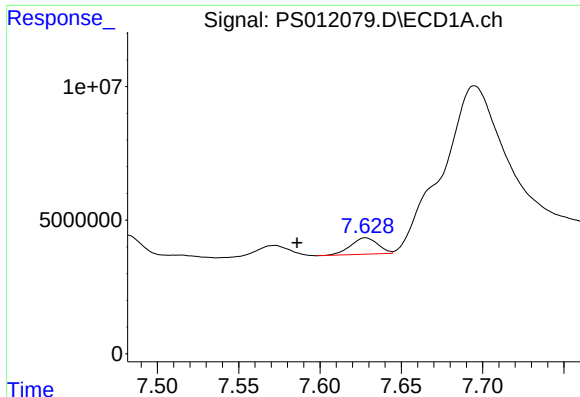

#6 MCPP


R.T.: 7.628 min
Delta R.T.: 0.042 min
Response: 7119607
Conc: 2.23 ug/ml

Instrument :
ECD_S
ClientSampleId :

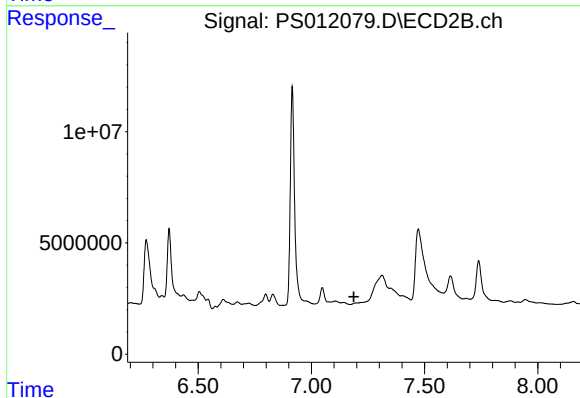


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

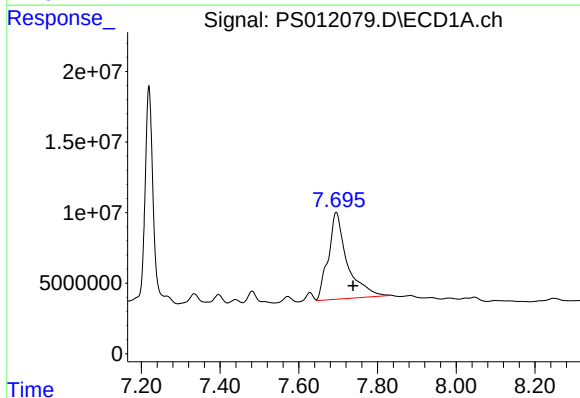


#7 MCPA

R.T.: 7.695 min
Delta R.T.: -0.043 min
Response: 205100087
Conc: 45.09 ug/ml

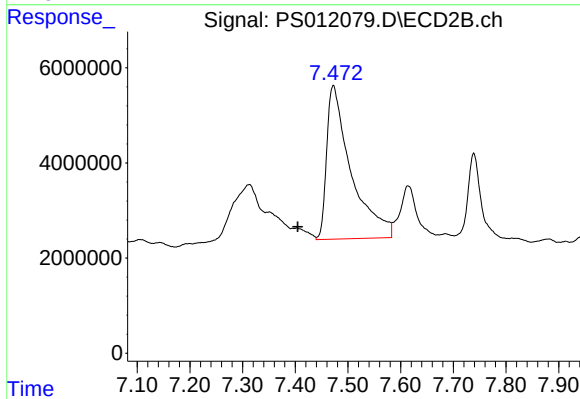

#7 MCPA


R.T.: 7.472 min
Delta R.T.: 0.067 min
Response: 103559329
Conc: 37.79 ug/ml

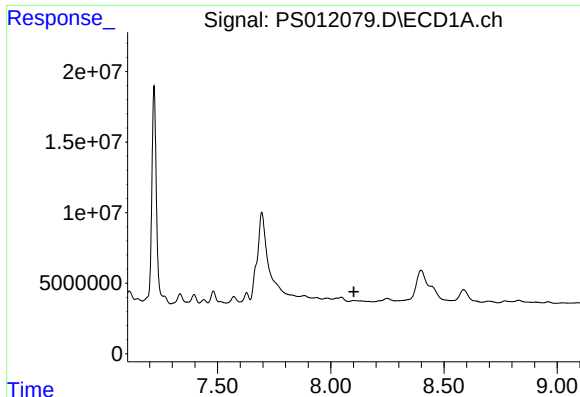

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

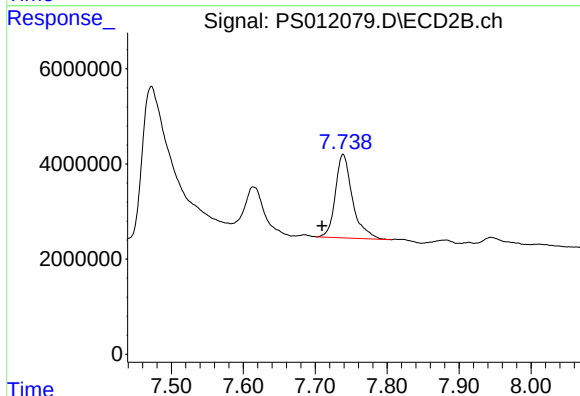


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.029 min
Response: 28984695
Conc: 51.33 ng/ml

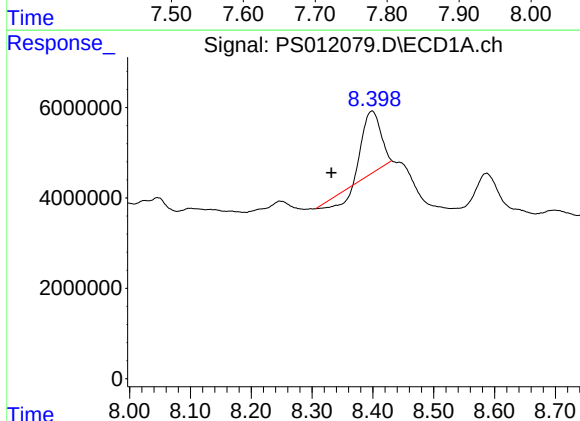


#9 2,4-D

R.T.: 8.399 min
Delta R.T.: 0.067 min
Response: 24234923
Conc: 21.46 ng/ml

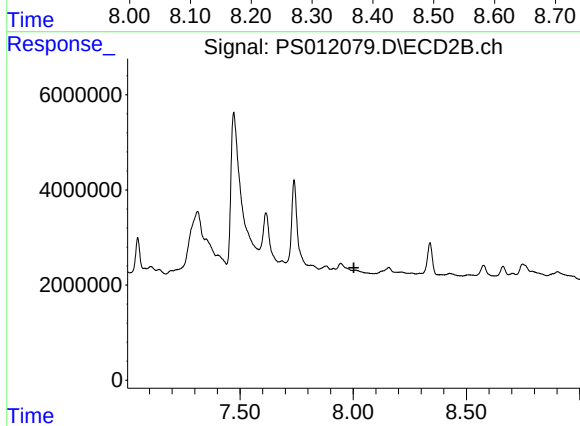

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

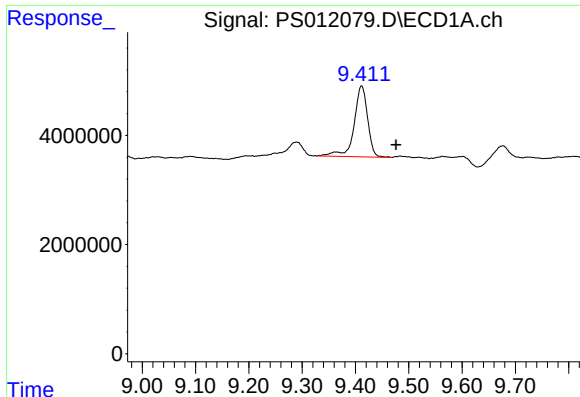

#12 2,4,5-T


R.T.: 9.411 min
Delta R.T.: -0.064 min
Response: 22873222
Conc: 3.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

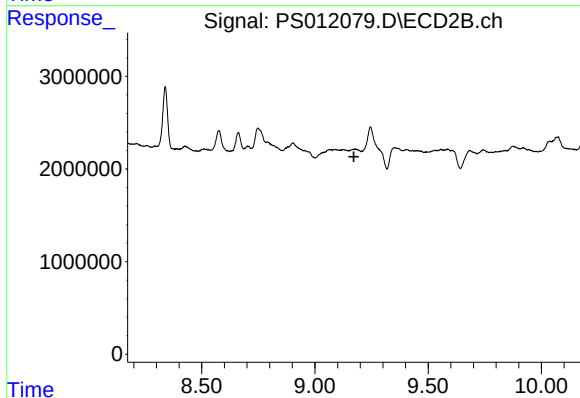


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

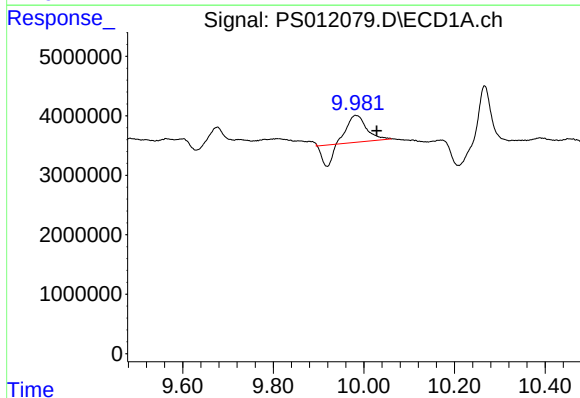


#13 2,4-DB

R.T.: 9.981 min
Delta R.T.: -0.047 min
Response: 9139931
Conc: 11.50 ng/ml

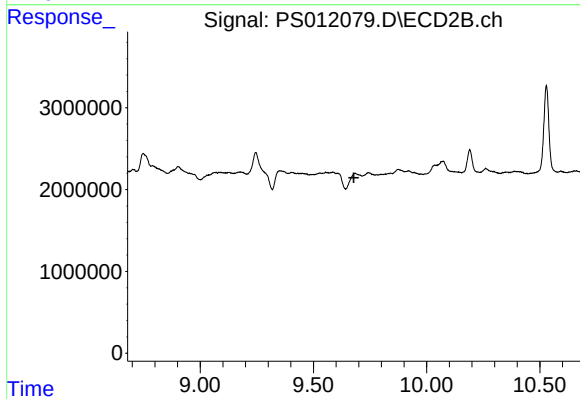

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.679 min
Response: 0
Conc: N.D.

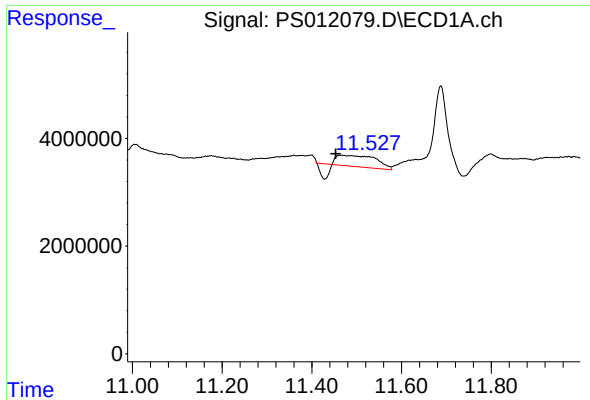

#16 DCPA

R.T.: 11.468 min
Delta R.T.: 0.014 min
Response: 10160712
Conc: 1.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

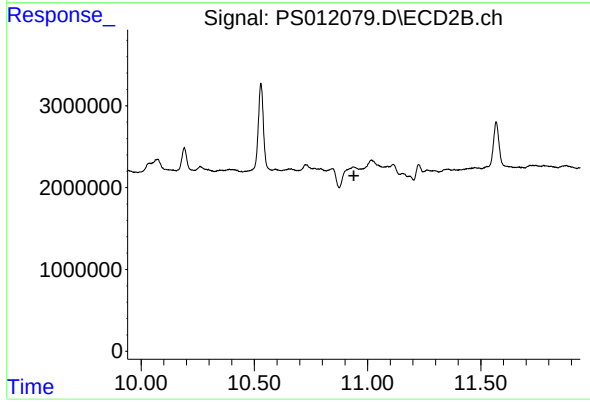

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.940 min
Response: 0
Conc: N.D.