

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090320\
 Data File : PS012080.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2020 12:33
 Operator : DD\AJ
 Sample : L3837-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 13:20:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.218	6.915	311.2E6	190.7E6	285.289	356.584
Target Compounds							
1) T	Dalapon	2.999	2.587	33943431	69749825	27.249	92.280 #
2) T	3,5-DICHL...	0.000	6.096	0	64407921	N.D.	78.296
3) T	4-Nitroph...	7.109	0.000	12195848	0	20.705	N.D. #
5) T	DICAMBA	7.395	7.048	5794745	8258230	1.415	3.822 #
6) T	MCPD	7.570	0.000	8305351	0	2.599	N.D. #
7) T	MCPA	7.691	7.466	281.2E6	152.7E6	61.829	55.712
8) T	DICHLORPROP	0.000	7.738	0	37646221	N.D.	66.673
9) T	2,4-D	8.398	0.000	23836842	0	21.112	N.D. #
10) T	Pentachlo...	8.695	0.000	14079162	0	<MDL	N.D. #
12) T	2,4,5-T	9.412	0.000	40421703	0	6.821	N.D. #
13) T	2,4-DB	9.989	0.000	8712347	0	10.965	N.D. #
15) T	Picloram	10.978	0.000	17022398	0	2.178	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090320\
Data File : PS012080.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2020 12:33
Operator : DD\AJ
Sample : L3837-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 13:20:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

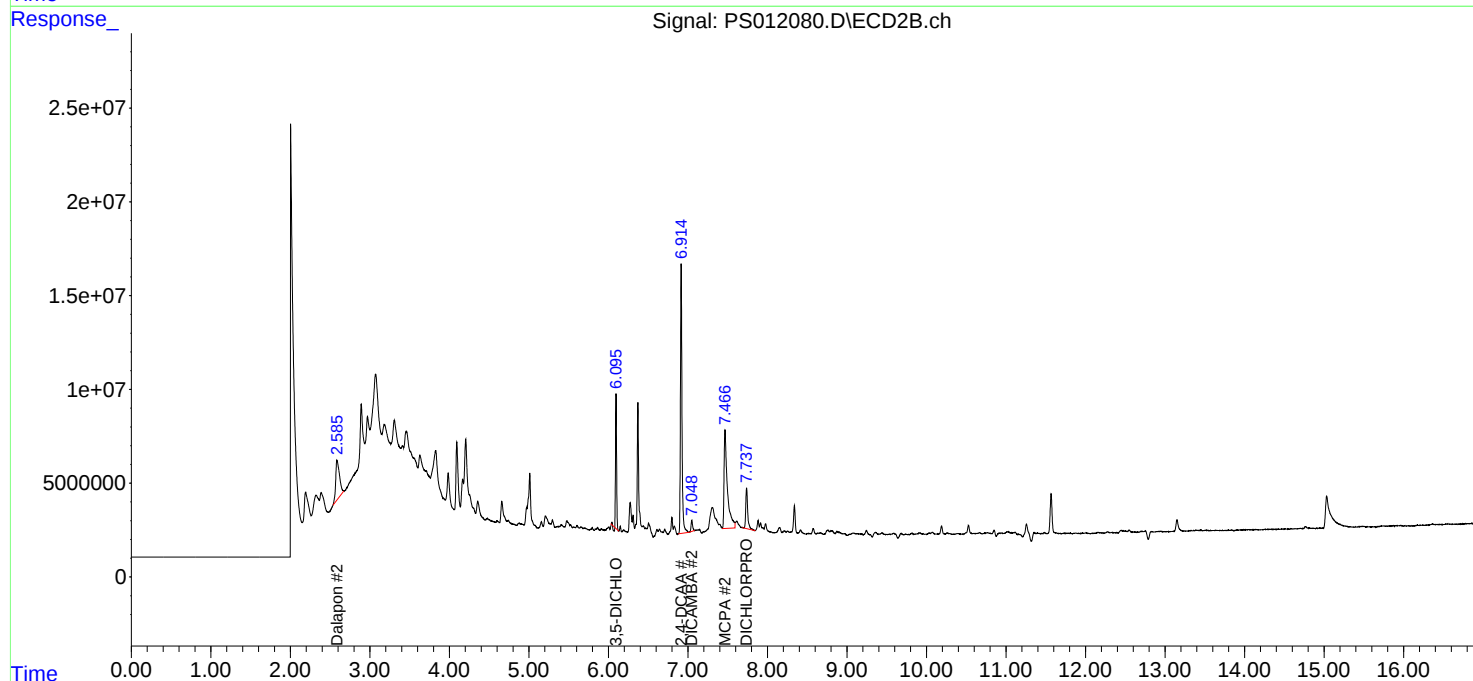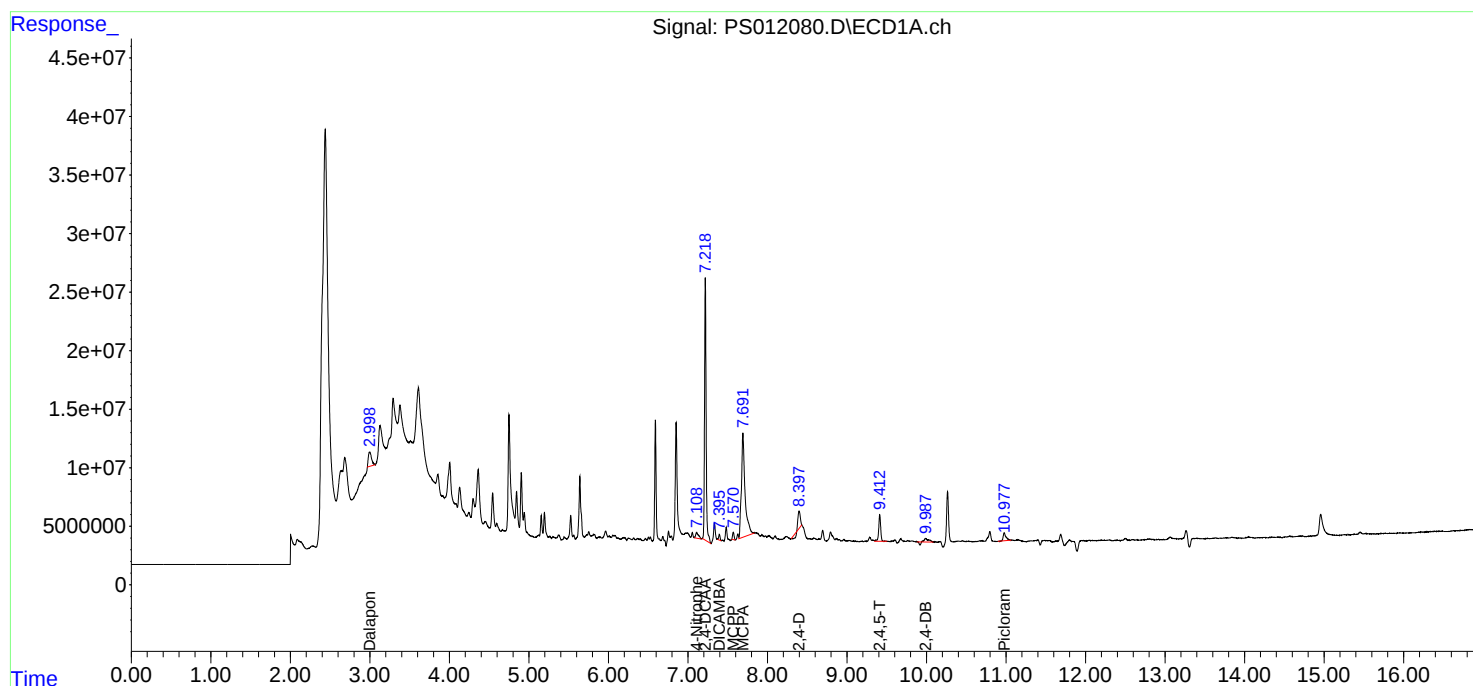


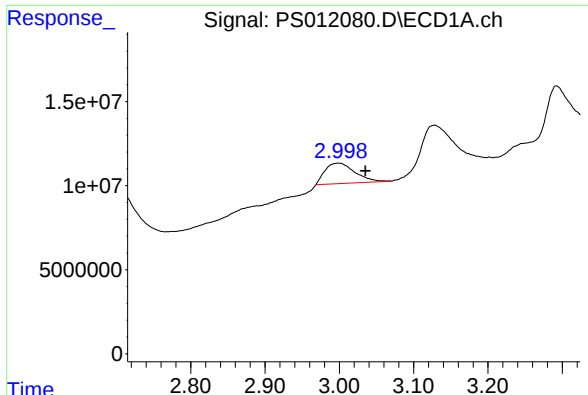

#1 Dalapon


R.T.: 2.999 min
Delta R.T.: -0.036 min
Response: 33943431
Conc: 27.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

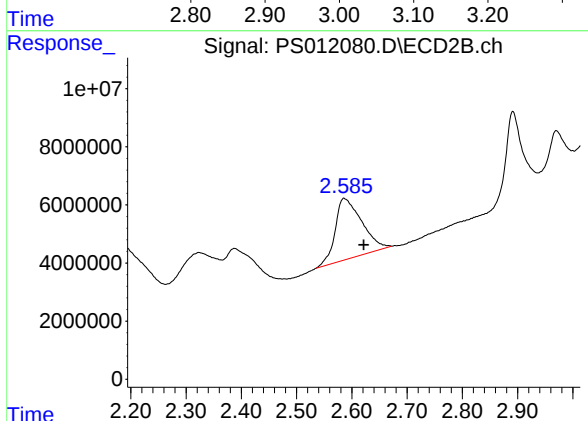


#1 Dalapon

R.T.: 2.587 min
Delta R.T.: -0.035 min
Response: 69749825
Conc: 92.28 ng/ml

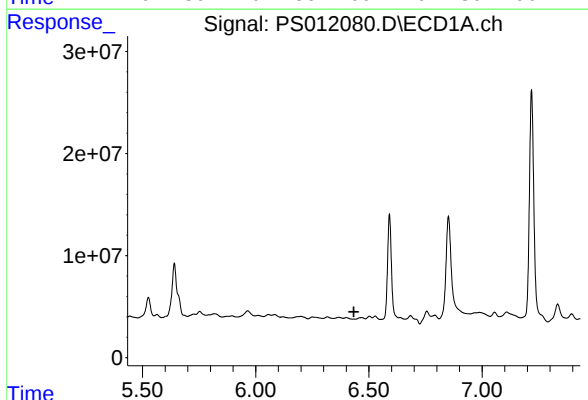


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

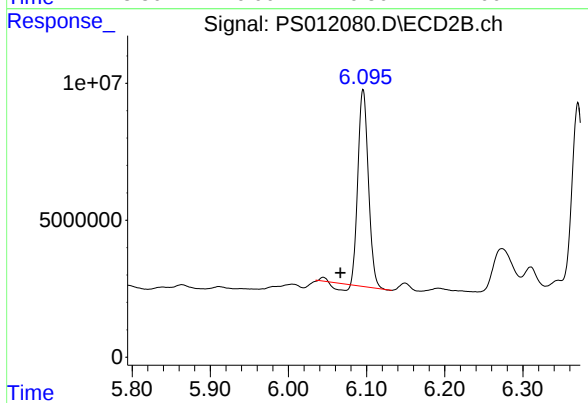

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 64407921
Conc: 78.30 ng/ml

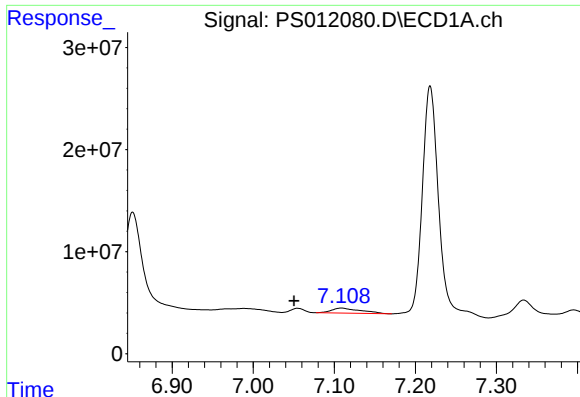

#3 4-Nitrophenol


R.T.: 7.109 min
Delta R.T.: 0.059 min
Response: 12195848
Conc: 20.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

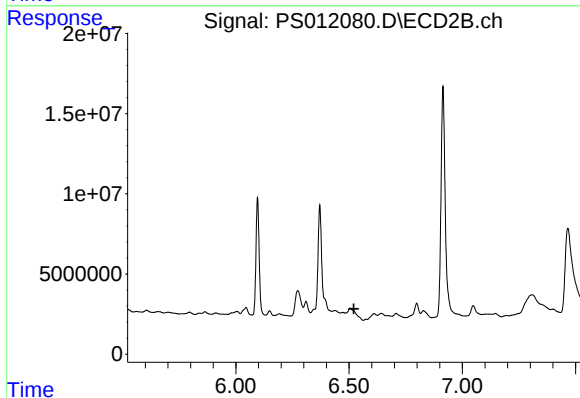


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.521 min
Response: 0
Conc: N.D.

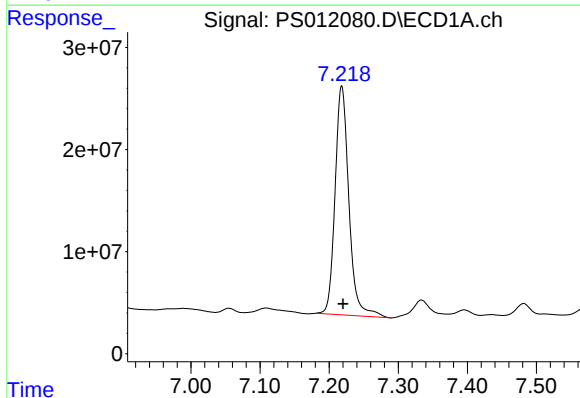


#4 2,4-DCAA

R.T.: 7.218 min
Delta R.T.: -0.002 min
Response: 311184415
Conc: 285.29 ng/ml

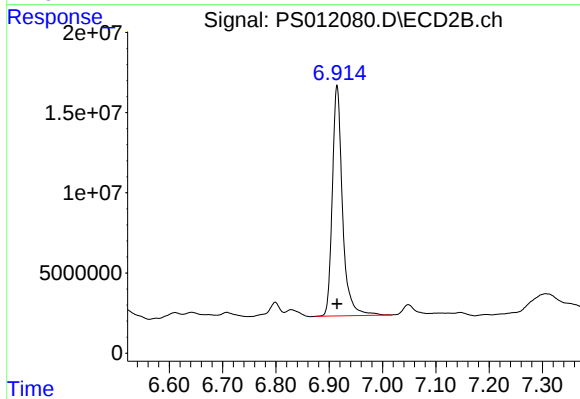

#4 2,4-DCAA


R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 190696479
Conc: 356.58 ng/ml

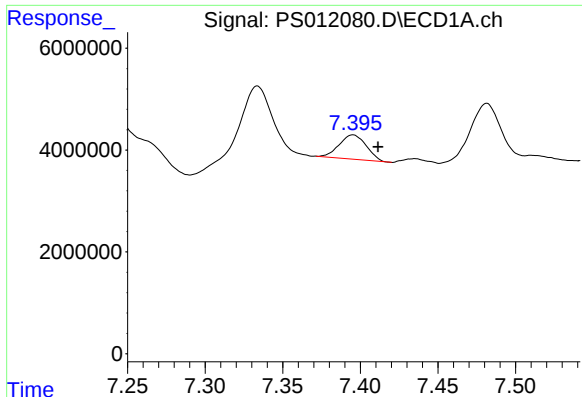

#5 DICAMBA


R.T.: 7.395 min
Delta R.T.: -0.016 min
Response: 5794745
Conc: 1.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

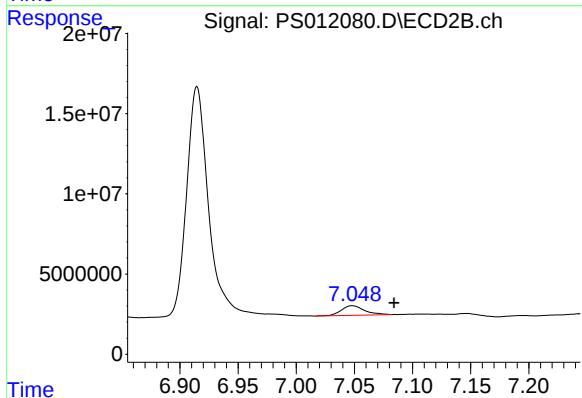


#5 DICAMBA

R.T.: 7.048 min
Delta R.T.: -0.036 min
Response: 8258230
Conc: 3.82 ng/ml

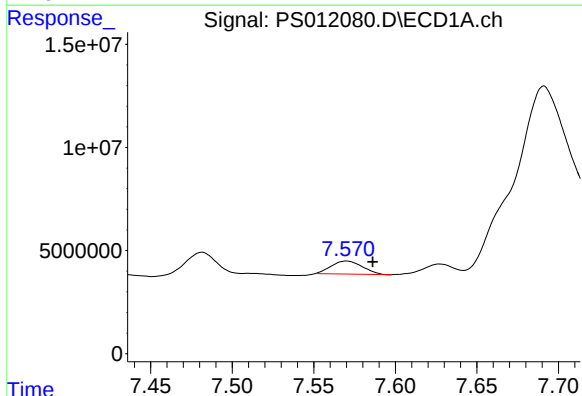


#6 MCP

R.T.: 7.570 min
Delta R.T.: -0.016 min
Response: 8305351
Conc: 2.60 ug/ml

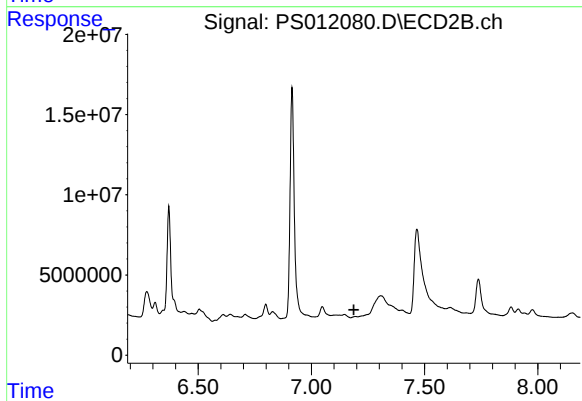

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

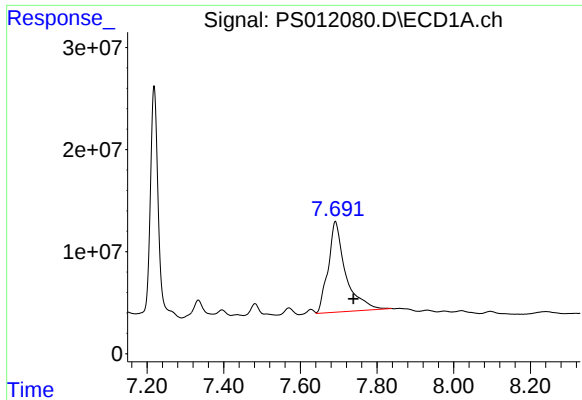

#7 MCPA


R.T.: 7.691 min
Delta R.T.: -0.047 min
Response: 281228614
Conc: 61.83 ug/ml

Instrument :
ECD_S
ClientSampleId :

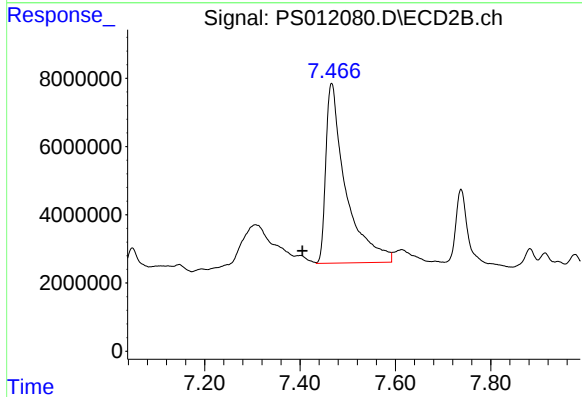


#7 MCPA

R.T.: 7.466 min
Delta R.T.: 0.061 min
Response: 152659783
Conc: 55.71 ug/ml

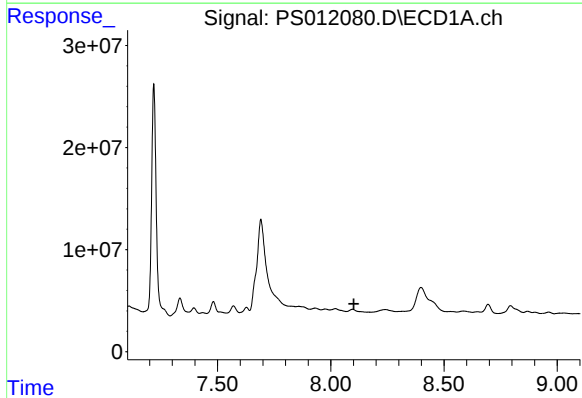


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

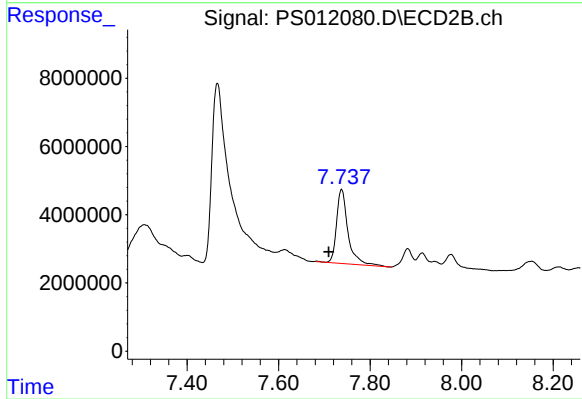

#8 DICHLORPROP


R.T.: 7.738 min
Delta R.T.: 0.028 min
Response: 37646221
Conc: 66.67 ng/ml

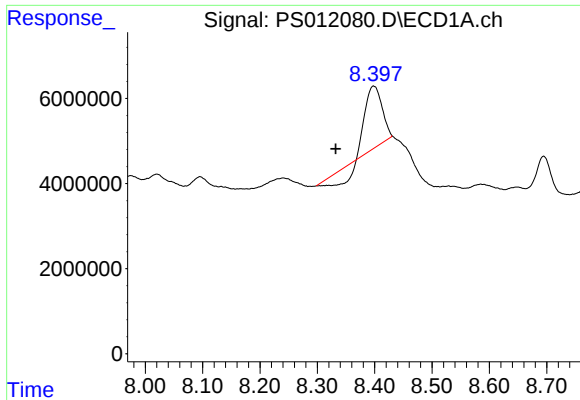

#9 2,4-D


R.T.: 8.398 min
Delta R.T.: 0.066 min
Response: 23836842
Conc: 21.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

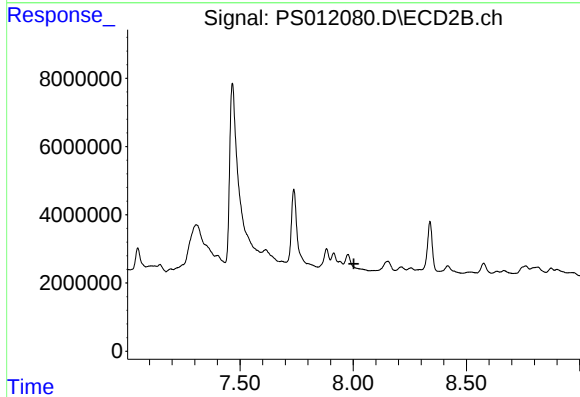


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

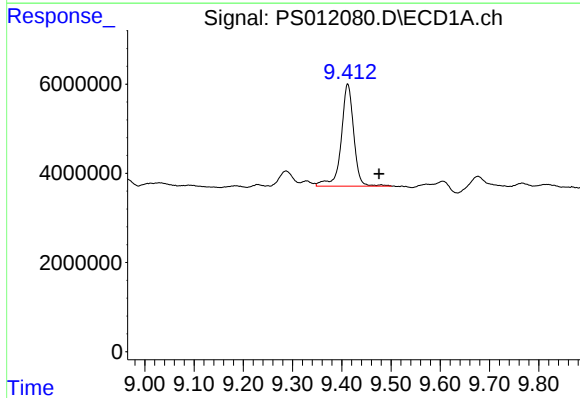


#12 2,4,5-T

R.T.: 9.412 min
Delta R.T.: -0.064 min
Response: 40421703
Conc: 6.82 ng/ml

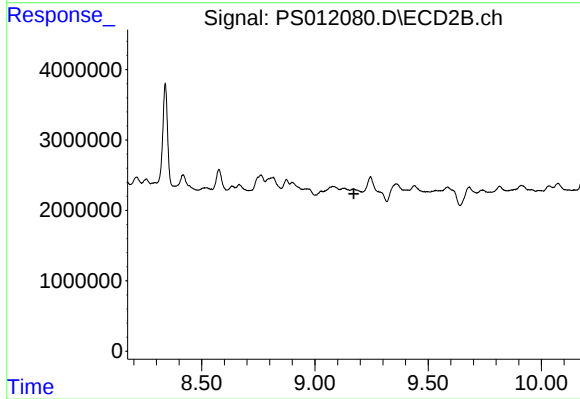

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

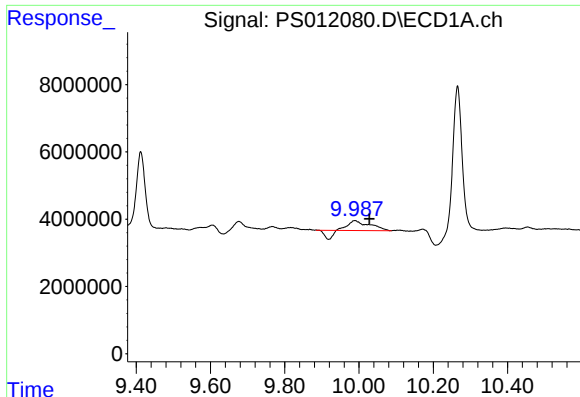

#13 2,4-DB


R.T.: 9.989 min
Delta R.T.: -0.039 min
Response: 8712347
Conc: 10.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

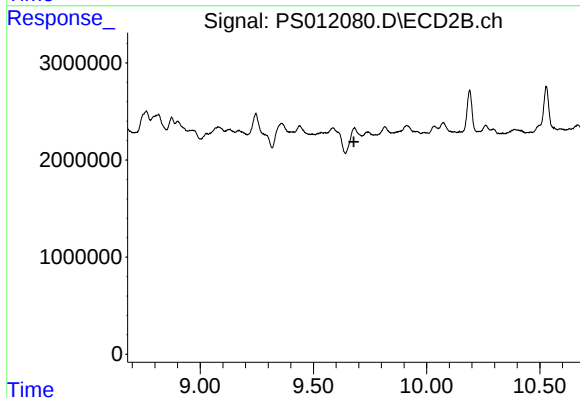


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.679 min
Response: 0
Conc: N.D.

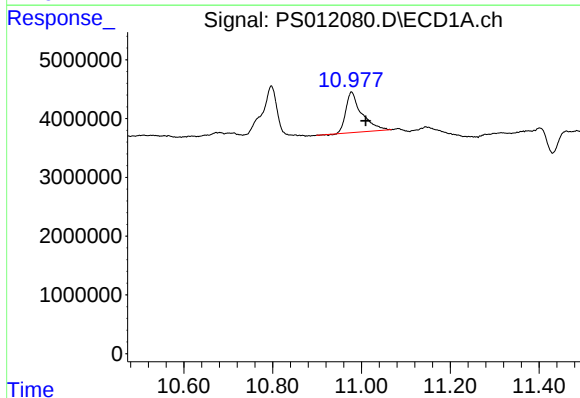

#15 Picloram

R.T.: 10.978 min
Delta R.T.: -0.032 min
Response: 17022398
Conc: 2.18 ng/ml

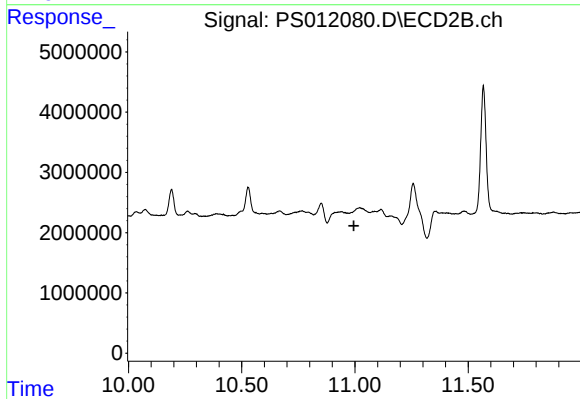

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.