

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090320\
 Data File : PS012083.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2020 13:42
 Operator : DD\AJ
 Sample : L3837-04RE
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 16:03:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	207.6E6	127.8E6	190.332	239.025 #
Target Compounds							
1) T	Dalapon	3.000	2.587	36915836	61592534	29.636	81.488 #
2) T	3,5-DICHL...	0.000	6.096	0	69770932	N.D.	84.816
3) T	4-Nitroph...	6.987	0.000	5388045	0	9.147	N.D. #
5) T	DICAMBA	7.396	7.049	6174512	8488476	1.507	3.929 #
6) T	MCPD	7.571	0.000	7805426	0	2.443	N.D. #
7) T	MCPA	7.698	7.472	216.1E6	94699699	47.513	34.560 #
8) T	DICHLORPROP	0.000	7.739	0	27978908	N.D.	49.552
9) T	2,4-D	8.398	0.000	24793932	0	21.959	N.D. #
10) T	Pentachlo...	8.695	0.000	13817806	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.789	0	190.2E6	N.D.	65.071
12) T	2,4,5-T	9.412	0.000	46132075	0	7.785	N.D. #
13) T	2,4-DB	9.988	0.000	37909677	0	47.710	N.D. #
15) T	Picloram	11.009	0.000	17046644	0	2.181	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090320\
Data File : PS012083.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2020 13:42
Operator : DD\AJ
Sample : L3837-04RE
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 16:03:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

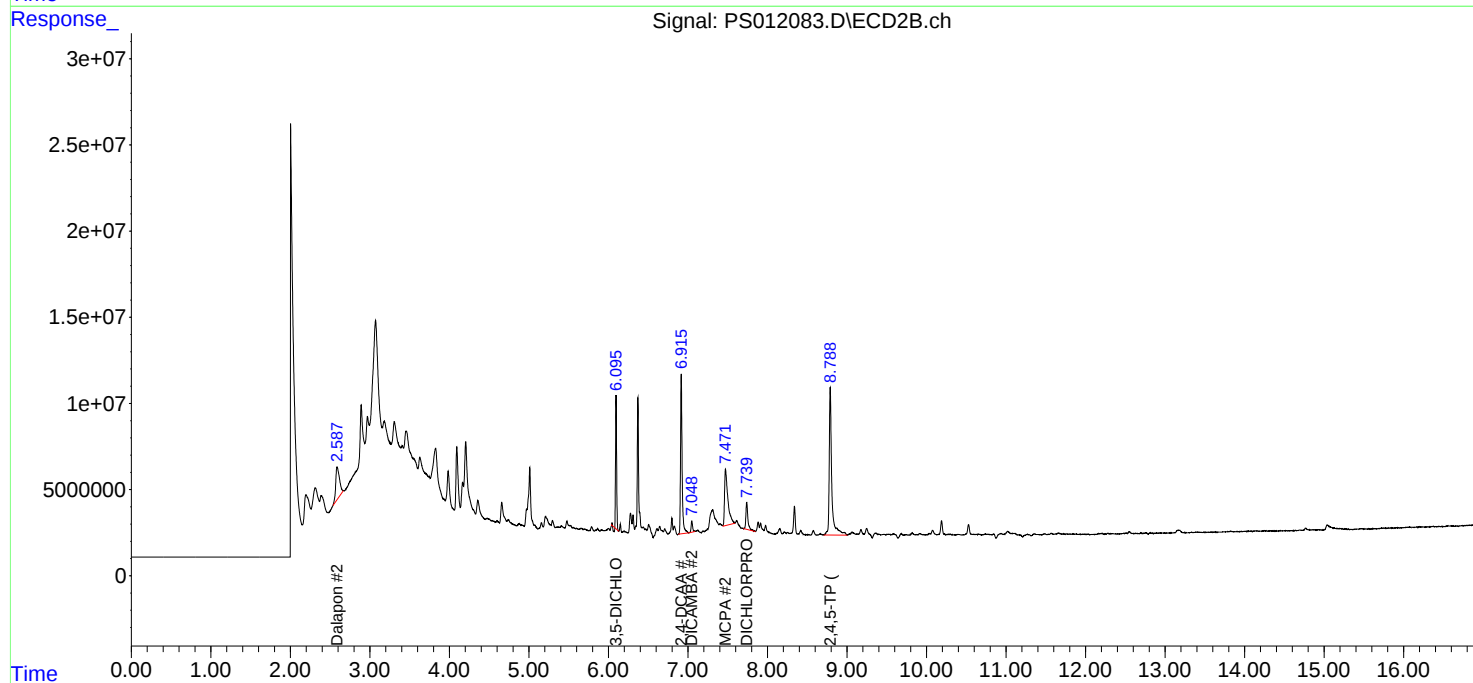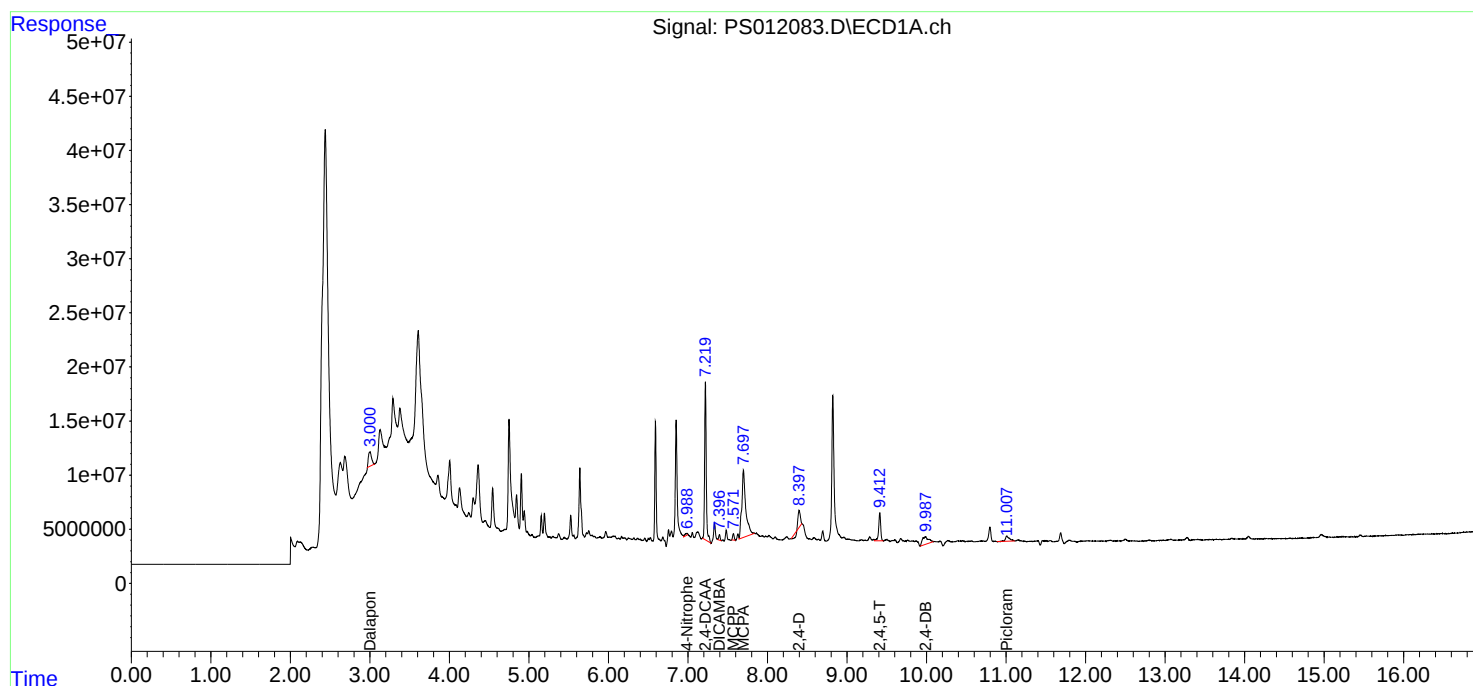


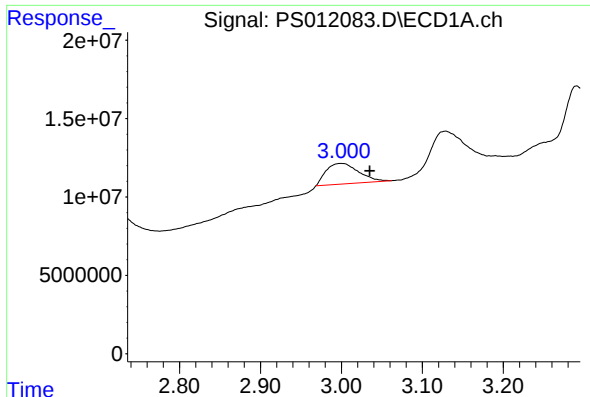

#1 Dalapon


R.T.: 3.000 min
Delta R.T.: -0.035 min
Response: 36915836
Conc: 29.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

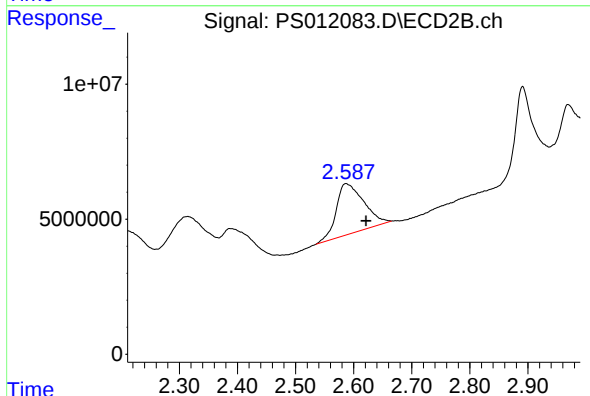


#1 Dalapon

R.T.: 2.587 min
Delta R.T.: -0.034 min
Response: 61592534
Conc: 81.49 ng/ml

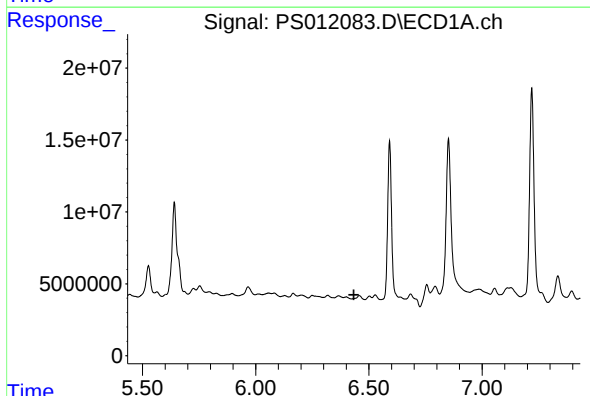


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

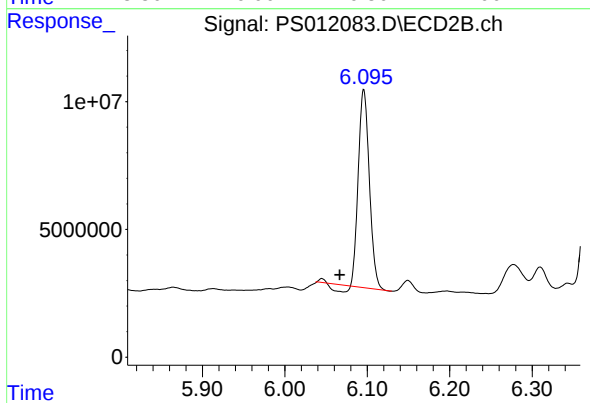

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 69770932
Conc: 84.82 ng/ml

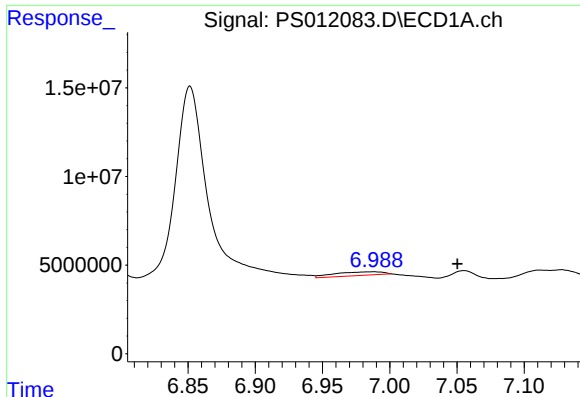

#3 4-Nitrophenol


R.T.: 6.987 min
Delta R.T.: -0.064 min
Response: 5388045
Conc: 9.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

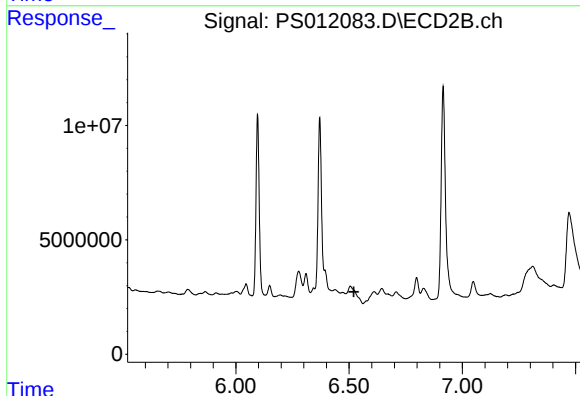


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.521 min
Response: 0
Conc: N.D.

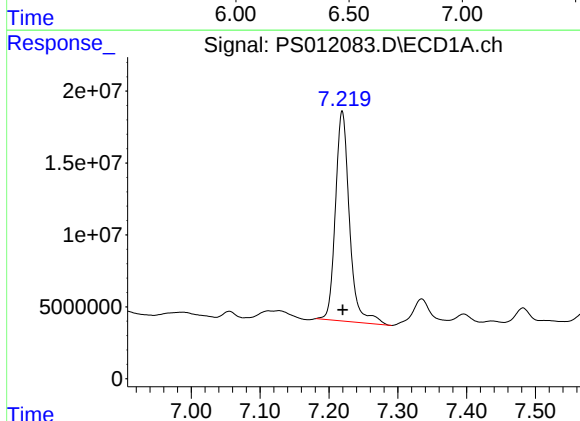


#4 2,4-DCAA

R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 207608055
Conc: 190.33 ng/ml

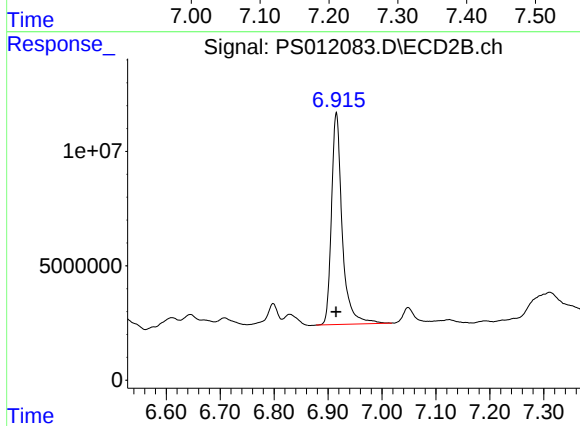

#4 2,4-DCAA


R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 127827393
Conc: 239.02 ng/ml

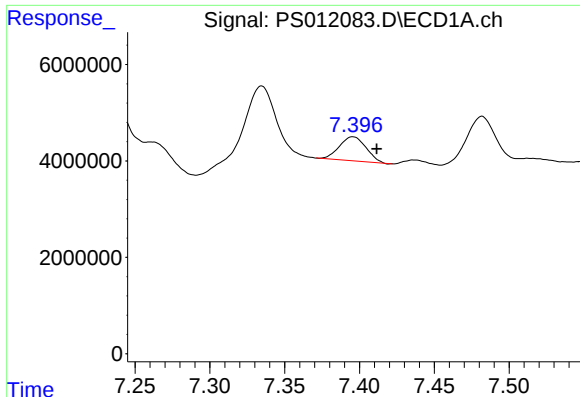

#5 DICAMBA


R.T.: 7.396 min
Delta R.T.: -0.016 min
Response: 6174512
Conc: 1.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

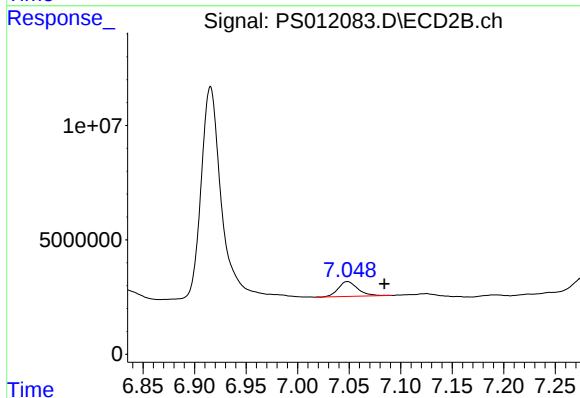


#5 DICAMBA

R.T.: 7.049 min
Delta R.T.: -0.036 min
Response: 8488476
Conc: 3.93 ng/ml

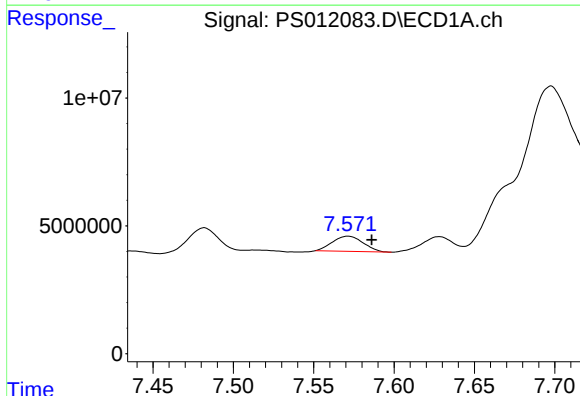


#6 MCPP

R.T.: 7.571 min
Delta R.T.: -0.015 min
Response: 7805426
Conc: 2.44 ug/ml

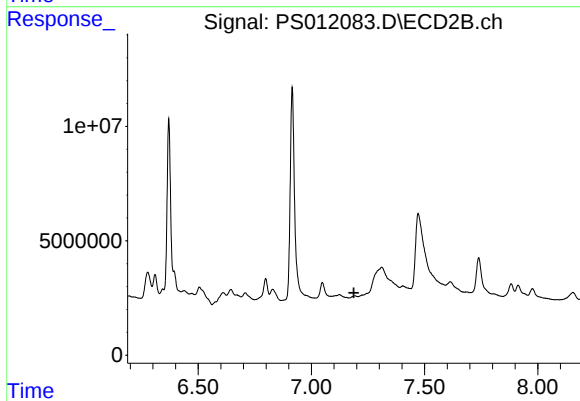

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

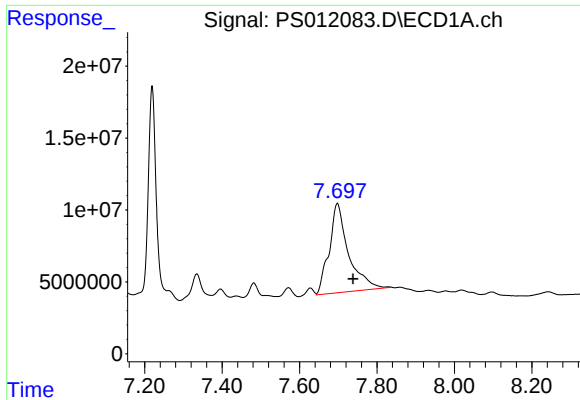

#7 MCPA


R.T.: 7.698 min
Delta R.T.: -0.041 min
Response: 216113364
Conc: 47.51 ug/ml

Instrument :
ECD_S
ClientSampleId :

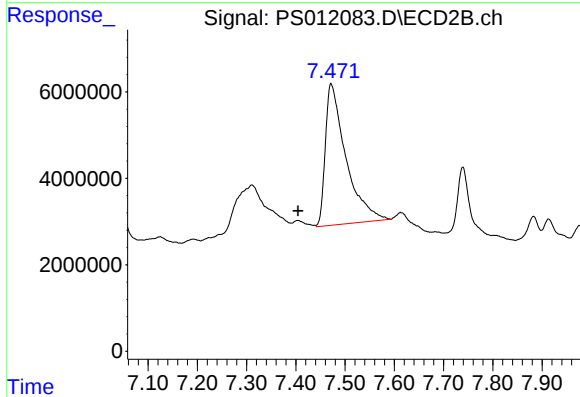


#7 MCPA

R.T.: 7.472 min
Delta R.T.: 0.067 min
Response: 94699699
Conc: 34.56 ug/ml

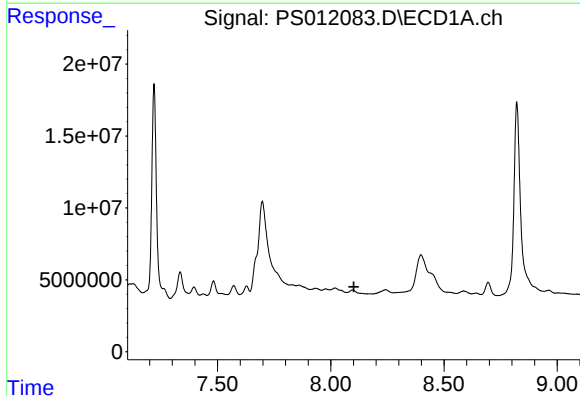


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

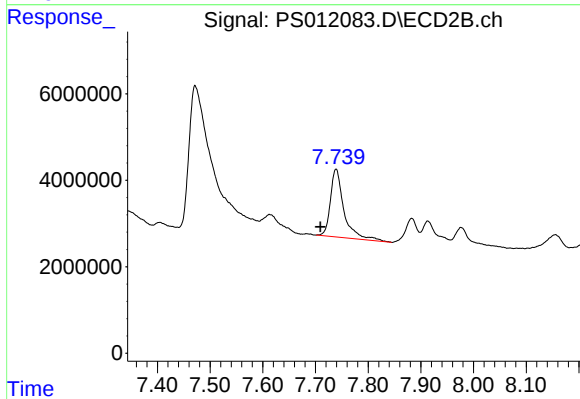

#8 DICHLORPROP


R.T.: 7.739 min
Delta R.T.: 0.030 min
Response: 27978908
Conc: 49.55 ng/ml

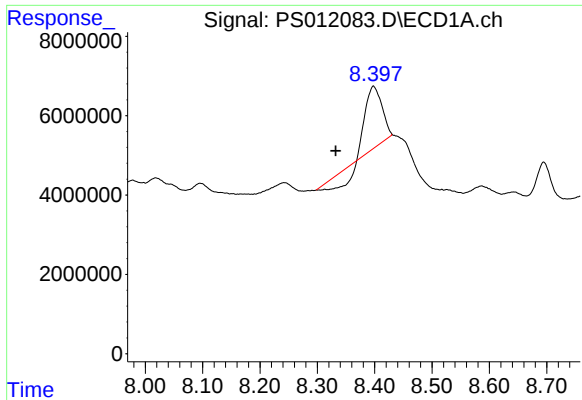

#9 2,4-D


R.T.: 8.398 min
Delta R.T.: 0.066 min
Response: 24793932
Conc: 21.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

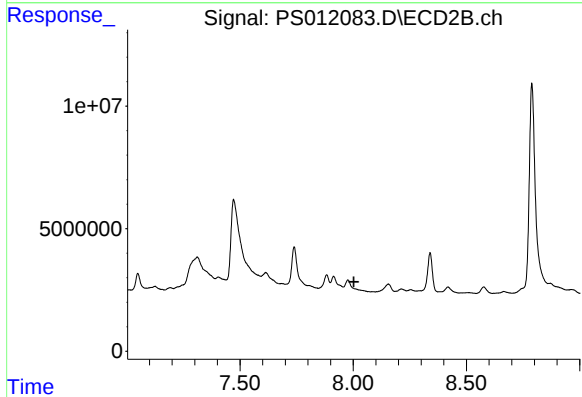


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

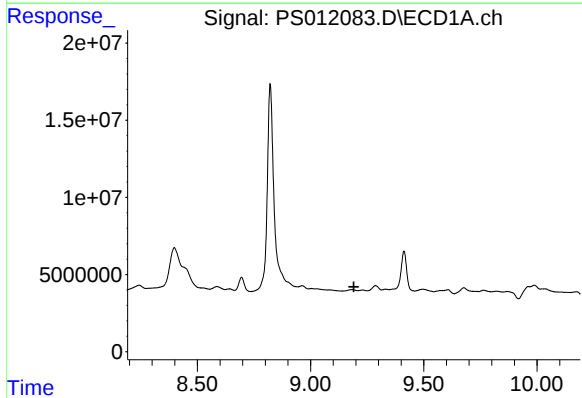


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

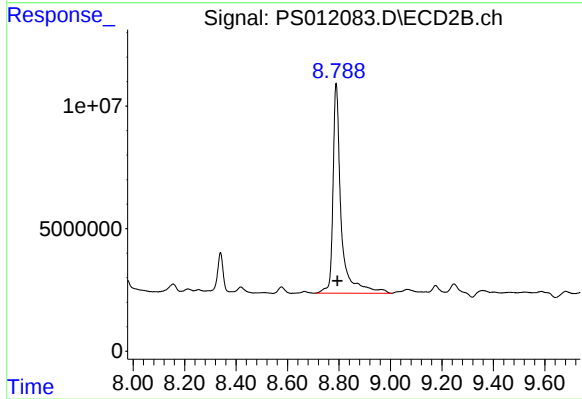

#11 2,4,5-TP (SILVEX)


R.T.: 8.789 min
Delta R.T.: -0.004 min
Response: 190243345
Conc: 65.07 ng/ml

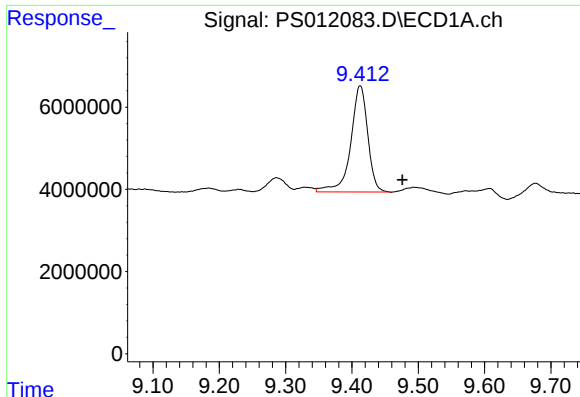

#12 2,4,5-T


R.T.: 9.412 min
Delta R.T.: -0.063 min
Response: 46132075
Conc: 7.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

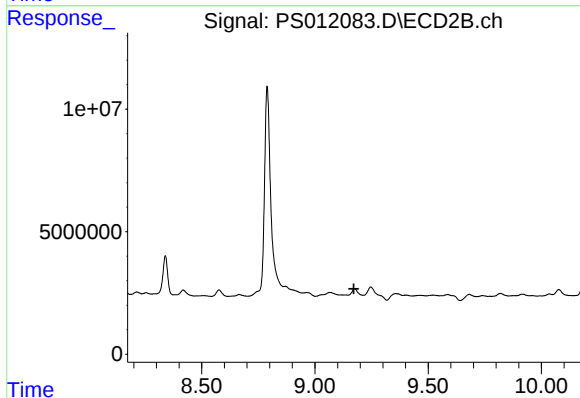


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

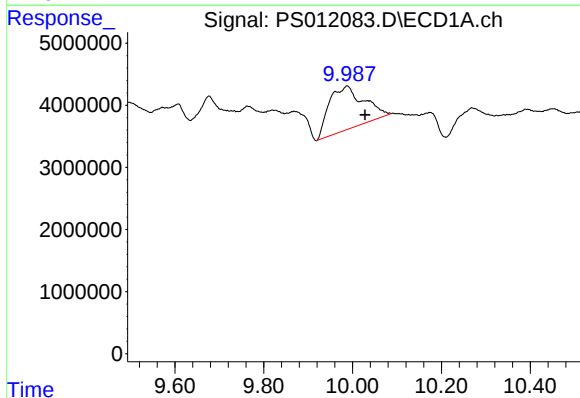


#13 2,4-DB

R.T.: 9.988 min
Delta R.T.: -0.040 min
Response: 37909677
Conc: 47.71 ng/ml

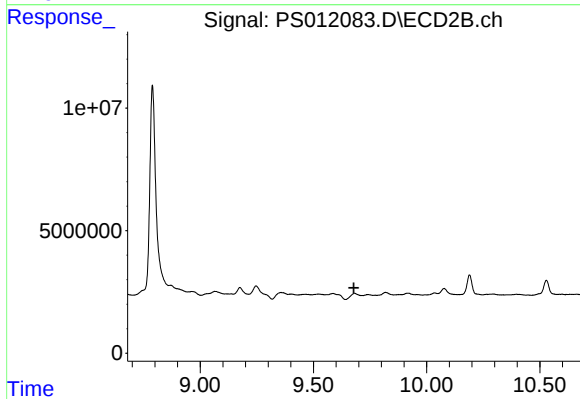

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.679 min
Response: 0
Conc: N.D.

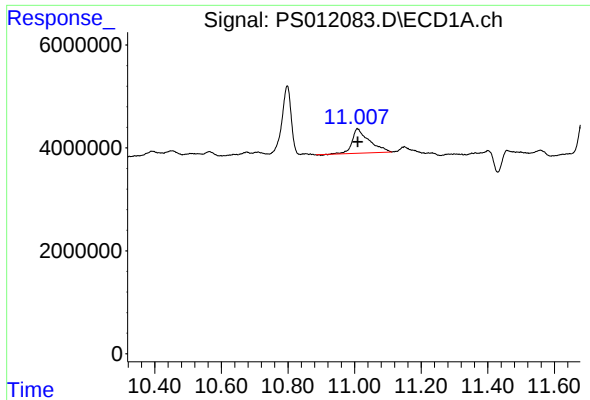

#15 Picloram

R.T.: 11.009 min
Delta R.T.: 0.000 min
Response: 17046644
Conc: 2.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

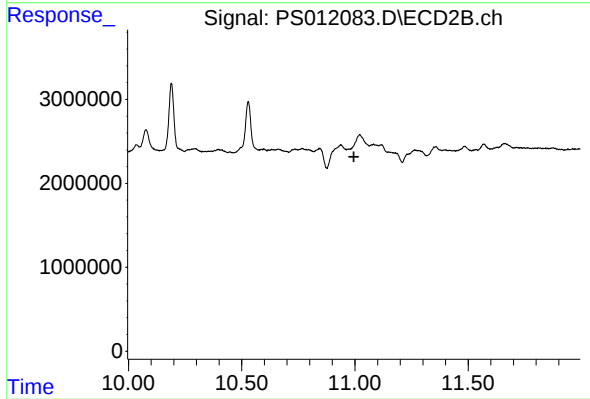

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.