

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090320\
 Data File : PS012085.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2020 14:28
 Operator : DD\AJ
 Sample : L3866-05RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 16:04:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	229.9E6	140.7E6	210.813	263.181
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	77290619	N.D.	93.957
3) T	4-Nitroph...	7.055	0.000	2760758	0	4.687	N.D. #
5) T	DICAMBA	7.396	7.049	8055612	8821178	1.967	4.083 #
6) T	MCP	7.629	0.000	8302730	0	2.599	N.D. #
7) T	MCPA	7.697	7.473	238.0E6	135.2E6	52.323	49.354
8) T	DICHLORPROP	0.000	7.741	0	29156752	N.D.	51.638
11) T	2,4,5-TP ...	0.000	8.795	0	17502378	N.D.	5.986
12) T	2,4,5-T	9.412	0.000	22119273	0	3.733	N.D. #
13) T	2,4-DB	9.993	0.000	7456915	0	9.385	N.D. #
16) T	DCPA	11.464	0.000	9900941	0	1.302	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090320\
Data File : PS012085.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2020 14:28
Operator : DD\AJ
Sample : L3866-05RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 16:04:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

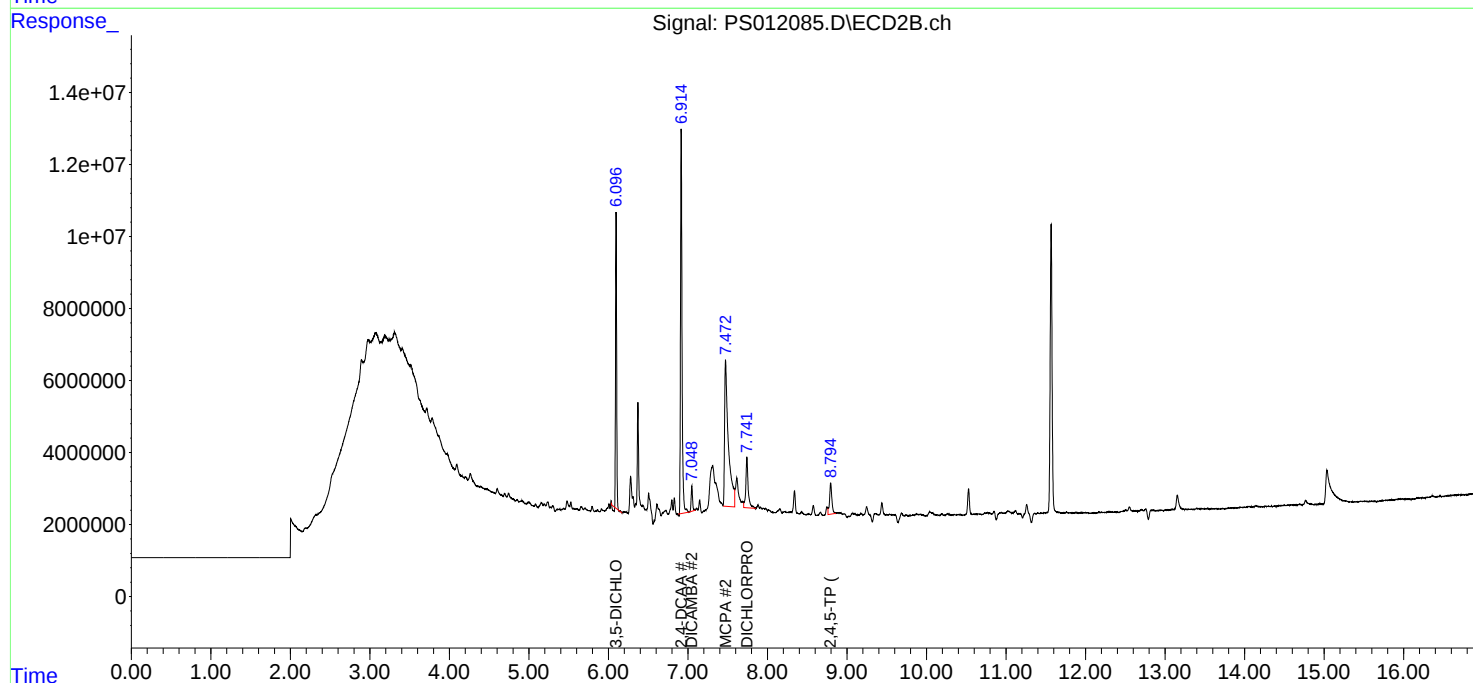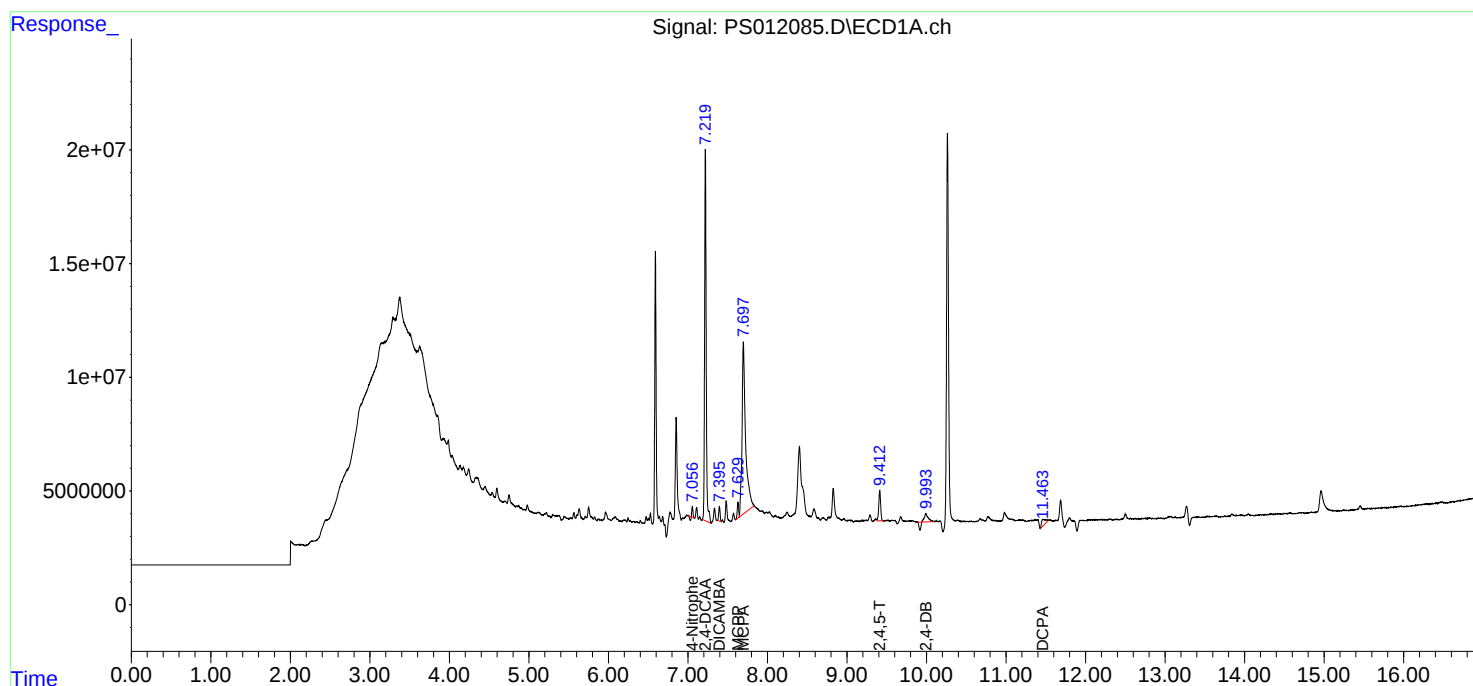


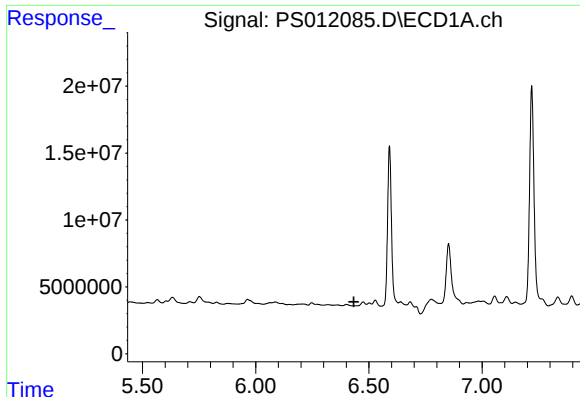

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

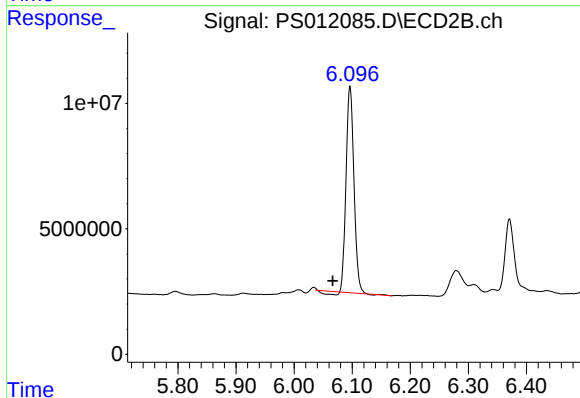


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.030 min
Response: 77290619
Conc: 93.96 ng/ml

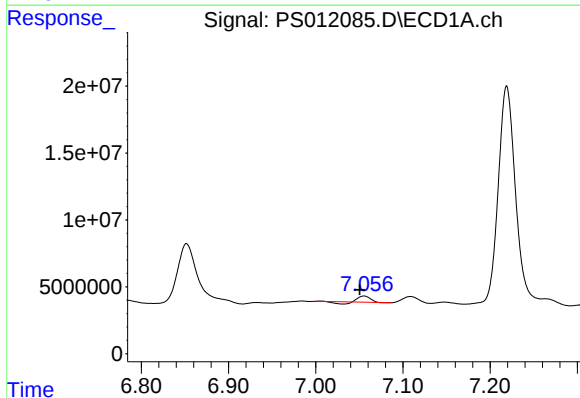


#3 4-Nitrophenol

R.T.: 7.055 min
Delta R.T.: 0.005 min
Response: 2760758
Conc: 4.69 ng/ml

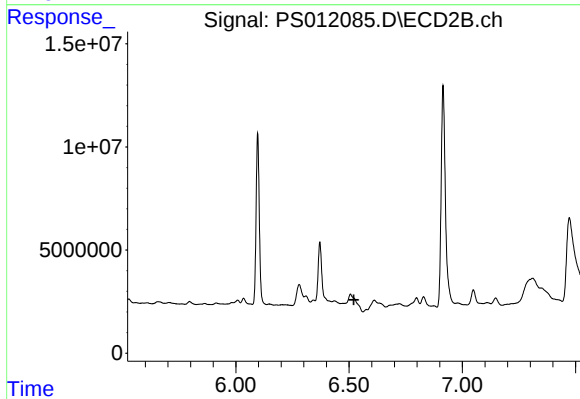

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

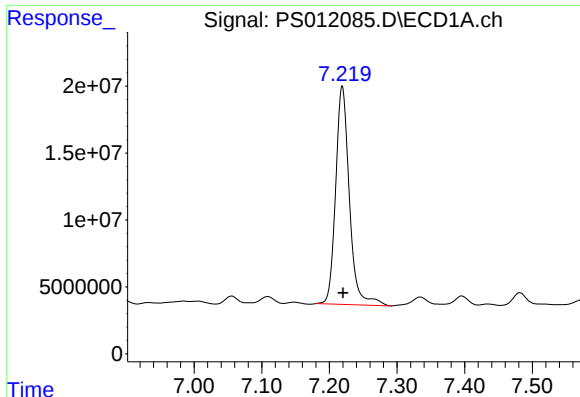

#4 2,4-DCAA


R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 229947662
Conc: 210.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

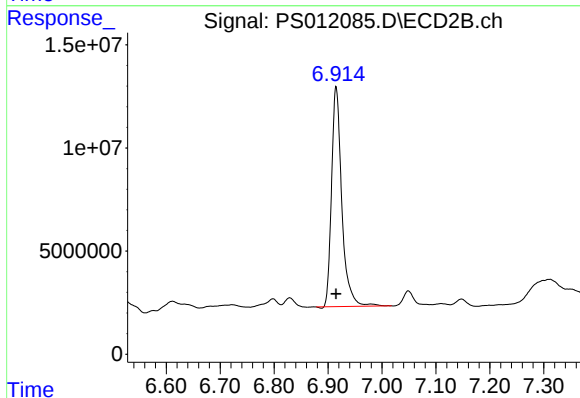


#4 2,4-DCAA

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 140745791
Conc: 263.18 ng/ml

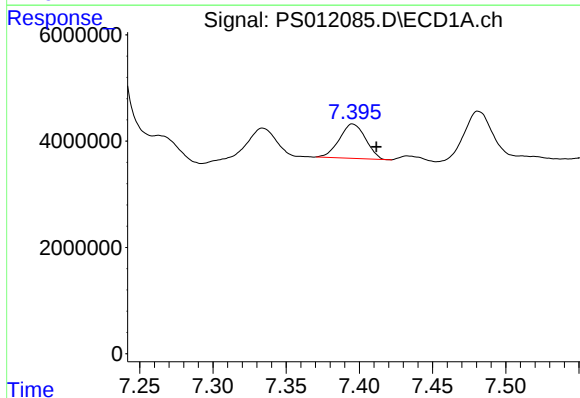


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.016 min
Response: 8055612
Conc: 1.97 ng/ml

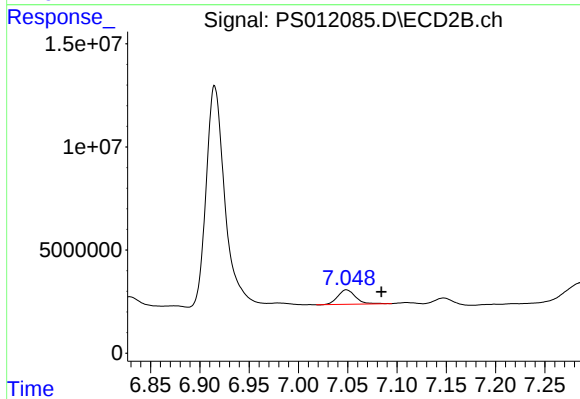

#5 DICAMBA


R.T.: 7.049 min
Delta R.T.: -0.035 min
Response: 8821178
Conc: 4.08 ng/ml

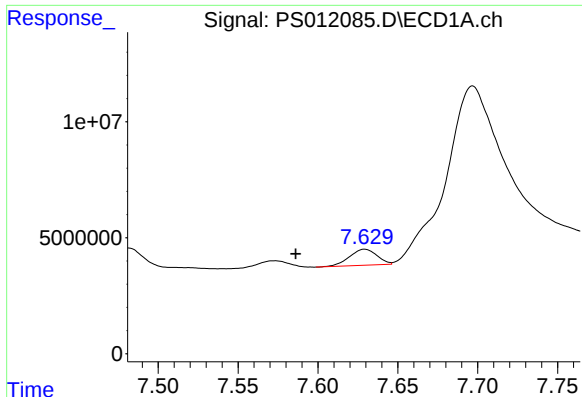

#6 MCPP


R.T.: 7.629 min
Delta R.T.: 0.043 min
Response: 8302730
Conc: 2.60 ug/ml

Instrument :
ECD_S
ClientSampleId :

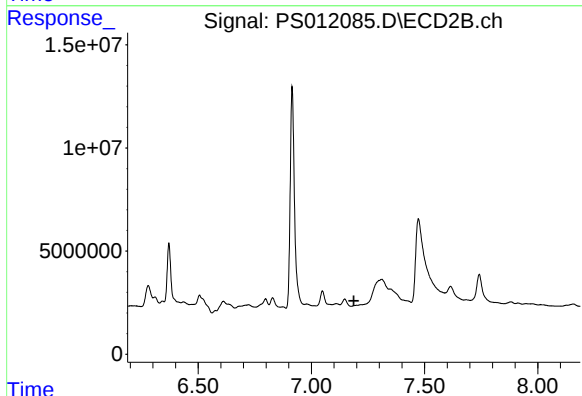


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

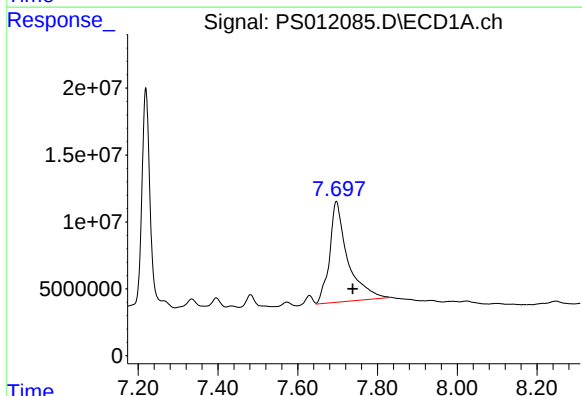


#7 MCPA

R.T.: 7.697 min
Delta R.T.: -0.041 min
Response: 237991175
Conc: 52.32 ug/ml

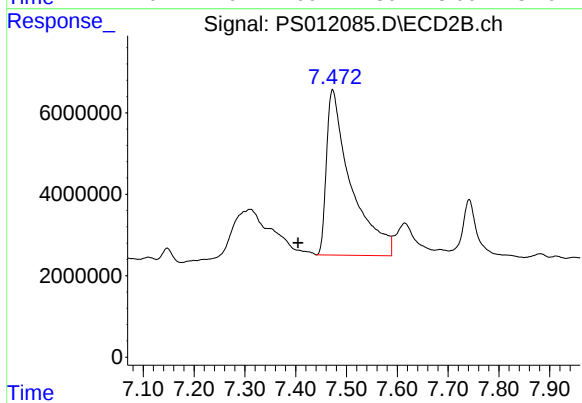

#7 MCPA


R.T.: 7.473 min
Delta R.T.: 0.068 min
Response: 135236286
Conc: 49.35 ug/ml

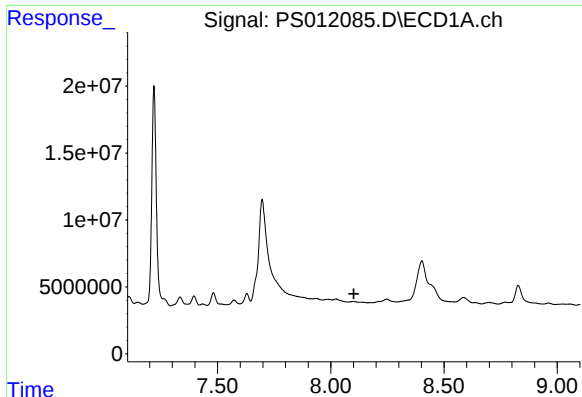

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

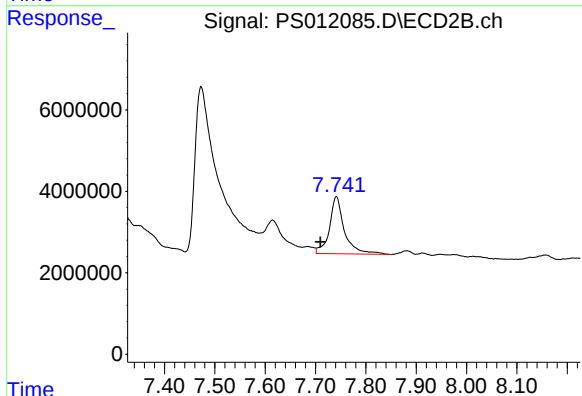


#8 DICHLORPROP

R.T.: 7.741 min
Delta R.T.: 0.032 min
Response: 29156752
Conc: 51.64 ng/ml

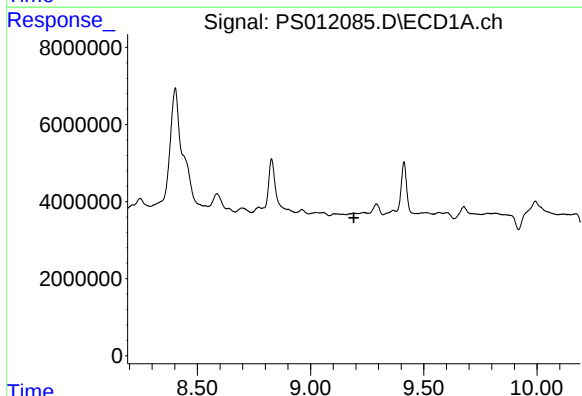


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

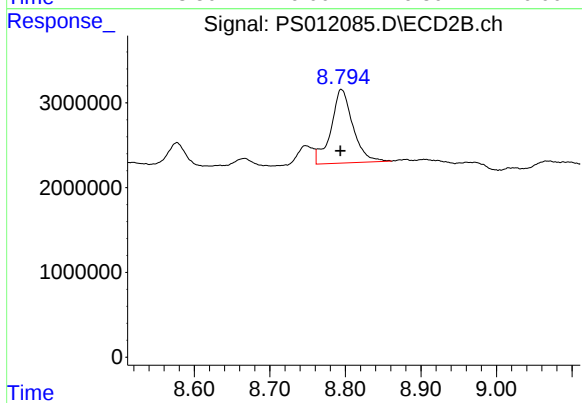

#11 2,4,5-TP (SILVEX)


R.T.: 8.795 min
Delta R.T.: 0.002 min
Response: 17502378
Conc: 5.99 ng/ml

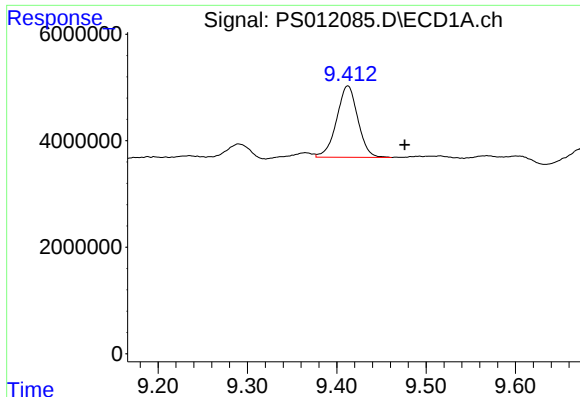

#12 2,4,5-T


R.T.: 9.412 min
Delta R.T.: -0.064 min
Response: 22119273
Conc: 3.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

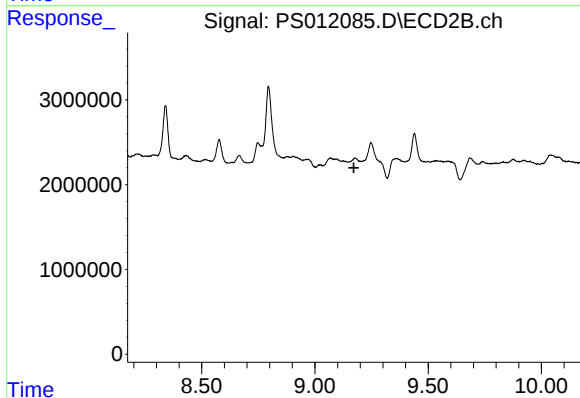


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

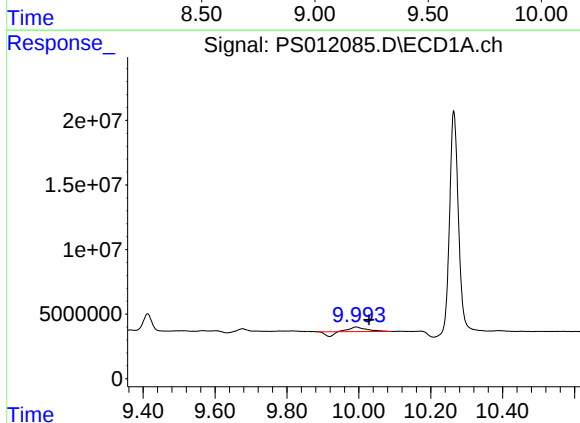


#13 2,4-DB

R.T.: 9.993 min
Delta R.T.: -0.035 min
Response: 7456915
Conc: 9.38 ng/ml

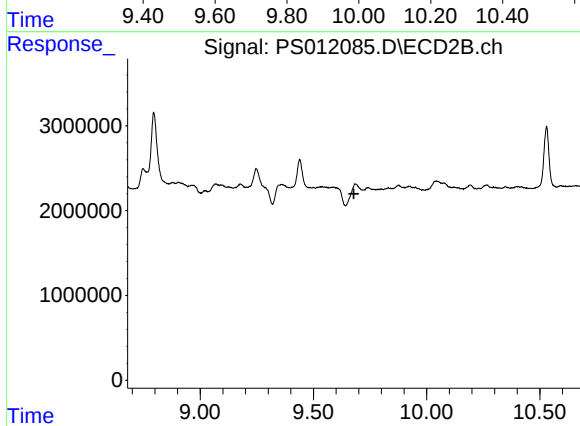

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.679 min
Response: 0
Conc: N.D.

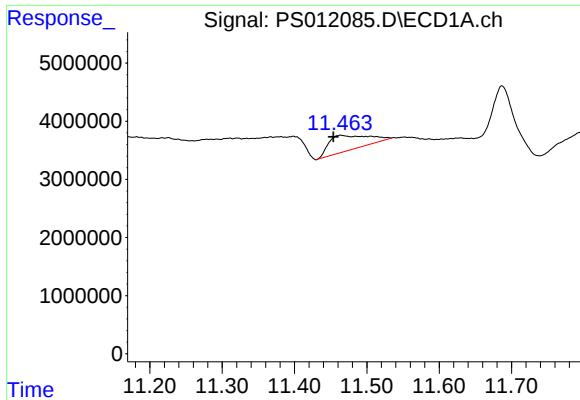

#16 DCPA

R.T.: 11.464 min
Delta R.T.: 0.011 min
Response: 9900941
Conc: 1.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

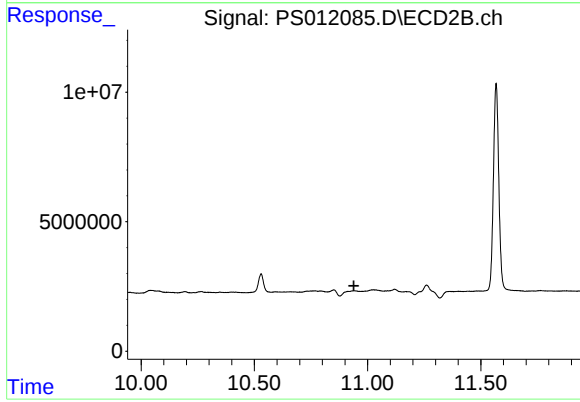

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.940 min
Response: 0
Conc: N.D.