

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090320\
 Data File : PS012096.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2020 18:41
 Operator : DD\AJ
 Sample : L3847-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 LINDEN-JOP-BH-08-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 06:11:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.916	44513164	27564409	40.809	51.543 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	65624591	N.D.	79.775
5) T	DICAMBA	7.396	7.049	7110701	8966900	1.736	4.150 #
6) T	MCPD	7.571	0.000	5826231	0	1.824	N.D. #
7) T	MCPA	7.764	7.374	21269694	32982243	4.676	12.037 #
9) T	2,4-D	8.395	0.000	25891020	0	22.931	N.D. #
10) T	Pentachlo...	8.704	0.000	11320533	0	<MDL	N.D. #
12) T	2,4,5-T	9.412	0.000	79495580	0	13.415	N.D. #
13) T	2,4-DB	10.050	0.000	23164009	0	29.153	N.D. #
15) T	Picloram	0.000	11.023	0	32263715	N.D.	7.118
16) T	DCPA	11.523	0.000	53437139	0	7.028	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090320\
Data File : PS012096.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2020 18:41
Operator : DD\AJ
Sample : L3847-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
LINDEN-JOP-BH-08-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 06:11:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

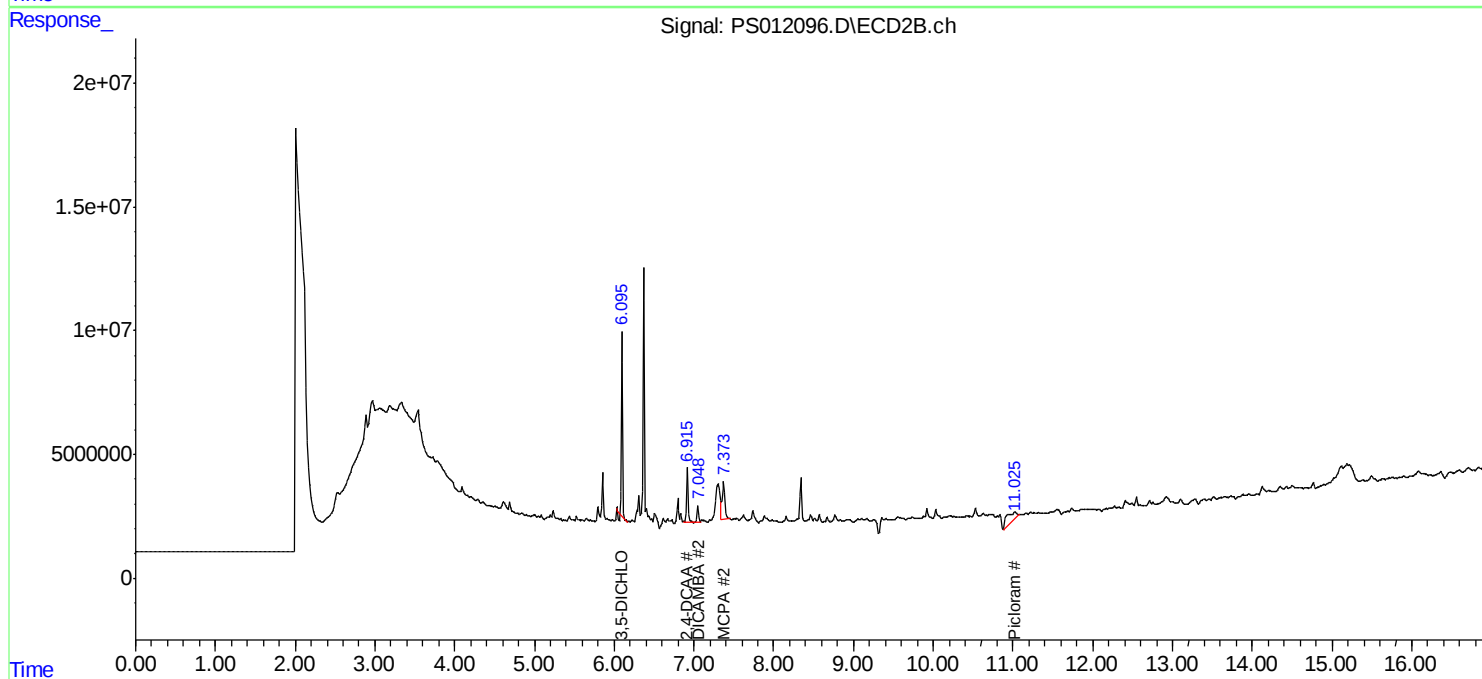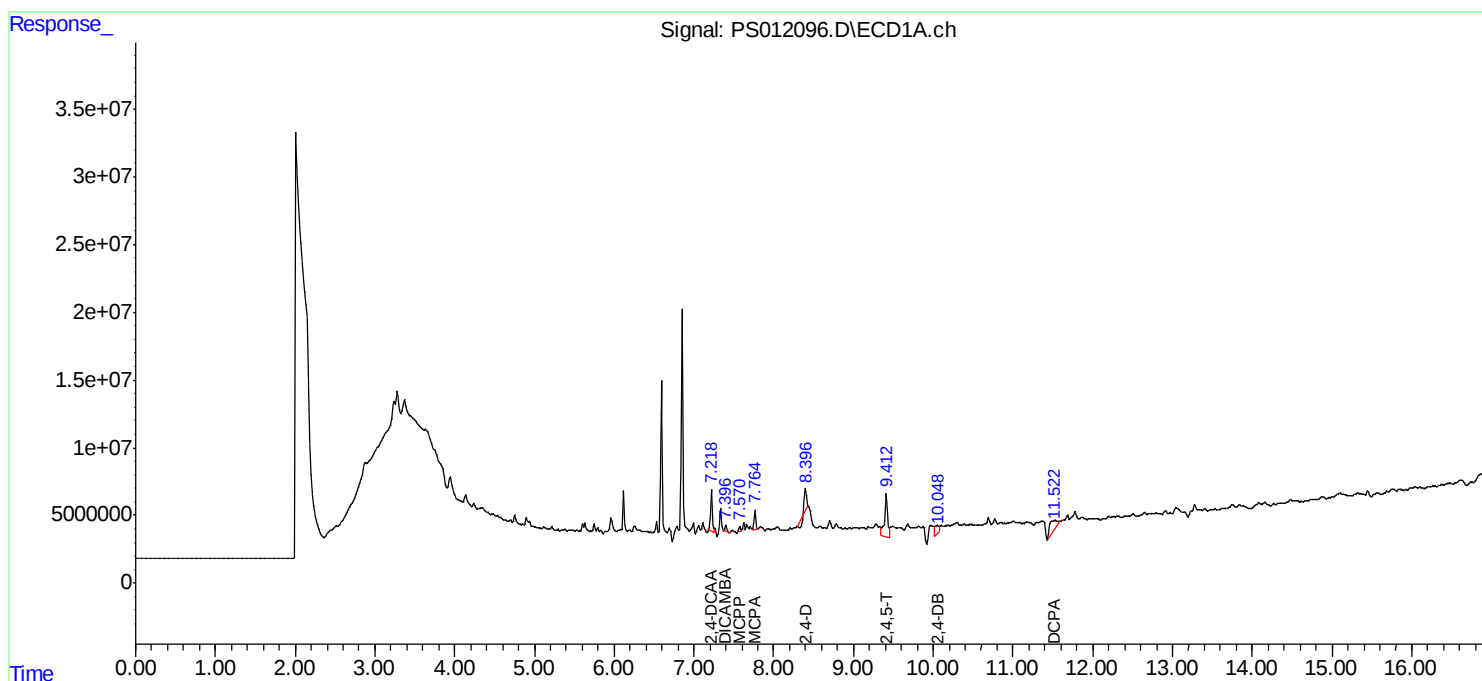


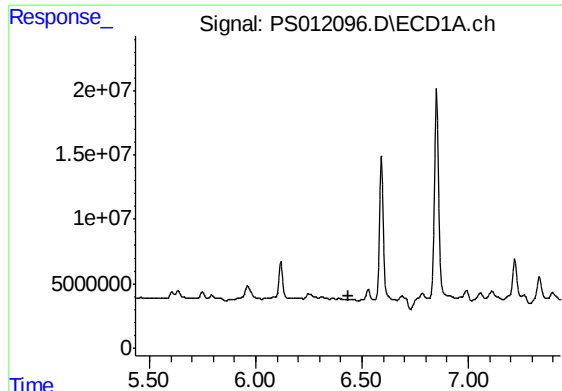

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
LINDEN-JOP-BH-08-A

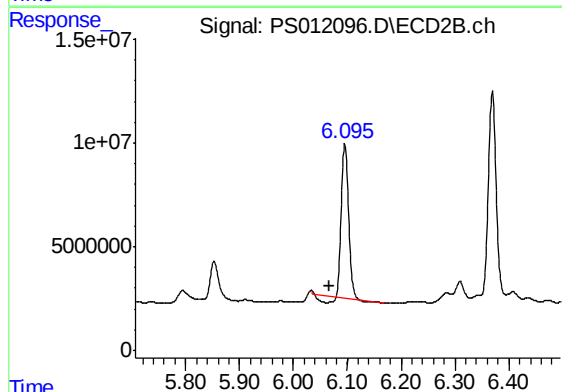


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 65624591
Conc: 79.78 ng/ml

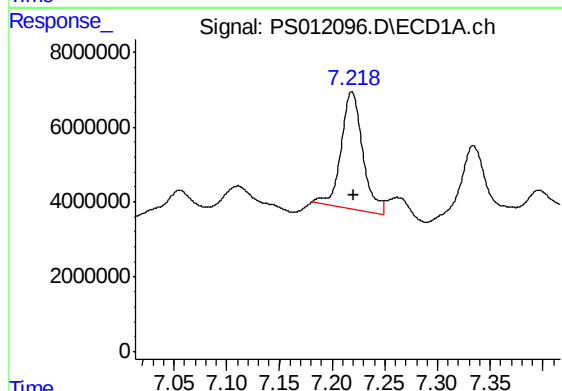


#4 2,4-DCAA

R.T.: 7.219 min
Delta R.T.: -0.001 min
Response: 44513164
Conc: 40.81 ng/ml

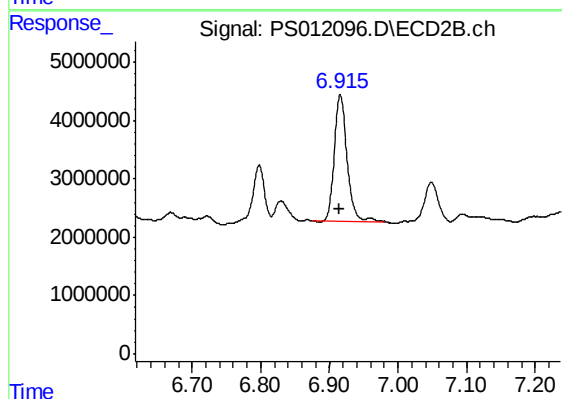

#4 2,4-DCAA


R.T.: 6.916 min
Delta R.T.: 0.001 min
Response: 27564409
Conc: 51.54 ng/ml

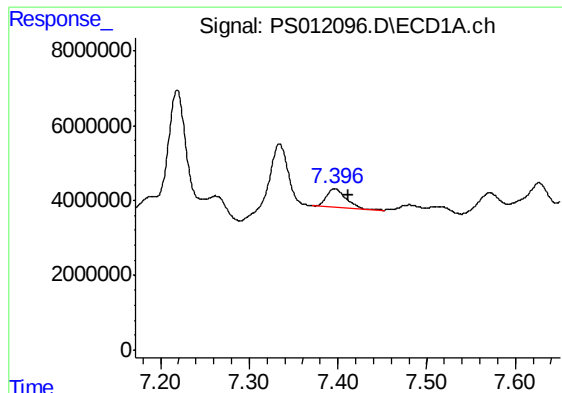

#5 DICAMBA


R.T.: 7.396 min
Delta R.T.: -0.015 min
Response: 7110701
Conc: 1.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
LINDEN-JOP-BH-08-A

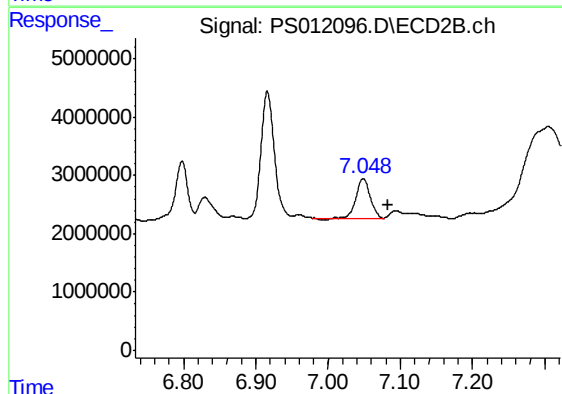


#5 DICAMBA

R.T.: 7.049 min
Delta R.T.: -0.036 min
Response: 8966900
Conc: 4.15 ng/ml

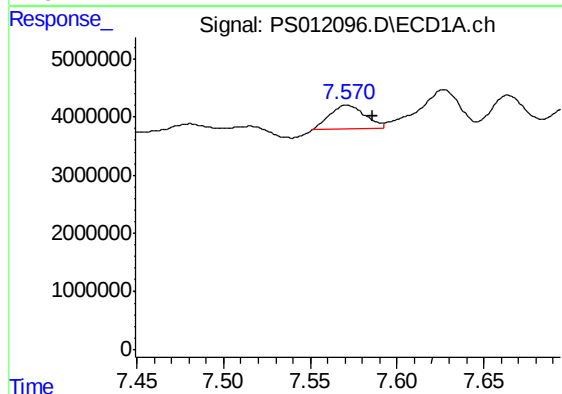


#6 MCPP

R.T.: 7.571 min
Delta R.T.: -0.015 min
Response: 5826231
Conc: 1.82 ug/ml

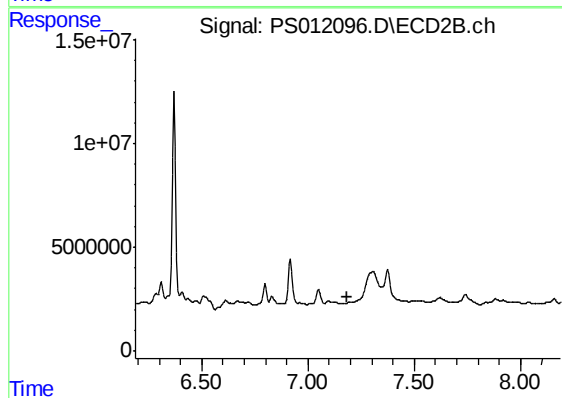

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

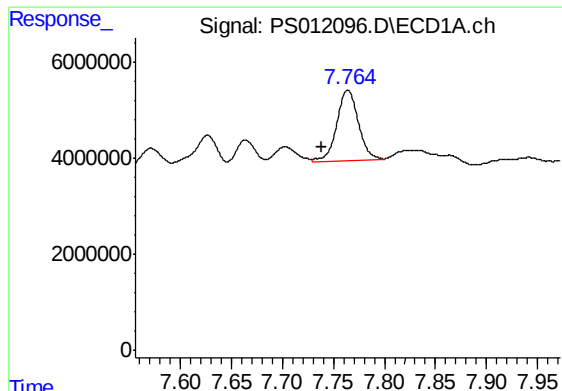

#7 MCPA


R.T.: 7.764 min
Delta R.T.: 0.026 min
Response: 21269694
Conc: 4.68 ug/ml

Instrument :
ECD_S
ClientSampleId :
LINDEN-JOP-BH-08-A

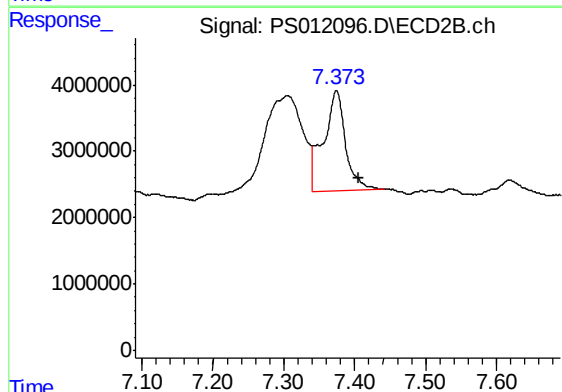


#7 MCPA

R.T.: 7.374 min
Delta R.T.: -0.031 min
Response: 32982243
Conc: 12.04 ug/ml

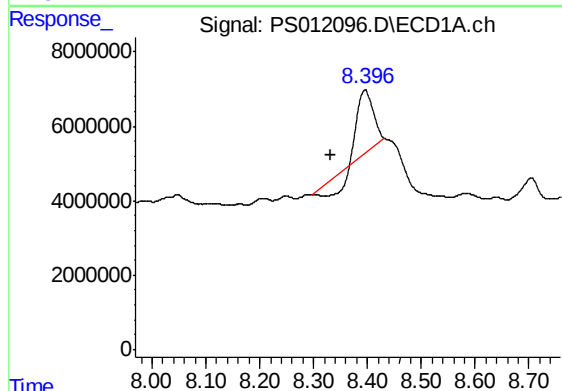


#9 2,4-D

R.T.: 8.395 min
Delta R.T.: 0.063 min
Response: 25891020
Conc: 22.93 ng/ml

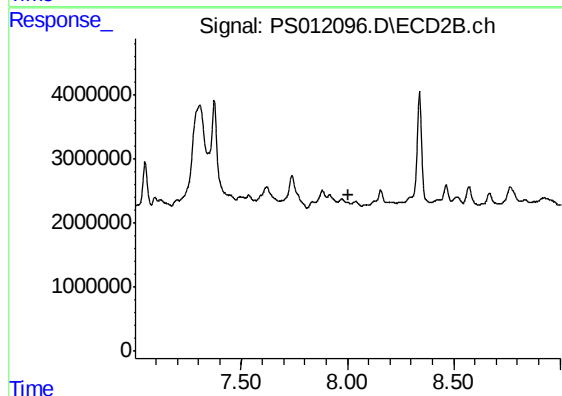

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

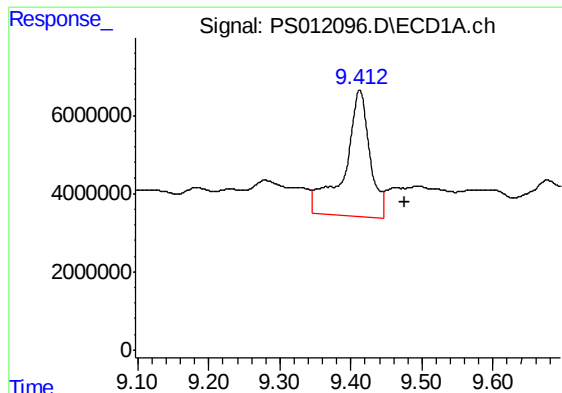

#12 2,4,5-T


R.T.: 9.412 min
Delta R.T.: -0.063 min
Response: 79495580
Conc: 13.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
LINDEN-JOP-BH-08-A

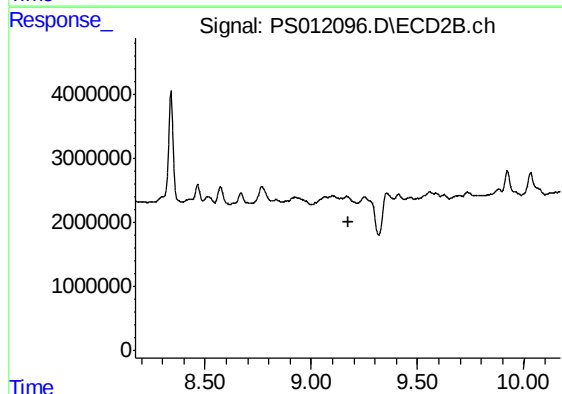


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

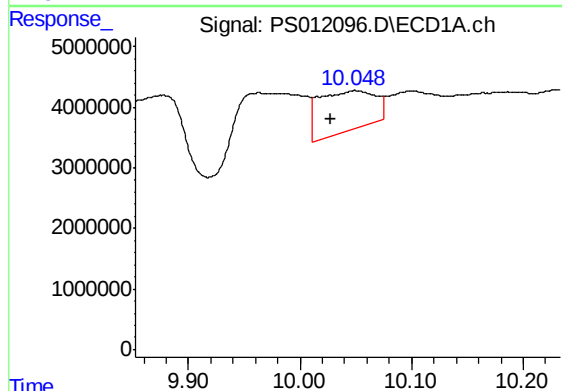


#13 2,4-DB

R.T.: 10.050 min
Delta R.T.: 0.022 min
Response: 23164009
Conc: 29.15 ng/ml

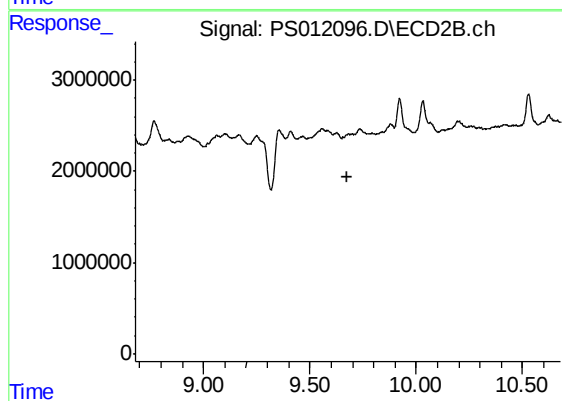

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.679 min
Response: 0
Conc: N.D.

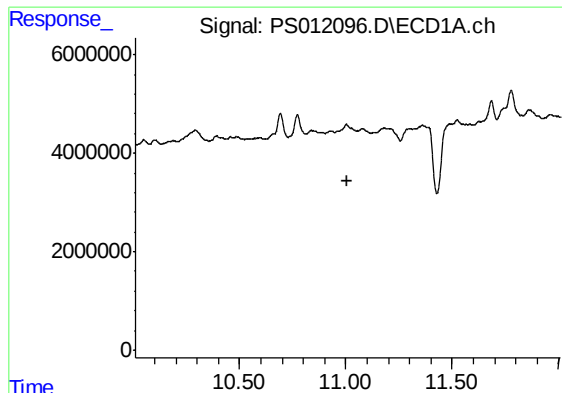

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 11.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
LINDEN-JOP-BH-08-A

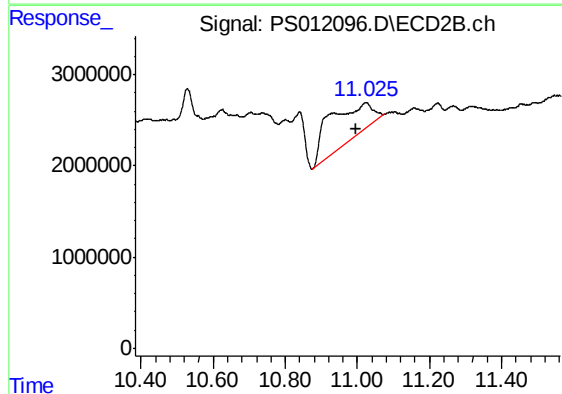


#15 Picloram

R.T.: 11.023 min
Delta R.T.: 0.028 min
Response: 32263715
Conc: 7.12 ng/ml

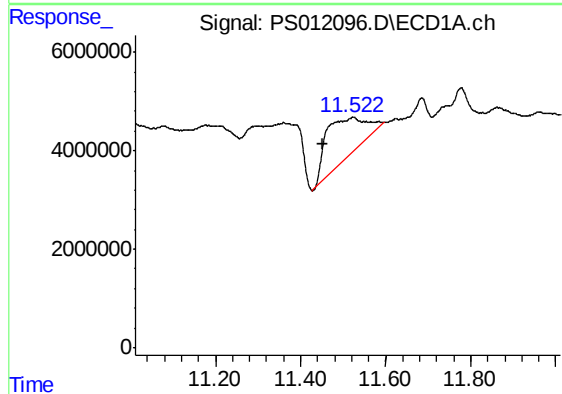

#16 DCPA

R.T.: 11.523 min
Delta R.T.: 0.070 min
Response: 53437139
Conc: 7.03 ng/ml

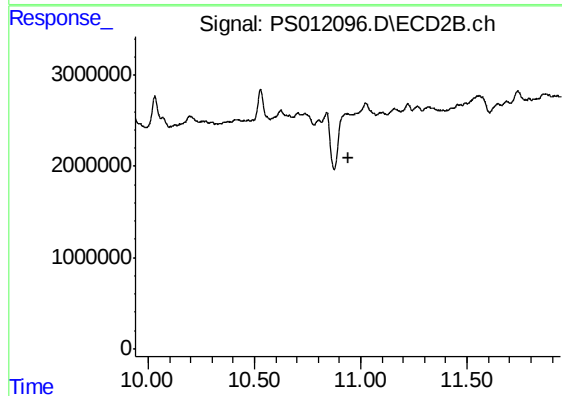

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.940 min
Response: 0
Conc: N.D.