

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090320\
 Data File : PS012104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2020 21:45
 Operator : DD\AJ
 Sample : L3848-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 LINDEN-BH-02-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 06:13:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.913	433.8E6	247.9E6	397.696	463.604
Target Compounds							
2) T	3,5-DICHL...	6.474	6.095	10675874	58424709	7.364	71.023 #
3) T	4-Nitroph...	7.053	0.000	9113993	0	15.473	N.D. #
5) T	DICAMBA	0.000	7.047	0	12586167	N.D.	5.826
6) T	MCPD	7.570	0.000	9202251	0	2.880	N.D. #
7) T	MCPA	7.763	7.374	22349186	29202854	4.914	10.657 #
8) T	DICHLORPROP	0.000	7.659	0	8687332	N.D.	15.386
9) T	2,4-D	8.399	0.000	53641002	0	47.508	N.D. #
10) T	Pentachlo...	8.638	8.430	18162810	22178224	1.263	3.264 #
11) T	2,4,5-TP ...	0.000	8.767	0	12600923	N.D.	4.310
12) T	2,4,5-T	9.460	0.000	25592920	0	4.319	N.D. #
13) T	2,4-DB	9.976	9.713	40334472	49327676	50.762	117.946 #
14) T	DINOSEB	0.000	10.032	0	56621573	N.D.	26.634
15) T	Picloram	11.041	11.019	64693128	7297883	8.277	1.610 #
16) T	DCPA	0.000	10.912	0	21757070	N.D.	5.917



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090320\
Data File : PS012104.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2020 21:45
Operator : DD\AJ
Sample : L3848-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
LINDEN-BH-02-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 06:13:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

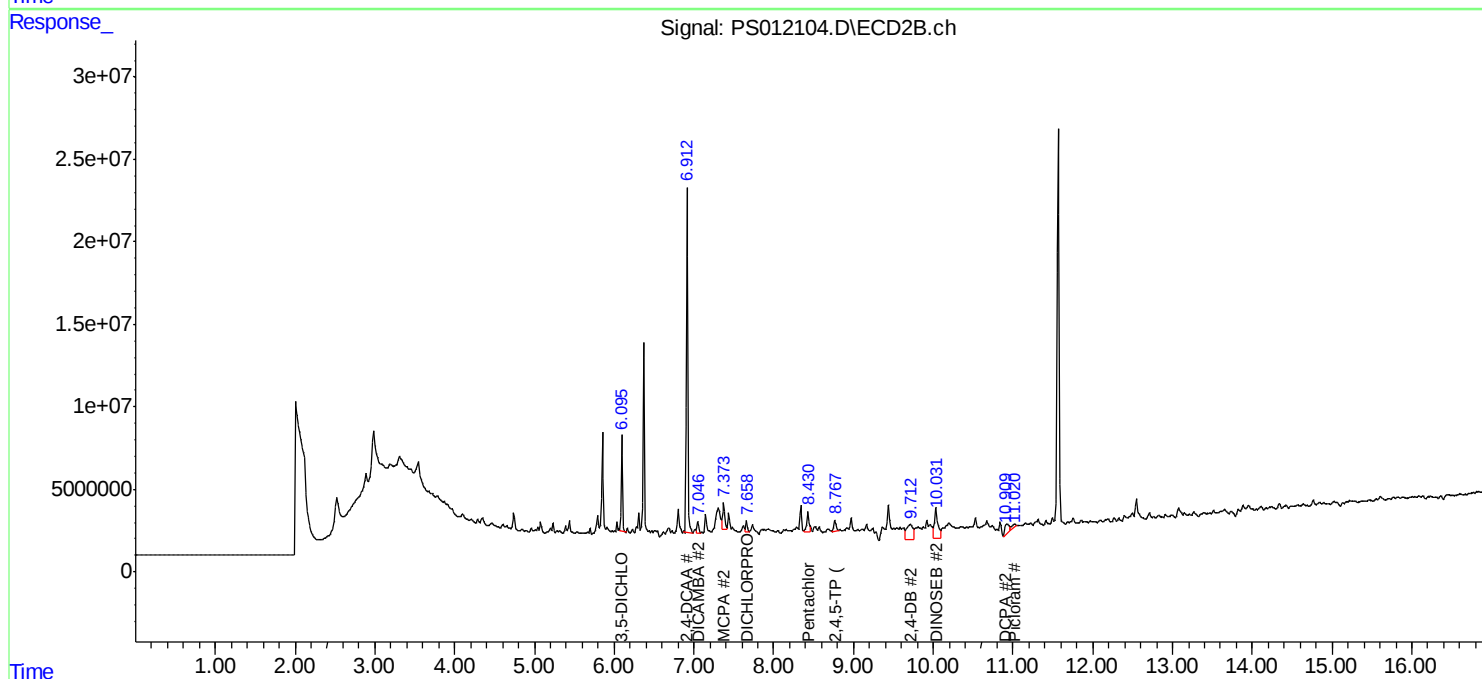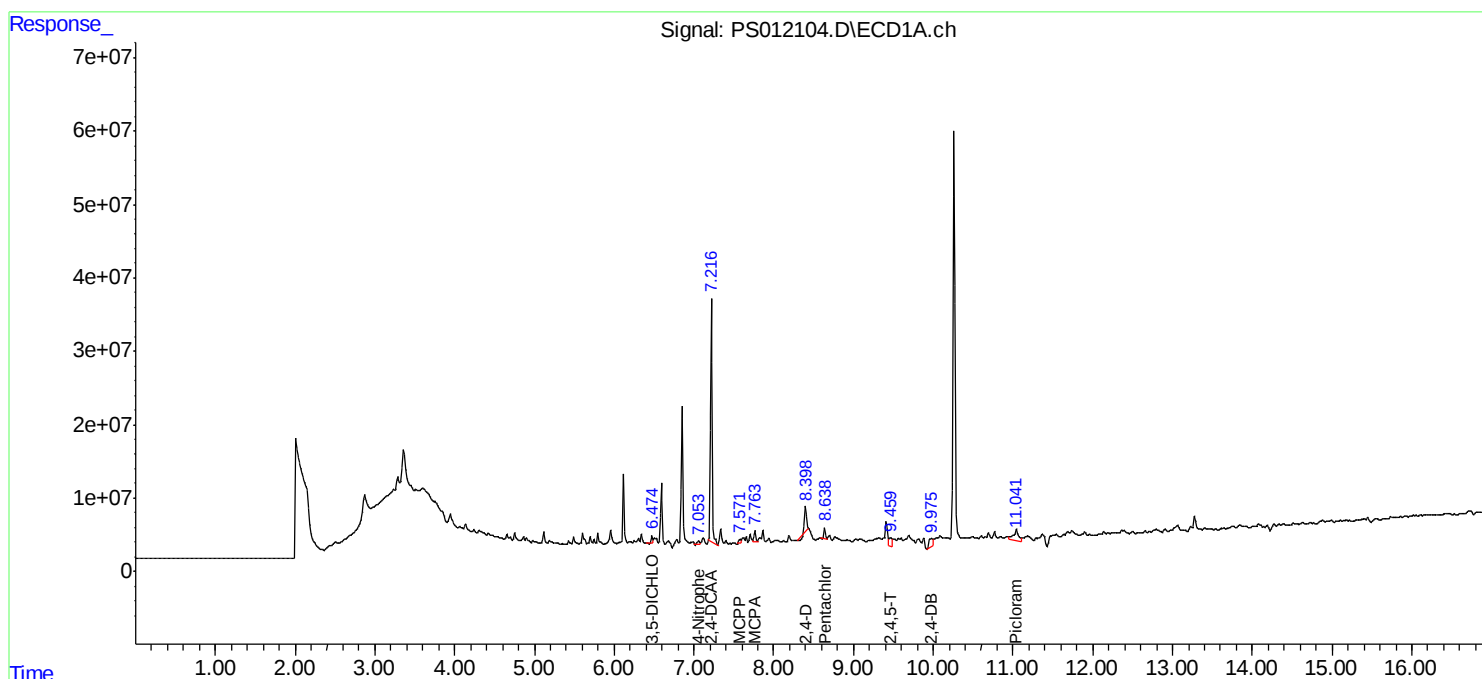


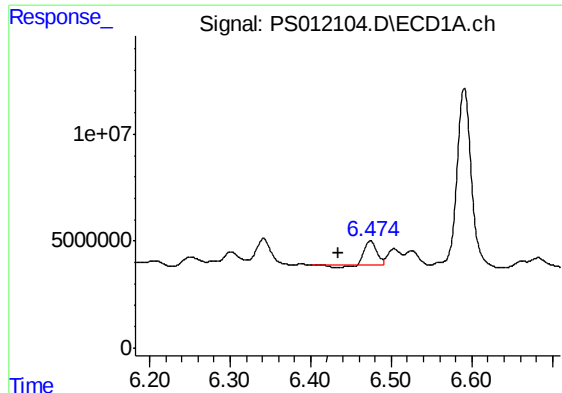

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.474 min
Delta R.T.: 0.040 min
Response: 10675874
Conc: 7.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-02-A

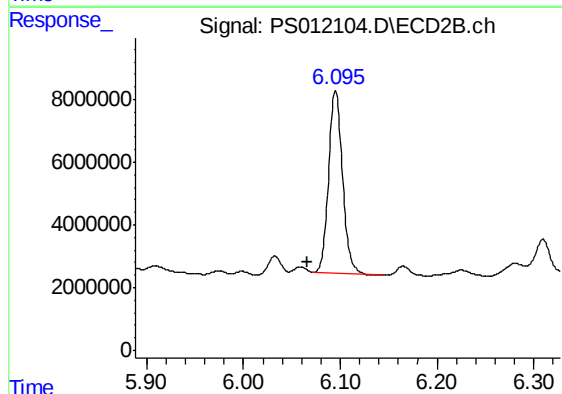


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.029 min
Response: 58424709
Conc: 71.02 ng/ml

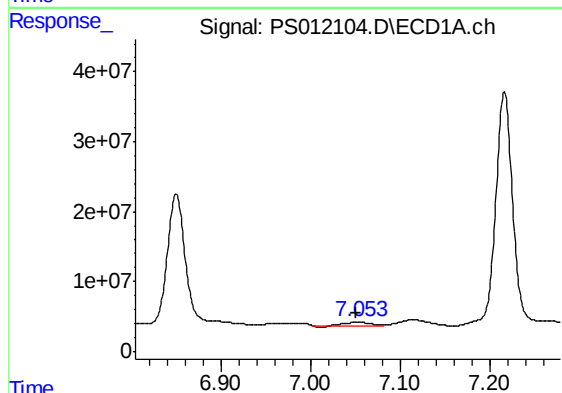


#3 4-Nitrophenol

R.T.: 7.053 min
Delta R.T.: 0.003 min
Response: 9113993
Conc: 15.47 ng/ml

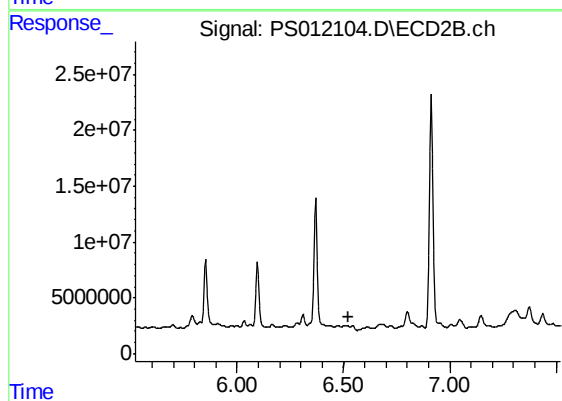

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.521 min
Response: 0
Conc: N.D.

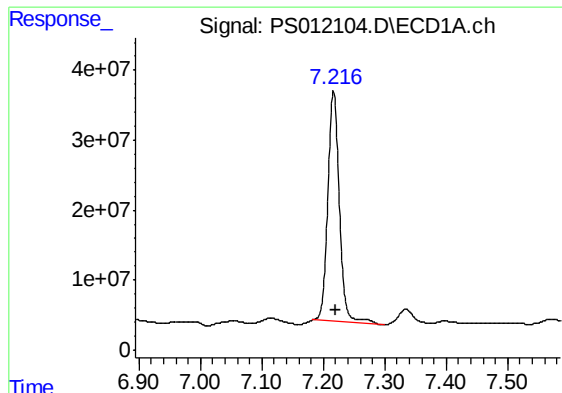

#4 2,4-DCAA


R.T.: 7.217 min
Delta R.T.: -0.004 min
Response: 433793916
Conc: 397.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-02-A

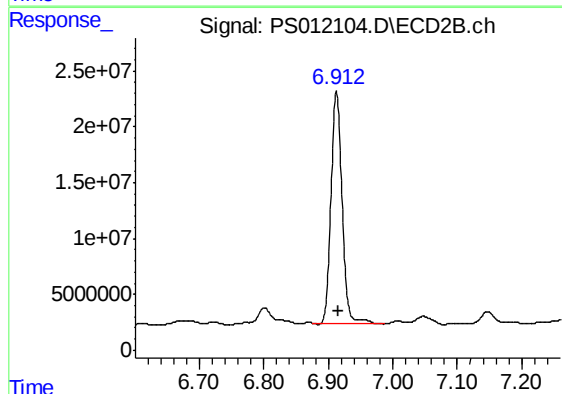


#4 2,4-DCAA

R.T.: 6.913 min
Delta R.T.: -0.002 min
Response: 247929513
Conc: 463.60 ng/ml

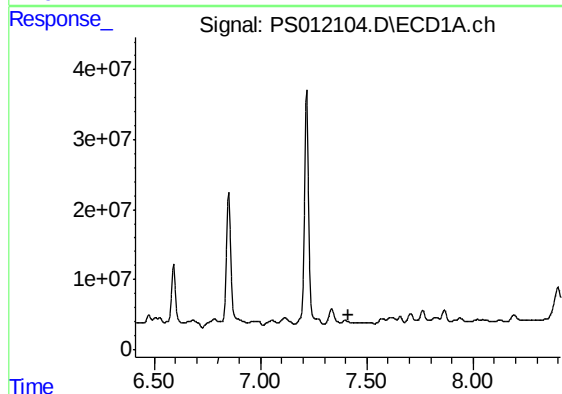


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.412 min
Response: 0
Conc: N.D.

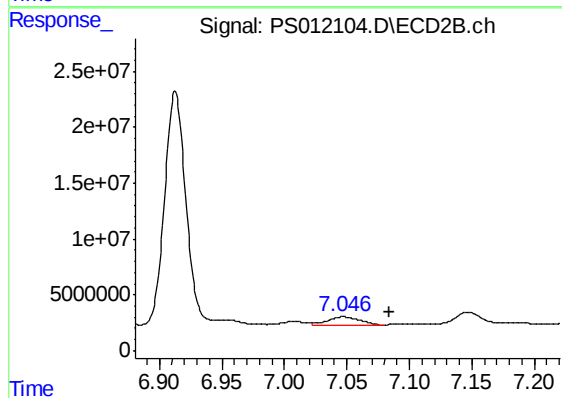

#5 DICAMBA


R.T.: 7.047 min
Delta R.T.: -0.037 min
Response: 12586167
Conc: 5.83 ng/ml

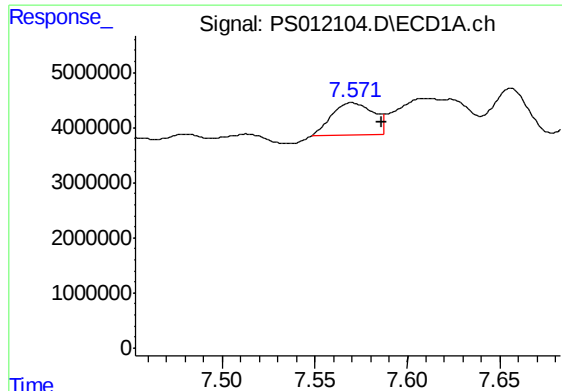

#6 MCPP


R.T.: 7.570 min
Delta R.T.: -0.016 min
Response: 9202251
Conc: 2.88 ug/ml

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-02-A

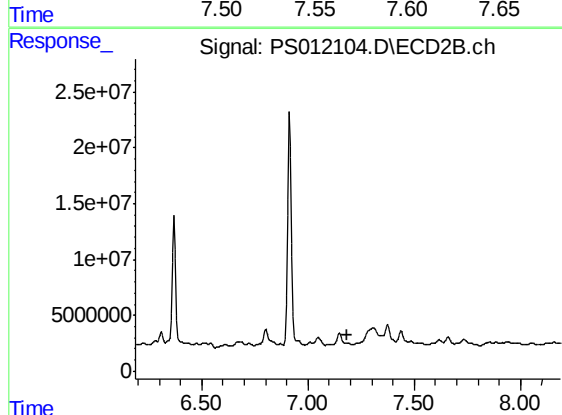


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

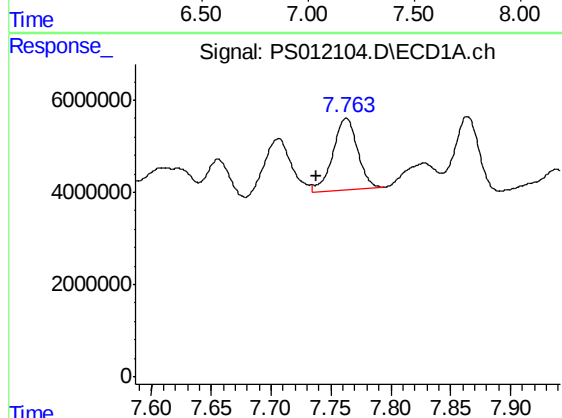


#7 MCPA

R.T.: 7.763 min
Delta R.T.: 0.024 min
Response: 22349186
Conc: 4.91 ug/ml

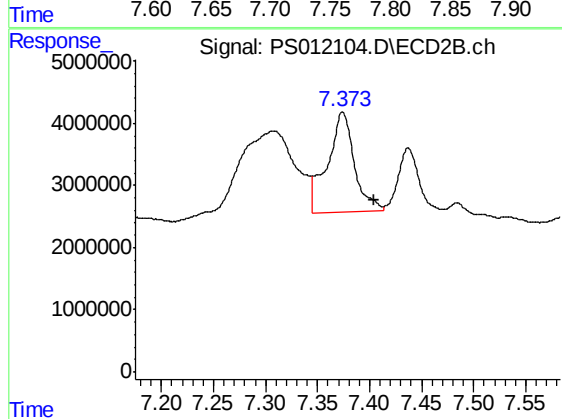

#7 MCPA


R.T.: 7.374 min
Delta R.T.: -0.031 min
Response: 29202854
Conc: 10.66 ug/ml

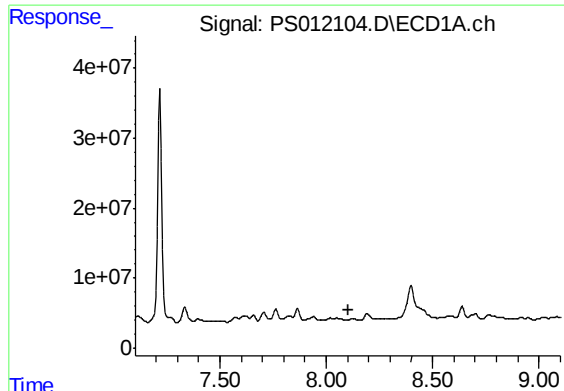

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-02-A

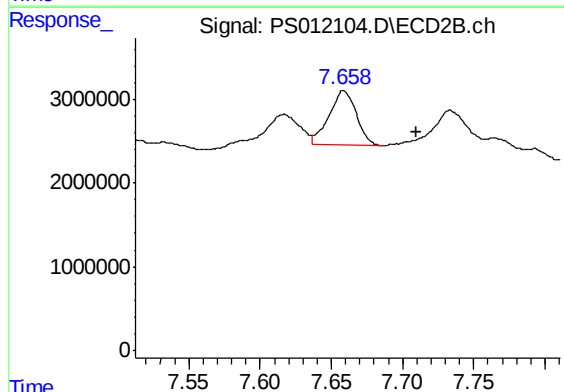


#8 DICHLORPROP

R.T.: 7.659 min
Delta R.T.: -0.051 min
Response: 8687332
Conc: 15.39 ng/ml

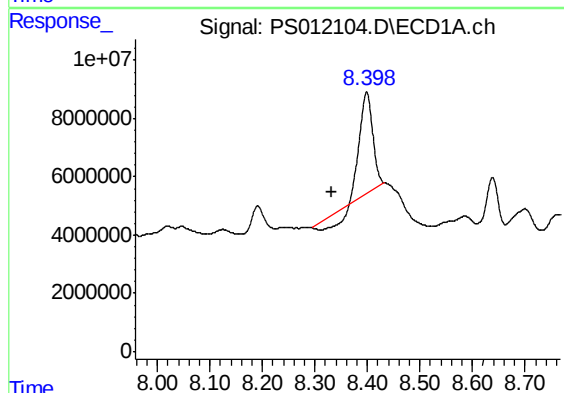


#9 2,4-D

R.T.: 8.399 min
Delta R.T.: 0.067 min
Response: 53641002
Conc: 47.51 ng/ml

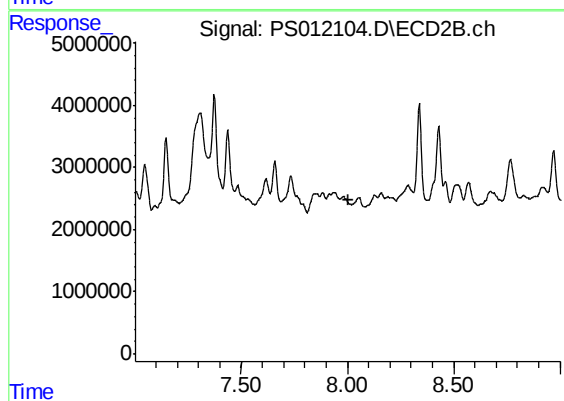

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

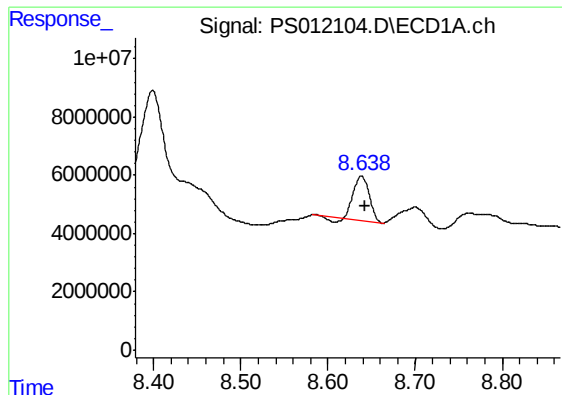

#10 Pentachlorophenol


R.T.: 8.638 min
Delta R.T.: -0.005 min
Response: 18162810
Conc: 1.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-02-A

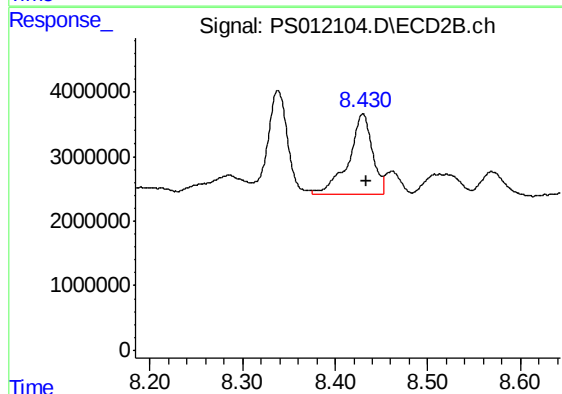


#10 Pentachlorophenol

R.T.: 8.430 min
Delta R.T.: -0.005 min
Response: 22178224
Conc: 3.26 ng/ml

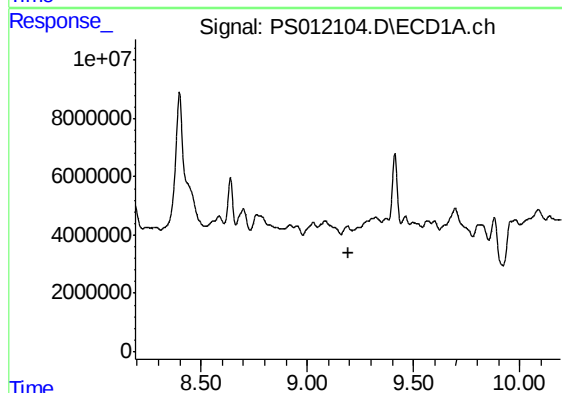


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

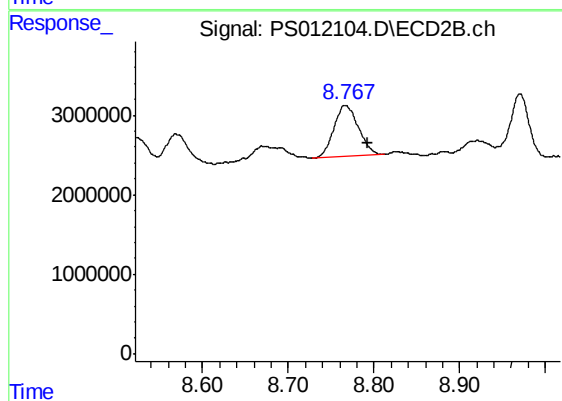

#11 2,4,5-TP (SILVEX)


R.T.: 8.767 min
Delta R.T.: -0.027 min
Response: 12600923
Conc: 4.31 ng/ml

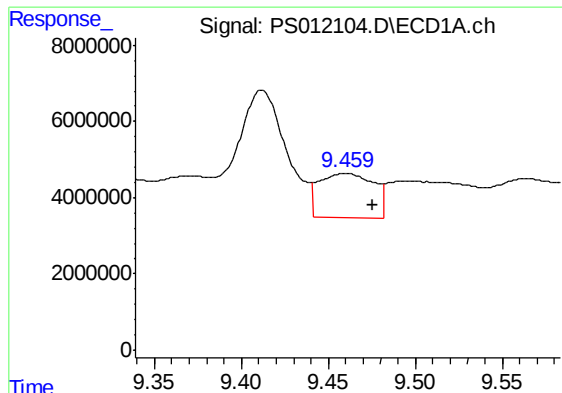

#12 2,4,5-T


R.T.: 9.460 min
Delta R.T.: -0.016 min
Response: 25592920
Conc: 4.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-02-A

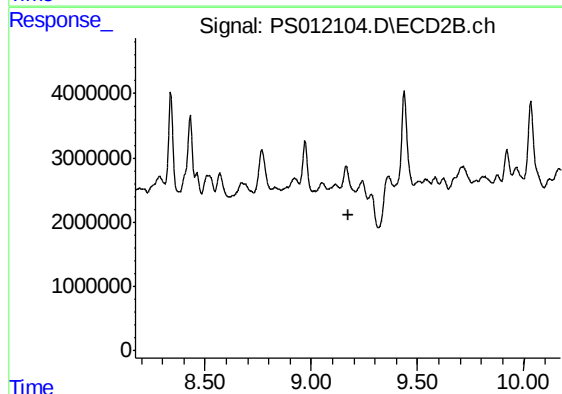


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

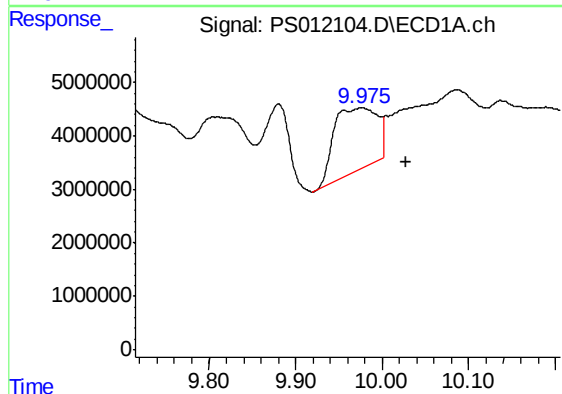


#13 2,4-DB

R.T.: 9.976 min
Delta R.T.: -0.052 min
Response: 40334472
Conc: 50.76 ng/ml

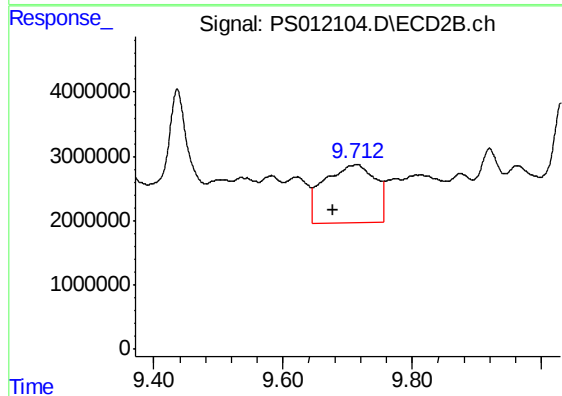

#13 2,4-DB


R.T.: 9.713 min
Delta R.T.: 0.034 min
Response: 49327676
Conc: 117.95 ng/ml

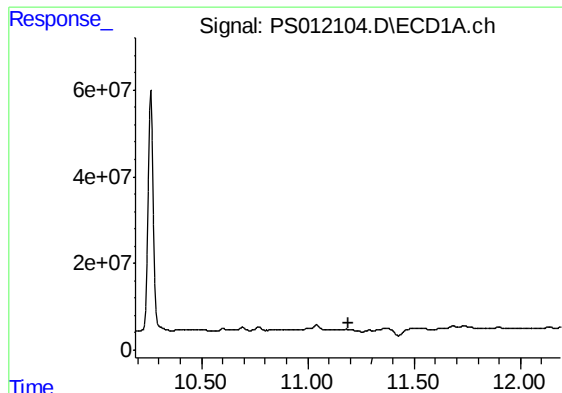

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.189 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-02-A

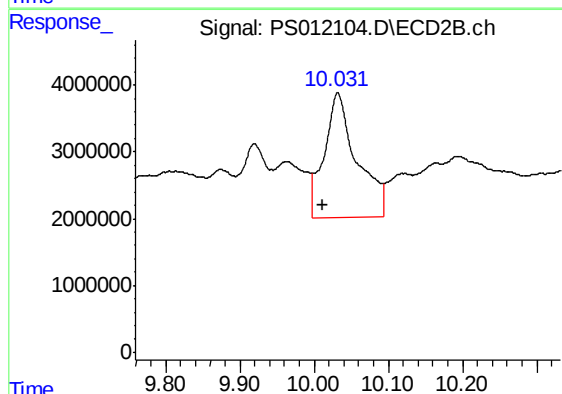


#14 DINOSEB

R.T.: 10.032 min
Delta R.T.: 0.020 min
Response: 56621573
Conc: 26.63 ng/ml

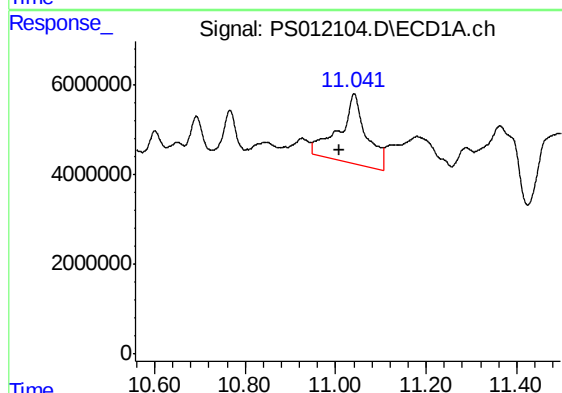


#15 Picloram

R.T.: 11.041 min
Delta R.T.: 0.031 min
Response: 64693128
Conc: 8.28 ng/ml

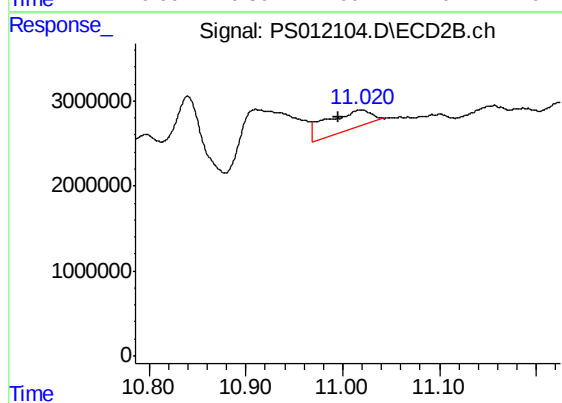

#15 Picloram


R.T.: 11.019 min
Delta R.T.: 0.024 min
Response: 7297883
Conc: 1.61 ng/ml

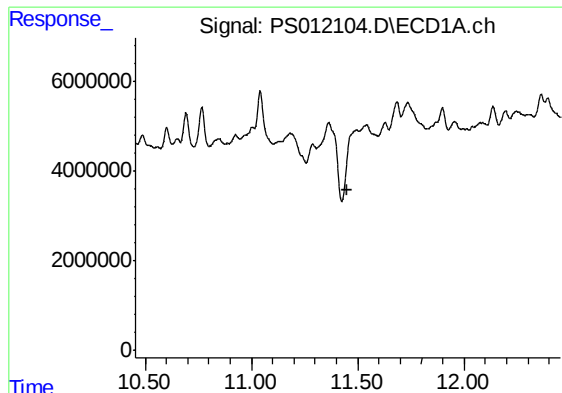

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.454 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-02-A

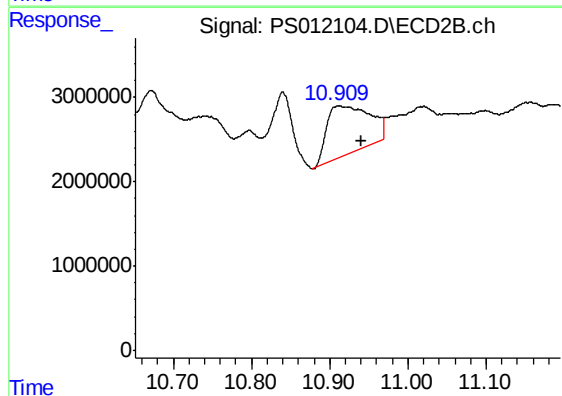

#16 DCPA

R.T.: 10.912 min
Delta R.T.: -0.028 min
Response: 21757070
Conc: 5.92 ng/ml