

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090320\
 Data File : PS012105.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2020 22:08
 Operator : DD\AJ
 Sample : L3848-09
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 LINDEN-BH-01-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 06:14:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.914	184.5E6	113.4E6	169.156	212.032 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	88874385	N.D.	108.038
3) T	4-Nitroph...	7.054	6.548	2720258	7047363	4.618	19.329 #
5) T	DICAMBA	7.396	7.048	11407450	12474612	2.785	5.774 #
6) T	MCPD	7.571	0.000	6741861	0	2.110	N.D. #
7) T	MCPA	7.764	7.375	21645788	34487244	4.759	12.586 #
9) T	2,4-D	8.392	0.000	25579369	0	22.655	N.D. #
10) T	Pentachlo...	8.638	8.430	10081576	11505728	<MDL	1.693 #
12) T	2,4,5-T	9.411	0.000	38284491	0	6.461	N.D. #
13) T	2,4-DB	10.045	0.000	25156461	0	31.660	N.D. #
14) T	DINOSEB	0.000	10.030	0	15420500	N.D.	7.254
15) T	Picloram	0.000	11.018	0	53447980	N.D.	11.792
16) T	DCPA	11.519	0.000	108.0E6	0	14.198	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090320\
Data File : PS012105.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2020 22:08
Operator : DD\AJ
Sample : L3848-09
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-01-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 06:14:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

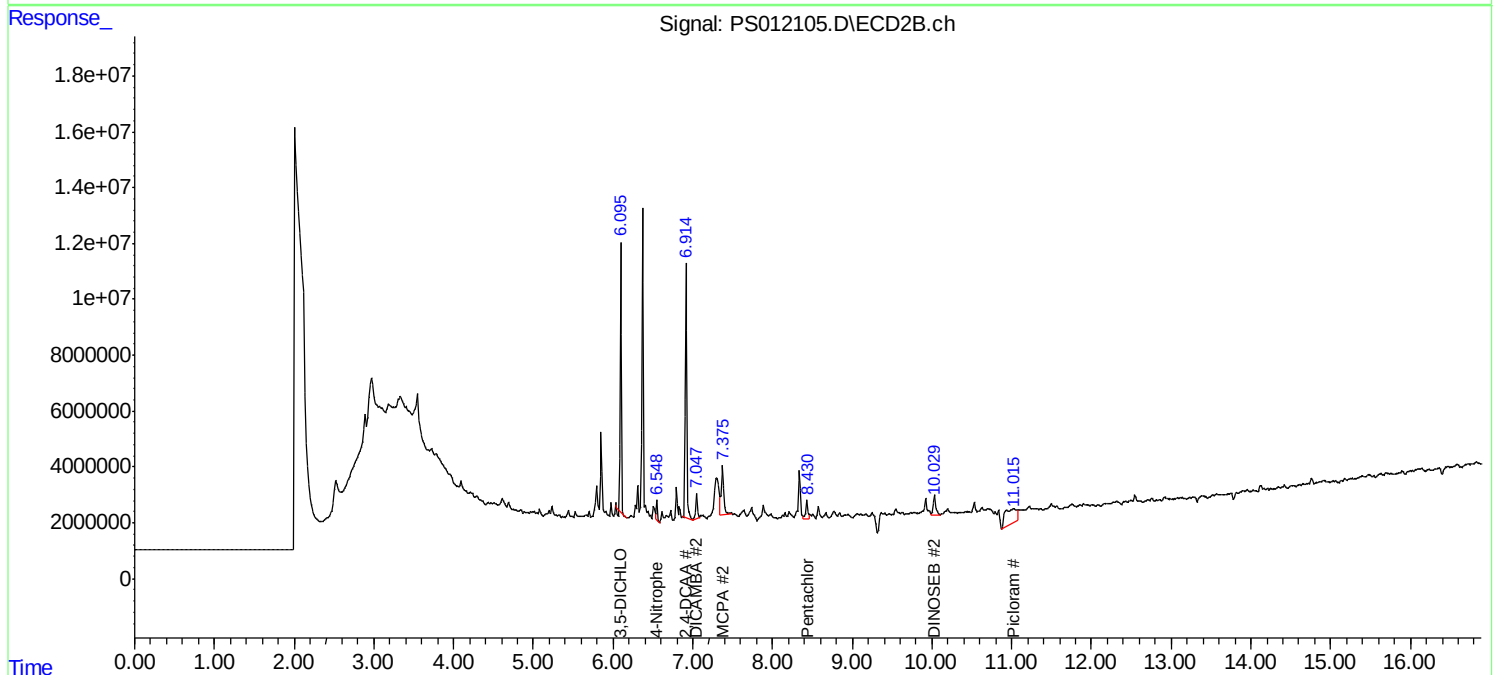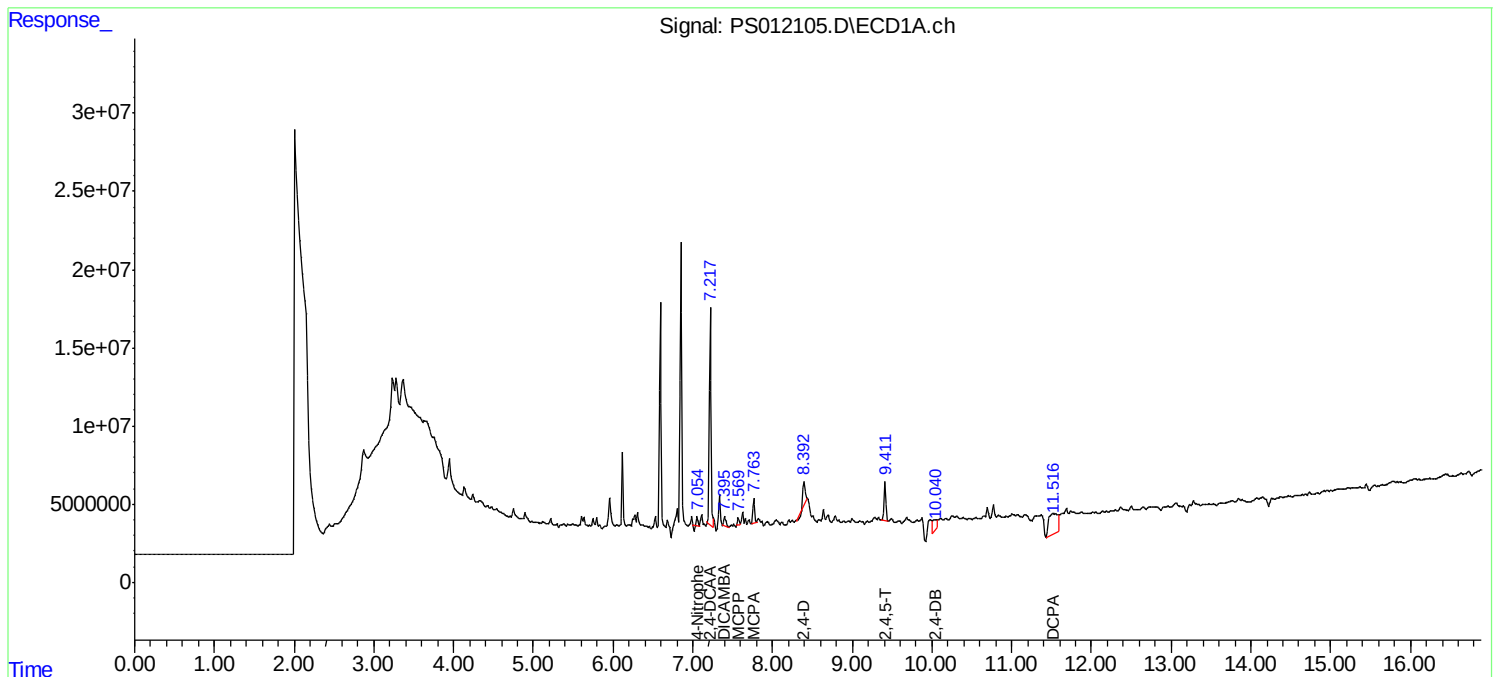


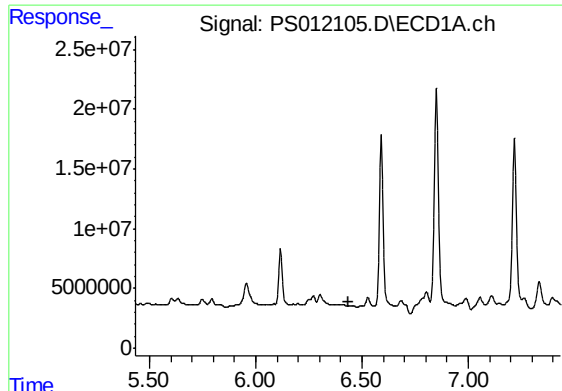

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-01-A

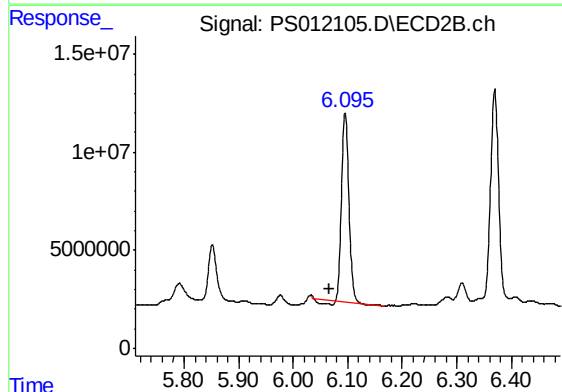


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 88874385
Conc: 108.04 ng/ml

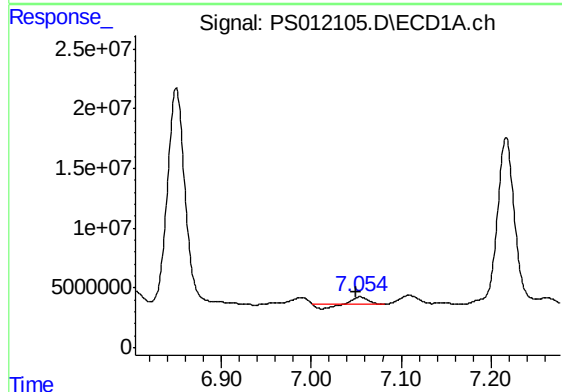


#3 4-Nitrophenol

R.T.: 7.054 min
Delta R.T.: 0.004 min
Response: 2720258
Conc: 4.62 ng/ml

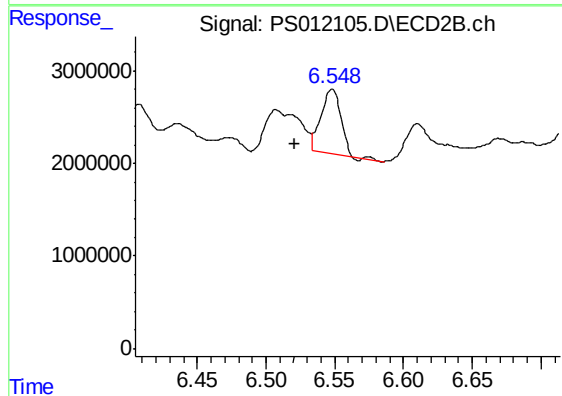

#3 4-Nitrophenol


R.T.: 6.548 min
Delta R.T.: 0.027 min
Response: 7047363
Conc: 19.33 ng/ml

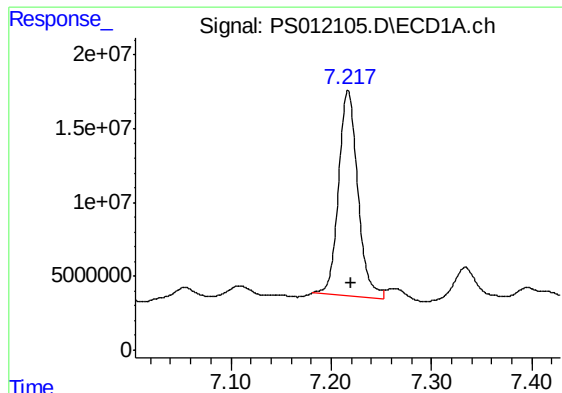

#4 2,4-DCAA


R.T.: 7.217 min
Delta R.T.: -0.003 min
Response: 184509599
Conc: 169.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-01-A

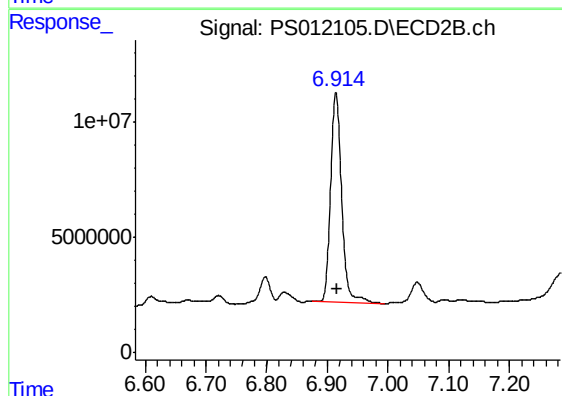


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 113392078
Conc: 212.03 ng/ml

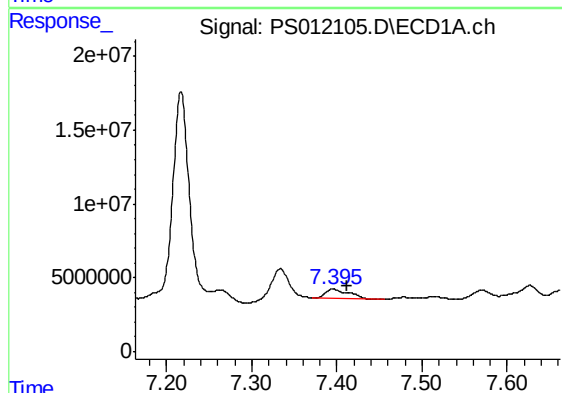


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.016 min
Response: 11407450
Conc: 2.79 ng/ml

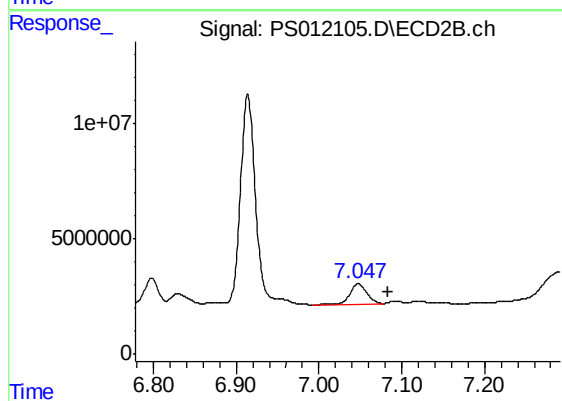

#5 DICAMBA


R.T.: 7.048 min
Delta R.T.: -0.037 min
Response: 12474612
Conc: 5.77 ng/ml

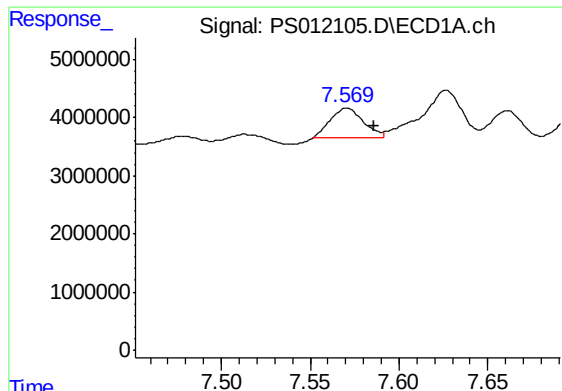

#6 MCPP


R.T.: 7.571 min
Delta R.T.: -0.016 min
Response: 6741861
Conc: 2.11 ug/ml

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-01-A

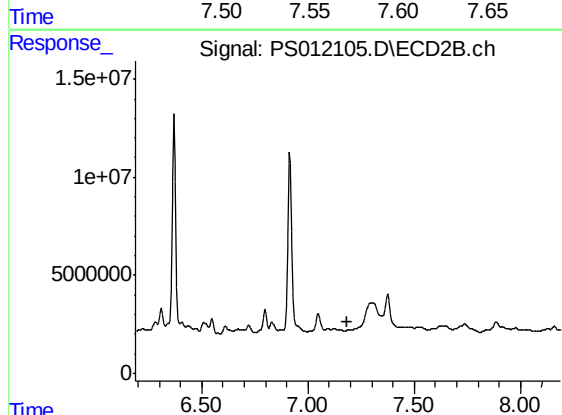


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

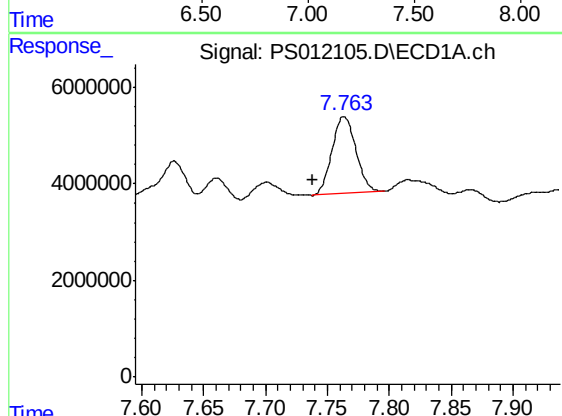


#7 MCPA

R.T.: 7.764 min
Delta R.T.: 0.025 min
Response: 21645788
Conc: 4.76 ug/ml

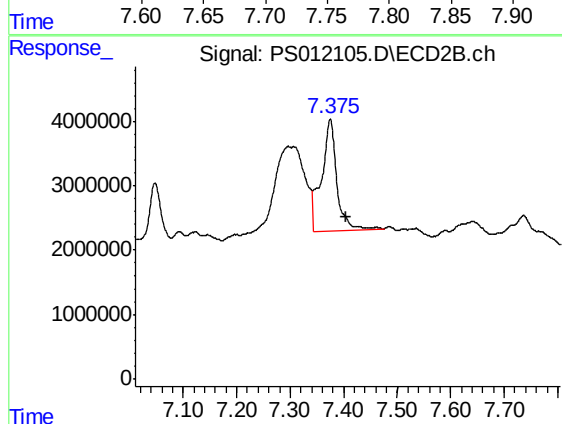

#7 MCPA


R.T.: 7.375 min
Delta R.T.: -0.030 min
Response: 34487244
Conc: 12.59 ug/ml

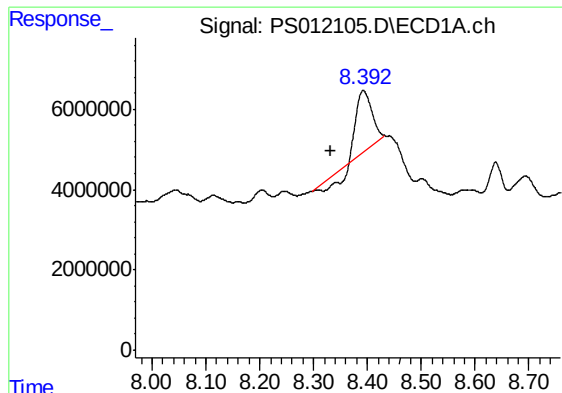

#9 2,4-D


R.T.: 8.392 min
Delta R.T.: 0.060 min
Response: 25579369
Conc: 22.65 ng/ml

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-01-A

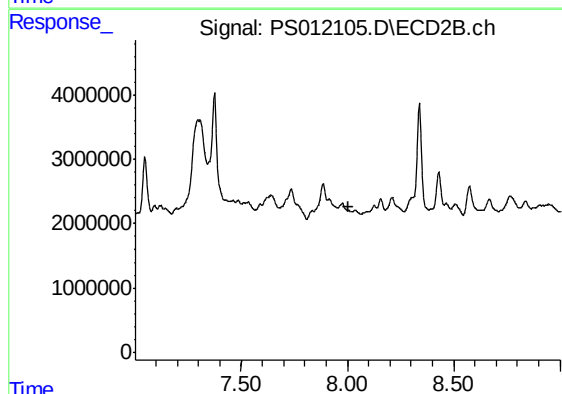


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

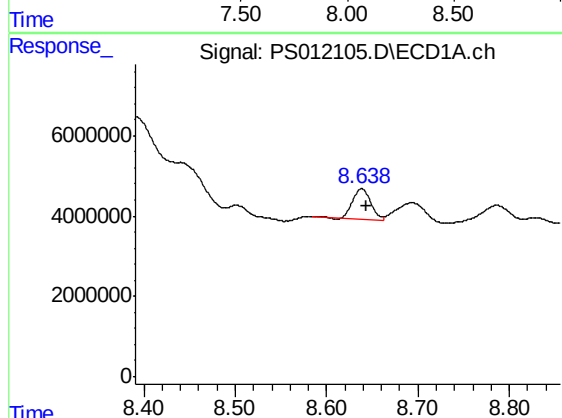


#10 Pentachlorophenol

R.T.: 8.638 min
Delta R.T.: -0.005 min
Response: 10081576
Conc: N.D.

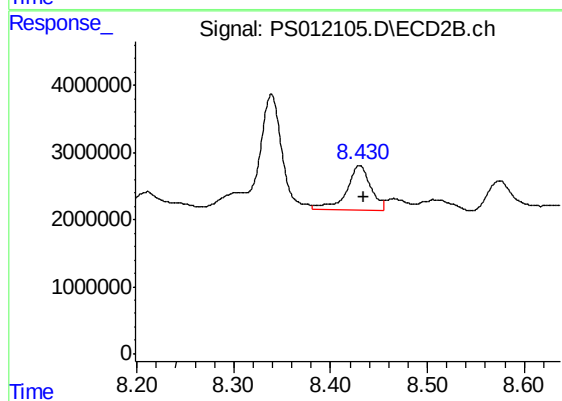

#10 Pentachlorophenol


R.T.: 8.430 min
Delta R.T.: -0.004 min
Response: 11505728
Conc: 1.69 ng/ml

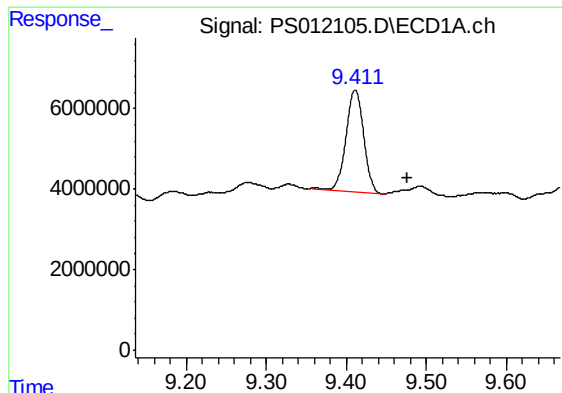

#12 2,4,5-T


R.T.: 9.411 min
Delta R.T.: -0.065 min
Response: 38284491
Conc: 6.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-01-A

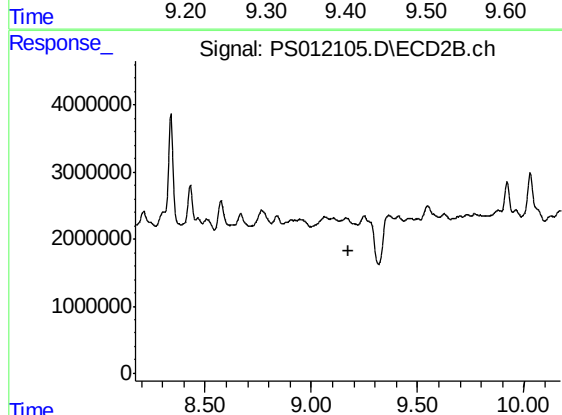


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

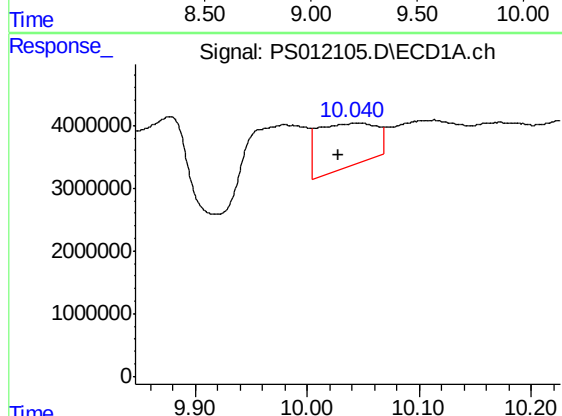


#13 2,4-DB

R.T.: 10.045 min
Delta R.T.: 0.017 min
Response: 25156461
Conc: 31.66 ng/ml

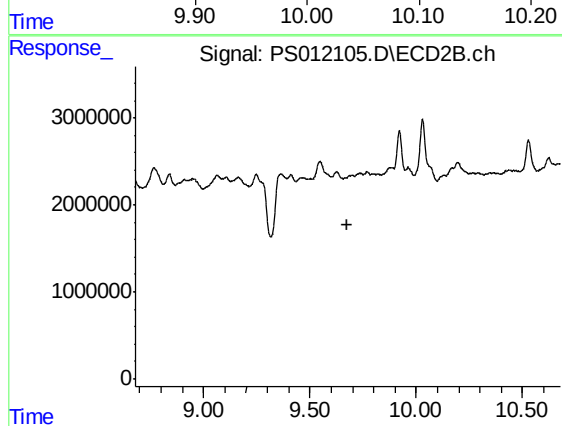

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.679 min
Response: 0
Conc: N.D.

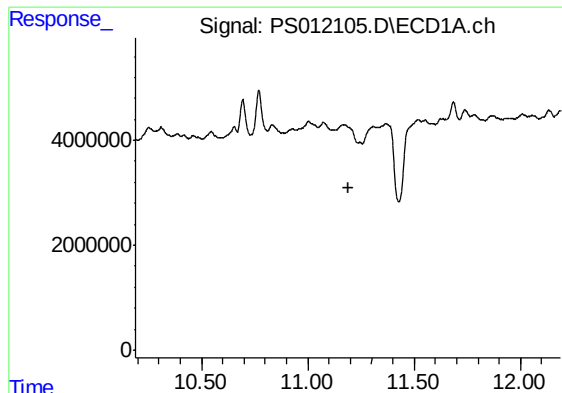

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.189 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-01-A

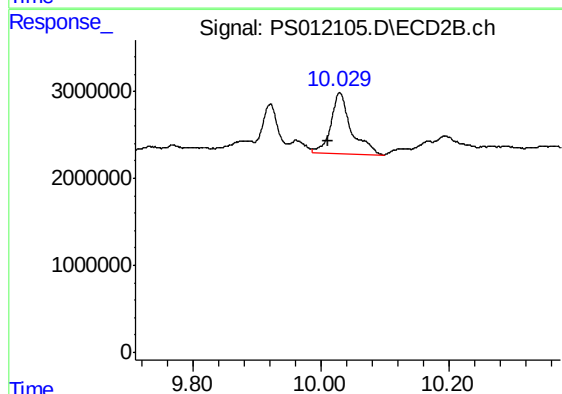


#14 DINOSEB

R.T.: 10.030 min
Delta R.T.: 0.018 min
Response: 15420500
Conc: 7.25 ng/ml

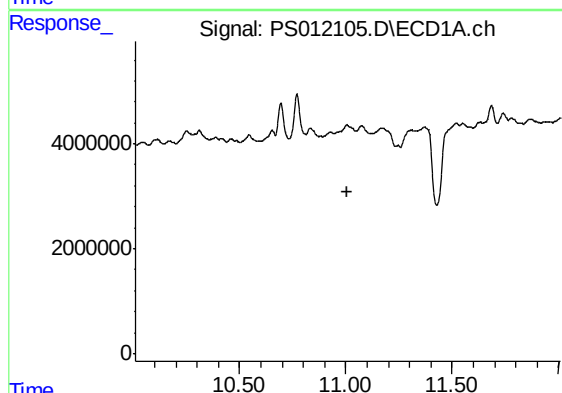


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.009 min
Response: 0
Conc: N.D.

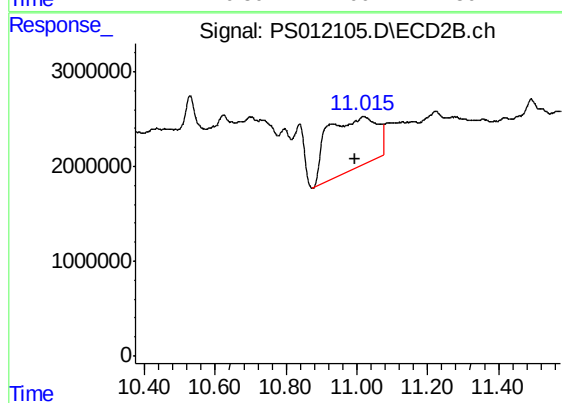

#15 Picloram


R.T.: 11.018 min
Delta R.T.: 0.023 min
Response: 53447980
Conc: 11.79 ng/ml

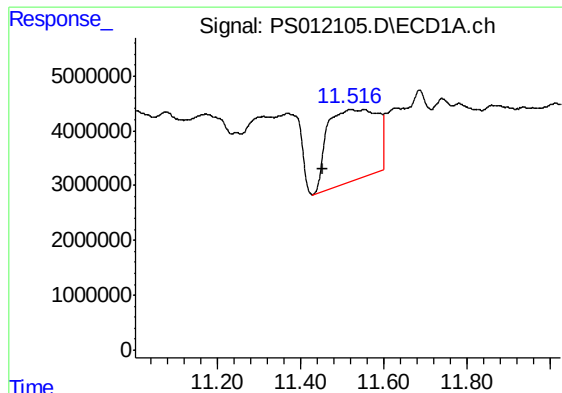

#16 DCPA

R.T.: 11.519 min
Delta R.T.: 0.065 min
Response: 107955994
Conc: 14.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-01-A

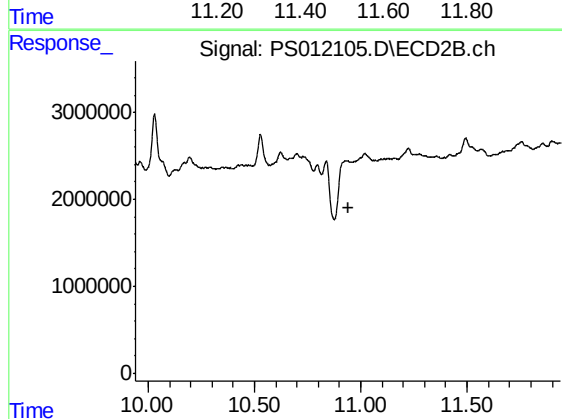

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.940 min
Response: 0
Conc: N.D.