

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090320\
 Data File : PS012106.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2020 22:31
 Operator : DD\AJ
 Sample : L3848-11
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 LINDEN-BH-04-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 06:14:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.913	279.0E6	159.1E6	255.793	297.525
Target Compounds							
2) T	3,5-DICHL...	0.000	6.095	0	75287014	N.D.	91.521
3) T	4-Nitroph...	7.055	0.000	6674142	0	11.331	N.D. #
5) T	DICAMBA	7.395	7.046	8735584	10881697	2.133	5.037 #
6) T	MCPD	7.572	0.000	8499404	0	2.660	N.D. #
7) T	MCPA	7.764	7.374	19898479	32580875	4.375	11.890 #
9) T	2,4-D	8.393	0.000	20107629	0	17.809	N.D. #
11) T	2,4,5-TP ...	0.000	8.763	0	8142996	N.D.	2.785
12) T	2,4,5-T	9.412	0.000	34159386	0	5.764	N.D. #
13) T	2,4-DB	10.036	0.000	26083137	0	32.826	N.D. #
14) T	DINOSEB	0.000	10.029	0	14139608	N.D.	6.651
15) T	Picloram	0.000	11.020	0	32571677	N.D.	7.186
16) T	DCPA	11.519	0.000	59256141	0	7.793	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090320\
Data File : PS012106.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2020 22:31
Operator : DD\AJ
Sample : L3848-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-04-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 06:14:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

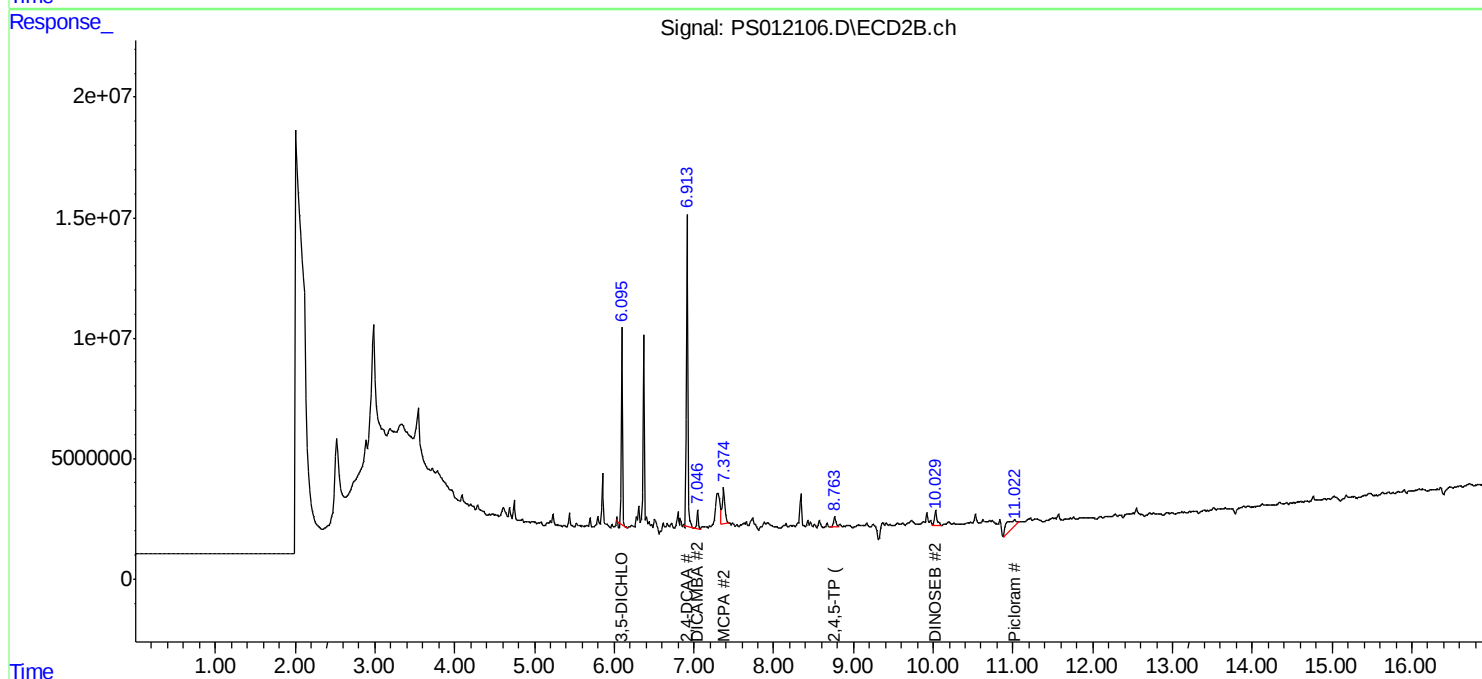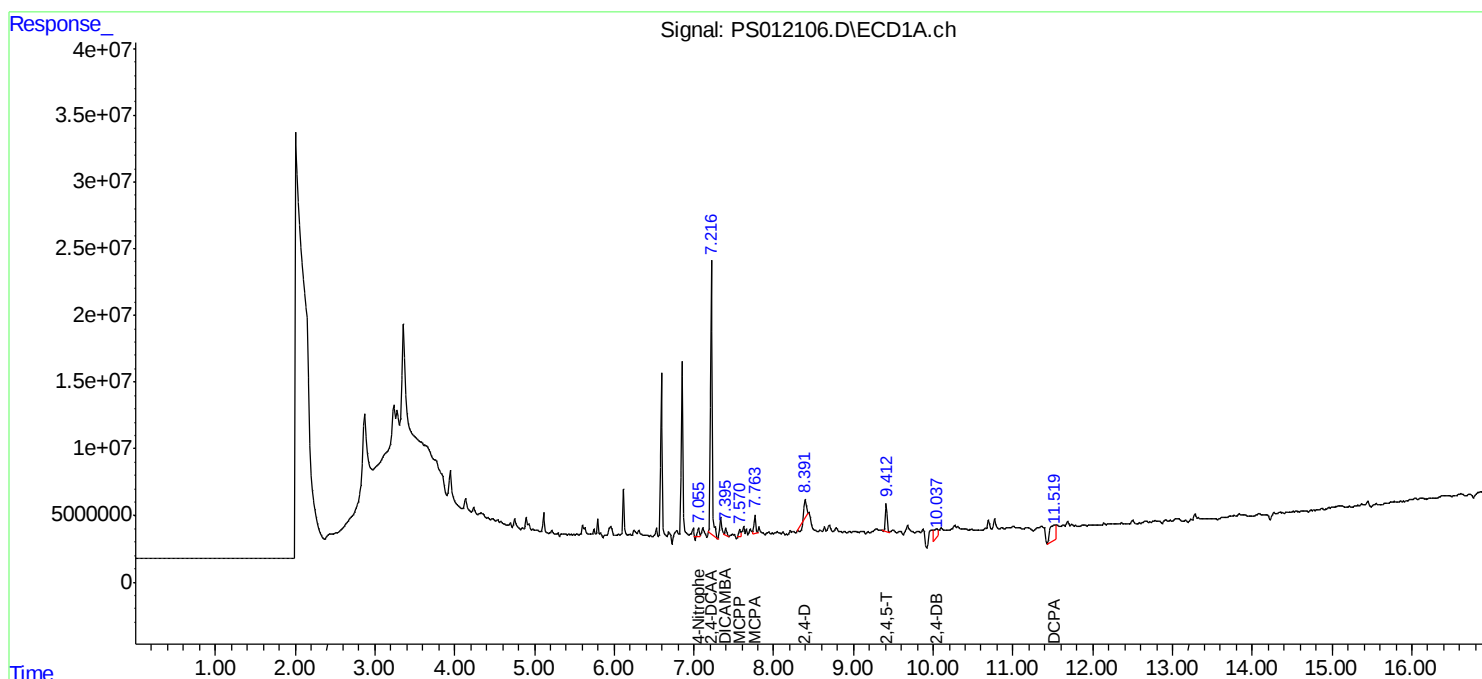


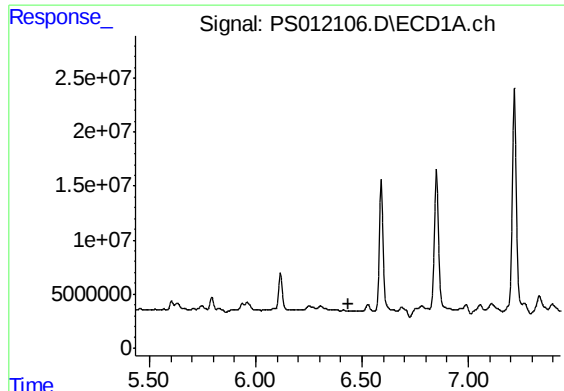

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-04-A

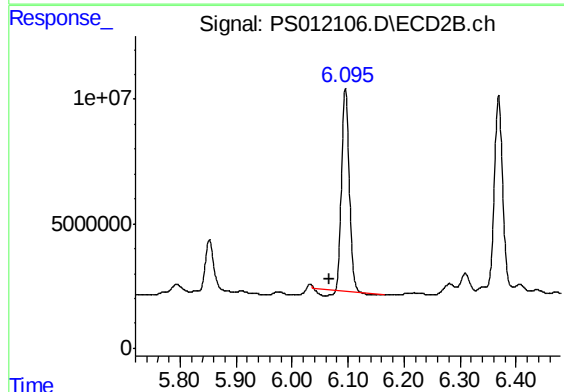


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.029 min
Response: 75287014
Conc: 91.52 ng/ml

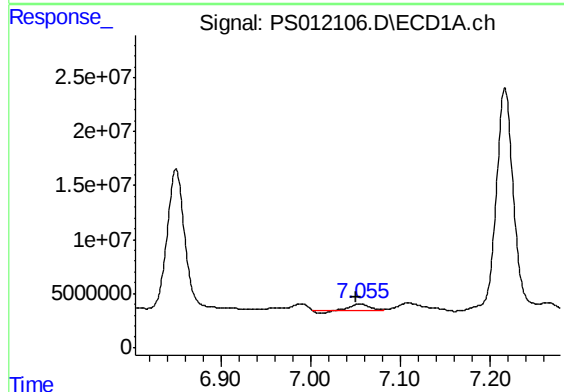


#3 4-Nitrophenol

R.T.: 7.055 min
Delta R.T.: 0.005 min
Response: 6674142
Conc: 11.33 ng/ml

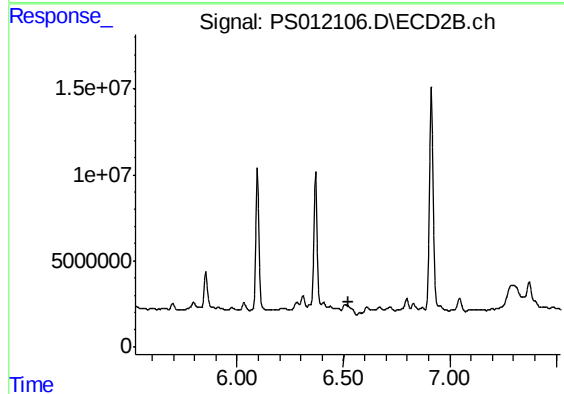

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.521 min
Response: 0
Conc: N.D.

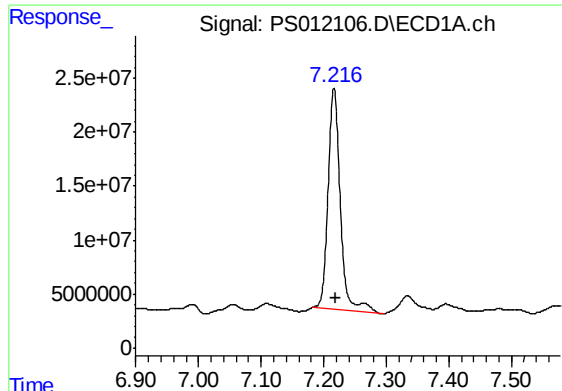

#4 2,4-DCAA


R.T.: 7.217 min
Delta R.T.: -0.004 min
Response: 279011175
Conc: 255.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-04-A

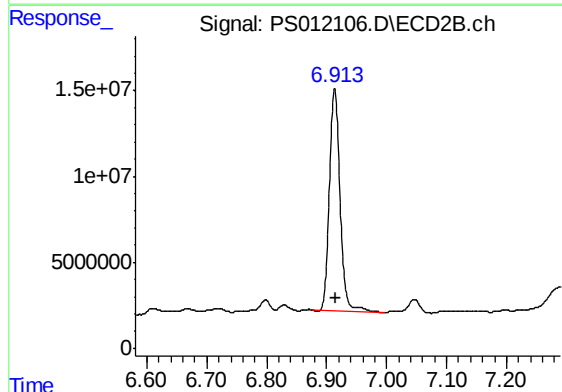


#4 2,4-DCAA

R.T.: 6.913 min
Delta R.T.: -0.002 min
Response: 159112257
Conc: 297.52 ng/ml

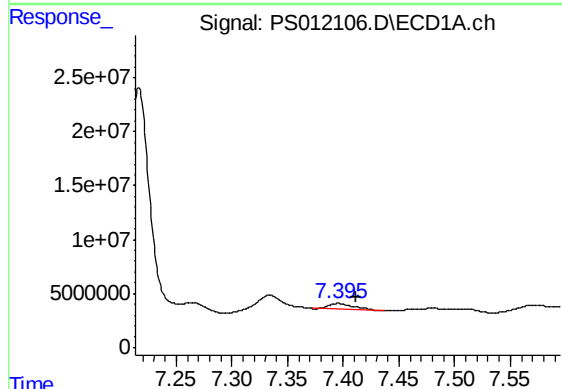


#5 DICAMBA

R.T.: 7.395 min
Delta R.T.: -0.016 min
Response: 8735584
Conc: 2.13 ng/ml

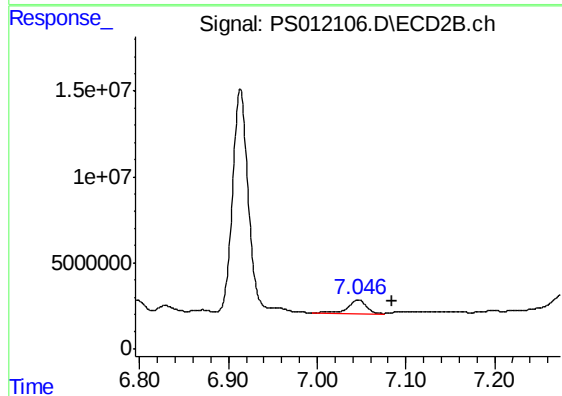

#5 DICAMBA


R.T.: 7.046 min
Delta R.T.: -0.038 min
Response: 10881697
Conc: 5.04 ng/ml

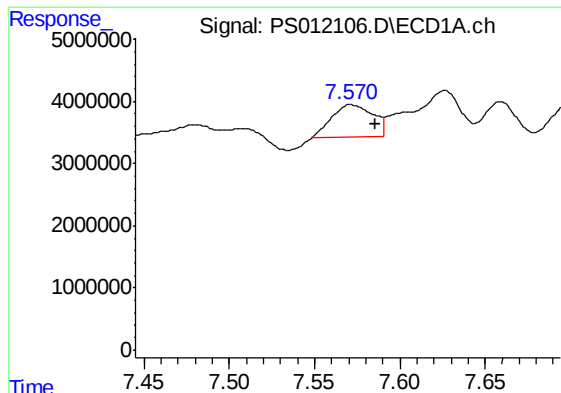

#6 MCPP


R.T.: 7.572 min
Delta R.T.: -0.014 min
Response: 8499404
Conc: 2.66 ug/ml

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-04-A

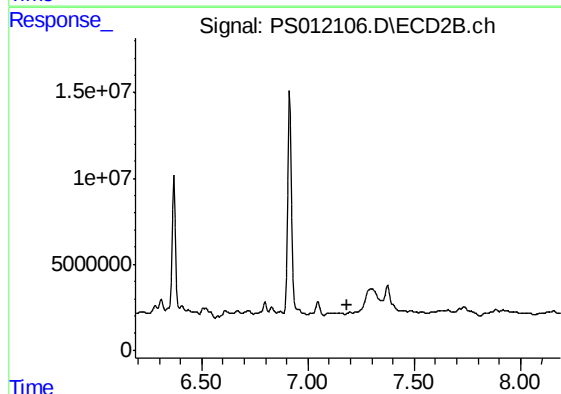


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

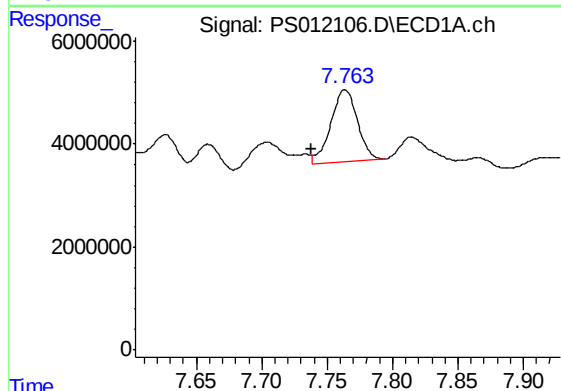


#7 MCPA

R.T.: 7.764 min
Delta R.T.: 0.025 min
Response: 19898479
Conc: 4.37 ug/ml

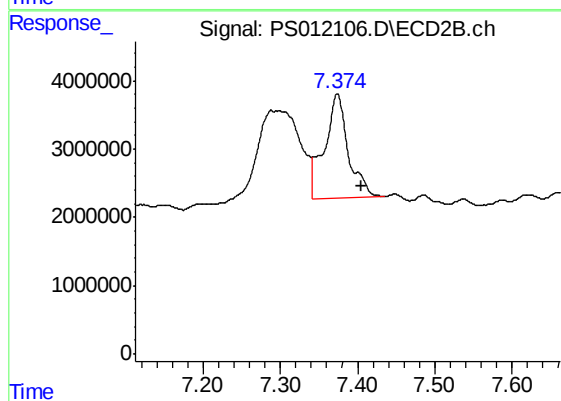

#7 MCPA


R.T.: 7.374 min
Delta R.T.: -0.031 min
Response: 32580875
Conc: 11.89 ug/ml

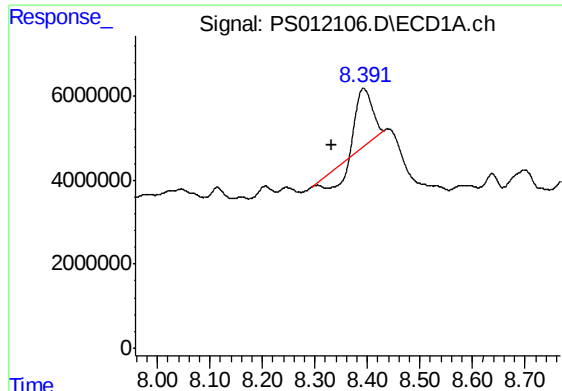

#9 2,4-D


R.T.: 8.393 min
Delta R.T.: 0.061 min
Response: 20107629
Conc: 17.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-04-A

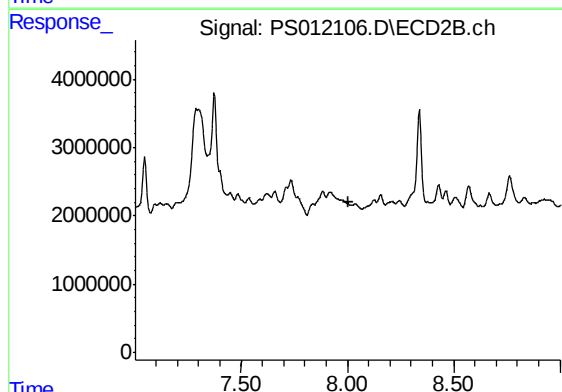


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

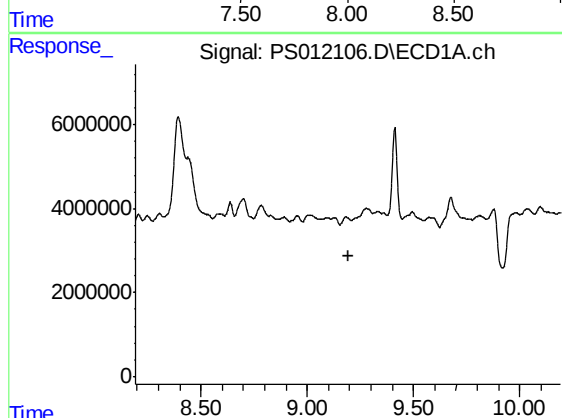


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

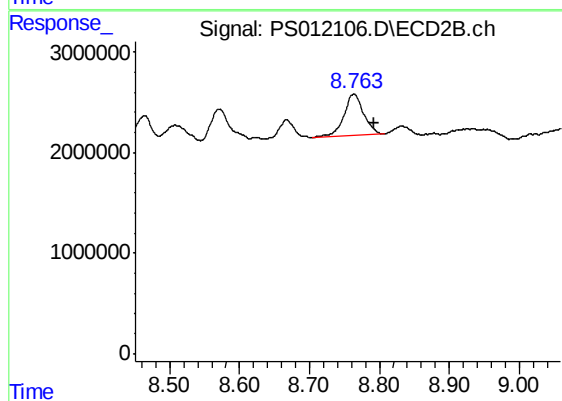

#11 2,4,5-TP (SILVEX)


R.T.: 8.763 min
Delta R.T.: -0.030 min
Response: 8142996
Conc: 2.79 ng/ml

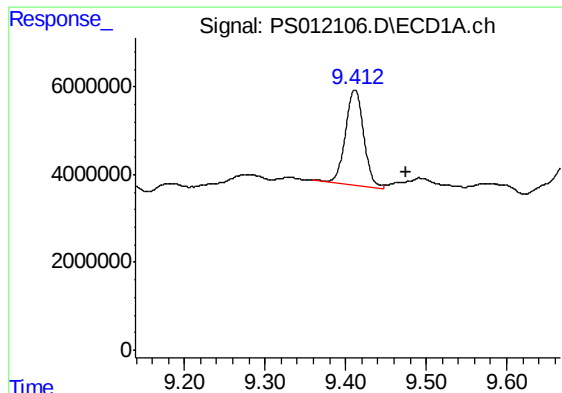

#12 2,4,5-T


R.T.: 9.412 min
Delta R.T.: -0.064 min
Response: 34159386
Conc: 5.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-04-A

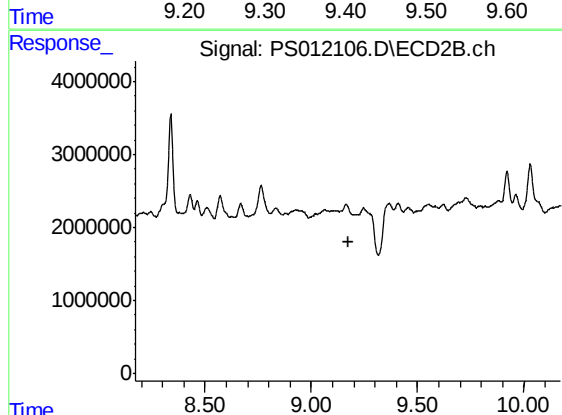


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

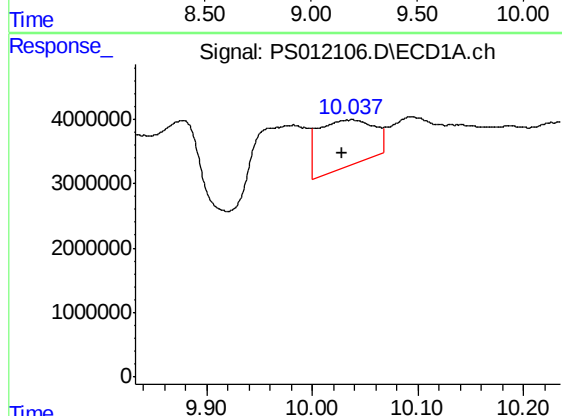


#13 2,4-DB

R.T.: 10.036 min
Delta R.T.: 0.008 min
Response: 26083137
Conc: 32.83 ng/ml

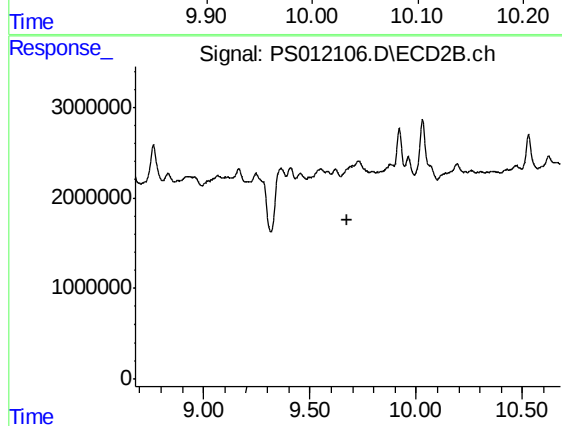

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.679 min
Response: 0
Conc: N.D.

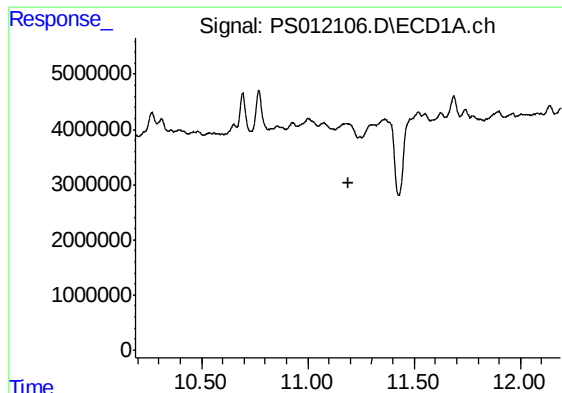

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.189 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-04-A

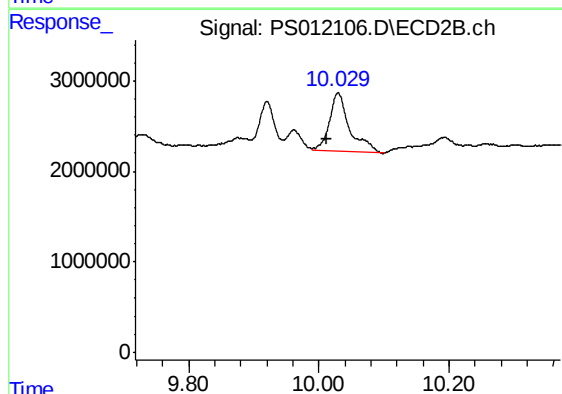


#14 DINOSEB

R.T.: 10.029 min
Delta R.T.: 0.018 min
Response: 14139608
Conc: 6.65 ng/ml

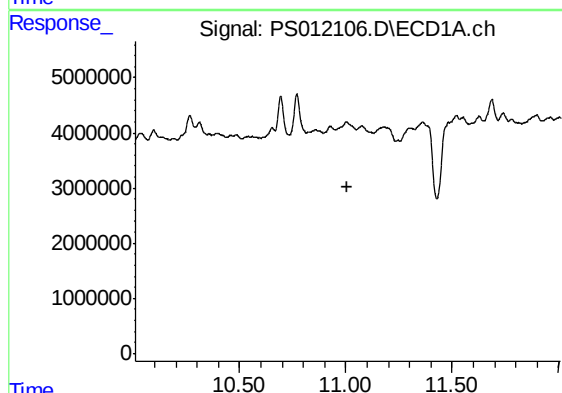


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.009 min
Response: 0
Conc: N.D.

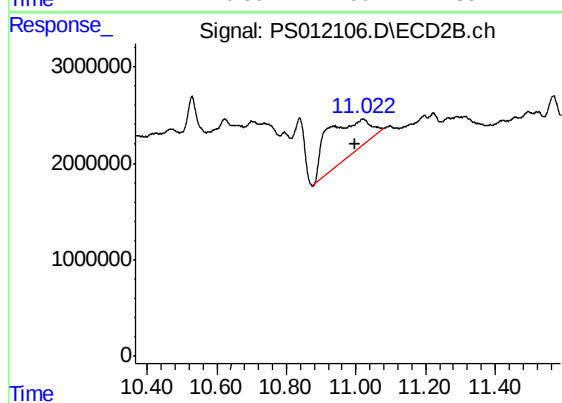

#15 Picloram


R.T.: 11.020 min
Delta R.T.: 0.024 min
Response: 32571677
Conc: 7.19 ng/ml

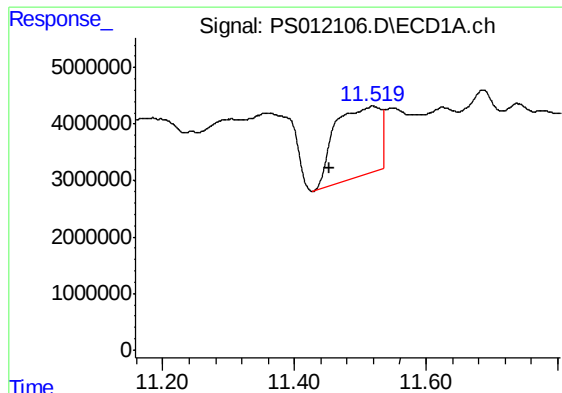

#16 DCPA

R.T.: 11.519 min
Delta R.T.: 0.065 min
Response: 59256141
Conc: 7.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
LINDEN-BH-04-A

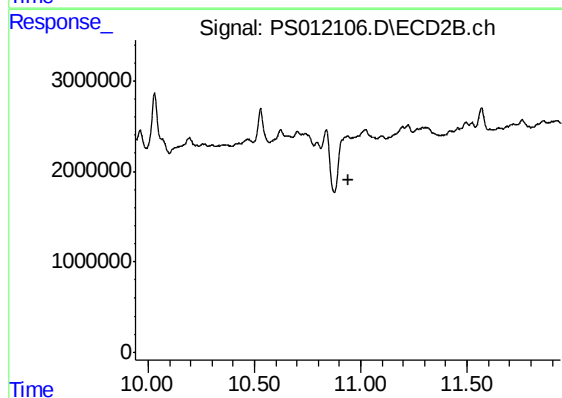

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.940 min
Response: 0
Conc: N.D.