

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090320\
 Data File : PS012116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2020 02:21
 Operator : DD\AJ
 Sample : L3871-04
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TR-05-090220

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 06:17:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.218	6.914	285.9E6	176.4E6	262.127	329.760 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.095	0	98995337	N.D.	120.342
3) T	4-Nitroph...	7.055	0.000	6350694	0	10.781	N.D. #
5) T	DICAMBA	7.395	7.046	9253283	12872423	2.259	5.958 #
6) T	MCP	7.628	0.000	8630345	0	2.701	N.D. #
7) T	MCPA	7.691	7.406	165.0E6	9862484	36.269	3.599 #
8) T	DICHLORPROP	0.000	7.735	0	25205179	N.D.	44.640
9) T	2,4-D	8.396	0.000	28111212	0	24.897	N.D. #
11) T	2,4,5-TP ...	0.000	8.761	0	21987204	N.D.	7.520
12) T	2,4,5-T	9.411	0.000	22252183	0	3.755	N.D. #
13) T	2,4-DB	9.989	0.000	11213476	0	14.113	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090320\
Data File : PS012116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2020 02:21
Operator : DD\AJ
Sample : L3871-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
TR-05-090220

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 06:17:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

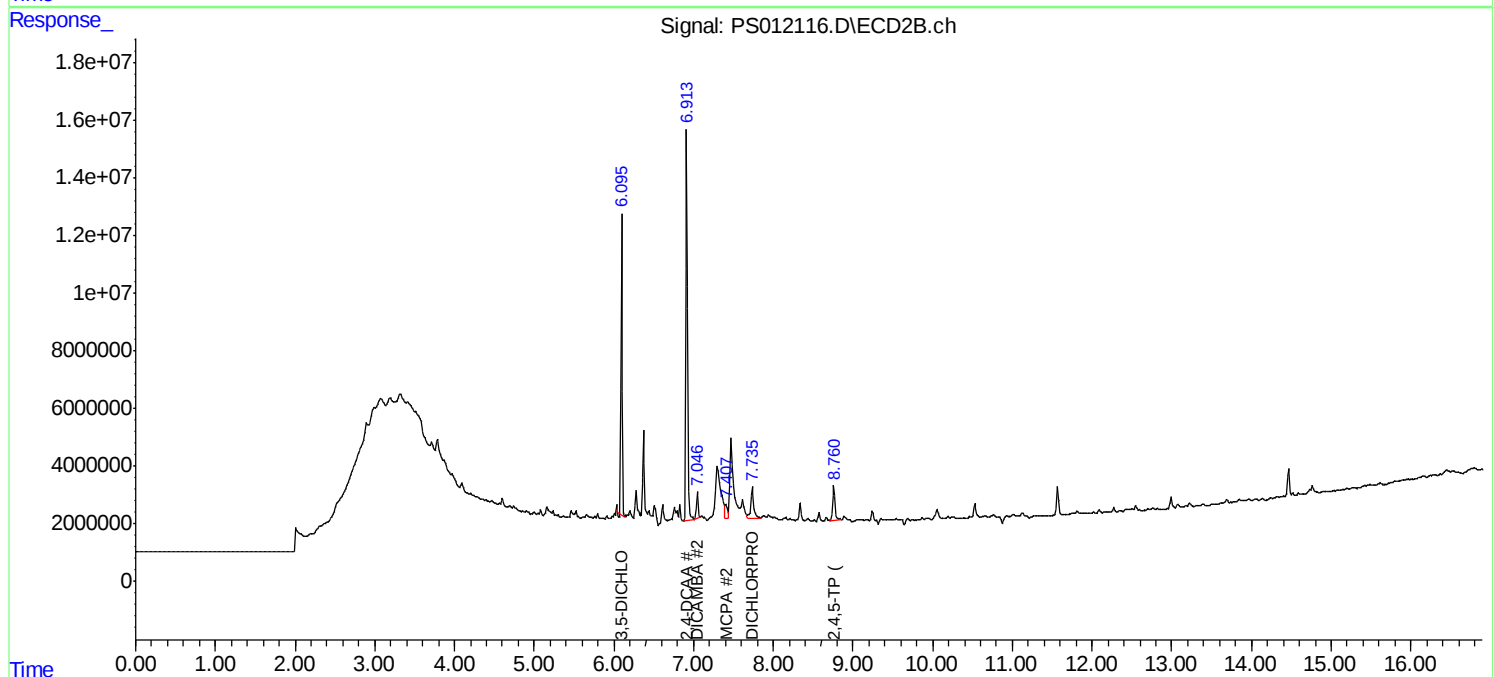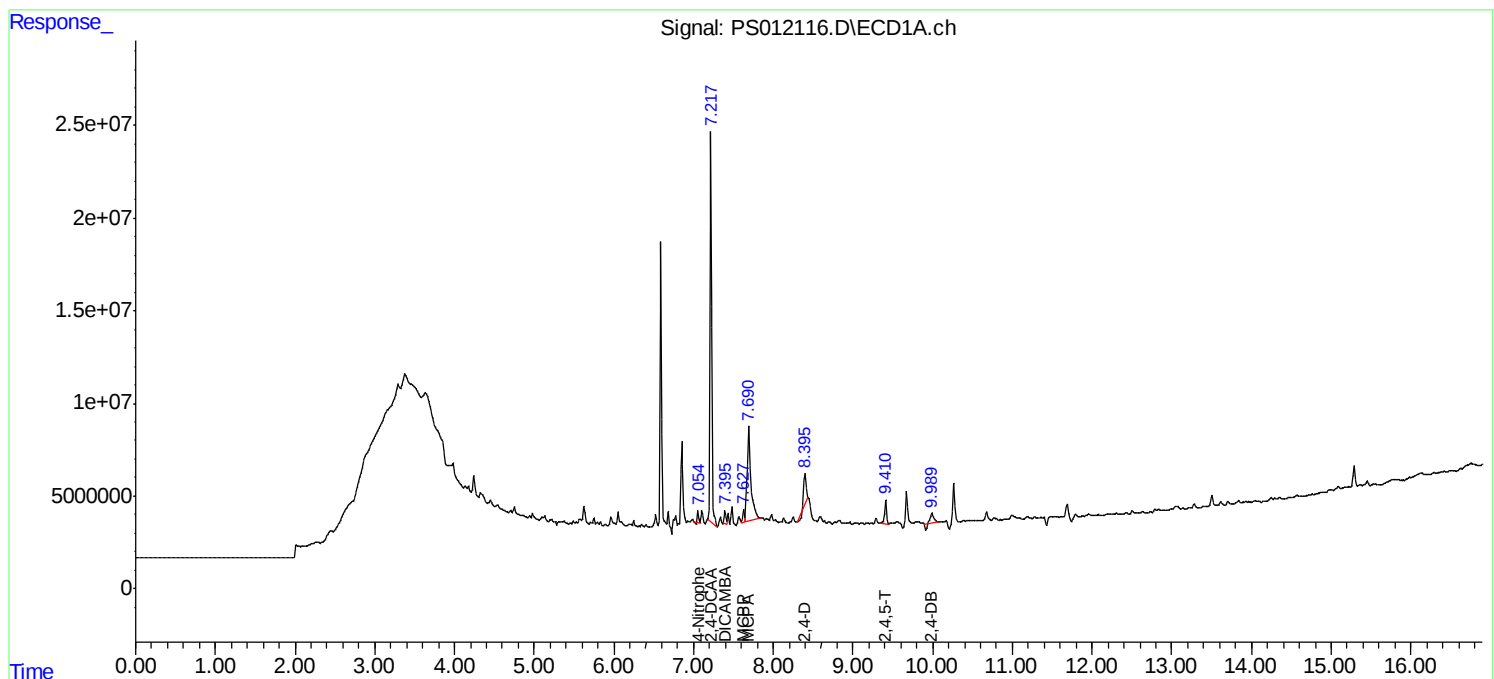


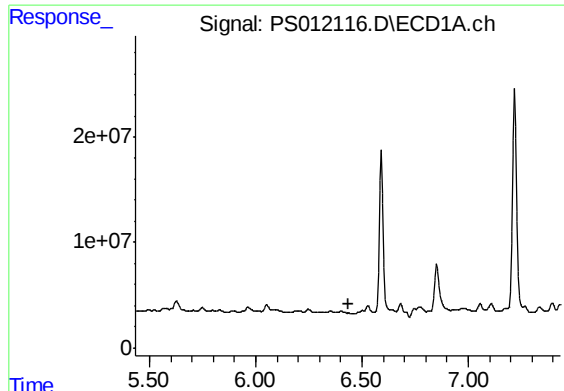

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-05-090220

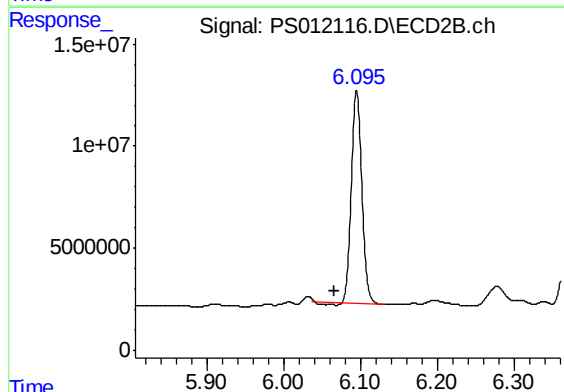


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.029 min
Response: 98995337
Conc: 120.34 ng/ml

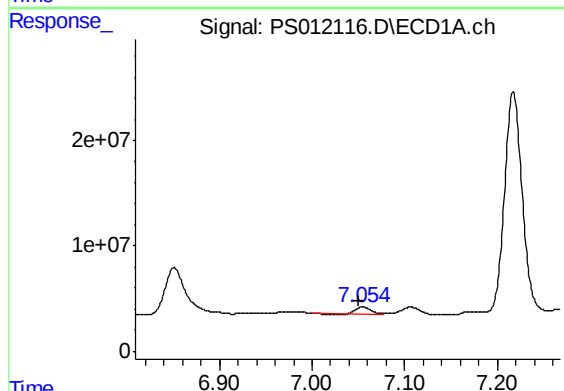


#3 4-Nitrophenol

R.T.: 7.055 min
Delta R.T.: 0.004 min
Response: 6350694
Conc: 10.78 ng/ml

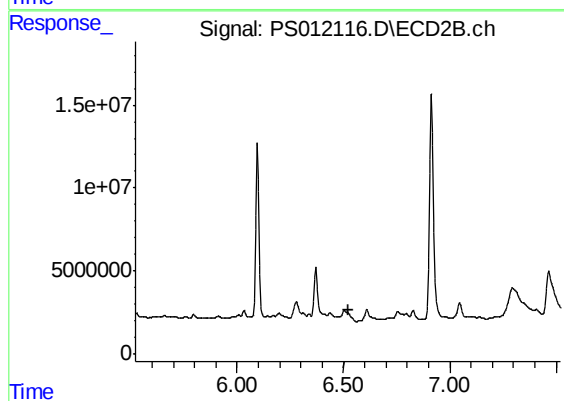

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.521 min
Response: 0
Conc: N.D.

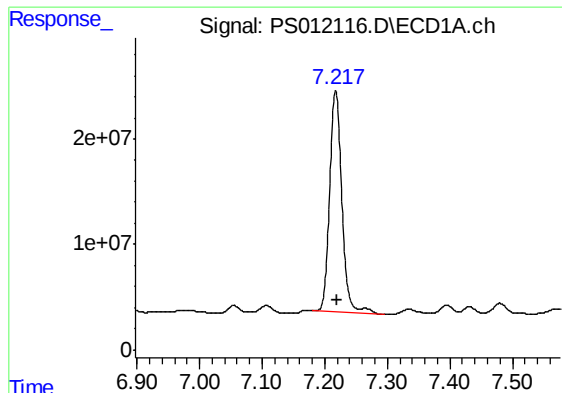

#4 2,4-DCAA


R.T.: 7.218 min
Delta R.T.: -0.003 min
Response: 285919745
Conc: 262.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-05-090220

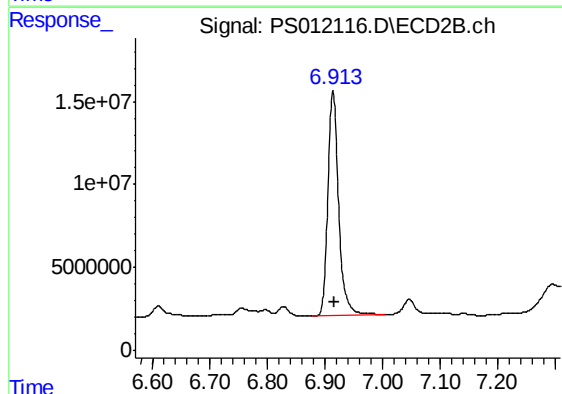


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: -0.001 min
Response: 176351121
Conc: 329.76 ng/ml

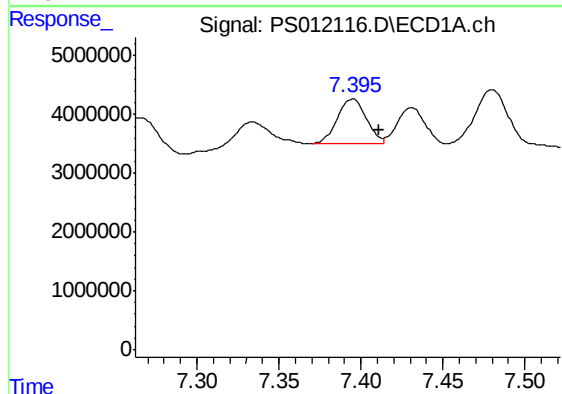


#5 DICAMBA

R.T.: 7.395 min
Delta R.T.: -0.017 min
Response: 9253283
Conc: 2.26 ng/ml

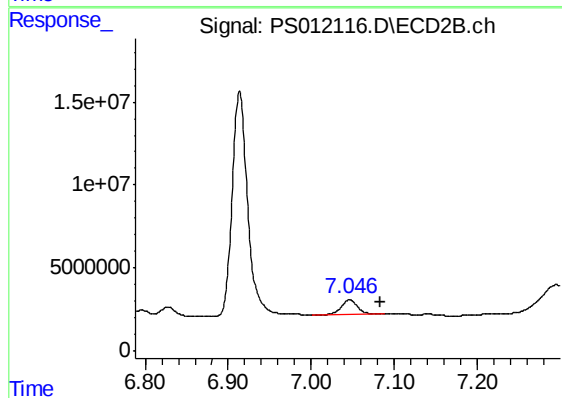

#5 DICAMBA


R.T.: 7.046 min
Delta R.T.: -0.038 min
Response: 12872423
Conc: 5.96 ng/ml

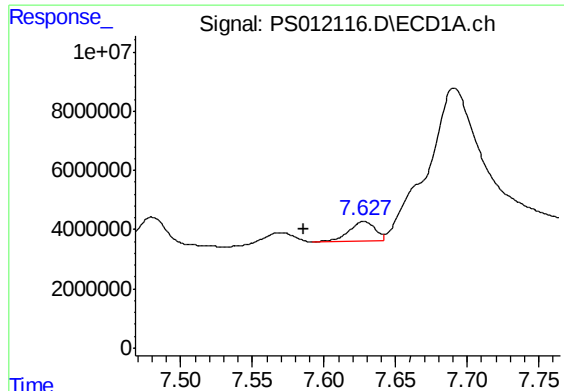

#6 MCPP


R.T.: 7.628 min
Delta R.T.: 0.042 min
Response: 8630345
Conc: 2.70 ug/ml

Instrument :
ECD_S
ClientSampleId :
TR-05-090220

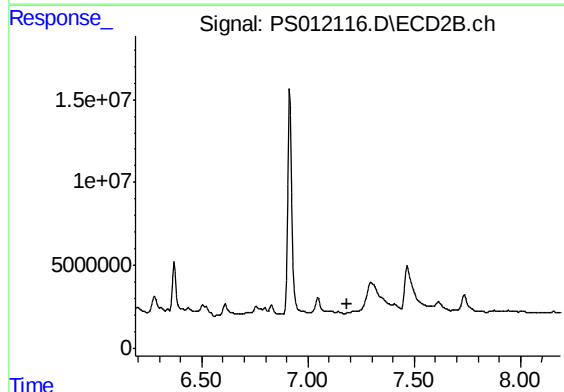


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

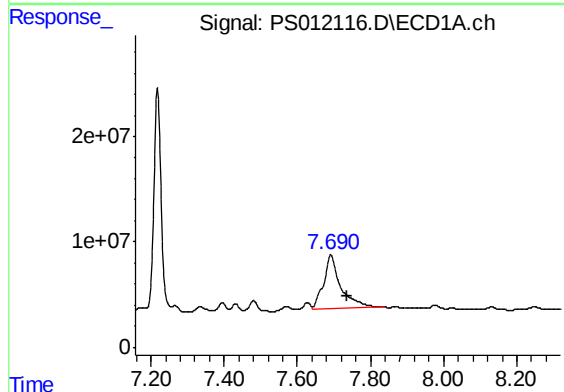


#7 MCPA

R.T.: 7.691 min
Delta R.T.: -0.047 min
Response: 164968181
Conc: 36.27 ug/ml

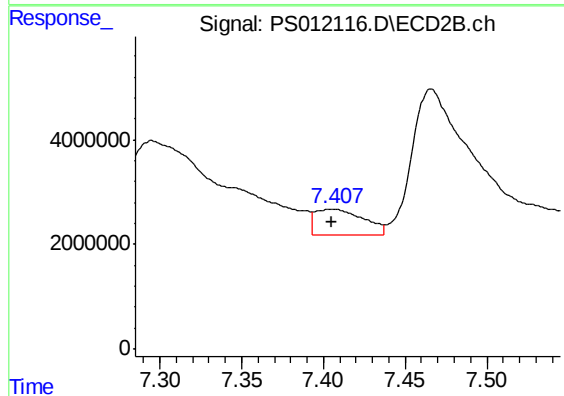

#7 MCPA


R.T.: 7.406 min
Delta R.T.: 0.000 min
Response: 9862484
Conc: 3.60 ug/ml

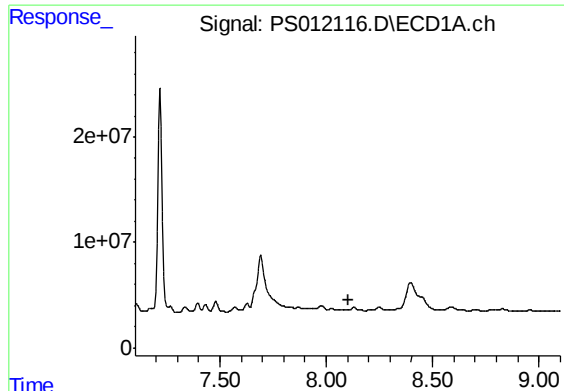

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-05-090220

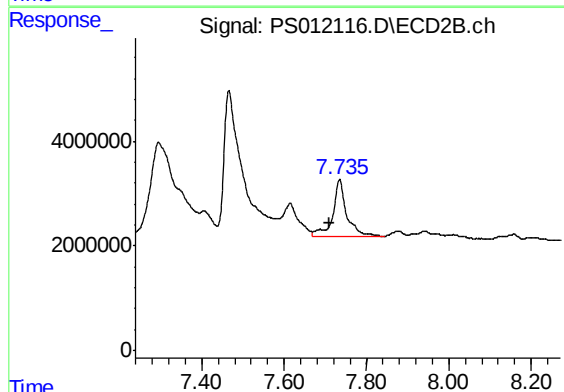


#8 DICHLORPROP

R.T.: 7.735 min
Delta R.T.: 0.025 min
Response: 25205179
Conc: 44.64 ng/ml

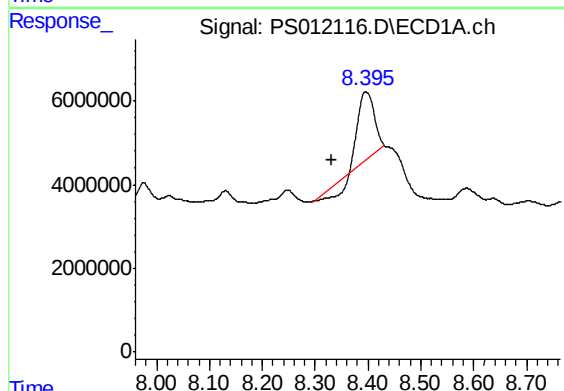


#9 2,4-D

R.T.: 8.396 min
Delta R.T.: 0.064 min
Response: 28111212
Conc: 24.90 ng/ml

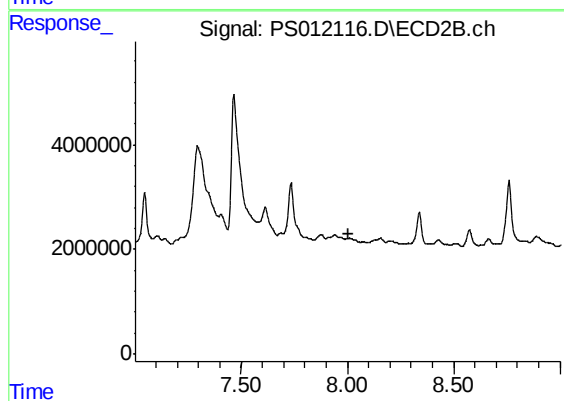

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

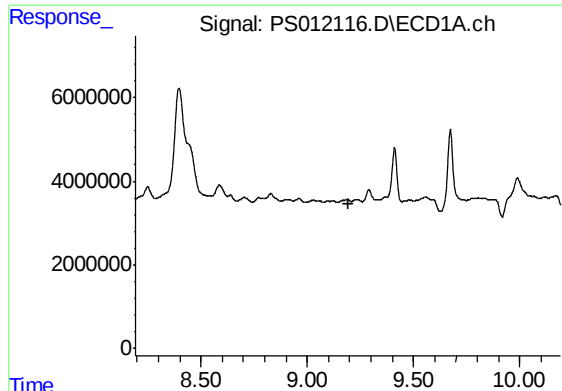

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-05-090220

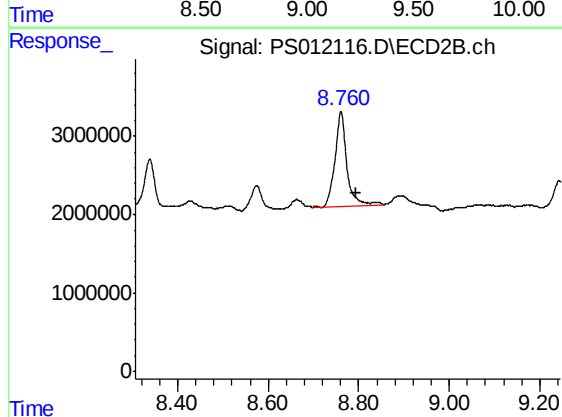


#11 2,4,5-TP (SILVEX)

R.T.: 8.761 min
Delta R.T.: -0.033 min
Response: 21987204
Conc: 7.52 ng/ml

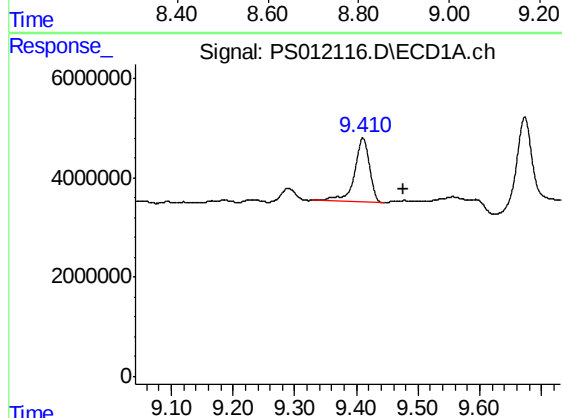


#12 2,4,5-T

R.T.: 9.411 min
Delta R.T.: -0.065 min
Response: 22252183
Conc: 3.76 ng/ml

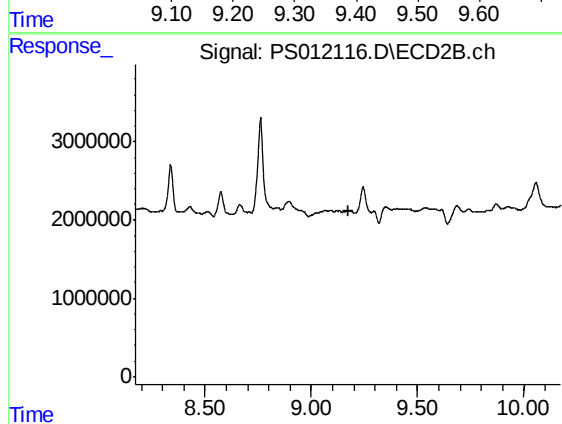

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.

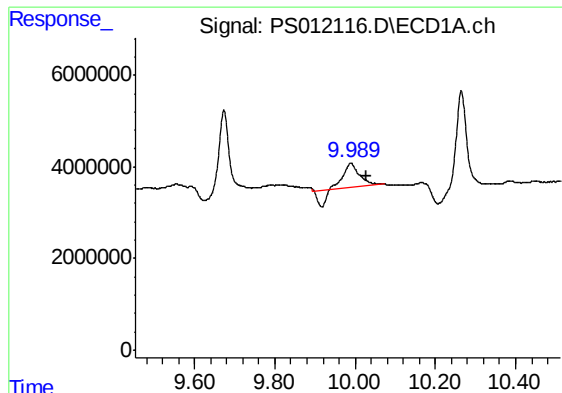

#13 2,4-DB

R.T.: 9.989 min
Delta R.T.: -0.039 min
Response: 11213476
Conc: 14.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-05-090220

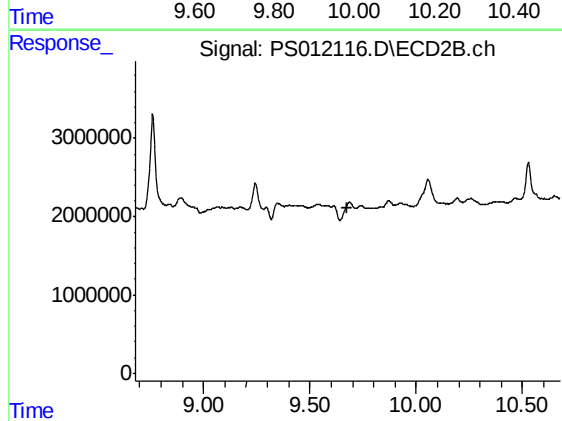

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.679 min
Response: 0
Conc: N.D.