

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090322\
 Data File : PS020445.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2022 06:49
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 21:52:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 03 01:09:33 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.176	6.756	1315.5E6	442.3E6	373.236	411.596
Target Compounds							
1) T	Dalapon	3.039f	0.000	666326	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.438	0.000	38995756	0	8.178	N.D. #
5) T	DICAMBA	7.427f	6.980f	943173	9672371	<MDL	2.021 #
6) T	MCP	7.591f	6.980	900221	9672371	<MDL	2.631 #
7) T	MCPA	7.670	0.000	27403742	0	1.777	N.D. #
8) T	DICHLORPROP	8.081	7.591f	4184781	7669868	1.137	6.137 #
9) T	2,4-D	8.360f	7.789f	195.4E6	1933475	41.651	1.273 #
10) T	Pentachlo...	8.622	0.000	907705	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.095f	0.000	12296946	0	<MDL	N.D. #
12) T	2,4,5-T	9.446	0.000	1510265	0	<MDL	N.D. #
13) T	2,4-DB	0.000	9.570f	0	6696092	N.D.	7.395
14) T	DINOSEB	11.103	9.837	18816645	1745925	<MDL	<MDL #
15) T	Picloram	10.987	10.828	74764122	17069362	1.806	1.662
16) T	DCPA	11.373	10.747	13775885	12678244	<MDL	1.423 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090322\
Data File : PS020445.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2022 06:49
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 21:52:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
Quant Title : 8080.M
QLast Update : Sat Sep 03 01:09:33 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

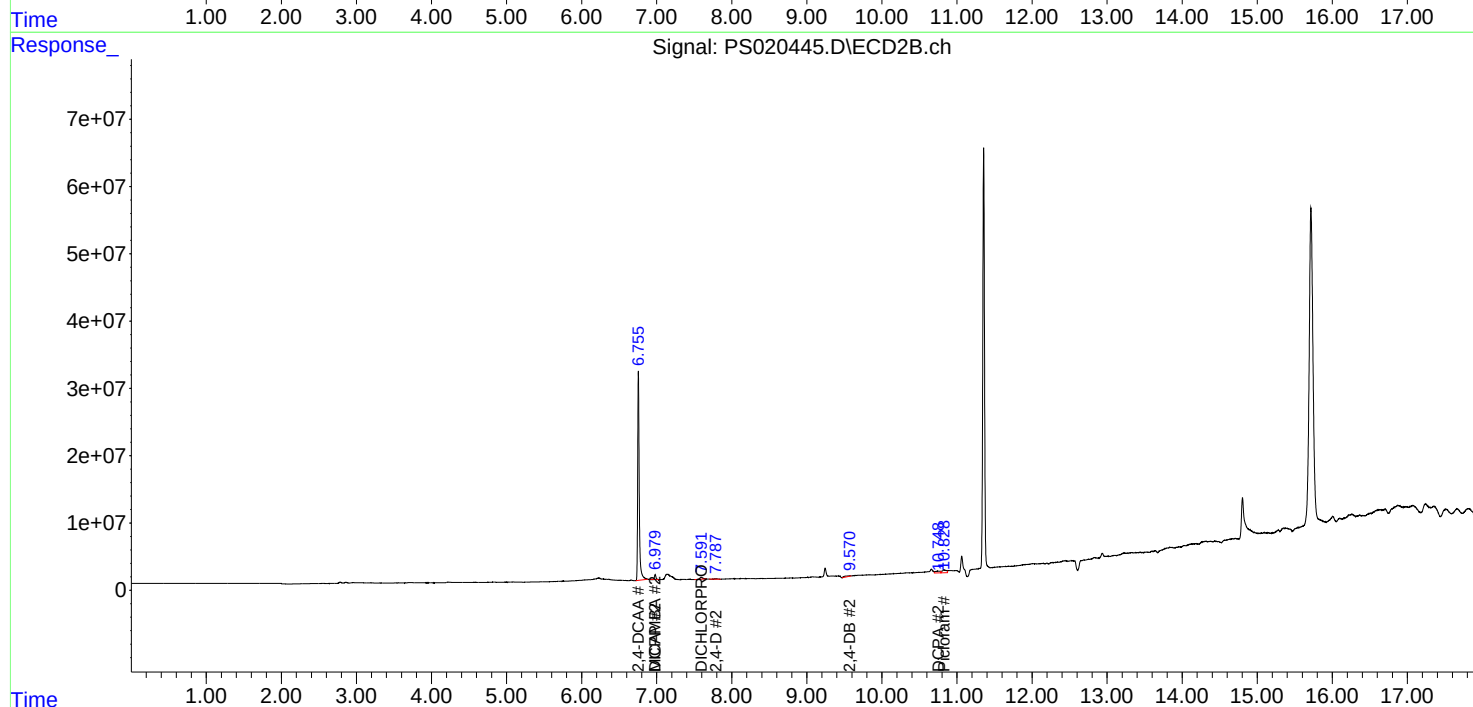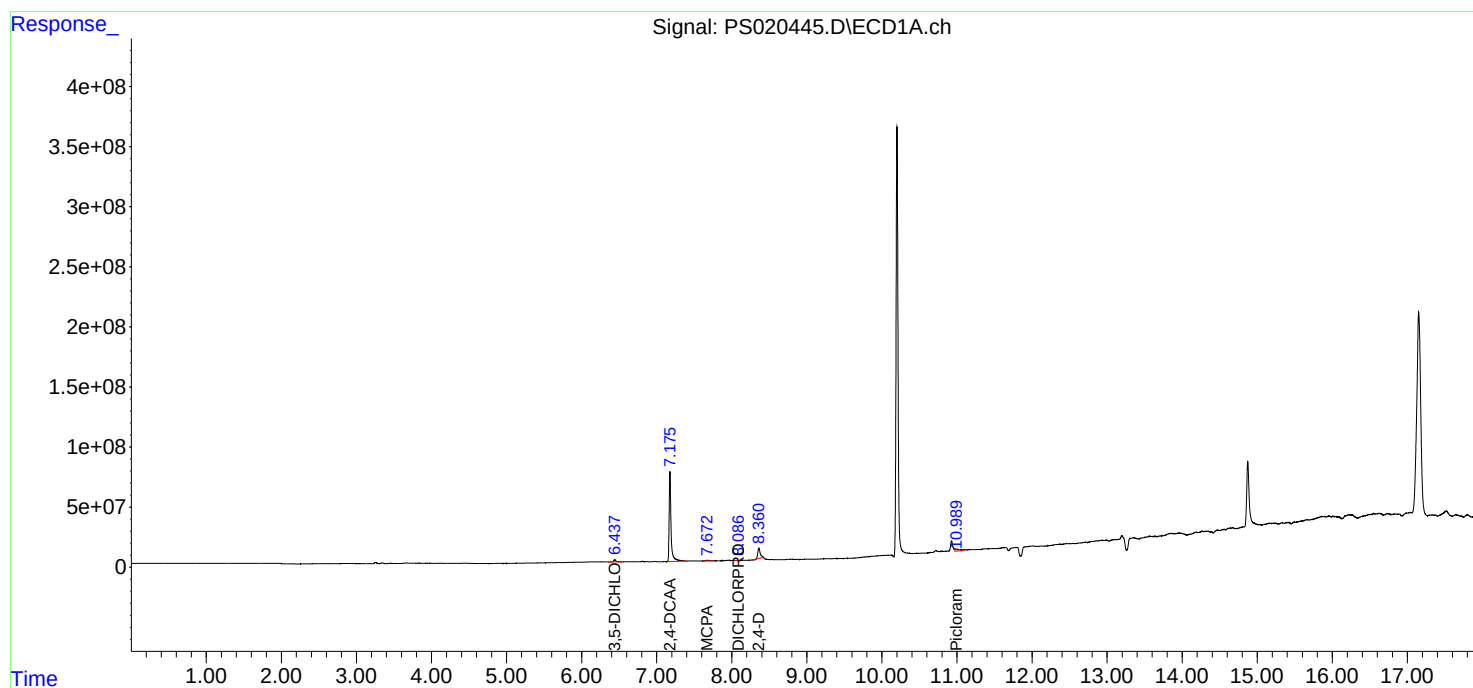


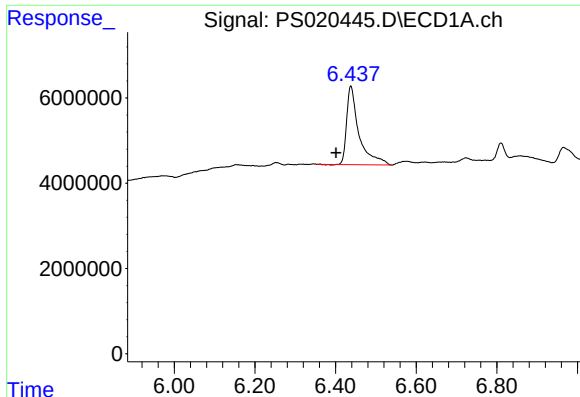

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.438 min
Delta R.T.: 0.037 min
Response: 38995756
Conc: 8.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

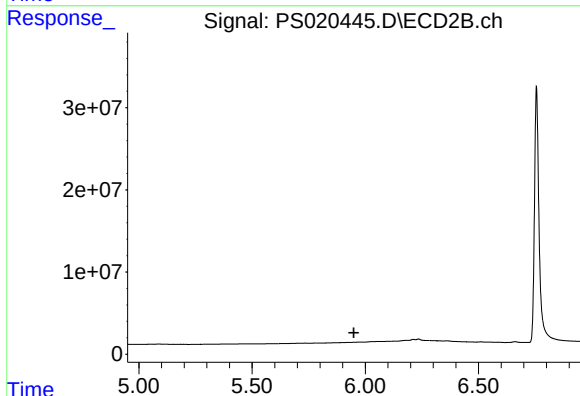


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.950 min
Response: 0
Conc: N.D.

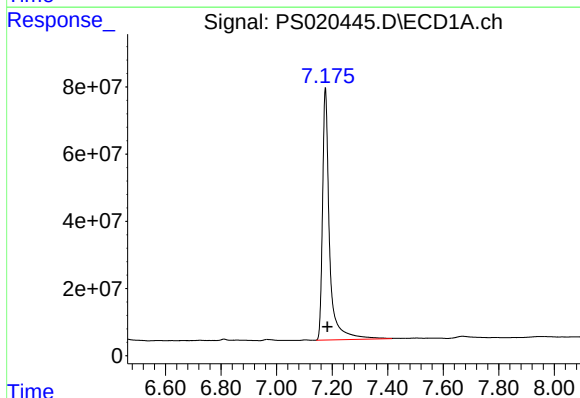


#4 2,4-DCAA

R.T.: 7.176 min
Delta R.T.: -0.007 min
Response: 1315531321
Conc: 373.24 ng/ml

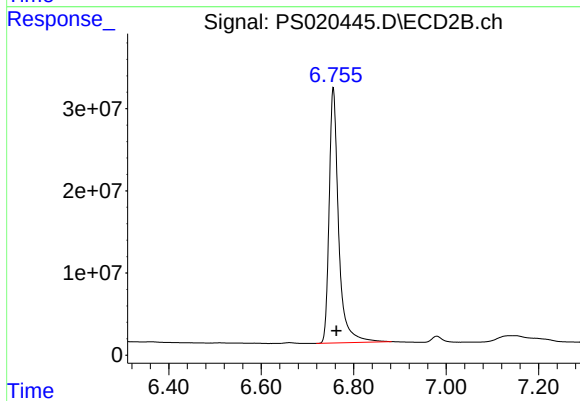

#4 2,4-DCAA


R.T.: 6.756 min
Delta R.T.: -0.007 min
Response: 442268707
Conc: 411.60 ng/ml

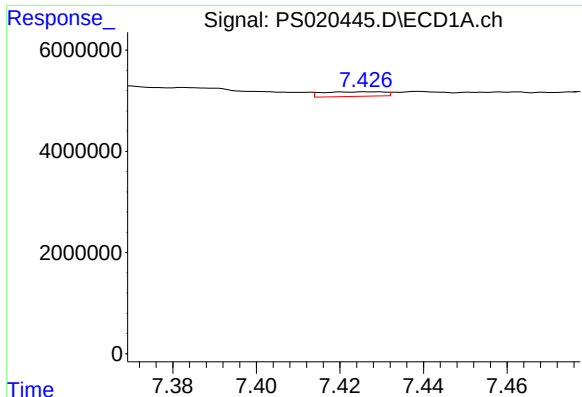

#5 DICAMBA


R.T.: 7.427 min
Delta R.T.: 0.061 min
Response: 943173
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

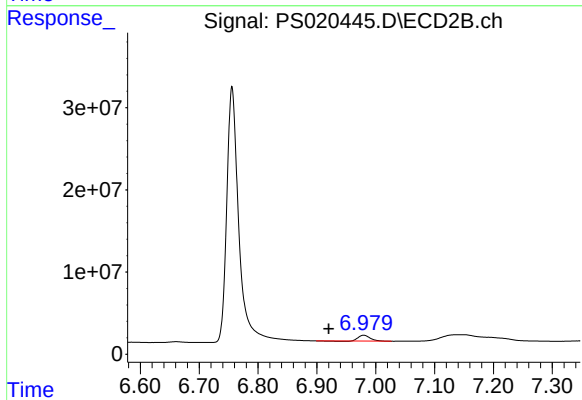


#5 DICAMBA

R.T.: 6.980 min
Delta R.T.: 0.060 min
Response: 9672371
Conc: 2.02 ng/ml

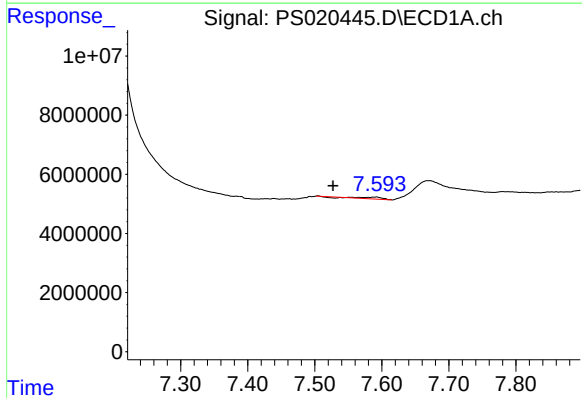


#6 MCP

R.T.: 7.591 min
Delta R.T.: 0.063 min
Response: 900221
Conc: N.D.

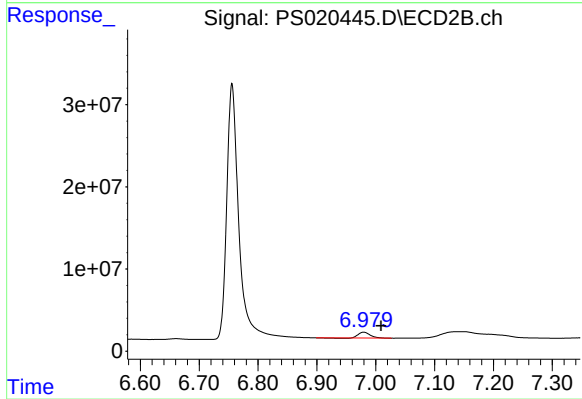

#6 MCP


R.T.: 6.980 min
Delta R.T.: -0.030 min
Response: 9672371
Conc: 2.63 ug/ml

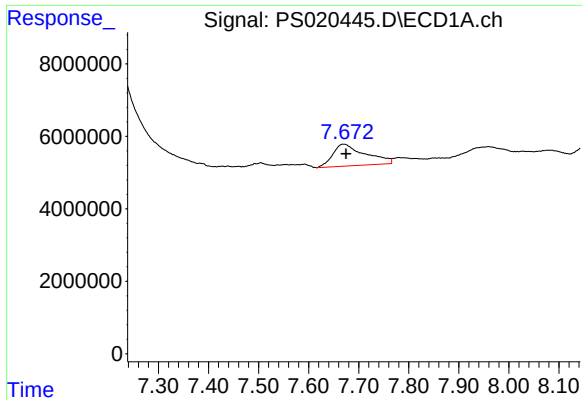

#7 MCPA


R.T.: 7.670 min
Delta R.T.: -0.005 min
Response: 27403742
Conc: 1.78 ug/ml

Instrument :
ECD_S
ClientSampleId :

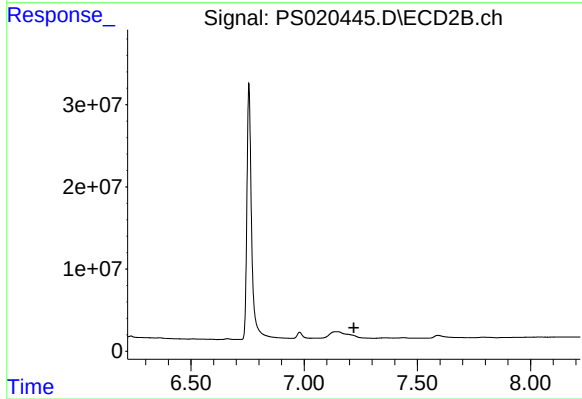


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.219 min
Response: 0
Conc: N.D.

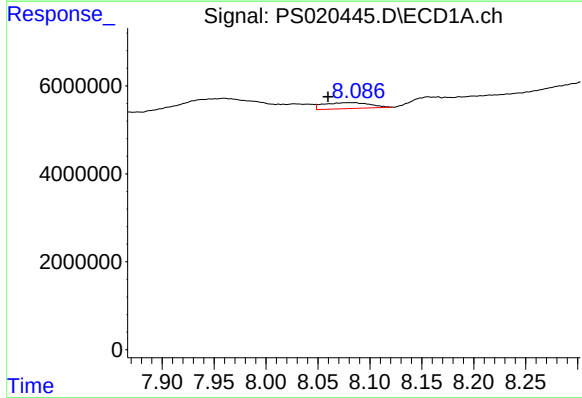


#8 DICHLORPROP

R.T.: 8.081 min
Delta R.T.: 0.021 min
Response: 4184781
Conc: 1.14 ng/ml

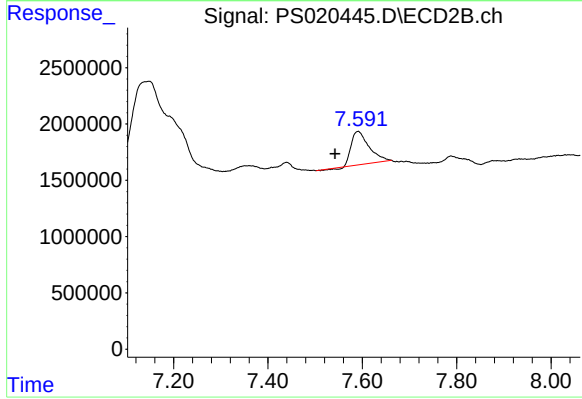

#8 DICHLORPROP


R.T.: 7.591 min
Delta R.T.: 0.049 min
Response: 7669868
Conc: 6.14 ng/ml

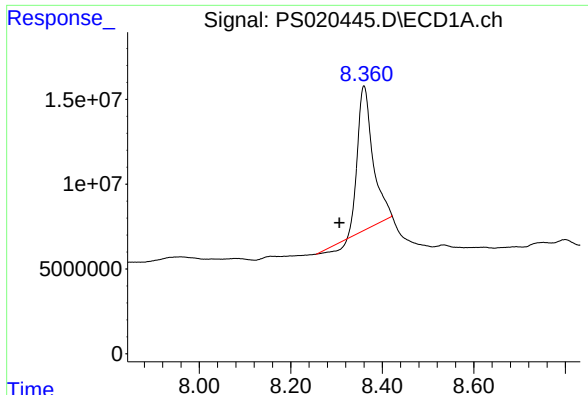

#9 2,4-D


R.T.: 8.360 min
Delta R.T.: 0.054 min
Response: 195404716
Conc: 41.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

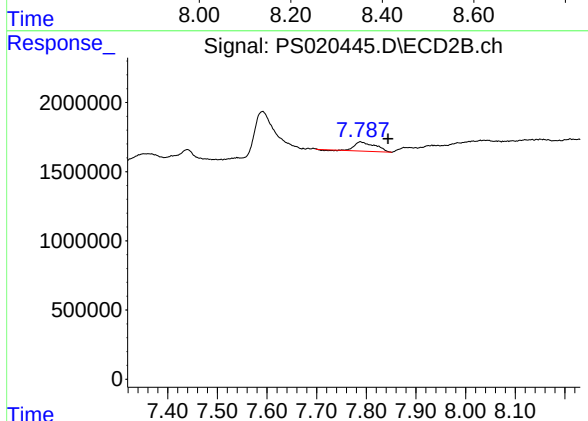


#9 2,4-D

R.T.: 7.789 min
Delta R.T.: -0.055 min
Response: 1933475
Conc: 1.27 ng/ml

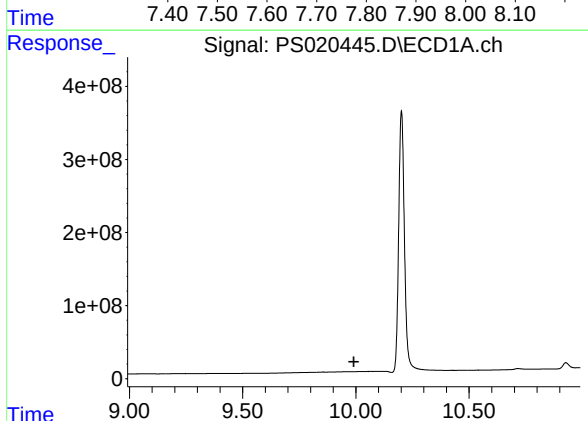


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.991 min
Response: 0
Conc: N.D.

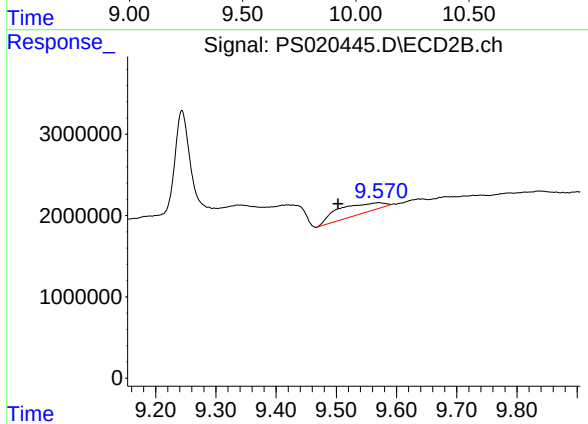

#13 2,4-DB


R.T.: 9.570 min
Delta R.T.: 0.067 min
Response: 6696092
Conc: 7.40 ng/ml

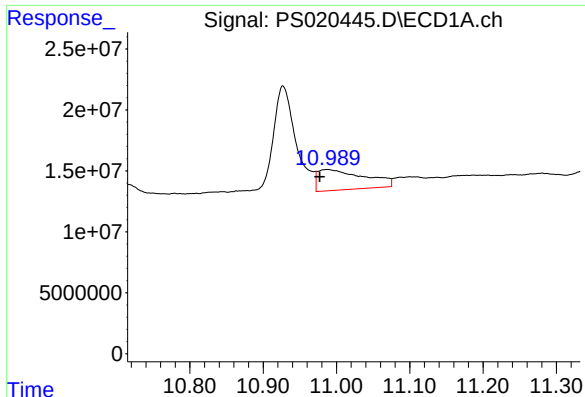

#15 Picloram


R.T.: 10.987 min
Delta R.T.: 0.010 min
Response: 74764122
Conc: 1.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

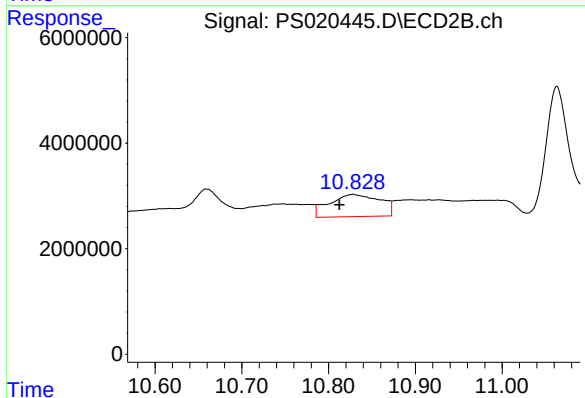


#15 Picloram

R.T.: 10.828 min
Delta R.T.: 0.016 min
Response: 17069362
Conc: 1.66 ng/ml

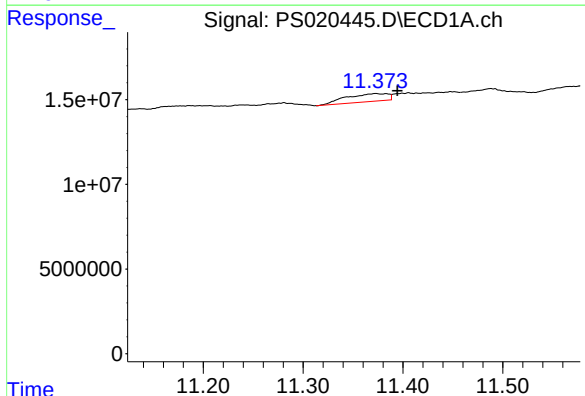

#16 DCPA

R.T.: 11.373 min
Delta R.T.: -0.022 min
Response: 13775885
Conc: N.D.

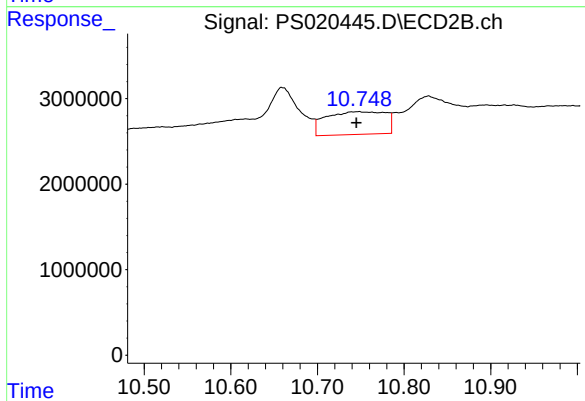

#16 DCPA

R.T.: 10.747 min
Delta R.T.: 0.002 min
Response: 12678244
Conc: 1.42 ng/ml