

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090322\
 Data File : PS020452.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2022 11:40
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 21:54:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 03 01:09:33 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.178	6.757	1336.8E6	441.3E6	379.264	410.719
Target Compounds							
1) T	Dalapon	3.040f	0.000	767896	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.400	0.000	72486	0	<MDL	N.D. #
3) T	4-Nitroph...	7.105f	0.000	721175	0	<MDL	N.D. #
5) T	DICAMBA	0.000	6.982f	0	21562082	N.D.	4.505
6) T	MCP	0.000	6.982	0	21562082	N.D.	5.866
7) T	MCPA	7.704	7.150f	18991297	43572541	1.232	8.034 #
8) T	DICHLORPROP	8.079	0.000	1171431	0	<MDL	N.D. #
9) T	2,4-D	8.364f	0.000	305.6E6	0	65.144	N.D. #
11) T	2,4,5-TP ...	9.160	0.000	1552643	0	<MDL	N.D. #
12) T	2,4,5-T	9.450	0.000	1241022	0	<MDL	N.D. #
13) T	2,4-DB	9.954	9.568f	4213291	164754	<MDL	<MDL #
15) T	Picloram	11.013	10.846	107.6E6	15825617	2.600	1.541 #
16) T	DCPA	11.401	10.744	6205280	4653091	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090322\
Data File : PS020452.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2022 11:40
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 21:54:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
Quant Title : 8080.M
QLast Update : Sat Sep 03 01:09:33 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

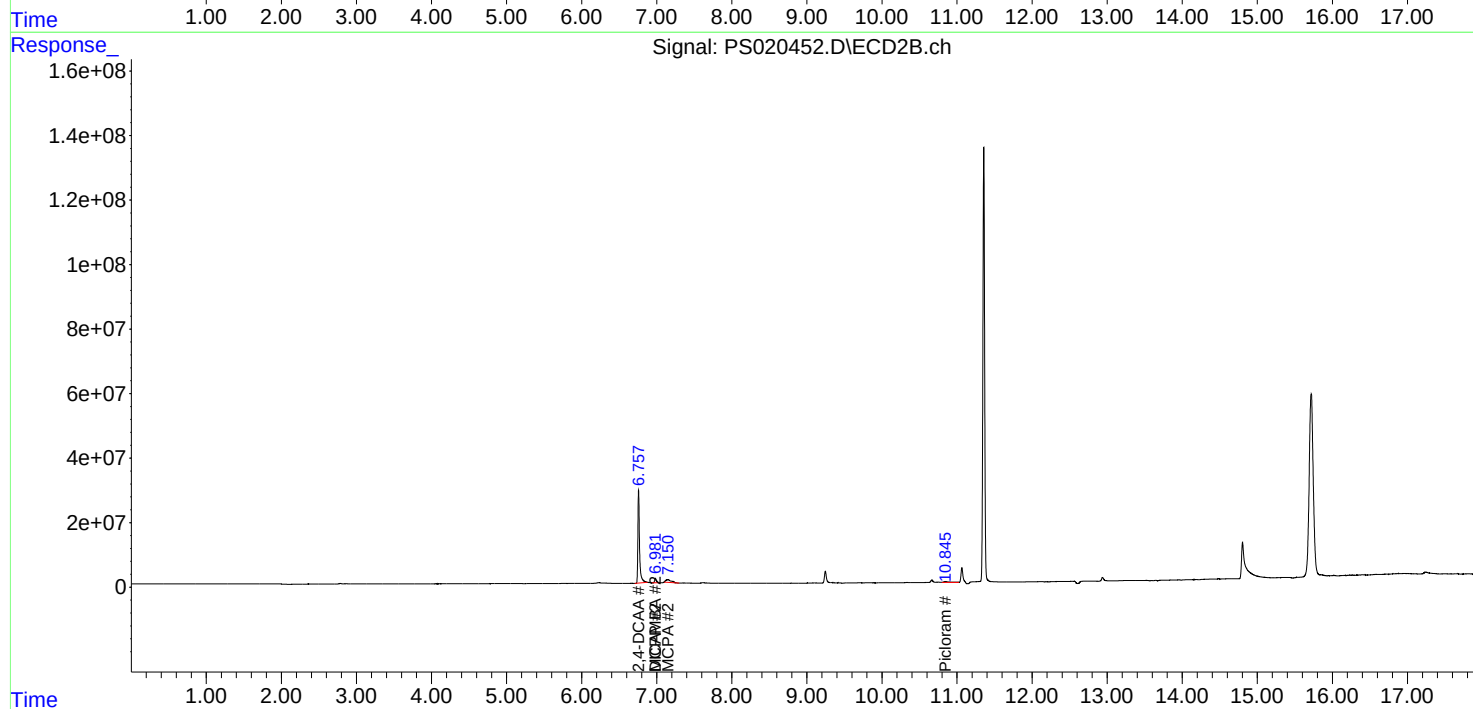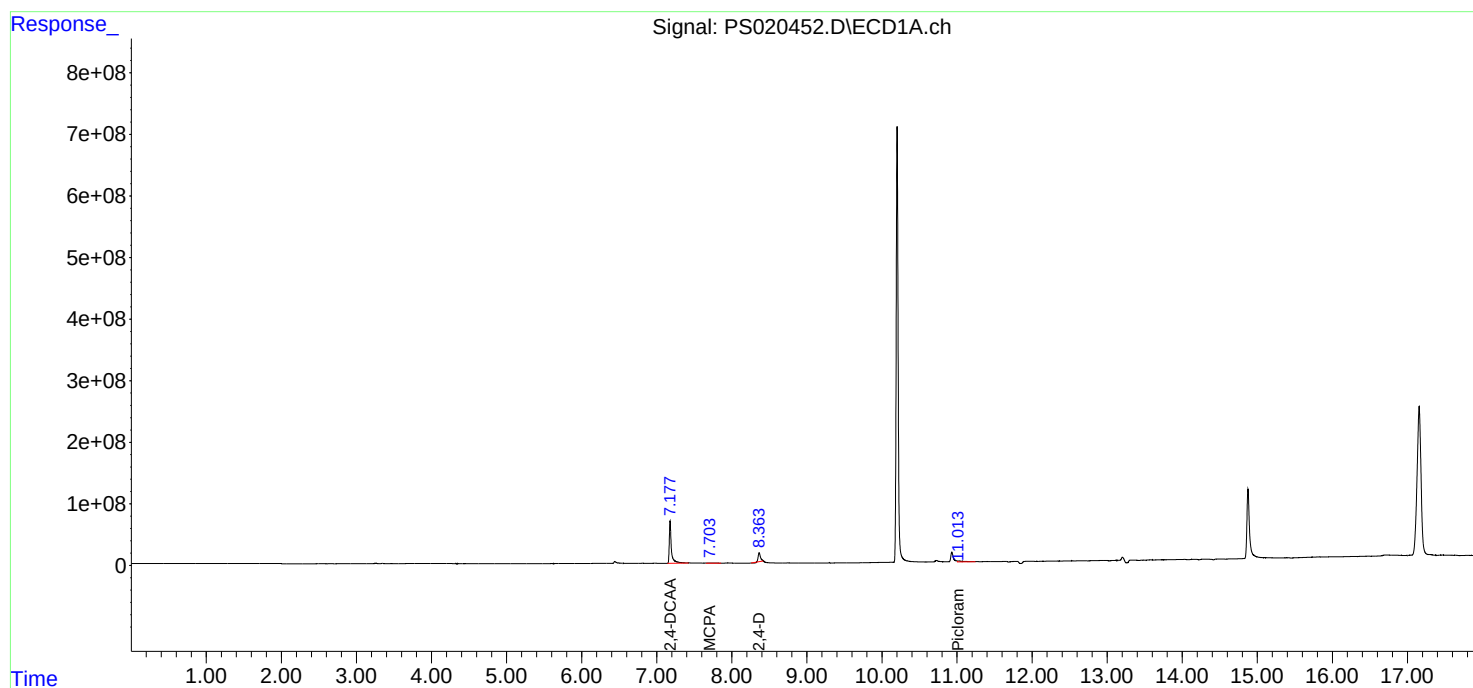


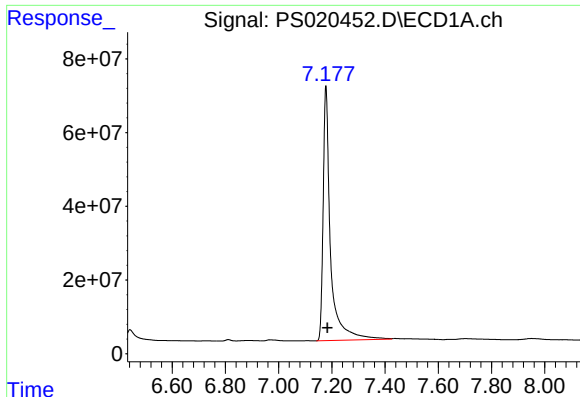

#4 2,4-DCAA


R.T.: 7.178 min
Delta R.T.: -0.005 min
Response: 1336779622
Conc: 379.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

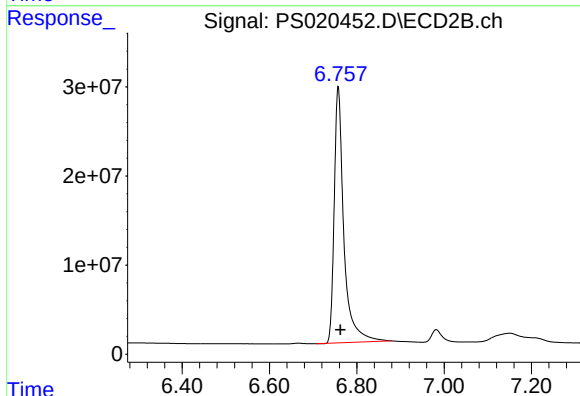


#4 2,4-DCAA

R.T.: 6.757 min
Delta R.T.: -0.005 min
Response: 441326675
Conc: 410.72 ng/ml

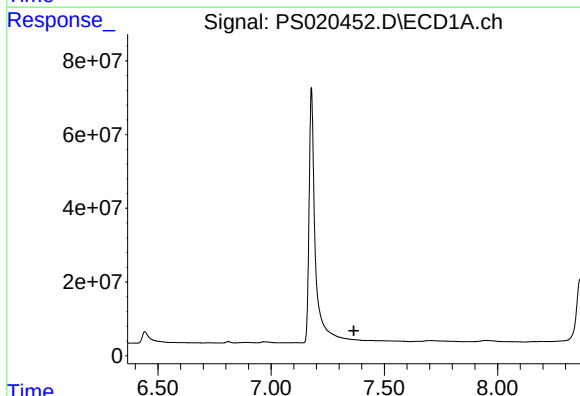


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.366 min
Response: 0
Conc: N.D.

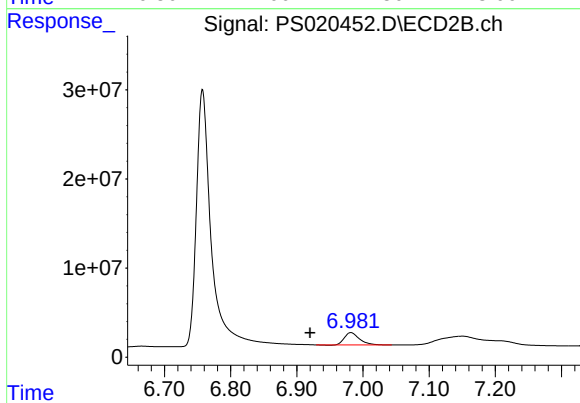

#5 DICAMBA


R.T.: 6.982 min
Delta R.T.: 0.062 min
Response: 21562082
Conc: 4.51 ng/ml

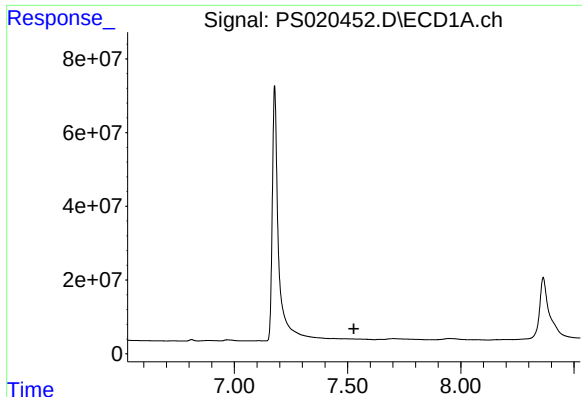

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.528 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

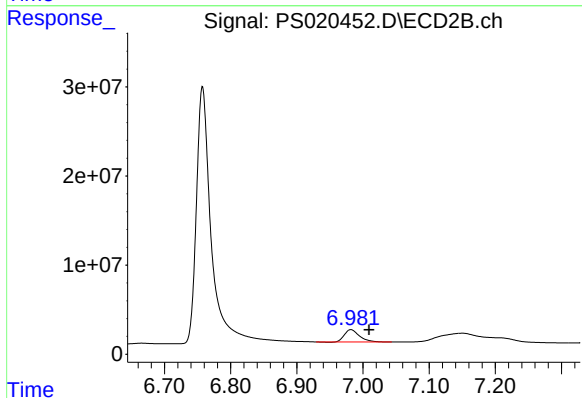


#6 MCPP

R.T.: 6.982 min
Delta R.T.: -0.027 min
Response: 21562082
Conc: 5.87 ug/ml

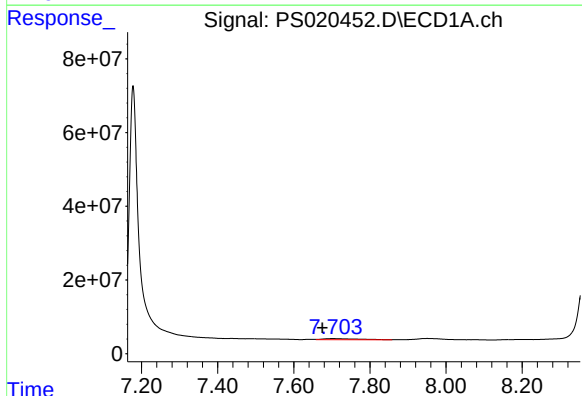


#7 MCPA

R.T.: 7.704 min
Delta R.T.: 0.029 min
Response: 18991297
Conc: 1.23 ug/ml

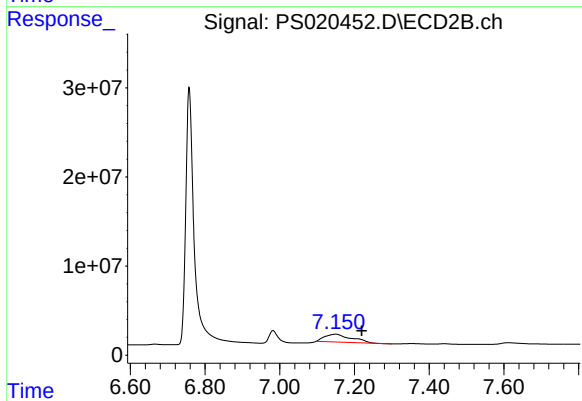

#7 MCPA


R.T.: 7.150 min
Delta R.T.: -0.069 min
Response: 43572541
Conc: 8.03 ug/ml

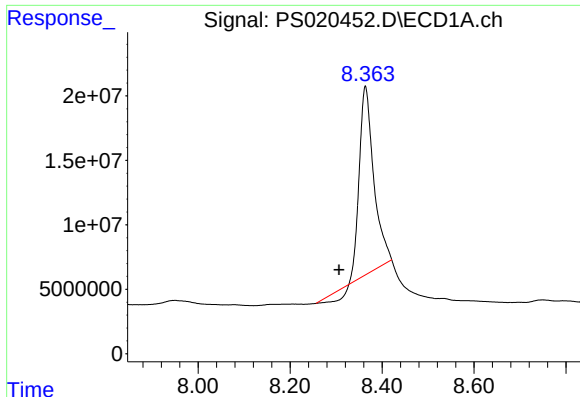

#9 2,4-D


R.T.: 8.364 min
Delta R.T.: 0.058 min
Response: 305617694
Conc: 65.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

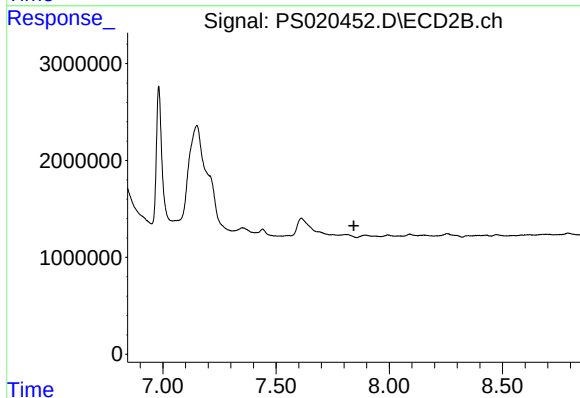


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.844 min
Response: 0
Conc: N.D.

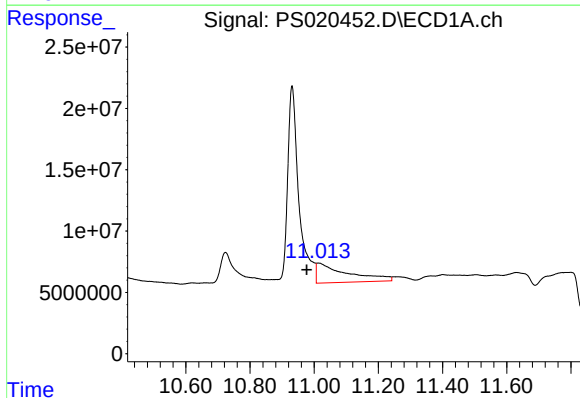

#15 Picloram

R.T.: 11.013 min
Delta R.T.: 0.036 min
Response: 107647253
Conc: 2.60 ng/ml

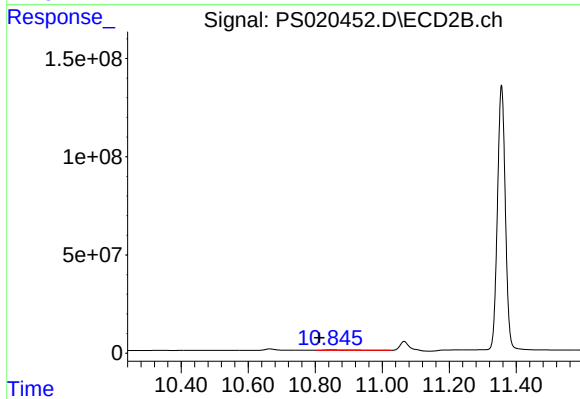

#15 Picloram

R.T.: 10.846 min
Delta R.T.: 0.034 min
Response: 15825617
Conc: 1.54 ng/ml