

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090324\
 Data File : PS027602.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2024 21:55
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 08:33:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090324.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 03 15:23:07 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.147	7.730	1221.4E6	974.0E6	481.657	506.661
Target Compounds							
1) T	Dalapon	0.000	2.686	0	3679854	N.D.	1.061
2) T	3,5-DICHL...	0.000	6.644f	0	15781	N.D.	<MDL
3) T	4-Nitroph...	6.944	7.230f	6674747	2384943	4.478	1.851 #
5) T	DICAMBA	0.000	7.923	0	6921951	N.D.	<MDL
6) T	MCPD	0.000	8.000f	0	81967	N.D.	<MDL
7) T	MCPA	0.000	8.252	0	25470895	N.D.	2.968
8) T	DICHLORPROP	8.006	8.633	1587092	461073	<MDL	<MDL #
9) T	2,4-D	0.000	8.943	0	120079	N.D.	<MDL
10) T	Pentachlo...	8.530	9.489	2834728	3846583	<MDL	<MDL #
11) T	2,4,5-TP ...	9.096	9.871	1580733	37798426	<MDL	2.864 #
12) T	2,4,5-T	9.398	10.291	2988209	26993416	<MDL	2.074 #
13) T	2,4-DB	9.945	0.000	2491054	0	1.171	N.D. #
14) T	DINOSEB	11.153	0.000	4598171	0	<MDL	N.D. #
15) T	Picloram	10.960	12.325	31674059	3966385	1.628	<MDL #
16) T	DCPA	11.408f	12.258	3354910	475035	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090324\
Data File : PS027602.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2024 21:55
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 08:33:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090324.M
Quant Title : 8080.M
QLast Update : Tue Sep 03 15:23:07 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

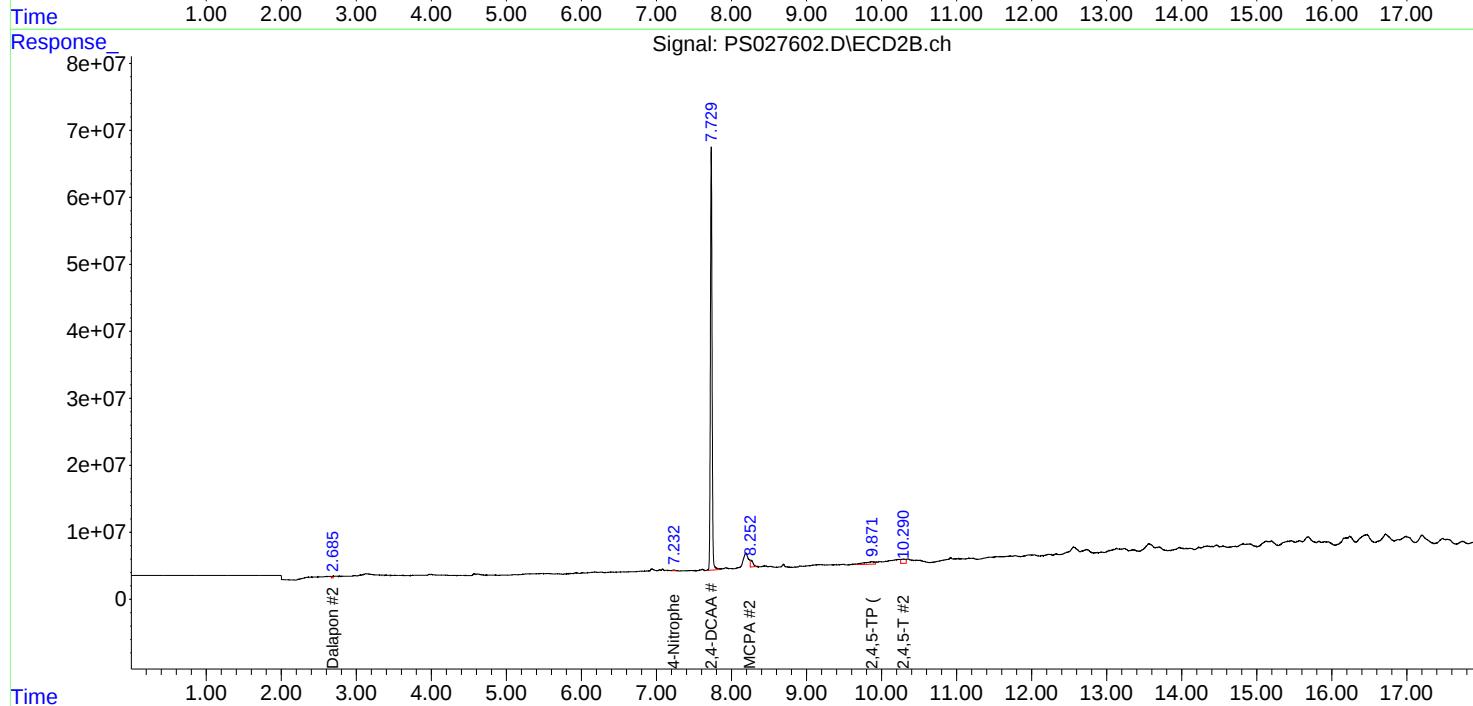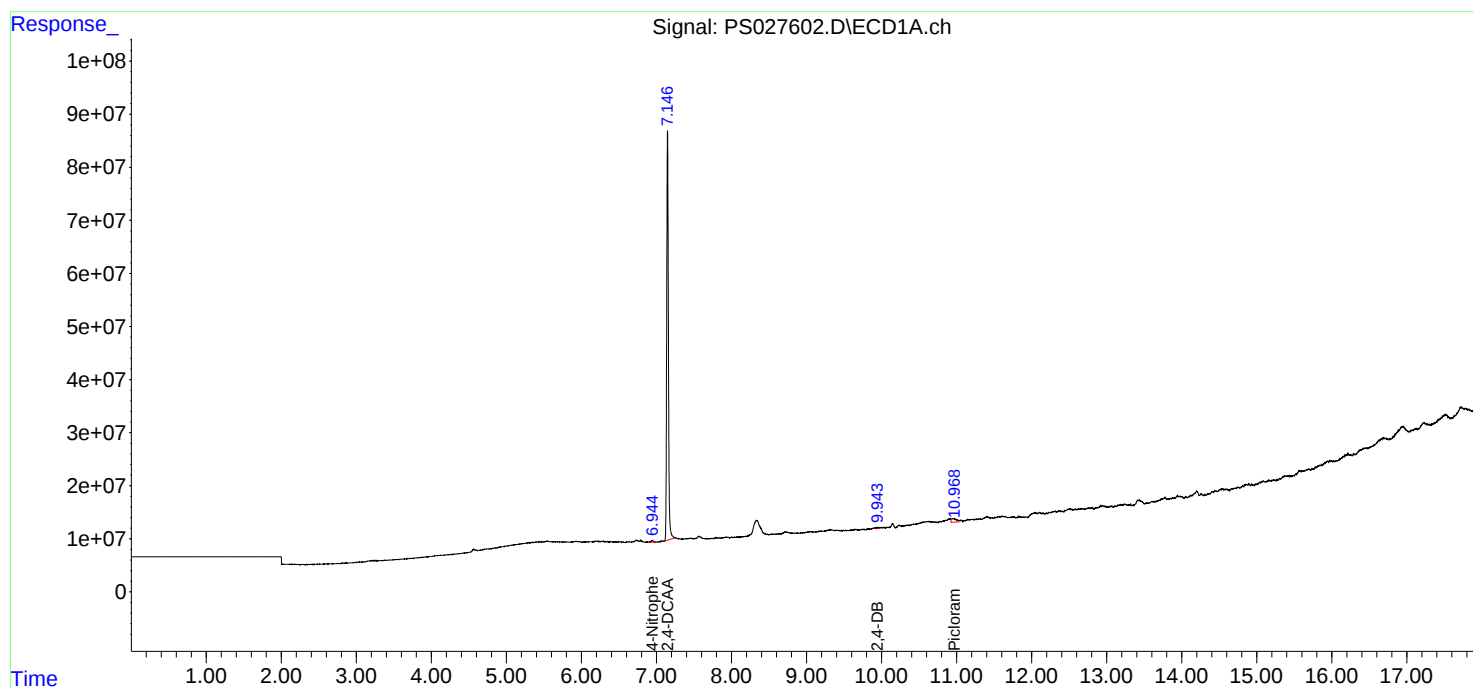


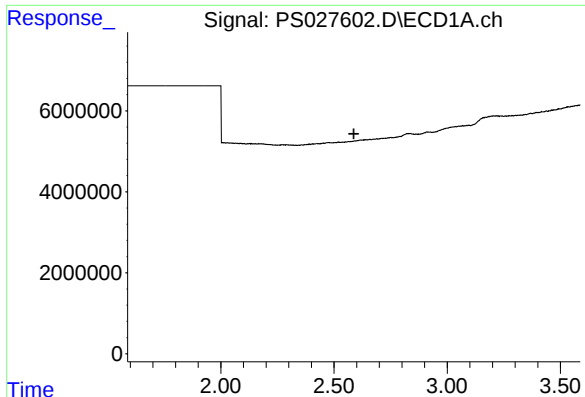

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.588 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

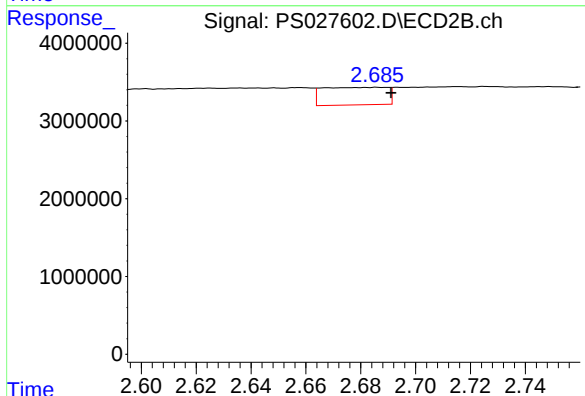


#1 Dalapon

R.T.: 2.686 min
Delta R.T.: -0.005 min
Response: 3679854
Conc: 1.06 ng/ml

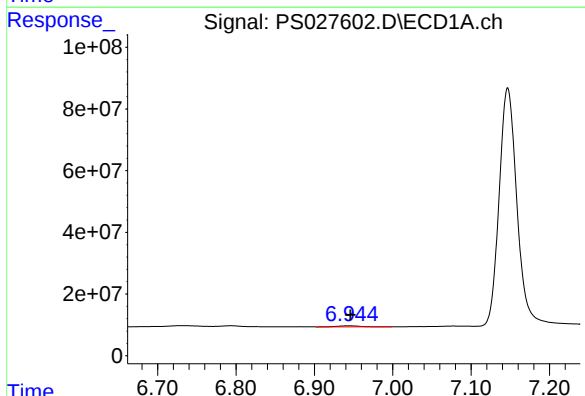


#3 4-Nitrophenol

R.T.: 6.944 min
Delta R.T.: -0.002 min
Response: 6674747
Conc: 4.48 ng/ml

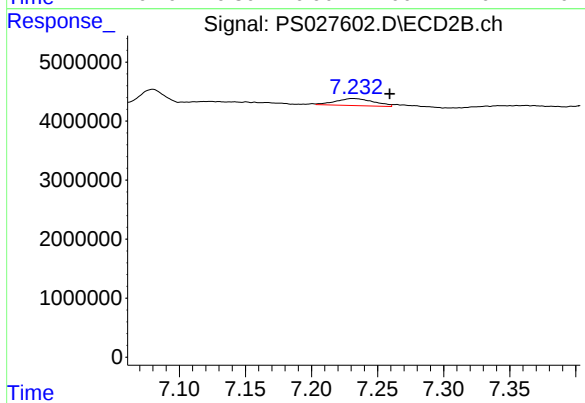

#3 4-Nitrophenol


R.T.: 7.230 min
Delta R.T.: -0.029 min
Response: 2384943
Conc: 1.85 ng/ml

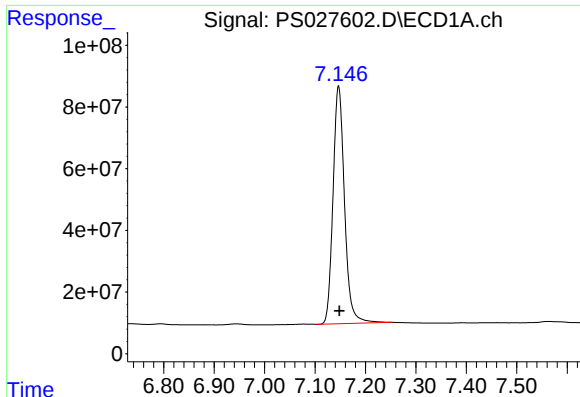

#4 2,4-DCAA


R.T.: 7.147 min
Delta R.T.: -0.002 min
Response: 1221393719
Conc: 481.66 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

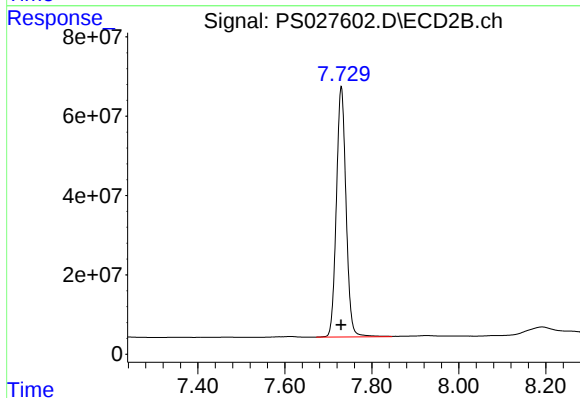


#4 2,4-DCAA

R.T.: 7.730 min
Delta R.T.: 0.000 min
Response: 973969142
Conc: 506.66 ng/ml

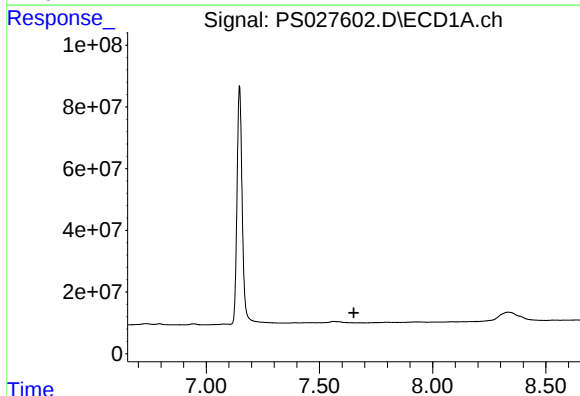


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.652 min
Response: 0
Conc: N.D.

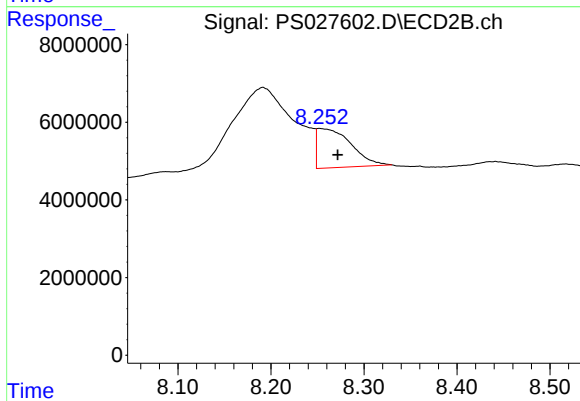

#7 MCPA


R.T.: 8.252 min
Delta R.T.: -0.020 min
Response: 25470895
Conc: 2.97 ug/ml

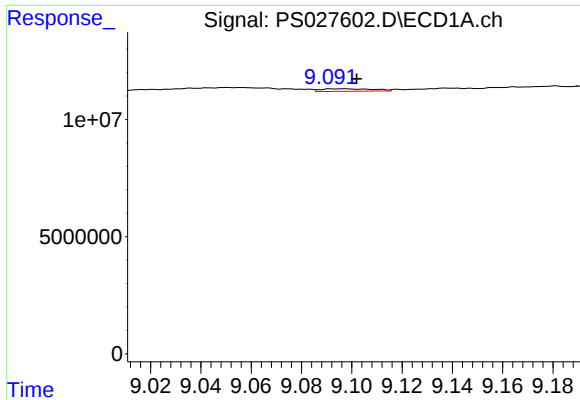

#11 2,4,5-TP (SILVEX)


R.T.: 9.096 min
Delta R.T.: -0.006 min
Response: 1580733
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

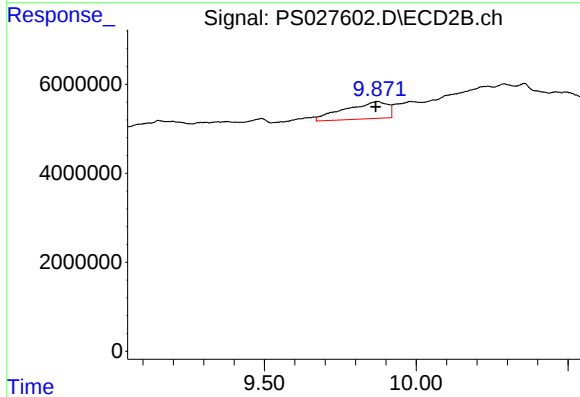


#11 2,4,5-TP (SILVEX)

R.T.: 9.871 min
Delta R.T.: 0.005 min
Response: 37798426
Conc: 2.86 ng/ml

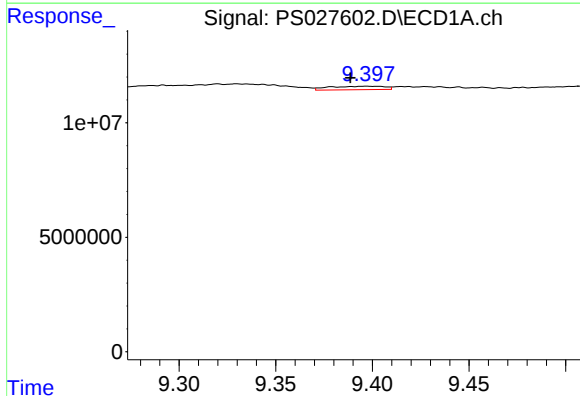


#12 2,4,5-T

R.T.: 9.398 min
Delta R.T.: 0.010 min
Response: 2988209
Conc: N.D.

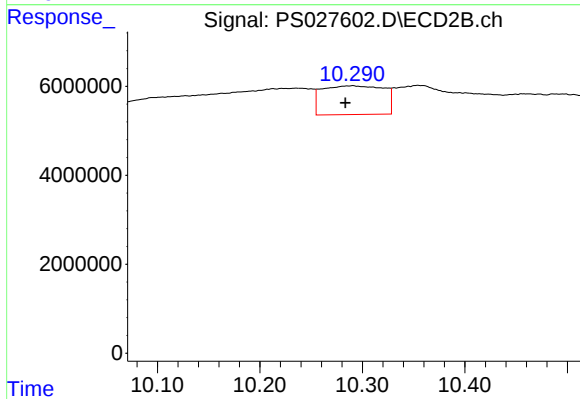

#12 2,4,5-T


R.T.: 10.291 min
Delta R.T.: 0.007 min
Response: 26993416
Conc: 2.07 ng/ml

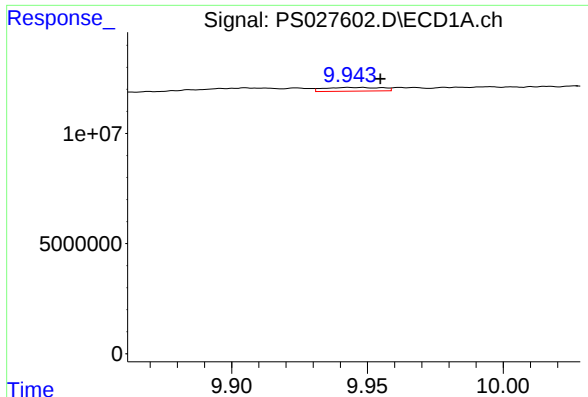

#13 2,4-DB


R.T.: 9.945 min
Delta R.T.: -0.010 min
Response: 2491054
Conc: 1.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

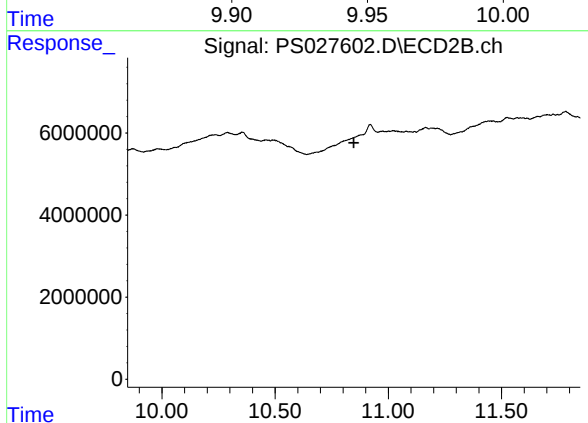


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.848 min
Response: 0
Conc: N.D.

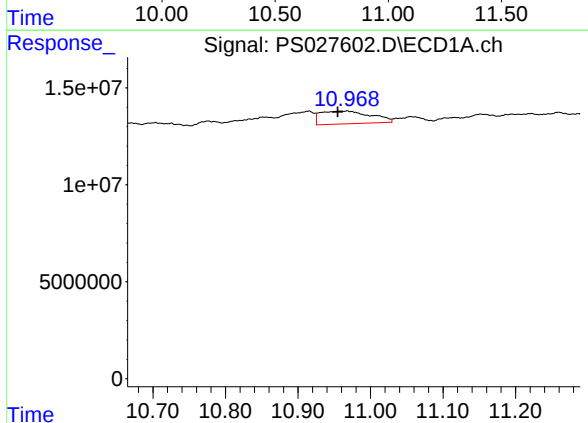

#15 Picloram

R.T.: 10.960 min
Delta R.T.: 0.005 min
Response: 31674059
Conc: 1.63 ng/ml

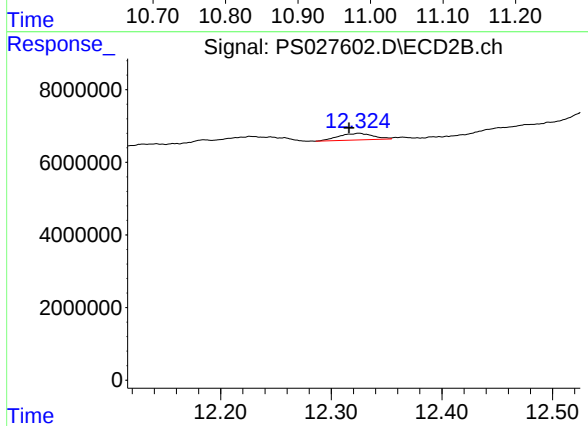

#15 Picloram

R.T.: 12.325 min
Delta R.T.: 0.009 min
Response: 3966385
Conc: N.D.