

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090325\
 Data File : PS031603.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2025 15:29
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 02:24:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:17:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.285	7.743	1788.6E6	486.1E6	563.522	575.075
Target Compounds							
1) T	Dalapon	0.000	2.657f	0	67696790	N.D.	25.440
2) T	3,5-DICHL...	6.455	0.000	1879406	0	<MDL	N.D. #
5) T	DICAMBA	7.506f	0.000	241742	0	<MDL	N.D. #
7) T	MCPA	7.823	0.000	364193	0	<MDL	N.D. #
8) T	DICHLORPROP	8.182	0.000	2278057	0	<MDL	N.D. #
10) T	Pentachlo...	8.710	9.511	8048760	7901633	<MDL	<MDL #
11) T	2,4,5-TP ...	9.290	9.908	5118737	3499237	<MDL	<MDL #
12) T	2,4,5-T	9.612	10.324	15058018	1949046	1.028	<MDL #
13) T	2,4-DB	10.170	0.000	793779	0	<MDL	N.D. #
14) T	DINOSEB	11.355	0.000	3569558	0	<MDL	N.D. #
15) T	Picloram	11.208	0.000	556328	0	<MDL	N.D. #
16) T	DCPA	11.675	0.000	288451	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090325\
Data File : PS031603.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2025 15:29
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 02:24:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:17:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

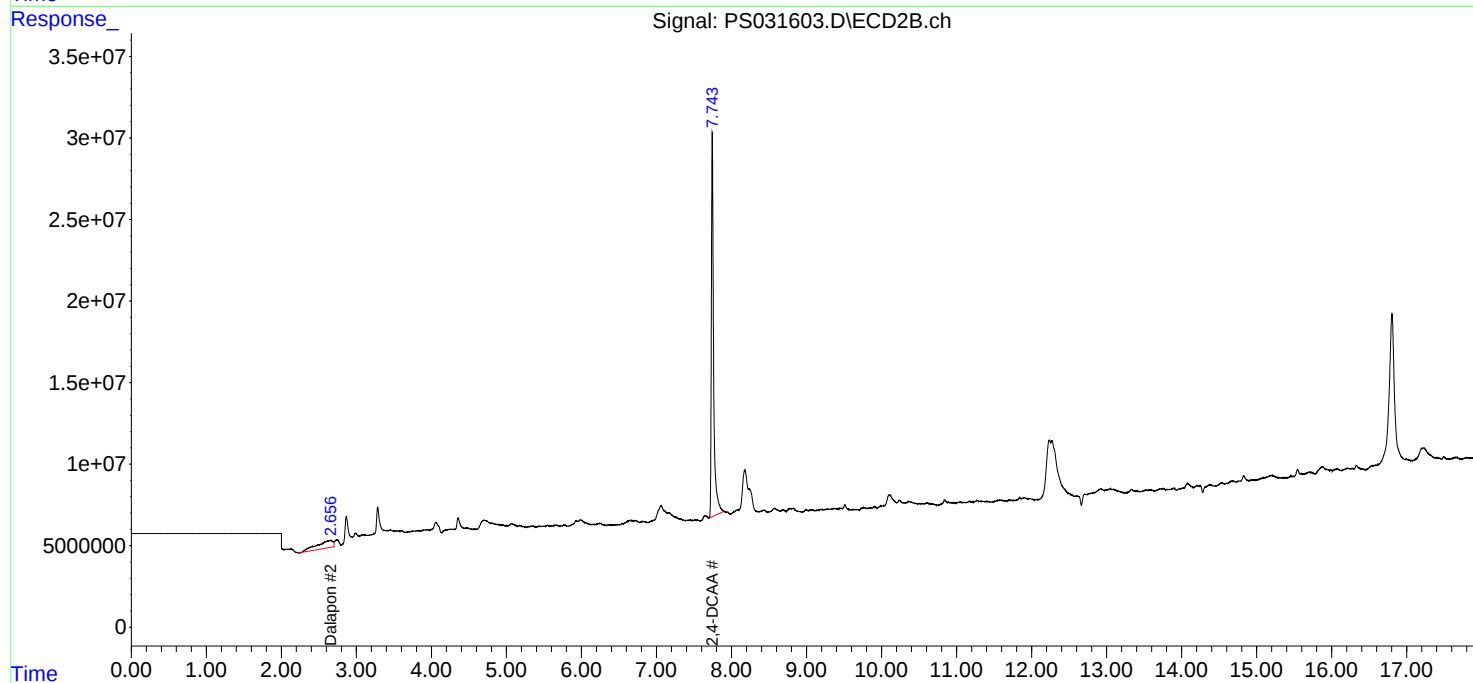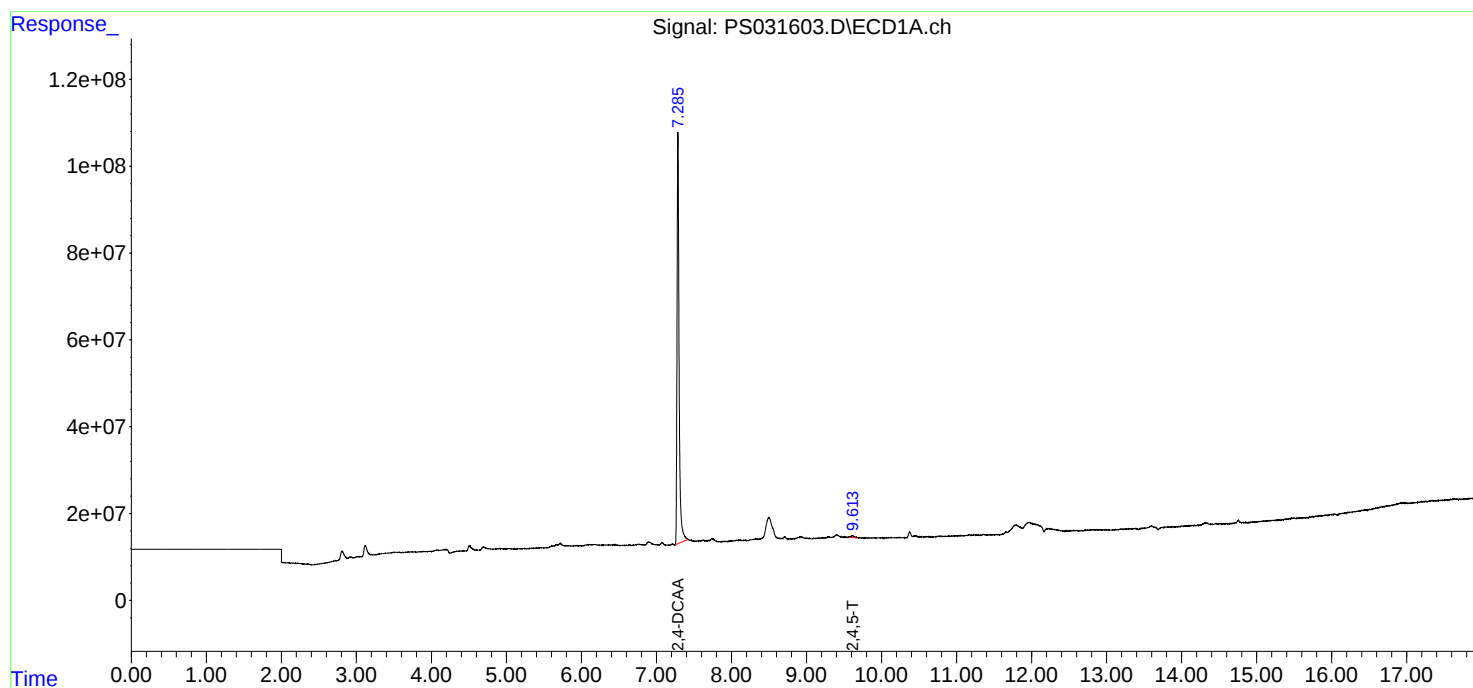


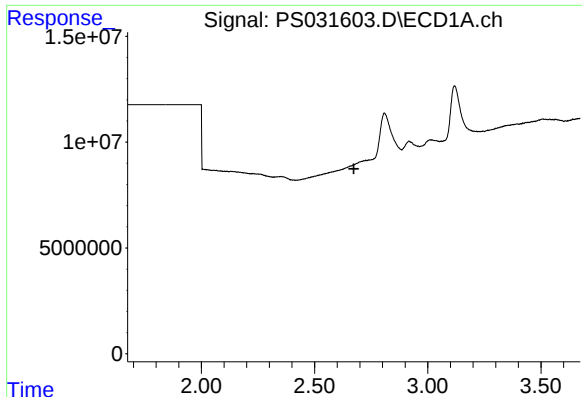

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

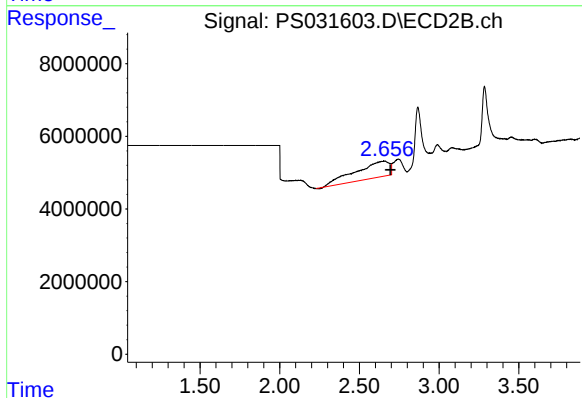


#1 Dalapon

R.T.: 2.657 min
Delta R.T.: -0.038 min
Response: 67696790
Conc: 25.44 ng/ml

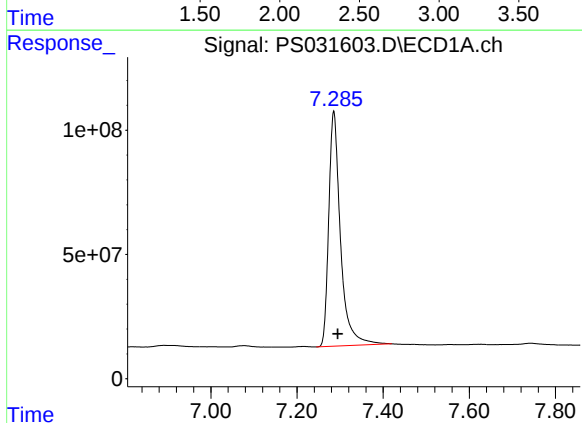


#4 2,4-DCAA

R.T.: 7.285 min
Delta R.T.: -0.009 min
Response: 1788613401
Conc: 563.52 ng/ml

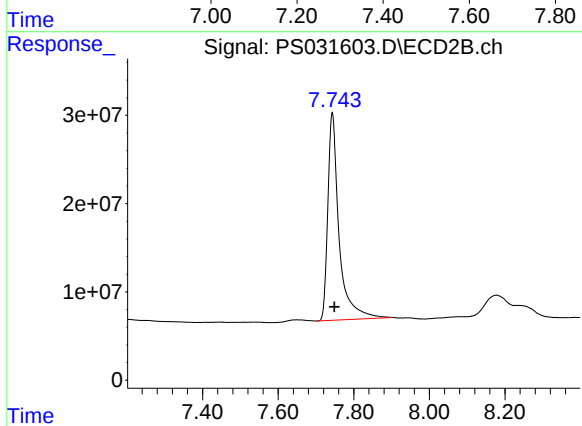

#4 2,4-DCAA


R.T.: 7.743 min
Delta R.T.: -0.006 min
Response: 486133770
Conc: 575.08 ng/ml

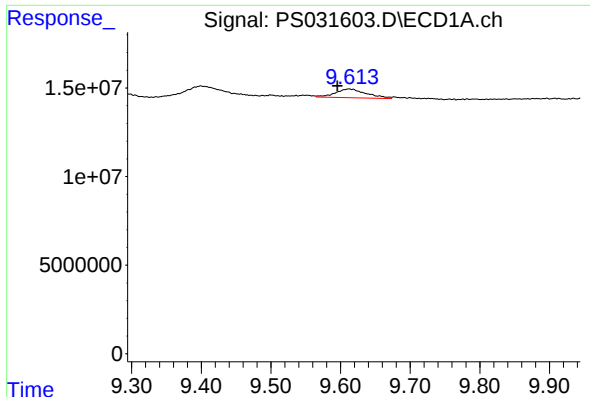

#12 2,4,5-T

R.T.: 9.612 min
Delta R.T.: 0.017 min
Response: 15058018
Conc: 1.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

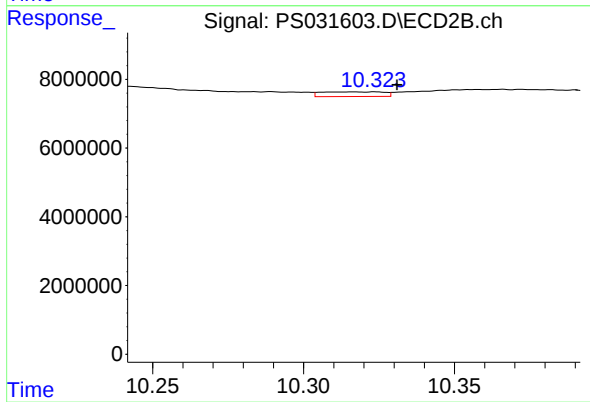

#12 2,4,5-T

R.T.: 10.324 min
Delta R.T.: -0.007 min
Response: 1949046
Conc: N.D.