

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090325\
 Data File : PS031613.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2025 19:31
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 02:26:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:17:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.286	7.745	1746.7E6	476.0E6	550.330	563.043
Target Compounds							
1) T	Dalapon	0.000	2.656f	0	10790498	N.D.	4.055
2) T	3,5-DICHL...	6.452	0.000	3317333	0	<MDL	N.D. #
6) T	MCP	7.669	8.083f	-731300	934055	N.D.	<MDL
7) T	MCPA	0.000	8.247f	0	45828353	N.D.	16.335
8) T	DICHLORPROP	8.183	8.709f	2935213	1607452	<MDL	1.204 #
9) T	2,4-D	0.000	9.004	0	1385436	N.D.	<MDL
10) T	Pentachlo...	8.710	9.514	9041829	6470421	<MDL	<MDL #
11) T	2,4,5-TP ...	9.294	9.914	5439855	2467253	<MDL	<MDL #
12) T	2,4,5-T	9.626f	0.000	7266522	0	<MDL	N.D. #
13) T	2,4-DB	10.181	0.000	2543723	0	1.324	N.D. #
14) T	DINOSEB	11.357	0.000	4284932	0	<MDL	N.D. #
15) T	Picloram	11.199	0.000	641805	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090325\
Data File : PS031613.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2025 19:31
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 02:26:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:17:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

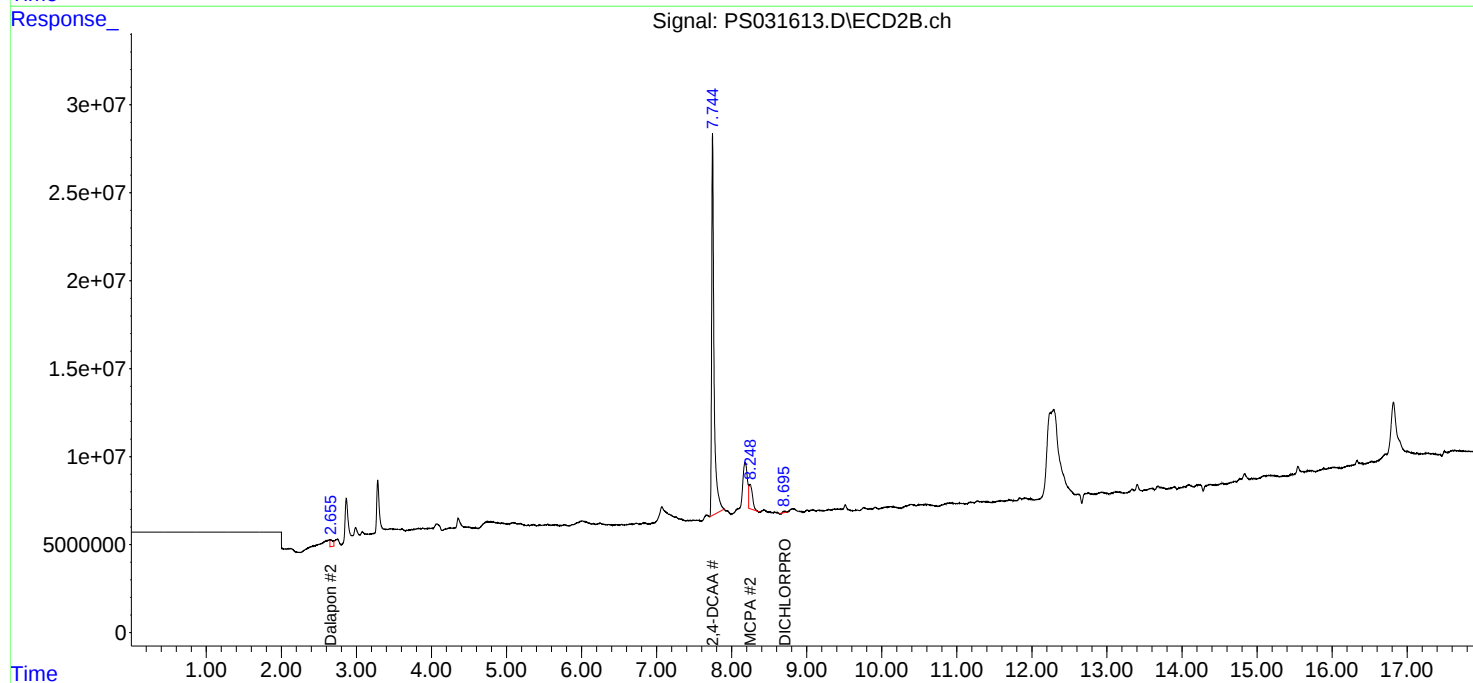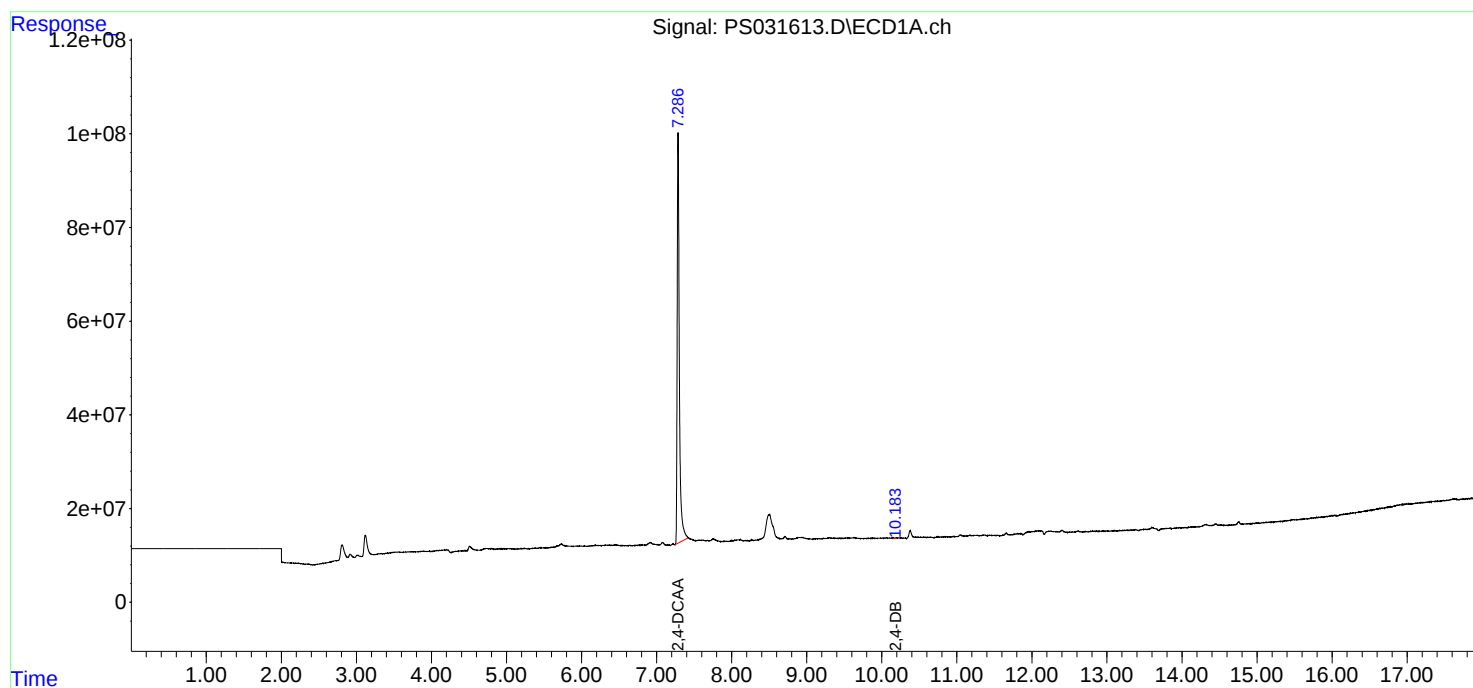


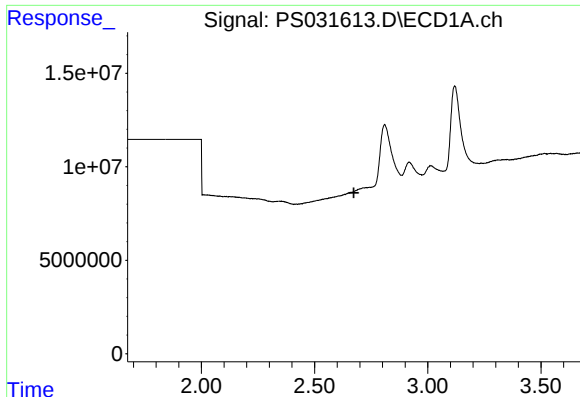

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

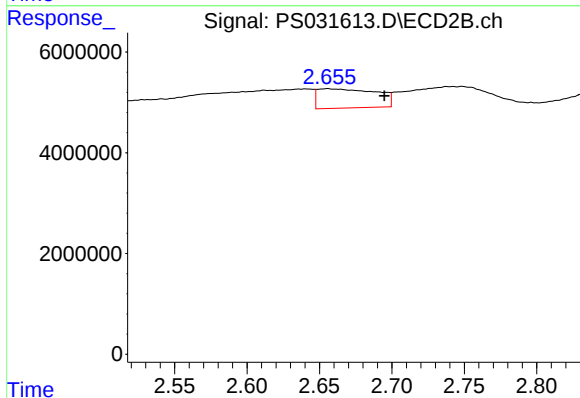


#1 Dalapon

R.T.: 2.656 min
Delta R.T.: -0.039 min
Response: 10790498
Conc: 4.06 ng/ml

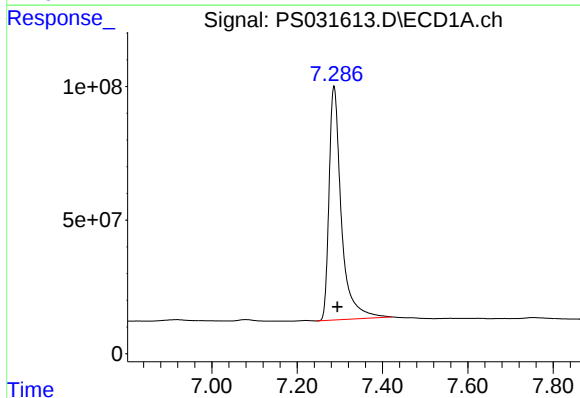


#4 2,4-DCAA

R.T.: 7.286 min
Delta R.T.: -0.009 min
Response: 1746741102
Conc: 550.33 ng/ml

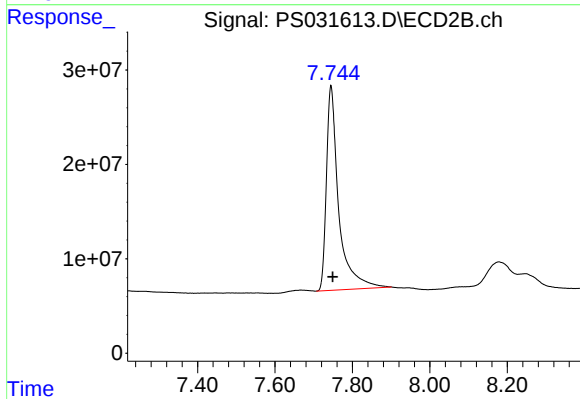

#4 2,4-DCAA


R.T.: 7.745 min
Delta R.T.: -0.004 min
Response: 475962927
Conc: 563.04 ng/ml

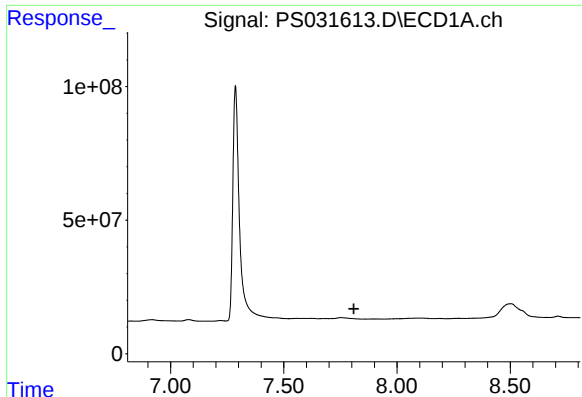

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.809 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

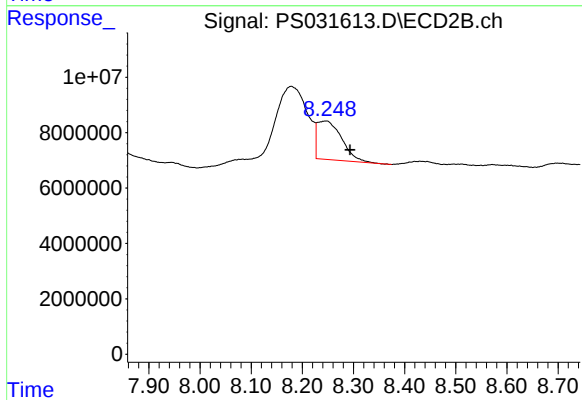


#7 MCPA

R.T.: 8.247 min
Delta R.T.: -0.046 min
Response: 45828353
Conc: 16.34 ug/ml

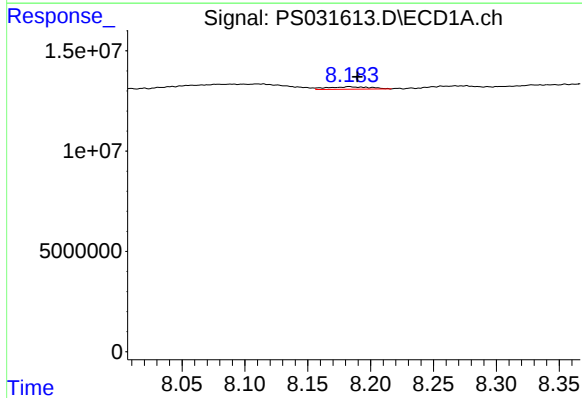


#8 DICHLORPROP

R.T.: 8.183 min
Delta R.T.: -0.007 min
Response: 2935213
Conc: N.D.

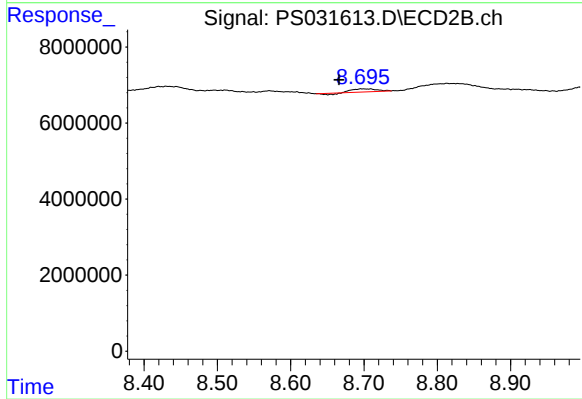

#8 DICHLORPROP


R.T.: 8.709 min
Delta R.T.: 0.043 min
Response: 1607452
Conc: 1.20 ng/ml

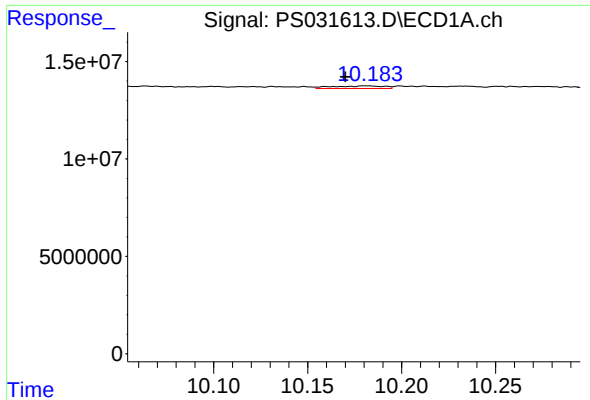

#13 2,4-DB

R.T.: 10.181 min
Delta R.T.: 0.011 min
Response: 2543723
Conc: 1.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

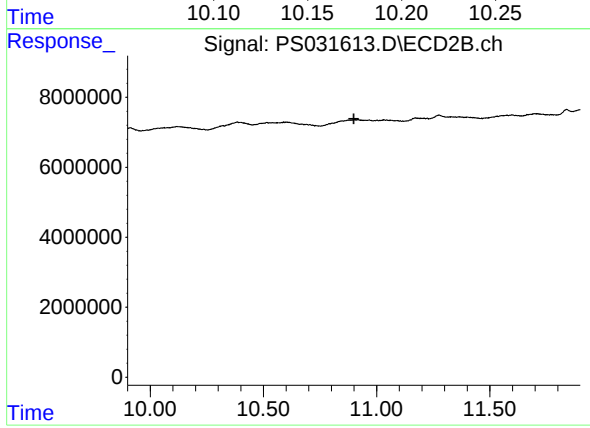

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.899 min
Response: 0
Conc: N.D.