

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090325\
 Data File : PS031619.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2025 22:21
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 02:27:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:17:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.287	7.746	1711.5E6	468.8E6	539.213	554.620
Target Compounds							
1) T	Dalapon	0.000	2.657f	0	62355020	N.D.	23.433
2) T	3,5-DICHL...	6.462	0.000	1626391	0	<MDL	N.D. #
6) T	MCP	7.683	0.000	822859	0	<MDL	N.D. #
7) T	MCPA	0.000	8.245f	0	39644986	N.D.	14.131
8) T	DICHLORPROP	8.189	8.703f	2149267	2327935	<MDL	1.744 #
10) T	Pentachlo...	8.711	9.514	9485672	5924915	<MDL	<MDL #
11) T	2,4,5-TP ...	9.300	9.913	7666202	2251362	<MDL	<MDL #
12) T	2,4,5-T	9.571	10.314	2137044	1770607	<MDL	<MDL #
13) T	2,4-DB	10.185	0.000	1665540	0	<MDL	N.D. #
14) T	DINOSEB	11.361	0.000	5211728	0	<MDL	N.D. #
15) T	Picloram	11.195	0.000	1717168	0	<MDL	N.D. #
16) T	DCPA	11.657	0.000	7415120	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090325\
Data File : PS031619.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2025 22:21
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 02:27:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:17:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

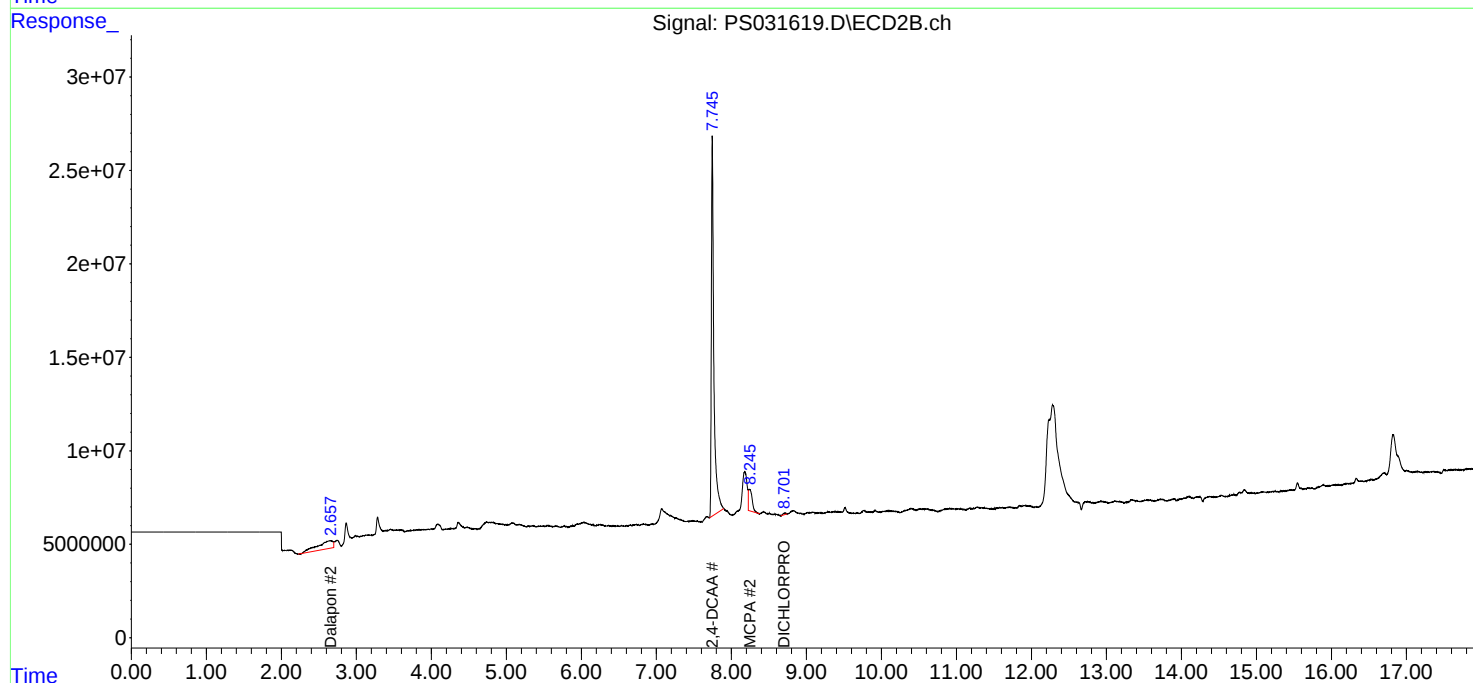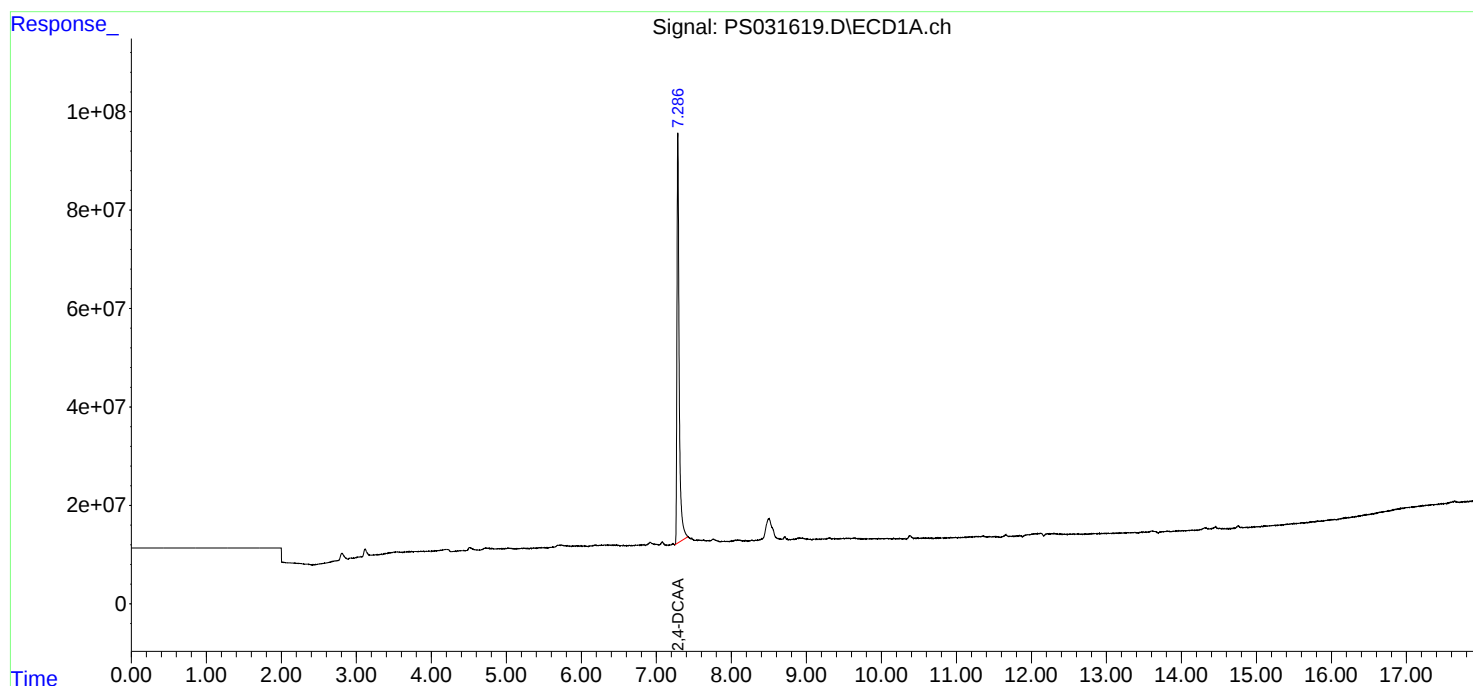


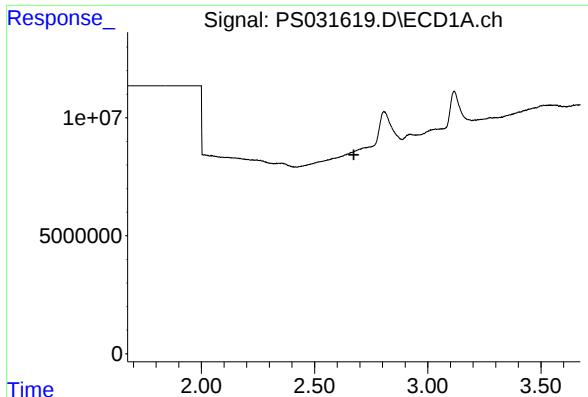

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

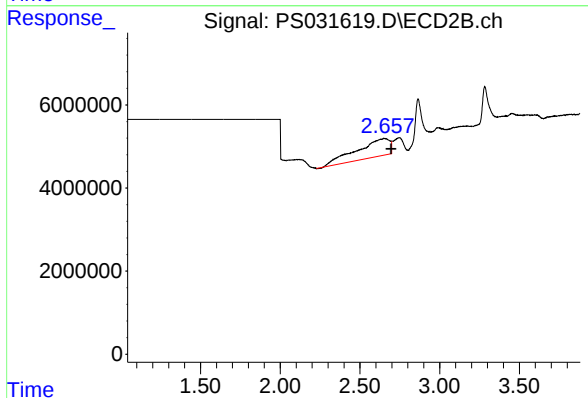


#1 Dalapon

R.T.: 2.657 min
Delta R.T.: -0.038 min
Response: 62355020
Conc: 23.43 ng/ml

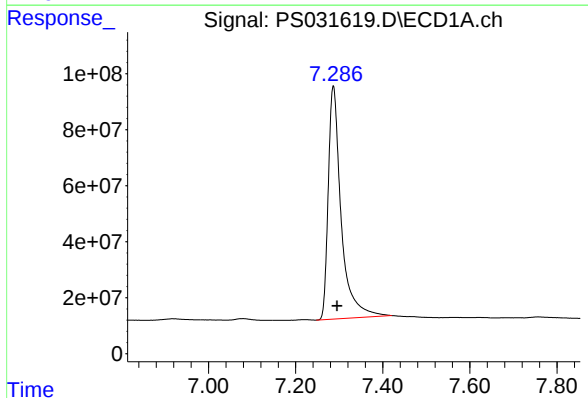


#4 2,4-DCAA

R.T.: 7.287 min
Delta R.T.: -0.008 min
Response: 1711456079
Conc: 539.21 ng/ml

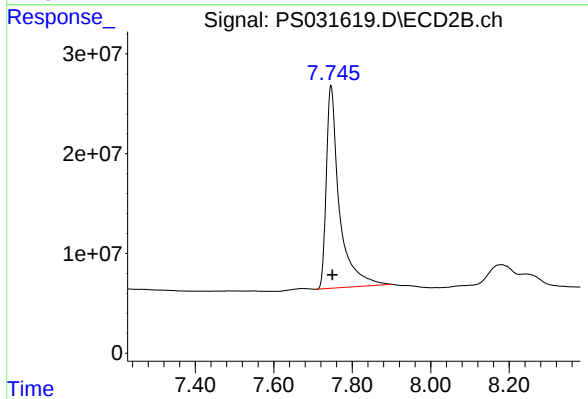

#4 2,4-DCAA


R.T.: 7.746 min
Delta R.T.: -0.003 min
Response: 468842237
Conc: 554.62 ng/ml

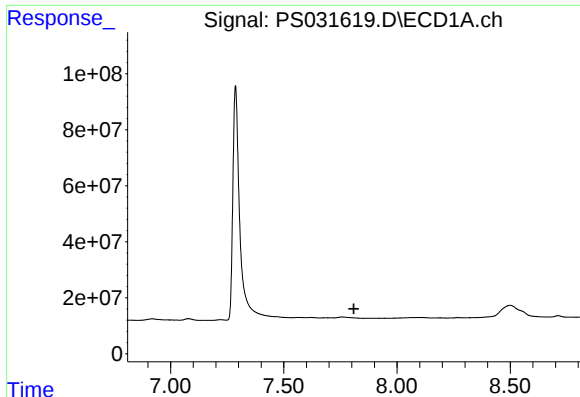

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.809 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

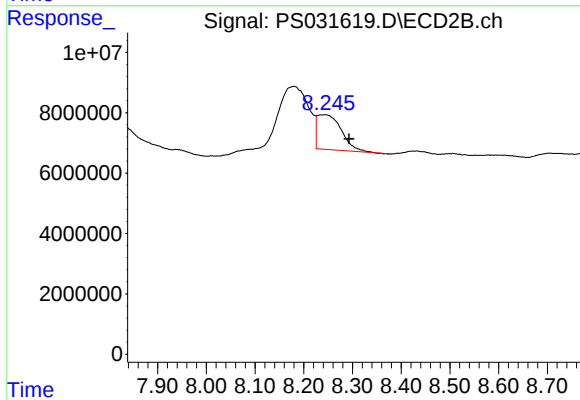


#7 MCPA

R.T.: 8.245 min
Delta R.T.: -0.048 min
Response: 39644986
Conc: 14.13 ug/ml

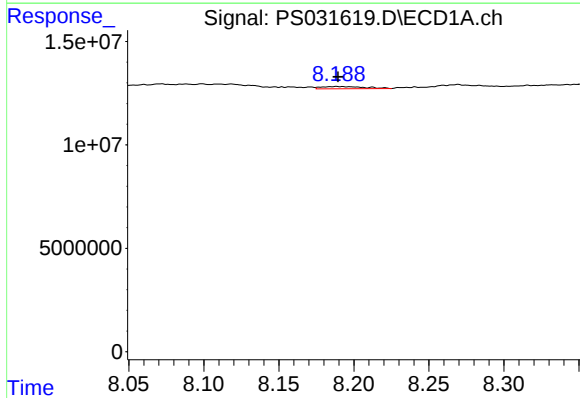

#8 DICHLORPROP

R.T.: 8.189 min
Delta R.T.: 0.000 min
Response: 2149267
Conc: N.D.

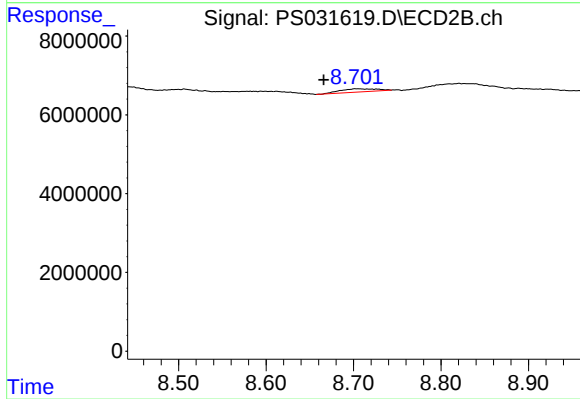

#8 DICHLORPROP

R.T.: 8.703 min
Delta R.T.: 0.037 min
Response: 2327935
Conc: 1.74 ng/ml