

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090419\
 Data File : PS006555.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2019 23:42
 Operator : SM\AJ
 Sample : K4554-55
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SB-5-(0-2)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 01:28:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.483	5.212	245.5E6	110.0E6	284.454	223.570
Target Compounds							
1) T	Dalapon	2.115	1.740	15099994	166.1E6	13.858	264.757 #
2) T	3,5-DICHL...	0.000	4.541	0	48598904	N.D.	80.235
5) T	DICAMBA	5.646	0.000	10347629	0	3.222	N.D. #
7) T	MCPA	5.960	5.613	2490506	52740881	<MDL	25.806 #
9) T	2,4-D	6.548	0.000	101.8E6	0	124.966	N.D. #
10) T	Pentachlo...	6.821	0.000	22453898	0	1.900	N.D. #
13) T	2,4-DB	8.112	7.733	327.5E6	24664386	525.847	74.111 #
14) T	DINOSEB	9.243	0.000	33218589	0	9.074	N.D. #
15) T	Picloram	0.000	9.017	0	60483728	N.D.	13.408
16) T	DCPA	0.000	9.017	0	60483728	N.D.	17.345



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090419\
Data File : PS006555.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2019 23:42
Operator : SM\AJ
Sample : K4554-55
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SB-5-(0-2)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 01:28:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

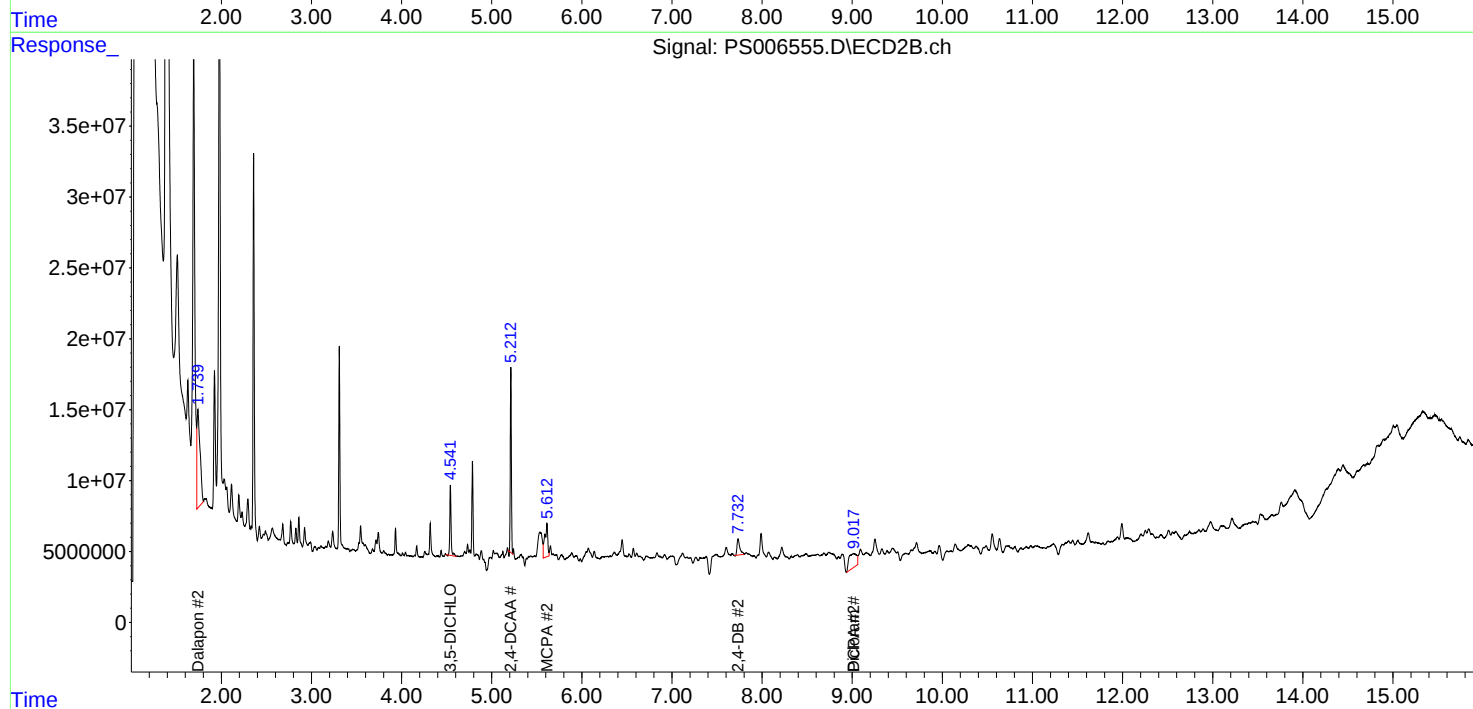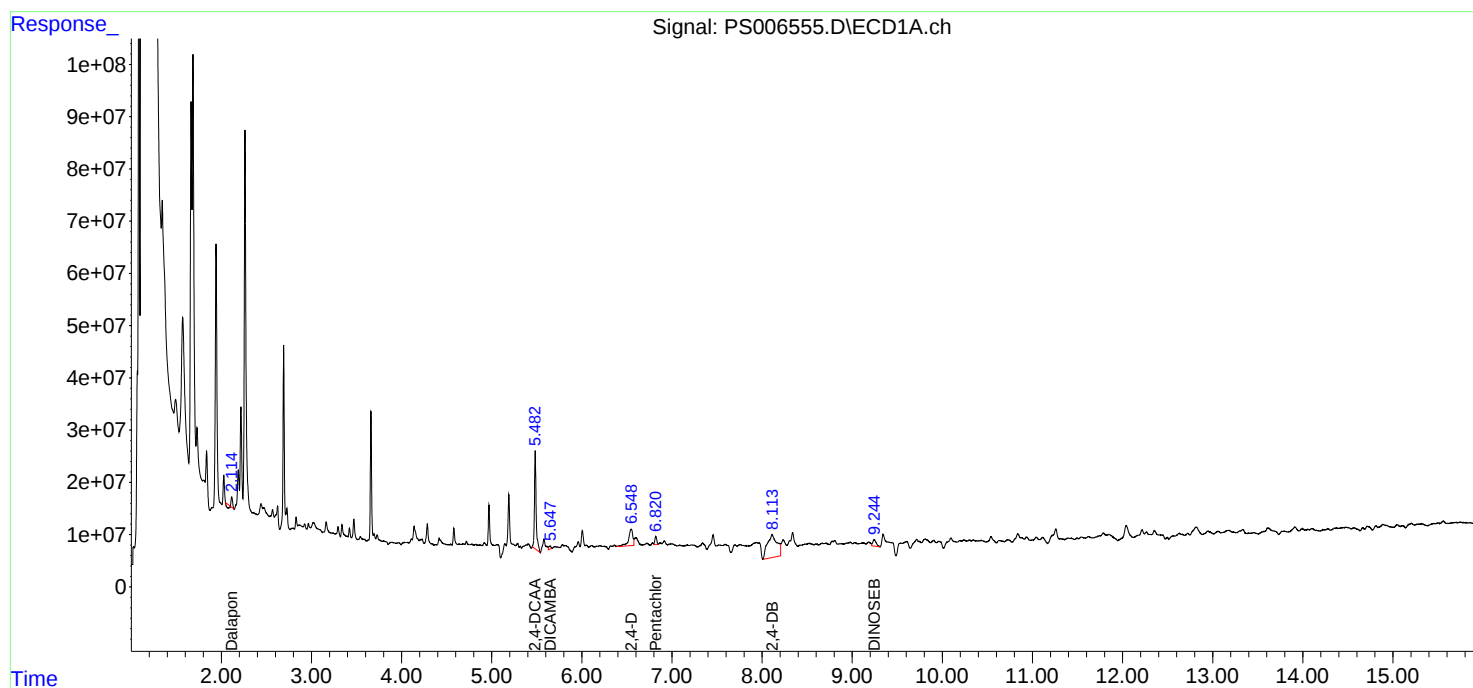


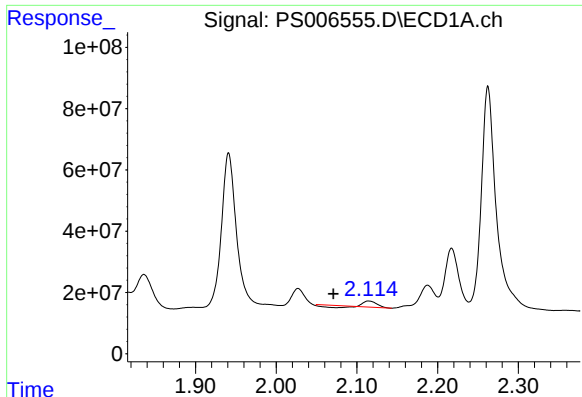

#1 Dalapon


R.T.: 2.115 min
Delta R.T.: 0.044 min
Response: 15099994
Conc: 13.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
SB-5-(0-2)

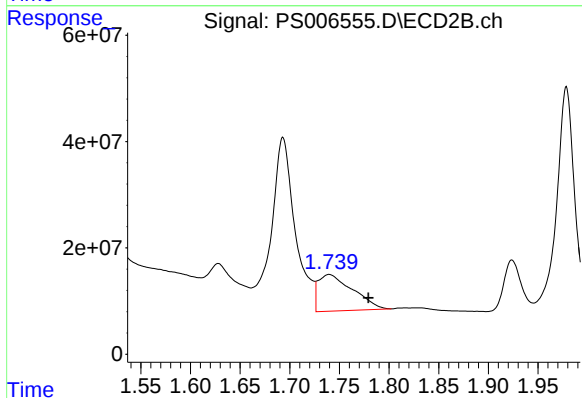


#1 Dalapon

R.T.: 1.740 min
Delta R.T.: -0.039 min
Response: 166133100
Conc: 264.76 ng/ml

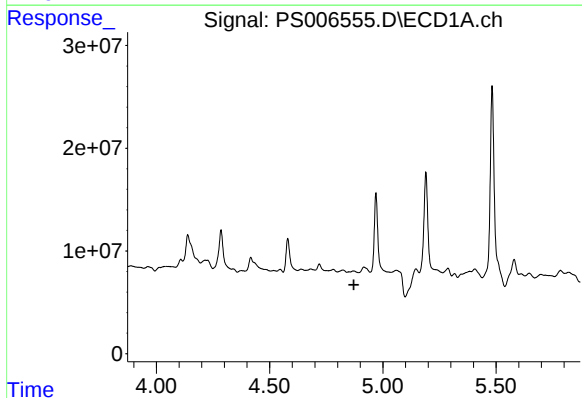


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.872 min
Response: 0
Conc: N.D.

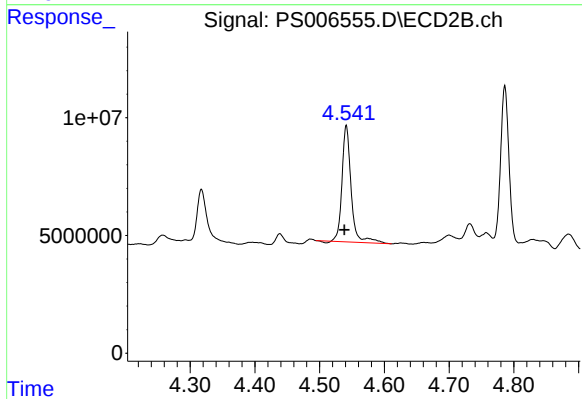

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.541 min
Delta R.T.: 0.003 min
Response: 48598904
Conc: 80.24 ng/ml

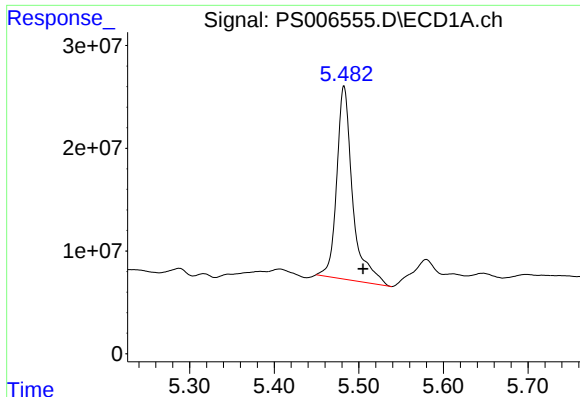

#4 2,4-DCAA


R.T.: 5.483 min
Delta R.T.: -0.023 min
Response: 245540720
Conc: 284.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
SB-5-(0-2)

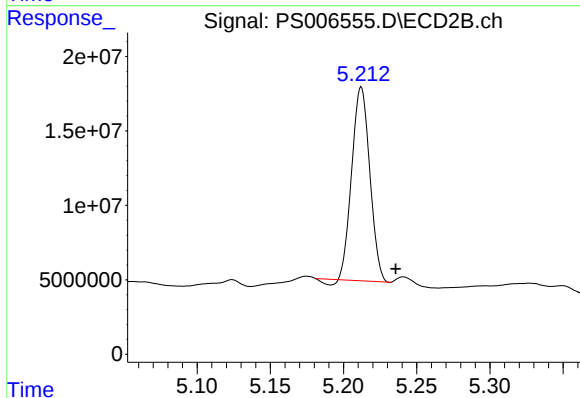


#4 2,4-DCAA

R.T.: 5.212 min
Delta R.T.: -0.024 min
Response: 109963140
Conc: 223.57 ng/ml

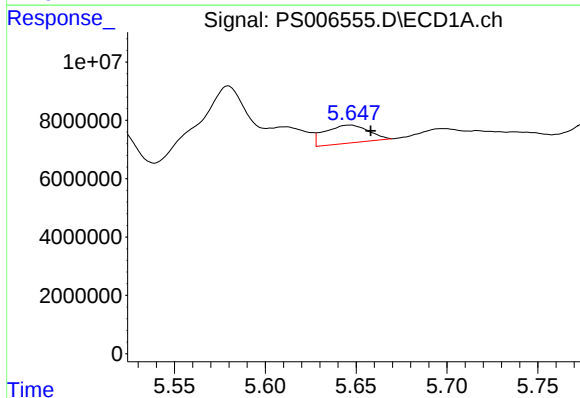


#5 DICAMBA

R.T.: 5.646 min
Delta R.T.: -0.012 min
Response: 10347629
Conc: 3.22 ng/ml

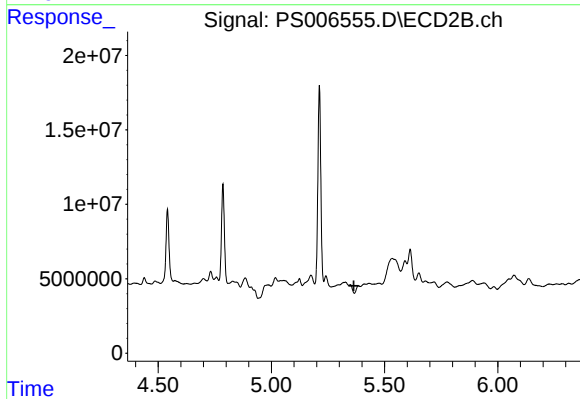

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.364 min
Response: 0
Conc: N.D.

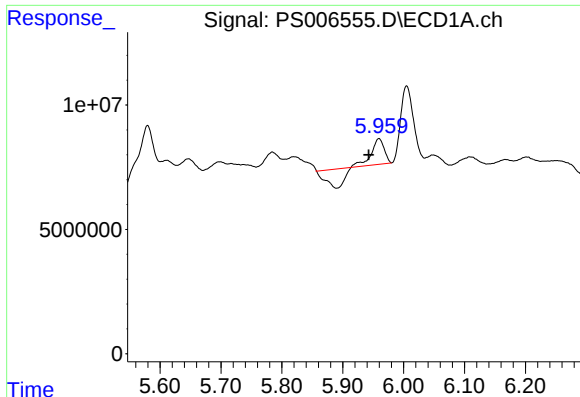

#7 MCPA


R.T.: 5.960 min
Delta R.T.: 0.017 min
Response: 2490506
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SB-5-(0-2)

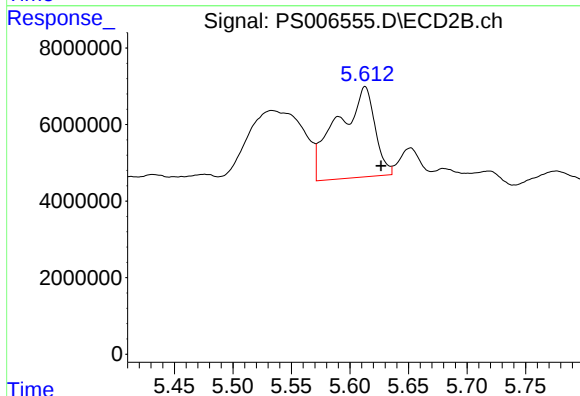


#7 MCPA

R.T.: 5.613 min
Delta R.T.: -0.014 min
Response: 52740881
Conc: 25.81 ug/ml

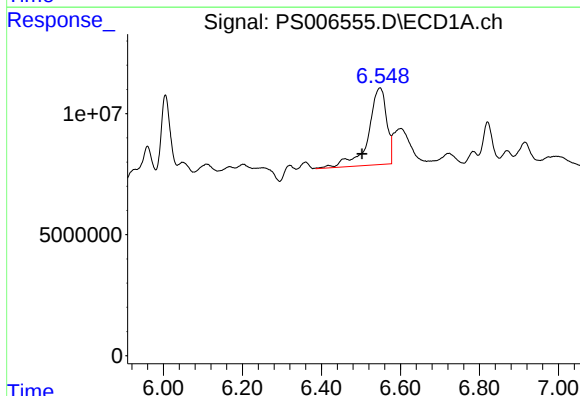


#9 2,4-D

R.T.: 6.548 min
Delta R.T.: 0.045 min
Response: 101819955
Conc: 124.97 ng/ml

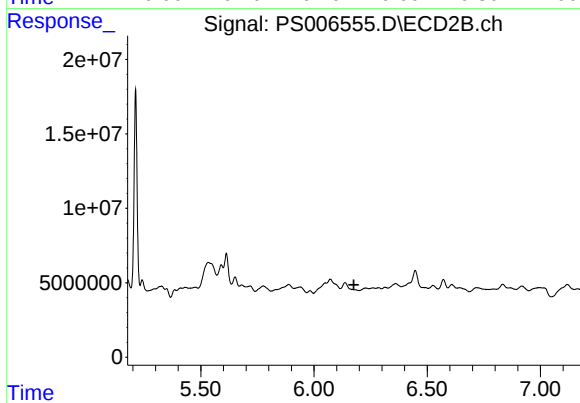

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

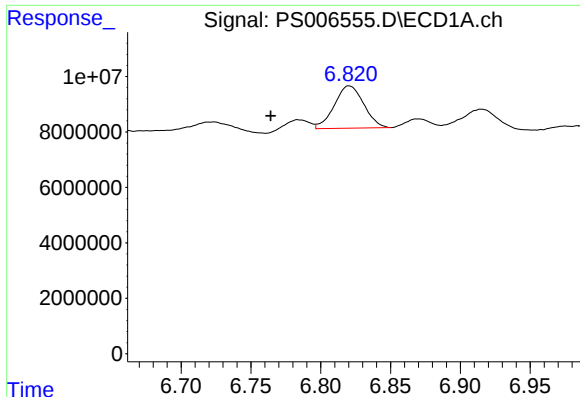

#10 Pentachlorophenol


R.T.: 6.821 min
Delta R.T.: 0.056 min
Response: 22453898
Conc: 1.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
SB-5-(0-2)

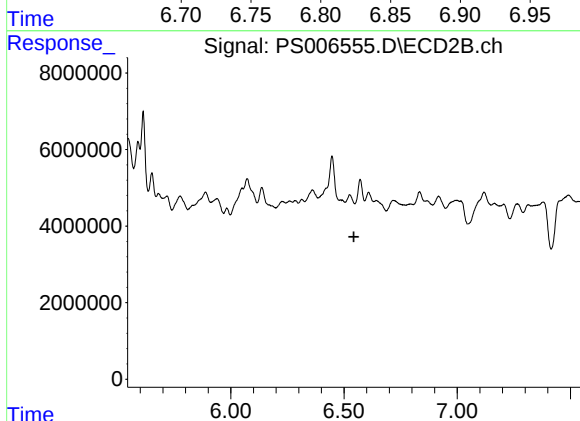


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.544 min
Response: 0
Conc: N.D.

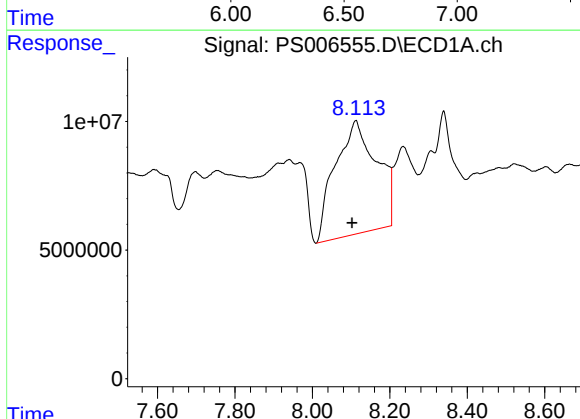


#13 2,4-DB

R.T.: 8.112 min
Delta R.T.: 0.009 min
Response: 327490112
Conc: 525.85 ng/ml

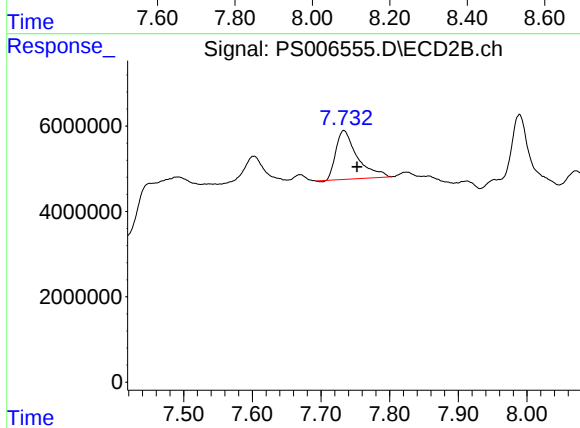

#13 2,4-DB


R.T.: 7.733 min
Delta R.T.: -0.019 min
Response: 24664386
Conc: 74.11 ng/ml

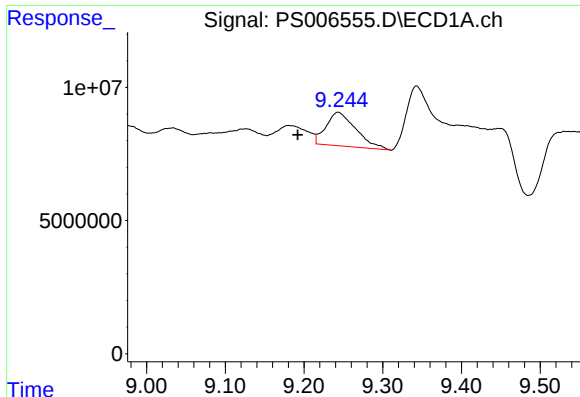

#14 DINoseb


R.T.: 9.243 min
Delta R.T.: 0.051 min
Response: 33218589
Conc: 9.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
SB-5-(0-2)

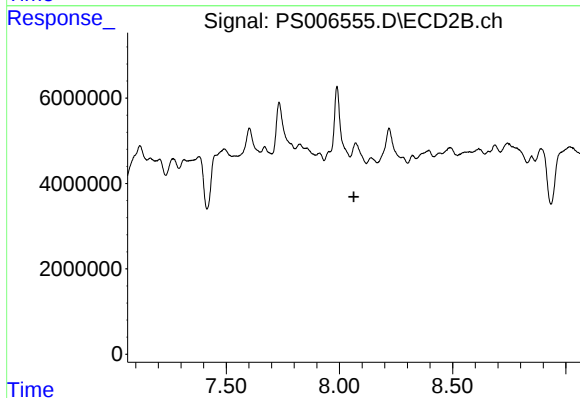


#14 DINoseb

R.T.: 0.000 min
Exp R.T. : 8.064 min
Response: 0
Conc: N.D.

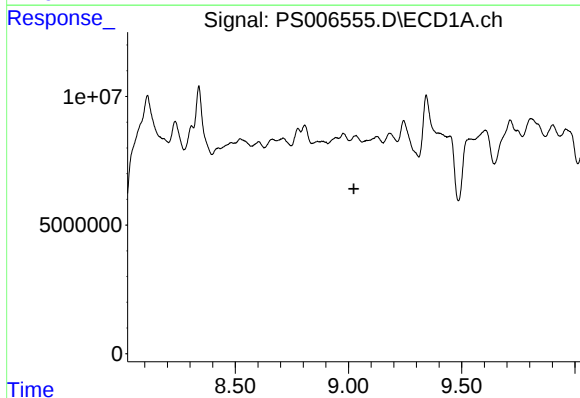


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.024 min
Response: 0
Conc: N.D.

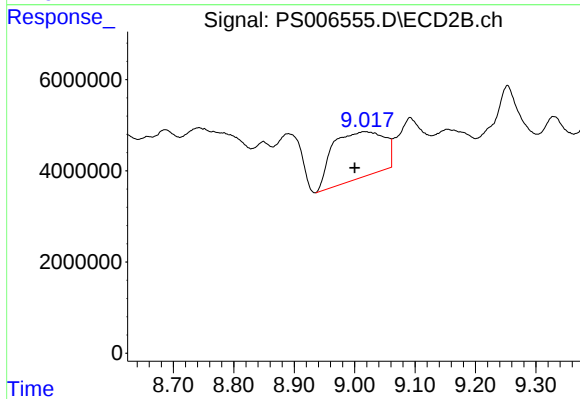

#15 Picloram


R.T.: 9.017 min
Delta R.T.: 0.017 min
Response: 60483728
Conc: 13.41 ng/ml

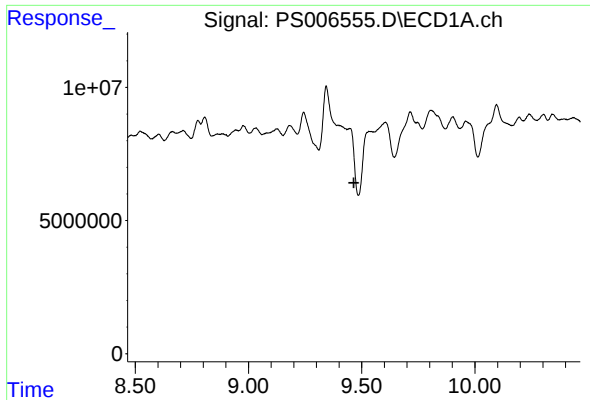

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SB-5-(0-2)

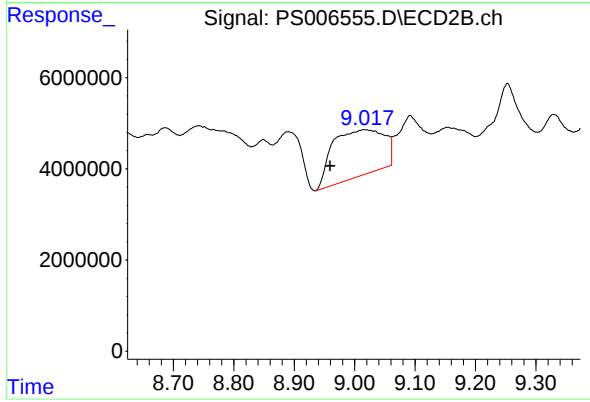

#16 DCPA

R.T.: 9.017 min
Delta R.T.: 0.057 min
Response: 60483728
Conc: 17.34 ng/ml