

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090419\
 Data File : PS006542.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2019 18:56
 Operator : SM\AJ
 Sample : K4554-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SB-15-(0-2)

Manual Integrations
 APPROVED

Ankita
 9/5/2019 12:29:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 01:22:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.482	5.212	463.6E6	211.9E6	537.115m	430.760m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090419\
Data File : PS006542.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2019 18:56
Operator : SM\AJ
Sample : K4554-07
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
SB-15-(0-2)


Manual Integrations
APPROVED

Ankita
9/5/2019 12:29:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 01:22:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

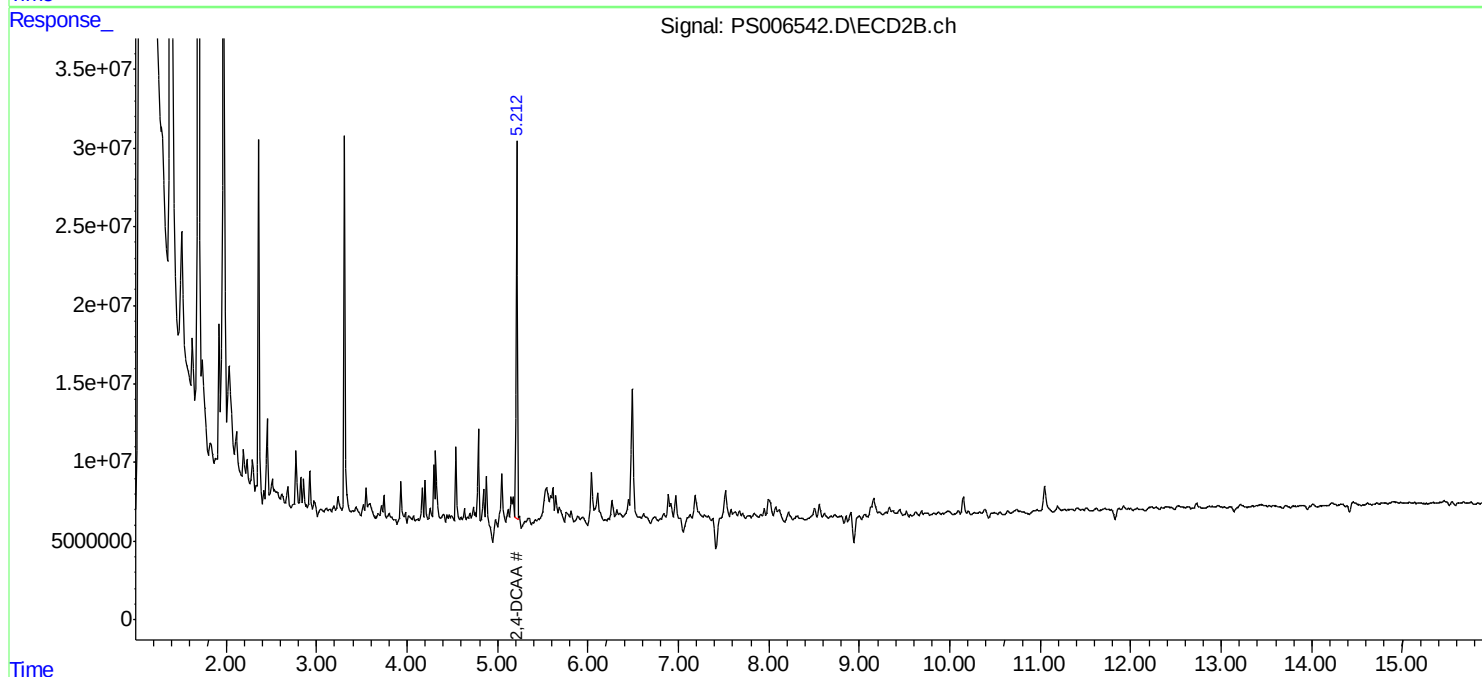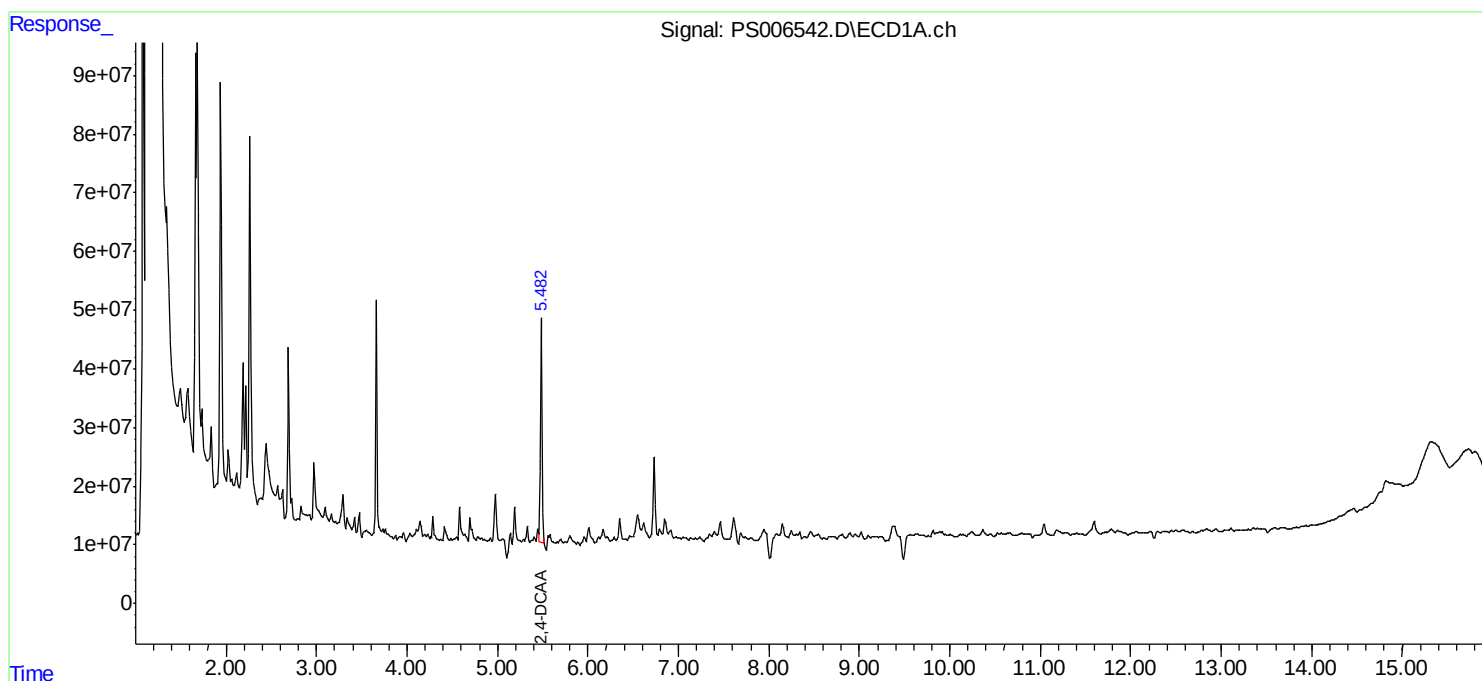

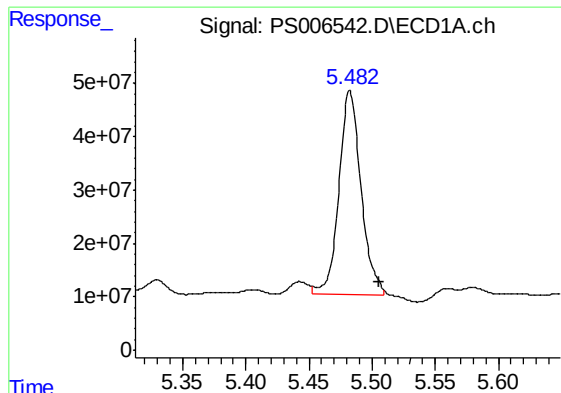


#4 2,4-DCAA

R.T.: 5.482 min
Delta R.T.: -0.023 min
Response: 463638021
Conc: 537.11 ng/ml m

Instrument :
ECD_S
ClientSampleId :
SB-15-(0-2)

Manual Integrations
APPROVED

Ankita
9/5/2019 12:29:16 PM

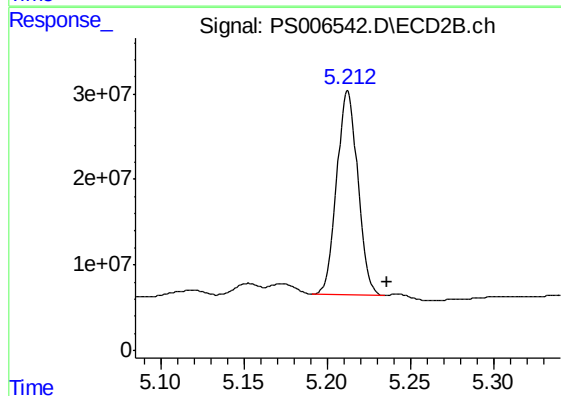

#4 2,4-DCAA

R.T.: 5.212 min
Delta R.T.: -0.024 min
Response: 211870114
Conc: 430.76 ng/ml m